

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080620\
 Data File : P0070364.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 Aug 2020 6:28
 Operator : DD\AJ
 Sample : L3574-03
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-GF-02-060-B

Manual Integrations
 APPROVED

Ankita
 8/7/2020 1:14:36 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 07 08:22:41 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0080620.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Aug 06 13:04:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.376	3.562	2009871	1325273	30.395m	30.079
2) SA Decachlor...	10.005	8.754	1487628	900785	17.374	16.228

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO080620\
Data File : PO070364.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Aug 2020 6:28
Operator : DD\AJ
Sample : L3574-03
Misc :
ALS Vial : 47 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
FK-GF-02-060-B


Manual Integrations
APPROVED

Ankita
8/7/2020 1:14:36 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 07 08:22:41 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO080620.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Aug 06 13:04:06 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

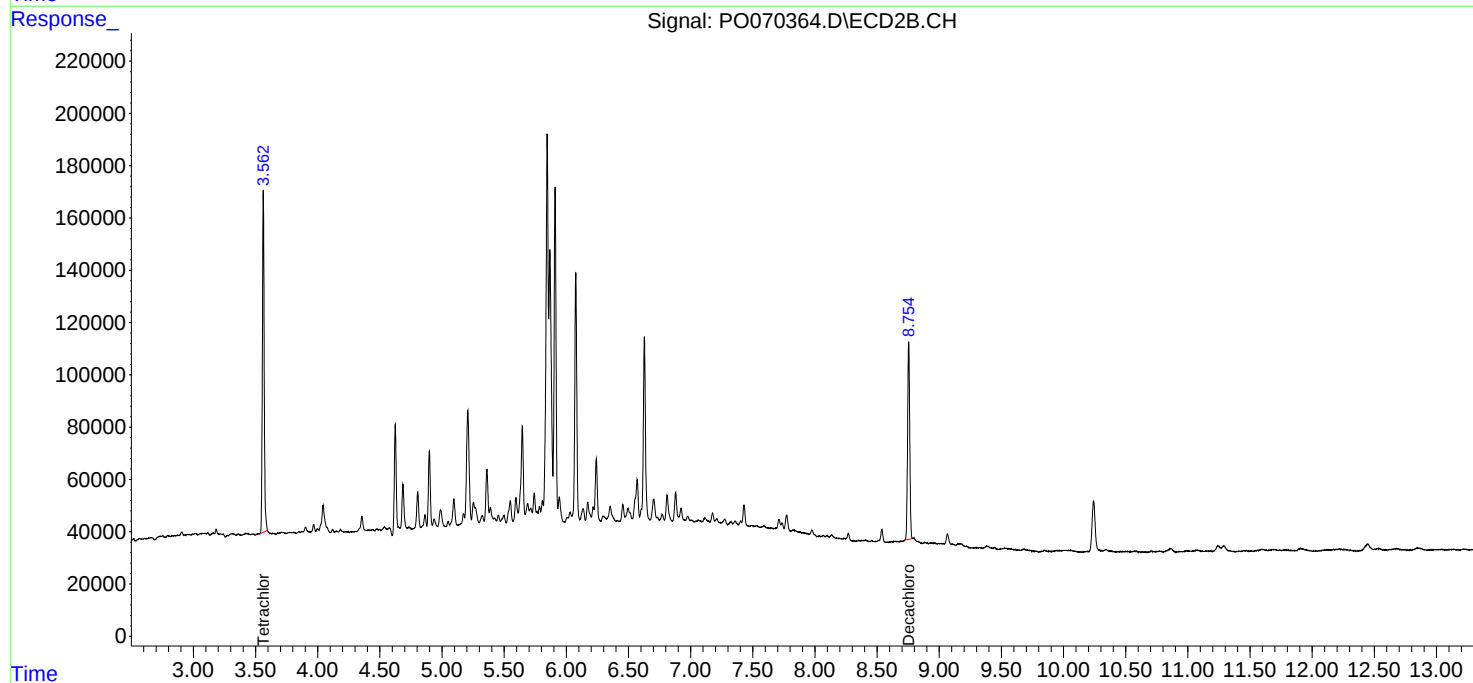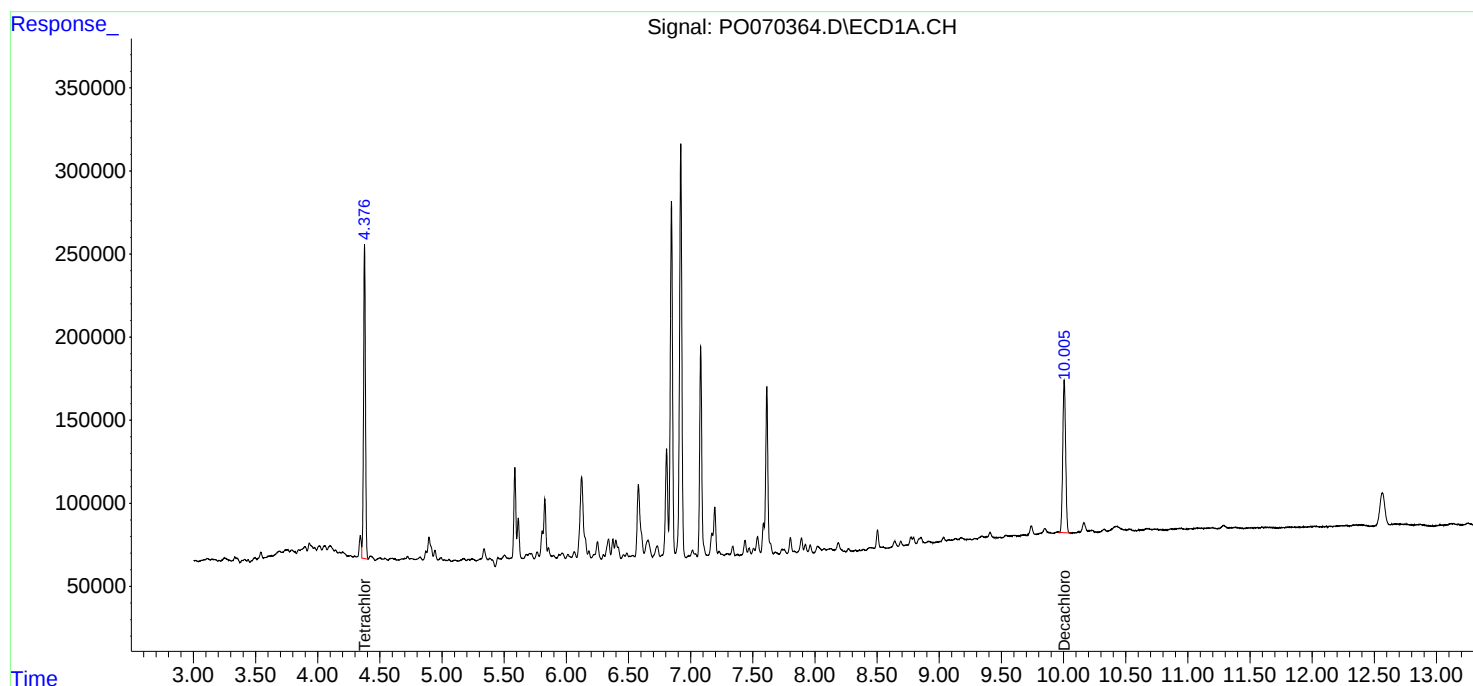

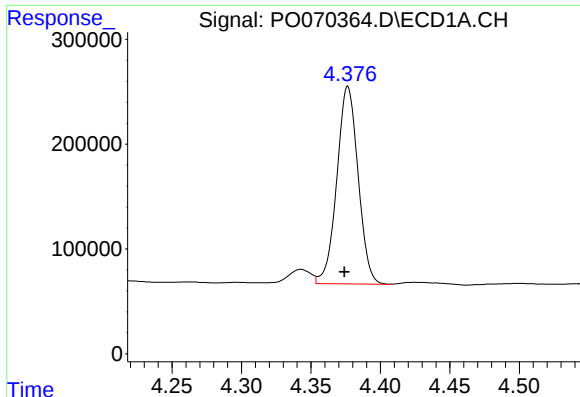


#1 Tetrachloro-m-xylene

R.T.: 4.376 min
Delta R.T.: 0.002 min
Response: 2009871
Conc: 30.39 ng/ml m

Instrument :
ECD_O
ClientSampleId :
FK-GF-02-060-B


Manual Integrations
APPROVED

Ankita
8/7/2020 1:14:36 PM

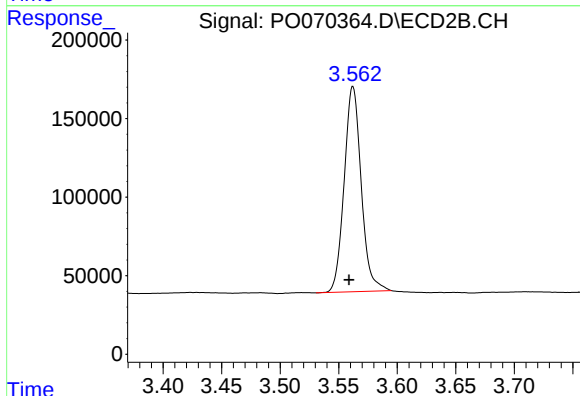


#1 Tetrachloro-m-xylene

R.T.: 3.562 min
Delta R.T.: 0.003 min
Response: 1325273
Conc: 30.08 ng/ml

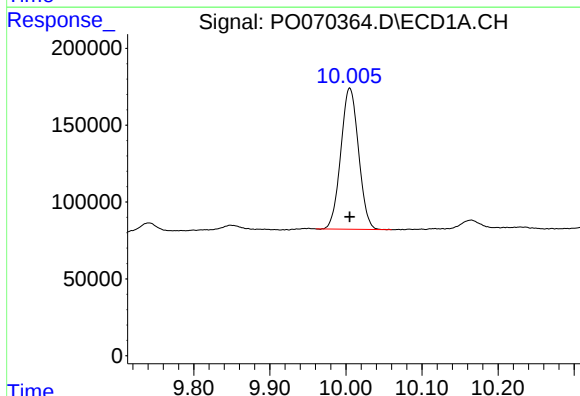

#2 Decachlorobiphenyl

R.T.: 10.005 min
Delta R.T.: 0.000 min
Response: 1487628
Conc: 17.37 ng/ml

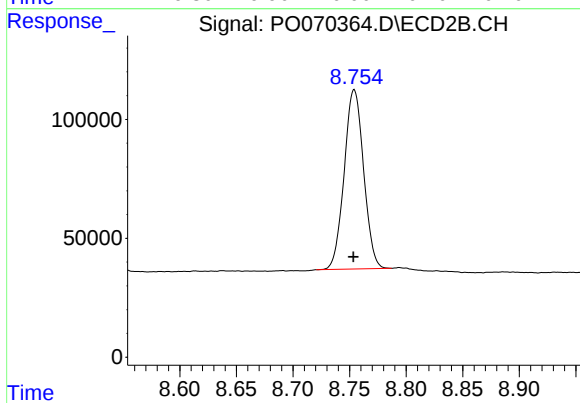

#2 Decachlorobiphenyl

R.T.: 8.754 min
Delta R.T.: 0.000 min
Response: 900785
Conc: 16.23 ng/ml