

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080621\
 Data File : P0080244.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Aug 2021 9:39
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 06 15:30:03 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 28 18:45:36 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.999	4.114	1457660	558227	24.190	24.376
2)	SA Decachlor...	11.104	9.518	1083068	512928	23.088	24.682

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO080621\
Data File : PO080244.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Aug 2021 9:39
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 06 15:30:03 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO072821.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 28 18:45:36 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

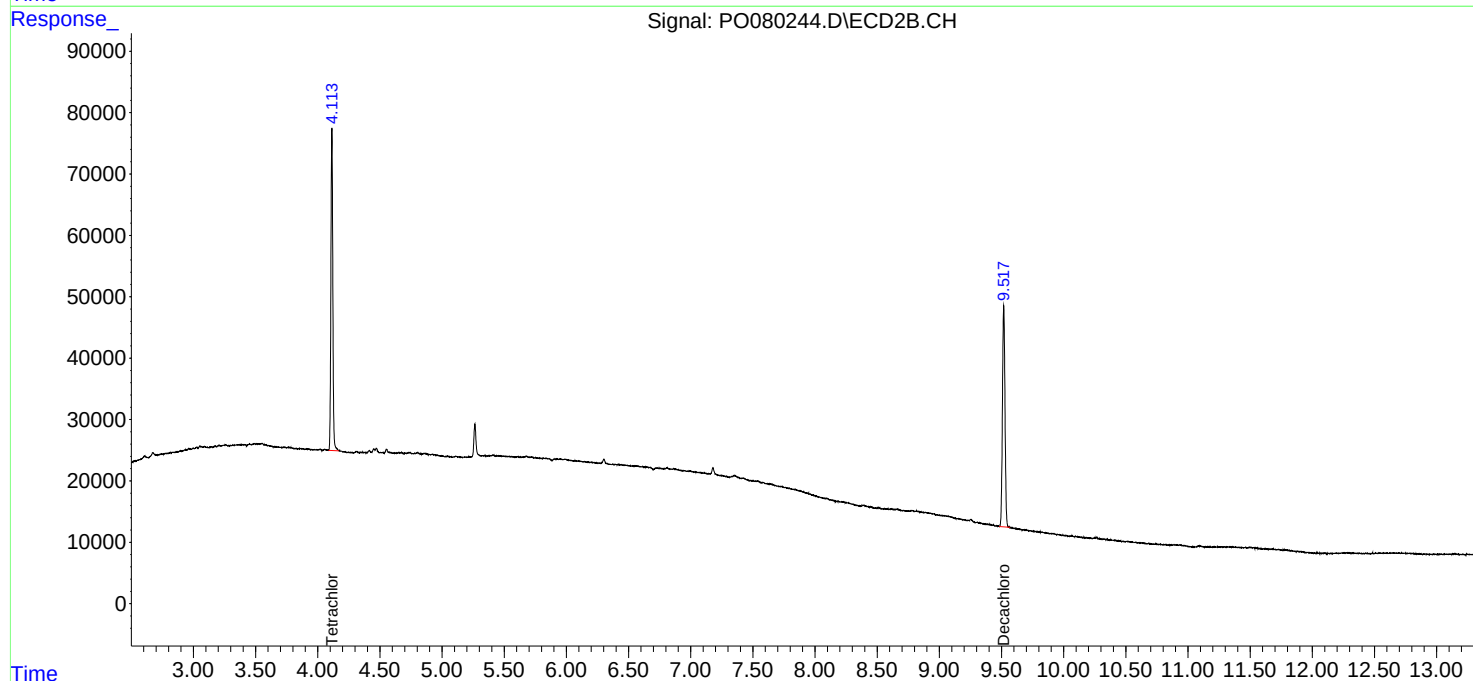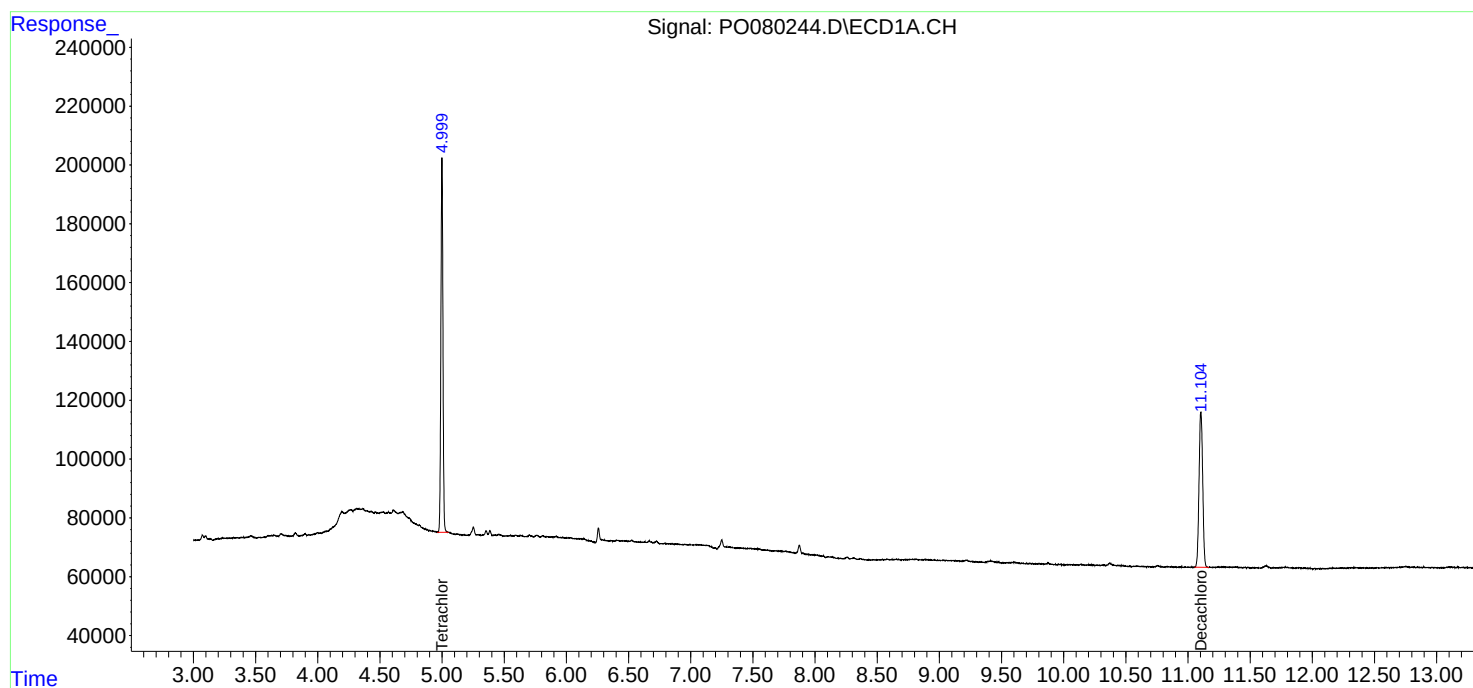


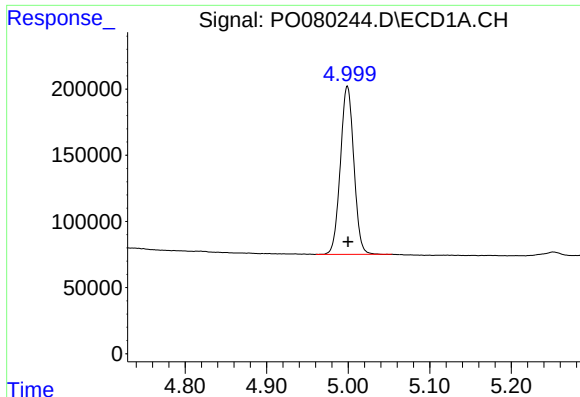

#1 Tetrachloro-m-xylene


R.T.: 4.999 min
Delta R.T.: -0.001 min
Response: 1457660
Conc: 24.19 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

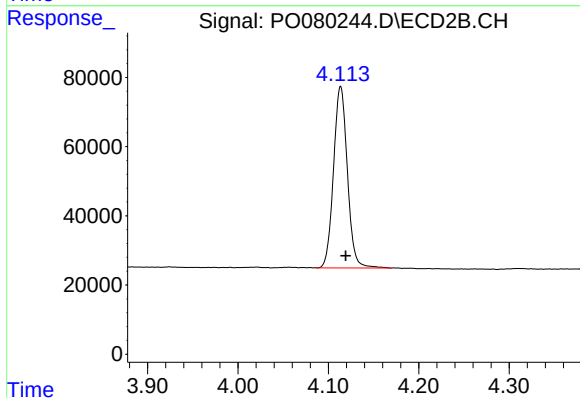


#1 Tetrachloro-m-xylene

R.T.: 4.114 min
Delta R.T.: -0.006 min
Response: 558227
Conc: 24.38 ng/ml

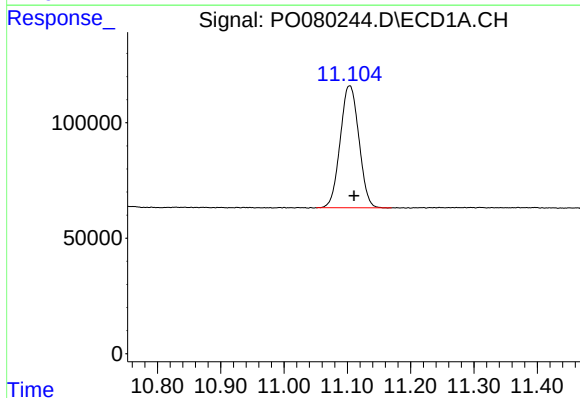

#2 Decachlorobiphenyl

R.T.: 11.104 min
Delta R.T.: -0.007 min
Response: 1083068
Conc: 23.09 ng/ml

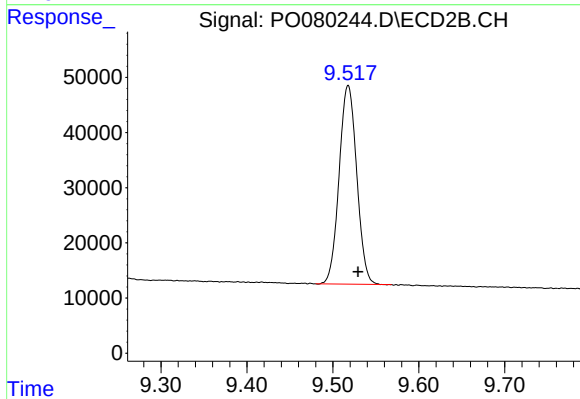

#2 Decachlorobiphenyl

R.T.: 9.518 min
Delta R.T.: -0.012 min
Response: 512928
Conc: 24.68 ng/ml