

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080621\
 Data File : P0080250.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Aug 2021 11:22
 Operator : DD\AJ
 Sample : M3279-04
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 20210571-COM-44

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 09 13:02:54 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 28 18:45:36 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.997	4.115	1078292	419487	17.895	18.317
2) SA Decachlor...	11.102	9.516	500077	245931	10.660	11.834

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080621\
Data File : P0080250.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Aug 2021 11:22
Operator : DD\AJ
Sample : M3279-04
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
20210571-COM-44

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 09 13:02:54 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072821.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 28 18:45:36 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

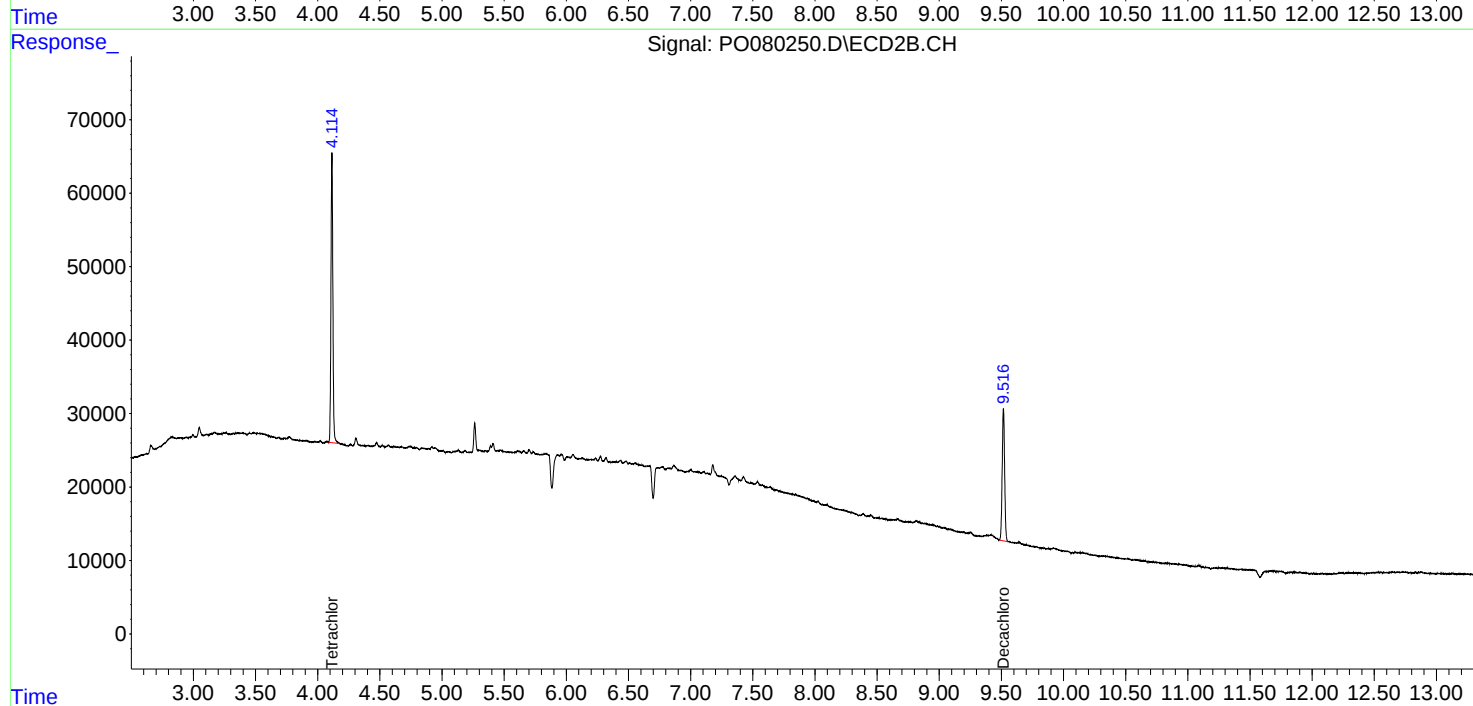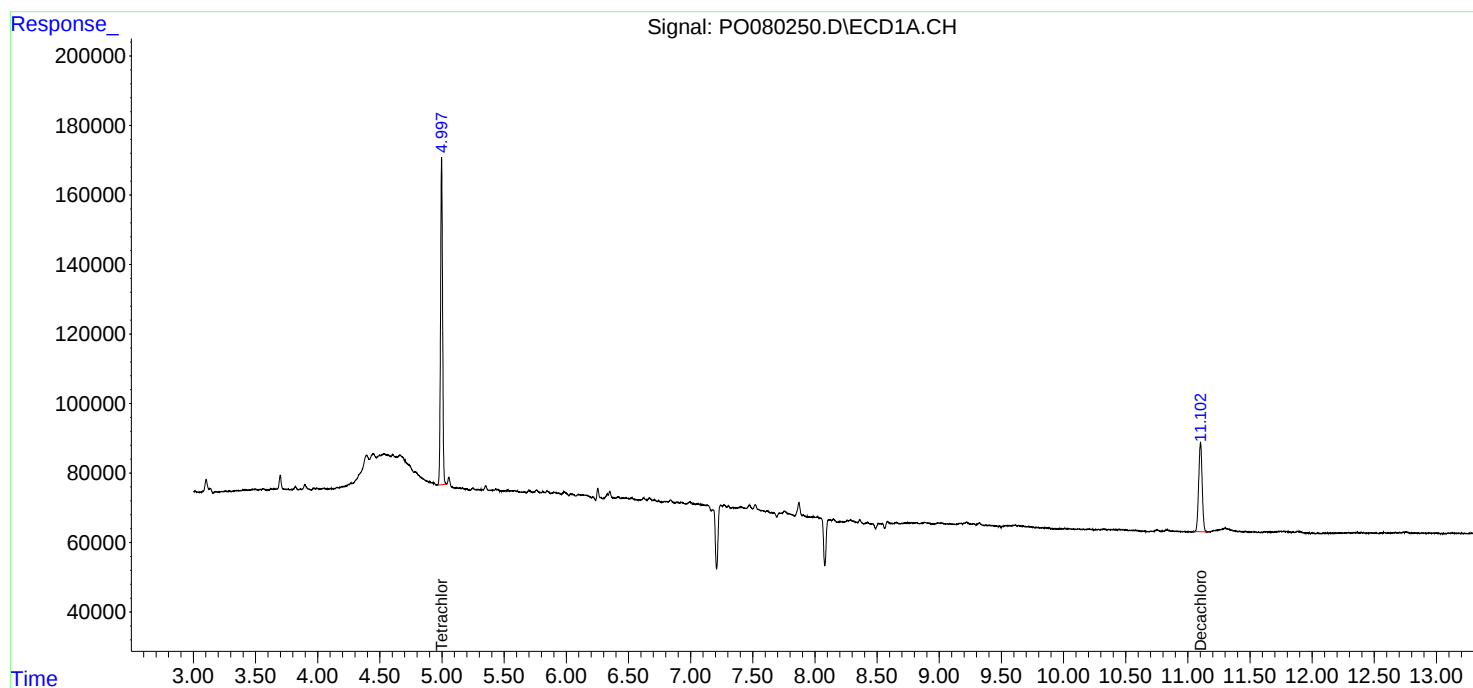


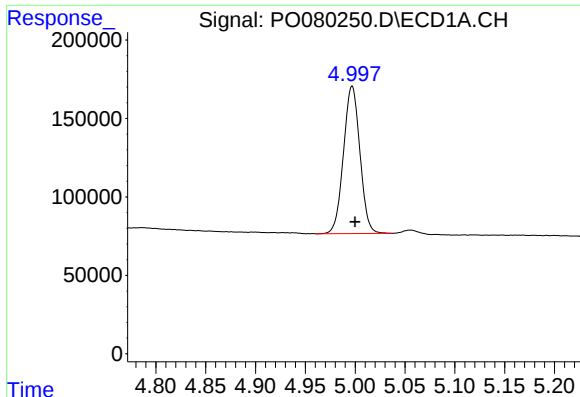

#1 Tetrachloro-m-xylene


R.T.: 4.997 min
Delta R.T.: -0.003 min
Response: 1078292
Conc: 17.89 ng/ml

Instrument :
ECD_O
ClientSampleId :
20210571-COM-44

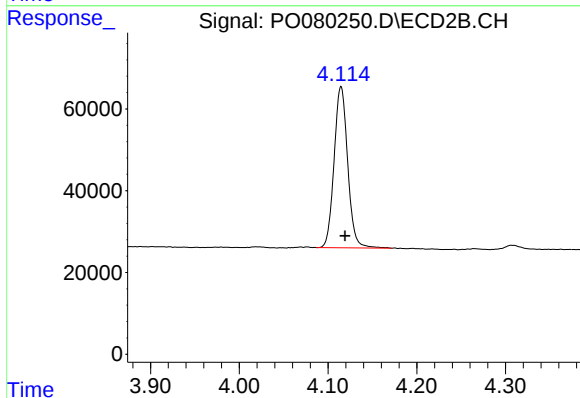


#1 Tetrachloro-m-xylene

R.T.: 4.115 min
Delta R.T.: -0.005 min
Response: 419487
Conc: 18.32 ng/ml

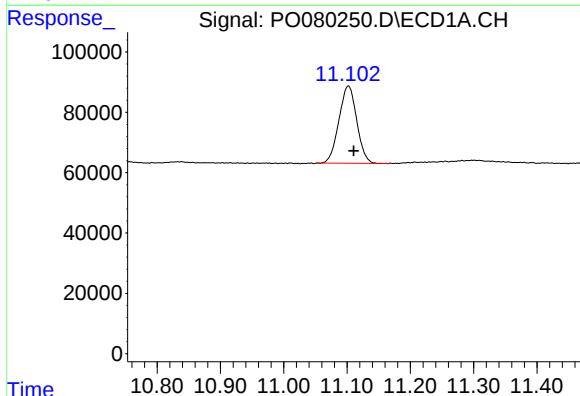

#2 Decachlorobiphenyl

R.T.: 11.102 min
Delta R.T.: -0.008 min
Response: 500077
Conc: 10.66 ng/ml

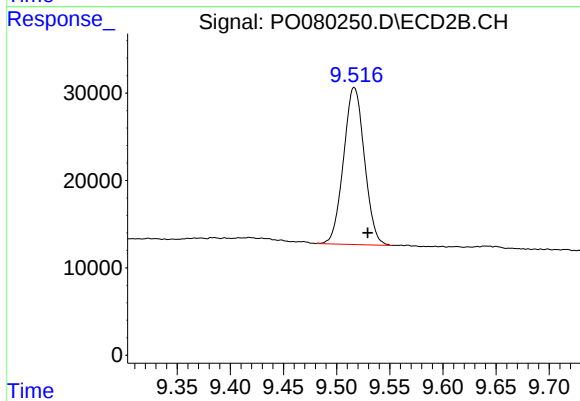

#2 Decachlorobiphenyl

R.T.: 9.516 min
Delta R.T.: -0.013 min
Response: 245931
Conc: 11.83 ng/ml