

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080621\
 Data File : P0080292.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 Aug 2021 00:06
 Operator : DD\AJ
 Sample : M3293-11
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 2055-57

Manual Integrations
 APPROVED

mohammad
 8/9/2021 5:05:15 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 09 01:45:38 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 28 18:45:36 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.993	4.112	1334885	715060	22.153m	31.224m#
2) SA Decachlor...	11.098	9.513f	738960	332294	15.753	15.990

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080621\
Data File : P0080292.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Aug 2021 00:06
Operator : DD\AJ
Sample : M3293-11
Misc :
ALS Vial : 42 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
2055-57


Manual Integrations
APPROVED

mohammad
8/9/2021 5:05:15 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 09 01:45:38 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072821.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 28 18:45:36 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

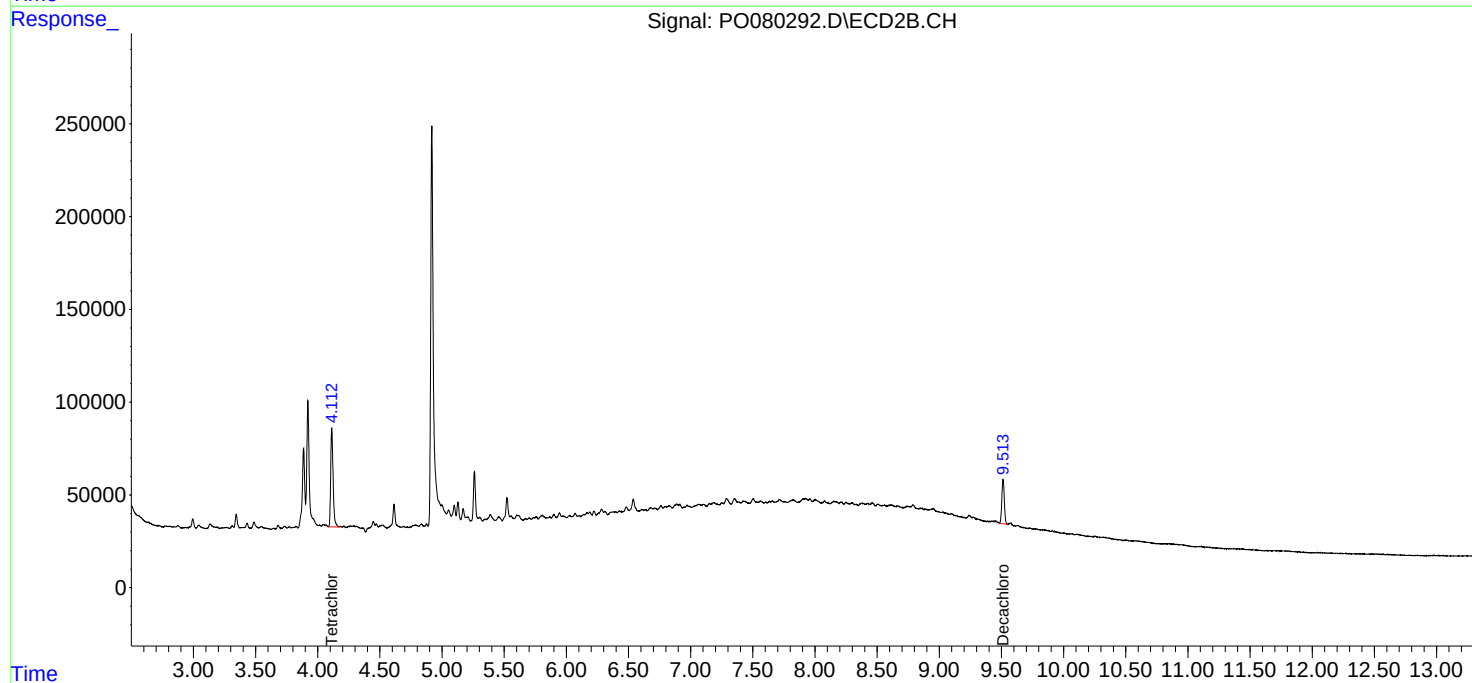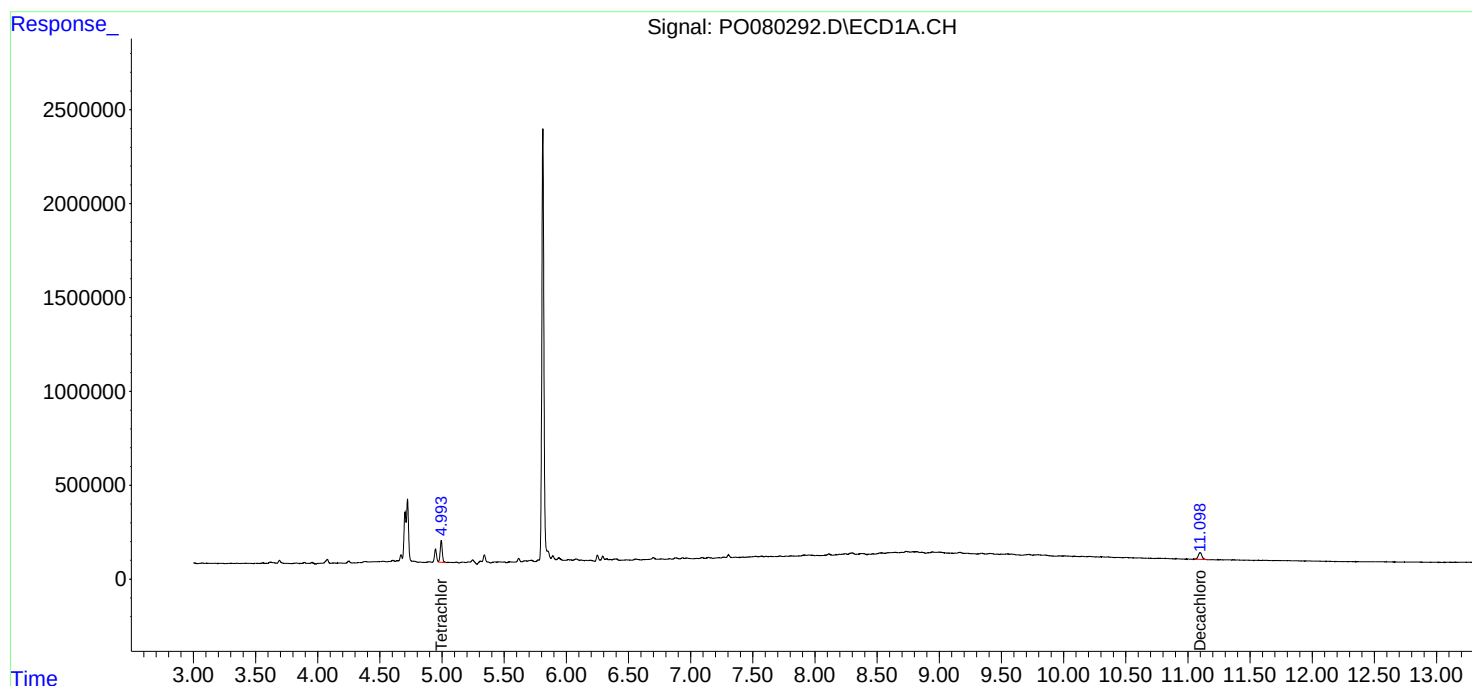

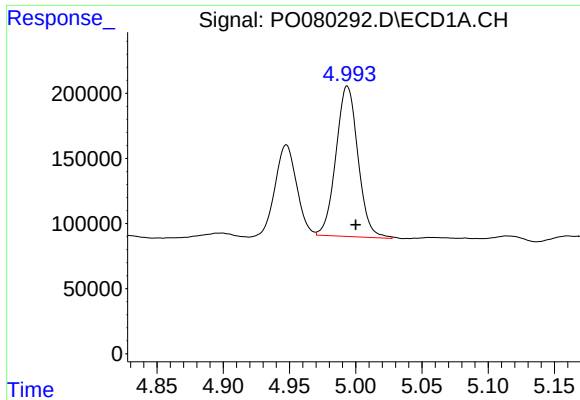


#1 Tetrachloro-m-xylene

R.T.: 4.993 min
Delta R.T.: -0.007 min
Response: 1334885
Conc: 22.15 ng/ml m

Instrument :
ECD_O
ClientSampleId :
2055-57


Manual Integrations
APPROVED

mohammad
8/9/2021 5:05:15 PM

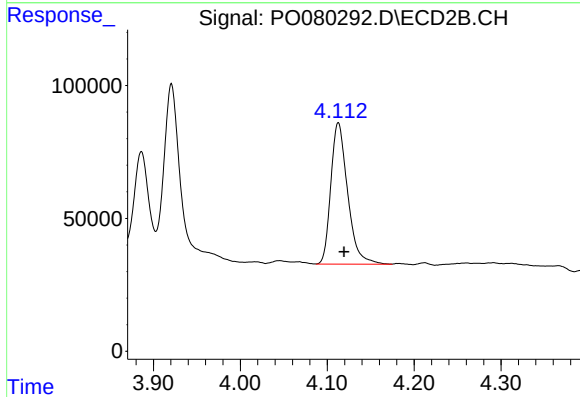


#1 Tetrachloro-m-xylene

R.T.: 4.112 min
Delta R.T.: -0.007 min
Response: 715060
Conc: 31.22 ng/ml m

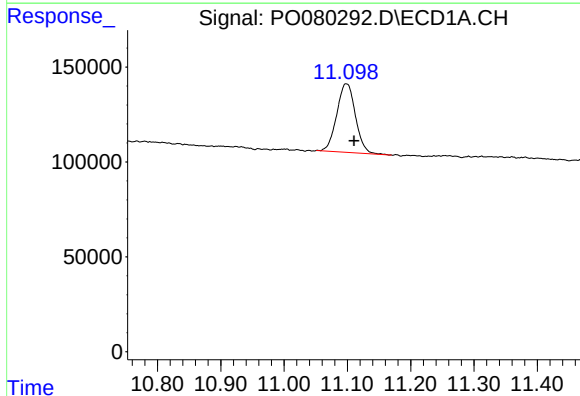

#2 Decachlorobiphenyl

R.T.: 11.098 min
Delta R.T.: -0.012 min
Response: 738960
Conc: 15.75 ng/ml

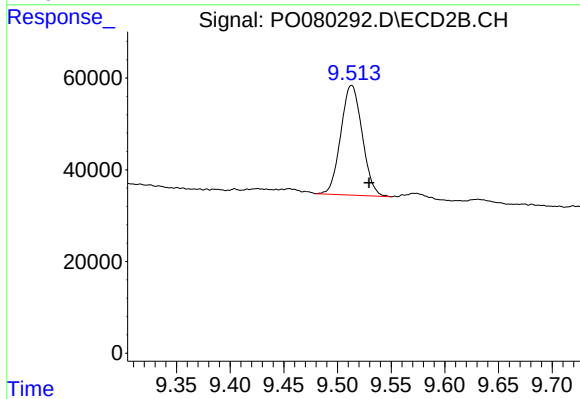

#2 Decachlorobiphenyl

R.T.: 9.513 min
Delta R.T.: -0.016 min
Response: 332294
Conc: 15.99 ng/ml