

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080719\
 Data File : P0058984.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 Aug 2019 13:48
 Operator : SM/AJ
 Sample : K4189-03
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 HA-24

Manual Integrations
 APPROVED

Ankita
 8/8/2019 2:47:11 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 07 16:12:31 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072819.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jul 27 06:49:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.157	3.516	1038506	884866	24.608m	22.149m
2)	SA Decachlor...	9.664	8.399	1921775	792268	35.486	20.071m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO080719\
Data File : PO058984.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Aug 2019 13:48
Operator : SM/AJ
Sample : K4189-03
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
HA-24


Manual Integrations
APPROVED

Ankita
8/8/2019 2:47:11 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 07 16:12:31 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO072819.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jul 27 06:49:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

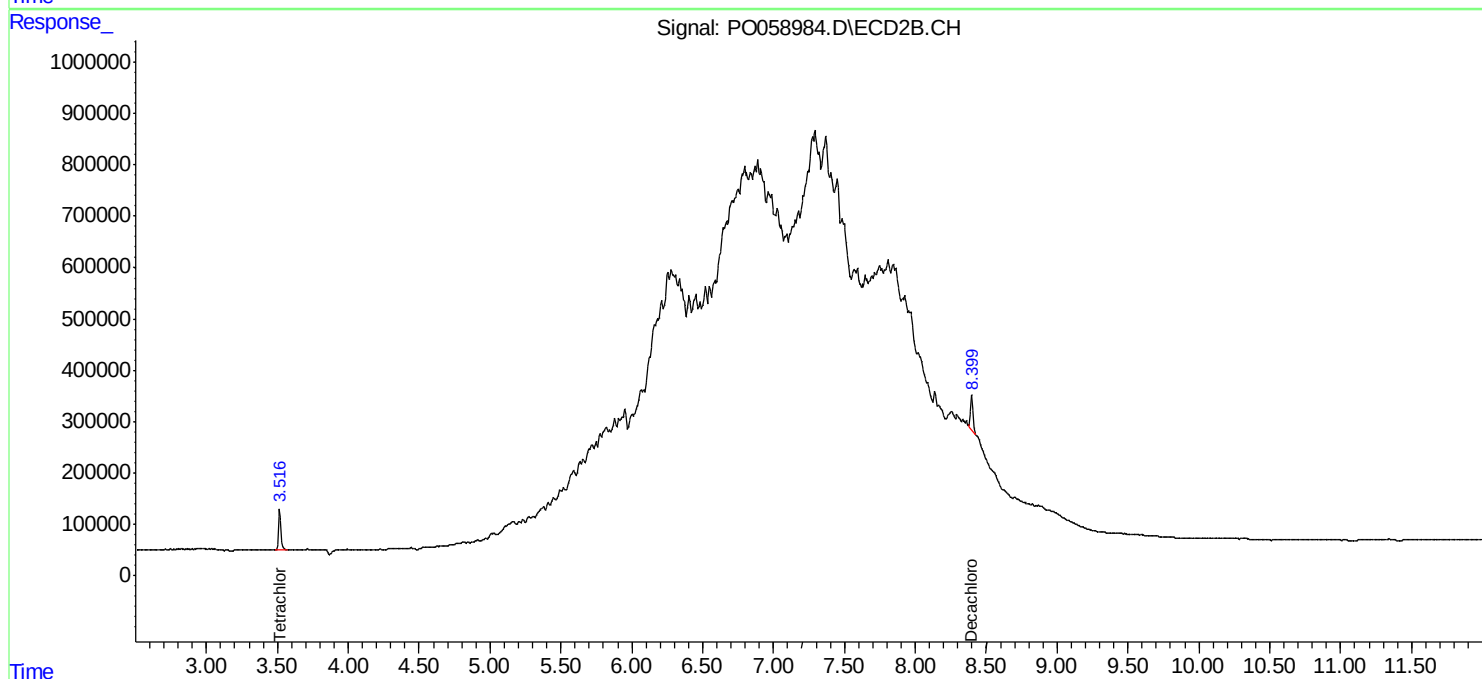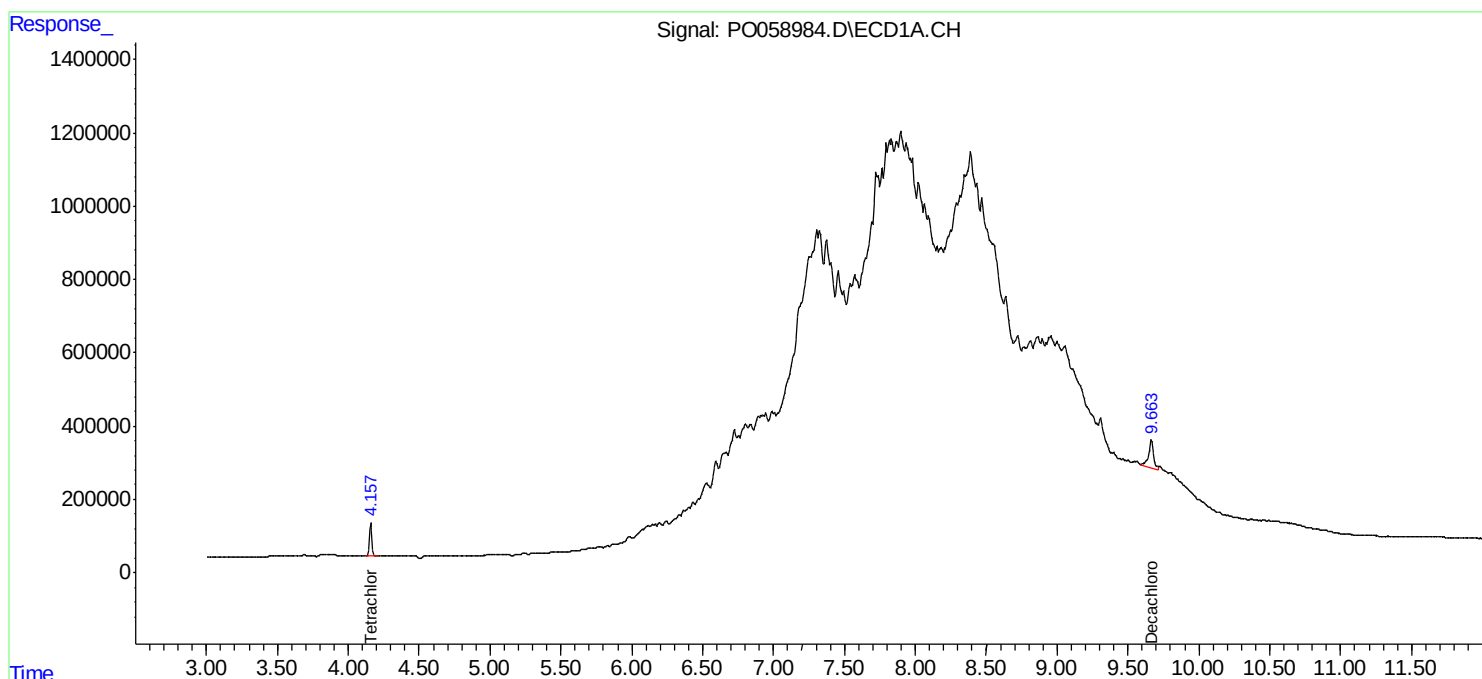

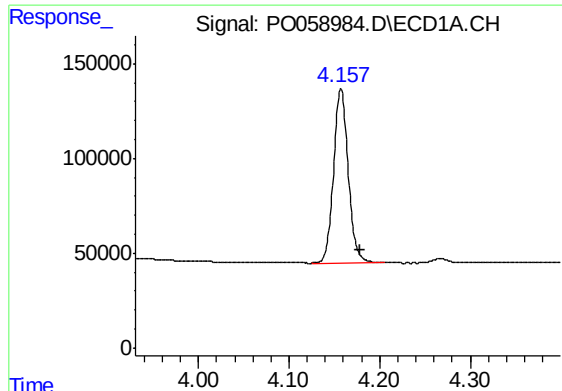

#1 Tetrachloro-m-xylene

R.T.: 4.157 min

Delta R.T.: -0.022 min


Response: 1038506

Conc: 24.61 ng/ml m

Instrument :
ECD_O
ClientSampleId :
HA-24

Manual Integrations
APPROVED

Ankita
8/8/2019 2:47:11 PM

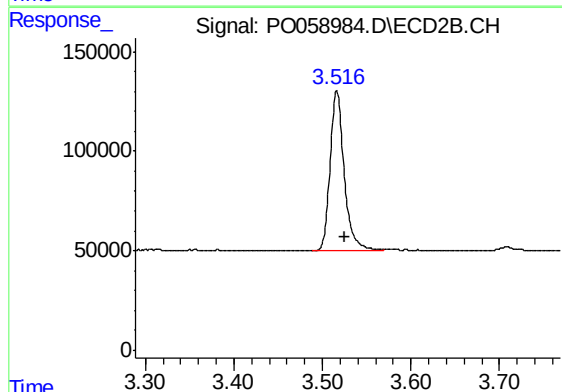


#1 Tetrachloro-m-xylene

R.T.: 3.516 min

Delta R.T.: -0.009 min

Response: 884866

Conc: 22.15 ng/ml m

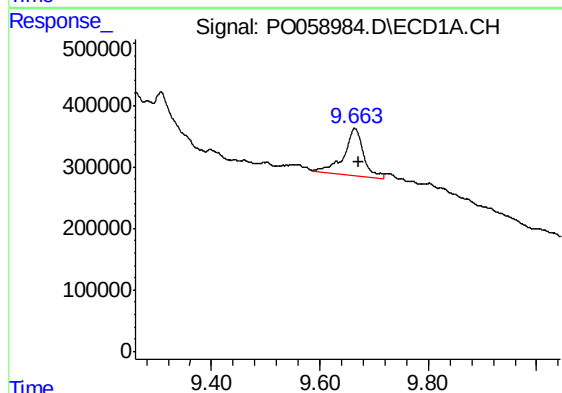


#2 Decachlorobiphenyl

R.T.: 9.664 min

Delta R.T.: -0.008 min

Response: 1921775

Conc: 35.49 ng/ml

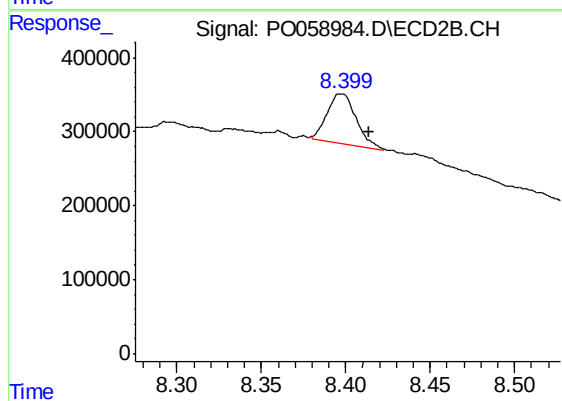

#2 Decachlorobiphenyl

R.T.: 8.399 min

Delta R.T.: -0.015 min

Response: 792268

Conc: 20.07 ng/ml m