

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080719\
 Data File : P0058998.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 Aug 2019 19:53
 Operator : SM/SJ
 Sample : K4174-01
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 VW-PAINT-CHIPS

Manual Integrations
 APPROVED

Ankita
 8/8/2019 2:47:26 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 08 08:20:41 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072819.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jul 27 06:49:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.152	3.514	821678	786289	19.470m	19.682m
2)	SA Decachlor...	9.659	8.394	1447253	1010465	26.724	25.599
Target Compounds							
26)	L6 AR-1254-1	6.148	5.353	1460300	2684357	618.433m	1036.216 #
27)	L6 AR-1254-2	6.366	5.499	3713001	1443317	963.427	630.427 #
28)	L6 AR-1254-3	6.730	5.896	3272770	3233255	808.164	878.754
29)	L6 AR-1254-4	7.014	6.123	3594536	2325604	998.304m	1000.167
30)	L6 AR-1254-5	7.430	6.532	5129716	3701990	1415.187m	1073.179

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO080719\
Data File : PO058998.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Aug 2019 19:53
Operator : SM/SJ
Sample : K4174-01
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
VW-PAINT-CHIPS


Manual Integrations
APPROVED

Ankita
8/8/2019 2:47:26 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 08 08:20:41 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO072819.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jul 27 06:49:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

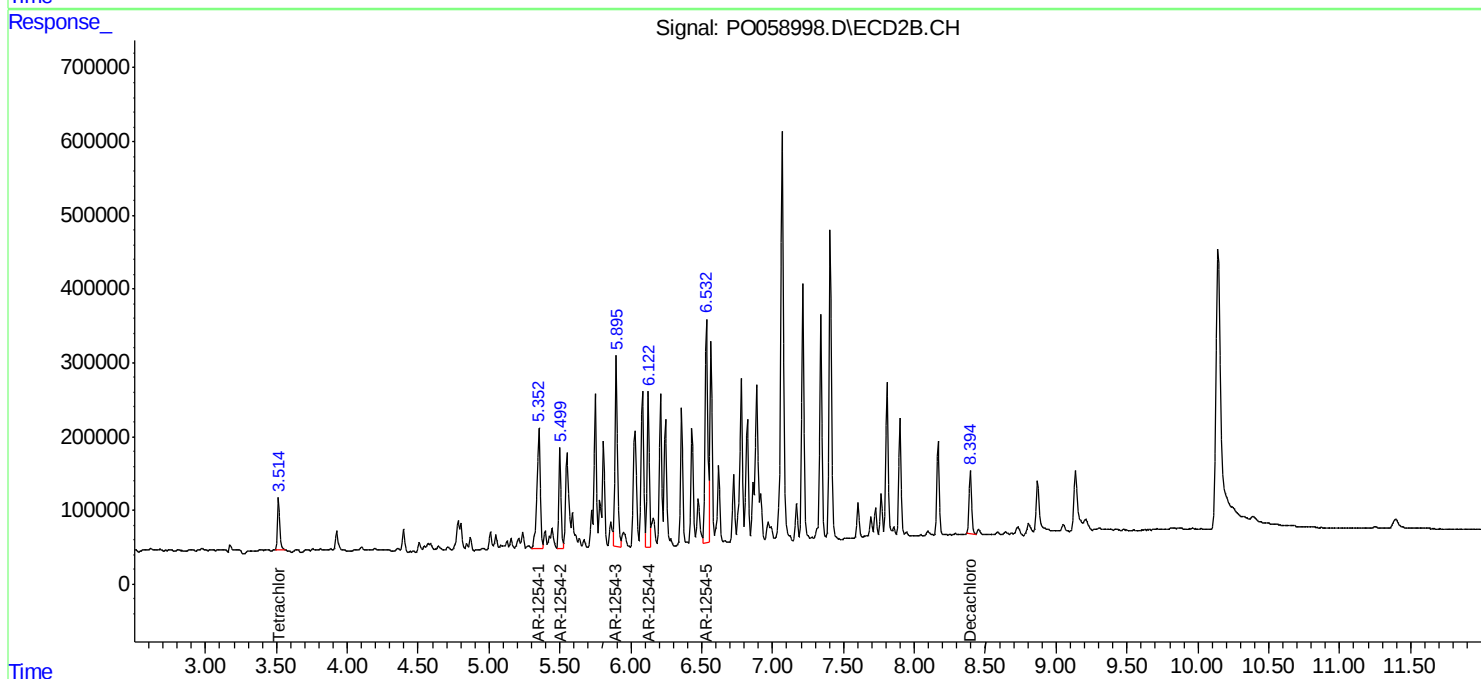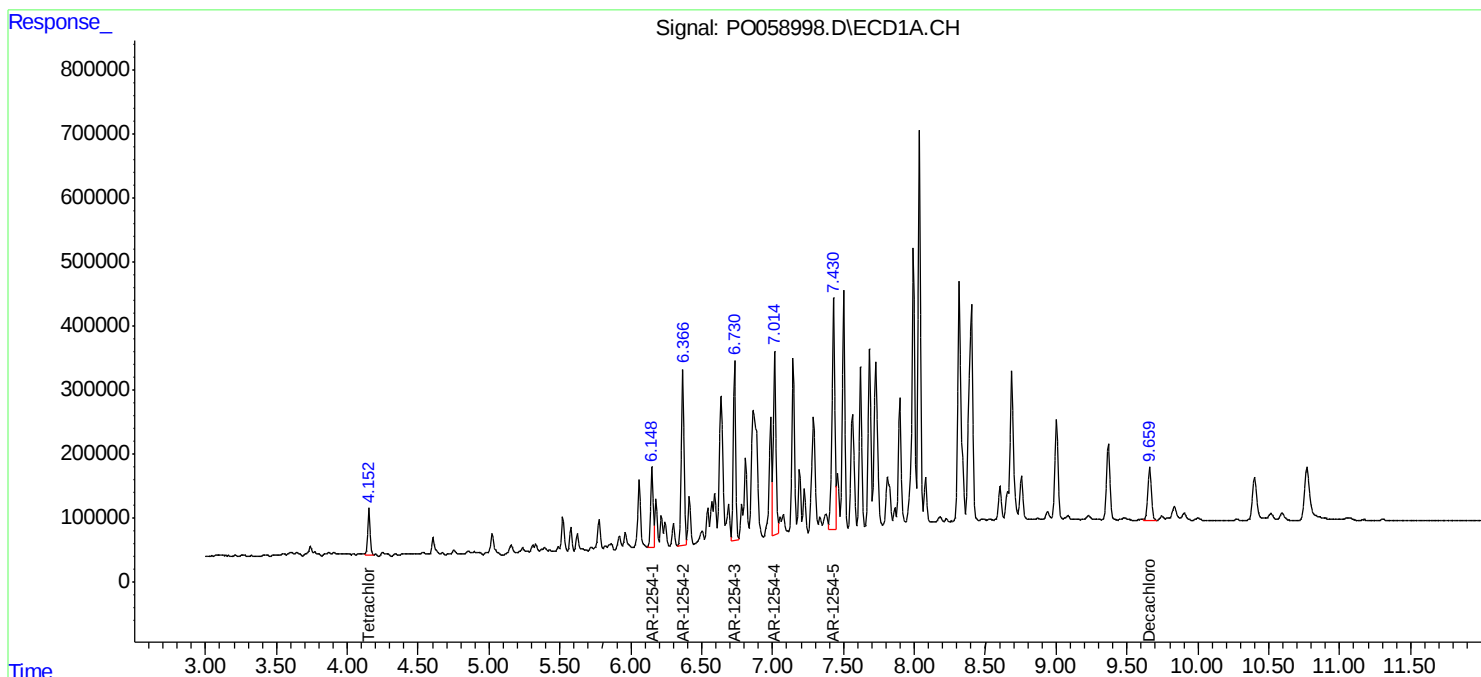

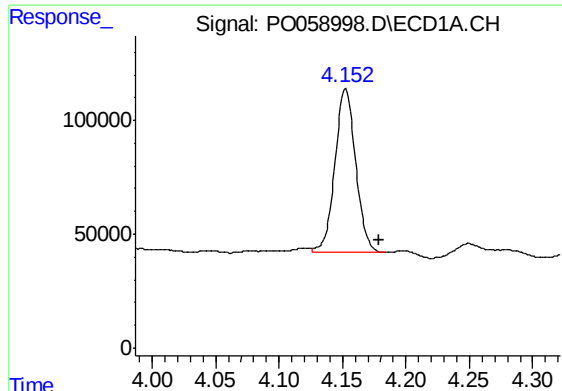


#1 Tetrachloro-m-xylene

R.T.: 4.152 min
Delta R.T.: -0.027 min
Response: 821678
Conc: 19.47 ng/ml m

Instrument :
ECD_O
ClientSampleId :
VW-PAINT-CHIPS


Manual Integrations
APPROVED

Ankita
8/8/2019 2:47:26 PM

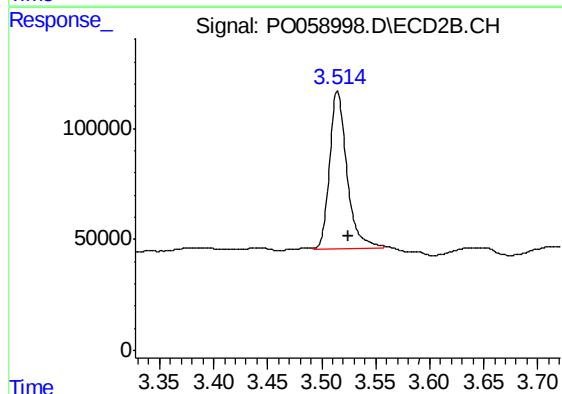


#1 Tetrachloro-m-xylene

R.T.: 3.514 min
Delta R.T.: -0.011 min
Response: 786289
Conc: 19.68 ng/ml m

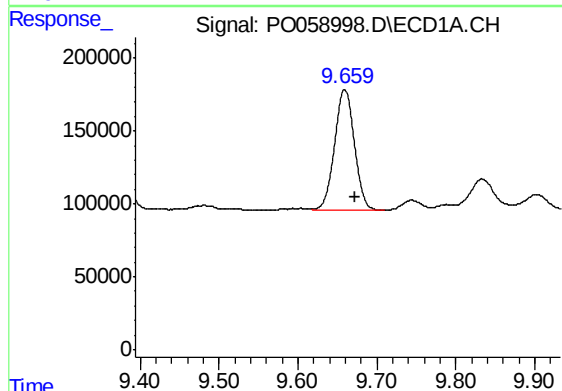


#2 Decachlorobiphenyl

R.T.: 9.659 min
Delta R.T.: -0.013 min
Response: 1447253
Conc: 26.72 ng/ml

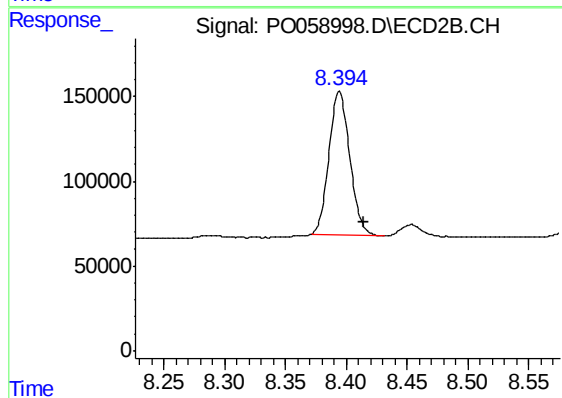

#2 Decachlorobiphenyl

R.T.: 8.394 min
Delta R.T.: -0.020 min
Response: 1010465
Conc: 25.60 ng/ml

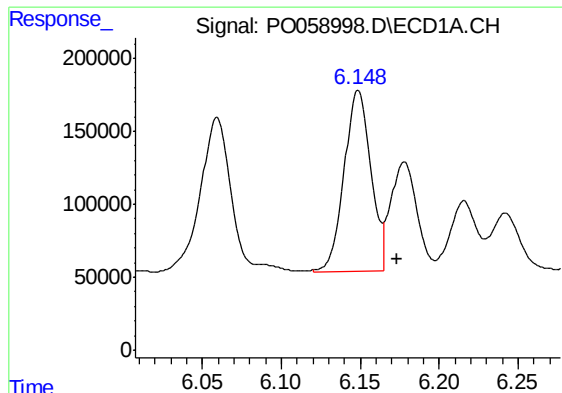


#26 AR-1254-1

R.T.: 6.148 min
Delta R.T.: -0.025 min
Response: 1460300
Conc: 618.43 ng/ml m

Instrument :
ECD_O
ClientSampleId :
VW-PAINT-CHIPS


Manual Integrations
APPROVED

Ankita
8/8/2019 2:47:26 PM

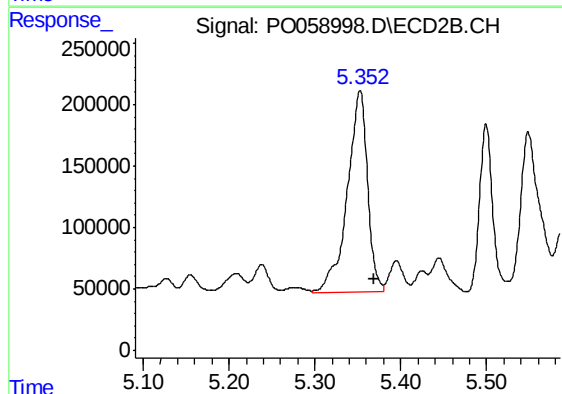


#26 AR-1254-1

R.T.: 5.353 min
Delta R.T.: -0.016 min
Response: 2684357
Conc: 1036.22 ng/ml

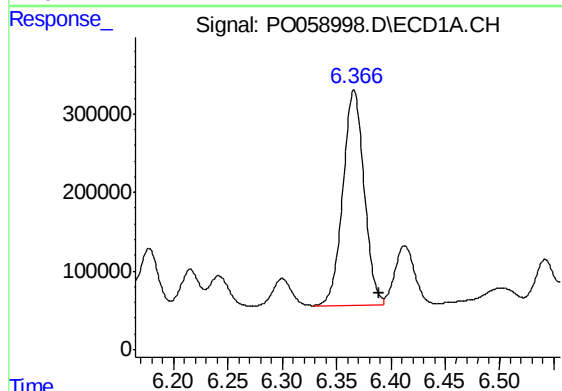


#27 AR-1254-2

R.T.: 6.366 min
Delta R.T.: -0.023 min
Response: 3713001
Conc: 963.43 ng/ml

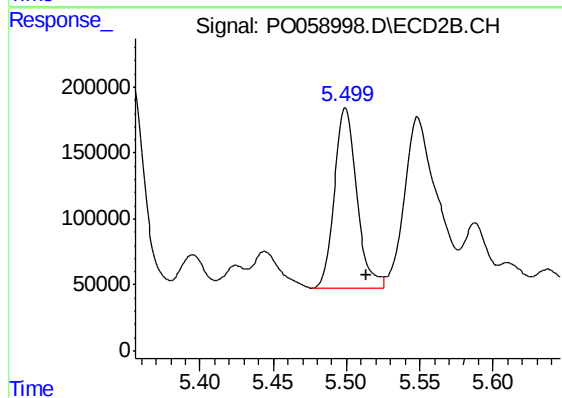

#27 AR-1254-2

R.T.: 5.499 min
Delta R.T.: -0.014 min
Response: 1443317
Conc: 630.43 ng/ml

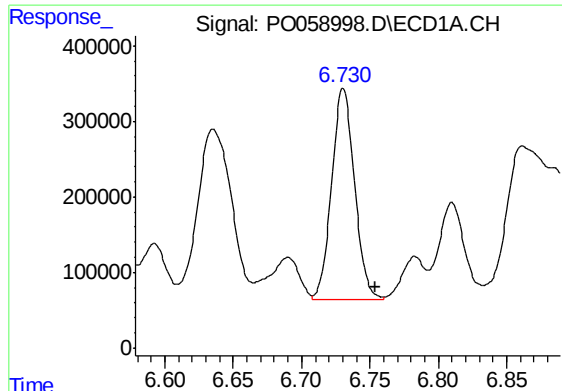


#28 AR-1254-3

R.T.: 6.730 min
Delta R.T.: -0.023 min
Response: 3272770
Conc: 808.16 ng/ml

Instrument :
ECD_O
ClientSampleId :
VW-PAINT-CHIPS


Manual Integrations
APPROVED

Ankita
8/8/2019 2:47:26 PM

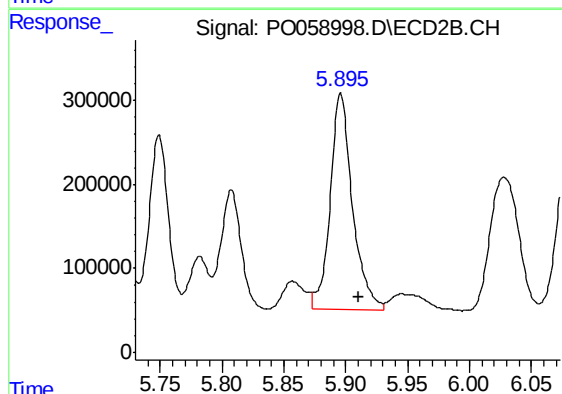


#28 AR-1254-3

R.T.: 5.896 min
Delta R.T.: -0.015 min
Response: 3233255
Conc: 878.75 ng/ml

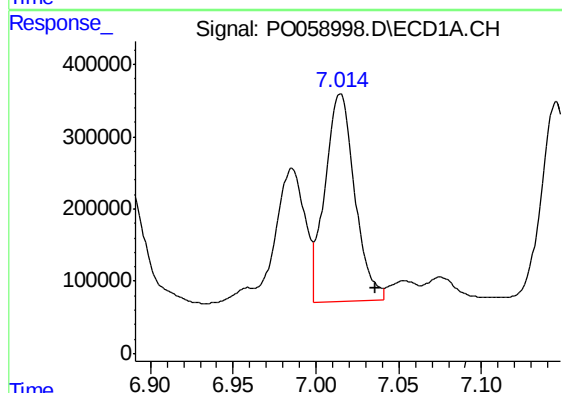


#29 AR-1254-4

R.T.: 7.014 min
Delta R.T.: -0.022 min
Response: 3594536
Conc: 998.30 ng/ml m

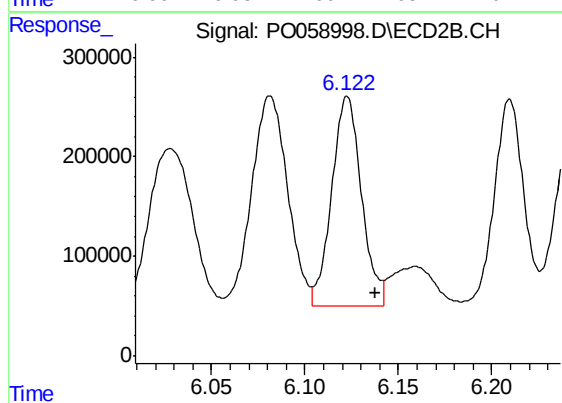

#29 AR-1254-4

R.T.: 6.123 min
Delta R.T.: -0.015 min
Response: 2325604
Conc: 1000.17 ng/ml

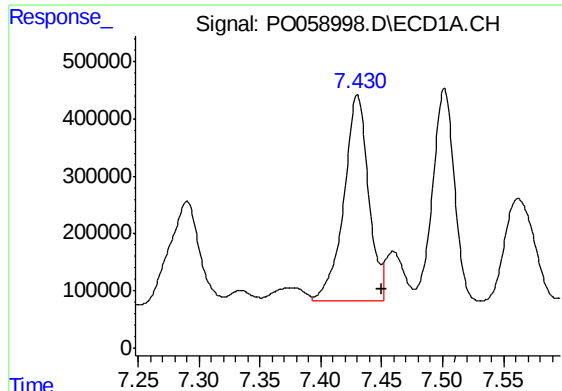


#30 AR-1254-5

R.T.: 7.430 min
Delta R.T.: -0.021 min
Response: 5129716
Conc: 1415.19 ng/ml m

Instrument :
ECD_O
ClientSampleId :
VW-PAINT-CHIPS

Manual Integrations
APPROVED

Ankita
8/8/2019 2:47:26 PM

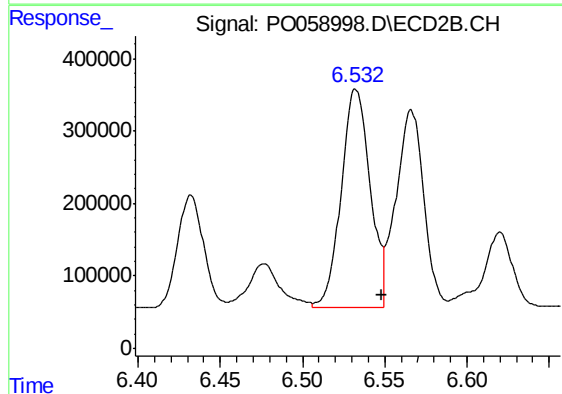

#30 AR-1254-5

R.T.: 6.532 min
Delta R.T.: -0.016 min
Response: 3701990
Conc: 1073.18 ng/ml