

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080719\
 Data File : P0059006.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 Aug 2019 22:02
 Operator : SM/SJ
 Sample : PB122062BL
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB122062BL

Manual Integrations
 APPROVED

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 08 08:26:00 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072819.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jul 27 06:49:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.153	3.516	855060	773789	20.261m	19.369
2) SA Decachlor...	9.659	8.395	1205248	875998	22.255	22.192m

Ankita

8/8/2019 2:47:42 PM

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.



Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO080719\
Data File : PO059006.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Aug 2019 22:02
Operator : SM/SJ
Sample : PB122062BL
Misc :
ALS Vial : 30 Sample Multiplier: 1


Instrument :
ECD_O
ClientSampleId :
PB122062BL

Manual Integrations
APPROVED

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 08 08:26:00 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO072819.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jul 27 06:49:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

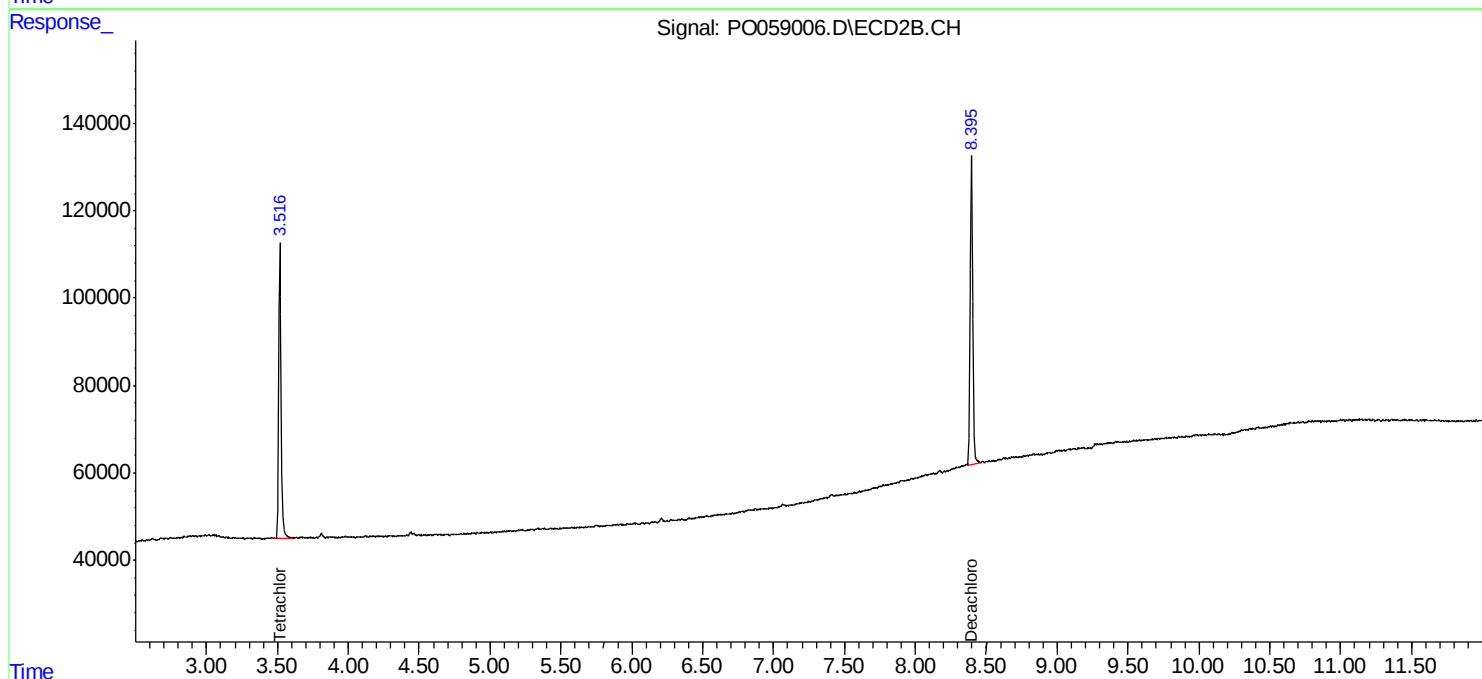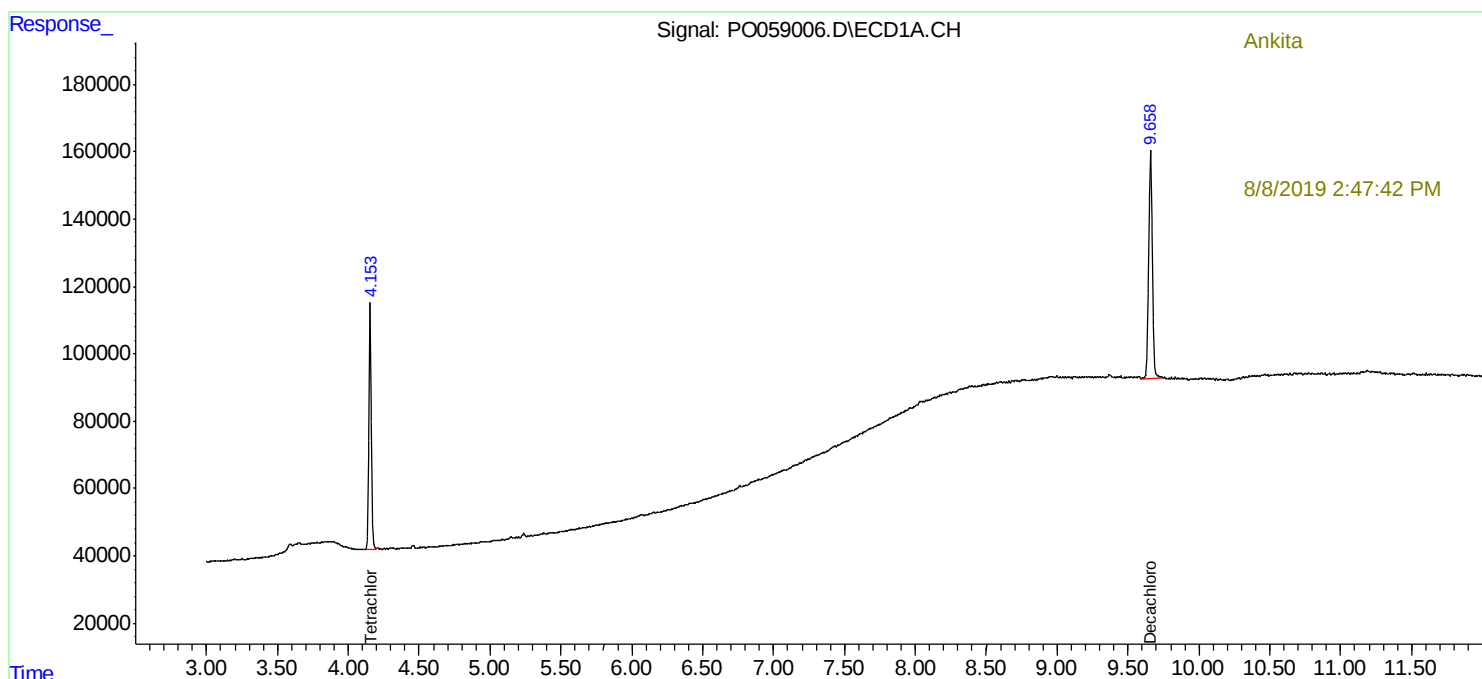

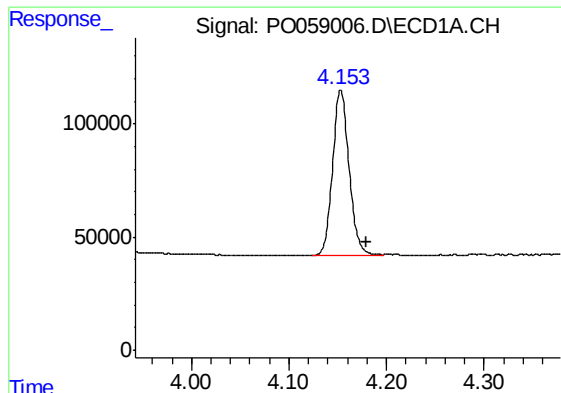


#1 Tetrachloro-m-xylene

R.T.: 4.153 min
Delta R.T.: -0.026 min
Response: 855060
Conc: 20.26 ng/ml m

Instrument :
ECD_O
ClientSampleId :
PB122062BL


Manual Integrations
APPROVED

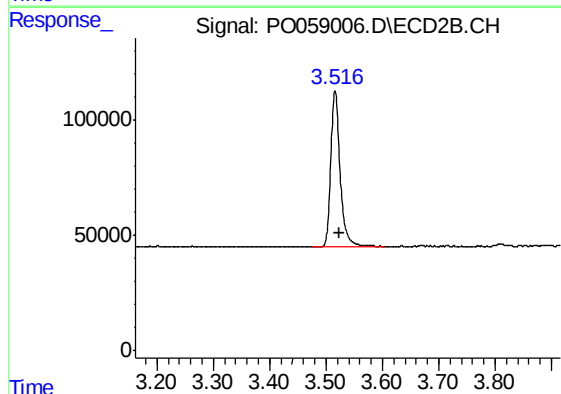

#1 Tetrachloro-m-xylene

R.T.: 3.516 min
Delta R.T.: -0.009 min
Response: 773789
Conc: 19.37 ng/ml


Ankita

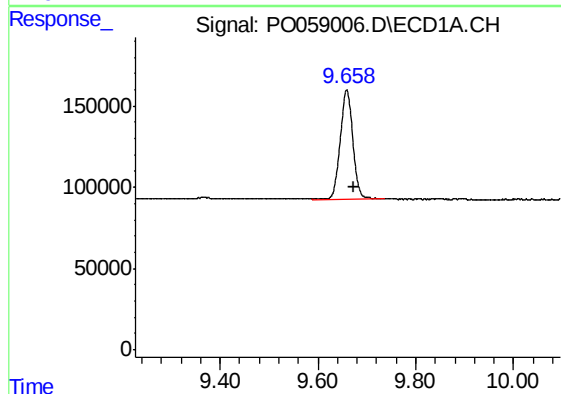

#2 Decachlorobiphenyl

R.T.: 9.659 min
Delta R.T.: -0.014 min
Response: 1205248
Conc: 22.26 ng/ml

8/8/2019 2:47:42 PM

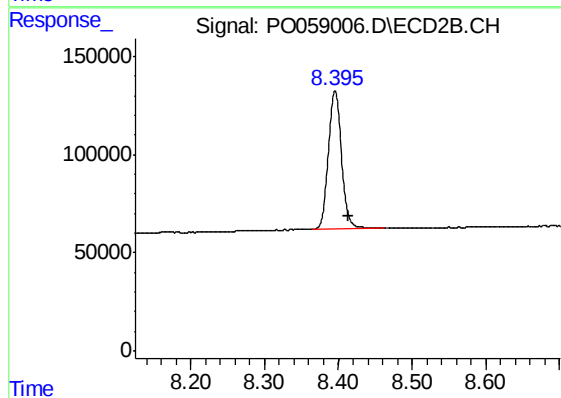

#2 Decachlorobiphenyl

R.T.: 8.395 min
Delta R.T.: -0.019 min
Response: 875998
Conc: 22.19 ng/ml m