Quantitation Report (QT Reviewed)

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO080719\
Data File : PO059019.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Aug 2019 2:04
Operator : SM/SJ
Sample : K4208-02
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
SB-02(0-2)

Manual Integrations APPROVED
Ankita
8/8/2019 2:48:17 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 08 08:34:22 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO072819.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jul 27 06:49:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
	System Monitoring Compounds						
1)	SA Tetrachlo...	4.152	3.515	758151	677382	17.964	16.956
2)	SA Decachlor...	9.658	8.394	800496	598169	14.781	15.154m
	Target Compounds						

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Quantitation Report (QT Reviewed)

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO080719\
Data File : PO059019.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Aug 2019 2:04
Operator : SM/SJ
Sample : K4208-02
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
SB-02(0-2)

Manual Integrations APPROVED
Ankita
8/8/2019 2:48:17 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 08 08:34:22 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO072819.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jul 27 06:49:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

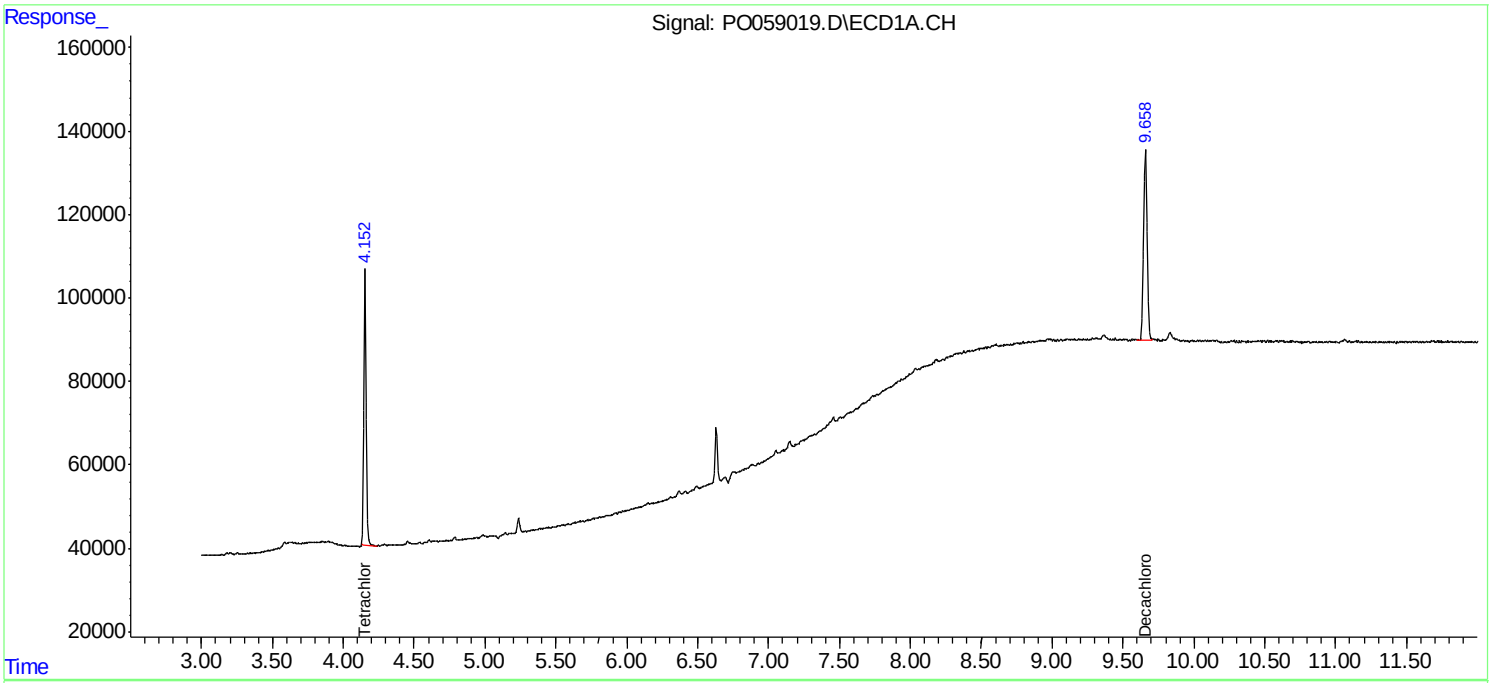

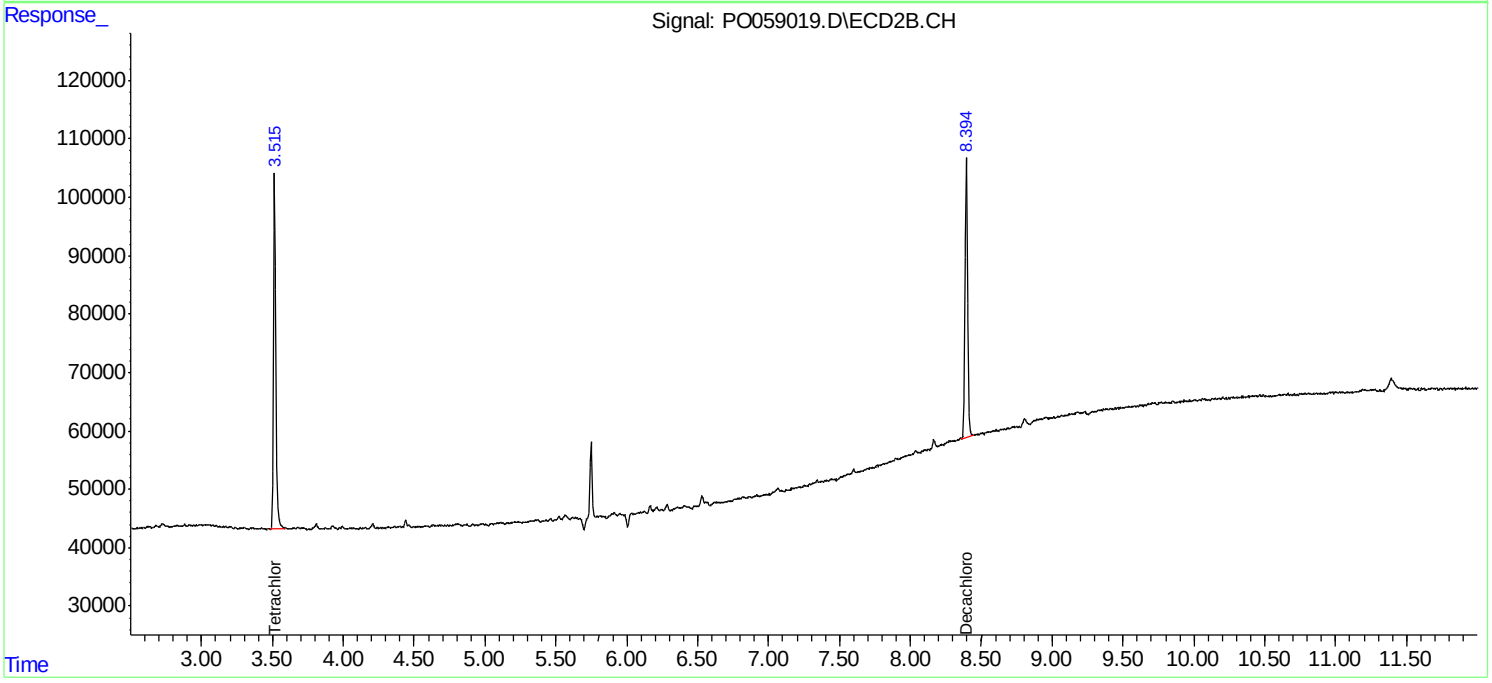

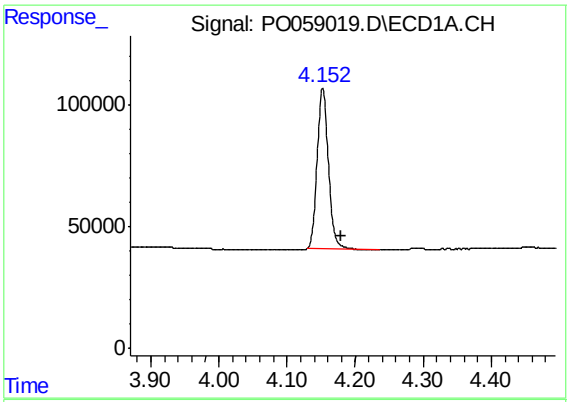

#1 Tetrachloro-m-xylene

R.T.: 4.152 min
Delta R.T.: -0.027 min
Response: 758151
Conc: 17.96 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-02(0-2)

Manual Integrations APPROVED
Ankita
8/8/2019 2:48:17 PM

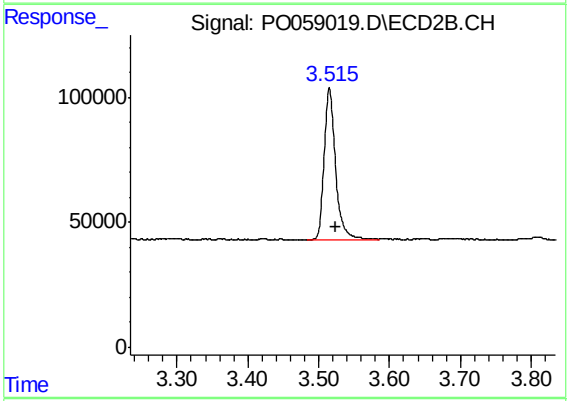

#1 Tetrachloro-m-xylene

R.T.: 3.515 min
Delta R.T.: -0.010 min
Response: 677382
Conc: 16.96 ng/ml

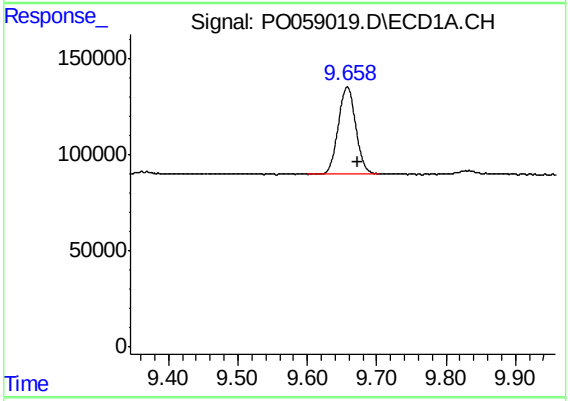

#2 Decachlorobiphenyl

R.T.: 9.658 min
Delta R.T.: -0.015 min
Response: 800496
Conc: 14.78 ng/ml

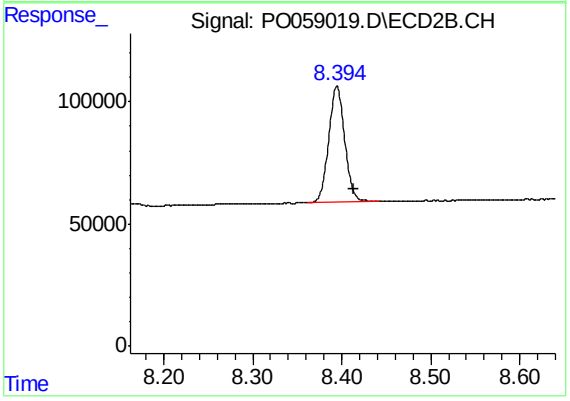

#2 Decachlorobiphenyl

R.T.: 8.394 min
Delta R.T.: -0.020 min
Response: 598169
Conc: 15.15 ng/ml m