

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080720\
 Data File : P0070379.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 Aug 2020 11:31
 Operator : DD\AJ
 Sample : L3563-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 NB-30860

Manual Integrations
 APPROVED

Ankita
 8/10/2020 1:22:35 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 08 04:36:52 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0080620.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Aug 06 13:04:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.377	3.564	1372065	1099195	20.749	24.948
2) SA Decachlor...	10.042f	8.791f	1576438	908584	18.411m	16.368m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO080720\
Data File : PO070379.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Aug 2020 11:31
Operator : DD\AJ
Sample : L3563-01
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
NB-30860


Manual Integrations
APPROVED

Ankita
8/10/2020 1:22:35 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 08 04:36:52 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO080620.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Aug 06 13:04:06 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

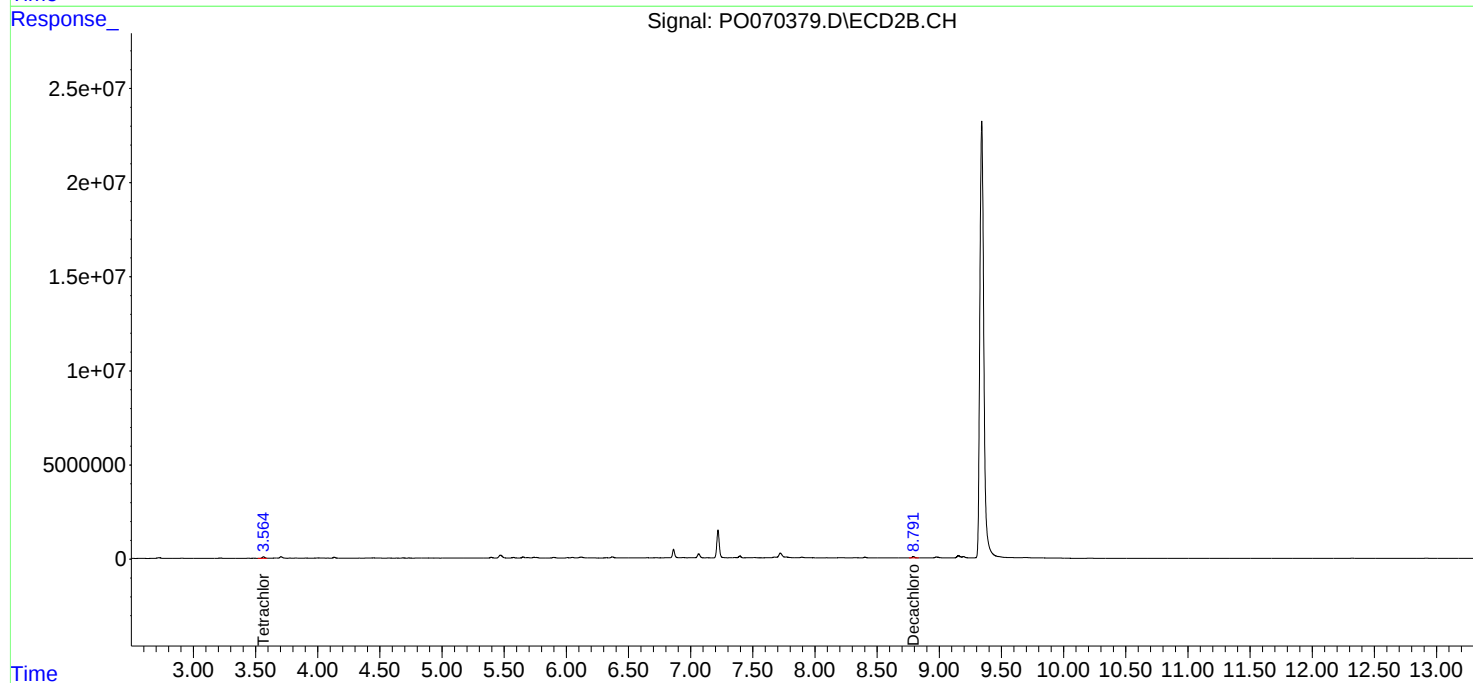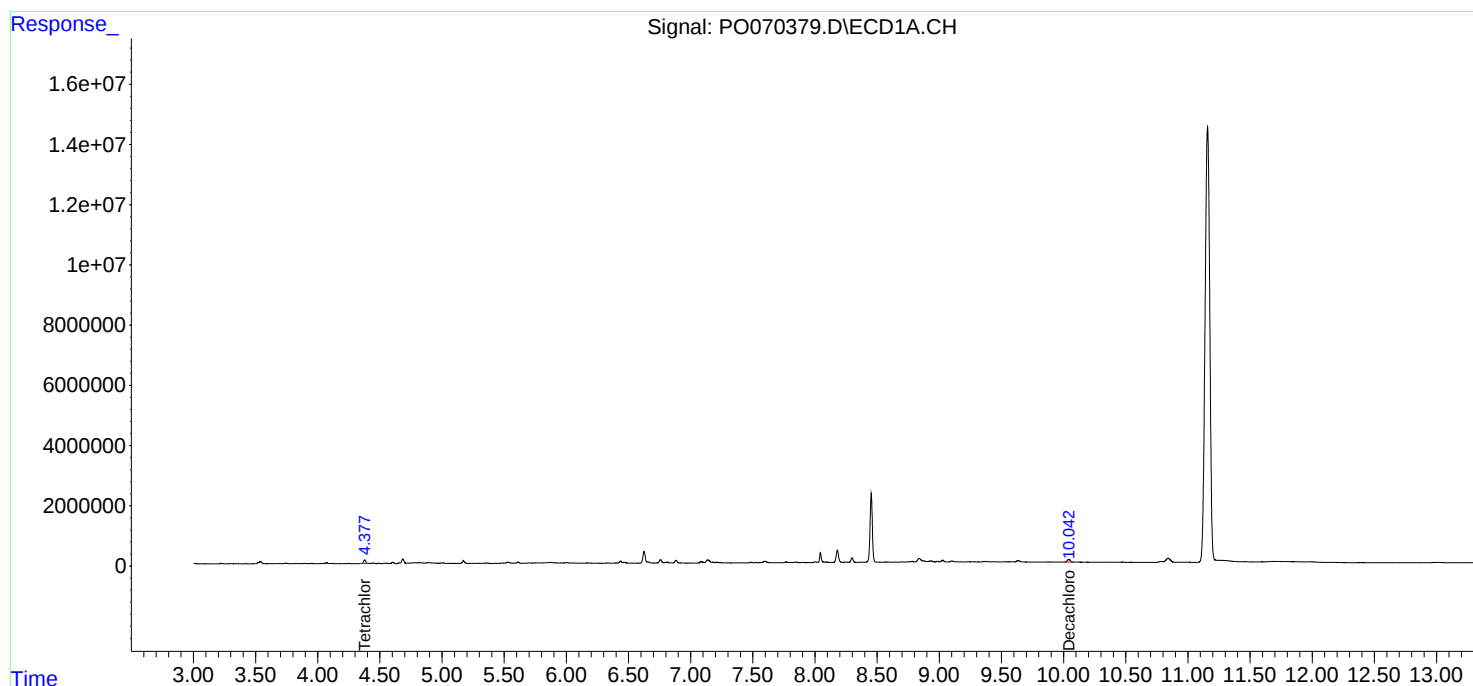

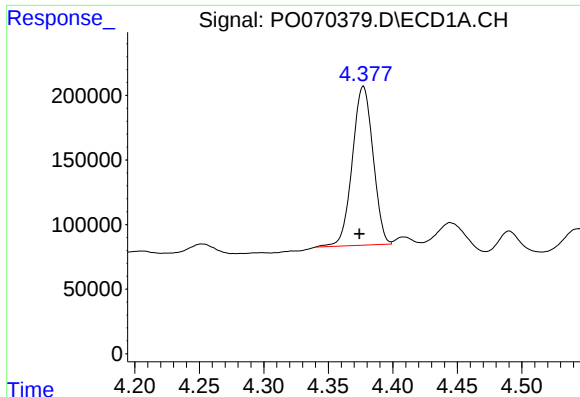


#1 Tetrachloro-m-xylene

R.T.: 4.377 min
Delta R.T.: 0.003 min
Response: 1372065
Conc: 20.75 ng/ml

Instrument :
ECD_O
ClientSampleId :
NB-30860


Manual Integrations
APPROVED

Ankita
8/10/2020 1:22:35 PM

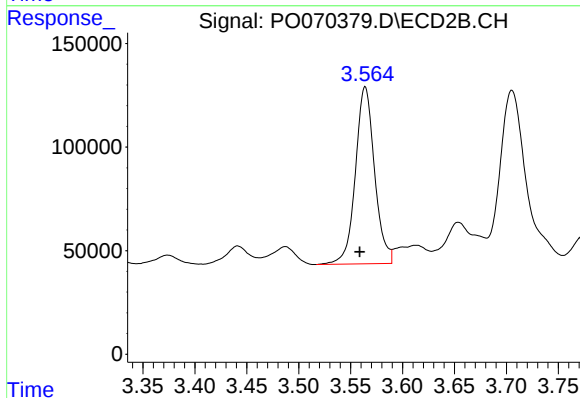


#1 Tetrachloro-m-xylene

R.T.: 3.564 min
Delta R.T.: 0.005 min
Response: 1099195
Conc: 24.95 ng/ml

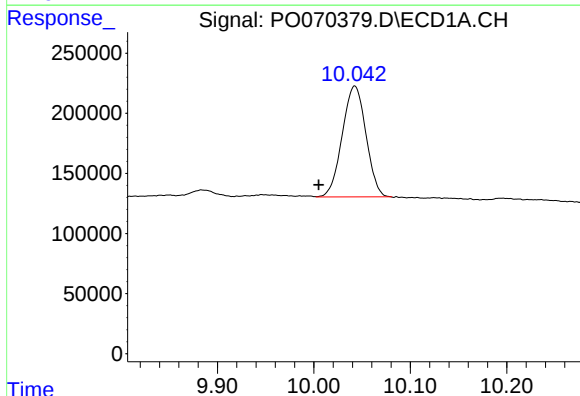

#2 Decachlorobiphenyl

R.T.: 10.042 min
Delta R.T.: 0.037 min
Response: 1576438
Conc: 18.41 ng/ml m

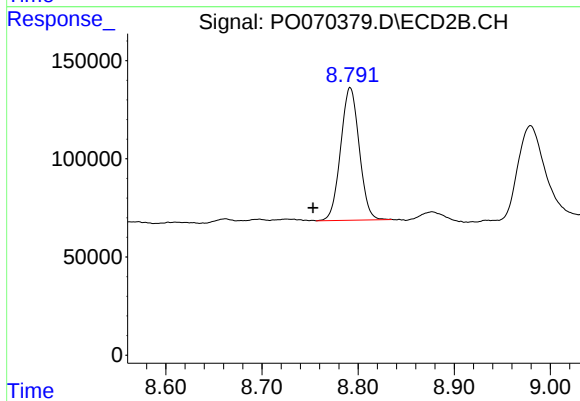

#2 Decachlorobiphenyl

R.T.: 8.791 min
Delta R.T.: 0.038 min
Response: 908584
Conc: 16.37 ng/ml m