

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080720\
 Data File : P0070390.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 Aug 2020 14:38
 Operator : DD\AJ
 Sample : L3597-01
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 20200446-CORE-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 08 04:41:16 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0080620.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Aug 06 13:04:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.373	3.558	1273040	746386	19.252	16.940
2)	SA Decachlor...	10.002	8.750	1107205	706605	12.931	12.730

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080720\
Data File : P0070390.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Aug 2020 14:38
Operator : DD\AJ
Sample : L3597-01
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
20200446-CORE-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 08 04:41:16 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0080620.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Aug 06 13:04:06 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

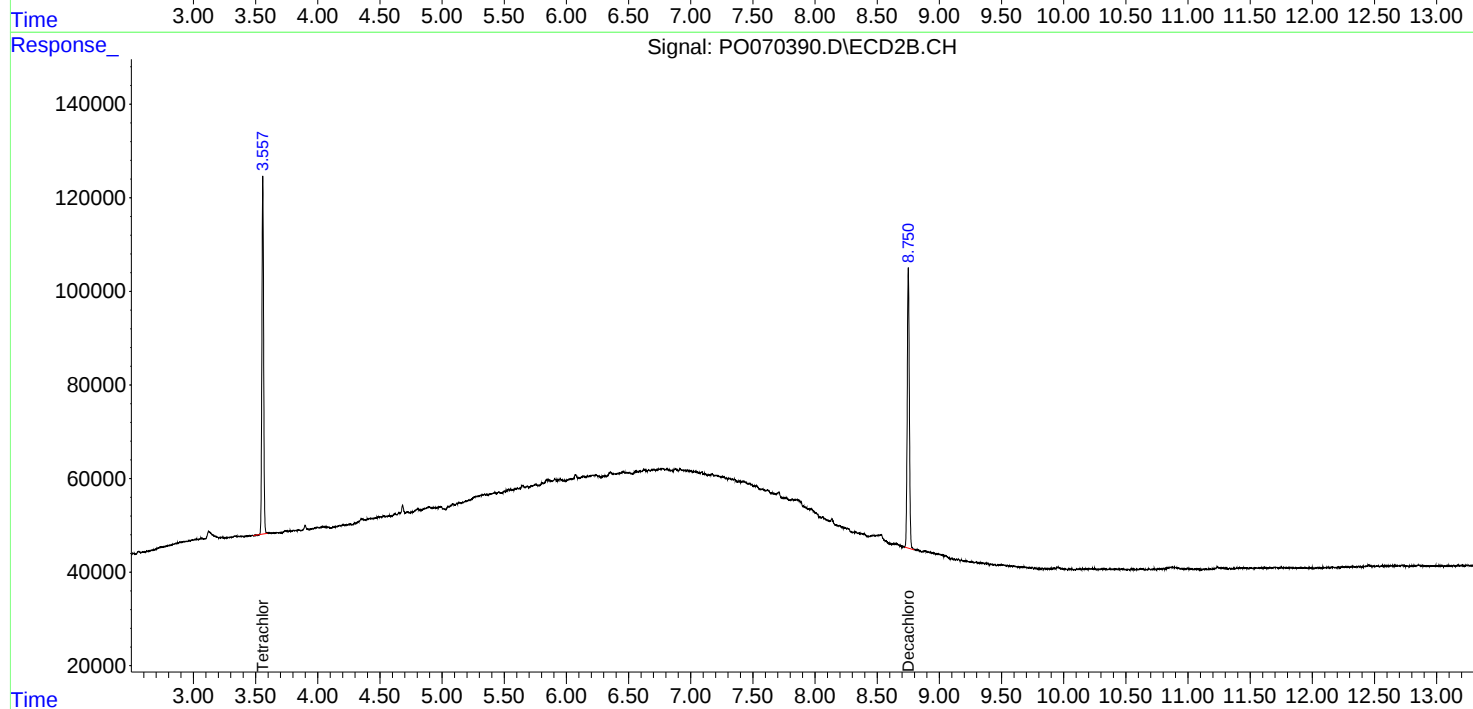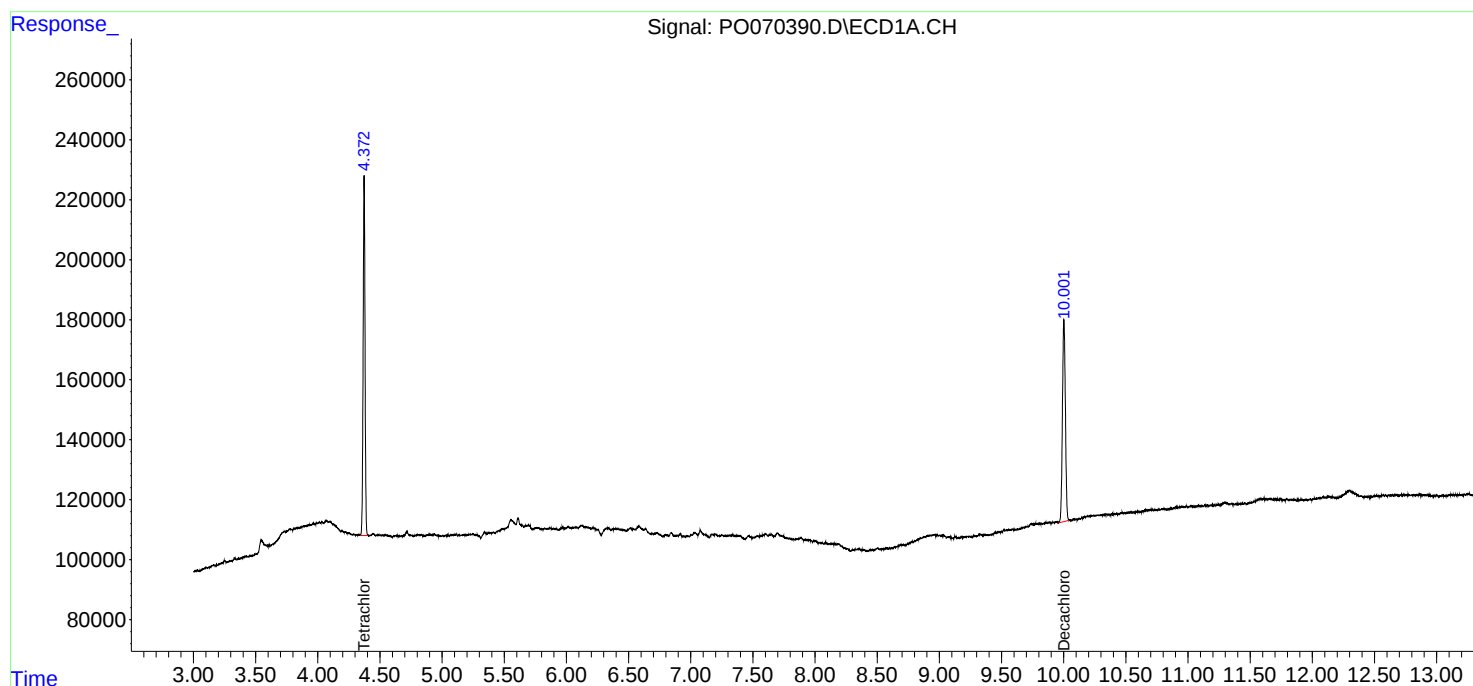


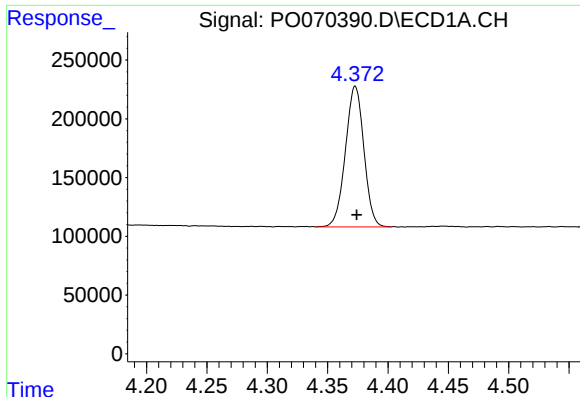

#1 Tetrachloro-m-xylene


R.T.: 4.373 min
Delta R.T.: -0.001 min
Response: 1273040
Conc: 19.25 ng/ml

Instrument :
ECD_O
ClientSampleId :
20200446-CORE-2

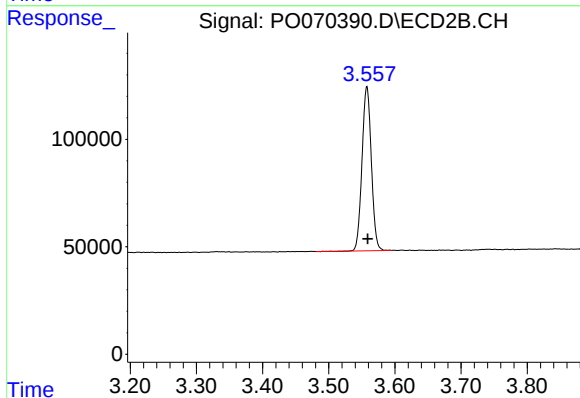


#1 Tetrachloro-m-xylene

R.T.: 3.558 min
Delta R.T.: -0.001 min
Response: 746386
Conc: 16.94 ng/ml

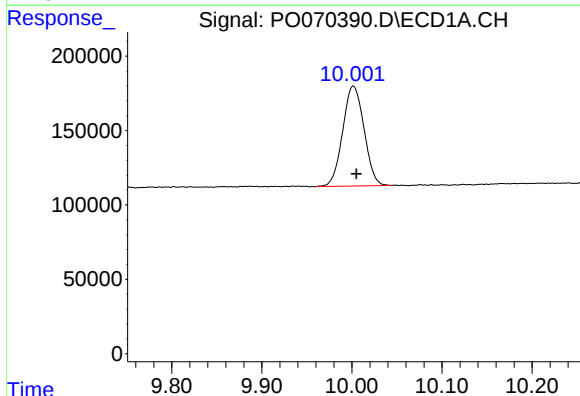

#2 Decachlorobiphenyl

R.T.: 10.002 min
Delta R.T.: -0.003 min
Response: 1107205
Conc: 12.93 ng/ml

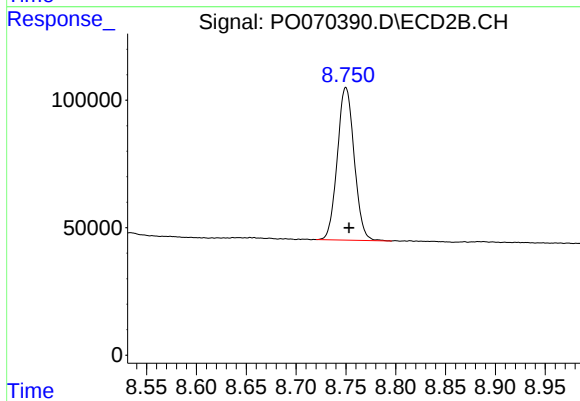

#2 Decachlorobiphenyl

R.T.: 8.750 min
Delta R.T.: -0.003 min
Response: 706605
Conc: 12.73 ng/ml