

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080723\
 Data File : P0096726.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Aug 2023 17:47
 Operator : YP/AJ
 Sample : AR1221ICC500
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1221ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 08 04:17:13 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0080723.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 08 04:11:26 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.407	3.621	170.0E6	64052333	50.000	50.000
2) SA Decachlor...	10.340	8.644	110.0E6	56949008	50.000	50.000
Target Compounds						
8) L2 AR-1221-1	4.618	3.835	20377534	8678527	500.000	500.000
9) L2 AR-1221-2	4.705	3.921	15189923	6460357	500.000	500.000
10) L2 AR-1221-3	4.782	3.997	43765798	19847014	500.000	500.000
36) L8 AR-1262-1	7.878	6.824	887840	224991	5.978	5.715
37) L8 AR-1262-2	8.433	0.000	277734	0	1.200	N.D. #
38) L8 AR-1262-3	8.770	7.534	481017	147237	2.884	2.294
39) L8 AR-1262-4	8.848	7.606	105270	88585	1.444	0.780 #
40) L8 AR-1262-5	9.537	0.000	166504	0	1.999	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO080723\
Data File : PO096726.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Aug 2023 17:47
Operator : YP/AJ
Sample : AR1221ICC500
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1221ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 08 04:17:13 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO080723.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 08 04:11:26 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

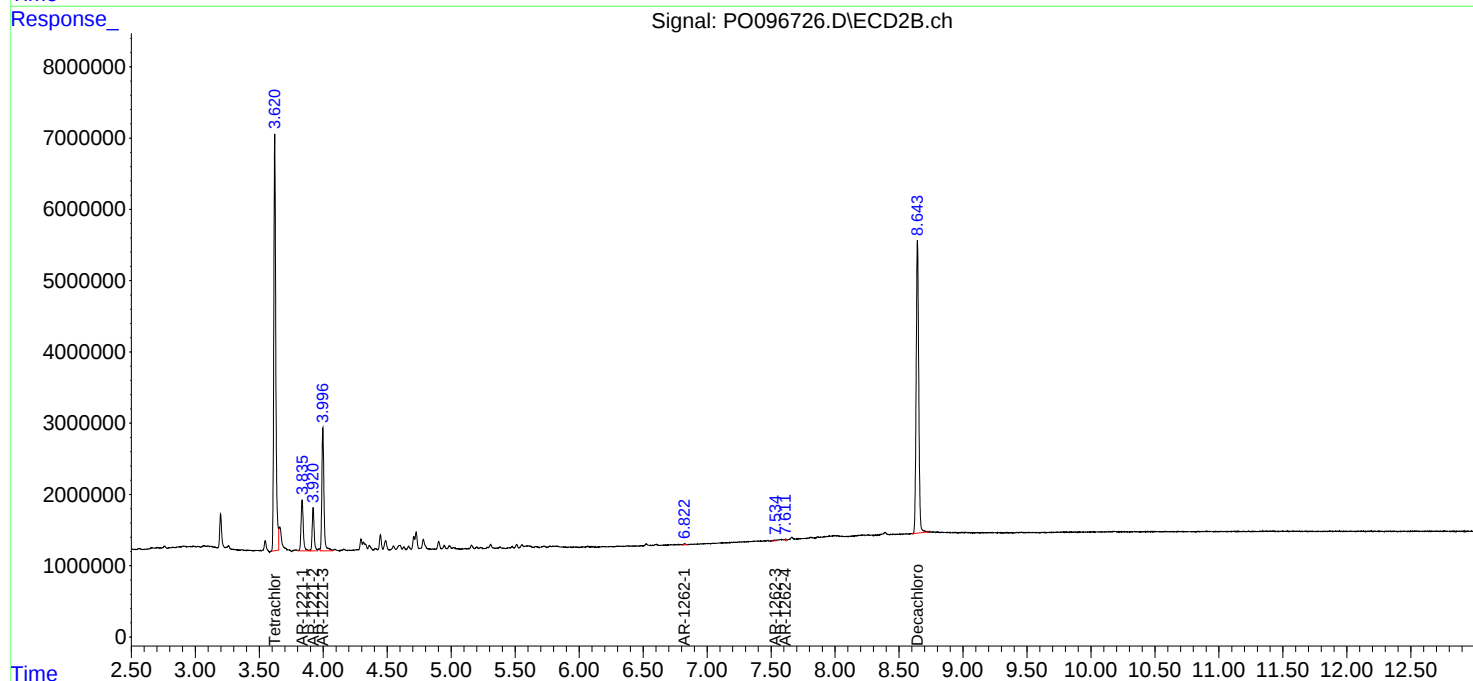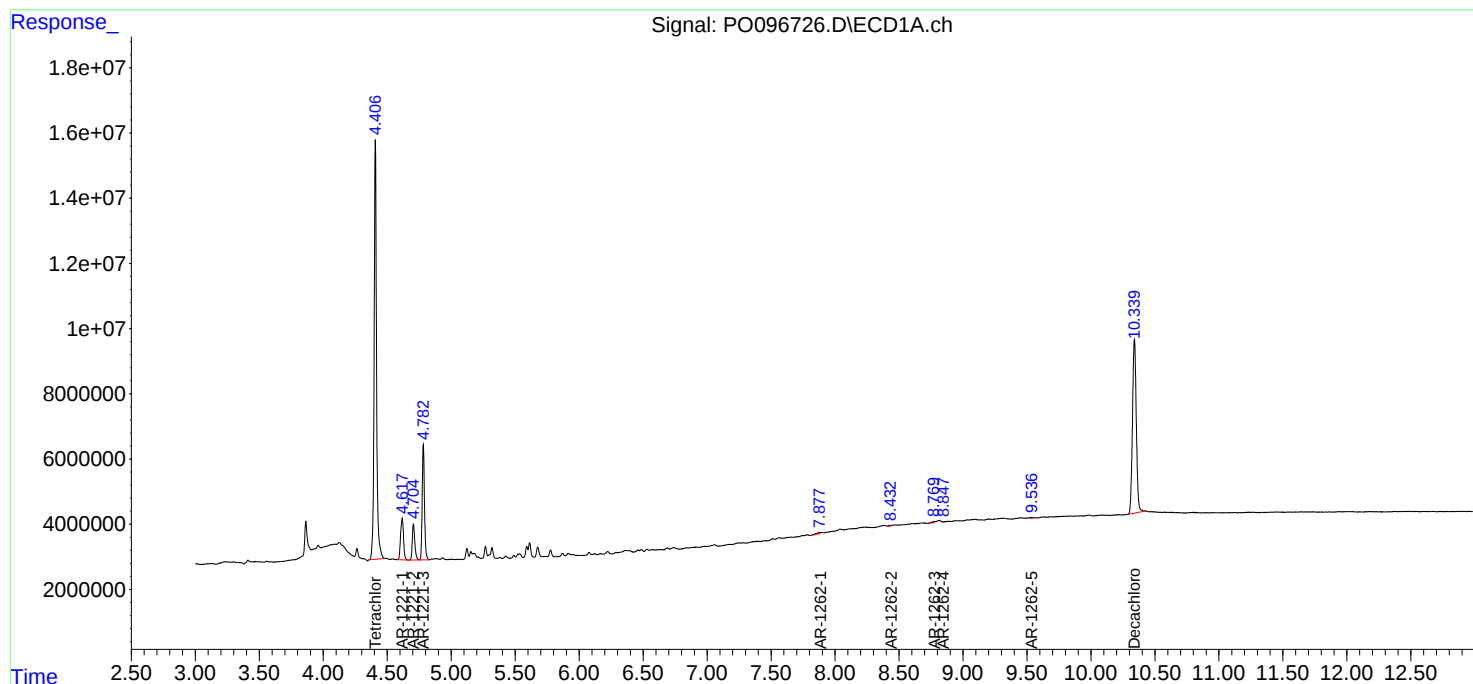


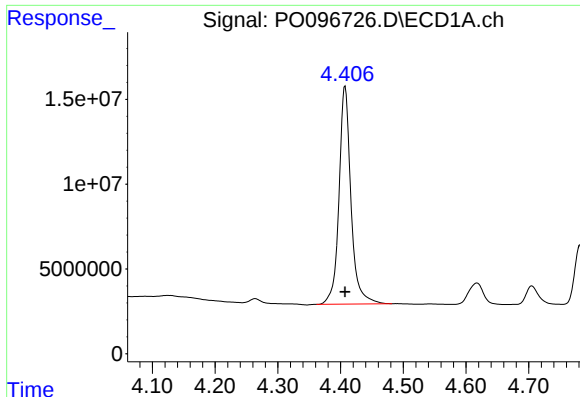

#1 Tetrachloro-m-xylene


R.T.: 4.407 min
Delta R.T.: 0.000 min
Response: 170019218
Conc: 50.00 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1221ICC500

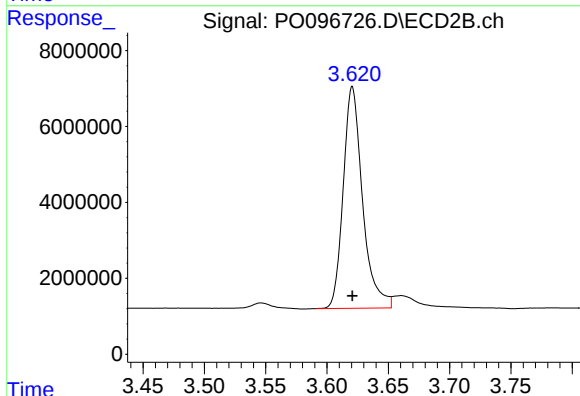


#1 Tetrachloro-m-xylene

R.T.: 3.621 min
Delta R.T.: 0.000 min
Response: 64052333
Conc: 50.00 ng/ml

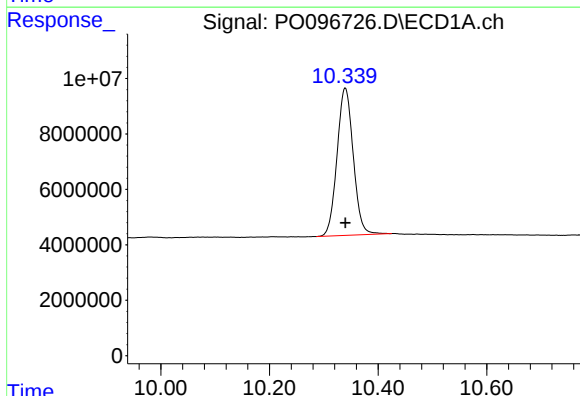


#2 Decachlorobiphenyl

R.T.: 10.340 min
Delta R.T.: 0.000 min
Response: 110015763
Conc: 50.00 ng/ml

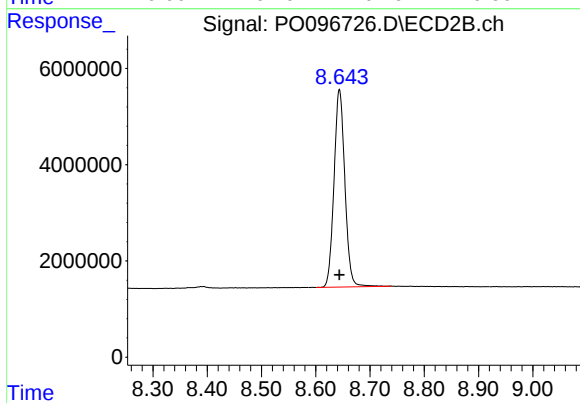

#2 Decachlorobiphenyl


R.T.: 8.644 min
Delta R.T.: 0.000 min
Response: 56949008
Conc: 50.00 ng/ml

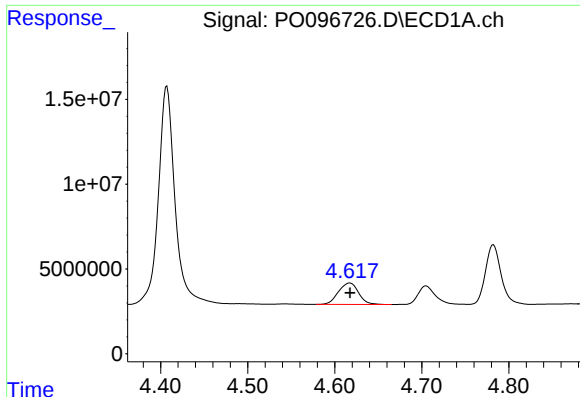

#8 AR-1221-1


R.T.: 4.618 min
Delta R.T.: 0.000 min
Response: 20377534
Conc: 500.00 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1221ICC500

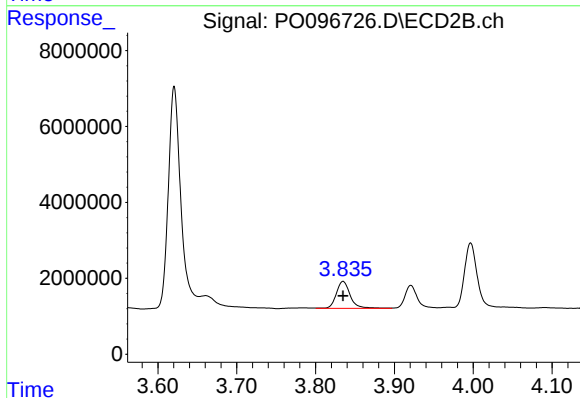


#8 AR-1221-1

R.T.: 3.835 min
Delta R.T.: 0.000 min
Response: 8678527
Conc: 500.00 ng/ml

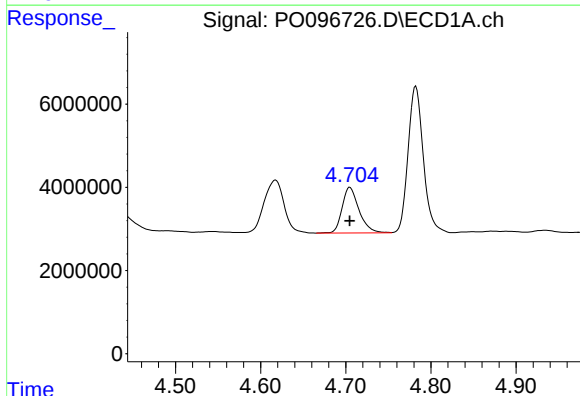


#9 AR-1221-2

R.T.: 4.705 min
Delta R.T.: 0.000 min
Response: 15189923
Conc: 500.00 ng/ml

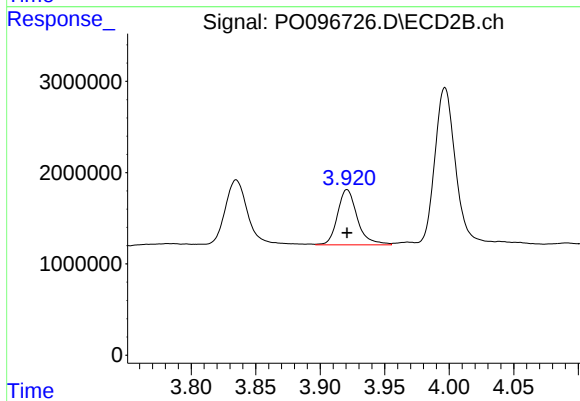

#9 AR-1221-2


R.T.: 3.921 min
Delta R.T.: 0.000 min
Response: 6460357
Conc: 500.00 ng/ml

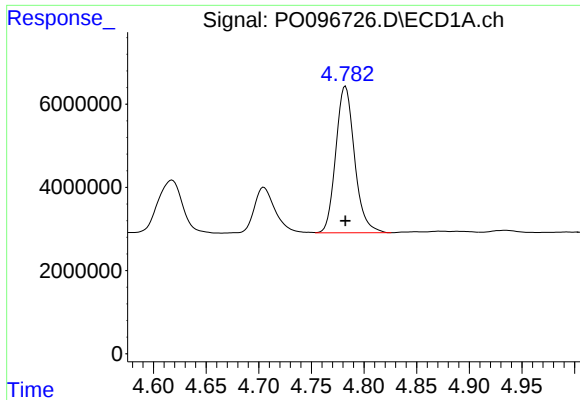

#10 AR-1221-3


R.T.: 4.782 min
Delta R.T.: 0.000 min
Response: 43765798
Conc: 500.00 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1221ICC500

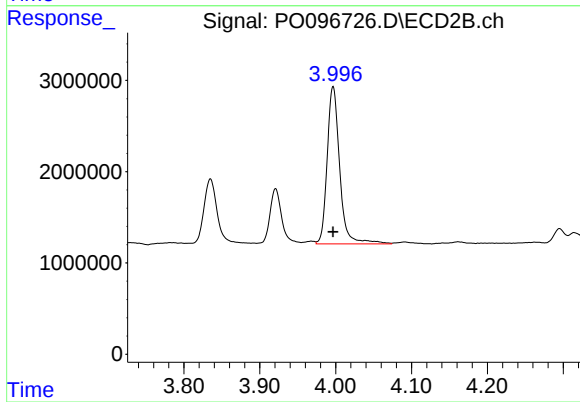


#10 AR-1221-3

R.T.: 3.997 min
Delta R.T.: 0.000 min
Response: 19847014
Conc: 500.00 ng/ml

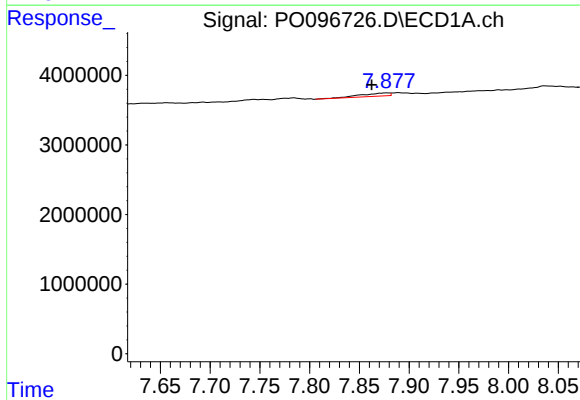


#36 AR-1262-1

R.T.: 7.878 min
Delta R.T.: 0.015 min
Response: 887840
Conc: 5.98 ng/ml

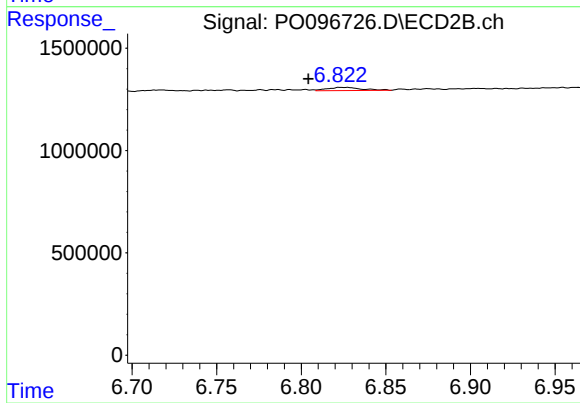

#36 AR-1262-1


R.T.: 6.824 min
Delta R.T.: 0.020 min
Response: 224991
Conc: 5.71 ng/ml

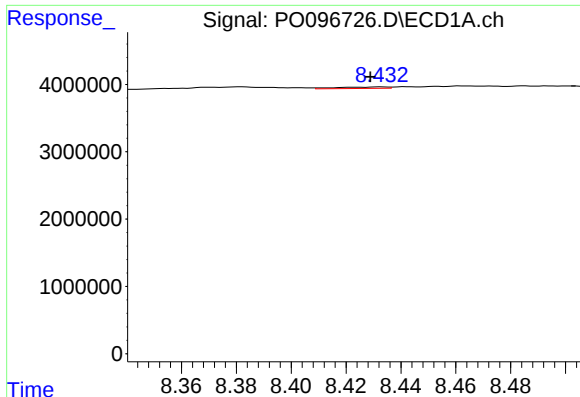

#37 AR-1262-2


R.T.: 8.433 min
Delta R.T.: 0.004 min
Response: 277734
Conc: 1.20 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1221ICC500

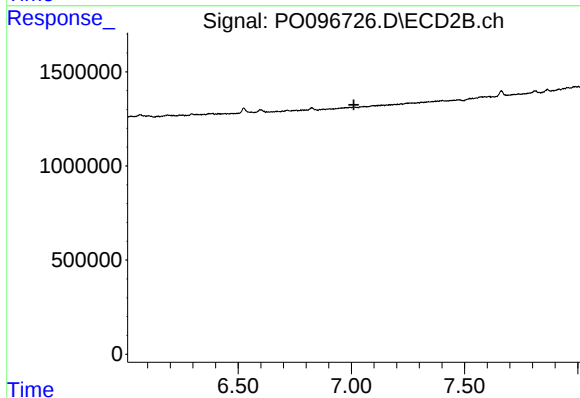


#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 7.011 min
Response: 0
Conc: N.D.

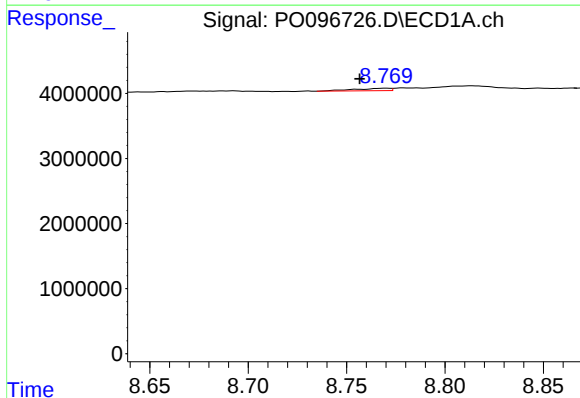


#38 AR-1262-3

R.T.: 8.770 min
Delta R.T.: 0.013 min
Response: 481017
Conc: 2.88 ng/ml

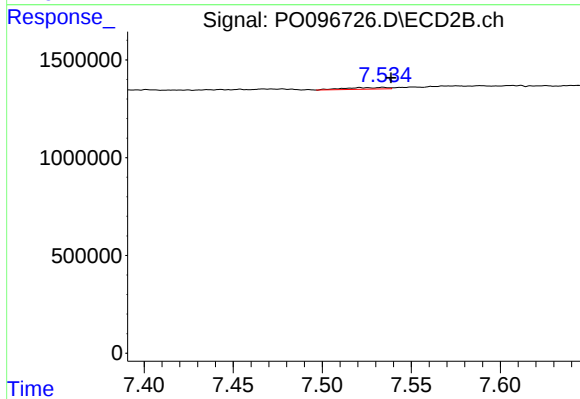

#38 AR-1262-3


R.T.: 7.534 min
Delta R.T.: -0.005 min
Response: 147237
Conc: 2.29 ng/ml

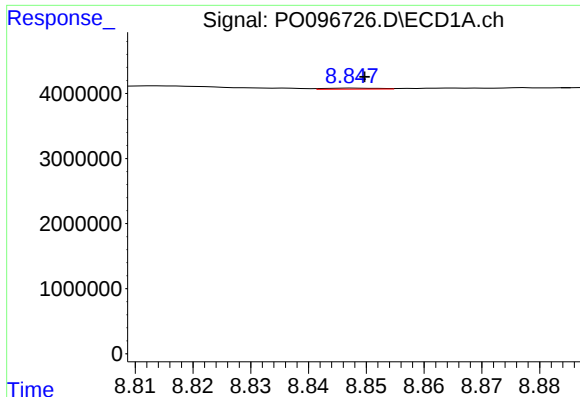

#39 AR-1262-4


R.T.: 8.848 min
Delta R.T.: -0.002 min
Response: 105270
Conc: 1.44 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1221ICC500

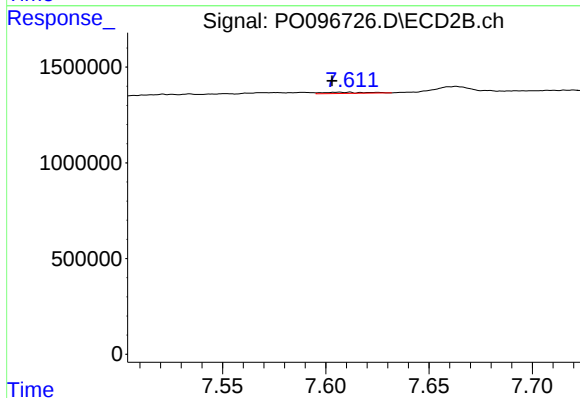


#39 AR-1262-4

R.T.: 7.606 min
Delta R.T.: 0.003 min
Response: 88585
Conc: 0.78 ng/ml

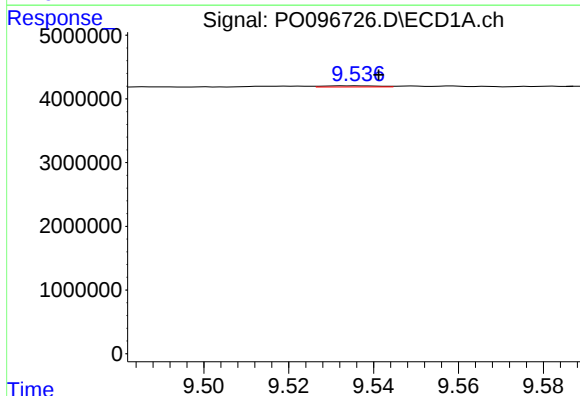

#40 AR-1262-5

R.T.: 9.537 min
Delta R.T.: -0.004 min
Response: 166504
Conc: 2.00 ng/ml

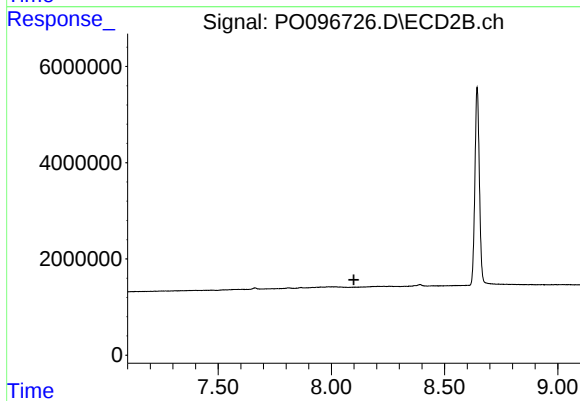

#40 AR-1262-5

R.T.: 0.000 min
Exp R.T. : 8.099 min
Response: 0
Conc: N.D.