

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080724\
 Data File : P0105267.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Aug 2024 18:39
 Operator : YP/AJ
 Sample : P3488-03
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 HD-02-080624

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/08/2024
 Supervised By :Ankita Jodhani 08/08/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 08 02:43:22 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072924.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 30 07:11:20 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.448	3.538	145.9E6	51626538	21.198m	20.261
2) SA Decachlor...	10.240	8.429	92797327	22207832	18.075m	13.980

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO080724\
Data File : PO105267.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Aug 2024 18:39
Operator : YP/AJ
Sample : P3488-03
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
HD-02-080624


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/08/2024
Supervised By :Ankita Jodhani 08/08/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 08 02:43:22 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO072924.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 30 07:11:20 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

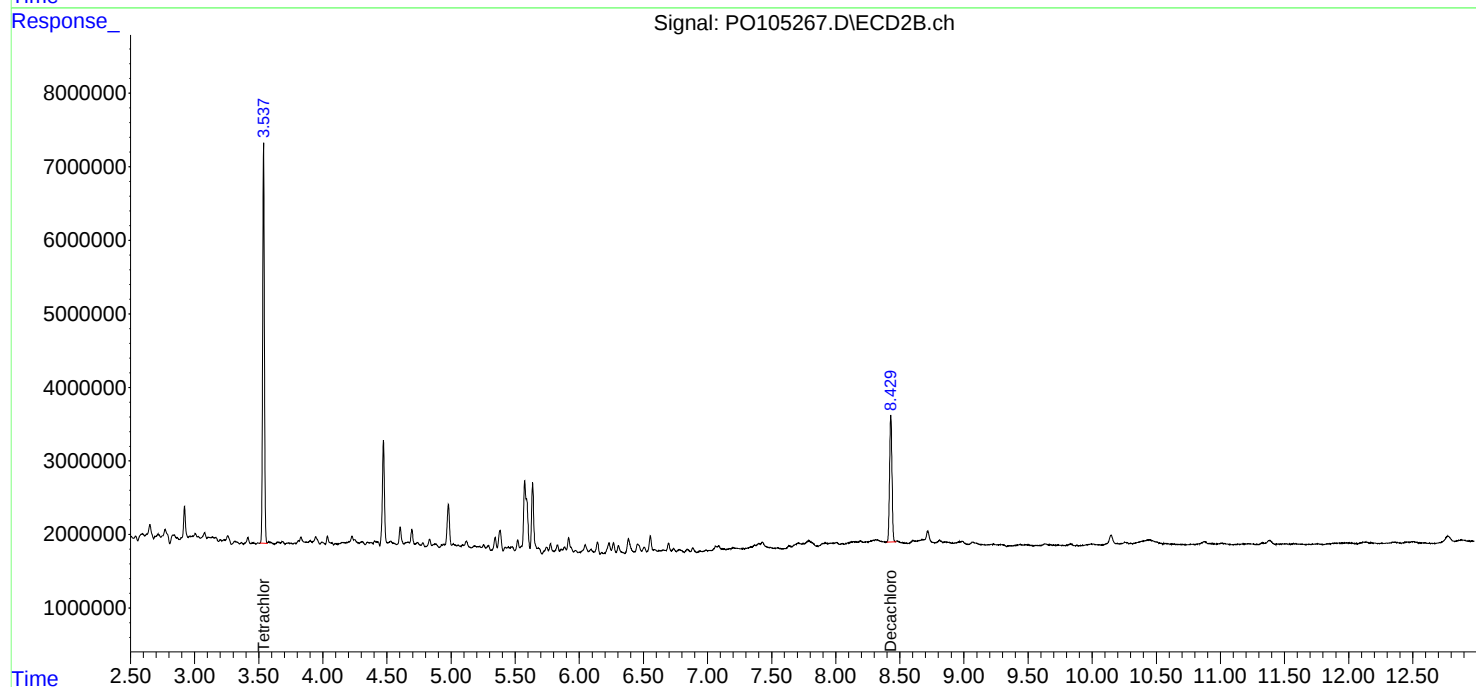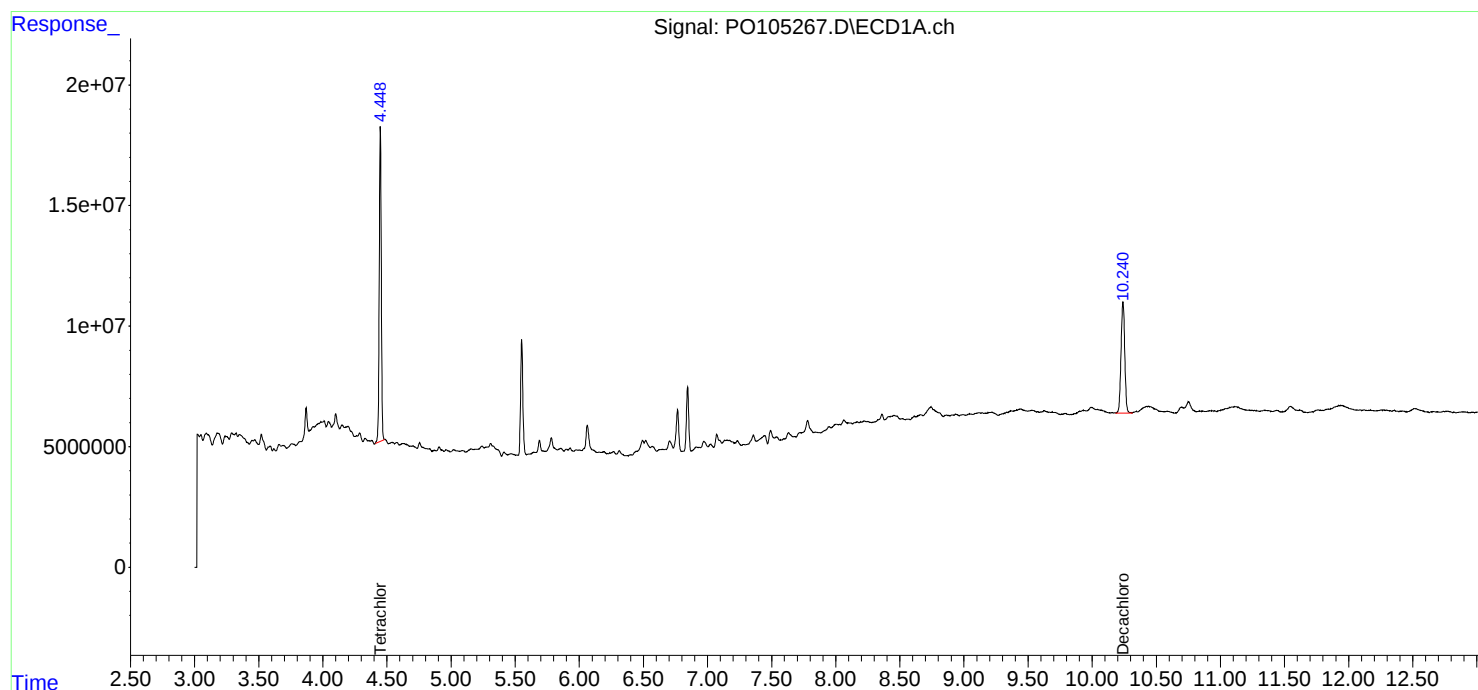

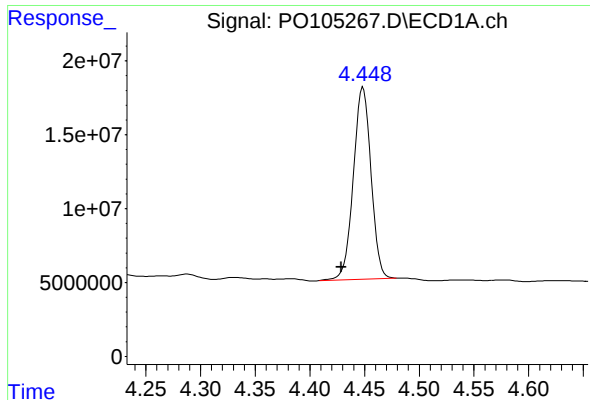


#1 Tetrachloro-m-xylene

R.T.: 4.448 min
Delta R.T.: 0.019 min
Response: 145932333
Conc: 21.20 ng/ml

Instrument :
ECD_O
ClientSampleId :
HD-02-080624


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/08/2024
Supervised By :Ankita Jodhani 08/08/2024

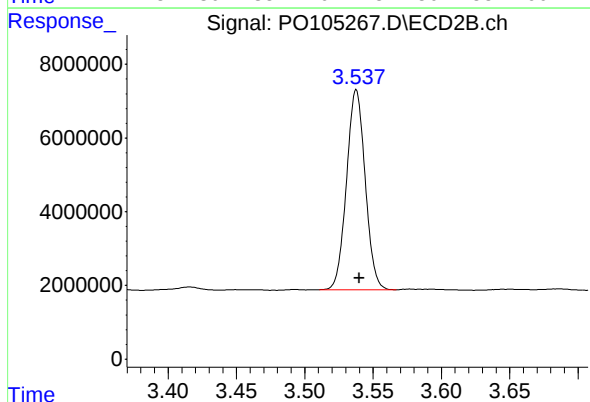


#1 Tetrachloro-m-xylene

R.T.: 3.538 min
Delta R.T.: -0.002 min
Response: 51626538
Conc: 20.26 ng/ml

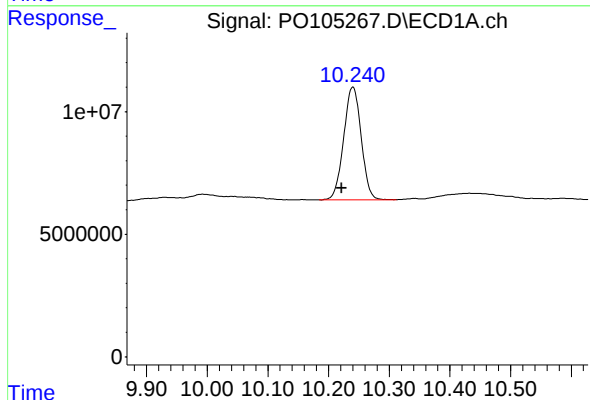

#2 Decachlorobiphenyl

R.T.: 10.240 min
Delta R.T.: 0.018 min
Response: 92797327
Conc: 18.08 ng/ml m

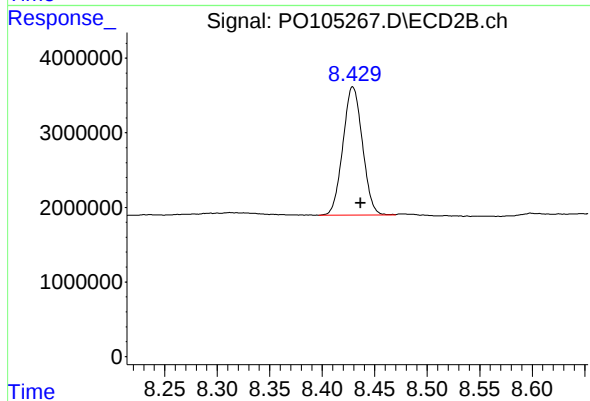

#2 Decachlorobiphenyl

R.T.: 8.429 min
Delta R.T.: -0.008 min
Response: 22207832
Conc: 13.98 ng/ml