

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0080818\
 Data File : P0047822.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Aug 2018 13:05
 Operator : SM/SJ
 Sample : J4347-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CONCRETE-PILE-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 08 13:59:05 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072718.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jul 27 02:33:29 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.406	3.639	5214754	6220899	25.829	25.317
2) SA Decachlor...	10.105	8.632	3418622	3057257	20.960	19.449

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0080818\
Data File : P0047822.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Aug 2018 13:05
Operator : SM/SJ
Sample : J4347-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
CONCRETE-PILE-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 08 13:59:05 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072718.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 27 02:33:29 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

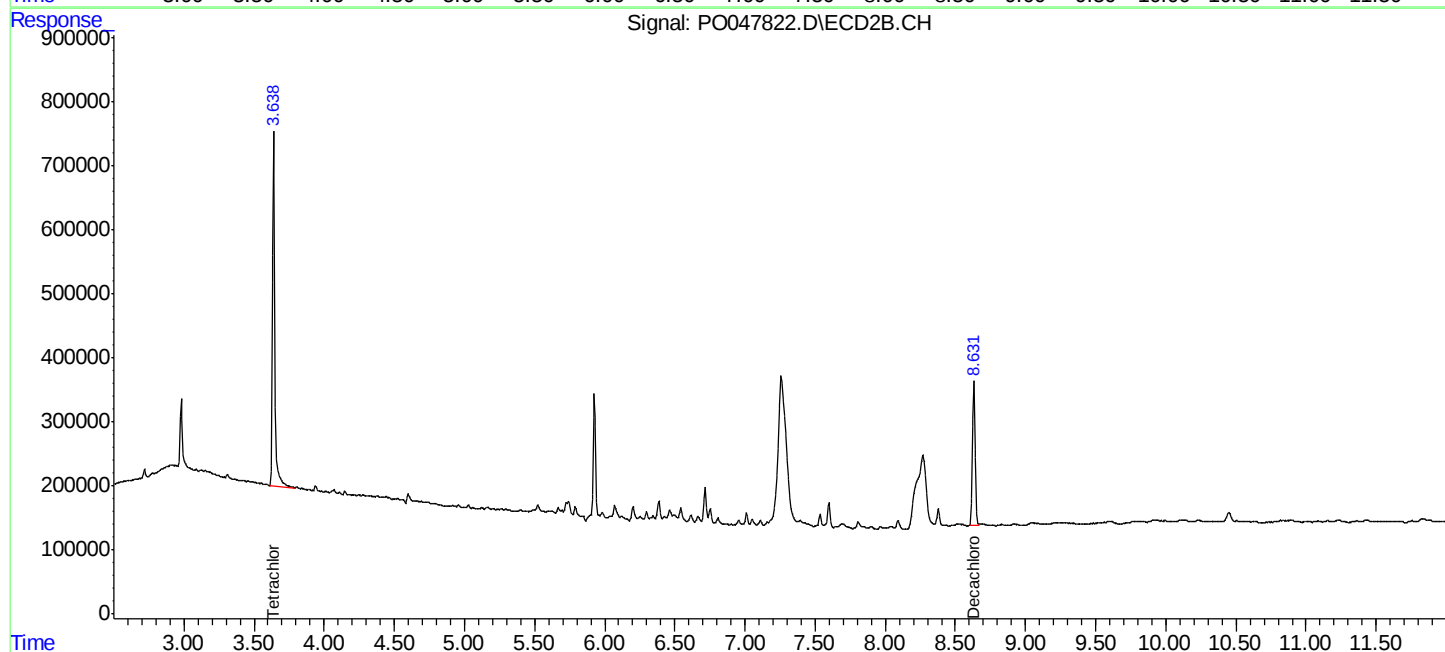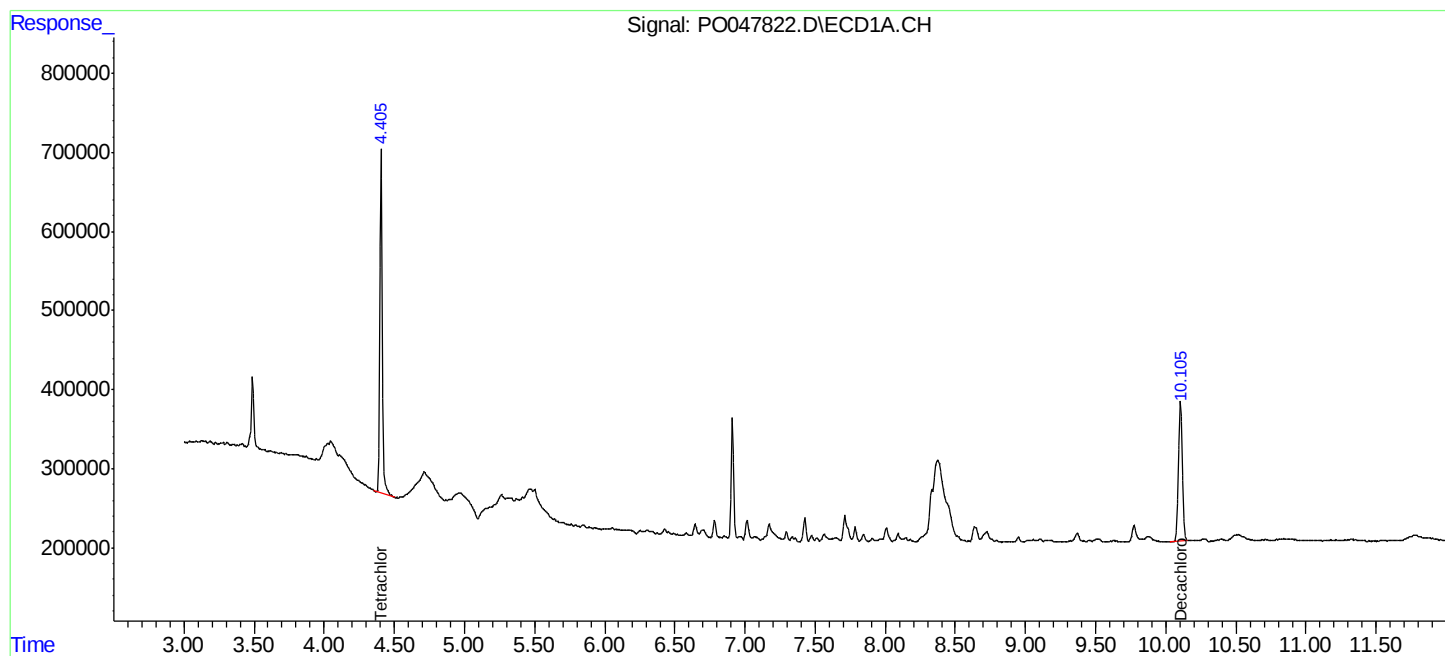


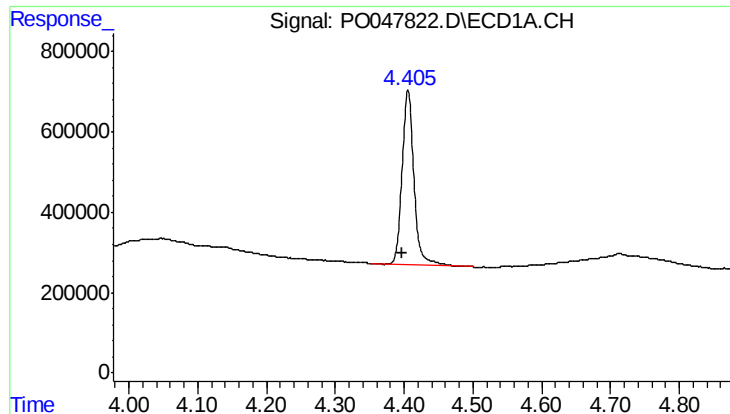

#1 Tetrachloro-m-xylene


R.T.: 4.406 min
Delta R.T.: 0.008 min
Response: 5214754
Conc: 25.83 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONCRETE-PILE-1

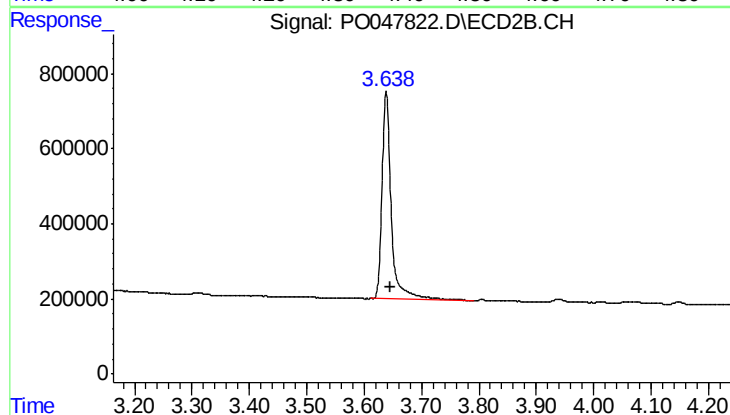


#1 Tetrachloro-m-xylene

R.T.: 3.639 min
Delta R.T.: -0.007 min
Response: 6220899
Conc: 25.32 ng/ml

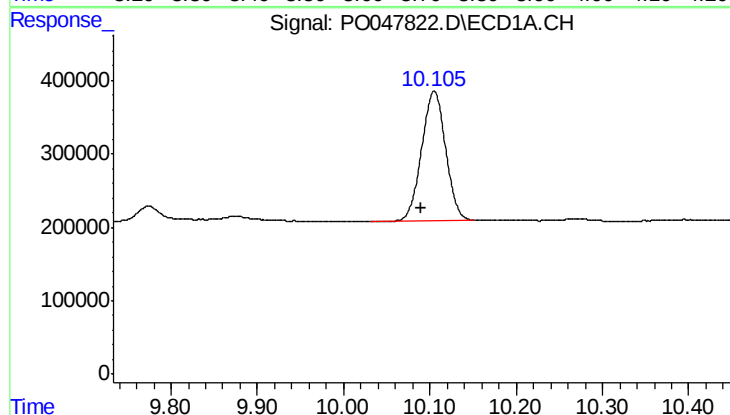

#2 Decachlorobiphenyl

R.T.: 10.105 min
Delta R.T.: 0.015 min
Response: 3418622
Conc: 20.96 ng/ml

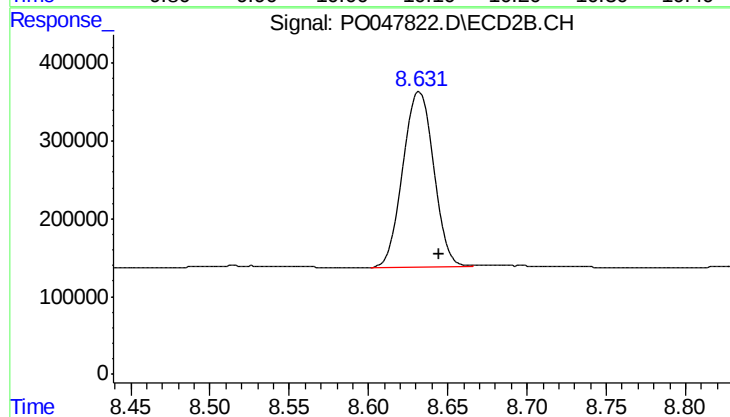

#2 Decachlorobiphenyl

R.T.: 8.632 min
Delta R.T.: -0.013 min
Response: 3057257
Conc: 19.45 ng/ml