

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0080818\
 Data File : P0047826.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Aug 2018 14:13
 Operator : SM/SJ
 Sample : J4275-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CL-02-080718-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 08 14:39:25 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072718.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jul 27 02:33:29 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.395	3.639	5334722	6305748	26.423	25.663
2) SA Decachlor...	10.088	8.627	3757359	3439404	23.037	21.880

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0080818\
Data File : P0047826.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Aug 2018 14:13
Operator : SM/SJ
Sample : J4275-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
CL-02-080718-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 08 14:39:25 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072718.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 27 02:33:29 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

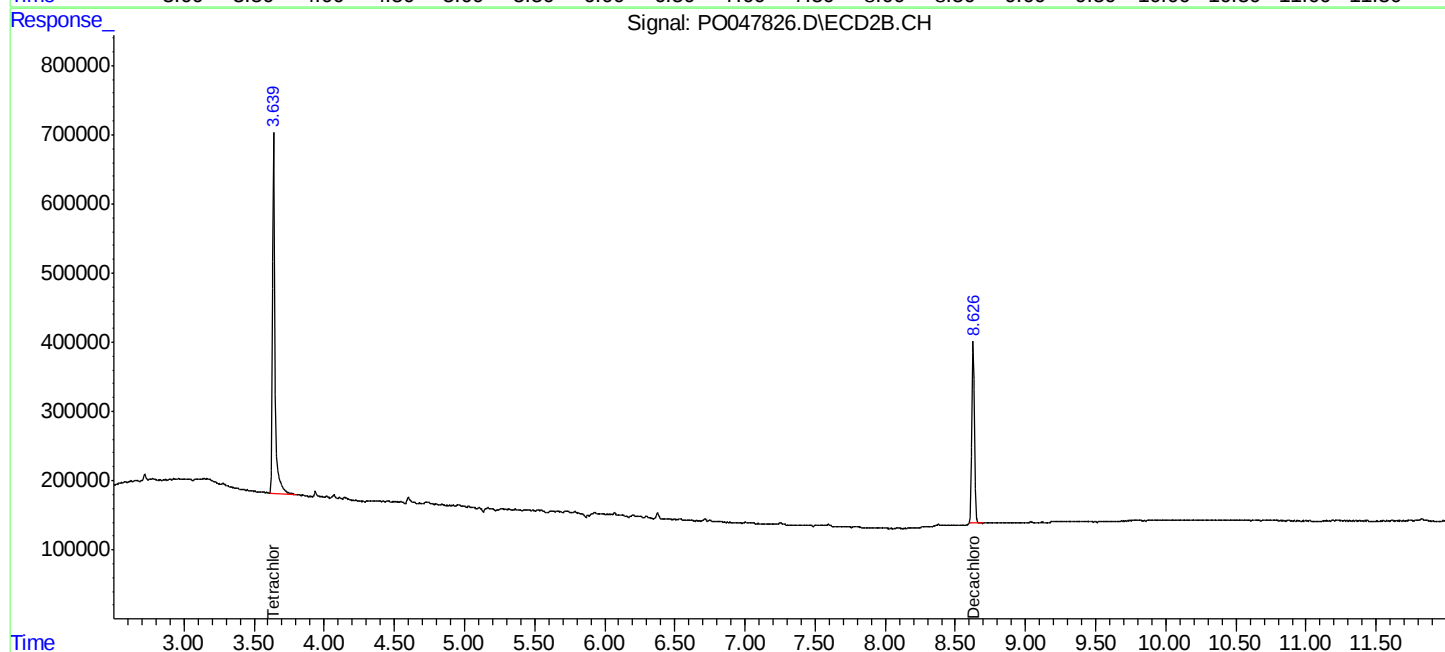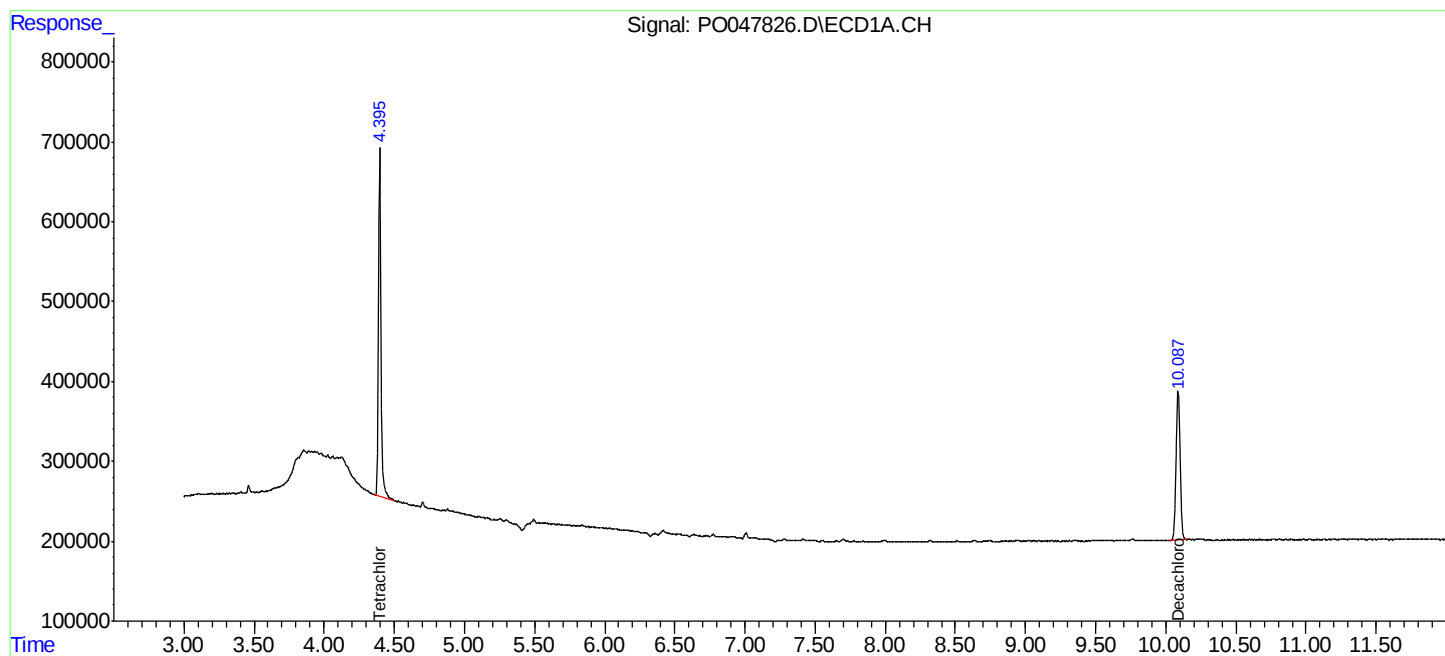


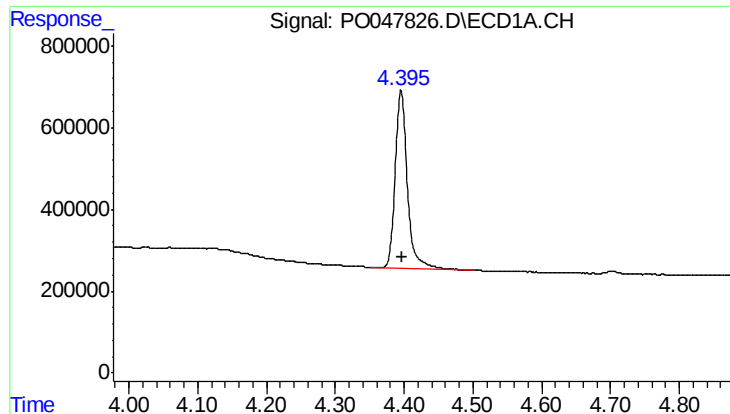

#1 Tetrachloro-m-xylene


R.T.: 4.395 min
Delta R.T.: -0.002 min
Response: 5334722
Conc: 26.42 ng/ml

Instrument :
ECD_O
ClientSampleId :
CL-02-080718-A

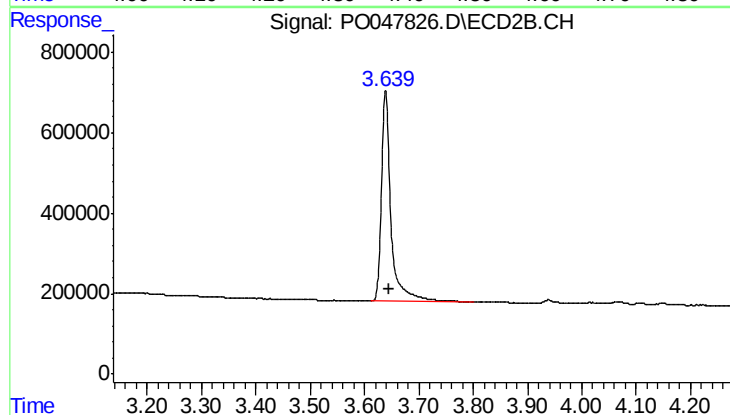


#1 Tetrachloro-m-xylene

R.T.: 3.639 min
Delta R.T.: -0.006 min
Response: 6305748
Conc: 25.66 ng/ml

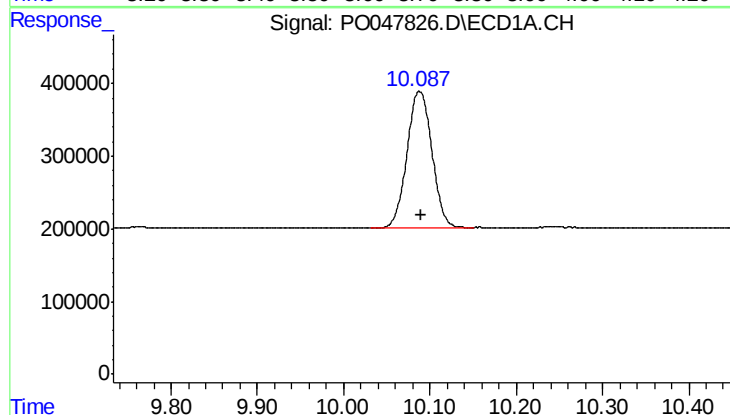

#2 Decachlorobiphenyl

R.T.: 10.088 min
Delta R.T.: -0.002 min
Response: 3757359
Conc: 23.04 ng/ml

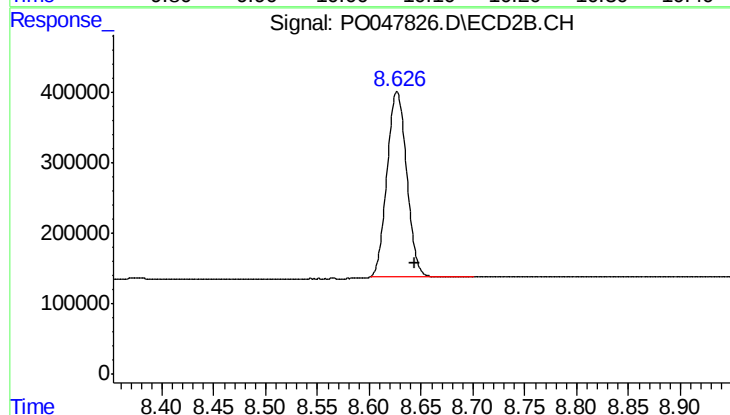

#2 Decachlorobiphenyl

R.T.: 8.627 min
Delta R.T.: -0.018 min
Response: 3439404
Conc: 21.88 ng/ml