

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080819\
Data File : P0059040.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Aug 2019 13:30
Operator : SM/SJ
Sample : K4195-01 5X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
COMP-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 08 15:41:17 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072819.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jul 27 06:49:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.157	3.516	132428	115847	3.138m	2.900
2)	SA Decachlor...	9.658	8.398	88753	73268	1.639m	1.856

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080819\
Data File : P0059040.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Aug 2019 13:30
Operator : SM/SJ
Sample : K4195-01 5X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampled :
COMP-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 08 15:41:17 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072819.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jul 27 06:49:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

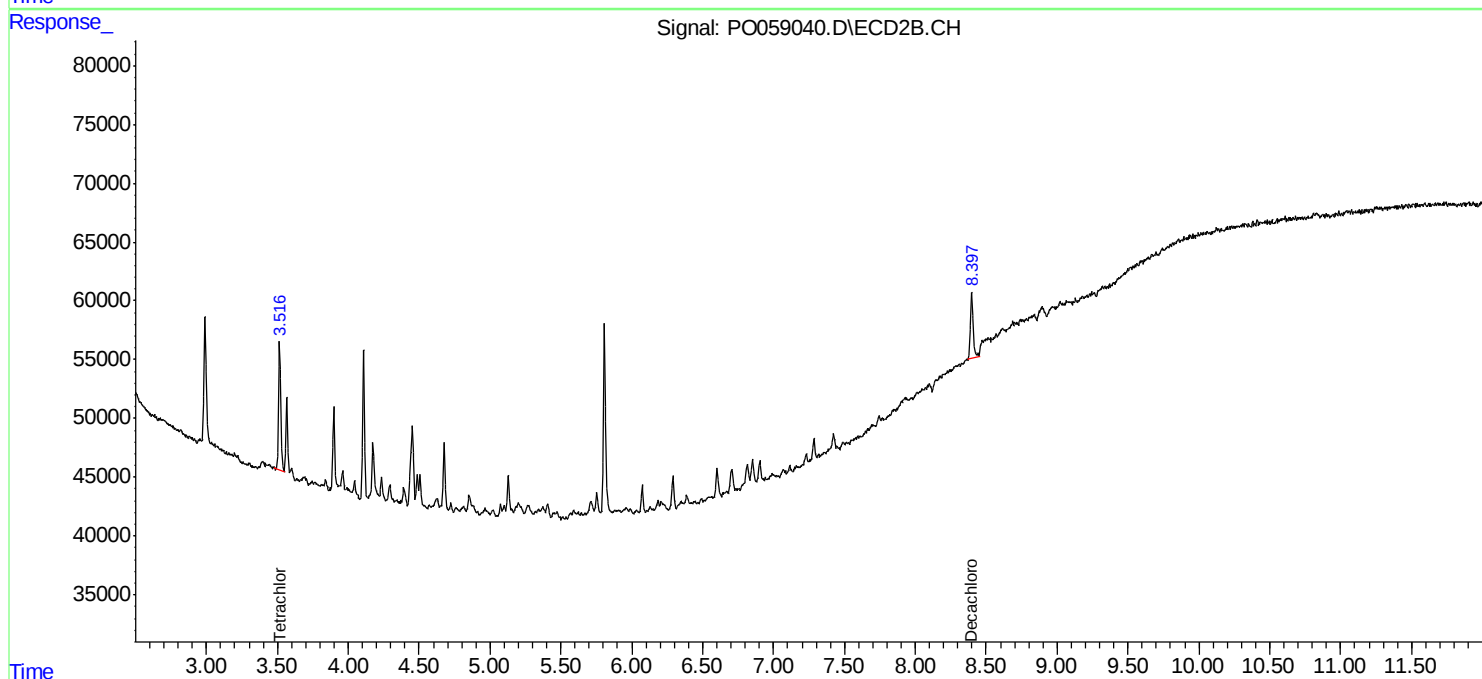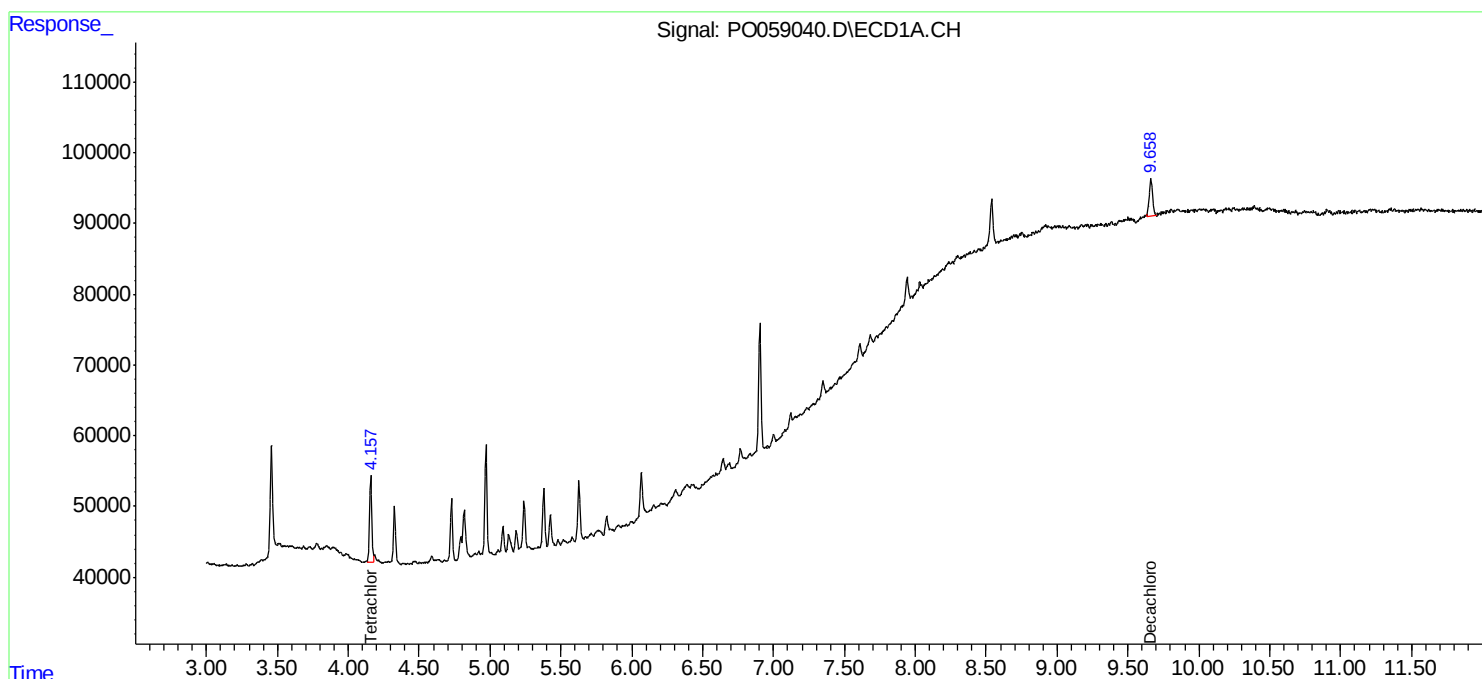


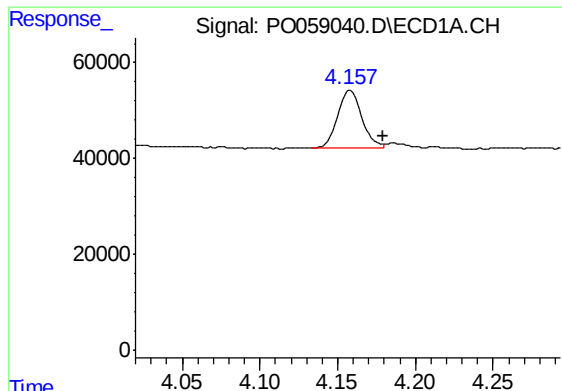

#1 Tetrachloro-m-xylene


R.T.: 4.157 min
Delta R.T.: -0.022 min
Response: 132428
Conc: 3.14 ng/ml m

Instrument :
ECD_O
ClientSampleId :
COMP-1

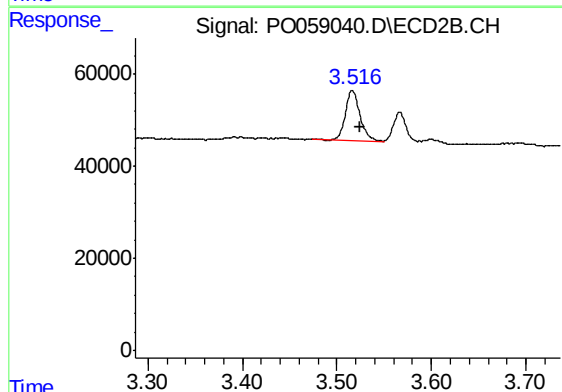


#1 Tetrachloro-m-xylene

R.T.: 3.516 min
Delta R.T.: -0.008 min
Response: 115847
Conc: 2.90 ng/ml

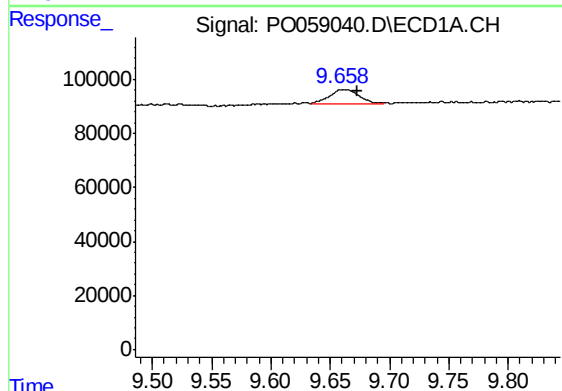

#2 Decachlorobiphenyl

R.T.: 9.658 min
Delta R.T.: -0.014 min
Response: 88753
Conc: 1.64 ng/ml m

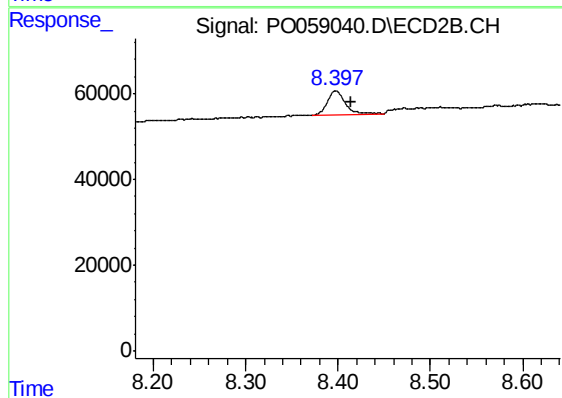

#2 Decachlorobiphenyl

R.T.: 8.398 min
Delta R.T.: -0.016 min
Response: 73268
Conc: 1.86 ng/ml