

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080819\
Data File : P0059051.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Aug 2019 16:41
Operator : SM/SJ
Sample : K4200-01
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP-14

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 09 03:14:10 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072819.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jul 27 06:49:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.158	3.517	812554	717214	19.254	17.953
2)	SA Decachlor...	9.663	8.398	839482	579262	15.501	14.675

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080819\
Data File : P0059051.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Aug 2019 16:41
Operator : SM/SJ
Sample : K4200-01
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP-14

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 09 03:14:10 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072819.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jul 27 06:49:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

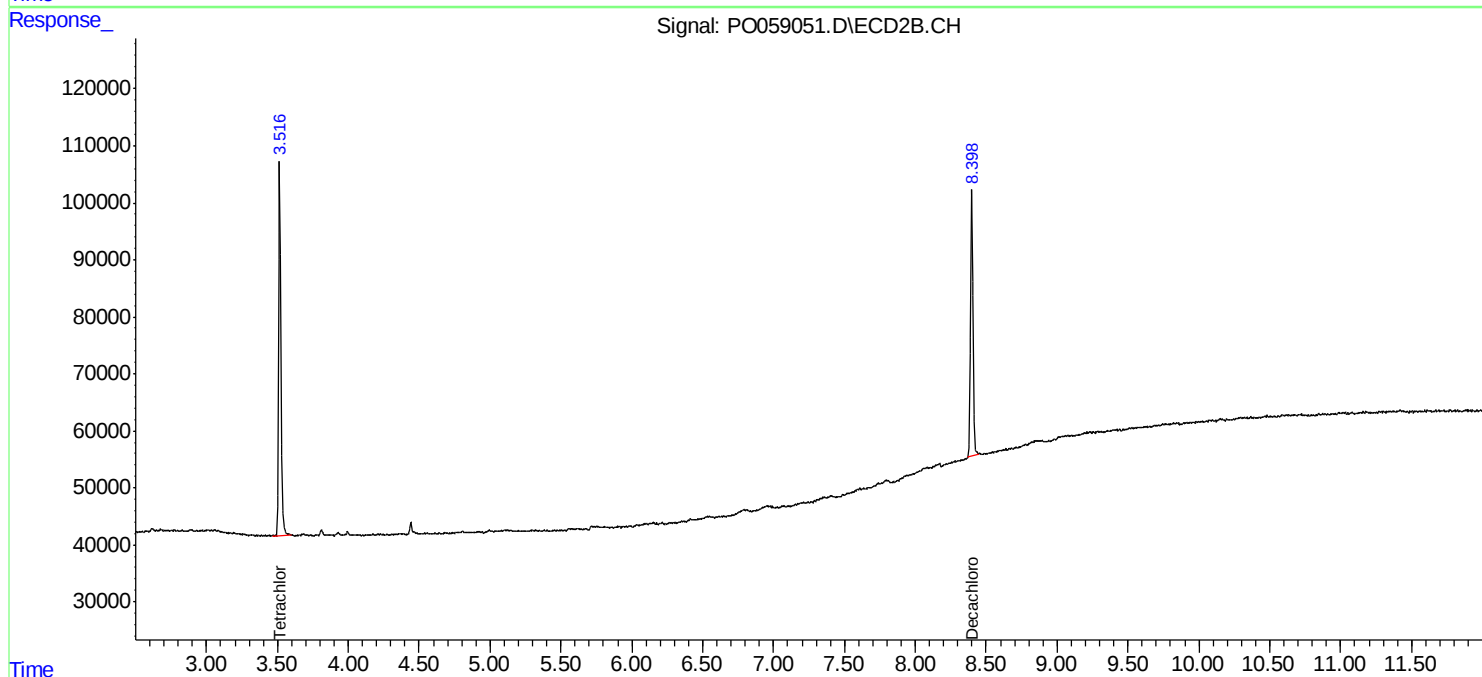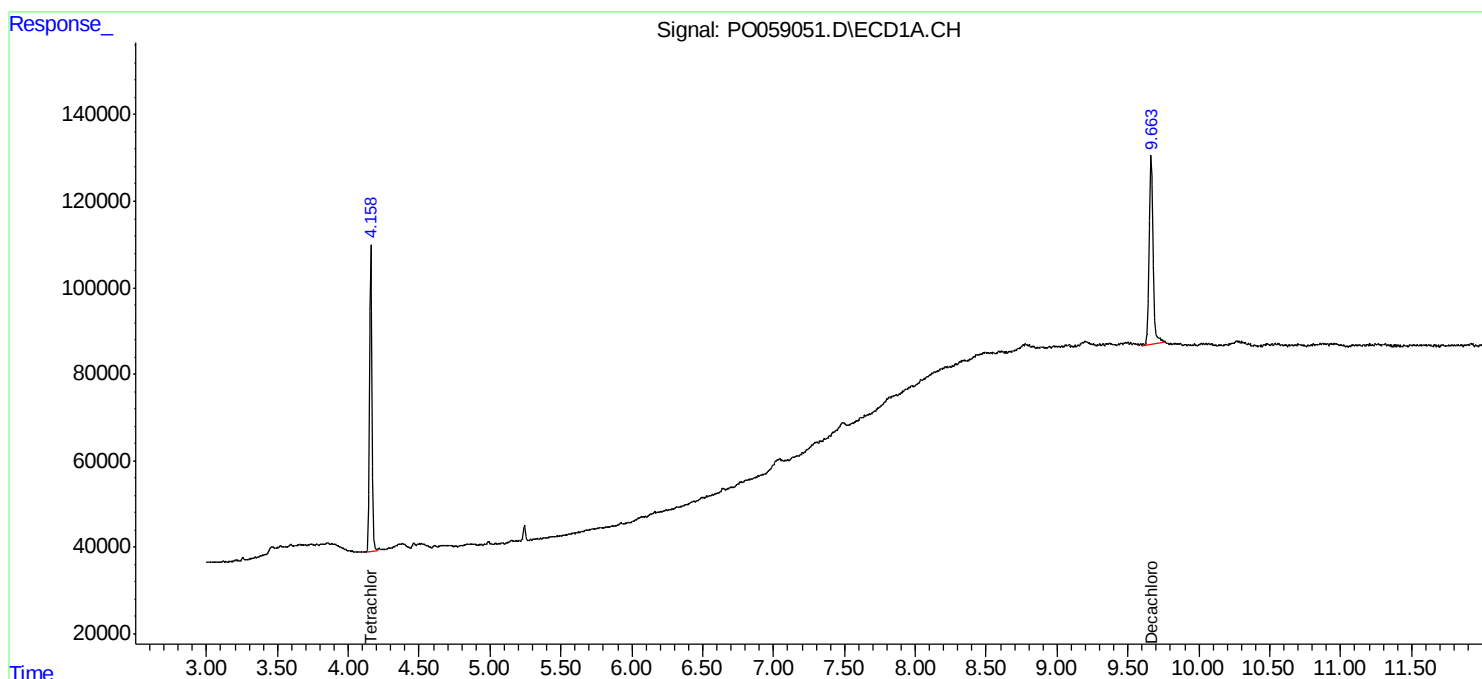


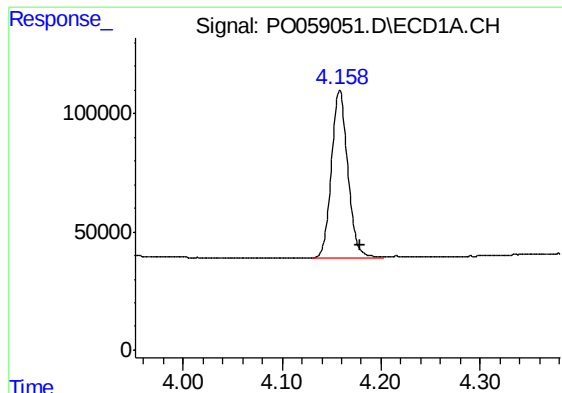

#1 Tetrachloro-m-xylene


R.T.: 4.158 min
Delta R.T.: -0.021 min
Response: 812554
Conc: 19.25 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-14

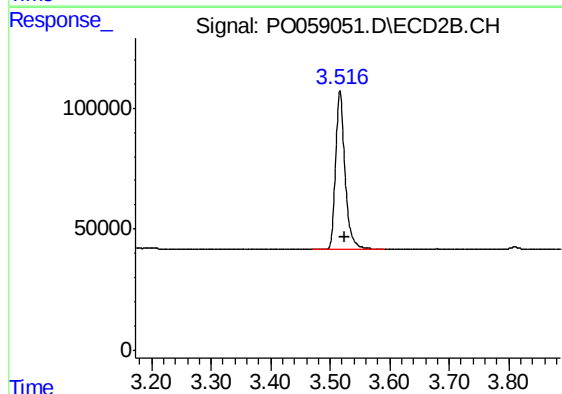


#1 Tetrachloro-m-xylene

R.T.: 3.517 min
Delta R.T.: -0.008 min
Response: 717214
Conc: 17.95 ng/ml

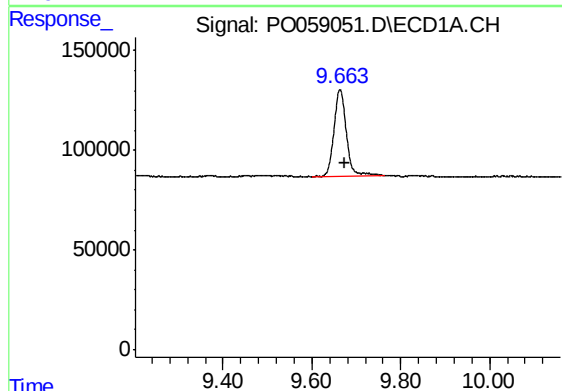

#2 Decachlorobiphenyl

R.T.: 9.663 min
Delta R.T.: -0.009 min
Response: 839482
Conc: 15.50 ng/ml

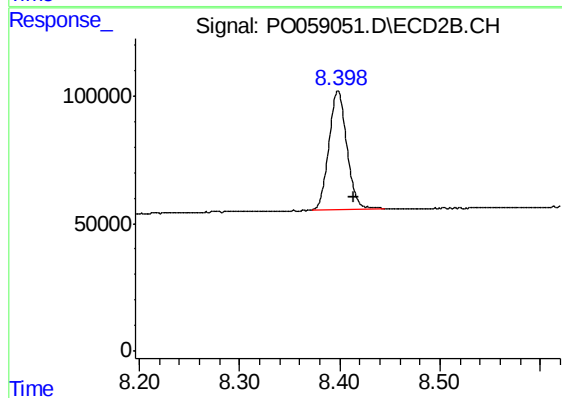

#2 Decachlorobiphenyl

R.T.: 8.398 min
Delta R.T.: -0.016 min
Response: 579262
Conc: 14.67 ng/ml