

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080819\
Data File : P0059060.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Aug 2019 19:12
Operator : SM/SJ
Sample : K4223-17
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
SP-9

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 09 03:20:11 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072819.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jul 27 06:49:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.156	3.516	832730	749560	19.732	18.762
2)	SA Decachlor...	9.659	8.397	589891	429521	10.893	10.881

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO080819\
Data File : PO059060.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Aug 2019 19:12
Operator : SM/SJ
Sample : K4223-17
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
SP-9

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 09 03:20:11 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO072819.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jul 27 06:49:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

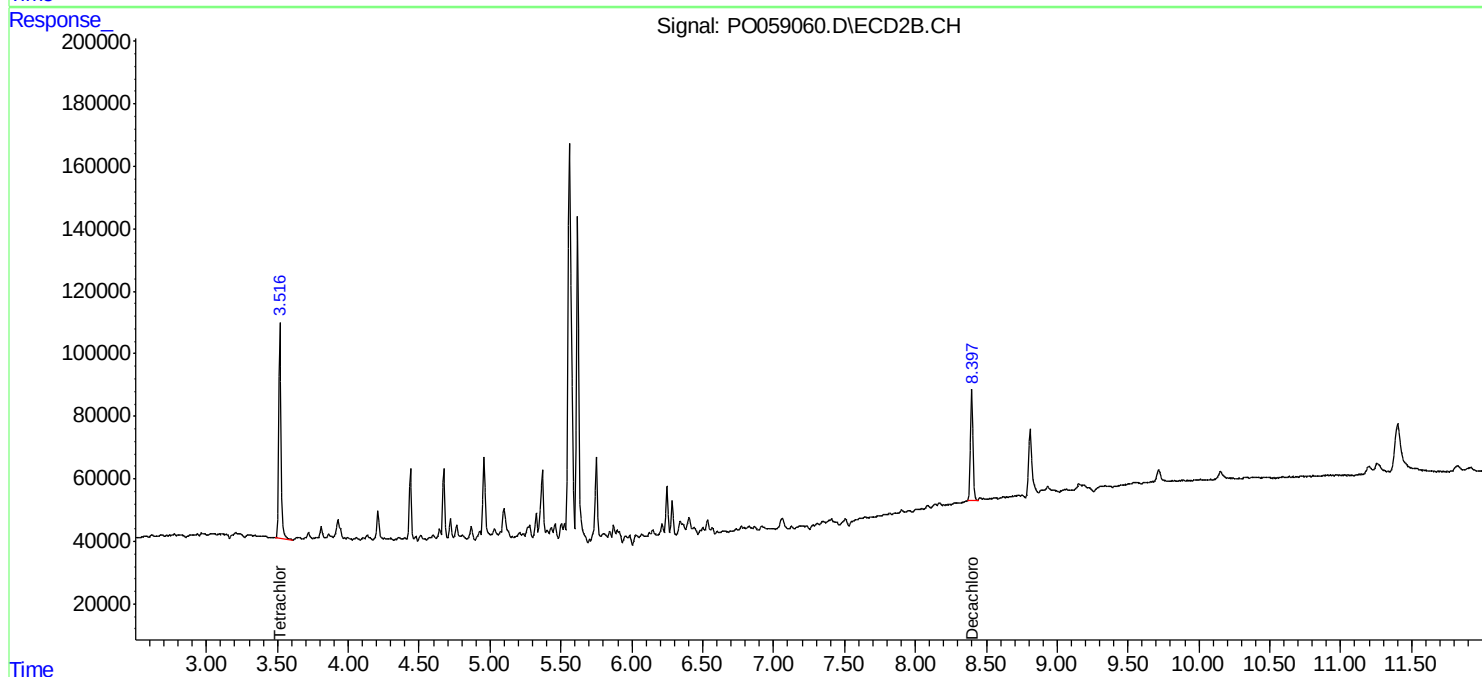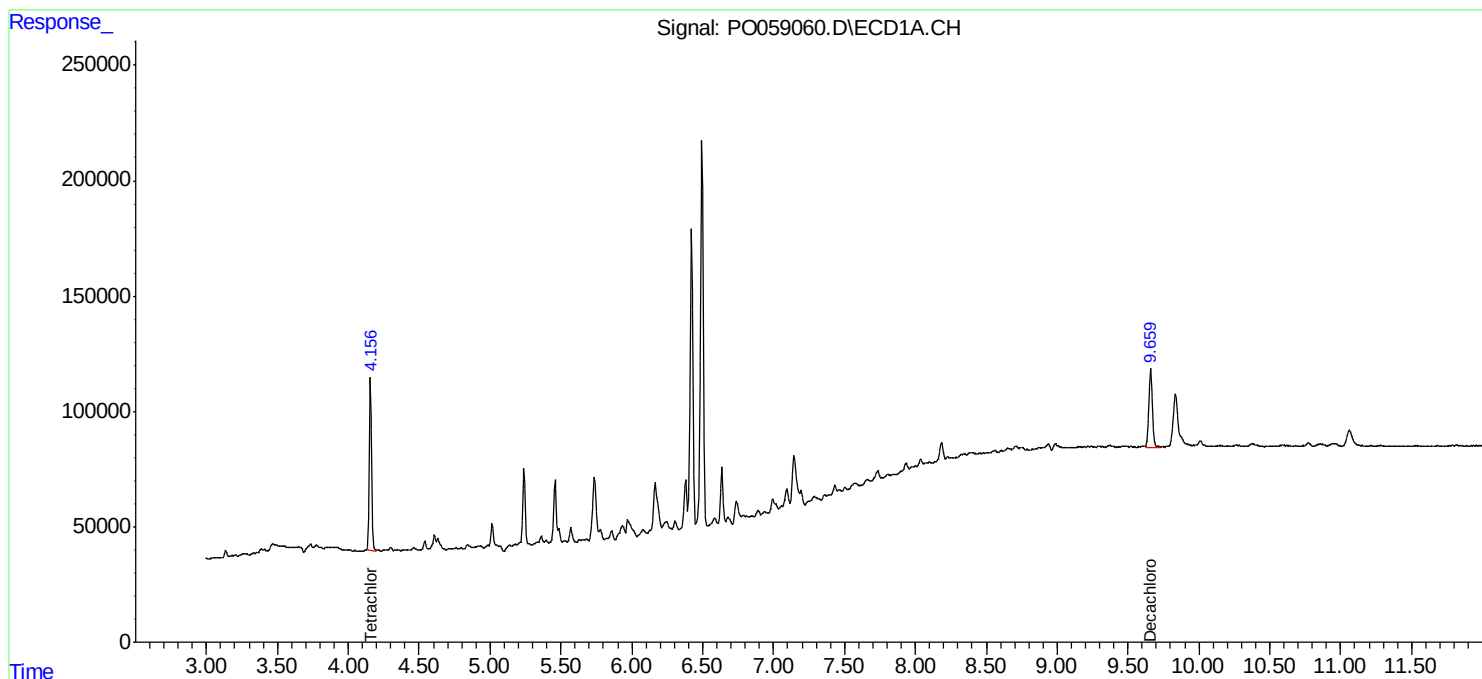


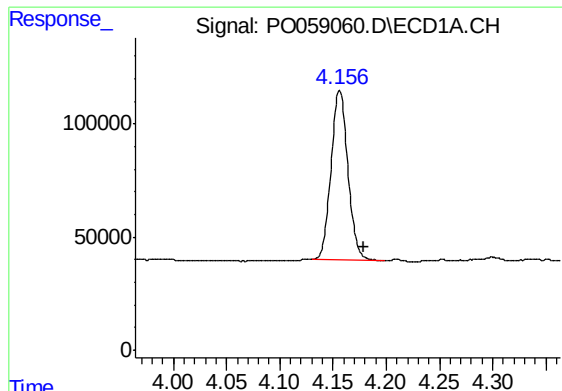

#1 Tetrachloro-m-xylene


R.T.: 4.156 min
Delta R.T.: -0.023 min
Response: 832730
Conc: 19.73 ng/ml

Instrument :
ECD_O
ClientSampleId :
SP-9

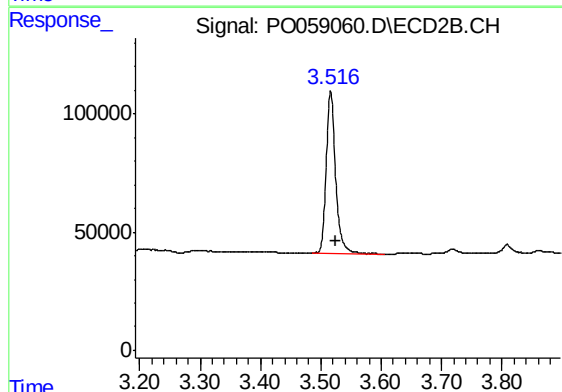


#1 Tetrachloro-m-xylene

R.T.: 3.516 min
Delta R.T.: -0.008 min
Response: 749560
Conc: 18.76 ng/ml

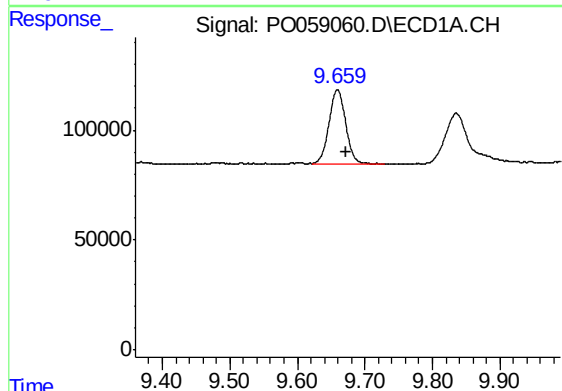

#2 Decachlorobiphenyl

R.T.: 9.659 min
Delta R.T.: -0.013 min
Response: 589891
Conc: 10.89 ng/ml

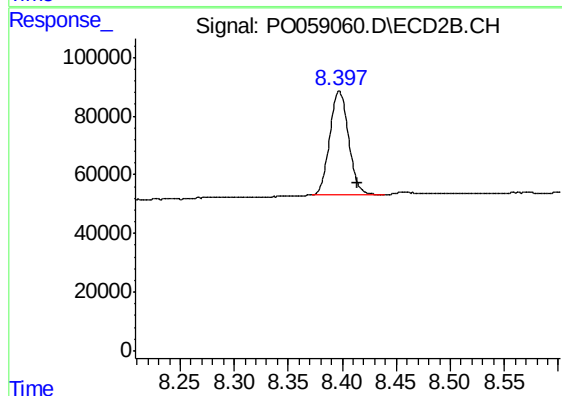

#2 Decachlorobiphenyl

R.T.: 8.397 min
Delta R.T.: -0.017 min
Response: 429521
Conc: 10.88 ng/ml