

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080822\
 Data File : P0088715.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Aug 2022 20:55
 Operator : YP/AJ
 Sample : N3980-09
 Misc : AR1242 MDL 25 PPB
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-WATER-03-QT3-2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 09 03:03:52 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0080422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 05 23:24:09 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.438	3.595	51579868	20275776	19.122	18.734
2)	SA Decachlor...	10.276	8.587	34889378	21836546	18.080	18.018
Target Compounds							
16)	L4 AR-1242-1	5.613	4.673	1727259	766679	25.699	25.006
17)	L4 AR-1242-2	5.636	4.692	2468671	1081927	25.580	25.111
18)	L4 AR-1242-3	5.699	4.868	1598694	571801	26.487	23.817
19)	L4 AR-1242-4	5.799	4.951	1188200	667817	24.649	26.487
20)	L4 AR-1242-5	6.539	5.474	1233410	701393	23.766	22.029



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO080822\
Data File : PO088715.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Aug 2022 20:55
Operator : YP/AJ
Sample : N3980-09
Misc : AR1242 MDL 25 PPB
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 09 03:03:52 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO080422.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 05 23:24:09 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

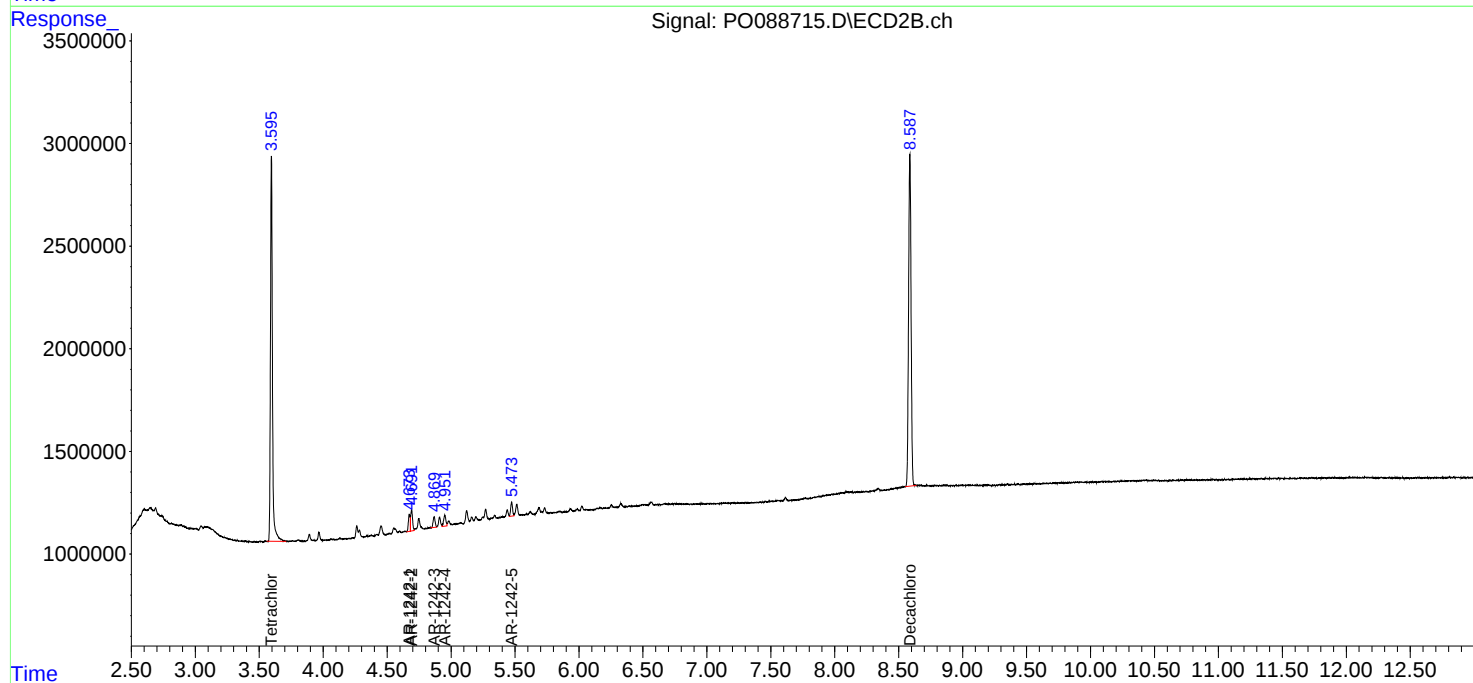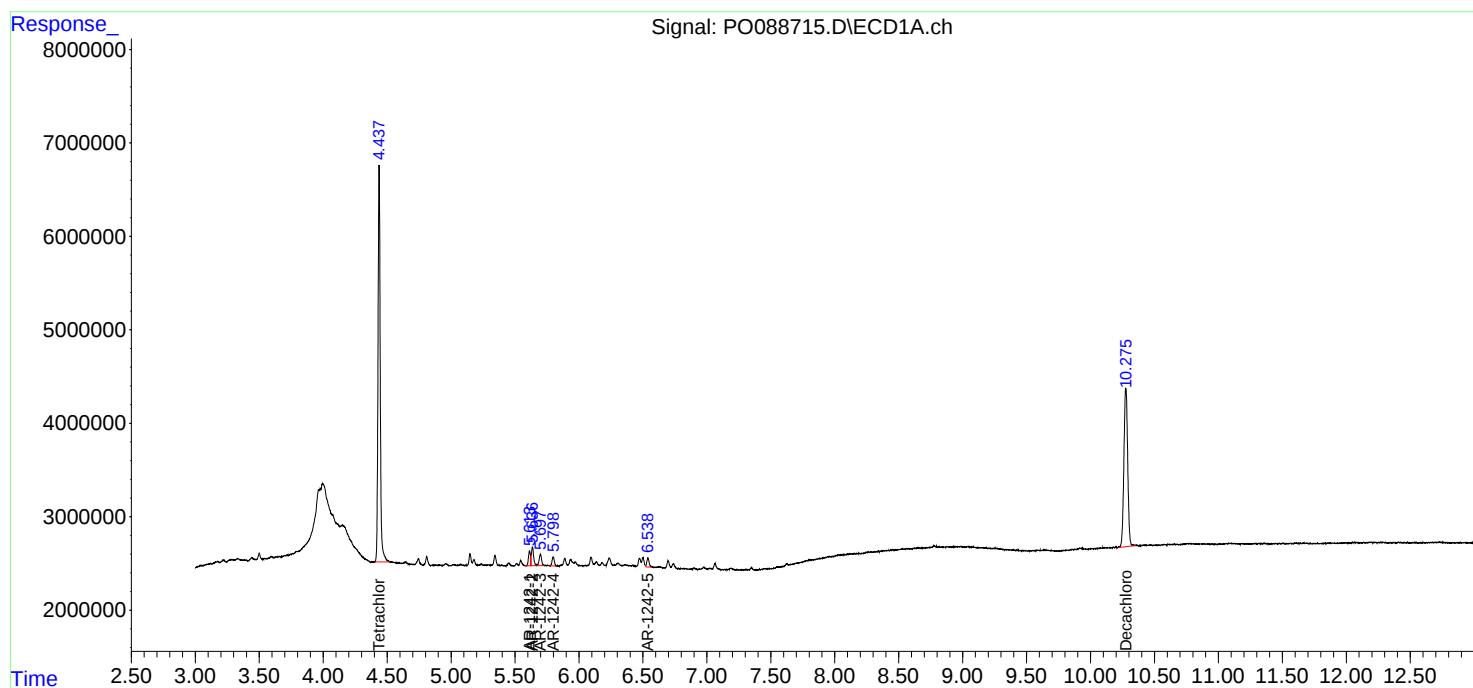


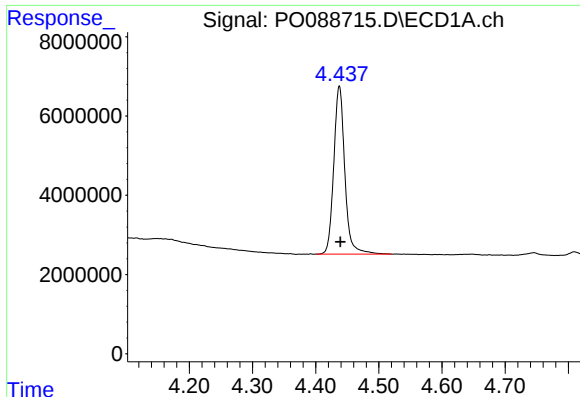

#1 Tetrachloro-m-xylene


R.T.: 4.438 min
Delta R.T.: -0.002 min
Response: 51579868
Conc: 19.12 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2022

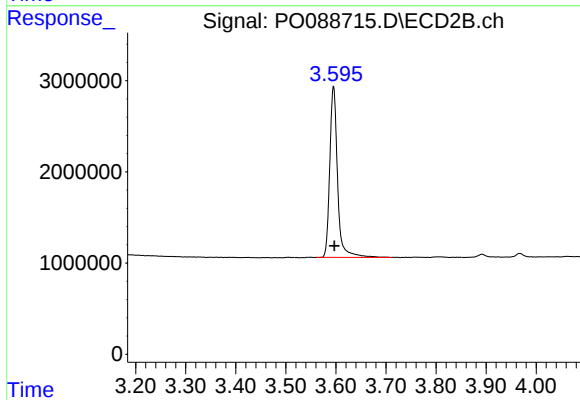


#1 Tetrachloro-m-xylene

R.T.: 3.595 min
Delta R.T.: -0.002 min
Response: 20275776
Conc: 18.73 ng/ml

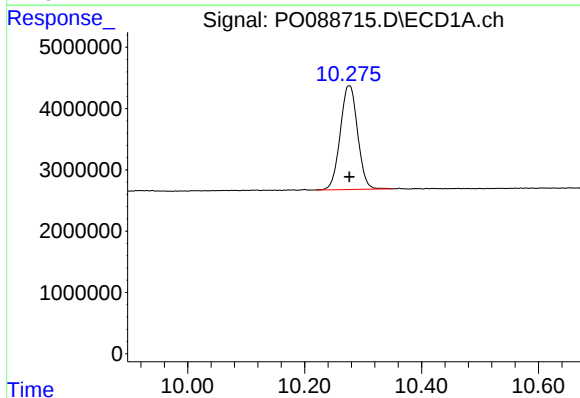


#2 Decachlorobiphenyl

R.T.: 10.276 min
Delta R.T.: 0.000 min
Response: 34889378
Conc: 18.08 ng/ml

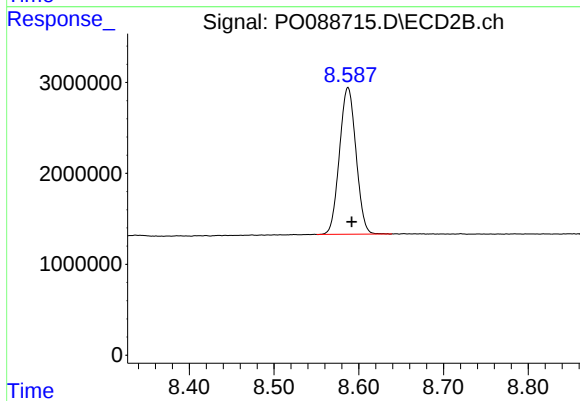

#2 Decachlorobiphenyl


R.T.: 8.587 min
Delta R.T.: -0.004 min
Response: 21836546
Conc: 18.02 ng/ml

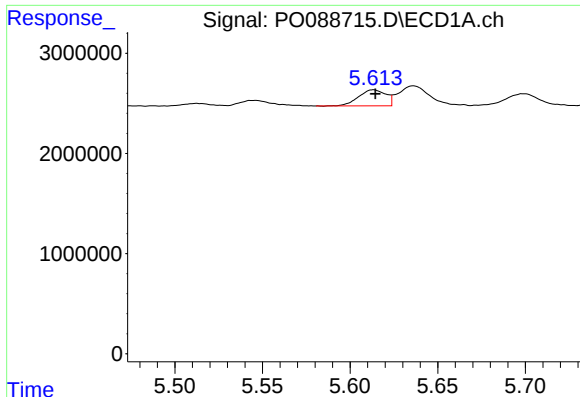

#16 AR-1242-1


R.T.: 5.613 min
Delta R.T.: -0.001 min
Response: 1727259
Conc: 25.70 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2022

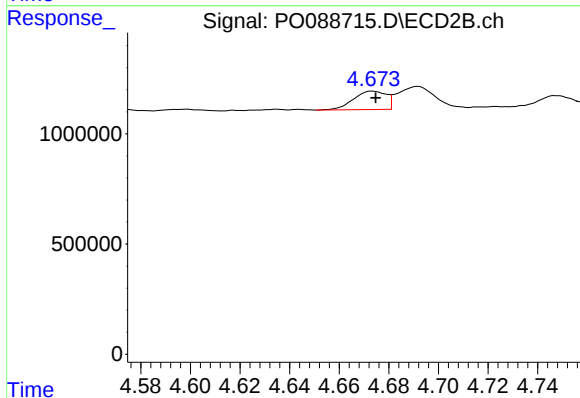


#16 AR-1242-1

R.T.: 4.673 min
Delta R.T.: -0.001 min
Response: 766679
Conc: 25.01 ng/ml

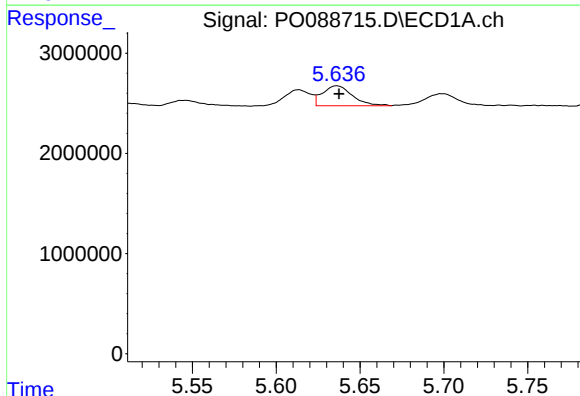


#17 AR-1242-2

R.T.: 5.636 min
Delta R.T.: -0.001 min
Response: 2468671
Conc: 25.58 ng/ml

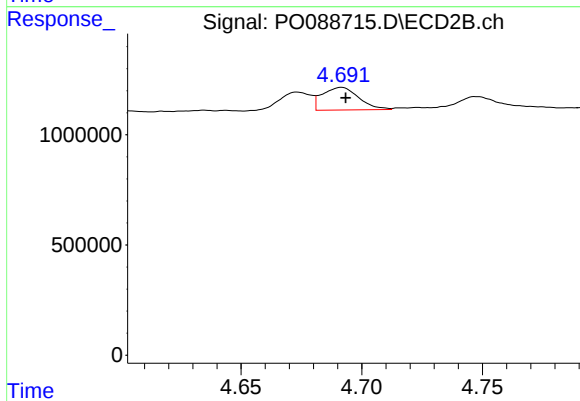

#17 AR-1242-2


R.T.: 4.692 min
Delta R.T.: -0.002 min
Response: 1081927
Conc: 25.11 ng/ml

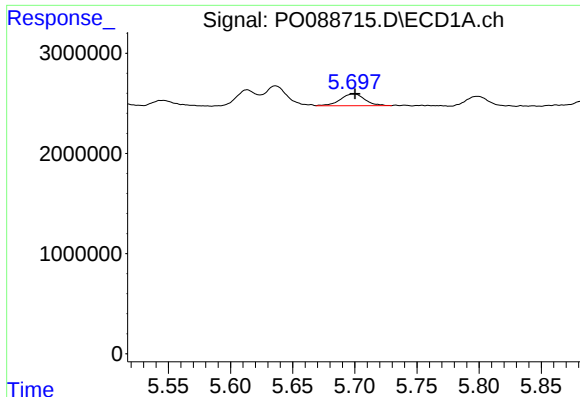

#18 AR-1242-3


R.T.: 5.699 min
Delta R.T.: -0.001 min
Response: 1598694
Conc: 26.49 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2022

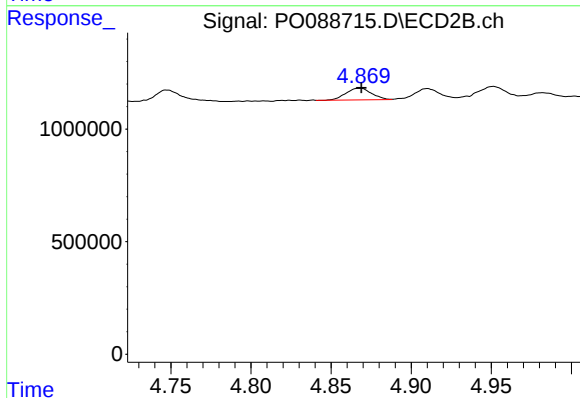


#18 AR-1242-3

R.T.: 4.868 min
Delta R.T.: 0.000 min
Response: 571801
Conc: 23.82 ng/ml

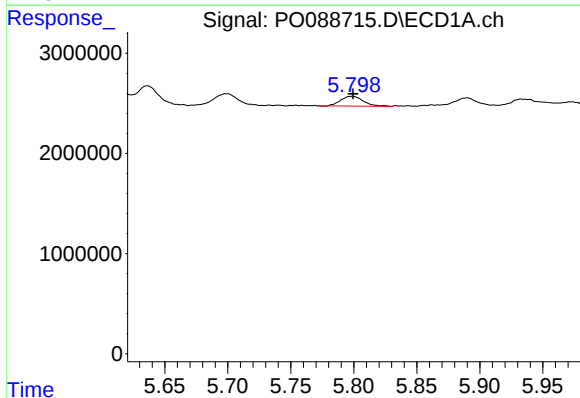


#19 AR-1242-4

R.T.: 5.799 min
Delta R.T.: 0.000 min
Response: 1188200
Conc: 24.65 ng/ml

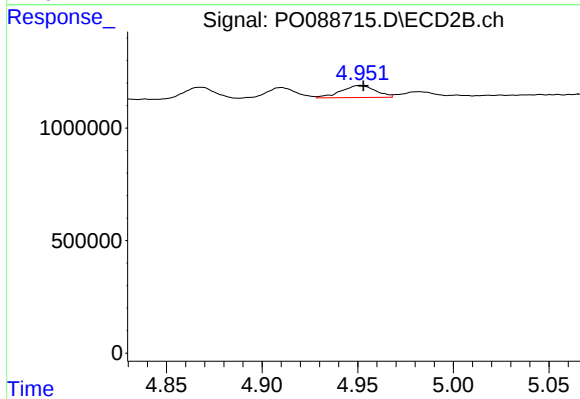

#19 AR-1242-4


R.T.: 4.951 min
Delta R.T.: -0.002 min
Response: 667817
Conc: 26.49 ng/ml

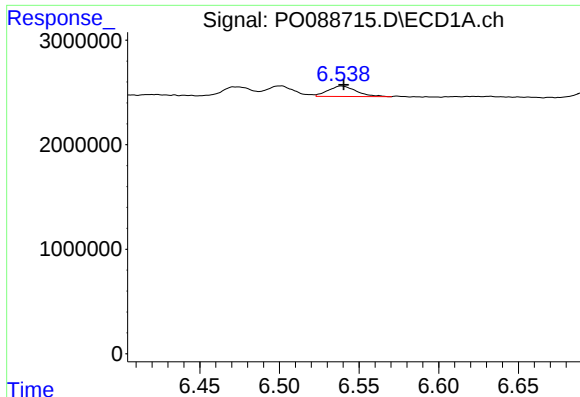

#20 AR-1242-5

R.T.: 6.539 min
Delta R.T.: -0.001 min
Response: 1233410
Conc: 23.77 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2022

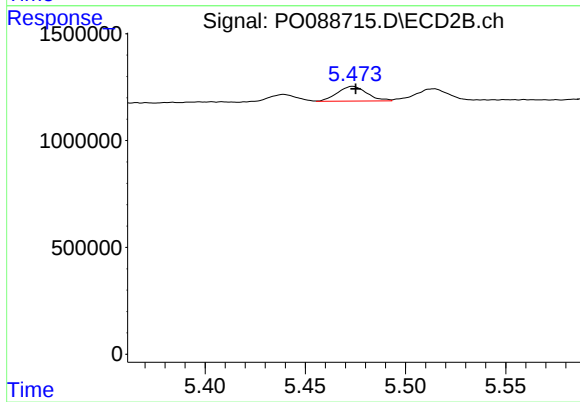

#20 AR-1242-5

R.T.: 5.474 min
Delta R.T.: -0.001 min
Response: 701393
Conc: 22.03 ng/ml