

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080822\
 Data File : P0088716.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Aug 2022 21:13
 Operator : YP/AJ
 Sample : N3980-09
 Misc : AR1248 MDL 25 PPB
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-WATER-03-QT3-2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 09 03:04:42 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0080422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 05 23:24:09 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.437	3.595	56008849	21962416	20.764	20.292
2)	SA Decachlor...	10.274	8.588	37429369	23587660	19.397	19.463
Target Compounds							
21)	L5 AR-1248-1	5.613	4.673	1487310	631508	28.828	26.895
22)	L5 AR-1248-2	5.889	4.910	2246408	1009172	29.262	28.119
23)	L5 AR-1248-3	6.095	4.950	2301111	1076469	27.859	28.272
24)	L5 AR-1248-4	6.501	5.121	2648074	1282988	29.486	27.938
25)	L5 AR-1248-5	6.539	5.514	2557057	1205083	28.847	27.601



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO080822\
Data File : PO088716.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Aug 2022 21:13
Operator : YP/AJ
Sample : N3980-09
Misc : AR1248 MDL 25 PPB
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 09 03:04:42 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO080422.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 05 23:24:09 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

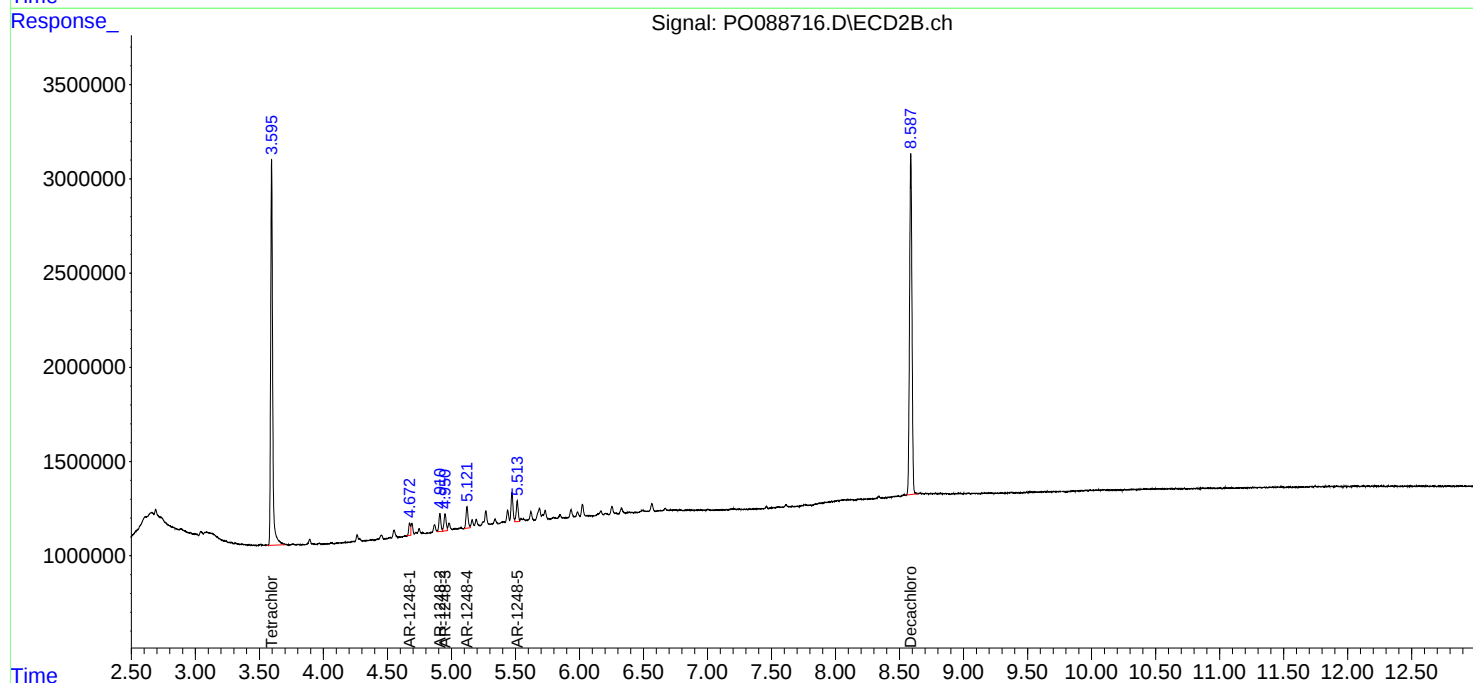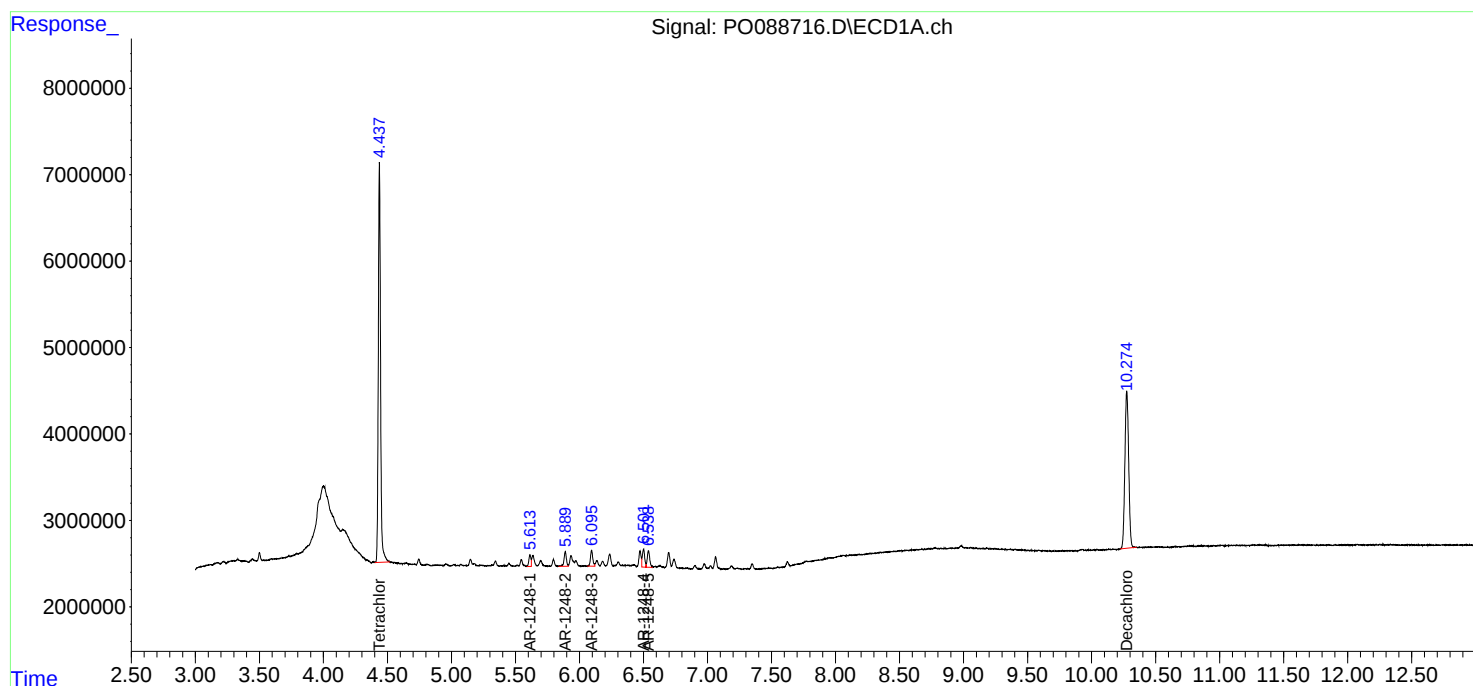


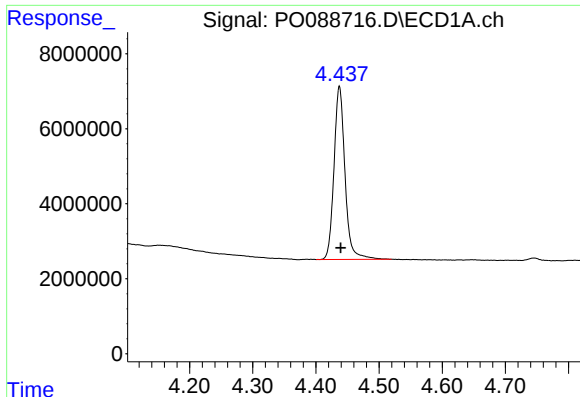

#1 Tetrachloro-m-xylene


R.T.: 4.437 min
Delta R.T.: -0.002 min
Response: 56008849
Conc: 20.76 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2022

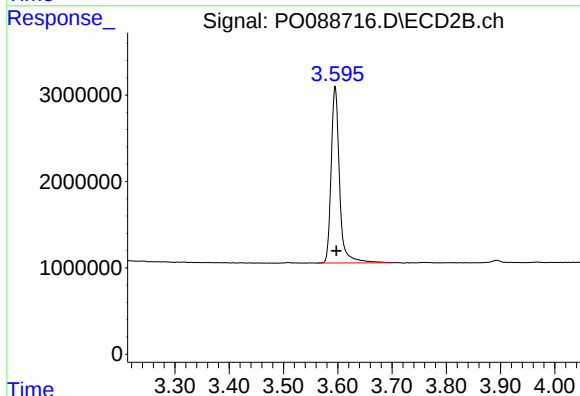


#1 Tetrachloro-m-xylene

R.T.: 3.595 min
Delta R.T.: -0.002 min
Response: 21962416
Conc: 20.29 ng/ml

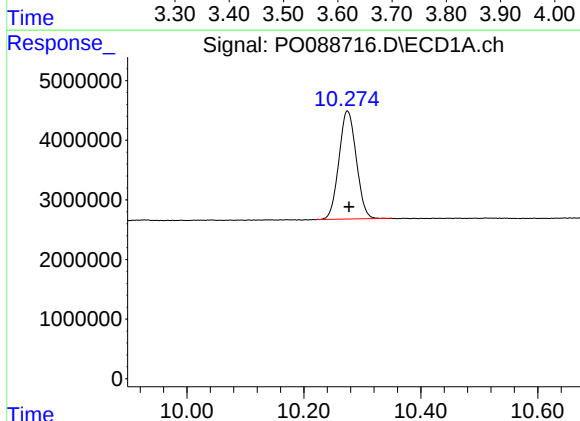


#2 Decachlorobiphenyl

R.T.: 10.274 min
Delta R.T.: -0.002 min
Response: 37429369
Conc: 19.40 ng/ml

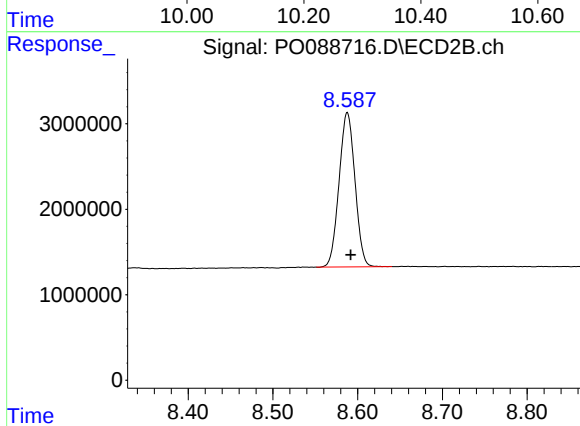

#2 Decachlorobiphenyl


R.T.: 8.588 min
Delta R.T.: -0.004 min
Response: 23587660
Conc: 19.46 ng/ml

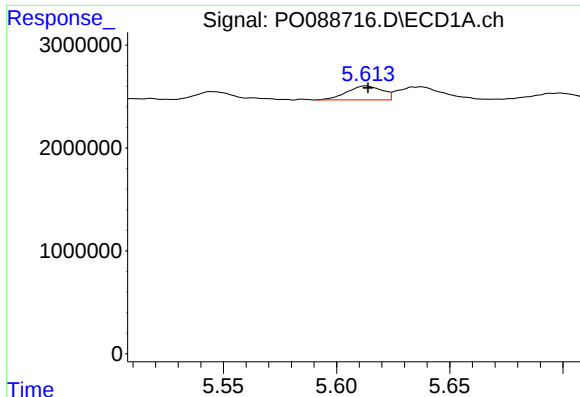

#21 AR-1248-1


R.T.: 5.613 min
Delta R.T.: 0.000 min
Response: 1487310
Conc: 28.83 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2022

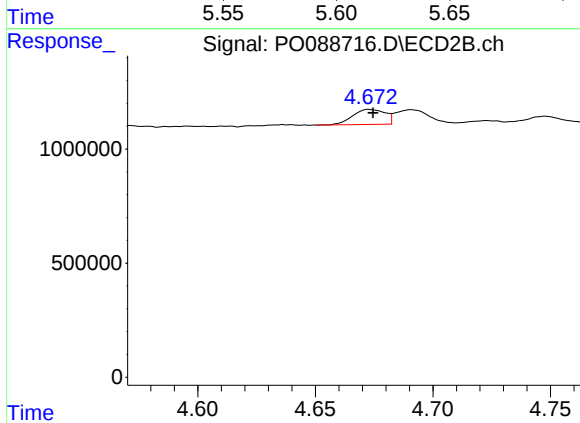


#21 AR-1248-1

R.T.: 4.673 min
Delta R.T.: -0.001 min
Response: 631508
Conc: 26.89 ng/ml

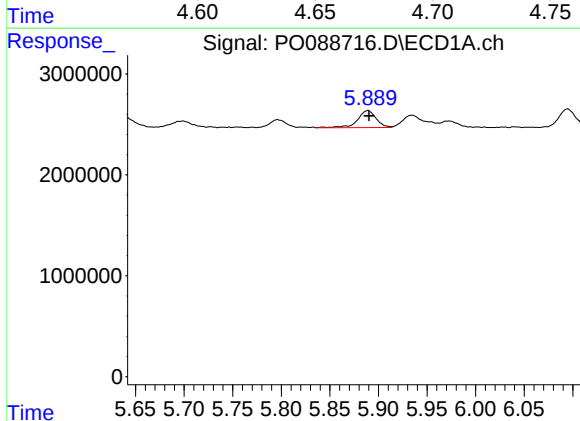


#22 AR-1248-2

R.T.: 5.889 min
Delta R.T.: -0.001 min
Response: 2246408
Conc: 29.26 ng/ml

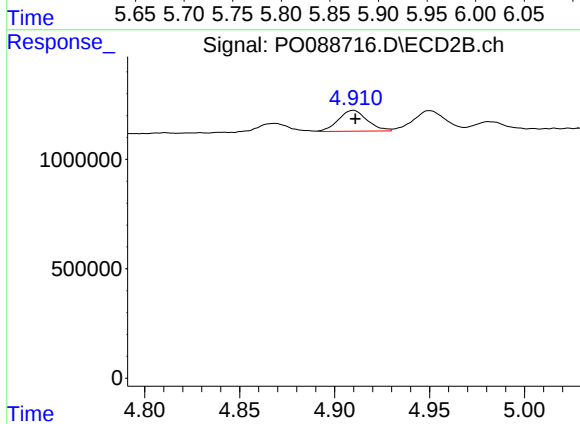

#22 AR-1248-2


R.T.: 4.910 min
Delta R.T.: -0.001 min
Response: 1009172
Conc: 28.12 ng/ml

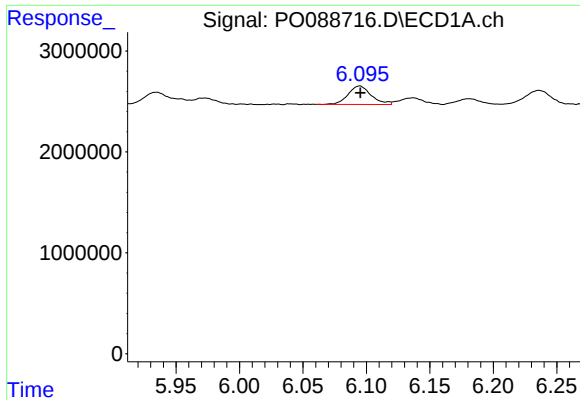

#23 AR-1248-3


R.T.: 6.095 min
Delta R.T.: 0.000 min
Response: 2301111
Conc: 27.86 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2022

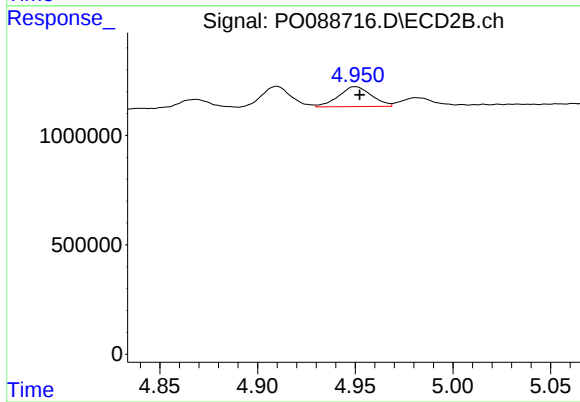


#23 AR-1248-3

R.T.: 4.950 min
Delta R.T.: -0.002 min
Response: 1076469
Conc: 28.27 ng/ml

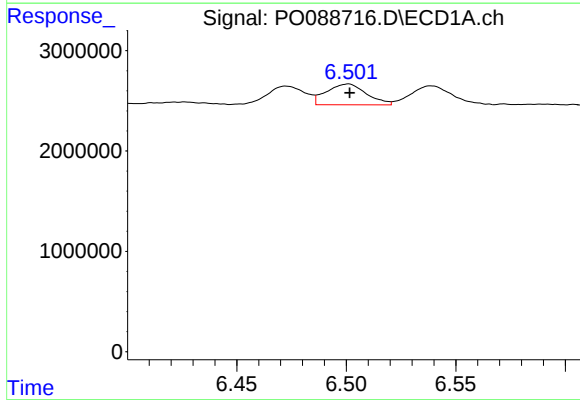


#24 AR-1248-4

R.T.: 6.501 min
Delta R.T.: 0.000 min
Response: 2648074
Conc: 29.49 ng/ml

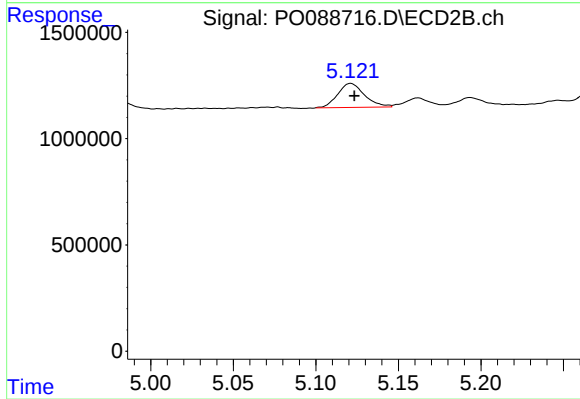

#24 AR-1248-4


R.T.: 5.121 min
Delta R.T.: -0.002 min
Response: 1282988
Conc: 27.94 ng/ml

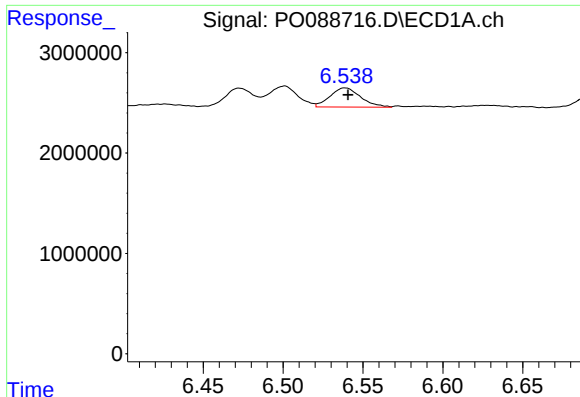

#25 AR-1248-5

R.T.: 6.539 min
Delta R.T.: -0.002 min
Response: 2557057
Conc: 28.85 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2022

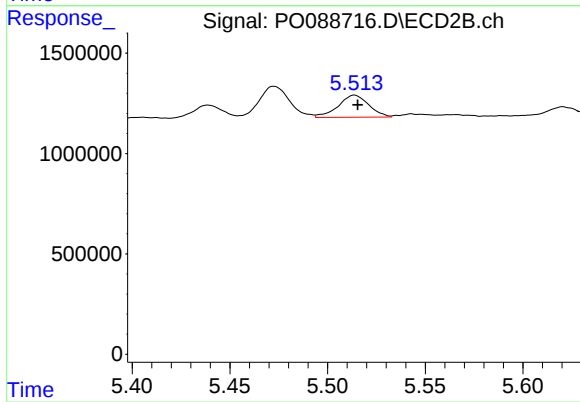

#25 AR-1248-5

R.T.: 5.514 min
Delta R.T.: -0.002 min
Response: 1205083
Conc: 27.60 ng/ml