

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080822\
 Data File : P0088717.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Aug 2022 21:30
 Operator : YP/AJ
 Sample : N3980-09
 Misc : AR1254 MDL 25 PPB
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-WATER-03-QT3-2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 09 03:05:33 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0080422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 05 23:24:09 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.438	3.595	47320735	18905812	17.543	17.468
2) SA Decachlor...	10.277	8.588	32013997	20185177	16.590	16.656
Target Compounds						
26) L6 AR-1254-1	6.475	5.473	2677163	1694244	29.308	24.599
27) L6 AR-1254-2	6.695	5.621	3769360	1546400	27.563	26.113
28) L6 AR-1254-3	7.064	6.024	3870584	2343080	27.504	25.198
29) L6 AR-1254-4	7.349	6.254	2476413	1392225	24.508	24.576
30) L6 AR-1254-5	7.771	6.670	2547574	1949162	23.923	23.879



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO080822\
Data File : PO088717.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Aug 2022 21:30
Operator : YP/AJ
Sample : N3980-09
Misc : AR1254 MDL 25 PPB
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 09 03:05:33 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO080422.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 05 23:24:09 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

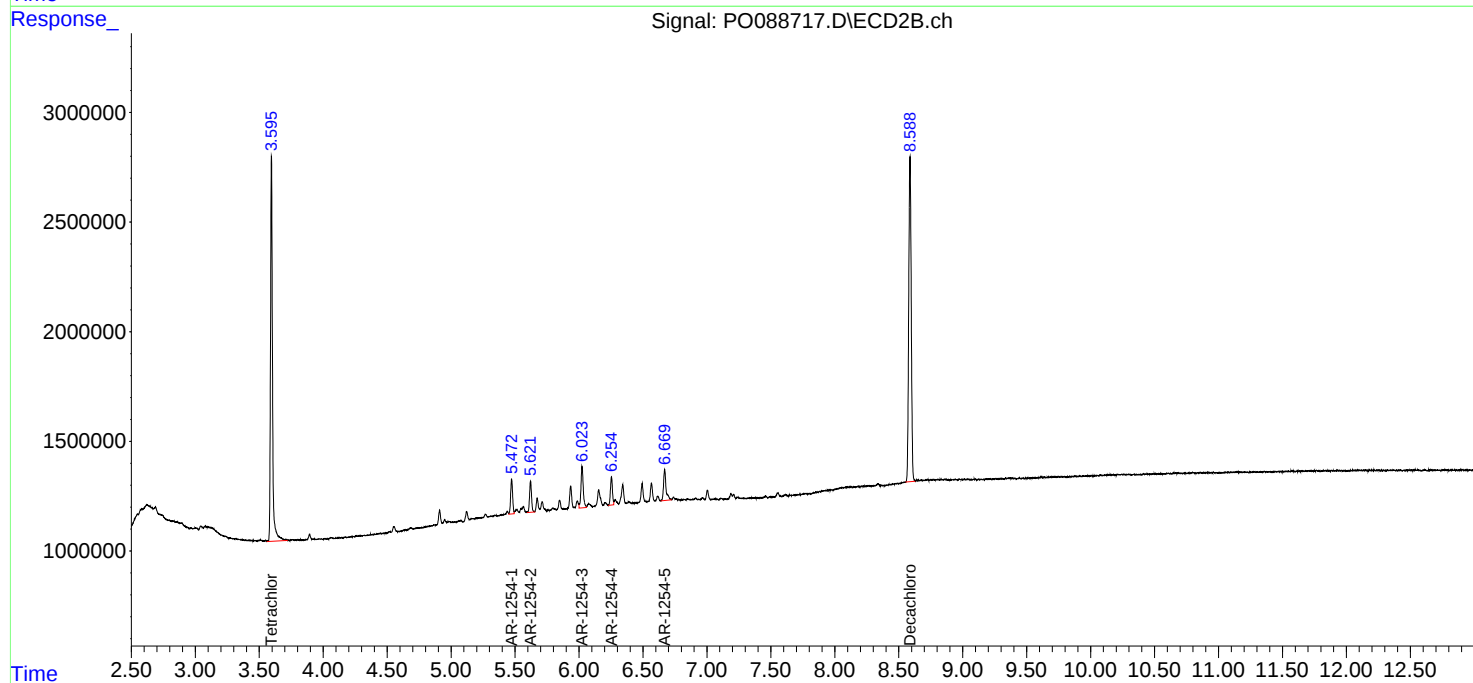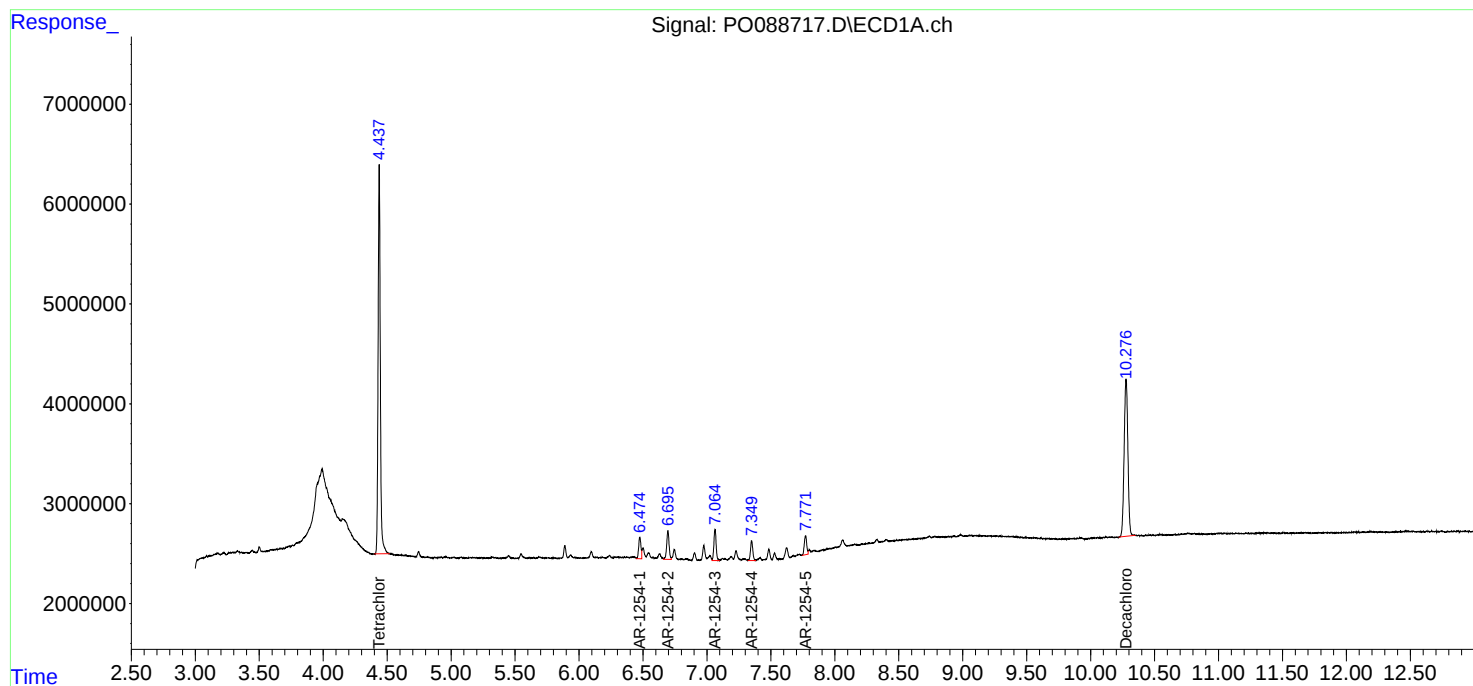


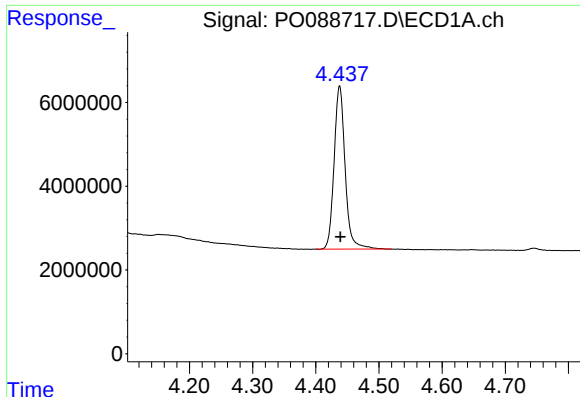

#1 Tetrachloro-m-xylene


R.T.: 4.438 min
Delta R.T.: -0.001 min
Response: 47320735
Conc: 17.54 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2022

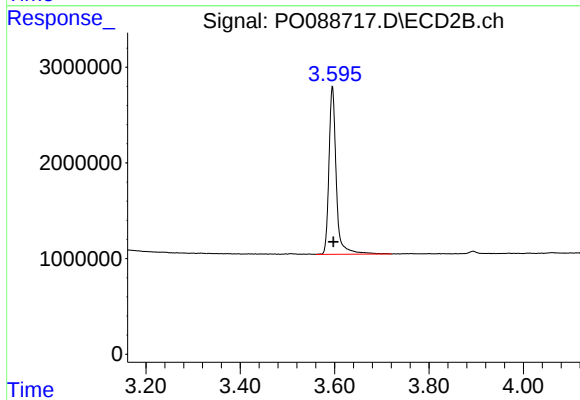


#1 Tetrachloro-m-xylene

R.T.: 3.595 min
Delta R.T.: -0.002 min
Response: 18905812
Conc: 17.47 ng/ml

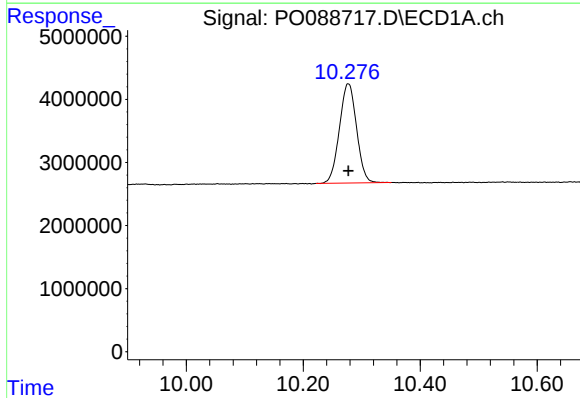


#2 Decachlorobiphenyl

R.T.: 10.277 min
Delta R.T.: 0.000 min
Response: 32013997
Conc: 16.59 ng/ml

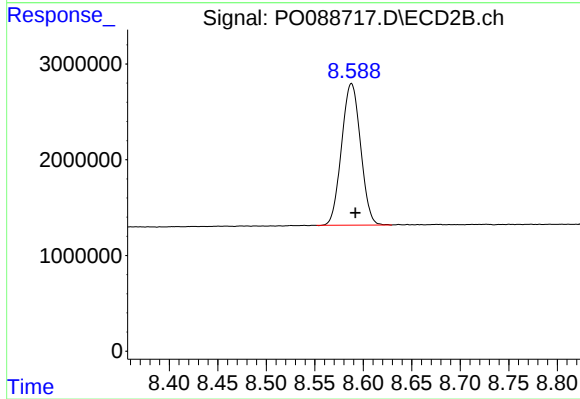

#2 Decachlorobiphenyl


R.T.: 8.588 min
Delta R.T.: -0.004 min
Response: 20185177
Conc: 16.66 ng/ml

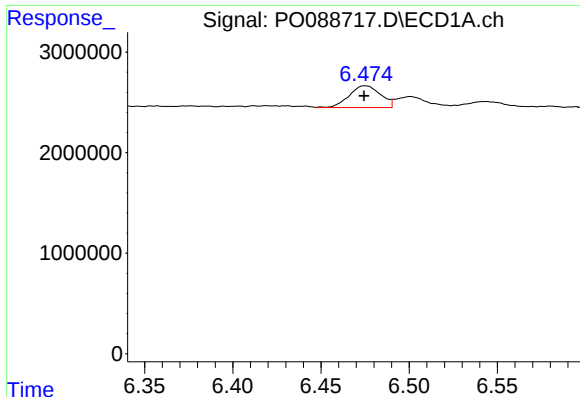

#26 AR-1254-1


R.T.: 6.475 min
Delta R.T.: 0.000 min
Response: 2677163
Conc: 29.31 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2022

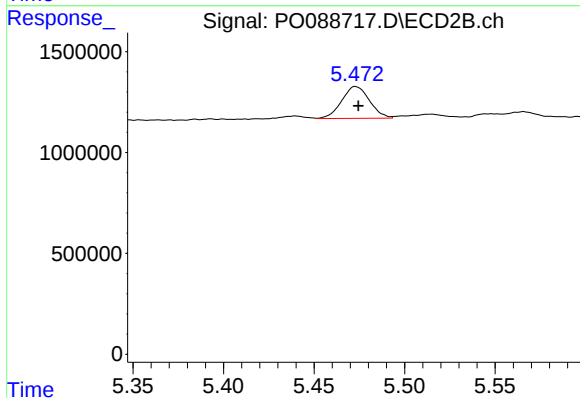


#26 AR-1254-1

R.T.: 5.473 min
Delta R.T.: -0.001 min
Response: 1694244
Conc: 24.60 ng/ml

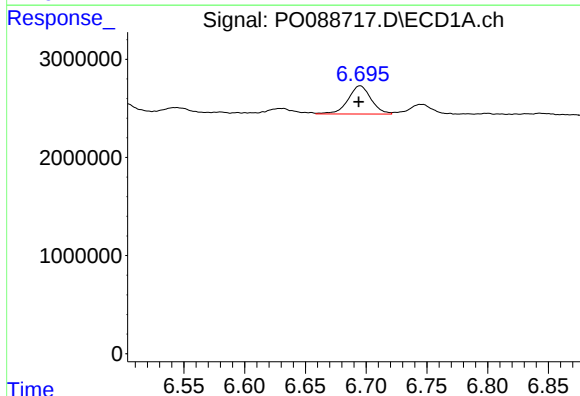


#27 AR-1254-2

R.T.: 6.695 min
Delta R.T.: 0.001 min
Response: 3769360
Conc: 27.56 ng/ml

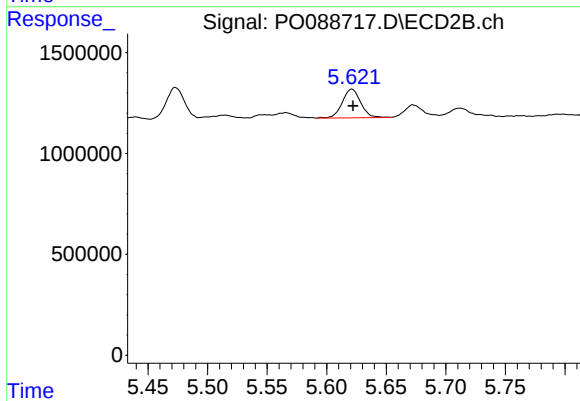

#27 AR-1254-2


R.T.: 5.621 min
Delta R.T.: -0.001 min
Response: 1546400
Conc: 26.11 ng/ml

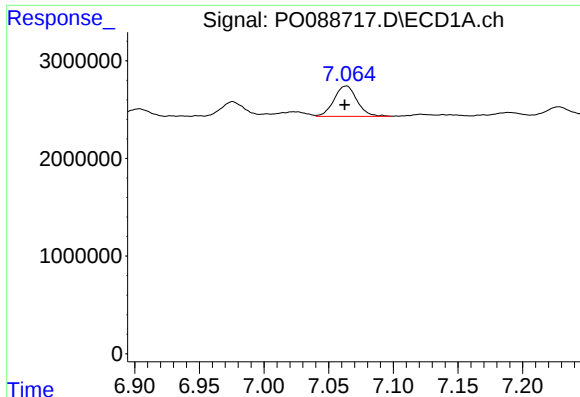

#28 AR-1254-3


R.T.: 7.064 min
Delta R.T.: 0.001 min
Response: 3870584
Conc: 27.50 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2022

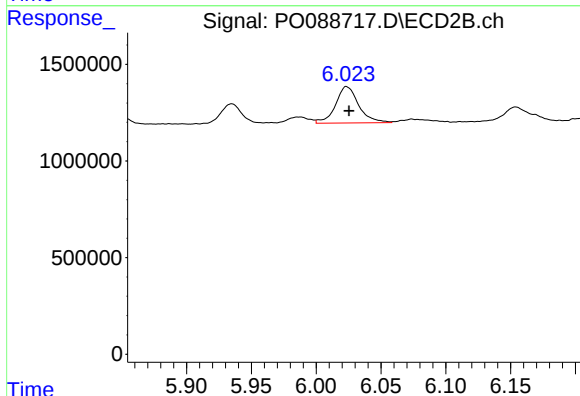


#28 AR-1254-3

R.T.: 6.024 min
Delta R.T.: -0.002 min
Response: 2343080
Conc: 25.20 ng/ml

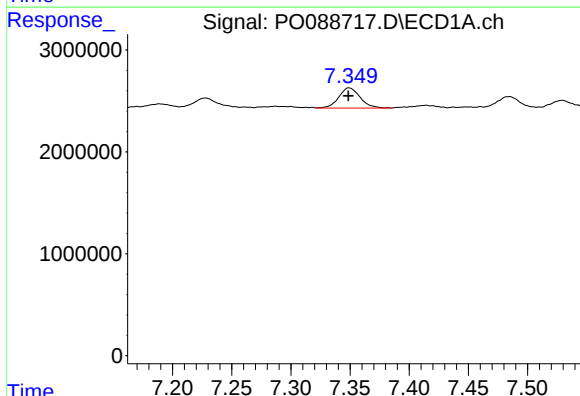


#29 AR-1254-4

R.T.: 7.349 min
Delta R.T.: 0.000 min
Response: 2476413
Conc: 24.51 ng/ml

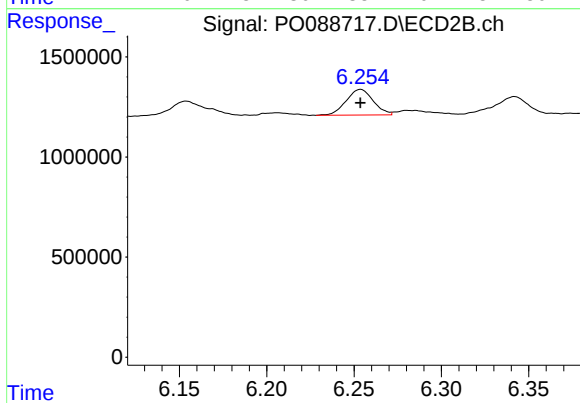

#29 AR-1254-4


R.T.: 6.254 min
Delta R.T.: 0.000 min
Response: 1392225
Conc: 24.58 ng/ml

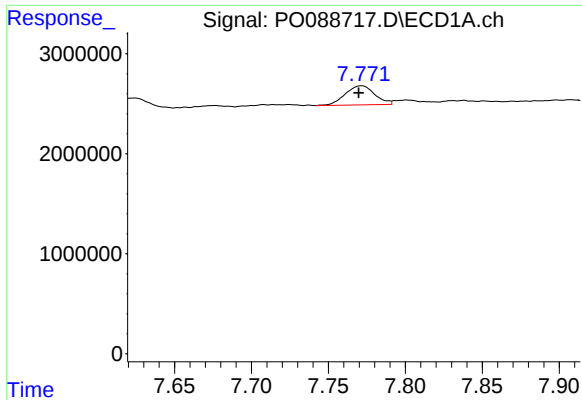

#30 AR-1254-5

R.T.: 7.771 min
Delta R.T.: 0.002 min
Response: 2547574
Conc: 23.92 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2022

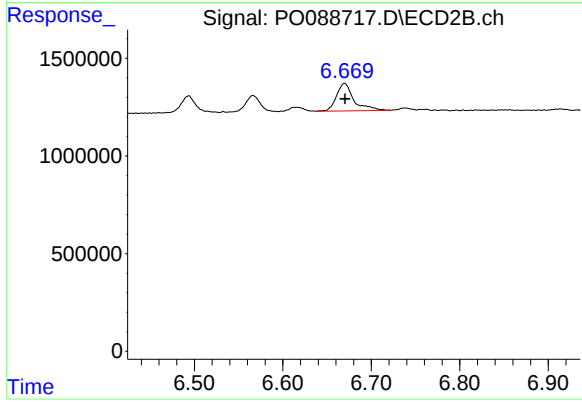

#30 AR-1254-5

R.T.: 6.670 min
Delta R.T.: 0.000 min
Response: 1949162
Conc: 23.88 ng/ml