

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080823\
 Data File : P0096793.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Aug 2023 23:05
 Operator : YP/AJ
 Sample : 03572-07
 Misc : AR1232 LOD 25 PPB
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 09 01:34:13 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0080723.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 08 04:34:41 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.411	3.620	67299106	26795479	20.331	20.241
2) SA Decachlor...	10.351	8.642	50230770	26857044	22.955	23.214
Target Compounds						
11) L3 AR-1232-1	4.788	3.996	1985123	777871	27.218	24.048
12) L3 AR-1232-2	5.325	4.725	1221255	728991	30.804	25.266
13) L3 AR-1232-3	5.620	4.903	1543270	415651	25.228	27.414
14) L3 AR-1232-4	5.783	4.987	724996	347741	23.760	23.269m
15) L3 AR-1232-5	5.877	5.155	749680	426298	26.790	26.078m



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO080823\
Data File : PO096793.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Aug 2023 23:05
Operator : YP/AJ
Sample : 03572-07
Misc : AR1232 LOD 25 PPB
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 09 01:34:13 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO080723.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 08 04:34:41 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

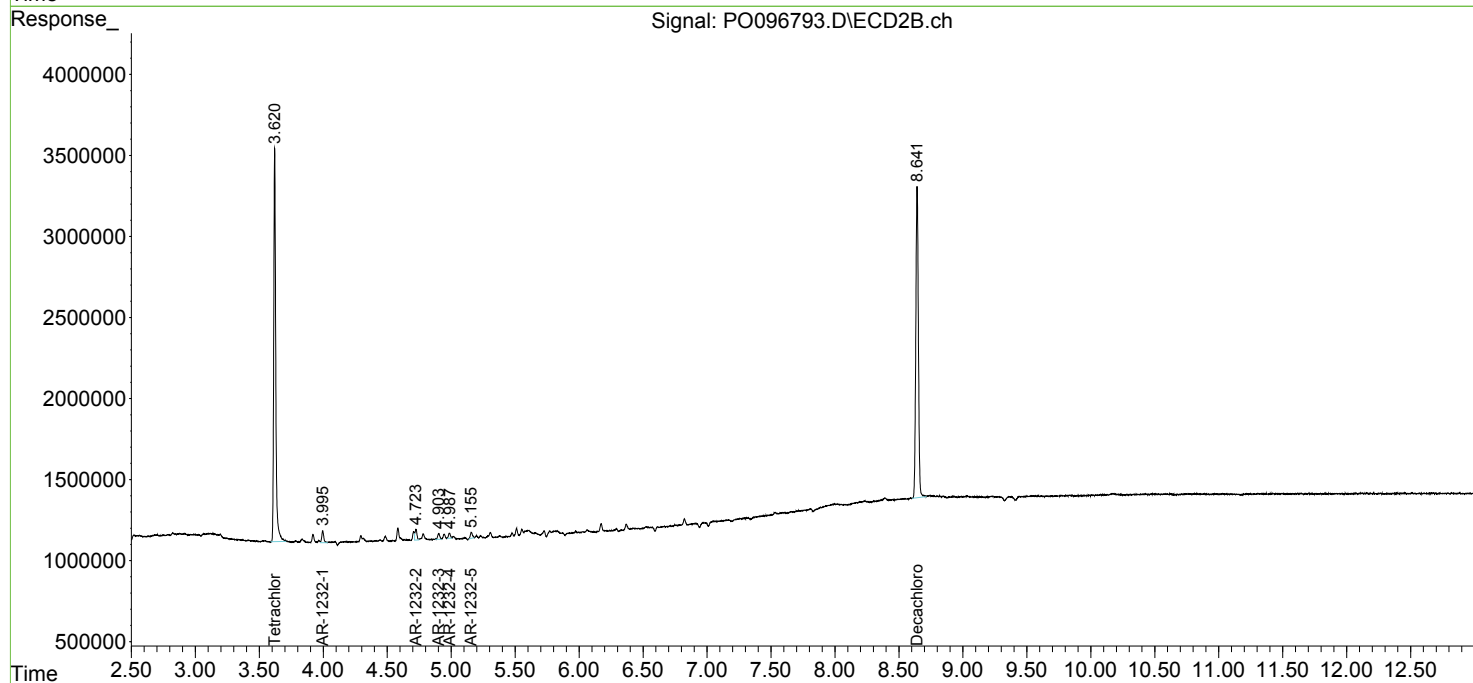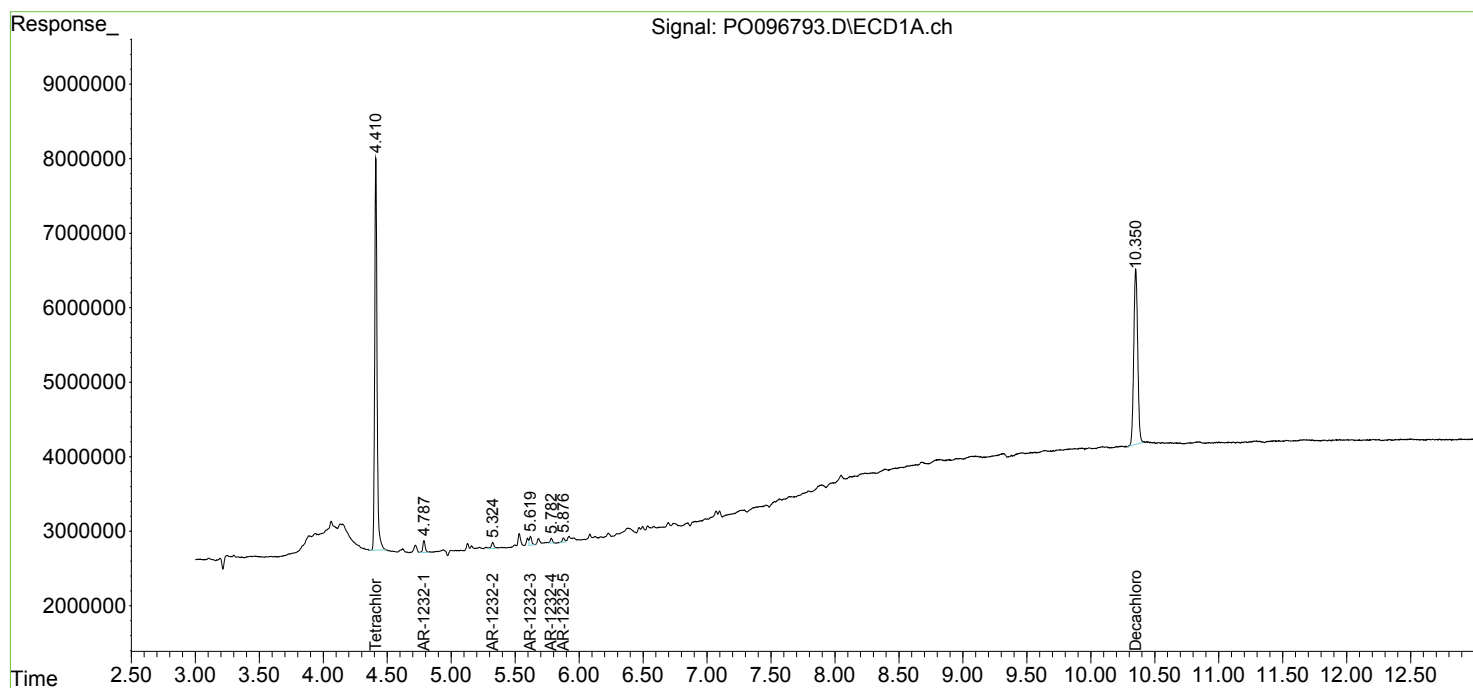


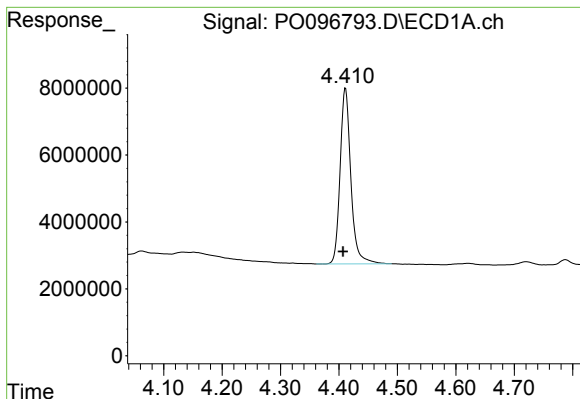

#1 Tetrachloro-m-xylene


R.T.: 4.411 min
Delta R.T.: 0.004 min
Response: 67299106
Conc: 20.33 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

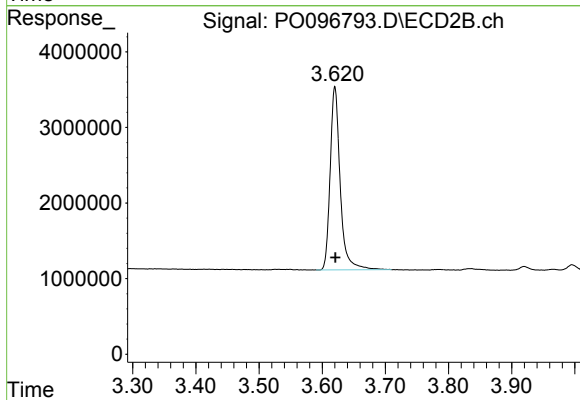


#1 Tetrachloro-m-xylene

R.T.: 3.620 min
Delta R.T.: 0.000 min
Response: 26795479
Conc: 20.24 ng/ml

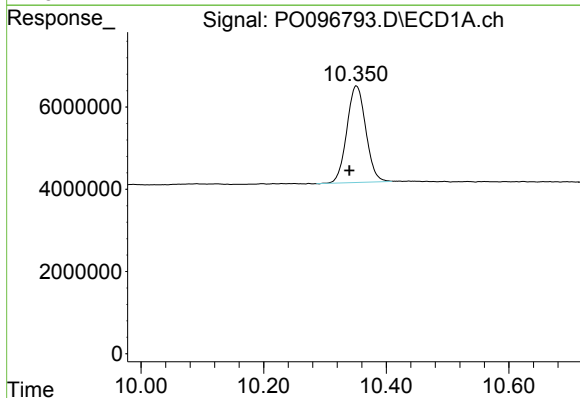


#2 Decachlorobiphenyl

R.T.: 10.351 min
Delta R.T.: 0.012 min
Response: 50230770
Conc: 22.96 ng/ml

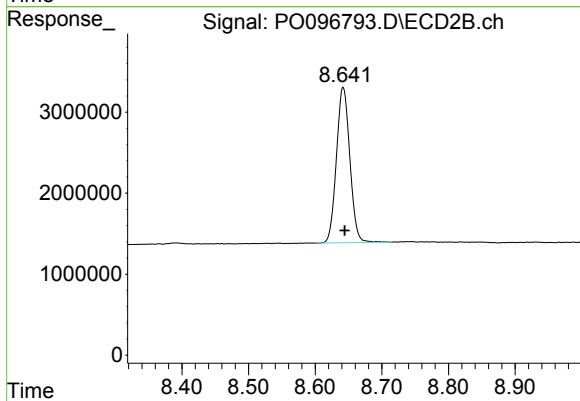

#2 Decachlorobiphenyl


R.T.: 8.642 min
Delta R.T.: -0.002 min
Response: 26857044
Conc: 23.21 ng/ml

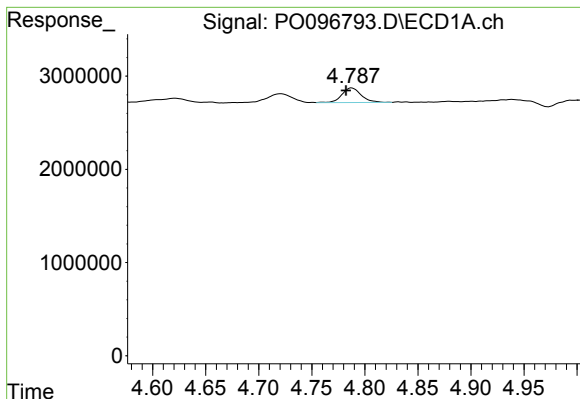

#11 AR-1232-1


R.T.: 4.788 min
Delta R.T.: 0.005 min
Response: 1985123
Conc: 27.22 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

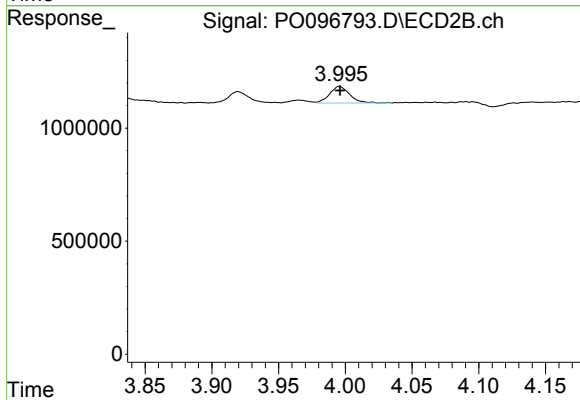


#11 AR-1232-1

R.T.: 3.996 min
Delta R.T.: 0.000 min
Response: 777871
Conc: 24.05 ng/ml

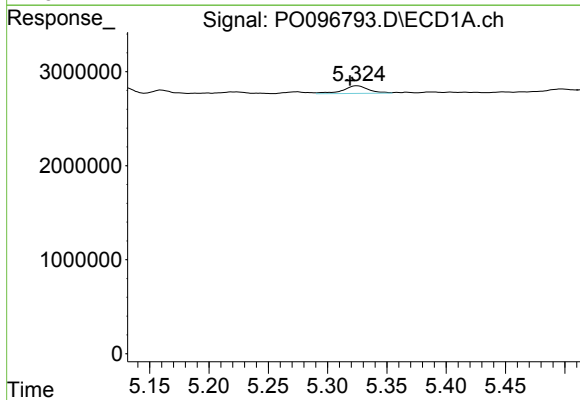


#12 AR-1232-2

R.T.: 5.325 min
Delta R.T.: 0.006 min
Response: 1221255
Conc: 30.80 ng/ml

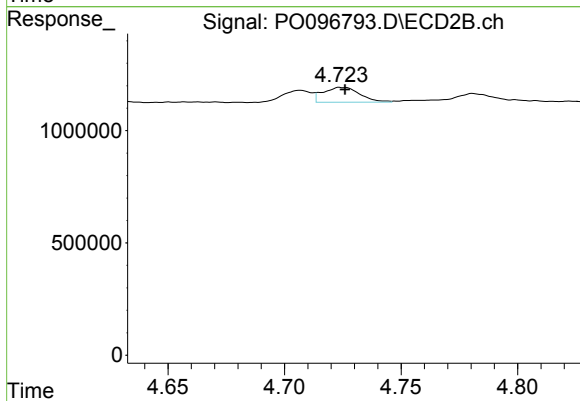

#12 AR-1232-2


R.T.: 4.725 min
Delta R.T.: -0.001 min
Response: 728991
Conc: 25.27 ng/ml

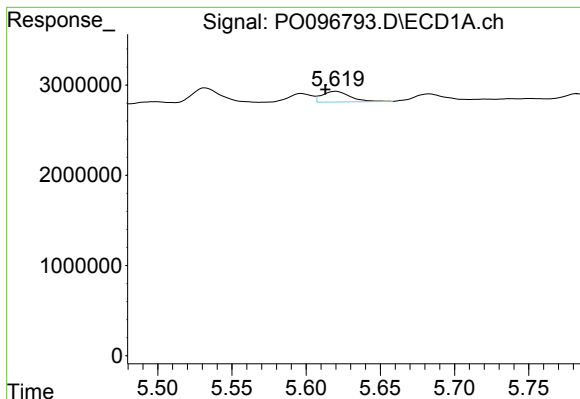

#13 AR-1232-3


R.T.: 5.620 min
Delta R.T.: 0.007 min
Response: 1543270
Conc: 25.23 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

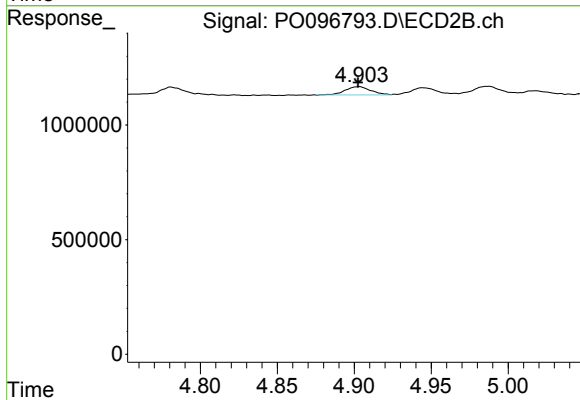


#13 AR-1232-3

R.T.: 4.903 min
Delta R.T.: 0.000 min
Response: 415651
Conc: 27.41 ng/ml

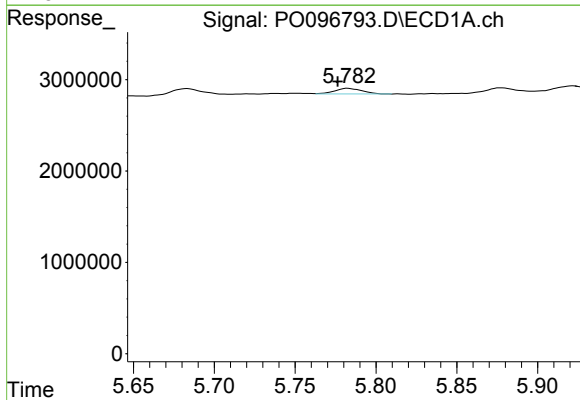


#14 AR-1232-4

R.T.: 5.783 min
Delta R.T.: 0.006 min
Response: 724996
Conc: 23.76 ng/ml

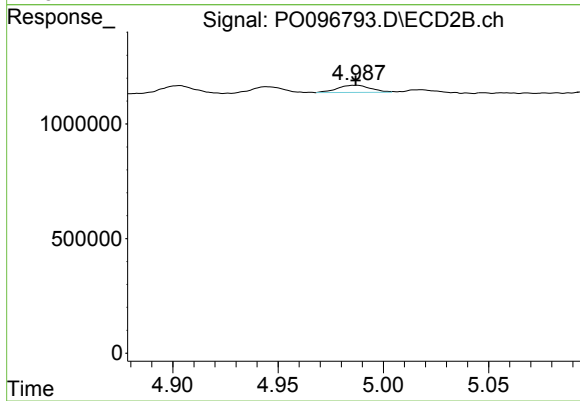

#14 AR-1232-4


R.T.: 4.987 min
Delta R.T.: 0.000 min
Response: 347741
Conc: 23.27 ng/ml m

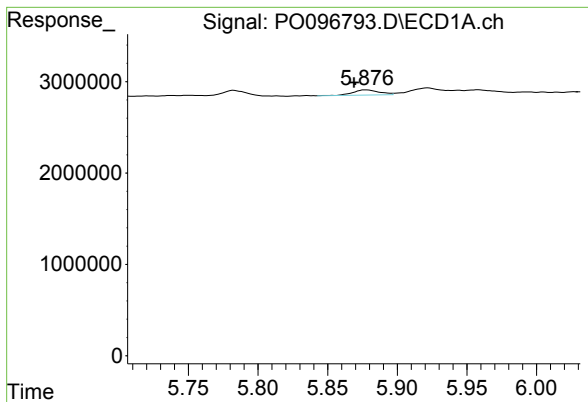

#15 AR-1232-5

R.T.: 5.877 min
Delta R.T.: 0.008 min
Response: 749680
Conc: 26.79 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

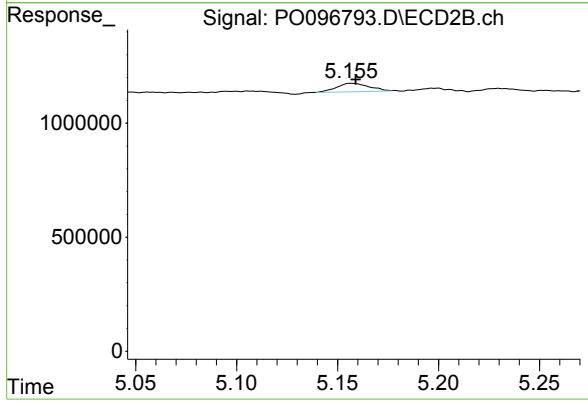

#15 AR-1232-5

R.T.: 5.155 min
Delta R.T.: -0.004 min
Response: 426298
Conc: 26.08 ng/ml m