

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080824\
 Data File : P0105293.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Aug 2024 13:01
 Operator : YP/AJ
 Sample : P3508-07 10X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TERMINATOR

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/09/2024
 Supervised By :Ankita Jodhani 08/09/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 08 13:24:20 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072924.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 30 07:11:20 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.428	3.537	8285723	3202385	1.204m	1.257
2) SA Decachlor...	10.196	8.426	162.2E6	2531881	31.588m	1.594m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO080824\
Data File : PO105293.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Aug 2024 13:01
Operator : YP/AJ
Sample : P3508-07 10X
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TERMINATOR


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/09/2024
Supervised By :Ankita Jodhani 08/09/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 08 13:24:20 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO072924.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 30 07:11:20 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

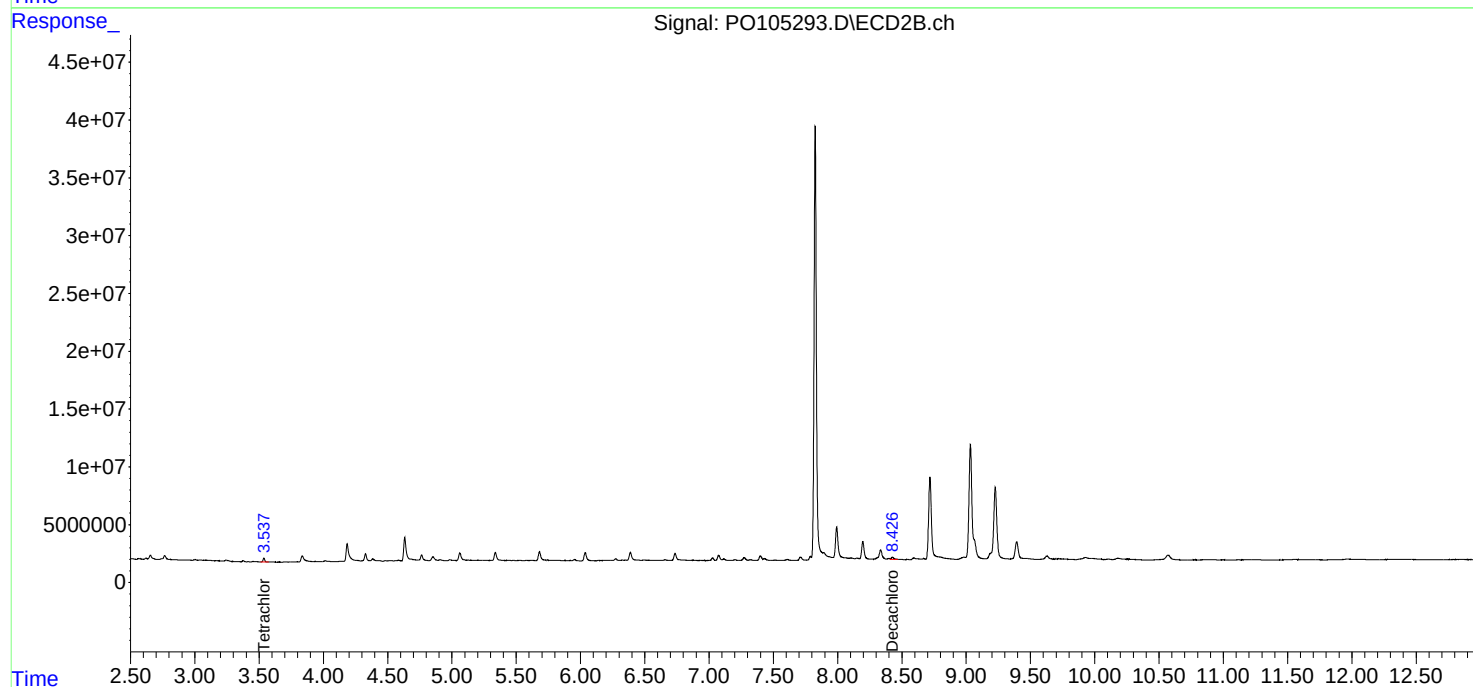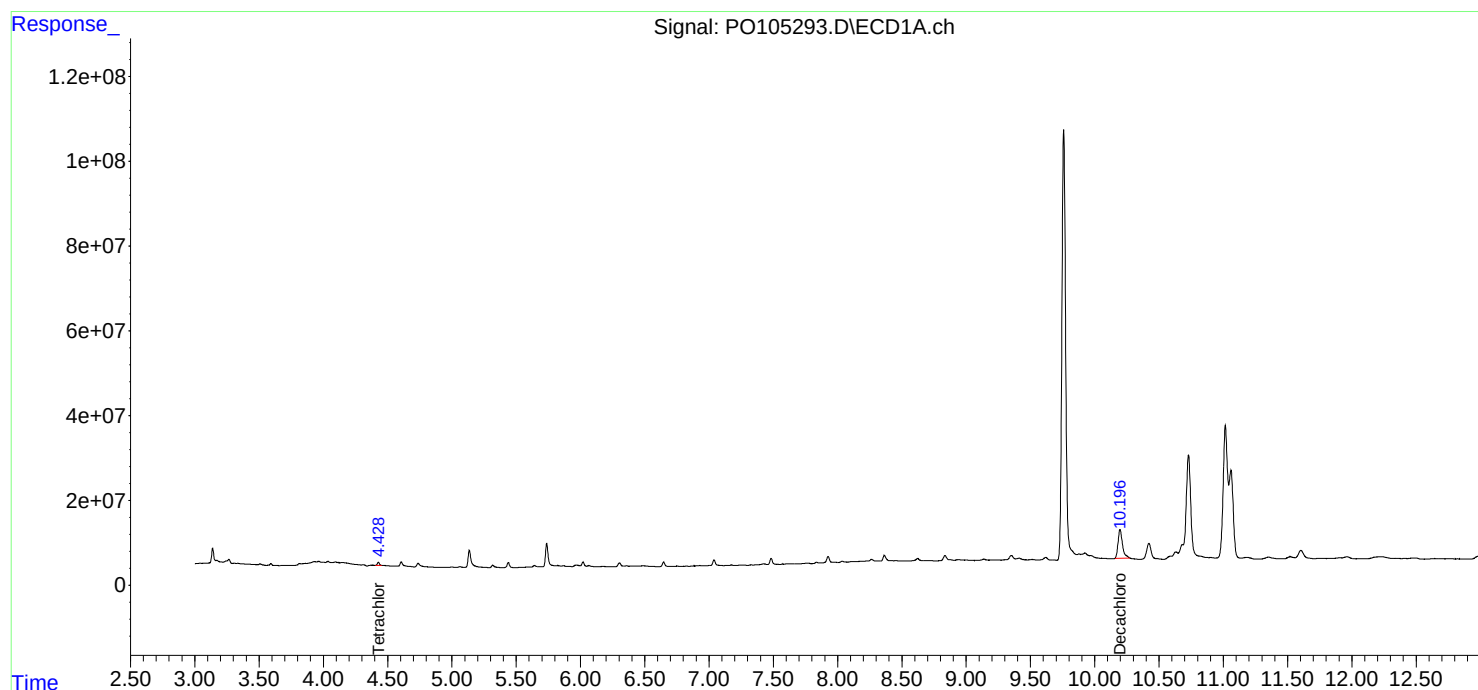

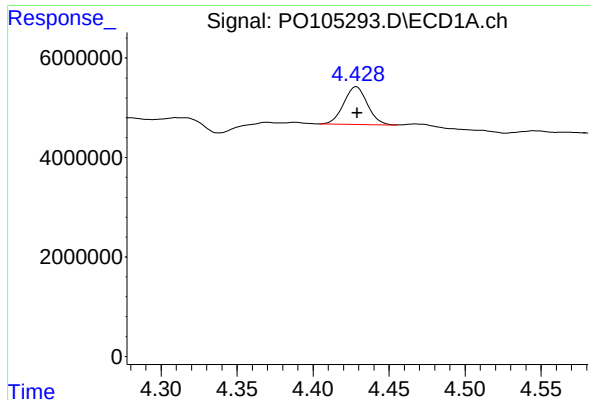


#1 Tetrachloro-m-xylene

R.T.: 4.428 min
Delta R.T.: -0.001 min
Response: 8285723
Conc: 1.20 ng/ml

Instrument :
ECD_O
ClientSampleId :
TERMINATOR


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/09/2024
Supervised By :Ankita Jodhani 08/09/2024

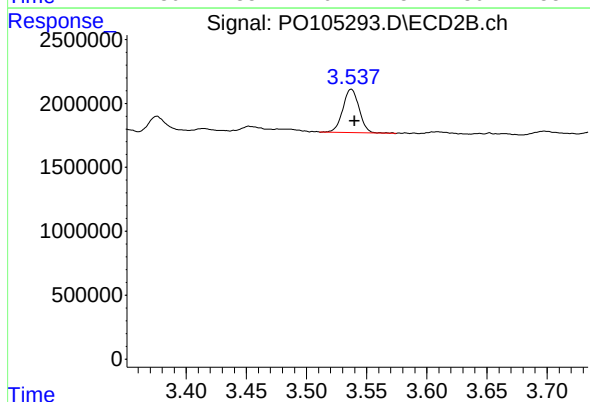


#1 Tetrachloro-m-xylene

R.T.: 3.537 min
Delta R.T.: -0.003 min
Response: 3202385
Conc: 1.26 ng/ml

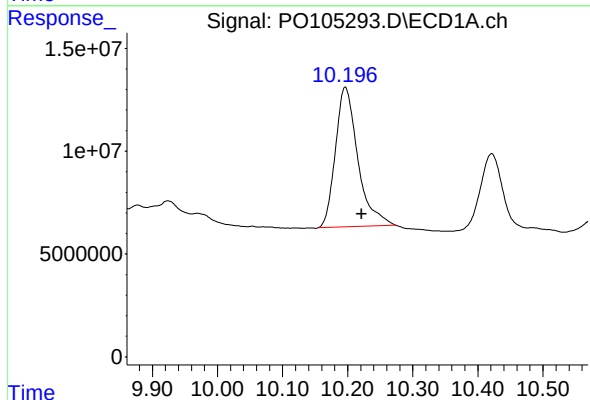

#2 Decachlorobiphenyl

R.T.: 10.196 min
Delta R.T.: -0.026 min
Response: 162170437
Conc: 31.59 ng/ml m

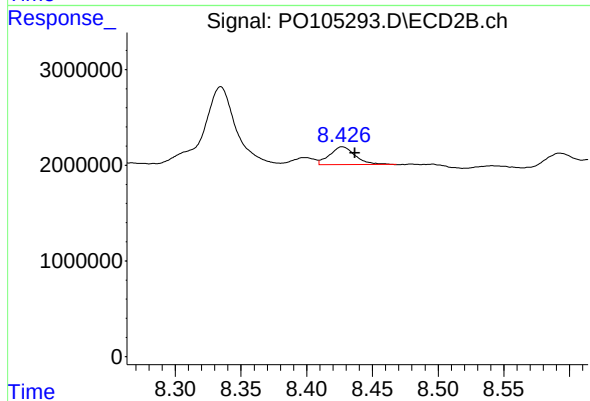

#2 Decachlorobiphenyl

R.T.: 8.426 min
Delta R.T.: -0.010 min
Response: 2531881
Conc: 1.59 ng/ml m