

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080918\
Data File : P0047865.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Aug 2018 10:26
Operator : SM/SJ
Sample : J4377-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
01-01-WINDOW-CAULKING-HALLW

Manual Integrations
APPROVED

Sohil
8/10/2018 4:14:00 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 09 10:45:03 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072718.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 27 02:33:29 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.395	3.638	5555247	5393128	27.515	21.949m
2)	SA Decachlor...	10.088	8.626	3675072	3522140	22.533	22.407

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080918\
Data File : P0047865.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Aug 2018 10:26
Operator : SM/SJ
Sample : J4377-01
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
01-01-WINDOW-CAULKING-HALLW


Manual Integrations
APPROVED

Sohil
8/10/2018 4:14:00 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 09 10:45:03 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072718.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 27 02:33:29 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

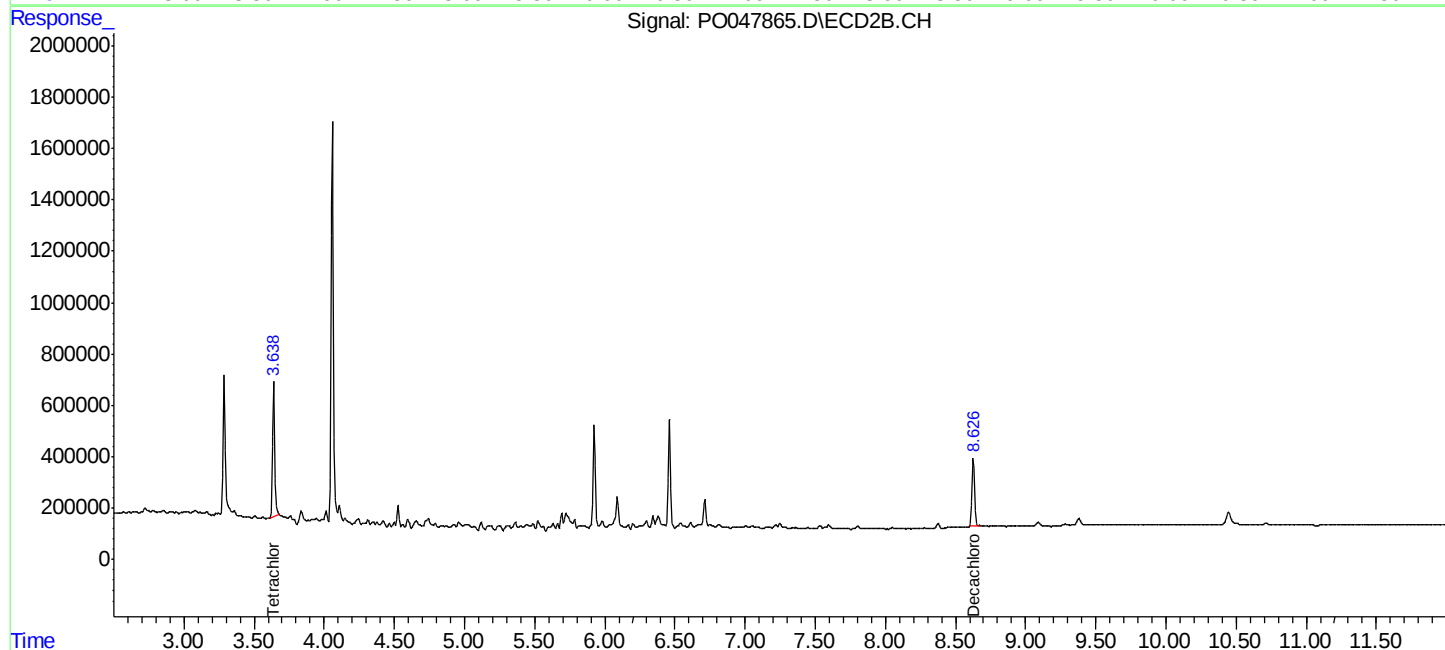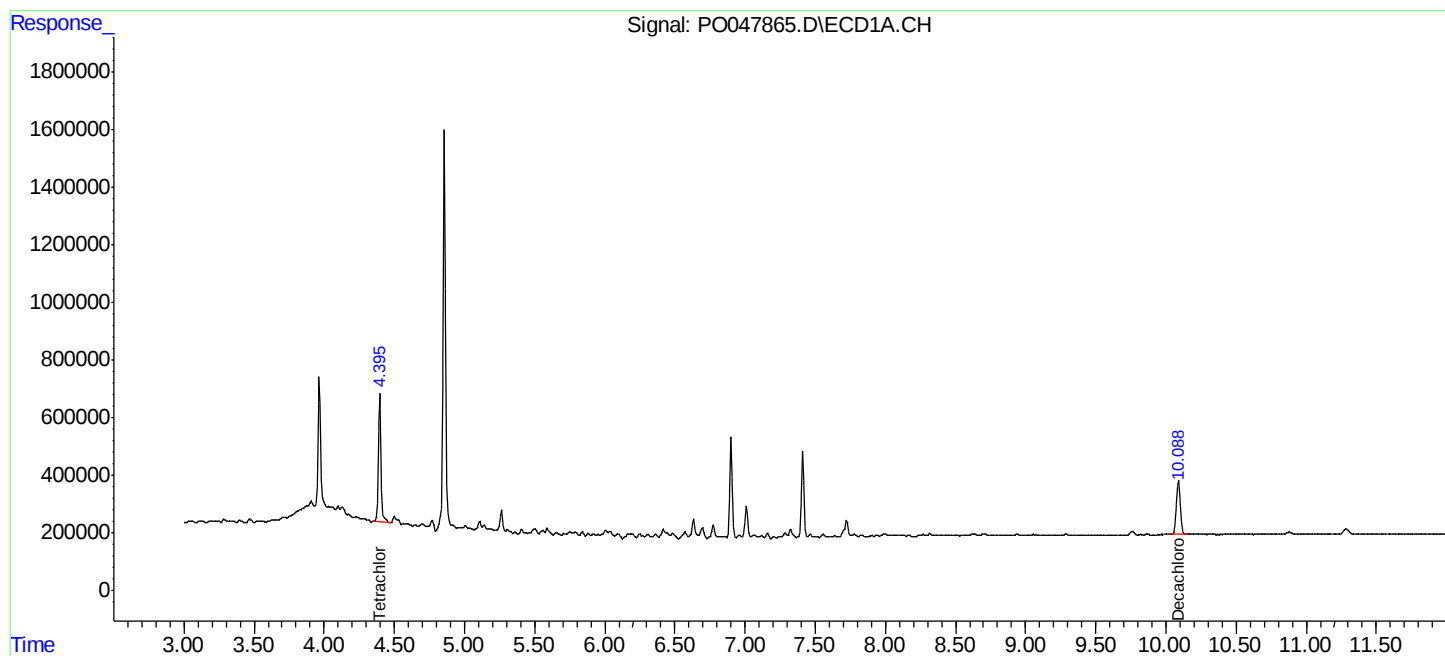

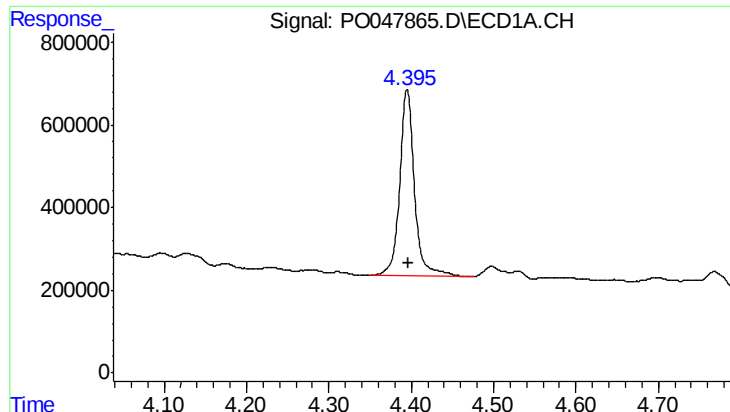


#1 Tetrachloro-m-xylene

R.T.: 4.395 min
Delta R.T.: -0.002 min
Response: 5555247
Conc: 27.52 ng/ml

Instrument :
ECD_O
ClientSampleId :
01-01-WINDOW-CAULKING-HALLW


Manual Integrations
APPROVED

Sohil
8/10/2018 4:14:00 PM

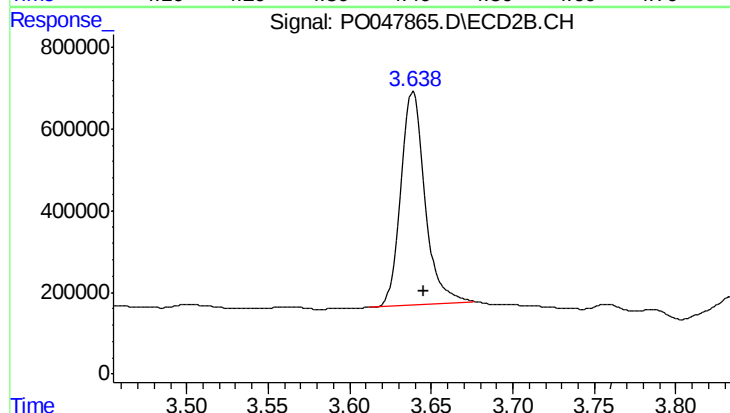


#1 Tetrachloro-m-xylene

R.T.: 3.638 min
Delta R.T.: -0.007 min
Response: 5393128
Conc: 21.95 ng/ml m

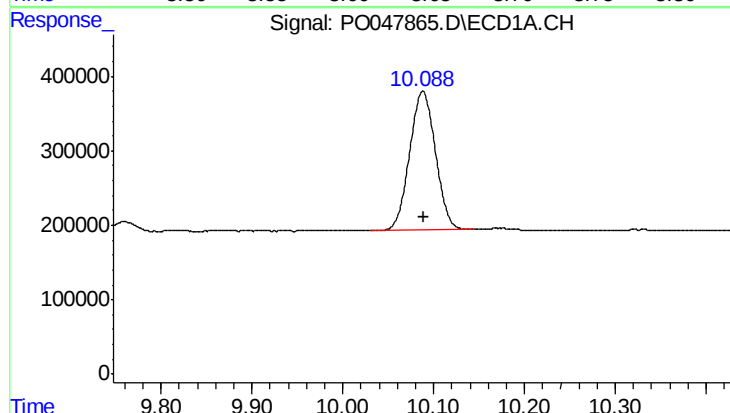

#2 Decachlorobiphenyl

R.T.: 10.088 min
Delta R.T.: -0.002 min
Response: 3675072
Conc: 22.53 ng/ml

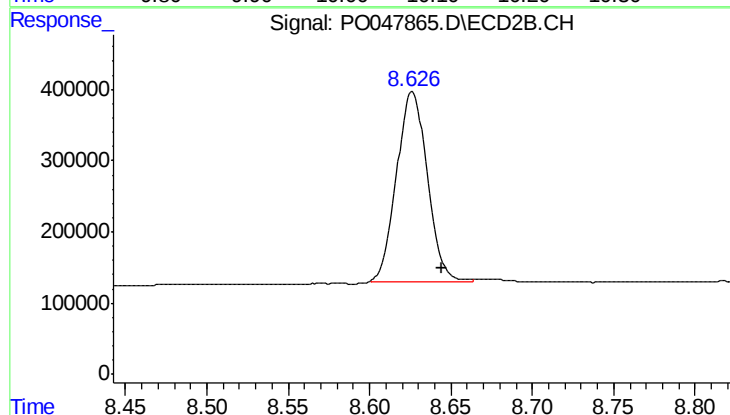

#2 Decachlorobiphenyl

R.T.: 8.626 min
Delta R.T.: -0.018 min
Response: 3522140
Conc: 22.41 ng/ml