

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0080918\
Data File : P0047889.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Aug 2018 21:23
Operator : SM/SJ
Sample : J4395-01
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FK-BPM-01-E7-F7-E7A-F7A

Manual Integrations
APPROVED

Sohil
8/10/2018 4:14:51 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 10 08:10:24 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072718.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 27 02:33:29 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.394	3.638	5213653	6609190	25.823	26.898
2) SA Decachlor...	10.087	8.626	3136699	3104299	19.232	19.748m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080918\
Data File : P0047889.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Aug 2018 21:23
Operator : SM/SJ
Sample : J4395-01
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
FK-BPM-01-E7-F7-E7A-F7A


Manual Integrations
APPROVED

Sohil
8/10/2018 4:14:51 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 10 08:10:24 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072718.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 27 02:33:29 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

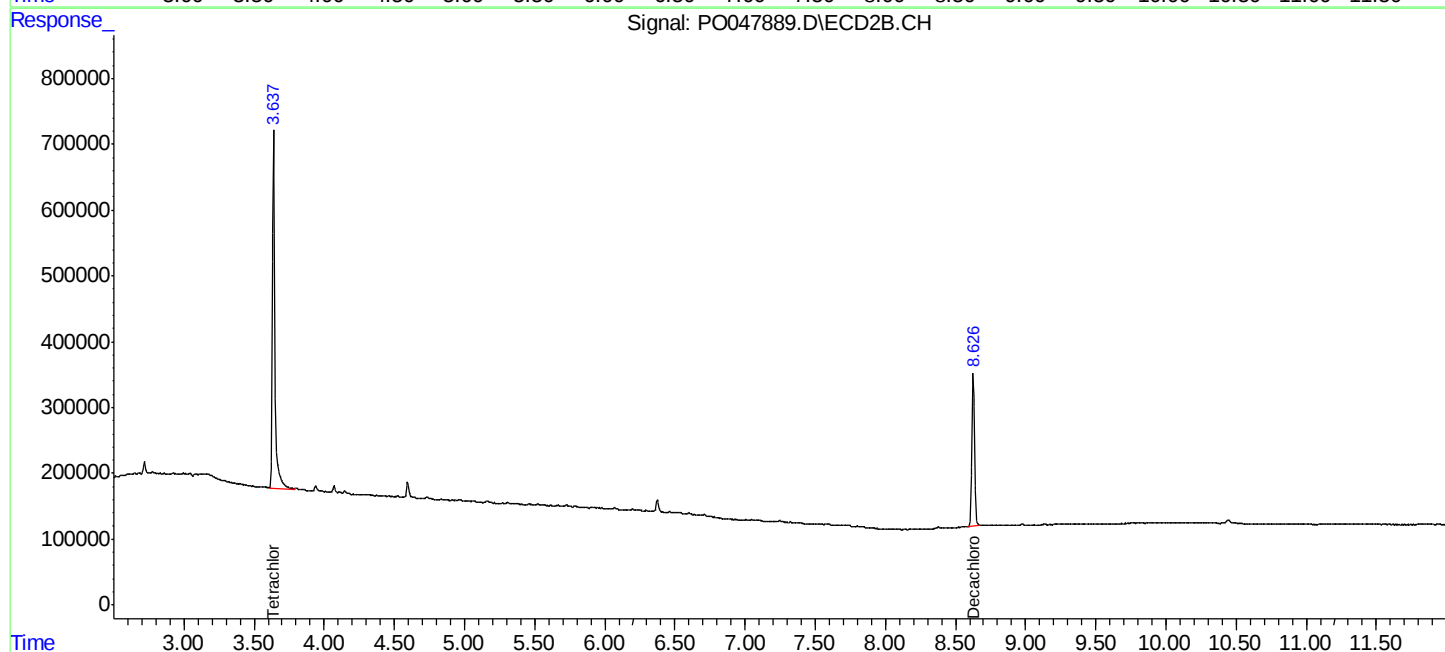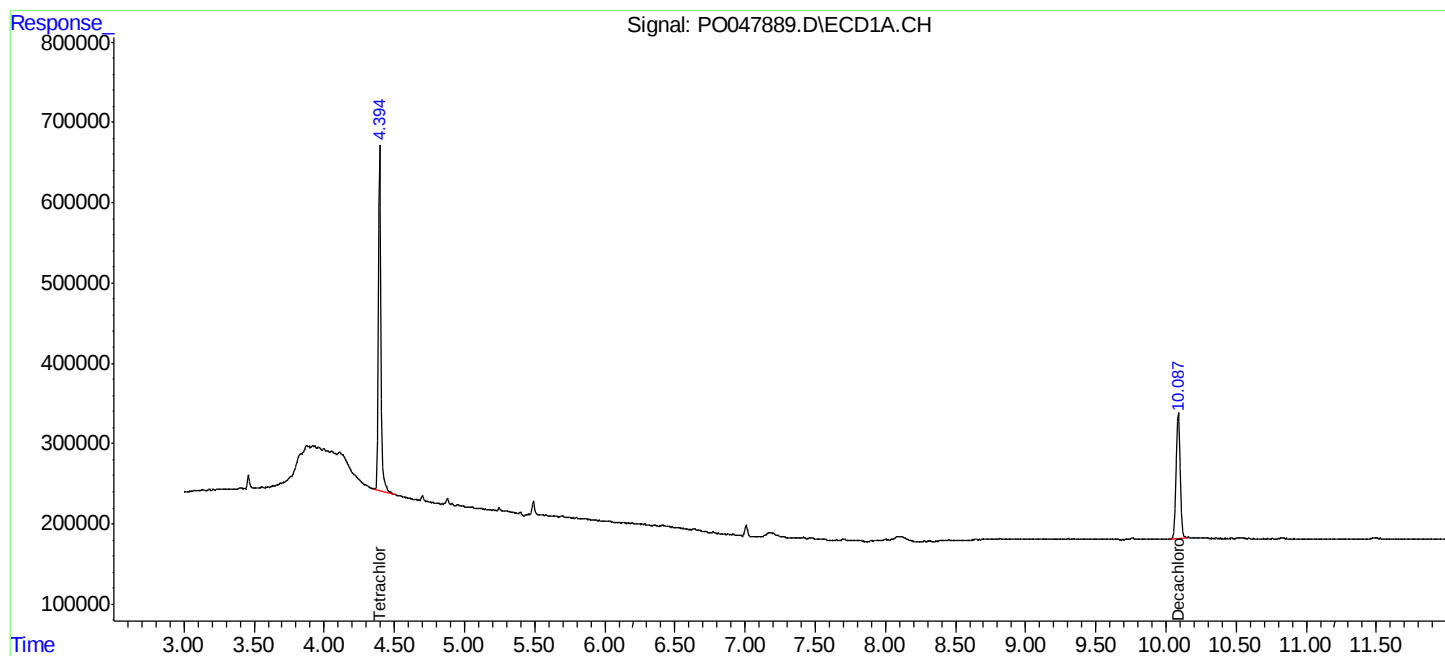

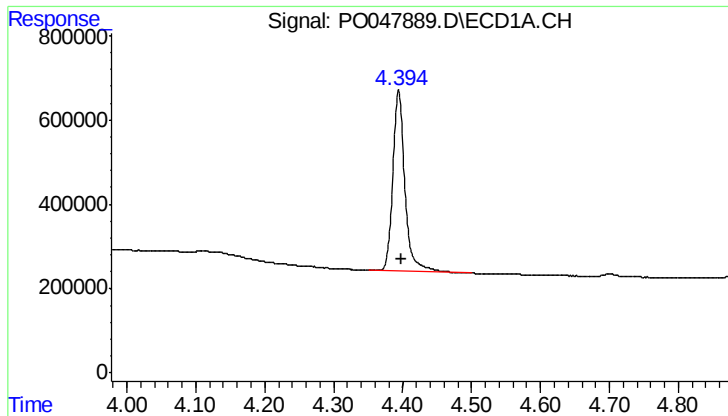


#1 Tetrachloro-m-xylene

R.T.: 4.394 min
Delta R.T.: -0.003 min
Response: 5213653
Conc: 25.82 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-01-E7-F7-E7A-F7A


Manual Integrations
APPROVED

Sohil
8/10/2018 4:14:51 PM

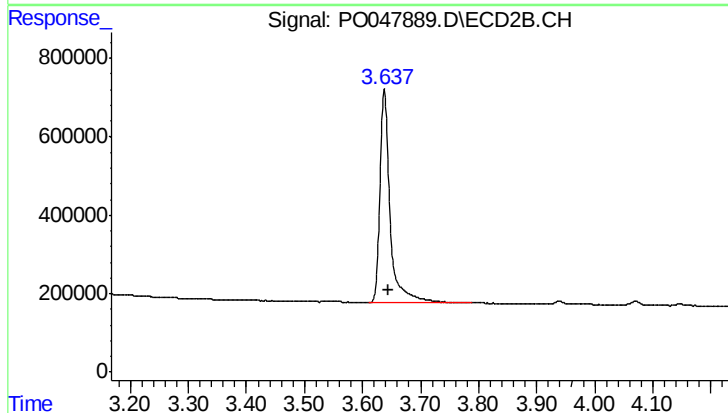


#1 Tetrachloro-m-xylene

R.T.: 3.638 min
Delta R.T.: -0.008 min
Response: 6609190
Conc: 26.90 ng/ml

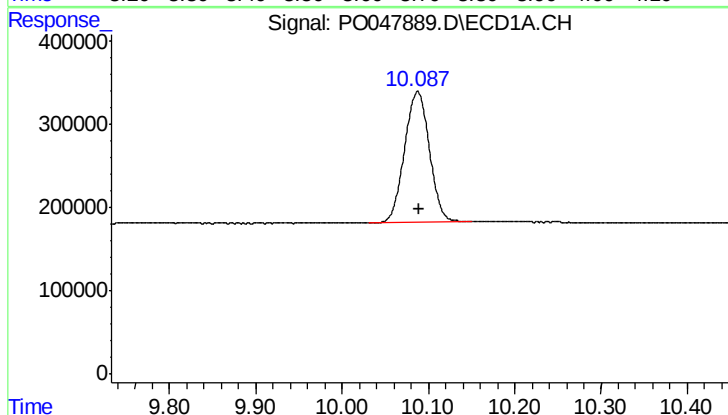

#2 Decachlorobiphenyl

R.T.: 10.087 min
Delta R.T.: -0.002 min
Response: 3136699
Conc: 19.23 ng/ml

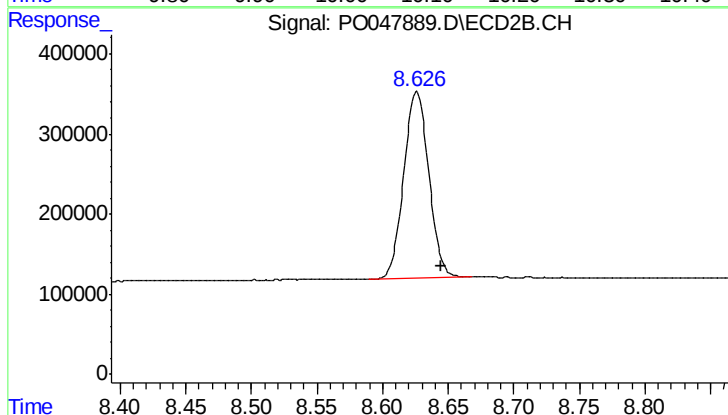

#2 Decachlorobiphenyl

R.T.: 8.626 min
Delta R.T.: -0.019 min
Response: 3104299
Conc: 19.75 ng/ml m