

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0080918\
Data File : P0047890.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Aug 2018 21:39
Operator : SM/SJ
Sample : J4396-01
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FK-BPM-01-E8-F8-E8A-F8A

Manual Integrations
APPROVED

Sohil
8/10/2018 4:14:52 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 10 08:10:49 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072718.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 27 02:33:29 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.395	3.638	4719694	5830429	23.377	23.728
2) SA Decachlor...	10.089	8.625	2862939	2855407	17.553	18.165m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080918\
Data File : P0047890.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Aug 2018 21:39
Operator : SM/SJ
Sample : J4396-01
Misc :
ALS Vial : 25 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
FK-BPM-01-E8-F8-E8A-F8A


Manual Integrations
APPROVED

Sohil
8/10/2018 4:14:52 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 10 08:10:49 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072718.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 27 02:33:29 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

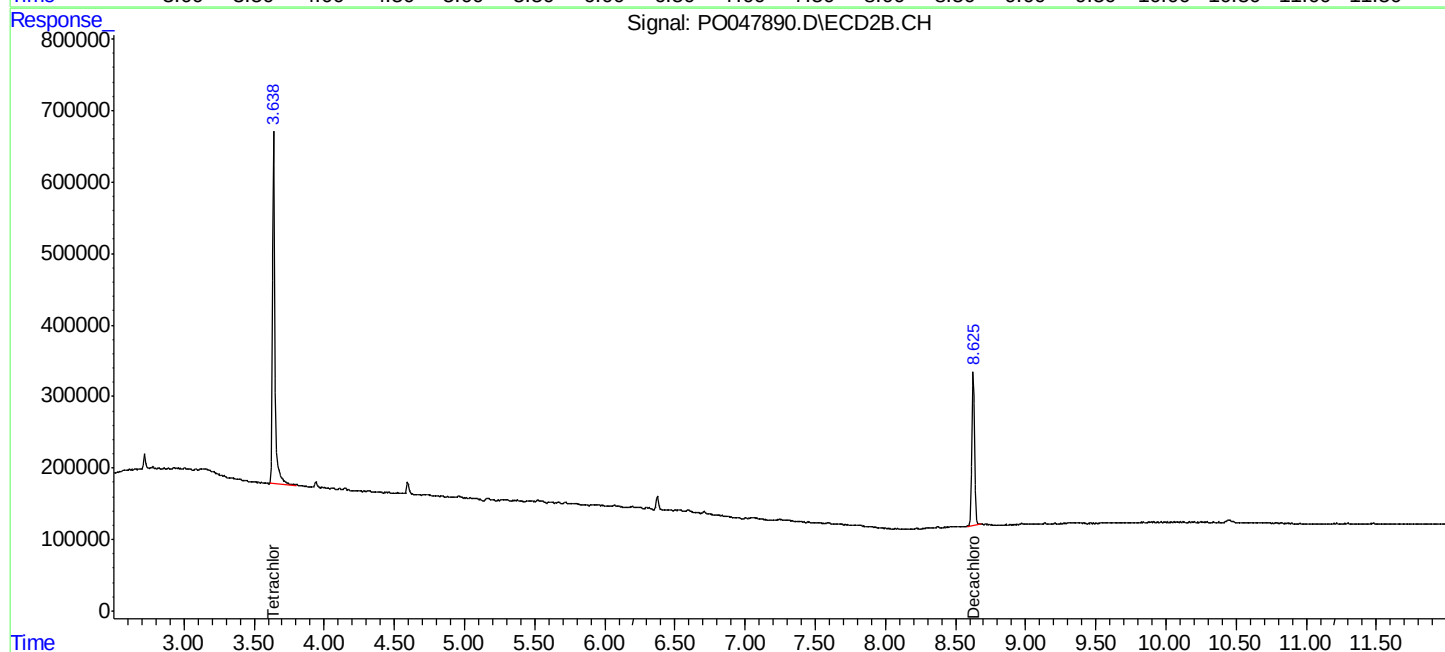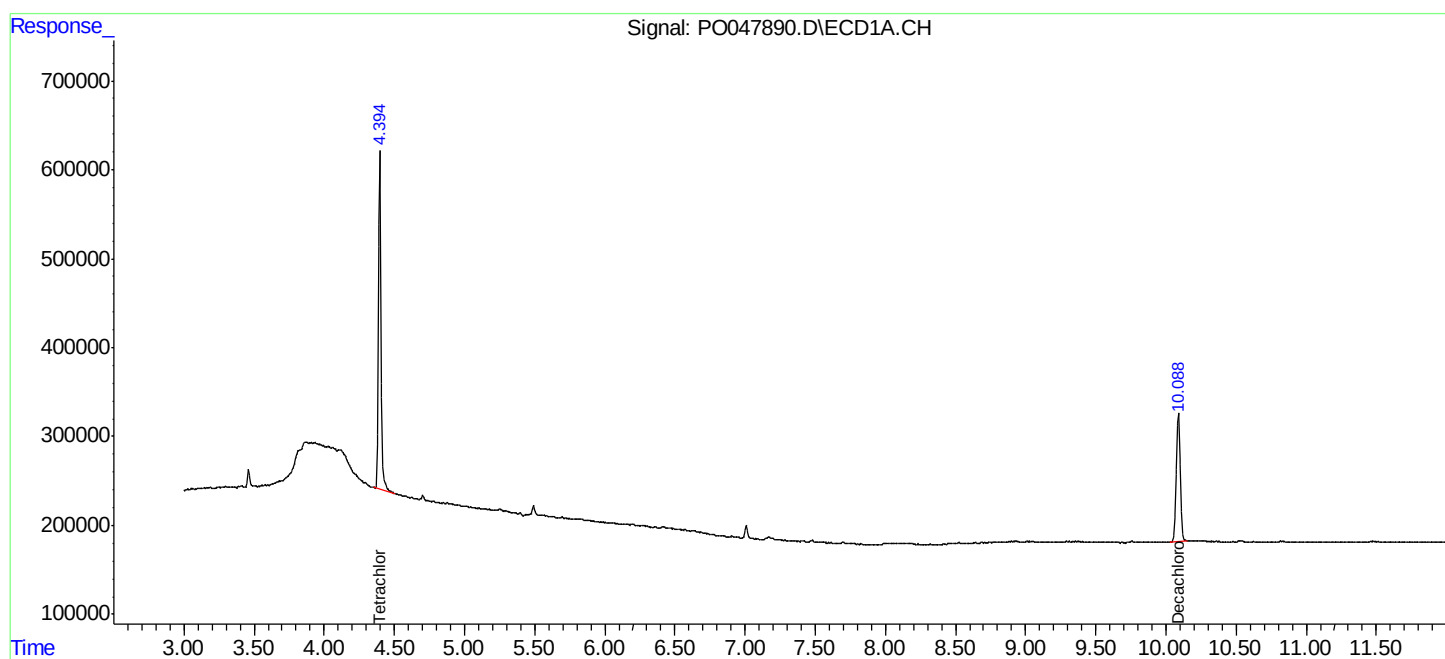

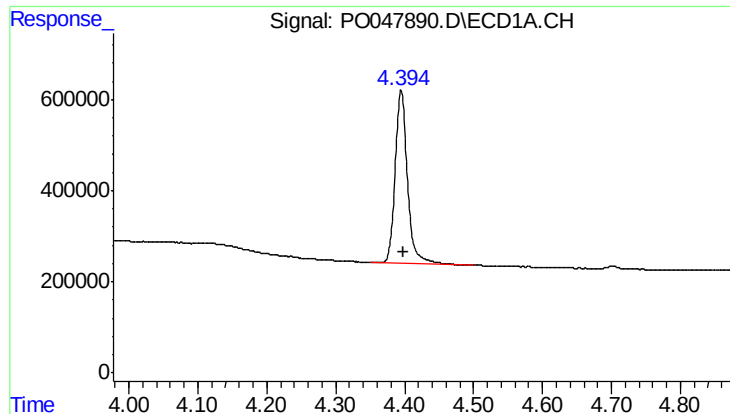


#1 Tetrachloro-m-xylene

R.T.: 4.395 min
Delta R.T.: -0.002 min
Response: 4719694
Conc: 23.38 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-01-E8-F8-E8A-F8A


Manual Integrations
APPROVED

Sohil
8/10/2018 4:14:52 PM

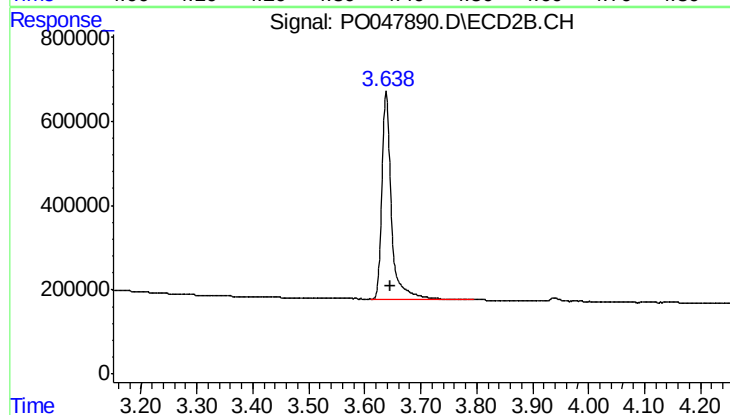


#1 Tetrachloro-m-xylene

R.T.: 3.638 min
Delta R.T.: -0.007 min
Response: 5830429
Conc: 23.73 ng/ml

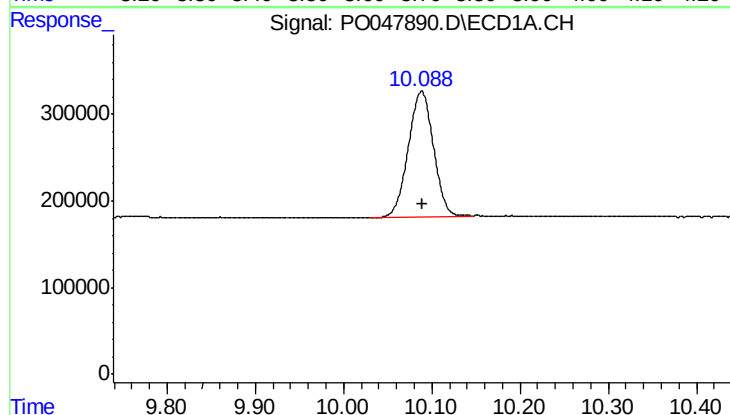

#2 Decachlorobiphenyl

R.T.: 10.089 min
Delta R.T.: -0.001 min
Response: 2862939
Conc: 17.55 ng/ml

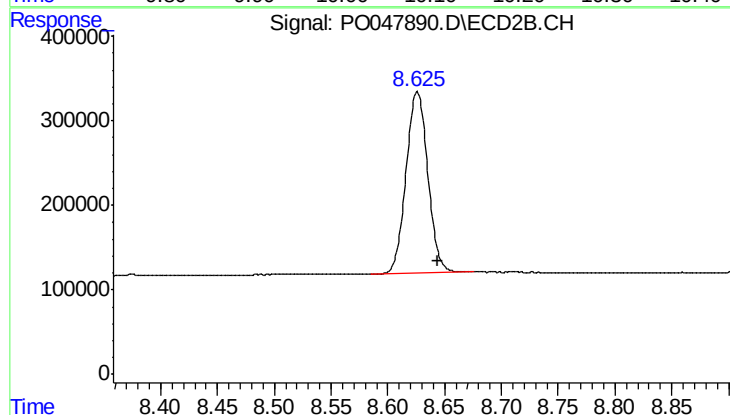

#2 Decachlorobiphenyl

R.T.: 8.625 min
Delta R.T.: -0.019 min
Response: 2855407
Conc: 18.17 ng/ml m