

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080922\
 Data File : P0088801.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Aug 2022 00:49
 Operator : YP/AJ
 Sample : N4106-20 10X
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BC216086-LOZ-END-1-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/10/2022
 Supervised By :Ankita Jodhani 08/10/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 10 03:06:34 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0080422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 05 23:24:09 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.436	3.594	5146720	1998012	1.908	1.846
2) SA Decachlor...	10.273	8.586	3220107	1830817	1.669	1.511m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO080922\
Data File : PO088801.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Aug 2022 00:49
Operator : YP/AJ
Sample : N4106-20 10X
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
BC216086-LOZ-END-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/10/2022
Supervised By :Ankita Jodhani 08/10/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 10 03:06:34 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO080422.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 05 23:24:09 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

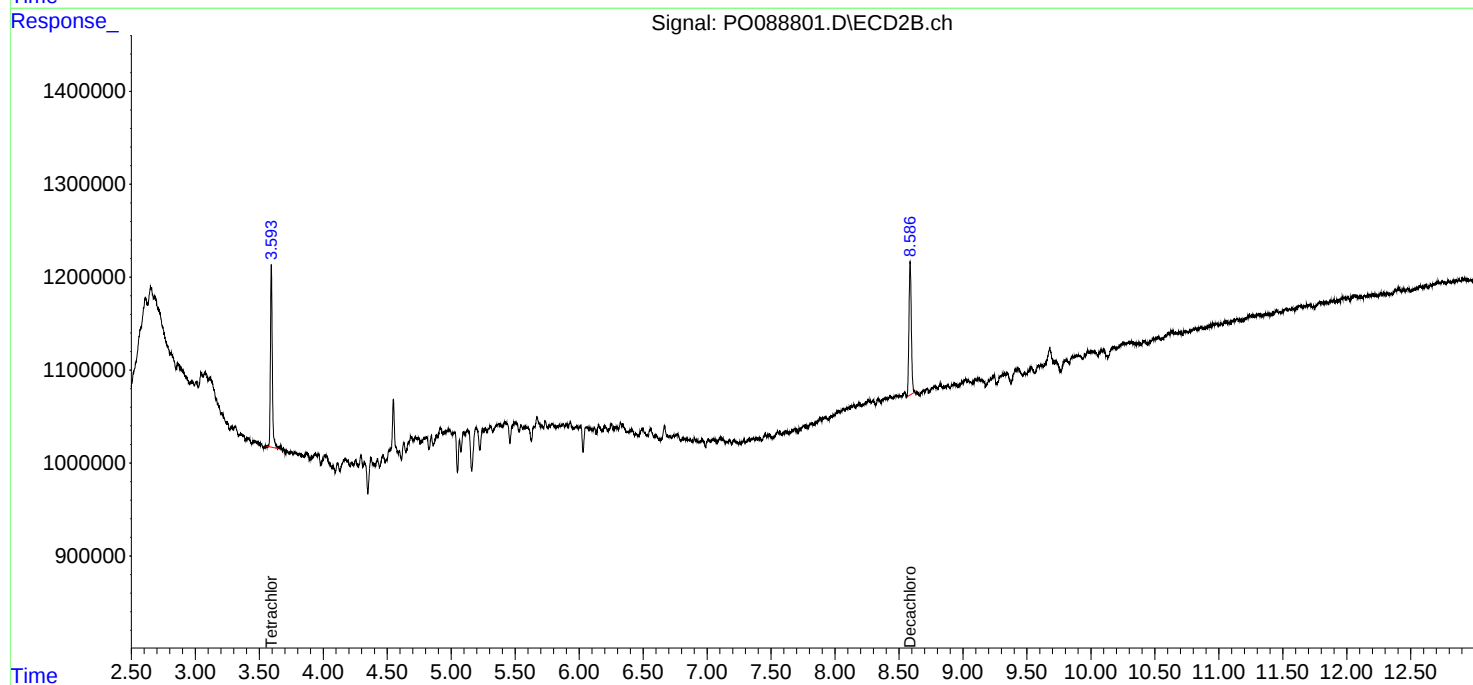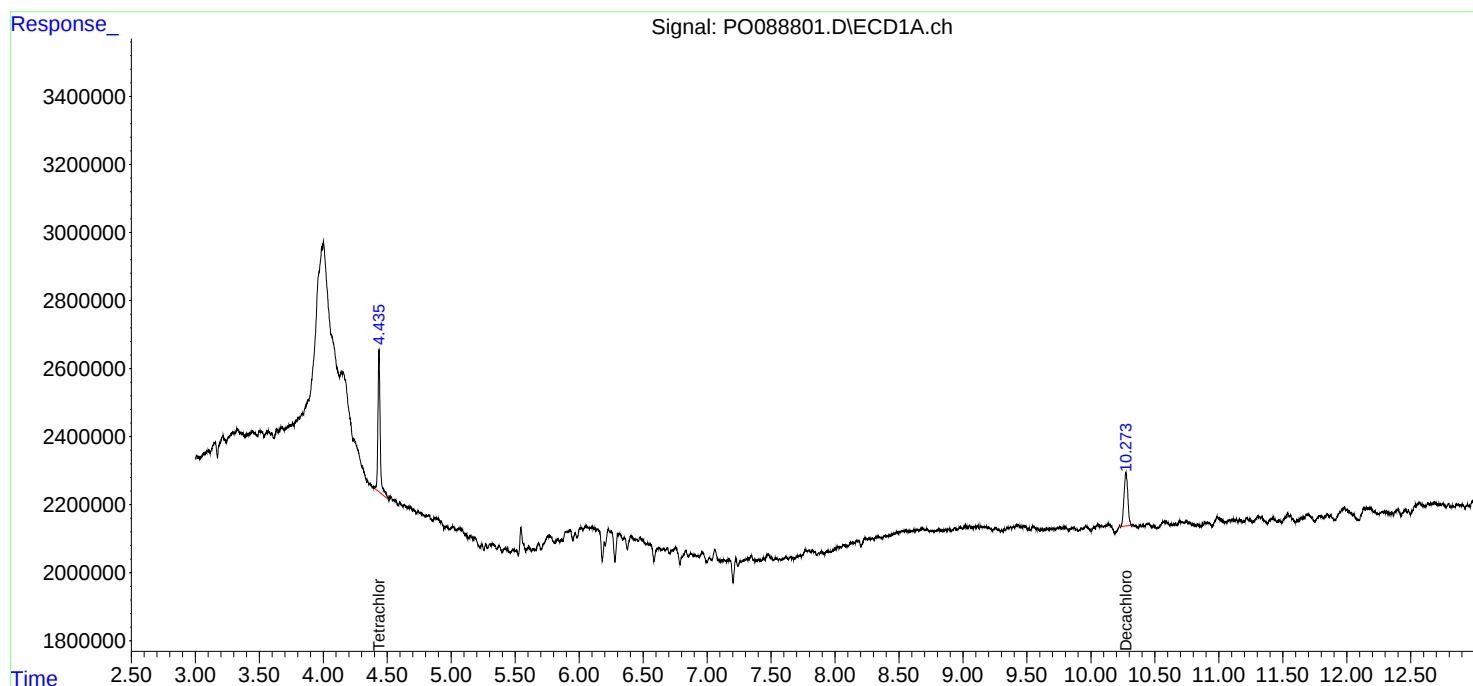

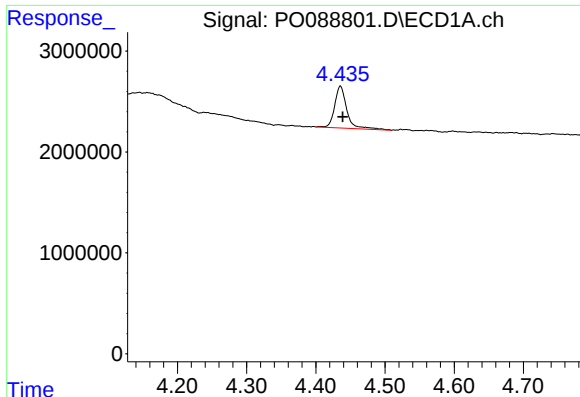


#1 Tetrachloro-m-xylene

R.T.: 4.436 min
Delta R.T.: -0.003 min
Response: 5146720
Conc: 1.91 ng/ml

Instrument :
ECD_O
ClientSampleId :
BC216086-LOZ-END-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/10/2022
Supervised By :Ankita Jodhani 08/10/2022

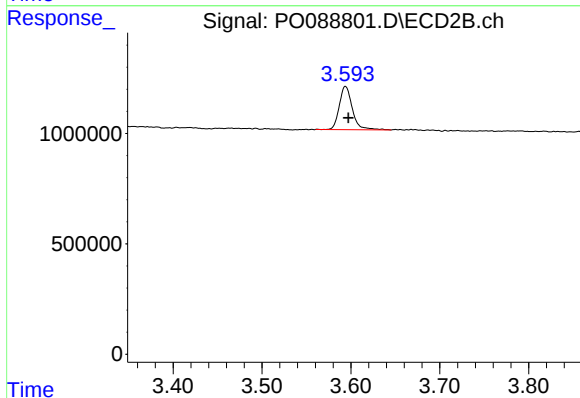


#1 Tetrachloro-m-xylene

R.T.: 3.594 min
Delta R.T.: -0.003 min
Response: 1998012
Conc: 1.85 ng/ml

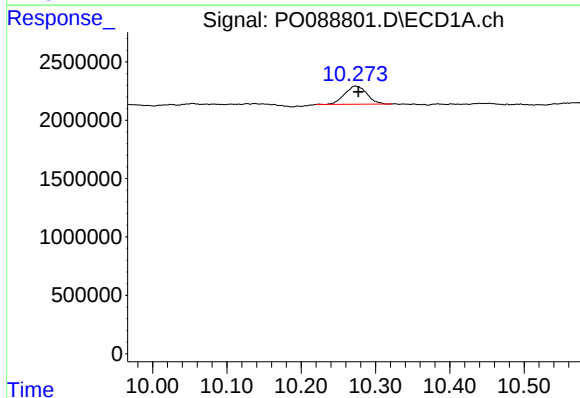

#2 Decachlorobiphenyl

R.T.: 10.273 min
Delta R.T.: -0.004 min
Response: 3220107
Conc: 1.67 ng/ml

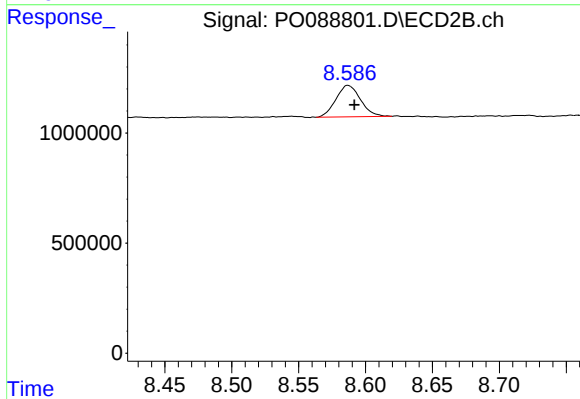

#2 Decachlorobiphenyl

R.T.: 8.586 min
Delta R.T.: -0.006 min
Response: 1830817
Conc: 1.51 ng/ml m