

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080922\
 Data File : P0088808.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Aug 2022 03:51
 Operator : YP/AJ
 Sample : N4106-03 10X
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SOM-2022-53-A

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/10/2022
 Supervised By :Ankita Jodhani 08/10/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 10 05:44:05 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0080422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 05 23:24:09 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.436	3.594	5265404	2272676	1.952	2.100m
2) SA Decachlor...	10.275	8.588	3928130	2142170	2.036	1.768m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO080922\
Data File : PO088808.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Aug 2022 03:51
Operator : YP/AJ
Sample : N4106-03 10X
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SOM-2022-53-A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/10/2022
Supervised By :Ankita Jodhani 08/10/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 10 05:44:05 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO080422.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 05 23:24:09 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

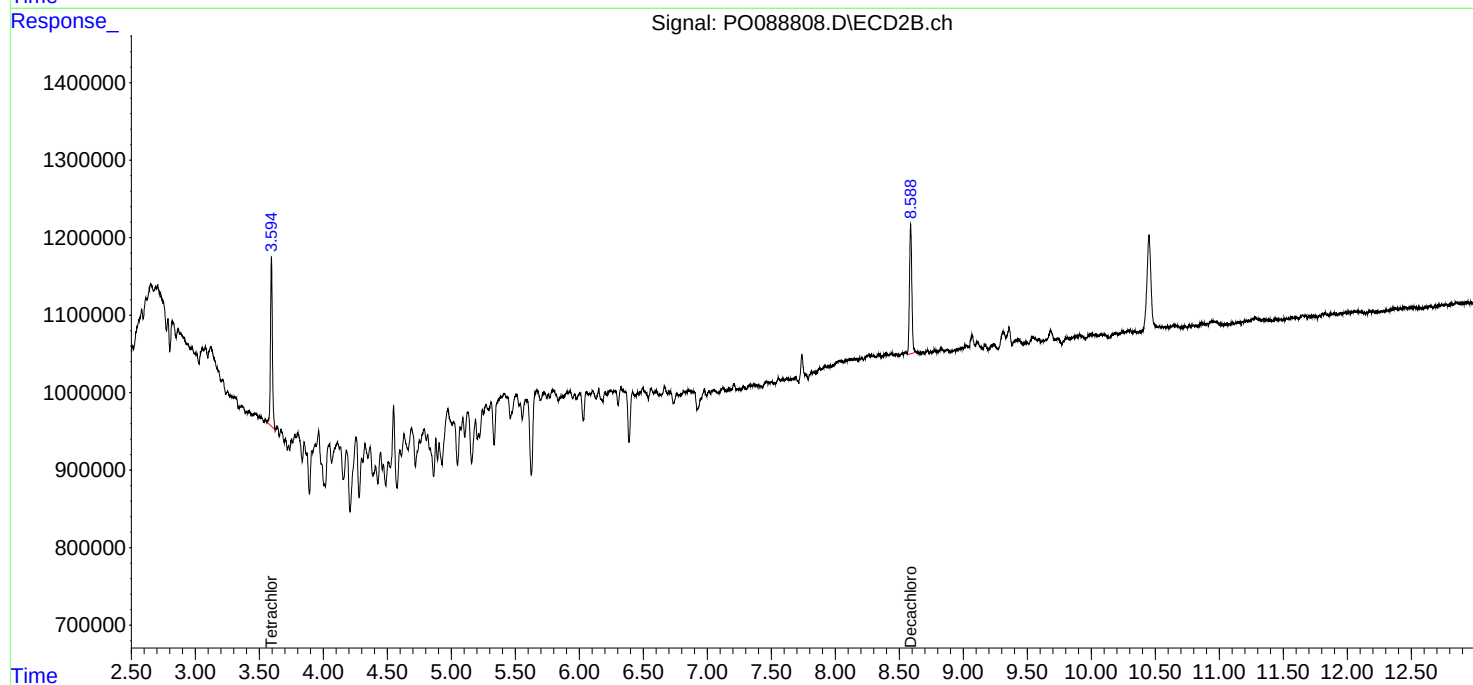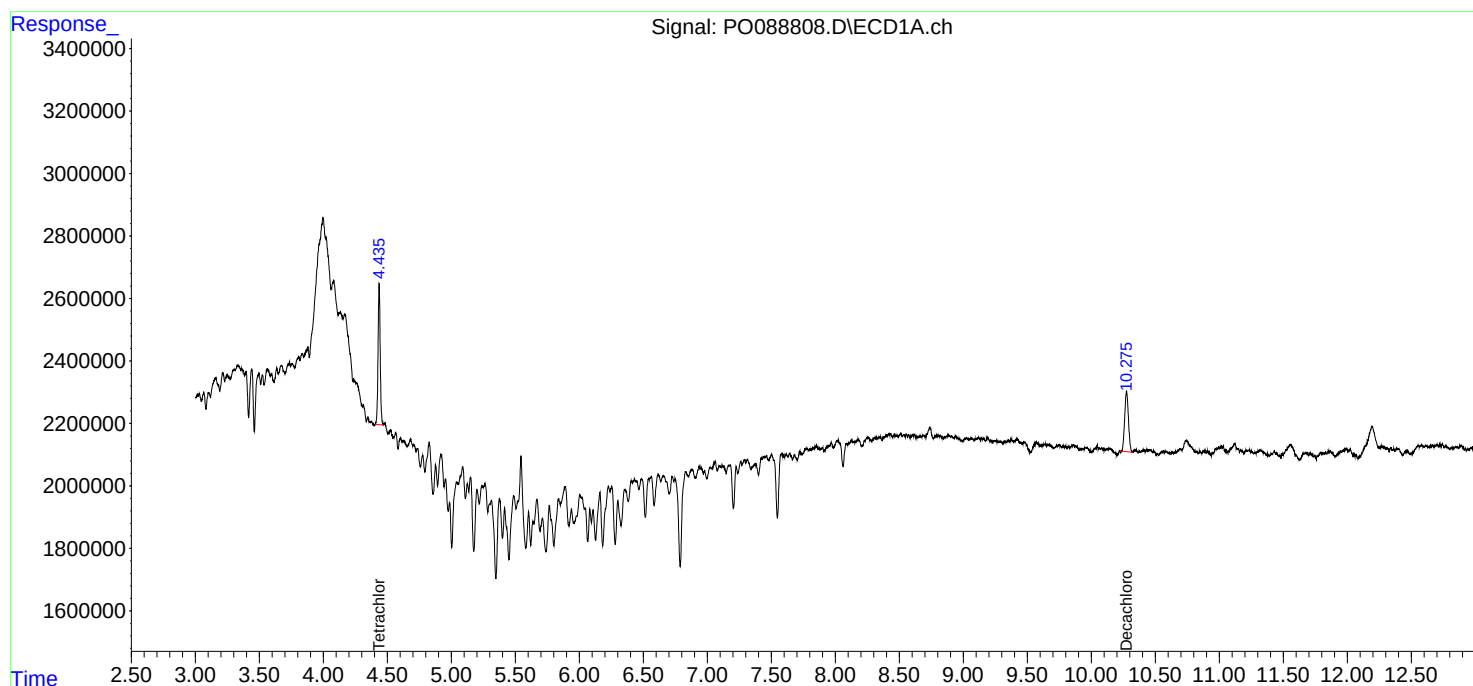

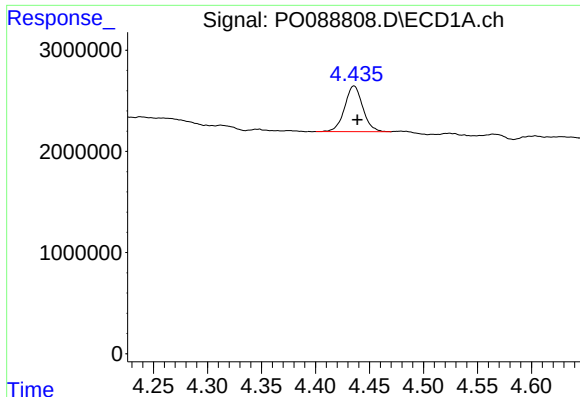


#1 Tetrachloro-m-xylene

R.T.: 4.436 min
Delta R.T.: -0.003 min
Response: 5265404
Conc: 1.95 ng/ml

Instrument :
ECD_O
ClientSampleId :
SOM-2022-53-A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/10/2022
Supervised By :Ankita Jodhani 08/10/2022

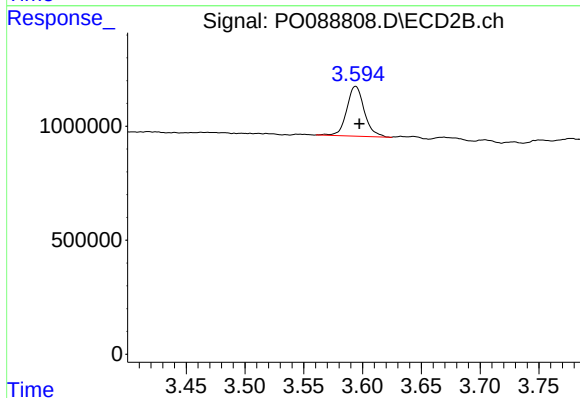


#1 Tetrachloro-m-xylene

R.T.: 3.594 min
Delta R.T.: -0.003 min
Response: 2272676
Conc: 2.10 ng/ml m

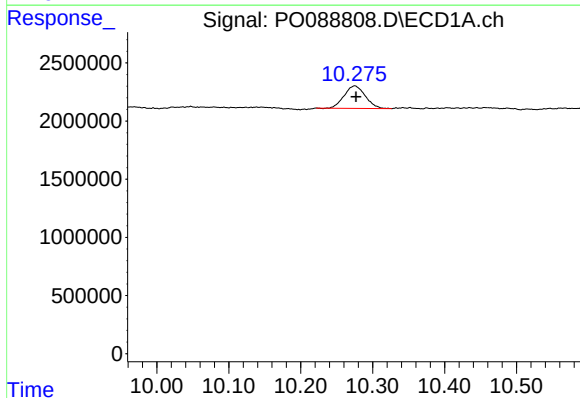

#2 Decachlorobiphenyl

R.T.: 10.275 min
Delta R.T.: -0.002 min
Response: 3928130
Conc: 2.04 ng/ml

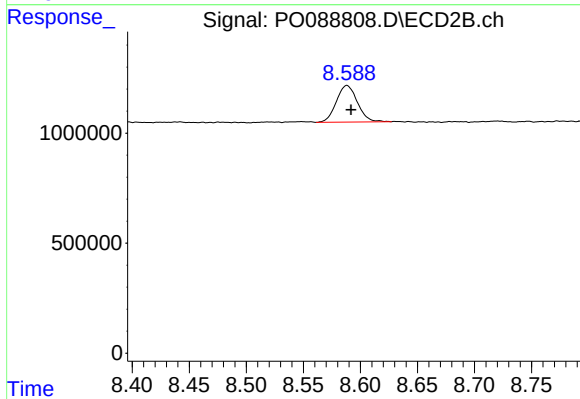

#2 Decachlorobiphenyl

R.T.: 8.588 min
Delta R.T.: -0.004 min
Response: 2142170
Conc: 1.77 ng/ml m