

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080923\
 Data File : P0096875.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Aug 2023 01:05
 Operator : YP/AJ
 Sample : 03932-03
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 NEVINS-SB-01-Z30-32

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/14/2023
 Supervised By :Ankita Jodhani 08/14/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 10 01:40:14 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0080723.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 08 04:34:41 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.412	3.620	39843501	16898294	12.037	12.765m
2) SA Decachlor...	10.351	8.639	48022856	18532684	21.946	16.019 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080923\
Data File : P0096875.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Aug 2023 01:05
Operator : YP/AJ
Sample : 03932-03
Misc :
ALS Vial : 36 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
NEVINS-SB-01-Z30-32


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/14/2023
Supervised By :Ankita Jodhani 08/14/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 10 01:40:14 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0080723.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 08 04:34:41 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

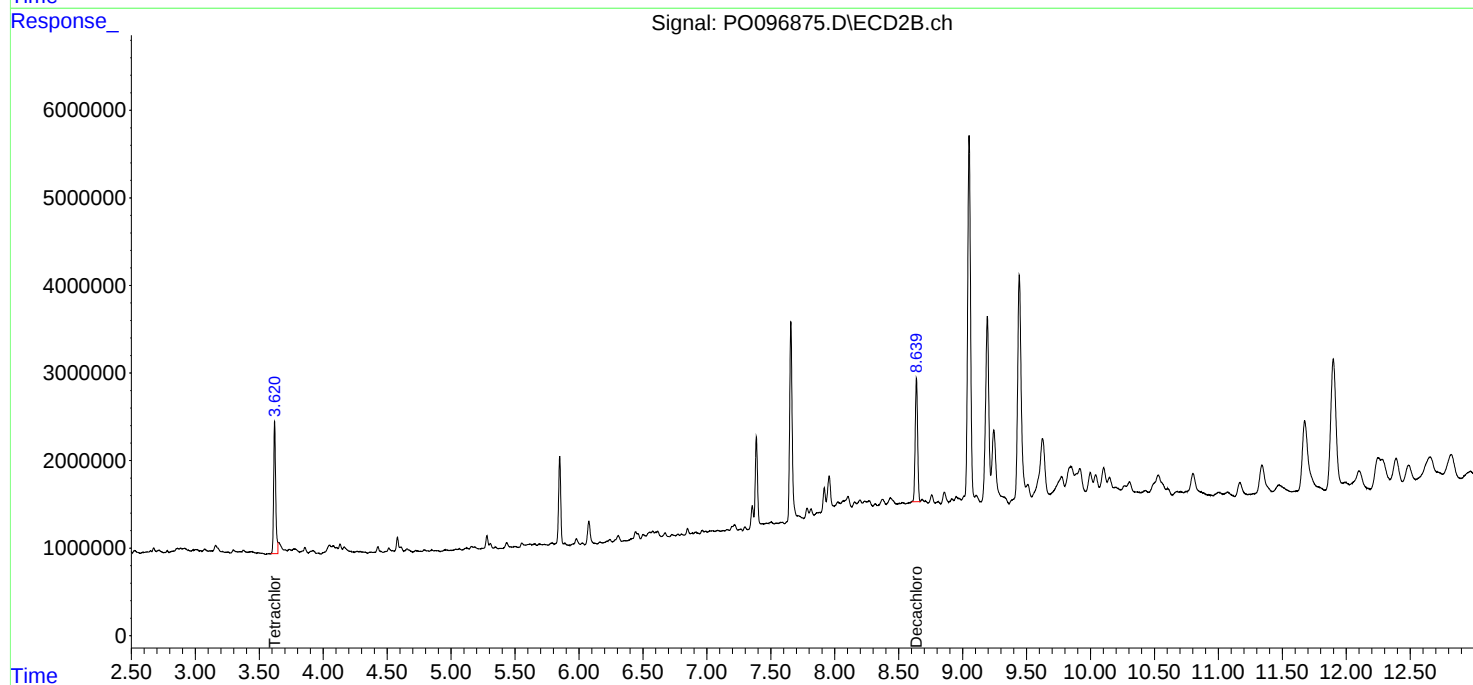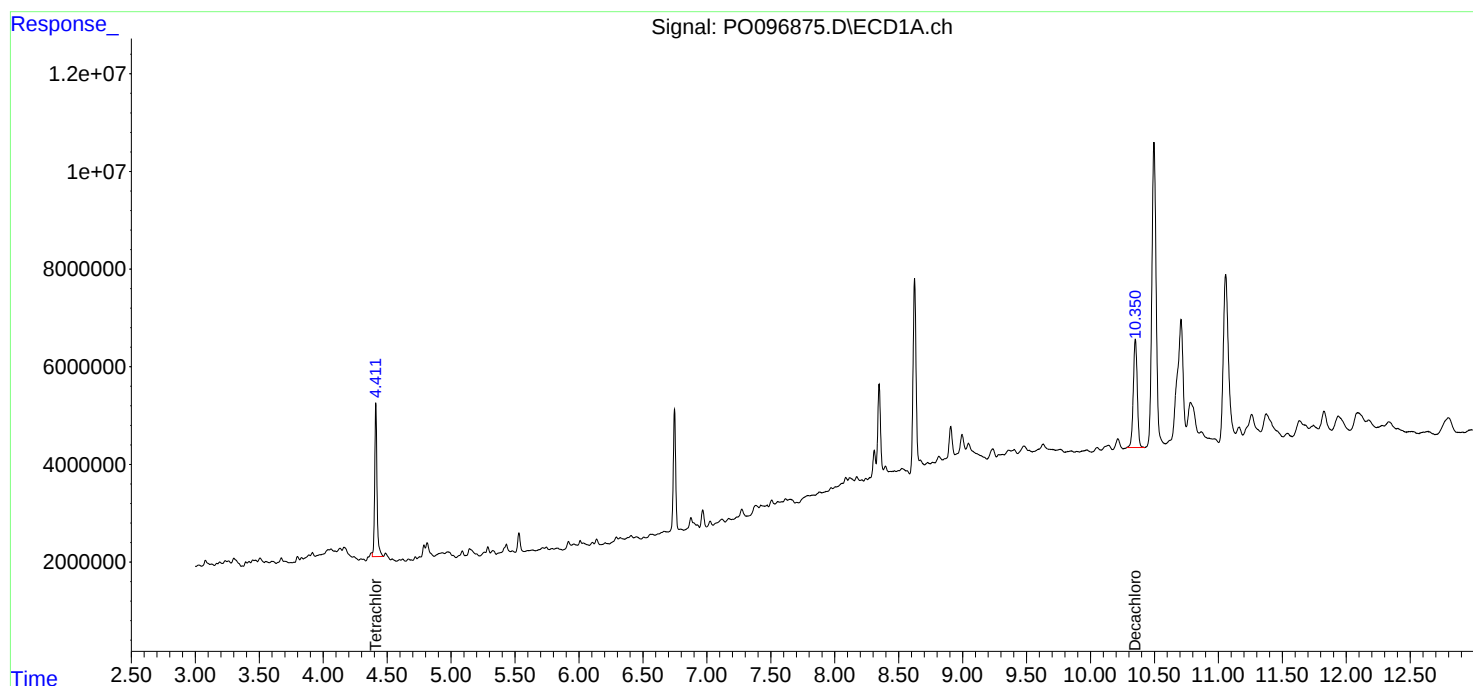

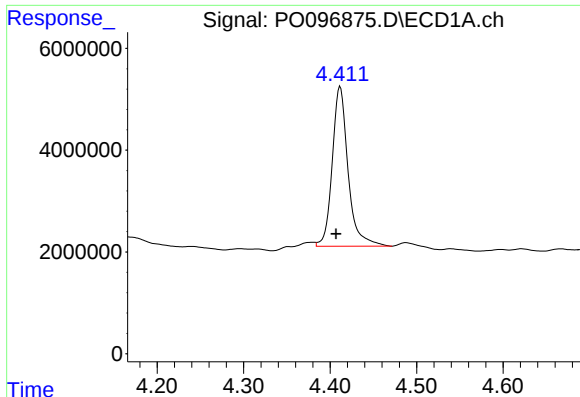


#1 Tetrachloro-m-xylene

R.T.: 4.412 min
Delta R.T.: 0.005 min
Response: 39843501
Conc: 12.04 ng/ml

Instrument :
ECD_O
ClientSampleId :
NEVINS-SB-01-Z30-32


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/14/2023
Supervised By :Ankita Jodhani 08/14/2023

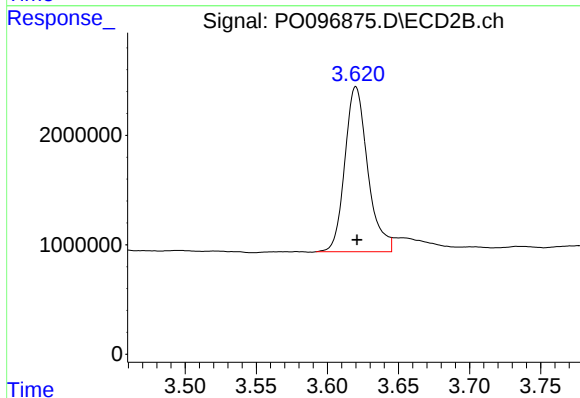


#1 Tetrachloro-m-xylene

R.T.: 3.620 min
Delta R.T.: -0.001 min
Response: 16898294
Conc: 12.77 ng/ml m

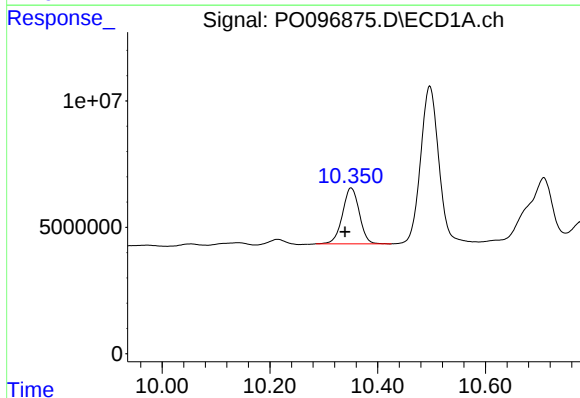

#2 Decachlorobiphenyl

R.T.: 10.351 min
Delta R.T.: 0.011 min
Response: 48022856
Conc: 21.95 ng/ml

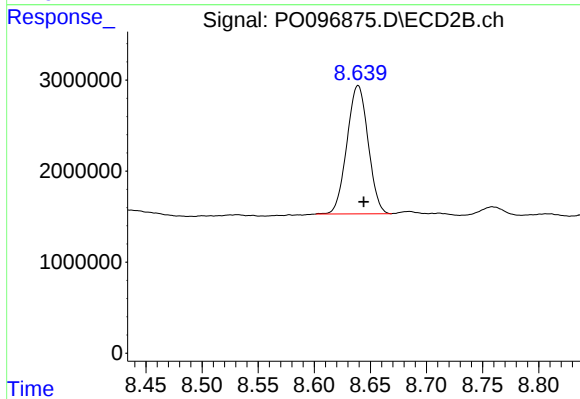

#2 Decachlorobiphenyl

R.T.: 8.639 min
Delta R.T.: -0.005 min
Response: 18532684
Conc: 16.02 ng/ml