

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080923\
 Data File : P0096876.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Aug 2023 01:22
 Operator : YP/AJ
 Sample : 03932-04
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 NEVINS-SB-01-Z67-69

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 10 02:45:23 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0080723.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 08 04:34:41 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.411	3.619	42807277	19202604	12.932	14.506
2) SA Decachlor...	10.352	8.639	47071330	20830516	21.512	18.005

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO080923\
Data File : PO096876.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Aug 2023 01:22
Operator : YP/AJ
Sample : 03932-04
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
NEVINS-SB-01-Z67-69

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 10 02:45:23 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO080723.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 08 04:34:41 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

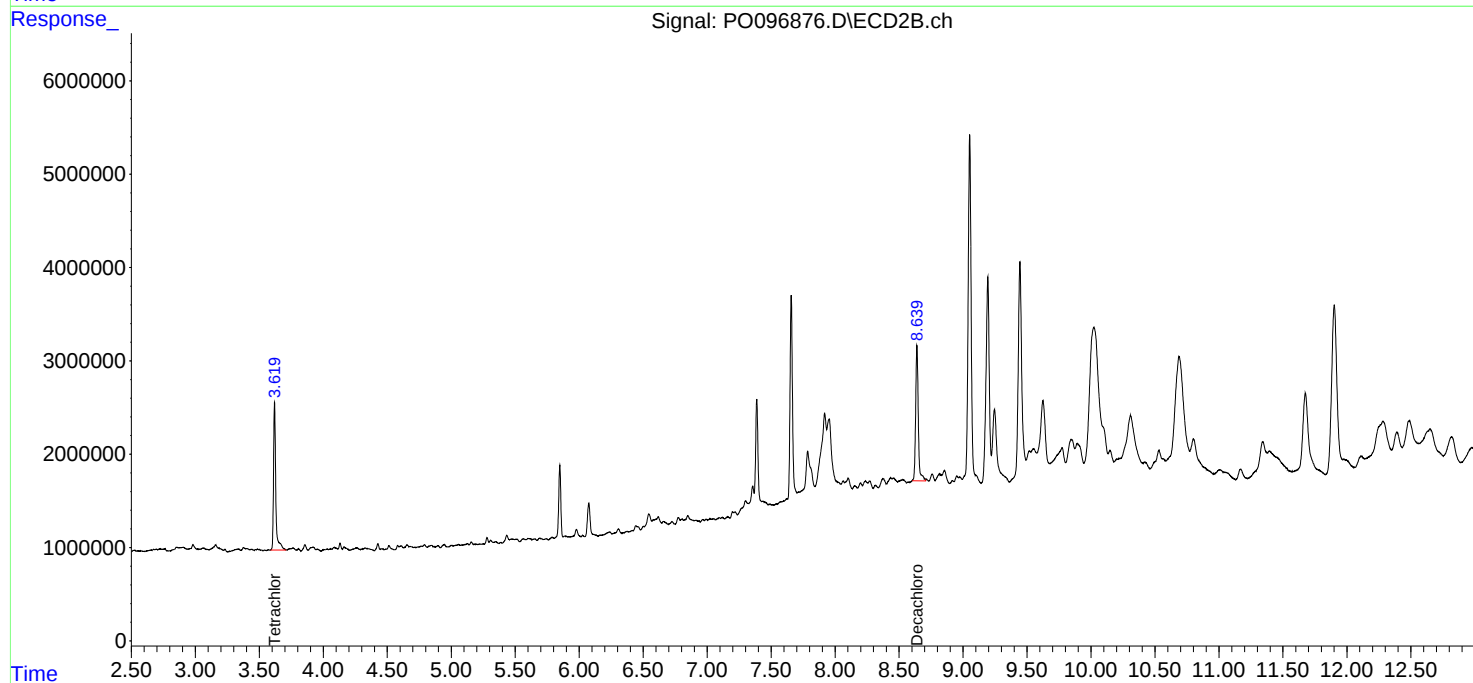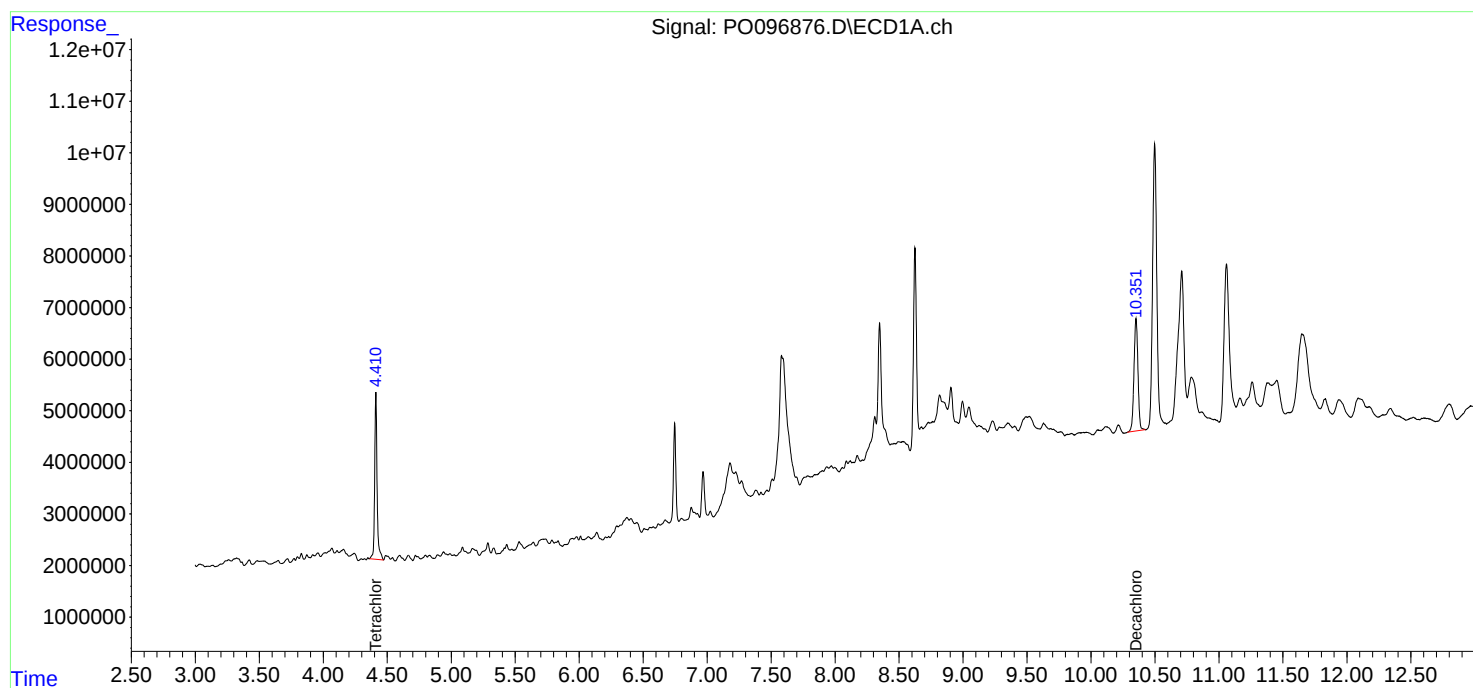


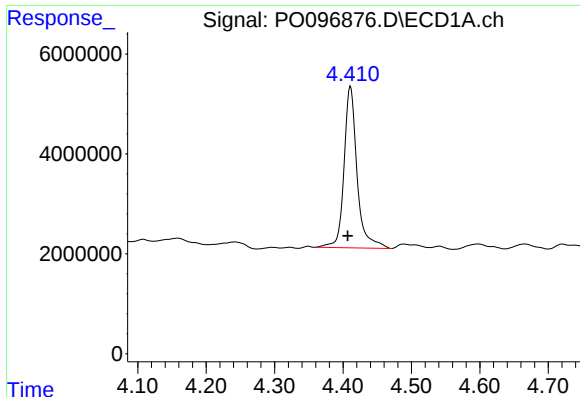

#1 Tetrachloro-m-xylene


R.T.: 4.411 min
Delta R.T.: 0.004 min
Response: 42807277
Conc: 12.93 ng/ml

Instrument :
ECD_O
ClientSampleId :
NEVINS-SB-01-Z67-69

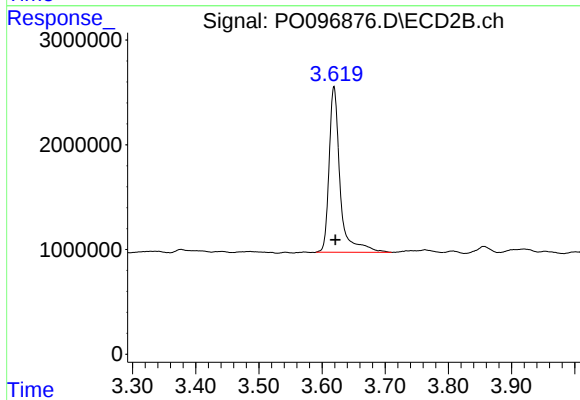


#1 Tetrachloro-m-xylene

R.T.: 3.619 min
Delta R.T.: -0.002 min
Response: 19202604
Conc: 14.51 ng/ml

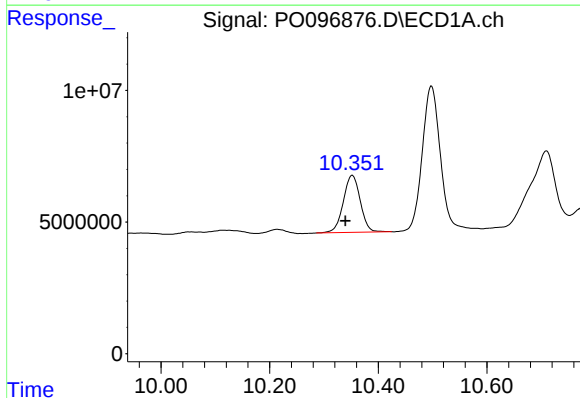

#2 Decachlorobiphenyl

R.T.: 10.352 min
Delta R.T.: 0.012 min
Response: 47071330
Conc: 21.51 ng/ml

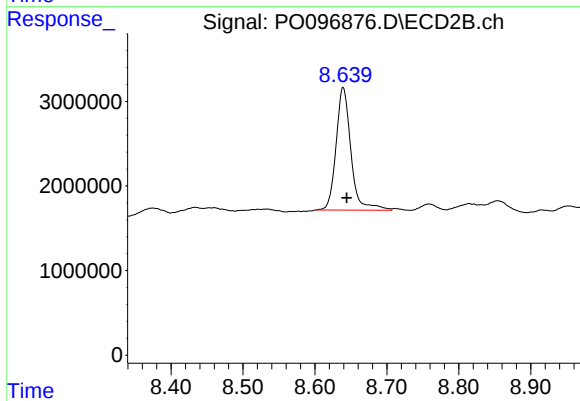

#2 Decachlorobiphenyl

R.T.: 8.639 min
Delta R.T.: -0.005 min
Response: 20830516
Conc: 18.00 ng/ml