

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080924\
 Data File : P0105347.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Aug 2024 10:49
 Operator : YP/AJ
 Sample : P3493-01DL 40X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 628-ADL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/12/2024
 Supervised By :Ankita Jodhani 08/12/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 09 12:04:03 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072924.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 30 07:11:20 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
26)	L6	AR-1254-1	6.461	5.376	156.3E6	88805831	540.074m 591.843
27)	L6	AR-1254-2	6.682	5.521	244.4E6	83906158	588.674 626.838
28)	L6	AR-1254-3	7.051	5.918	257.2E6	136.4E6	616.033 641.971
29)	L6	AR-1254-4	7.338	6.143	217.3E6	82437401	695.256 620.704
30)	L6	AR-1254-5	7.761	6.555	280.7E6	151.7E6	767.312 817.126

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO080924\
Data File : PO105347.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Aug 2024 10:49
Operator : YP/AJ
Sample : P3493-01DL 40X
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
628-ADL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/12/2024
Supervised By :Ankita Jodhani 08/12/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 09 12:04:03 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO072924.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 30 07:11:20 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

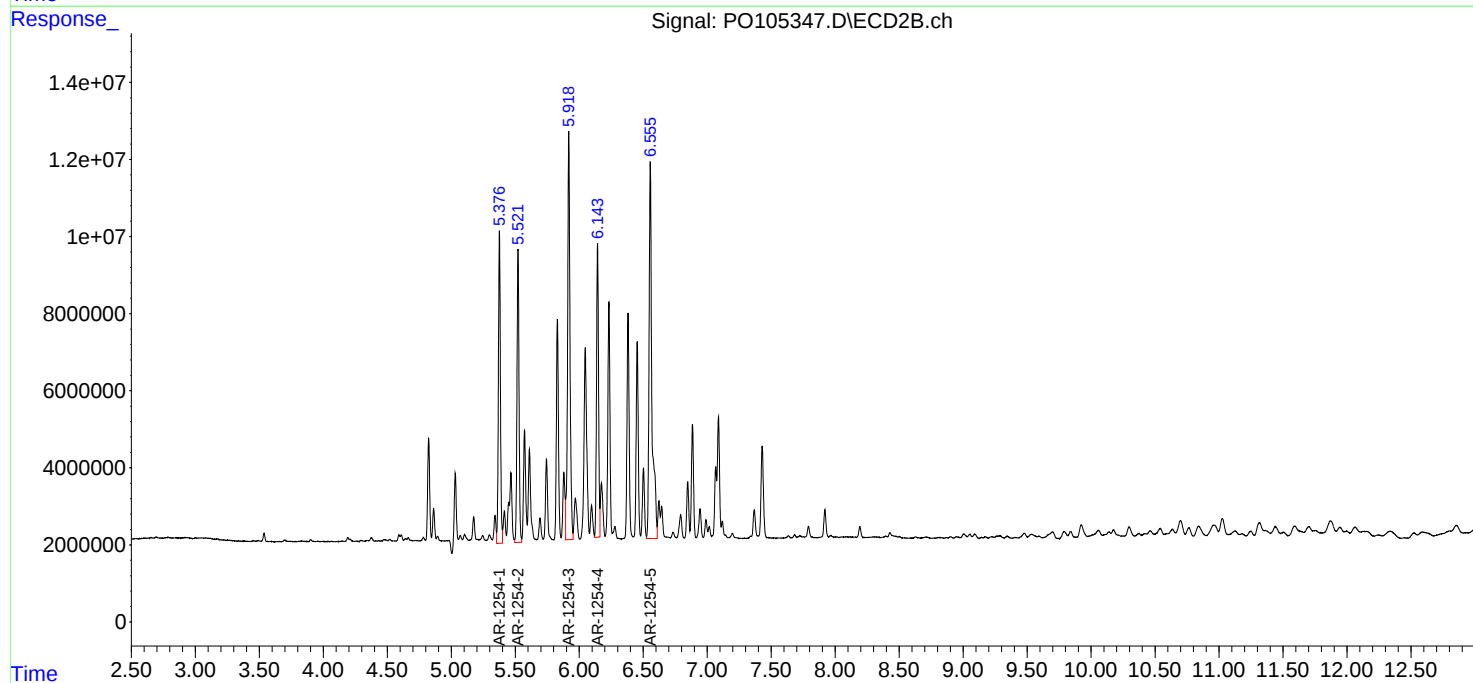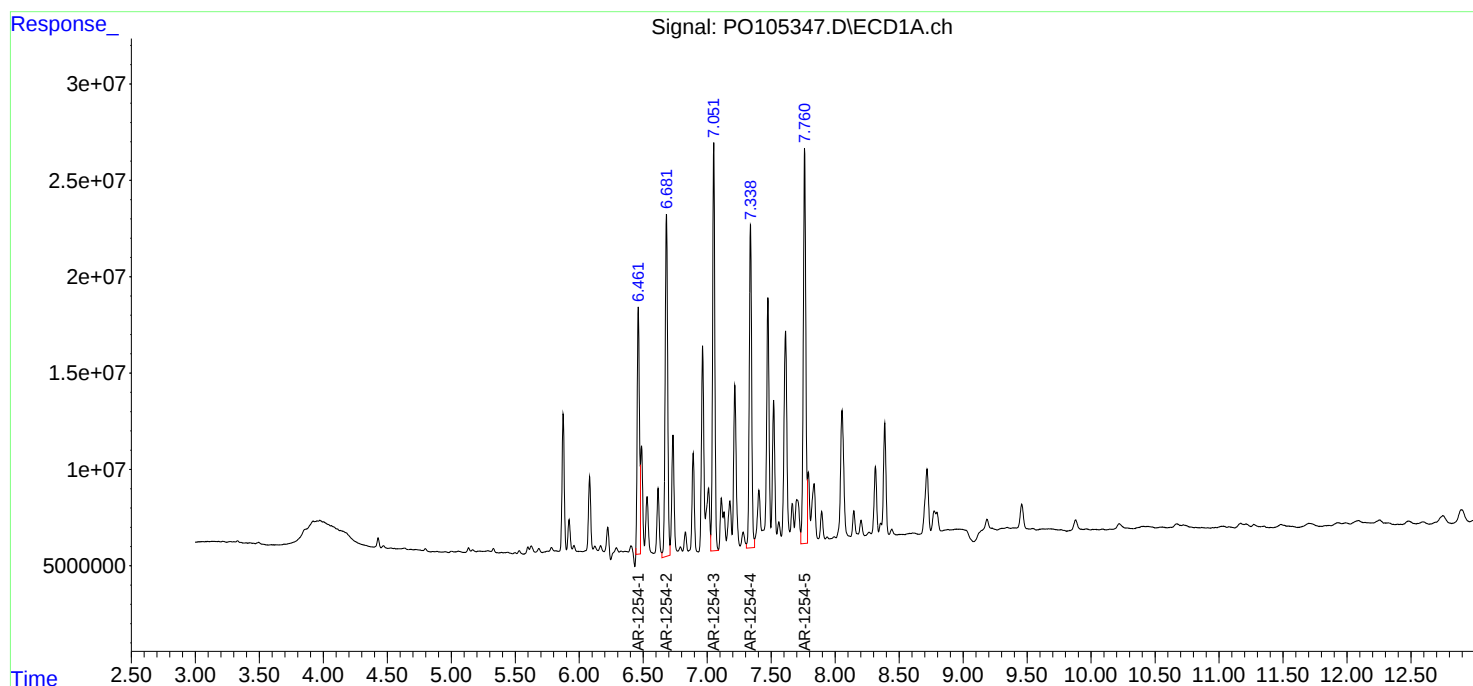

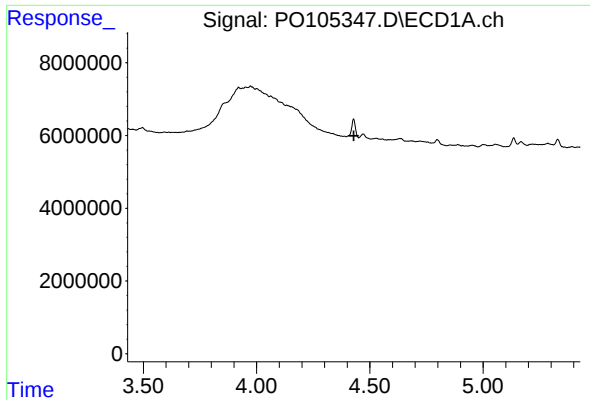


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.429 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
628-ADL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/12/2024
Supervised By :Ankita Jodhani 08/12/2024

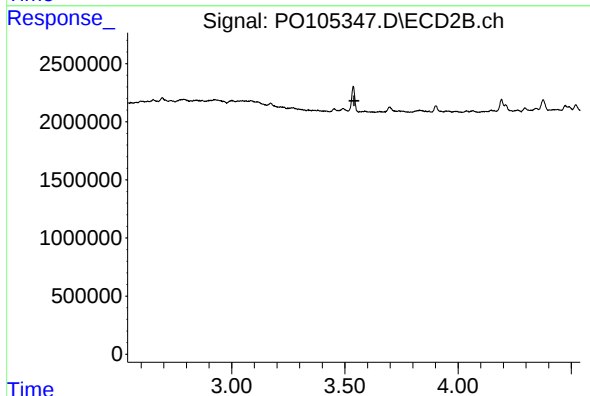


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.540 min
Response: 0
Conc: N.D.

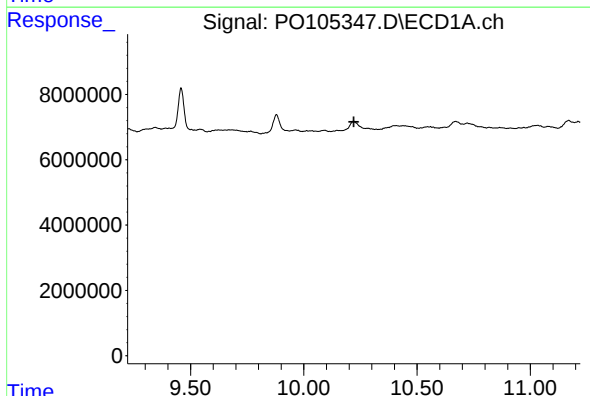


#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.221 min
Response: 0
Conc: N.D.

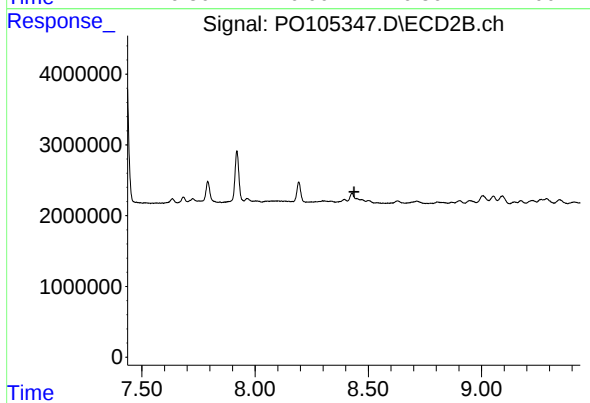

#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.437 min
Response: 0
Conc: N.D.

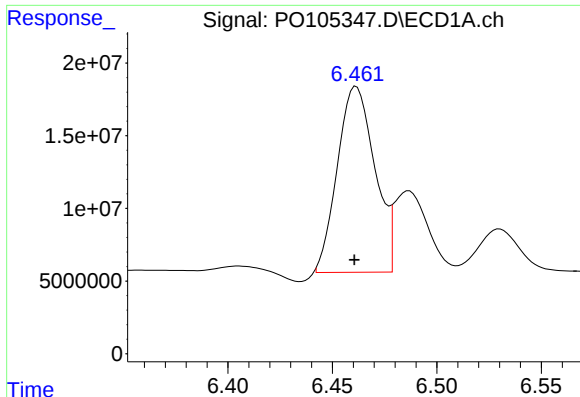


#26 AR-1254-1

R.T.: 6.461 min
Delta R.T.: 0.000 min
Response: 156313401
Conc: 540.07 ng/ml

Instrument :
ECD_O
ClientSampleId :
628-ADL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/12/2024
Supervised By :Ankita Jodhani 08/12/2024

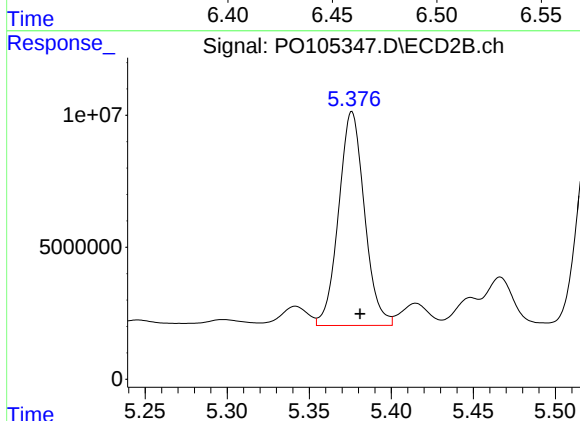


#26 AR-1254-1

R.T.: 5.376 min
Delta R.T.: -0.005 min
Response: 88805831
Conc: 591.84 ng/ml

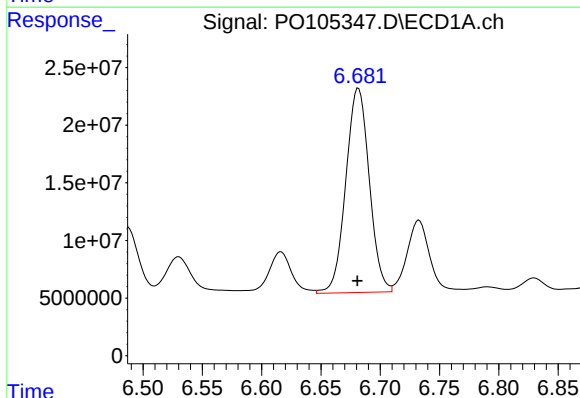


#27 AR-1254-2

R.T.: 6.682 min
Delta R.T.: 0.000 min
Response: 244446900
Conc: 588.67 ng/ml

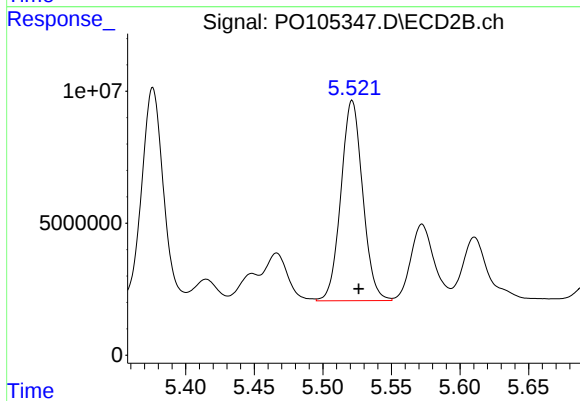

#27 AR-1254-2

R.T.: 5.521 min
Delta R.T.: -0.005 min
Response: 83906158
Conc: 626.84 ng/ml

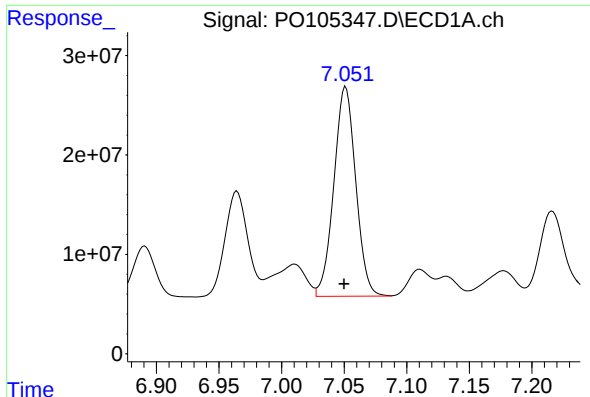


#28 AR-1254-3

R.T.: 7.051 min
Delta R.T.: 0.001 min
Response: 257184783
Conc: 616.03 ng/ml

Instrument :
ECD_O
ClientSampleId :
628-ADL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/12/2024
Supervised By :Ankita Jodhani 08/12/2024

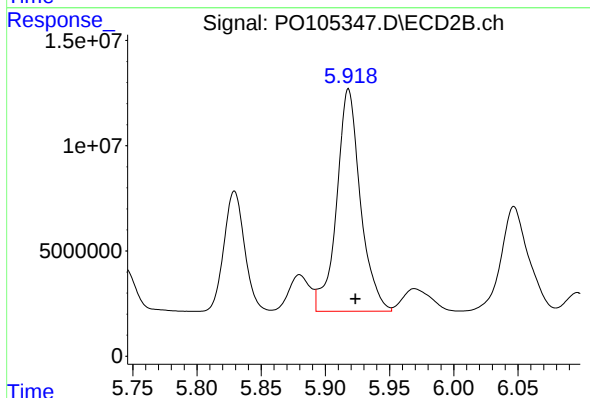


#28 AR-1254-3

R.T.: 5.918 min
Delta R.T.: -0.005 min
Response: 136400214
Conc: 641.97 ng/ml

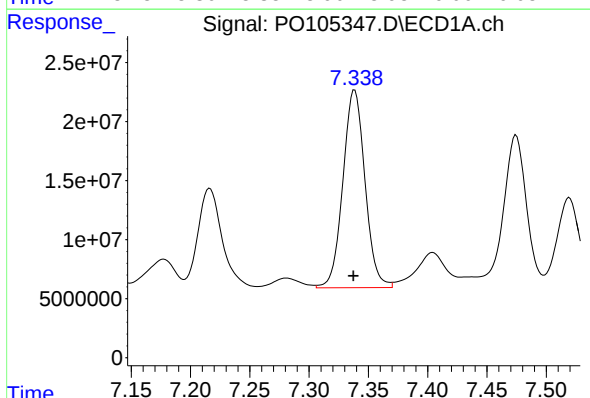


#29 AR-1254-4

R.T.: 7.338 min
Delta R.T.: 0.001 min
Response: 217295408
Conc: 695.26 ng/ml

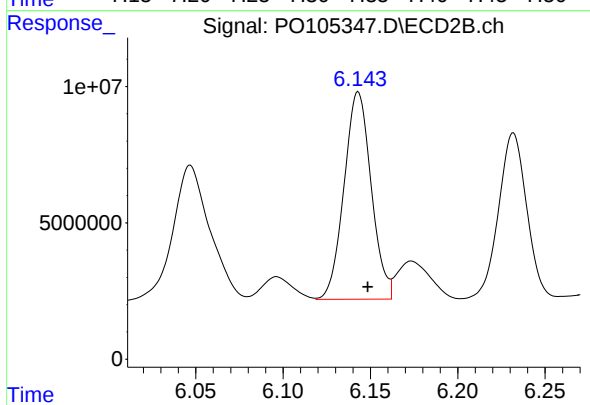

#29 AR-1254-4

R.T.: 6.143 min
Delta R.T.: -0.005 min
Response: 82437401
Conc: 620.70 ng/ml

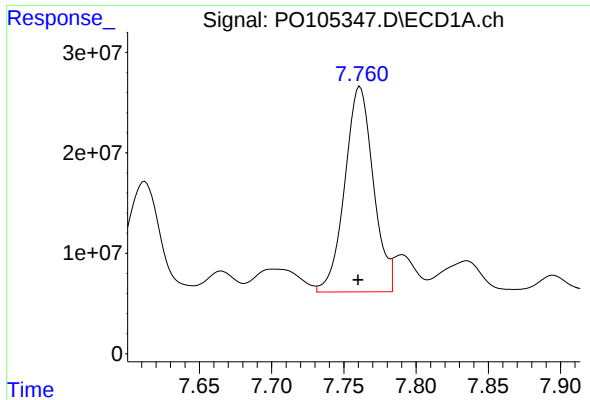


#30 AR-1254-5

R.T.: 7.761 min
Delta R.T.: 0.001 min
Response: 280742817
Conc: 767.31 ng/ml

Instrument :
ECD_O
ClientSampleId :
628-ADL

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/12/2024
Supervised By :Ankita Jodhani 08/12/2024

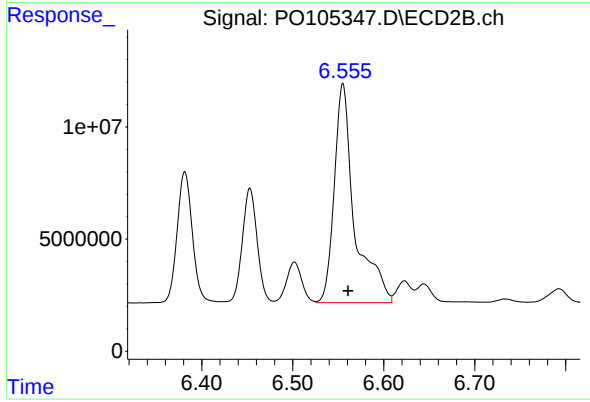

#30 AR-1254-5

R.T.: 6.555 min
Delta R.T.: -0.006 min
Response: 151677078
Conc: 817.13 ng/ml