

Data Path : Z:\bestpcbsrv\HPCHEM1\ECD 0\Data\P0081018\
 Data File : P0047930.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Aug 2018 23:00
 Operator : SM/SJ
 Sample : J4414-02
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 C0AY1

Manual Integrations
 APPROVED

Sohil
 8/13/2018 4:59:57 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 11 03:26:11 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072718.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jul 27 02:33:29 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.392	3.637	3353891	4008756	16.612	16.315
2) SA Decachlor...	10.081	8.621	1512587	1581621	9.274	10.062m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0081018\
Data File : P0047930.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Aug 2018 23:00
Operator : SM/SJ
Sample : J4414-02
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
C0AY1


Manual Integrations
APPROVED

Sohil
8/13/2018 4:59:57 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 11 03:26:11 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072718.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 27 02:33:29 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

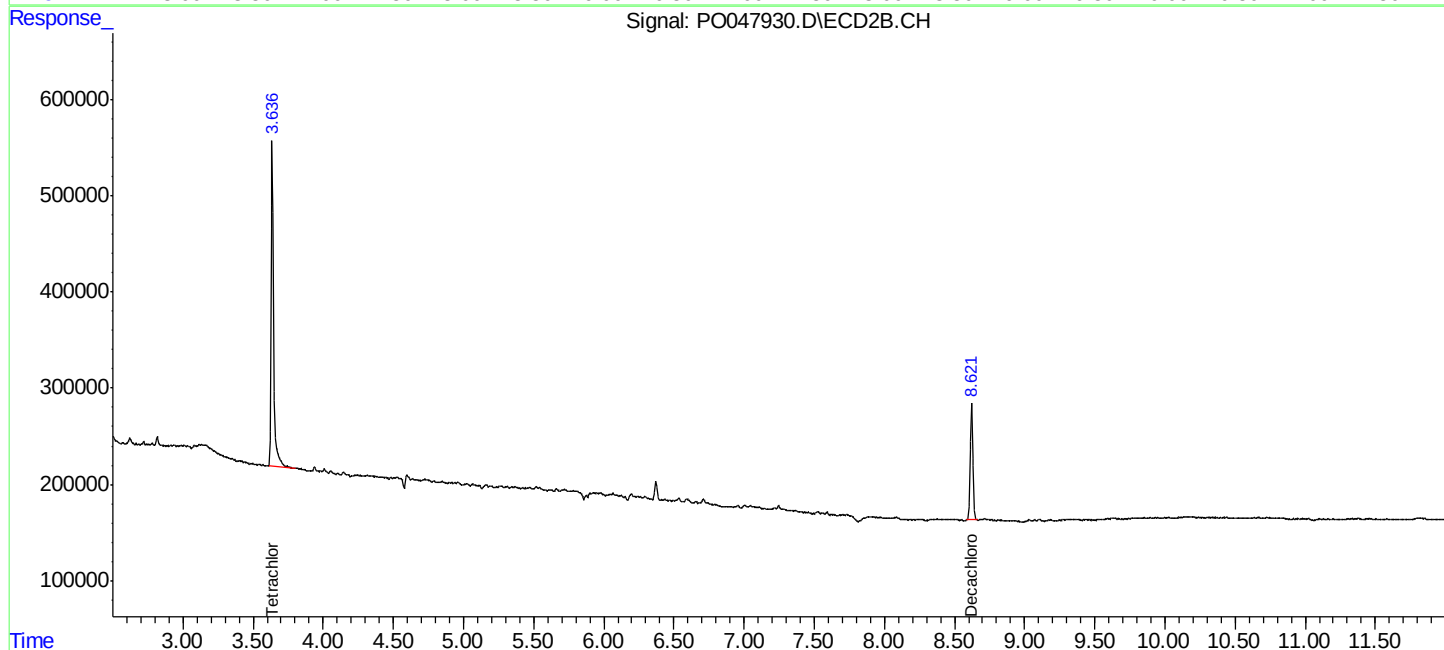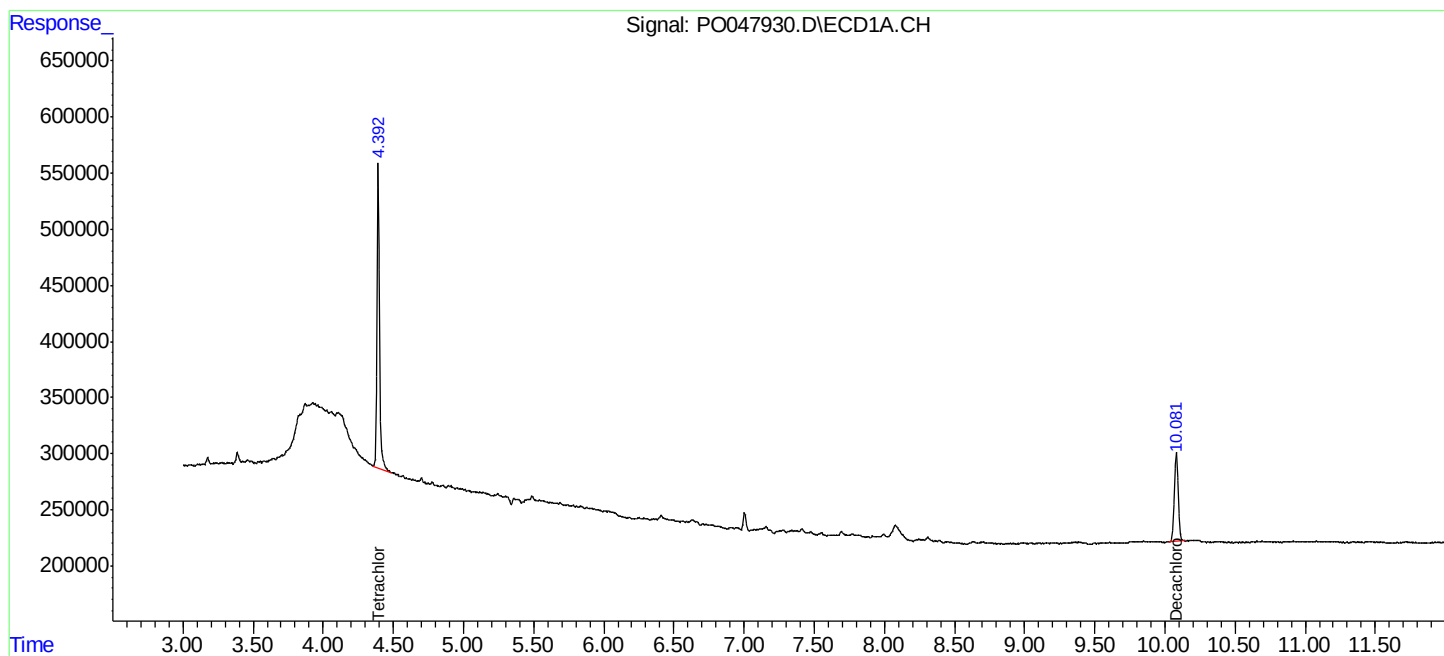

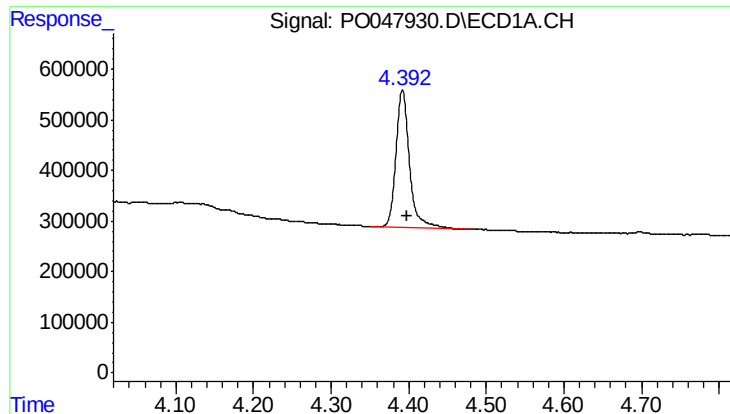


#1 Tetrachloro-m-xylene

R.T.: 4.392 min
Delta R.T.: -0.005 min
Response: 3353891
Conc: 16.61 ng/ml

Instrument :
ECD_O
ClientSampleId :
C0AY1


Manual Integrations
APPROVED

Sohil
8/13/2018 4:59:57 PM

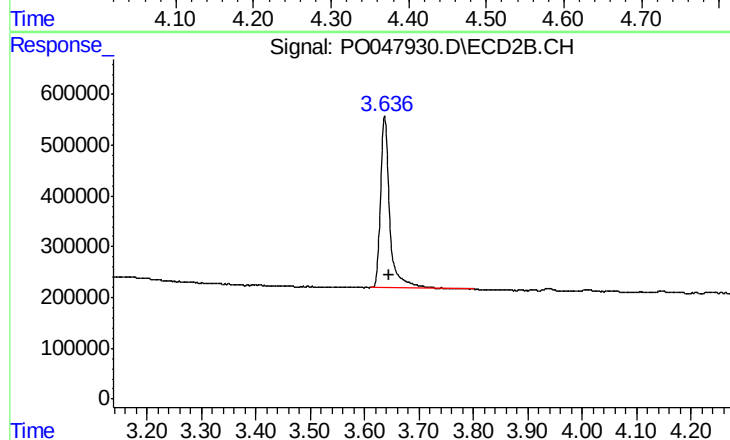


#1 Tetrachloro-m-xylene

R.T.: 3.637 min
Delta R.T.: -0.009 min
Response: 4008756
Conc: 16.31 ng/ml

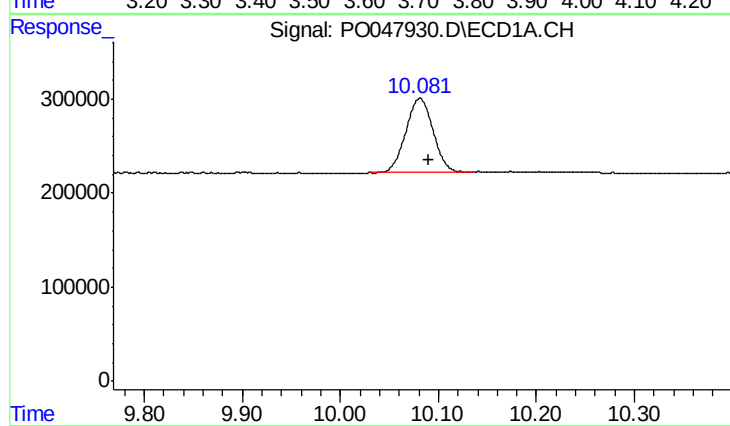

#2 Decachlorobiphenyl

R.T.: 10.081 min
Delta R.T.: -0.009 min
Response: 1512587
Conc: 9.27 ng/ml

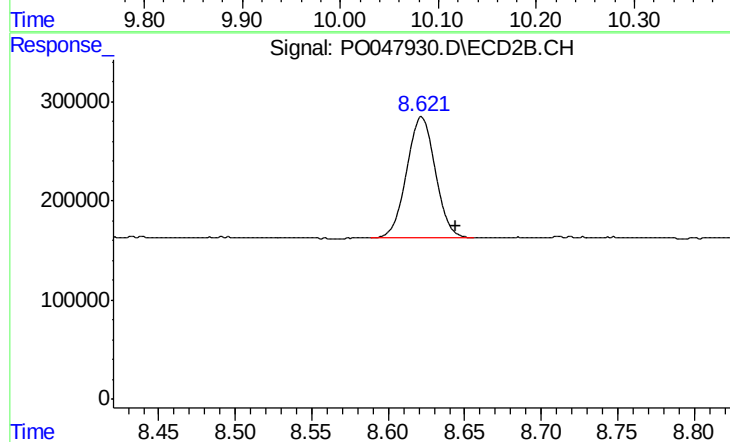

#2 Decachlorobiphenyl

R.T.: 8.621 min
Delta R.T.: -0.023 min
Response: 1581621
Conc: 10.06 ng/ml m