

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081023\
 Data File : P0096907.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Aug 2023 11:03
 Operator : YP/AJ
 Sample : 03572-09
 Misc : AR1248 MDL 25 PPB
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-WATER-03-QT3-2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 10 21:35:08 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0080723.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 08 04:34:41 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.412	3.619	50510634	20144370	15.259	15.217
2) SA Decachlor...	10.354	8.639	38079518	20298511	17.402	17.545
Target Compounds						
21) L5 AR-1248-1	5.597	4.705	1198057	550619	20.447	19.621
22) L5 AR-1248-2	5.877	4.943	1870729	894892	19.898	21.115
23) L5 AR-1248-3	6.085	4.984	2015475	943300	20.606	21.505
24) L5 AR-1248-4	6.497	5.155	1636903	1106902	18.019	21.683
25) L5 AR-1248-5	6.537	5.550	1530406	1147635	17.374	24.547 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081023\
Data File : PO096907.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Aug 2023 11:03
Operator : YP/AJ
Sample : 03572-09
Misc : AR1248 MDL 25 PPB
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 10 21:35:08 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO080723.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 08 04:34:41 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

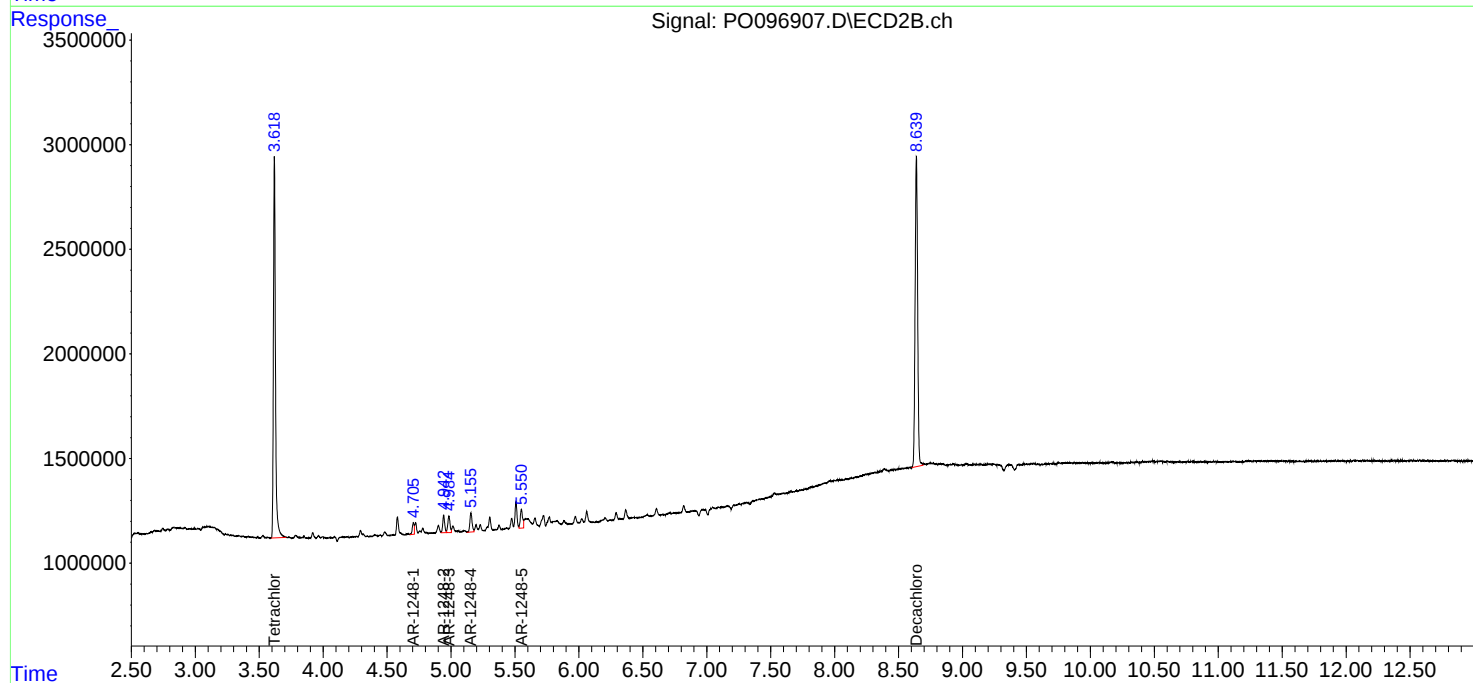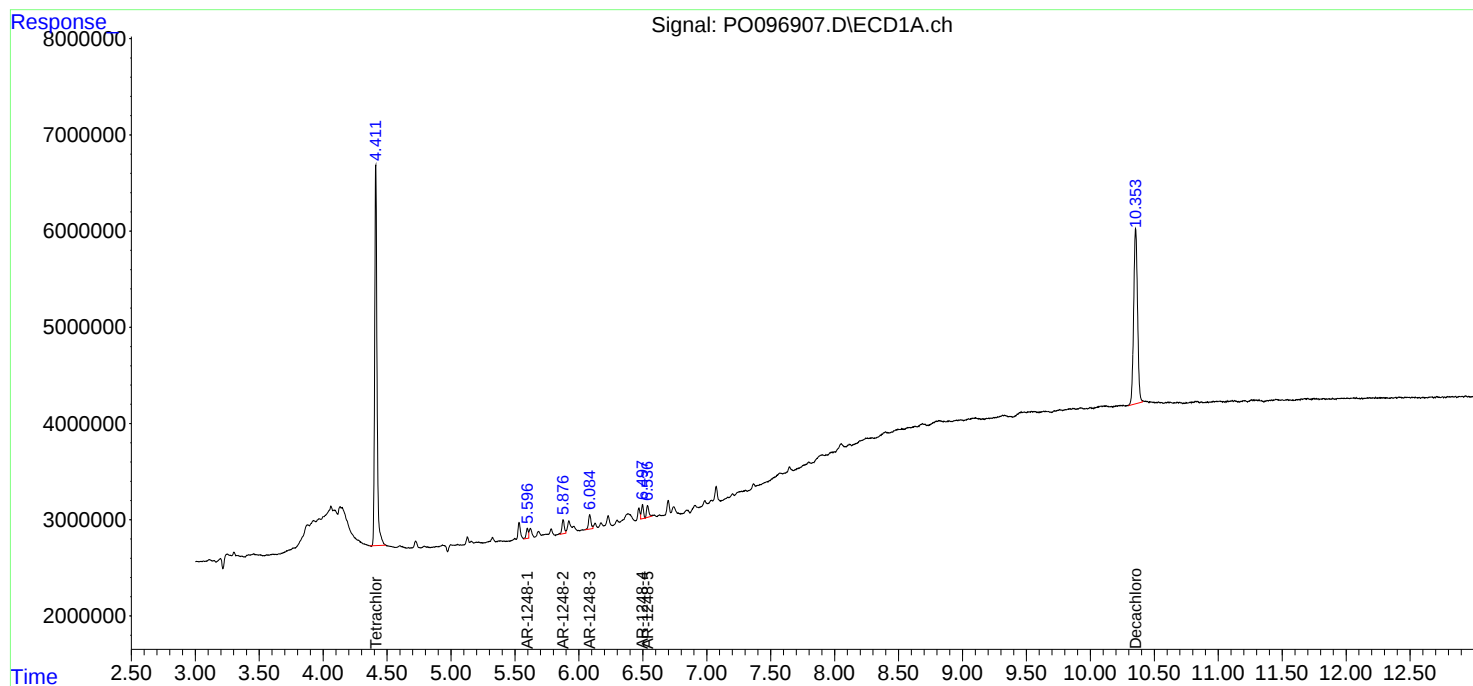


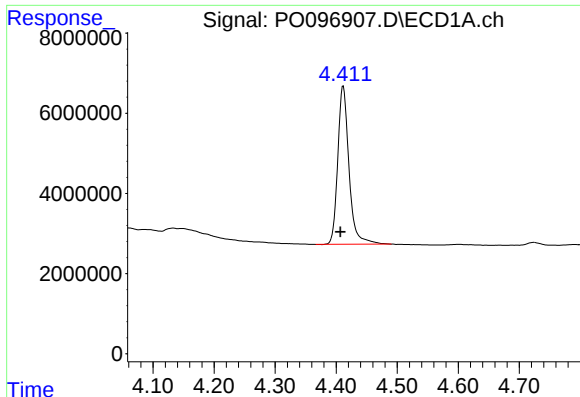

#1 Tetrachloro-m-xylene


R.T.: 4.412 min
Delta R.T.: 0.005 min
Response: 50510634
Conc: 15.26 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2023

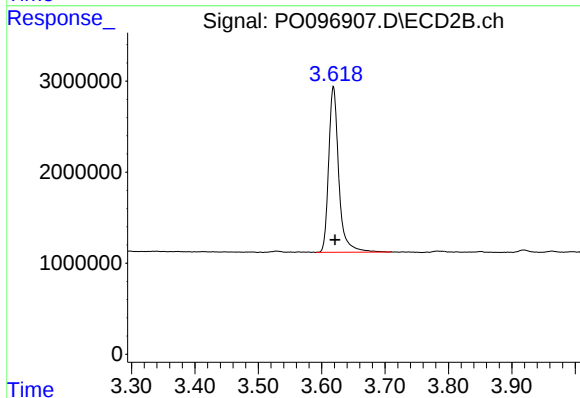


#1 Tetrachloro-m-xylene

R.T.: 3.619 min
Delta R.T.: -0.003 min
Response: 20144370
Conc: 15.22 ng/ml

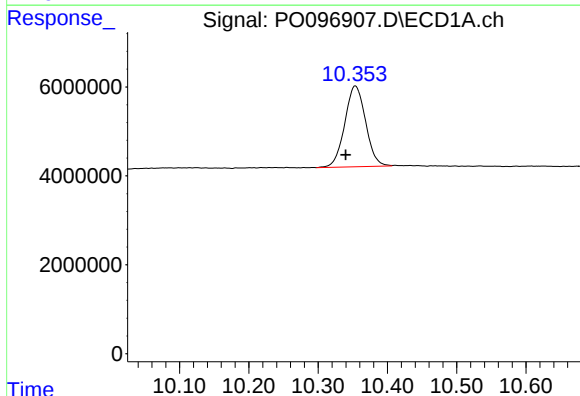


#2 Decachlorobiphenyl

R.T.: 10.354 min
Delta R.T.: 0.014 min
Response: 38079518
Conc: 17.40 ng/ml

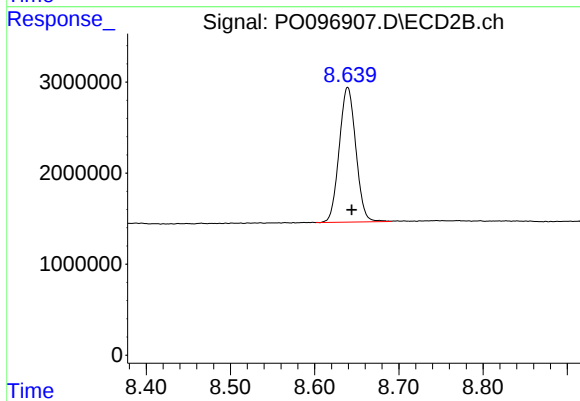

#2 Decachlorobiphenyl


R.T.: 8.639 min
Delta R.T.: -0.005 min
Response: 20298511
Conc: 17.55 ng/ml

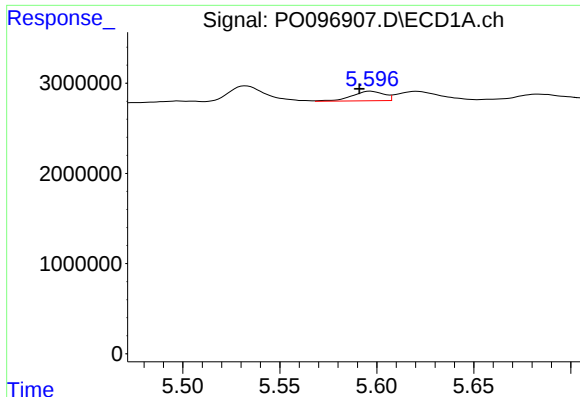

#21 AR-1248-1


R.T.: 5.597 min
Delta R.T.: 0.006 min
Response: 1198057
Conc: 20.45 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2023

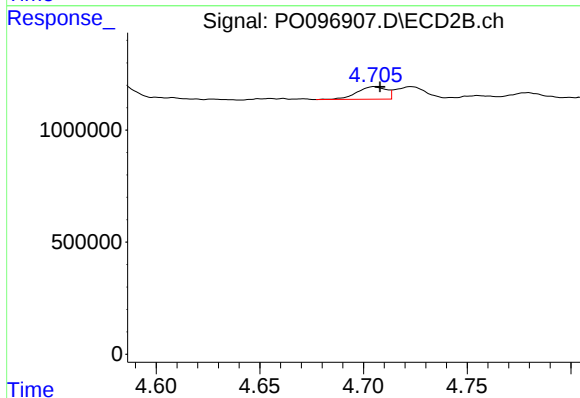


#21 AR-1248-1

R.T.: 4.705 min
Delta R.T.: -0.003 min
Response: 550619
Conc: 19.62 ng/ml

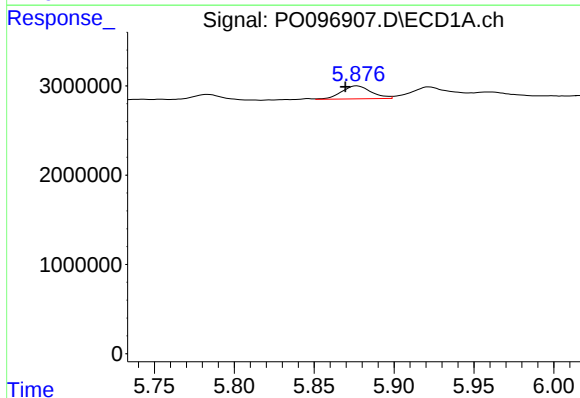


#22 AR-1248-2

R.T.: 5.877 min
Delta R.T.: 0.007 min
Response: 1870729
Conc: 19.90 ng/ml

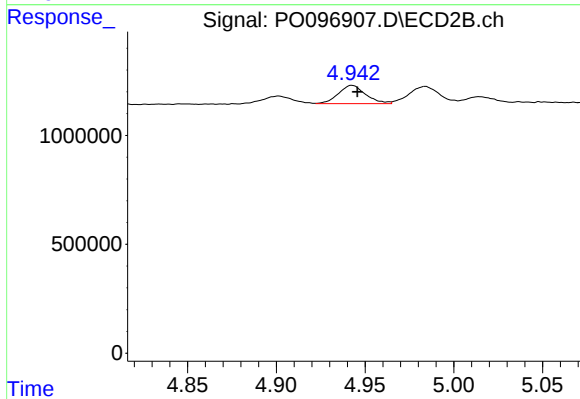

#22 AR-1248-2


R.T.: 4.943 min
Delta R.T.: -0.003 min
Response: 894892
Conc: 21.12 ng/ml

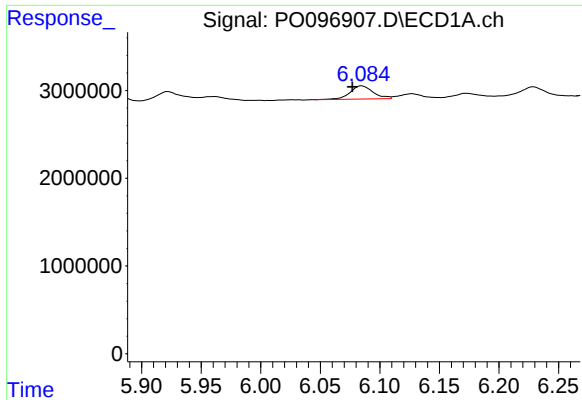

#23 AR-1248-3


R.T.: 6.085 min
Delta R.T.: 0.008 min
Response: 2015475
Conc: 20.61 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2023

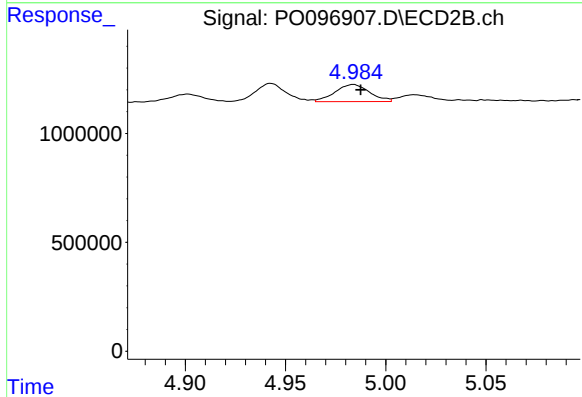


#23 AR-1248-3

R.T.: 4.984 min
Delta R.T.: -0.004 min
Response: 943300
Conc: 21.50 ng/ml

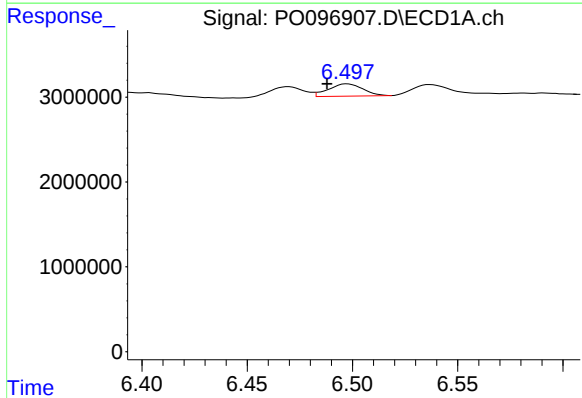


#24 AR-1248-4

R.T.: 6.497 min
Delta R.T.: 0.010 min
Response: 1636903
Conc: 18.02 ng/ml

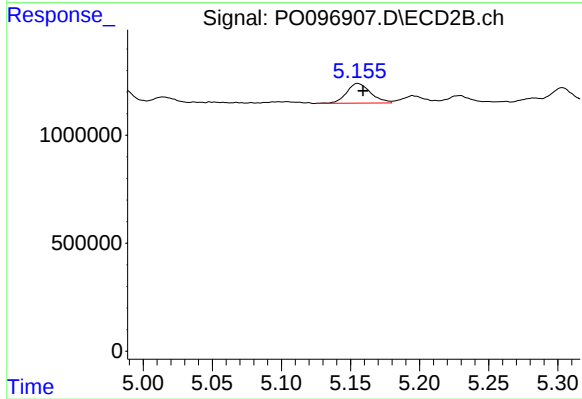

#24 AR-1248-4


R.T.: 5.155 min
Delta R.T.: -0.004 min
Response: 1106902
Conc: 21.68 ng/ml

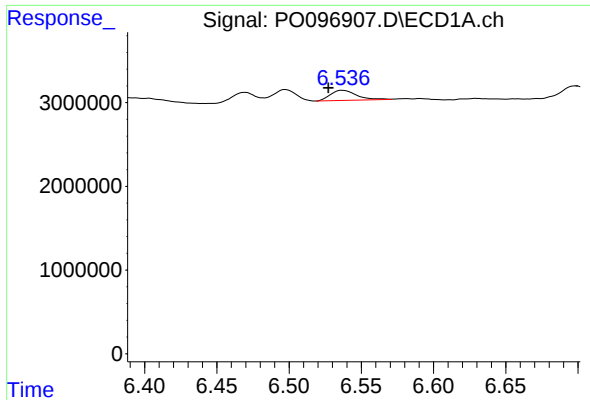

#25 AR-1248-5

R.T.: 6.537 min
Delta R.T.: 0.010 min
Response: 1530406
Conc: 17.37 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2023

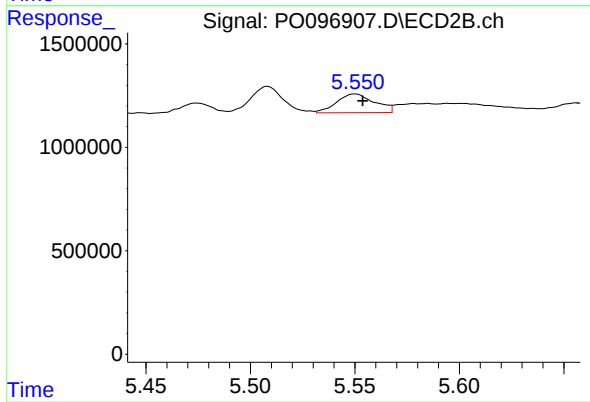

#25 AR-1248-5

R.T.: 5.550 min
Delta R.T.: -0.004 min
Response: 1147635
Conc: 24.55 ng/ml