

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081023\
 Data File : P0096908.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Aug 2023 11:20
 Operator : YP/AJ
 Sample : 03572-09
 Misc : AR1254 MDL 25 PPB
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-WATER-03-QT3-2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 10 21:35:37 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0080723.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 08 04:34:41 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.411	3.619	56215369	22602291	16.983	17.074
2) SA Decachlor...	10.356	8.640	41735986	22199855	19.073	19.189
Target Compounds						
26) L6 AR-1254-1	6.471	5.508	2263779	1733786	20.713	23.494
27) L6 AR-1254-2	6.696	5.656	3766036	1761752	23.359	26.742
28) L6 AR-1254-3	7.072	6.061	4197735	2372380	26.789	23.474
29) L6 AR-1254-4	7.367	6.291	2546728	1323075	25.261	22.861
30) L6 AR-1254-5	7.797	6.710	2501706	2474252	22.294	28.144 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081023\
Data File : PO096908.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Aug 2023 11:20
Operator : YP/AJ
Sample : 03572-09
Misc : AR1254 MDL 25 PPB
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 10 21:35:37 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO080723.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 08 04:34:41 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

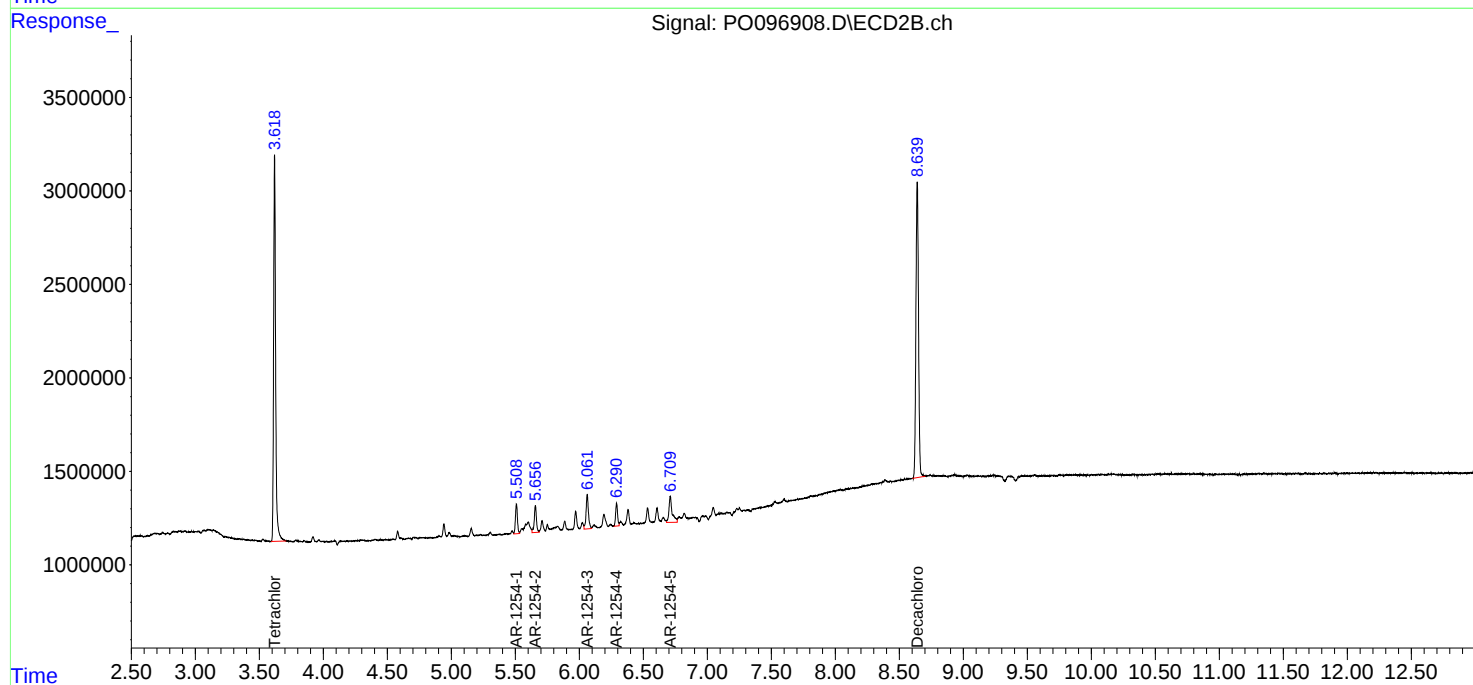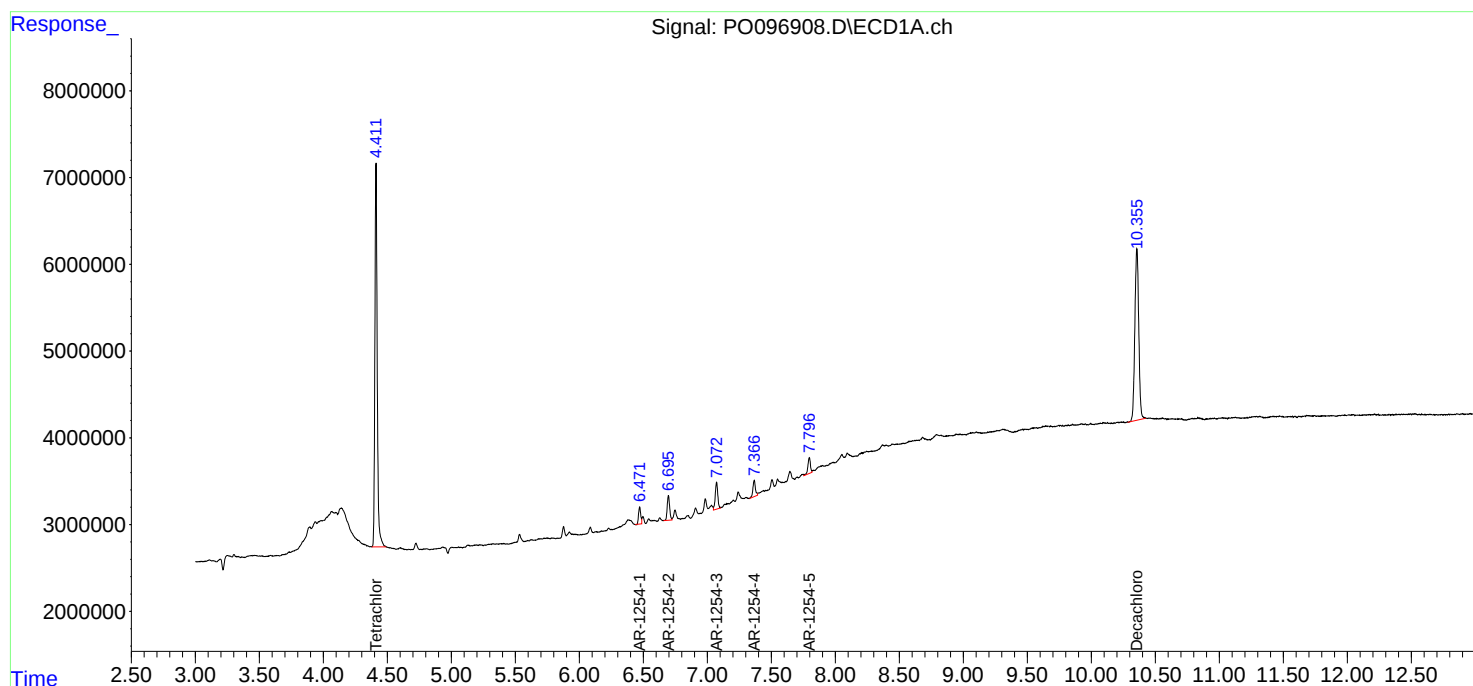


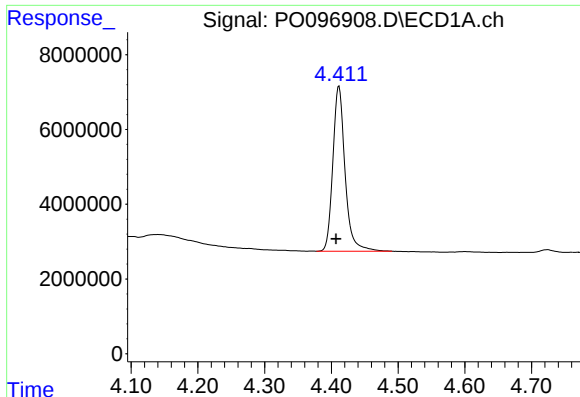

#1 Tetrachloro-m-xylene


R.T.: 4.411 min
Delta R.T.: 0.004 min
Response: 56215369
Conc: 16.98 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2023

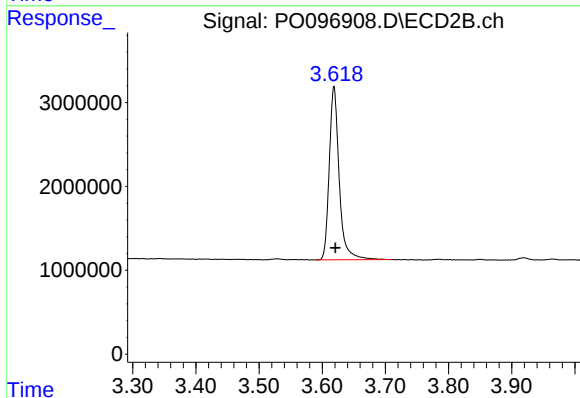


#1 Tetrachloro-m-xylene

R.T.: 3.619 min
Delta R.T.: -0.002 min
Response: 22602291
Conc: 17.07 ng/ml

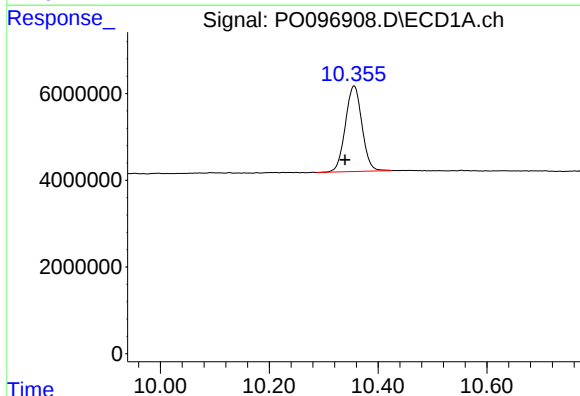


#2 Decachlorobiphenyl

R.T.: 10.356 min
Delta R.T.: 0.016 min
Response: 41735986
Conc: 19.07 ng/ml

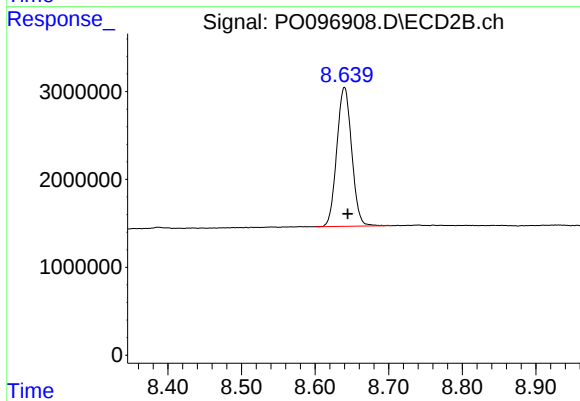

#2 Decachlorobiphenyl


R.T.: 8.640 min
Delta R.T.: -0.004 min
Response: 22199855
Conc: 19.19 ng/ml

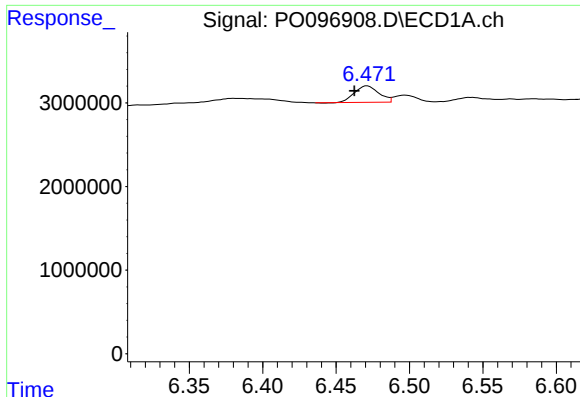

#26 AR-1254-1


R.T.: 6.471 min
Delta R.T.: 0.009 min
Response: 2263779
Conc: 20.71 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2023

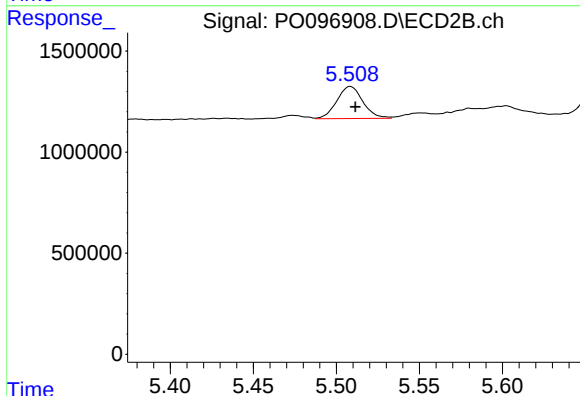


#26 AR-1254-1

R.T.: 5.508 min
Delta R.T.: -0.003 min
Response: 1733786
Conc: 23.49 ng/ml

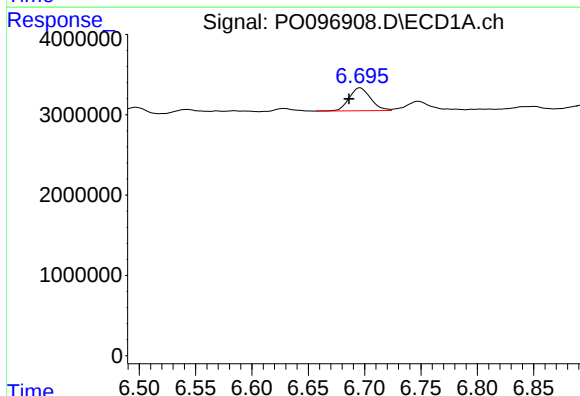


#27 AR-1254-2

R.T.: 6.696 min
Delta R.T.: 0.010 min
Response: 3766036
Conc: 23.36 ng/ml

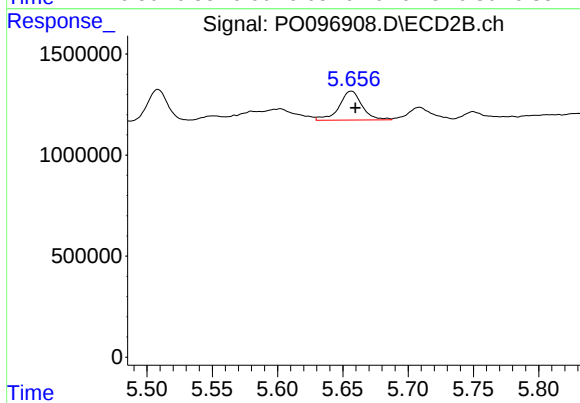

#27 AR-1254-2


R.T.: 5.656 min
Delta R.T.: -0.003 min
Response: 1761752
Conc: 26.74 ng/ml

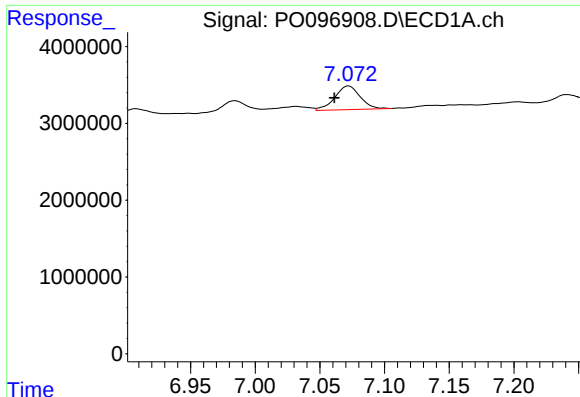

#28 AR-1254-3


R.T.: 7.072 min
Delta R.T.: 0.011 min
Response: 4197735
Conc: 26.79 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2023

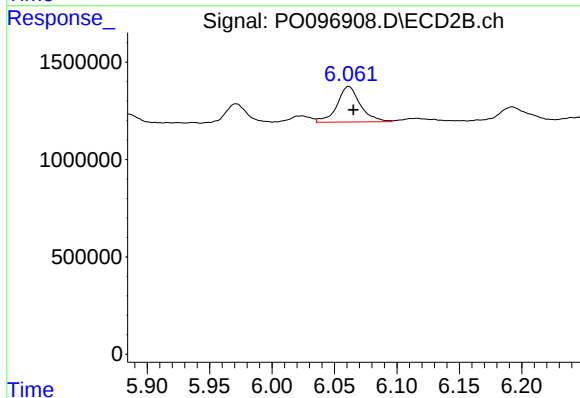


#28 AR-1254-3

R.T.: 6.061 min
Delta R.T.: -0.004 min
Response: 2372380
Conc: 23.47 ng/ml

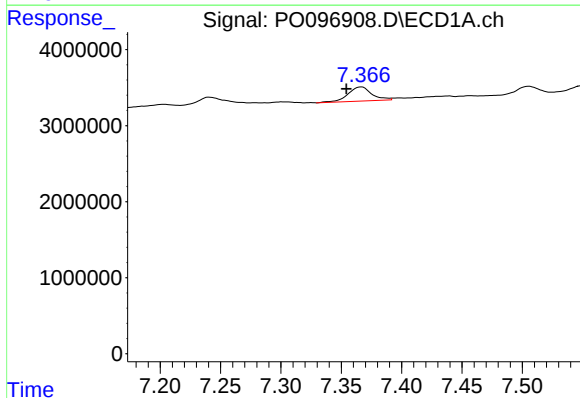


#29 AR-1254-4

R.T.: 7.367 min
Delta R.T.: 0.013 min
Response: 2546728
Conc: 25.26 ng/ml

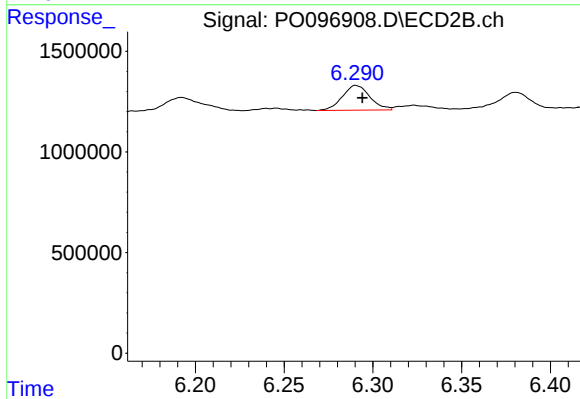

#29 AR-1254-4


R.T.: 6.291 min
Delta R.T.: -0.004 min
Response: 1323075
Conc: 22.86 ng/ml

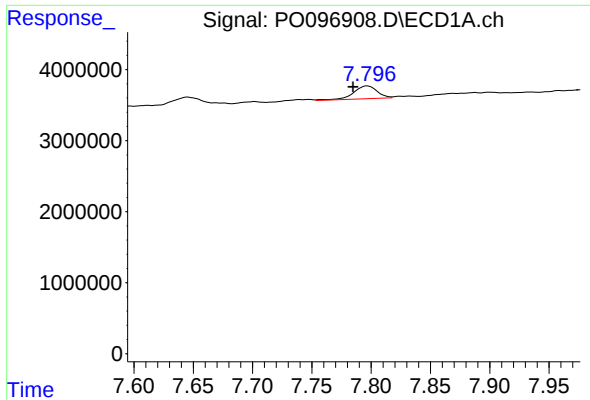

#30 AR-1254-5

R.T.: 7.797 min
Delta R.T.: 0.012 min
Response: 2501706
Conc: 22.29 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2023

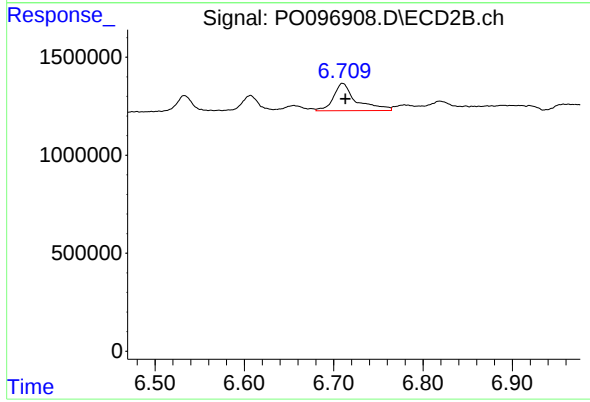

#30 AR-1254-5

R.T.: 6.710 min
Delta R.T.: -0.003 min
Response: 2474252
Conc: 28.14 ng/ml