

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081120\
 Data File : P0070491.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 11 Aug 2020 22:12
 Operator : DD\AJ
 Sample : L3650-13 10X
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PCB-080620-SR-13

Manual Integrations
 APPROVED

mohammad
 8/12/2020 2:48:17 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 12 03:28:39 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0080620.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Aug 06 13:04:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.375	3.561	311409	111214	4.709m	2.524 #
2) SA Decachlor...	10.009	8.753	139136	160564	1.625	2.893 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081120\
Data File : P0070491.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Aug 2020 22:12
Operator : DD\AJ
Sample : L3650-13 10X
Misc :
ALS Vial : 44 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PCB-080620-SR-13


Manual Integrations
APPROVED

mohammad
8/12/2020 2:48:17 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 12 03:28:39 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0080620.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Aug 06 13:04:06 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

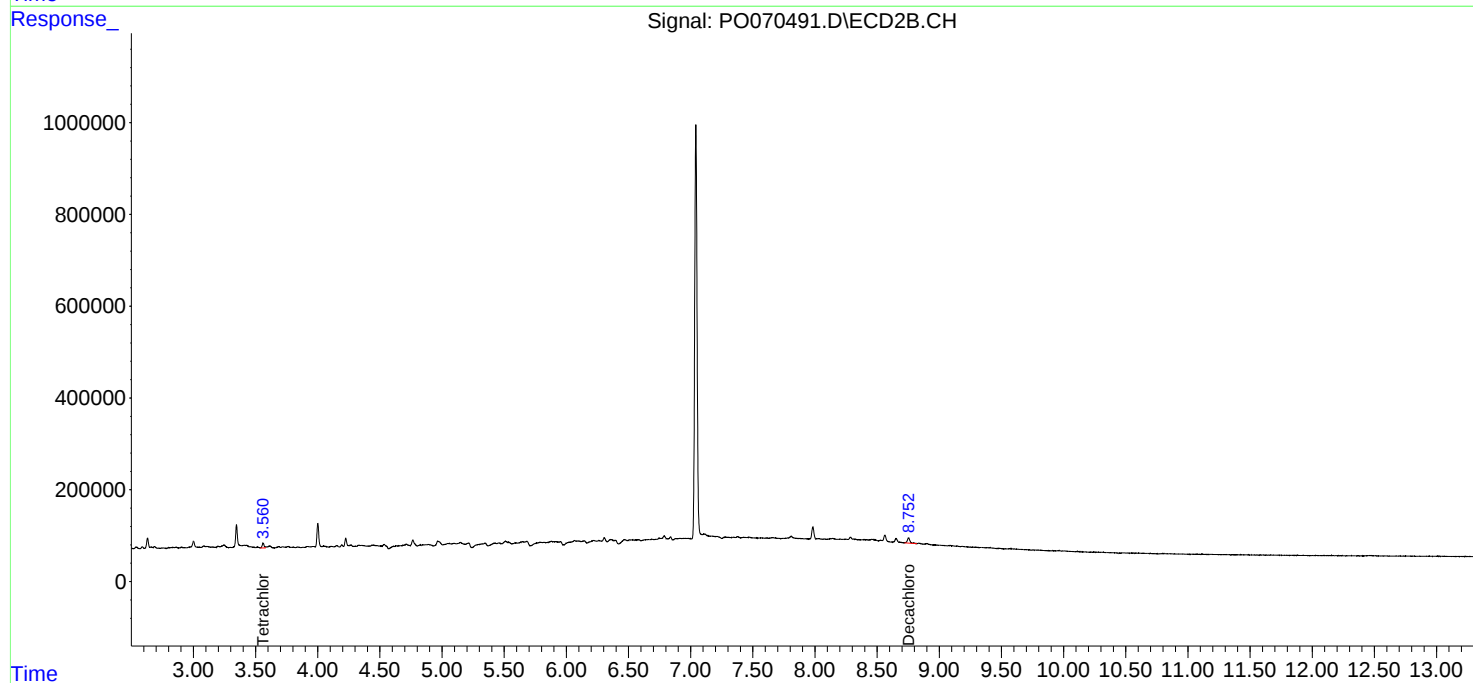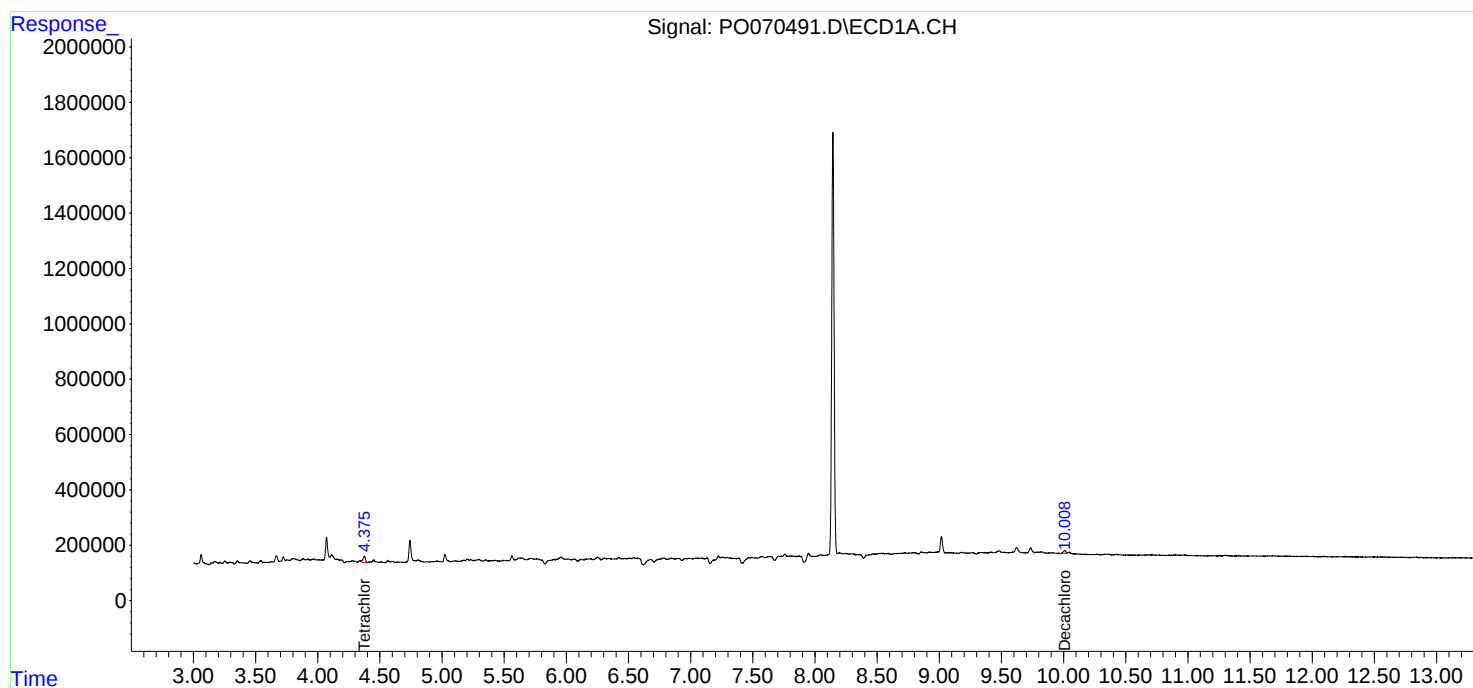

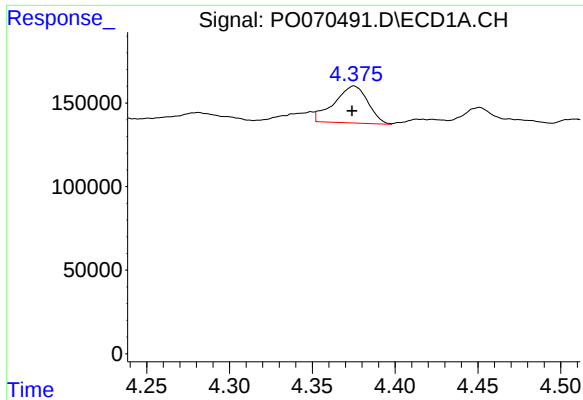


#1 Tetrachloro-m-xylene

R.T.: 4.375 min
Delta R.T.: 0.000 min
Response: 311409
Conc: 4.71 ng/ml m

Instrument :
ECD_O
ClientSampleId :
PCB-080620-SR-13


Manual Integrations
APPROVED

mohammad
8/12/2020 2:48:17 PM

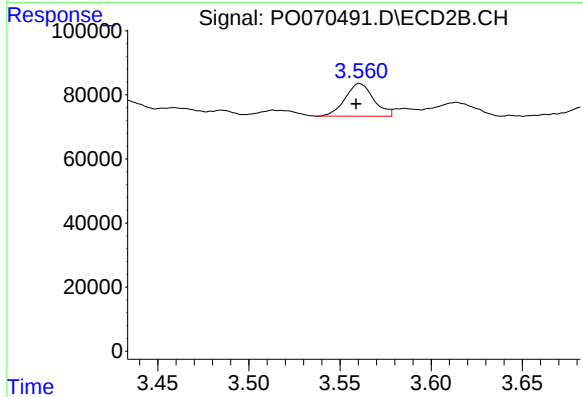


#1 Tetrachloro-m-xylene

R.T.: 3.561 min
Delta R.T.: 0.002 min
Response: 111214
Conc: 2.52 ng/ml

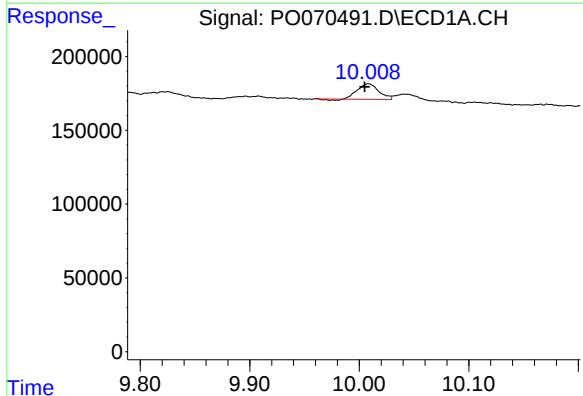

#2 Decachlorobiphenyl

R.T.: 10.009 min
Delta R.T.: 0.004 min
Response: 139136
Conc: 1.62 ng/ml

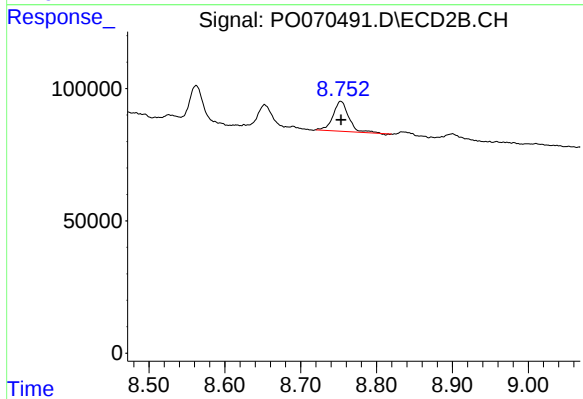

#2 Decachlorobiphenyl

R.T.: 8.753 min
Delta R.T.: 0.000 min
Response: 160564
Conc: 2.89 ng/ml