

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081219\
 Data File : P0059158.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Aug 2019 10:05
 Operator : SM/SJ
 Sample : K4227-04
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 1S-J-(0-1)-COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 00:56:35 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072819.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jul 27 06:49:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.150	3.513	993694	821163	23.546	20.555
2)	SA Decachlor...	9.648	8.389	937394	659803	17.309	16.715

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081219\
Data File : P0059158.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Aug 2019 10:05
Operator : SM/SJ
Sample : K4227-04
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
1S-J-(0-1)-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 13 00:56:35 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072819.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jul 27 06:49:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

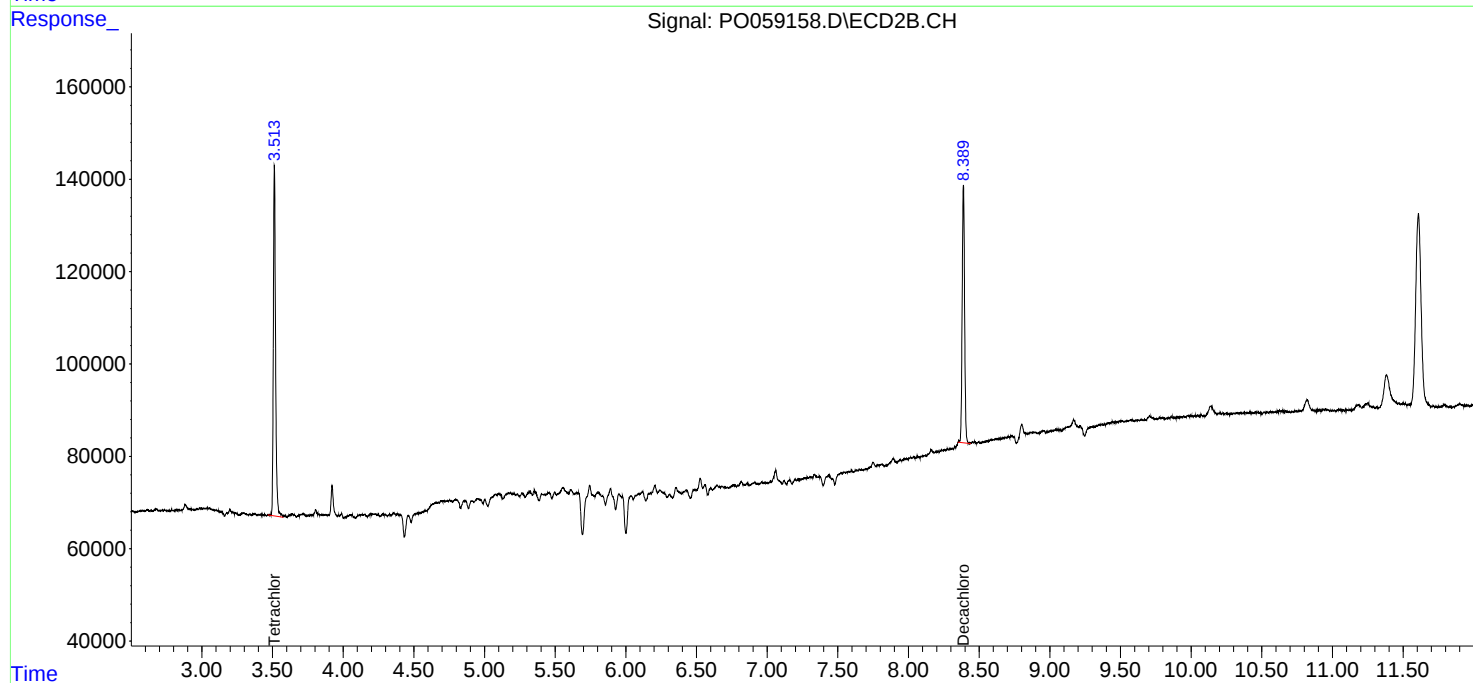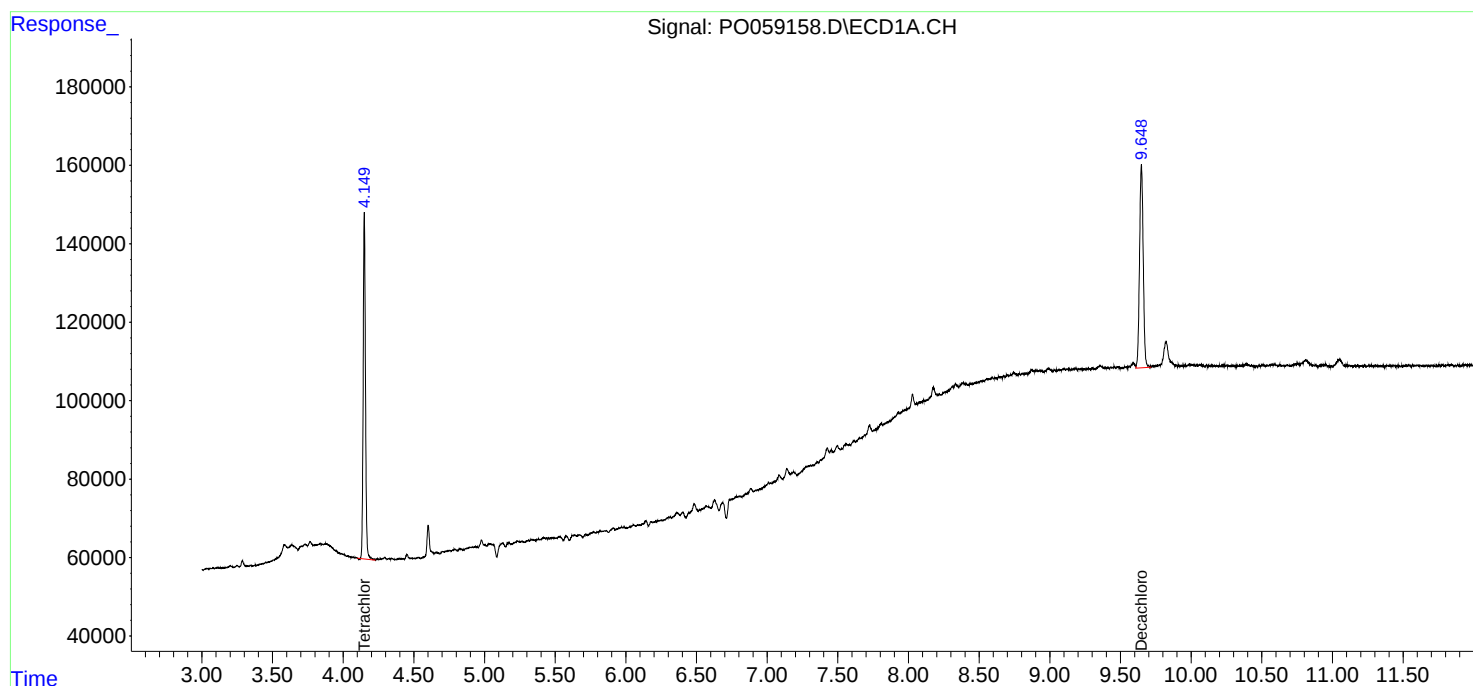


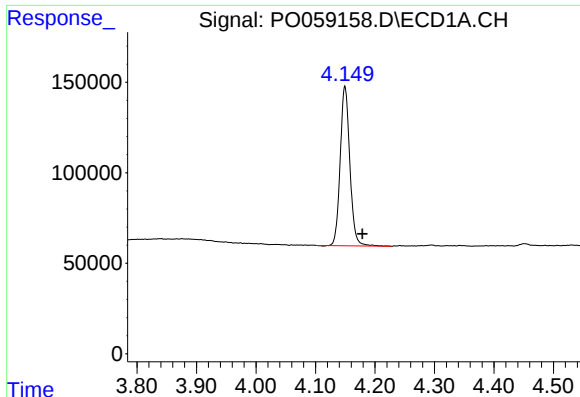

#1 Tetrachloro-m-xylene


R.T.: 4.150 min
Delta R.T.: -0.029 min
Response: 993694
Conc: 23.55 ng/ml

Instrument :
ECD_O
ClientSampleId :
1S-J-(0-1)-COMP

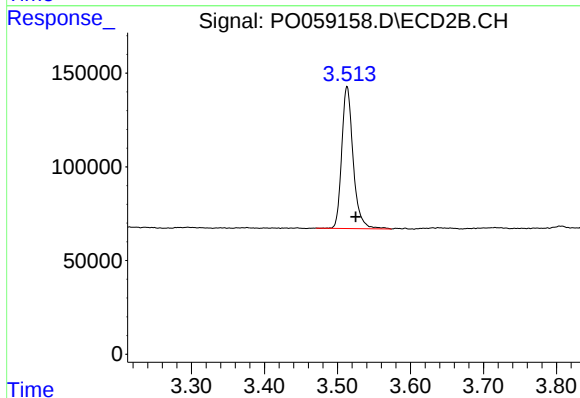


#1 Tetrachloro-m-xylene

R.T.: 3.513 min
Delta R.T.: -0.012 min
Response: 821163
Conc: 20.55 ng/ml

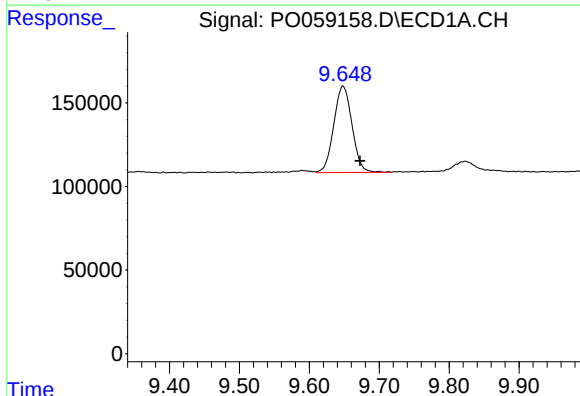

#2 Decachlorobiphenyl

R.T.: 9.648 min
Delta R.T.: -0.024 min
Response: 937394
Conc: 17.31 ng/ml

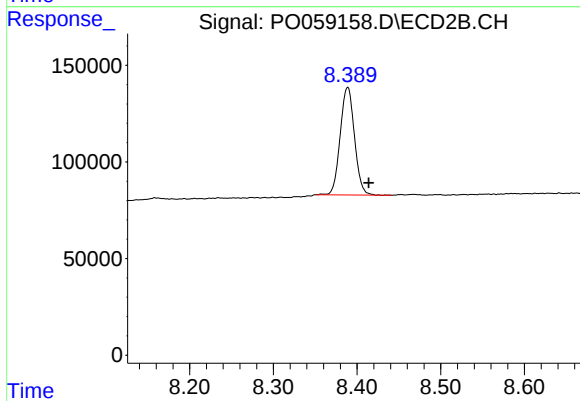

#2 Decachlorobiphenyl

R.T.: 8.389 min
Delta R.T.: -0.025 min
Response: 659803
Conc: 16.72 ng/ml