

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081219\
 Data File : P0059184.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Aug 2019 17:27
 Operator : SM/SJ
 Sample : K4267-05RE
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PS-05RE

Manual Integrations
 APPROVED

Ankita
 8/14/2019 9:36:39 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 01:06:53 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072819.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jul 27 06:49:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.154	3.514	830326	739412	19.675	18.508
2)	SA Decachlor...	9.656	8.391	556771	393710	10.281	9.974
Target Compounds							
26)	L6 AR-1254-1	6.147	5.351	685478	695757	290.298m	268.576m
27)	L6 AR-1254-2	6.363	5.496	1133354	619282	294.076m	270.496m
28)	L6 AR-1254-3	6.731	5.893	1105567	995901	273.004	270.672m
29)	L6 AR-1254-4	7.014	6.120	945628	617933	262.628	265.753m
30)	L6 AR-1254-5	7.429	6.530	913216	882985	251.938m	255.971

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081219\
Data File : PO059184.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Aug 2019 17:27
Operator : SM/SJ
Sample : K4267-05RE
Misc :
ALS Vial : 30 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
PS-05RE


Manual Integrations
APPROVED

Ankita
8/14/2019 9:36:39 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 13 01:06:53 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO072819.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jul 27 06:49:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

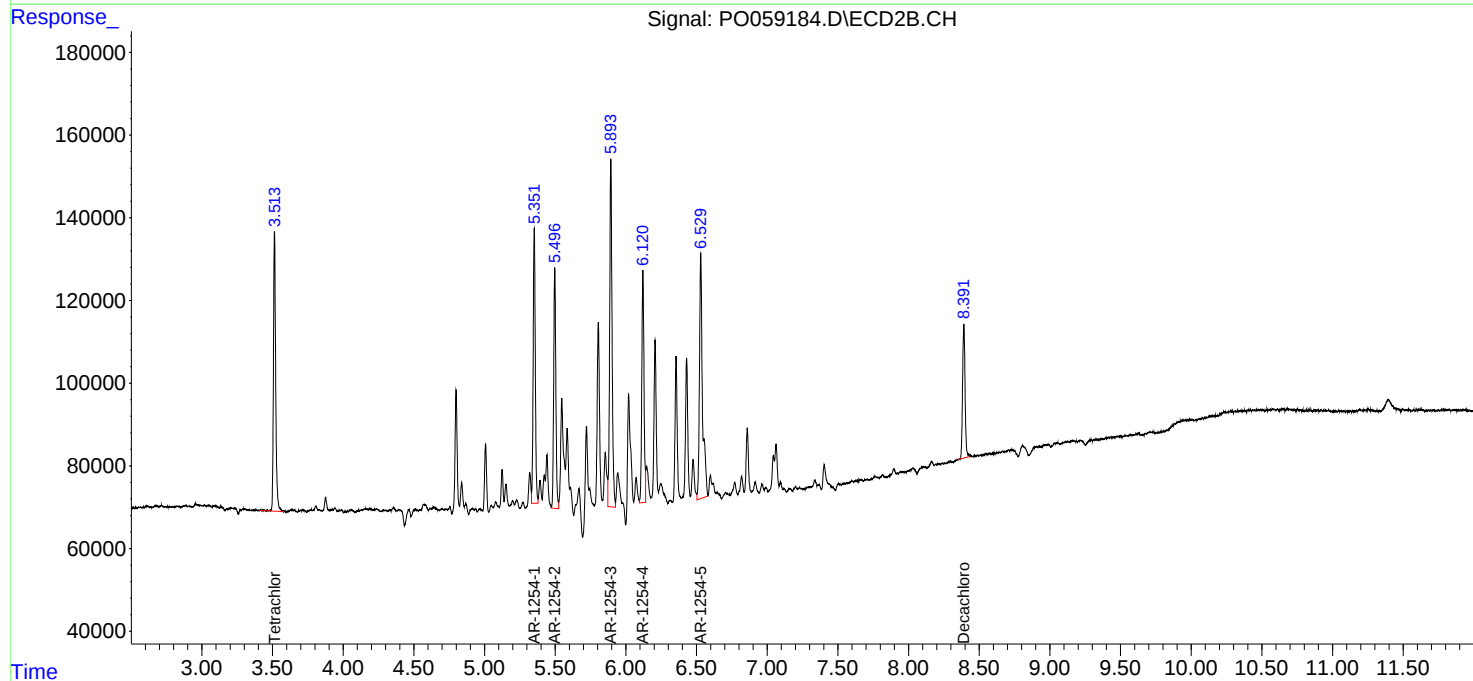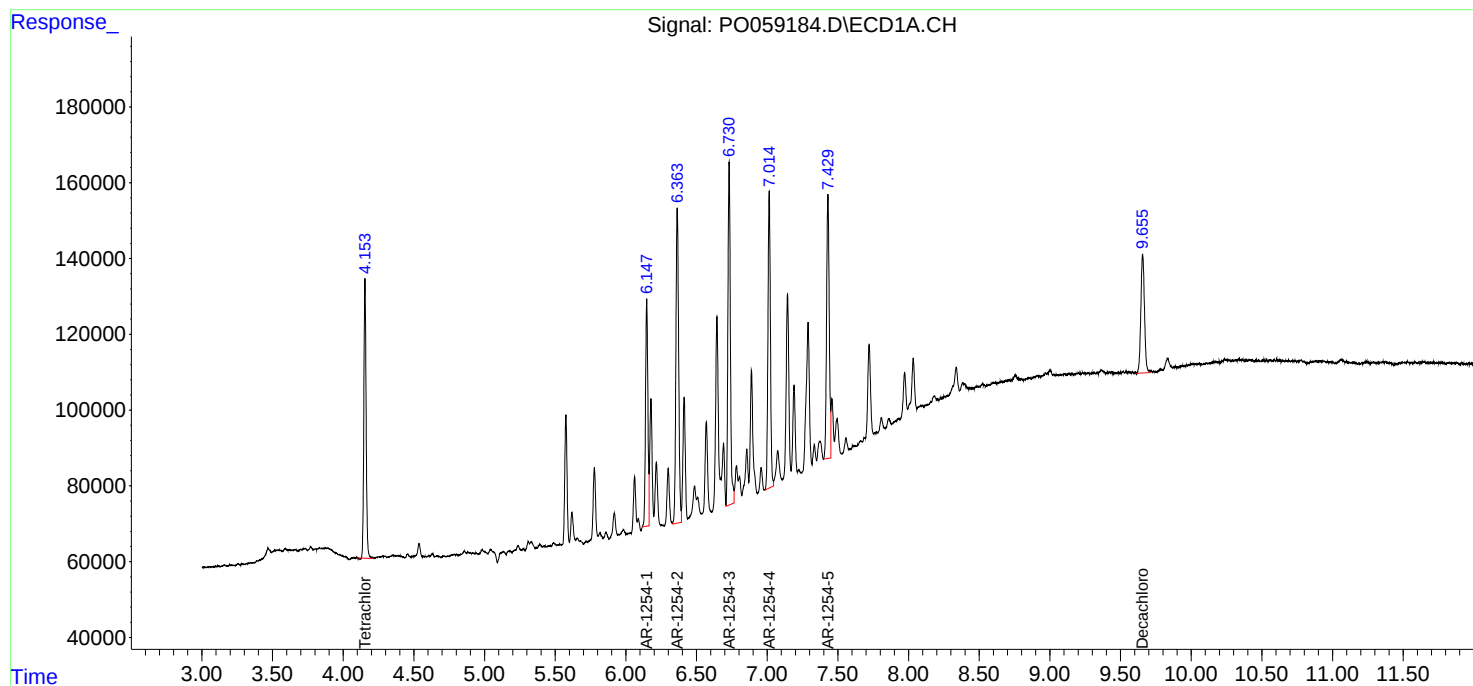

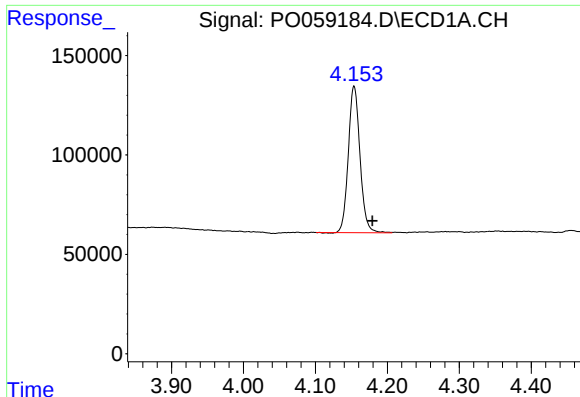


#1 Tetrachloro-m-xylene

R.T.: 4.154 min
Delta R.T.: -0.025 min
Response: 830326
Conc: 19.67 ng/ml

Instrument :
ECD_O
ClientSampleId :
PS-05RE


Manual Integrations
APPROVED

Ankita
8/14/2019 9:36:39 AM

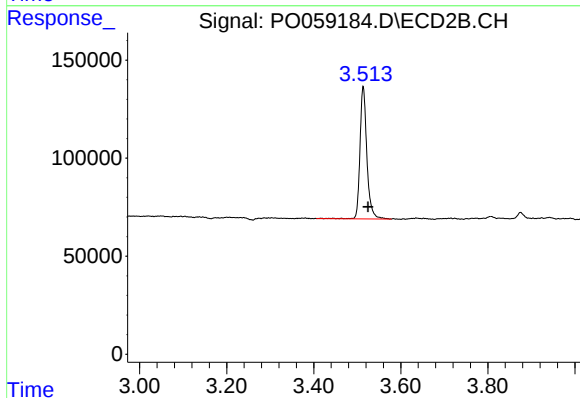


#1 Tetrachloro-m-xylene

R.T.: 3.514 min
Delta R.T.: -0.011 min
Response: 739412
Conc: 18.51 ng/ml

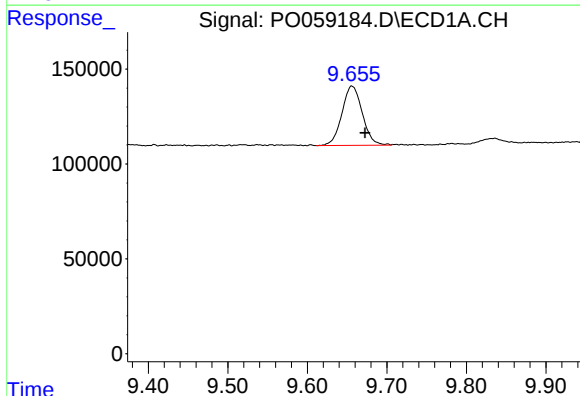


#2 Decachlorobiphenyl

R.T.: 9.656 min
Delta R.T.: -0.017 min
Response: 556771
Conc: 10.28 ng/ml

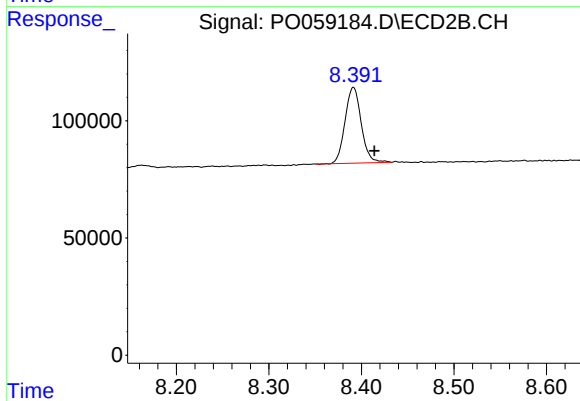

#2 Decachlorobiphenyl

R.T.: 8.391 min
Delta R.T.: -0.023 min
Response: 393710
Conc: 9.97 ng/ml

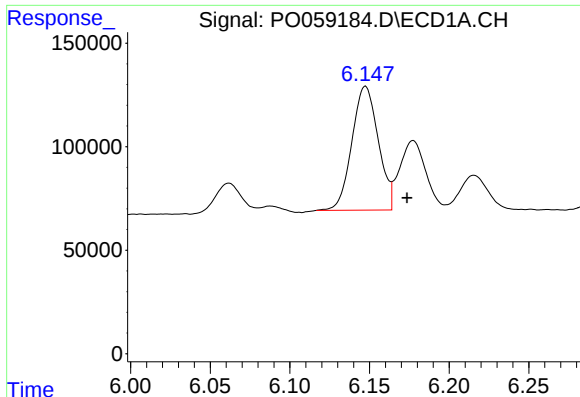


#26 AR-1254-1

R.T.: 6.147 min
Delta R.T.: -0.026 min
Response: 685478
Conc: 290.30 ng/ml m

Instrument :
ECD_O
ClientSampleId :
PS-05RE


Manual Integrations
APPROVED

Ankita
8/14/2019 9:36:39 AM

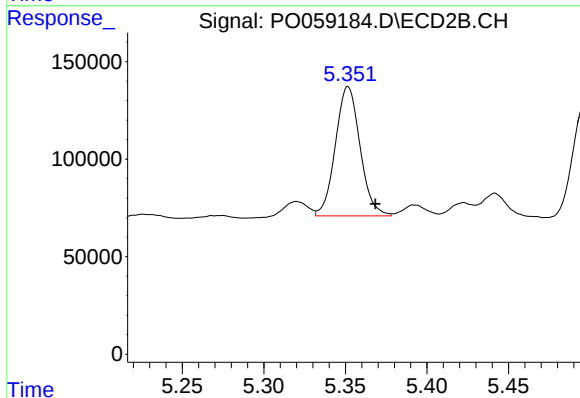


#26 AR-1254-1

R.T.: 5.351 min
Delta R.T.: -0.017 min
Response: 695757
Conc: 268.58 ng/ml m

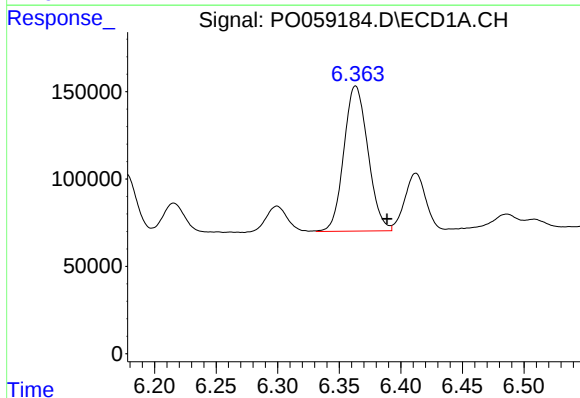


#27 AR-1254-2

R.T.: 6.363 min
Delta R.T.: -0.026 min
Response: 1133354
Conc: 294.08 ng/ml m

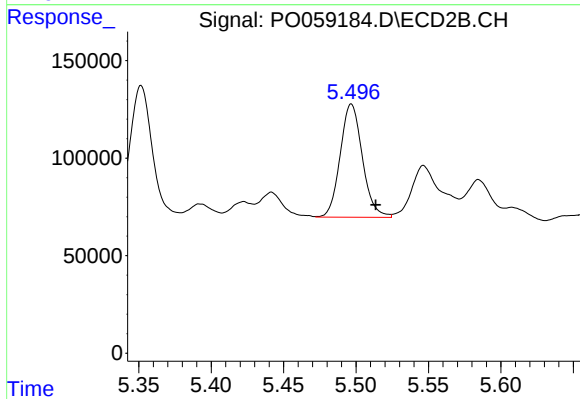

#27 AR-1254-2

R.T.: 5.496 min
Delta R.T.: -0.017 min
Response: 619282
Conc: 270.50 ng/ml m

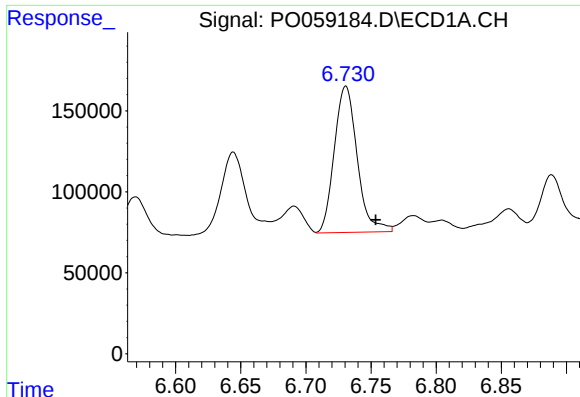


#28 AR-1254-3

R.T.: 6.731 min
Delta R.T.: -0.023 min
Response: 1105567
Conc: 273.00 ng/ml

Instrument :
ECD_O
ClientSampleId :
PS-05RE


Manual Integrations
APPROVED

Ankita
8/14/2019 9:36:39 AM

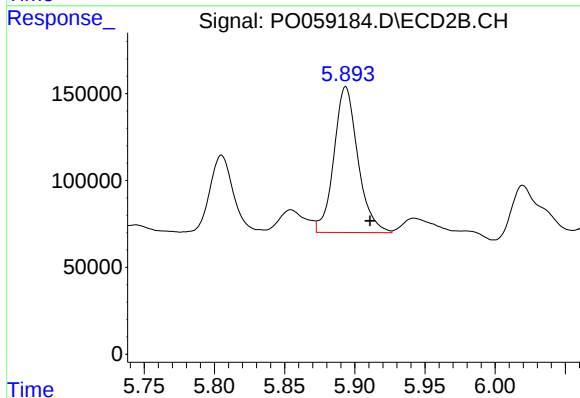


#28 AR-1254-3

R.T.: 5.893 min
Delta R.T.: -0.018 min
Response: 995901
Conc: 270.67 ng/ml m

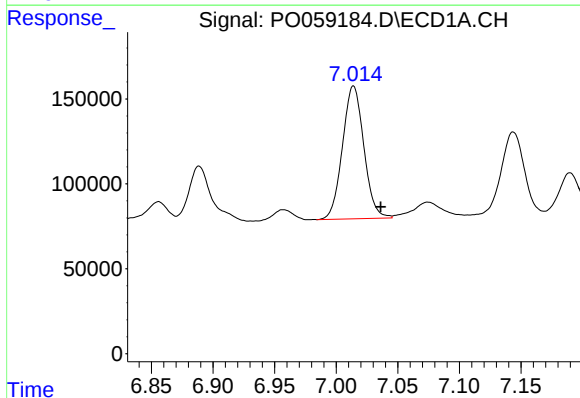


#29 AR-1254-4

R.T.: 7.014 min
Delta R.T.: -0.022 min
Response: 945628
Conc: 262.63 ng/ml

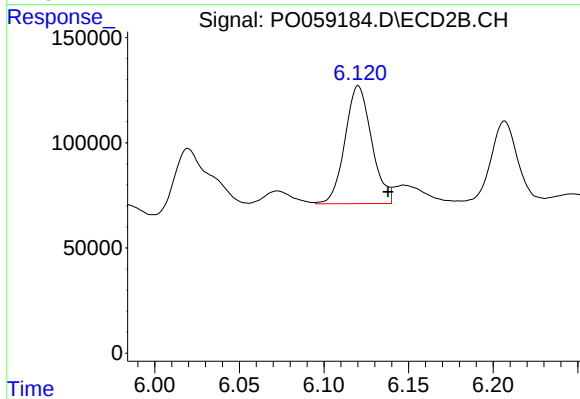

#29 AR-1254-4

R.T.: 6.120 min
Delta R.T.: -0.018 min
Response: 617933
Conc: 265.75 ng/ml m

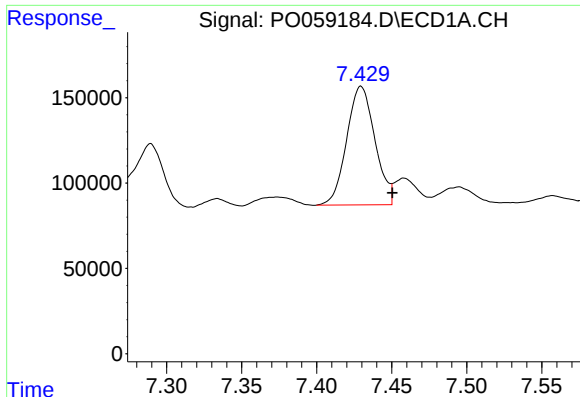


#30 AR-1254-5

R.T.: 7.429 min
Delta R.T.: -0.021 min
Response: 913216
Conc: 251.94 ng/ml m

Instrument :
ECD_O
ClientSampleId :
PS-05RE

Manual Integrations
APPROVED

Ankita
8/14/2019 9:36:39 AM

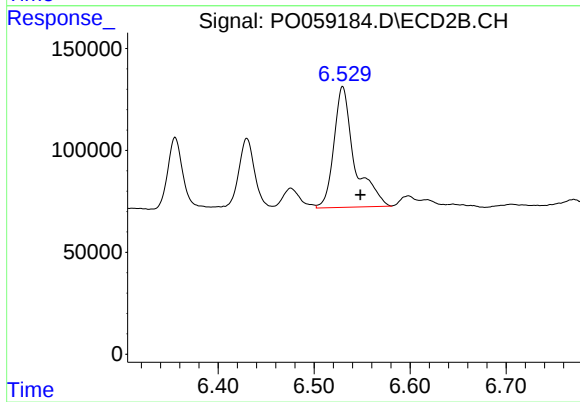

#30 AR-1254-5

R.T.: 6.530 min
Delta R.T.: -0.018 min
Response: 882985
Conc: 255.97 ng/ml