

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081219\
 Data File : P0059213.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Aug 2019 1:28
 Operator : SM/SJ
 Sample : K4292-01
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 RO-COMP-WS

Manual Integrations
 APPROVED

Ankita
 8/14/2019 9:37:29 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 04:22:25 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072819.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jul 27 06:49:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.151	3.512	801708	676487	18.997	16.933m
2) SA Decachlor...	9.651	8.389	803695	495447	14.841	12.552m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081219\
Data File : P0059213.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Aug 2019 1:28
Operator : SM/SJ
Sample : K4292-01
Misc :
ALS Vial : 57 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
RO-COMP-WS


Manual Integrations
APPROVED

Ankita
8/14/2019 9:37:29 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 13 04:22:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072819.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jul 27 06:49:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

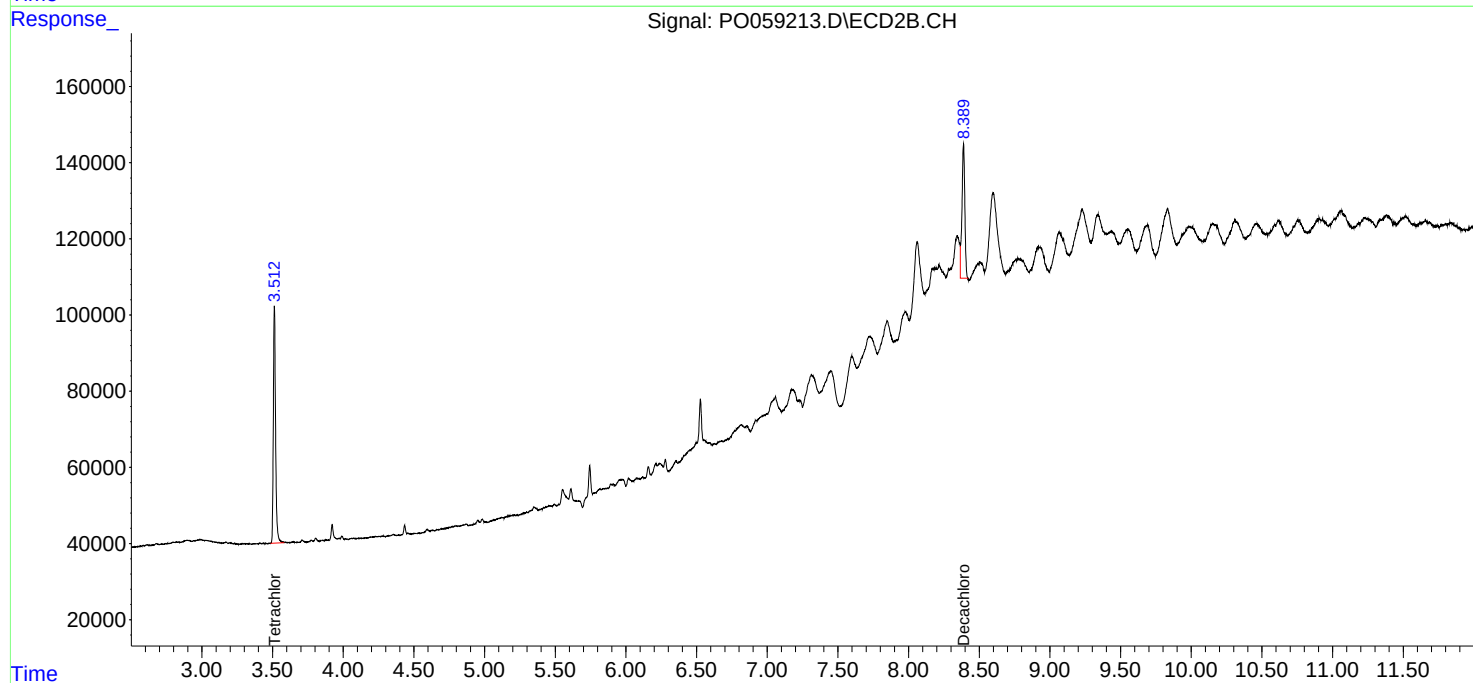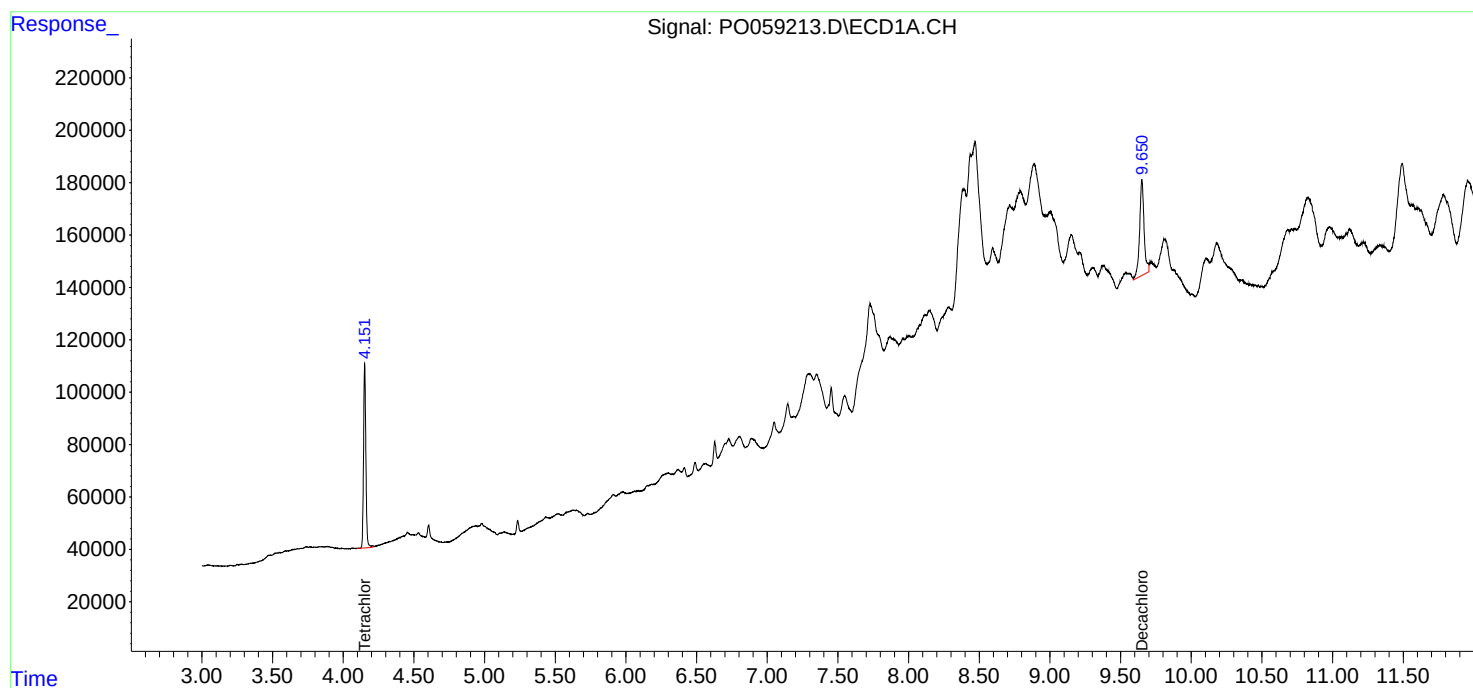

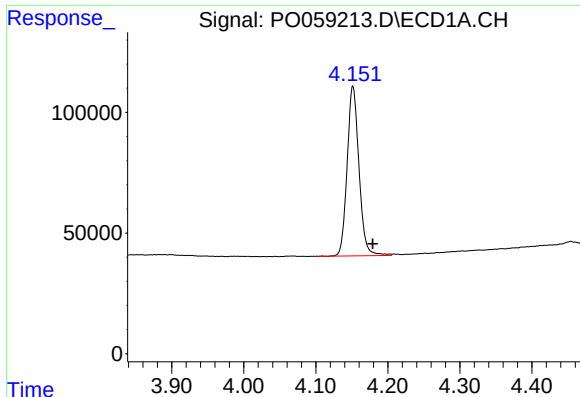


#1 Tetrachloro-m-xylene

R.T.: 4.151 min
Delta R.T.: -0.028 min
Response: 801708
Conc: 19.00 ng/ml

Instrument :
ECD_O
ClientSampleId :
RO-COMP-WS


Manual Integrations
APPROVED

Ankita
8/14/2019 9:37:29 AM

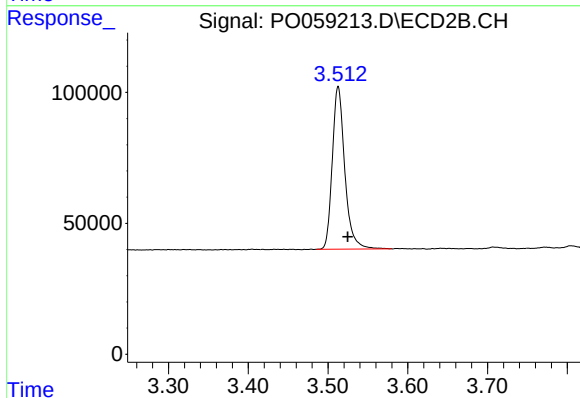


#1 Tetrachloro-m-xylene

R.T.: 3.512 min
Delta R.T.: -0.012 min
Response: 676487
Conc: 16.93 ng/ml m

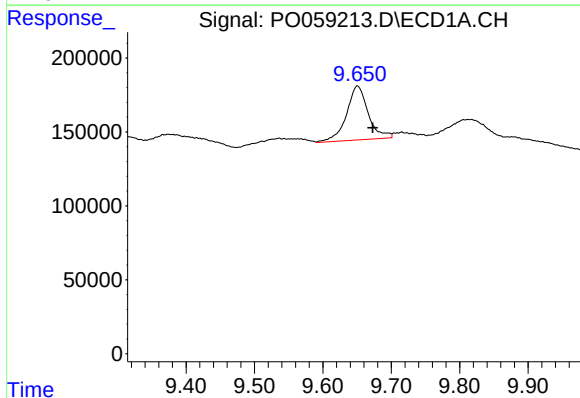

#2 Decachlorobiphenyl

R.T.: 9.651 min
Delta R.T.: -0.022 min
Response: 803695
Conc: 14.84 ng/ml

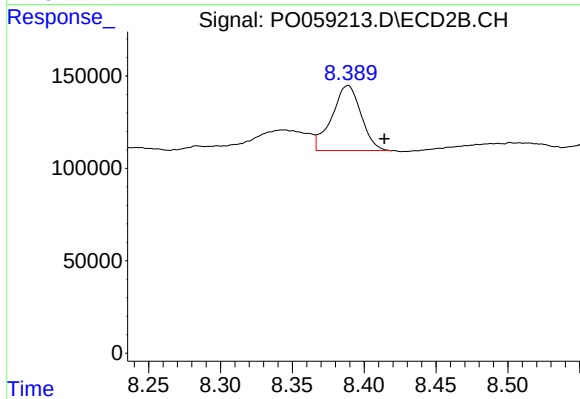

#2 Decachlorobiphenyl

R.T.: 8.389 min
Delta R.T.: -0.025 min
Response: 495447
Conc: 12.55 ng/ml m