

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081220\
 Data File : P0070527.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Aug 2020 18:31
 Operator : DD\AJ
 Sample : L3645-02
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 06:29:53 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0080620.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Aug 06 13:04:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.376	3.560	1881225	1168971	28.449	26.532
2) SA Decachlor...	10.005	8.750	1840616	1108938	21.496	19.978
Target Compounds						
3) L1 AR-1016-1	5.695	0.000	112619	0	39.004	N.D. #
4) L1 AR-1016-2	5.695	0.000	112619	0	27.233	N.D. #
9) L2 AR-1221-2	4.722	0.000	26691	0	42.426	N.D. #
13) L3 AR-1232-3	5.695	0.000	112619	0	63.157	N.D. #
16) L4 AR-1242-1	5.695f	0.000	112619	0	47.810	N.D. #
17) L4 AR-1242-2	5.695	0.000	112619	0	33.380	N.D. #
21) L5 AR-1248-1	5.695f	0.000	112619	0	63.354	N.D. #
43) L9 AR-1268-3	0.000	7.975	0	114761	N.D.	14.271 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081220\
Data File : PO070527.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Aug 2020 18:31
Operator : DD\AJ
Sample : L3645-02
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 13 06:29:53 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO080620.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Aug 06 13:04:06 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

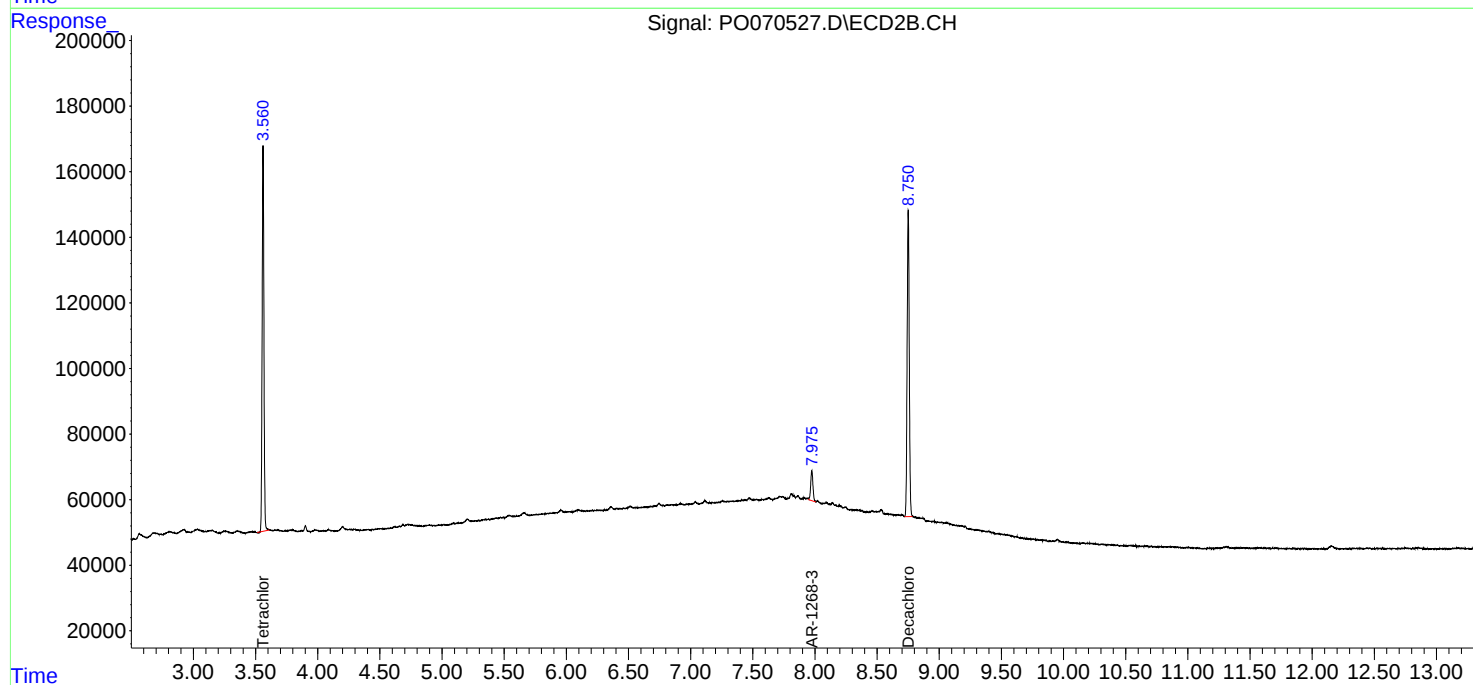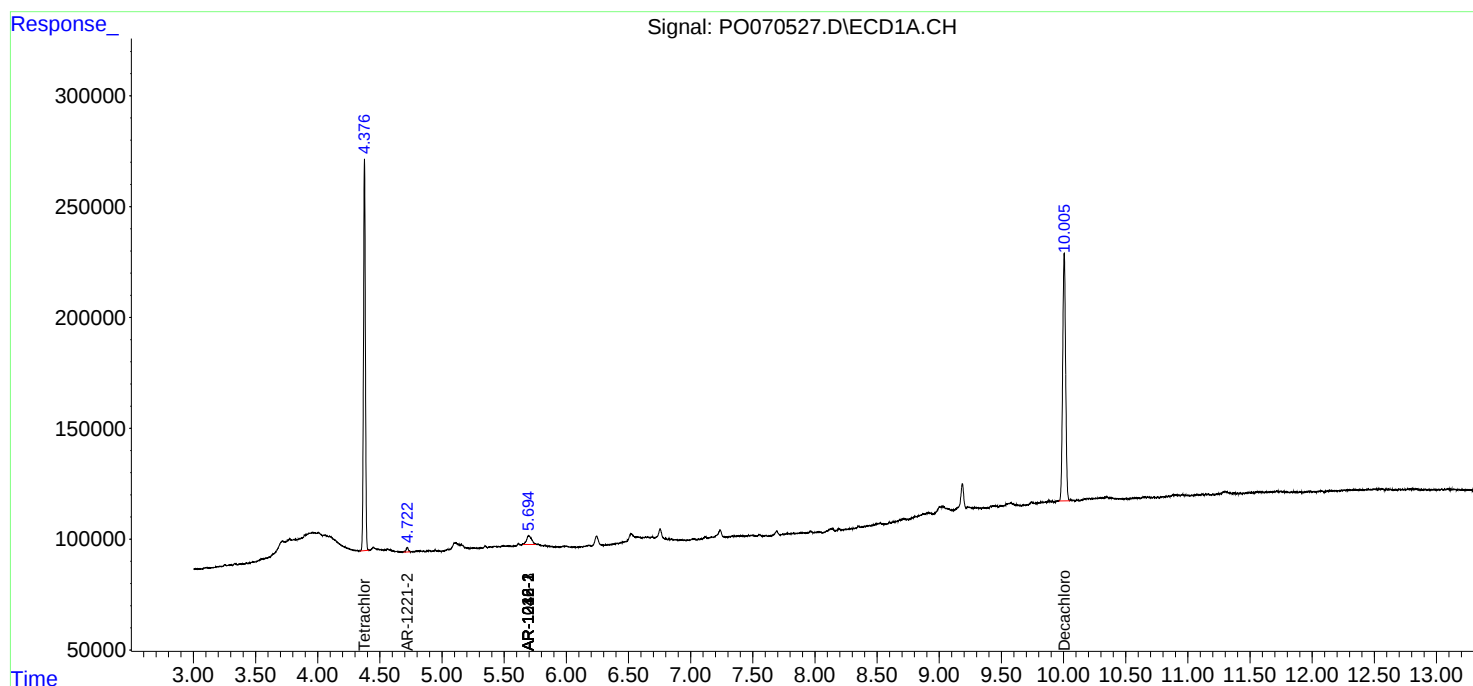


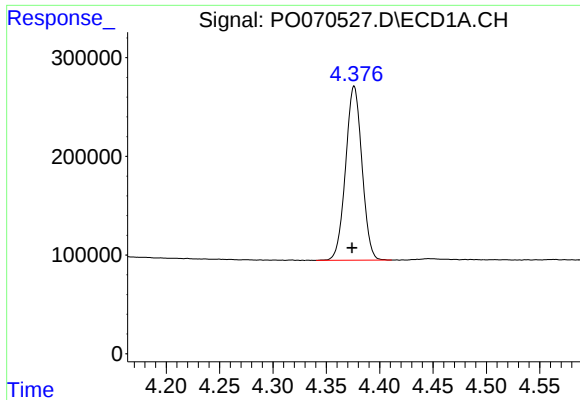

#1 Tetrachloro-m-xylene


R.T.: 4.376 min
Delta R.T.: 0.002 min
Response: 1881225
Conc: 28.45 ng/ml

Instrument :
ECD_O
ClientSampleId :

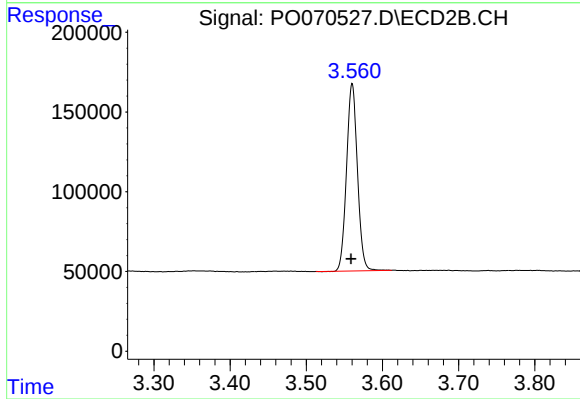


#1 Tetrachloro-m-xylene

R.T.: 3.560 min
Delta R.T.: 0.001 min
Response: 1168971
Conc: 26.53 ng/ml

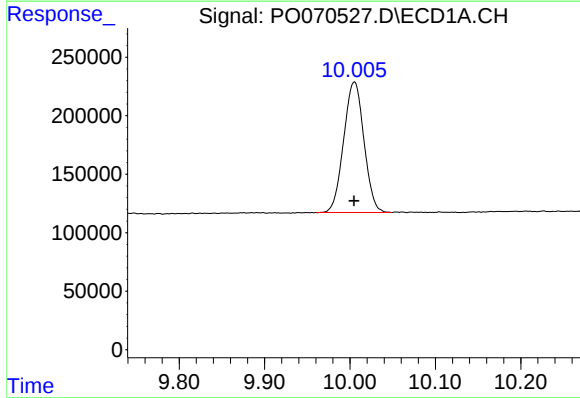


#2 Decachlorobiphenyl

R.T.: 10.005 min
Delta R.T.: 0.000 min
Response: 1840616
Conc: 21.50 ng/ml

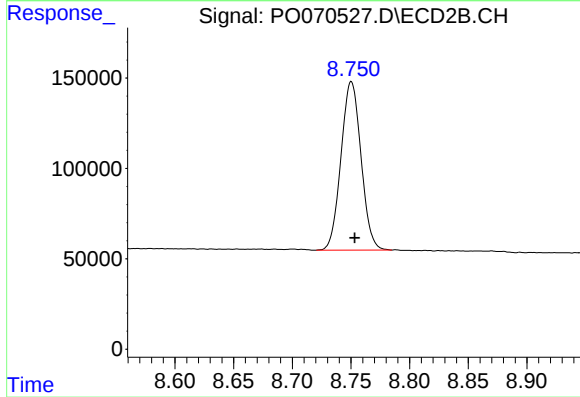

#2 Decachlorobiphenyl


R.T.: 8.750 min
Delta R.T.: -0.003 min
Response: 1108938
Conc: 19.98 ng/ml

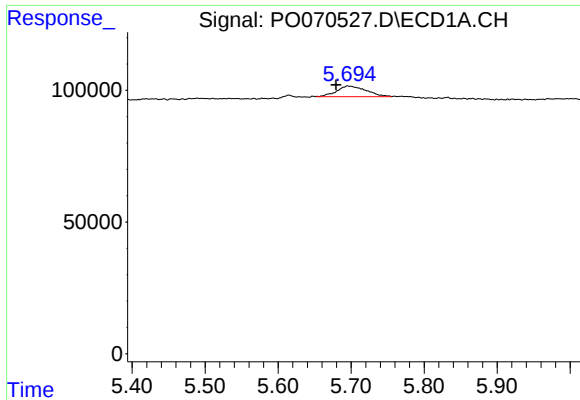

#3 AR-1016-1


R.T.: 5.695 min
Delta R.T.: 0.016 min
Response: 112619
Conc: 39.00 ng/ml

Instrument :
ECD_O
ClientSampleId :

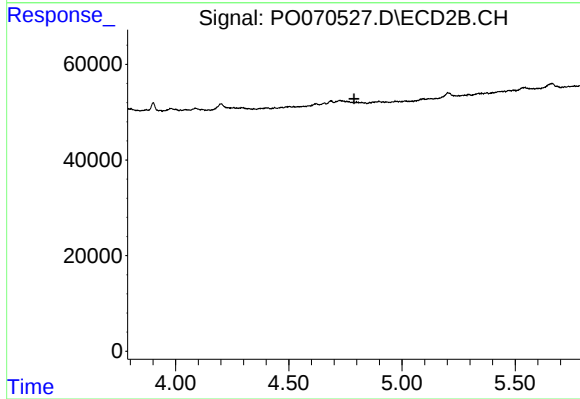


#3 AR-1016-1

R.T.: 0.000 min
Exp R.T. : 4.788 min
Response: 0
Conc: N.D.

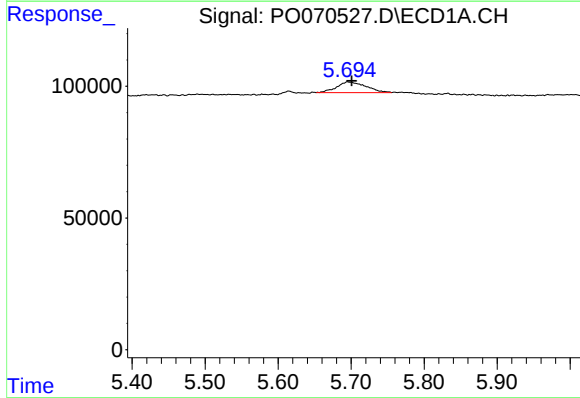


#4 AR-1016-2

R.T.: 5.695 min
Delta R.T.: -0.006 min
Response: 112619
Conc: 27.23 ng/ml

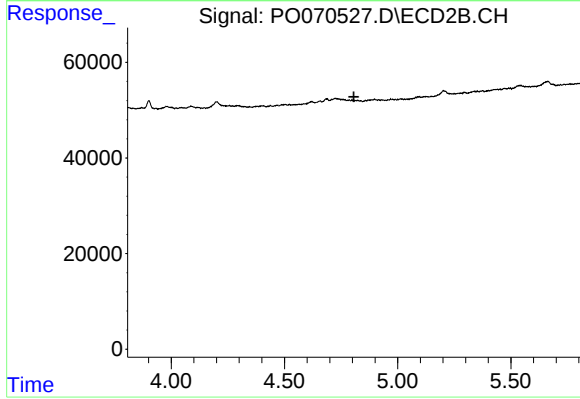

#4 AR-1016-2


R.T.: 0.000 min
Exp R.T. : 4.807 min
Response: 0
Conc: N.D.

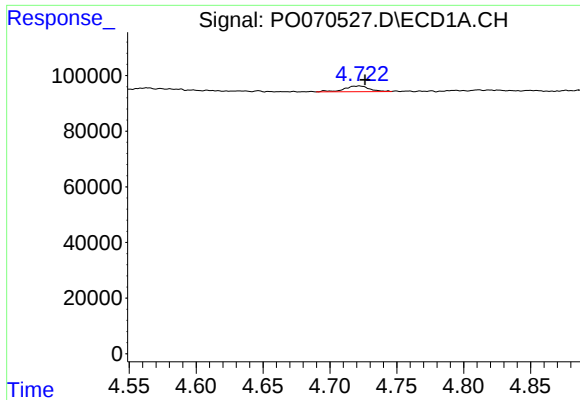

#9 AR-1221-2


R.T.: 4.722 min
Delta R.T.: -0.004 min
Response: 26691
Conc: 42.43 ng/ml

Instrument :
ECD_O
ClientSampleId :

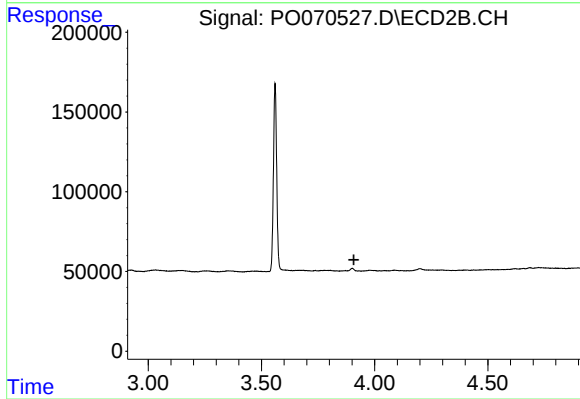


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 3.908 min
Response: 0
Conc: N.D.

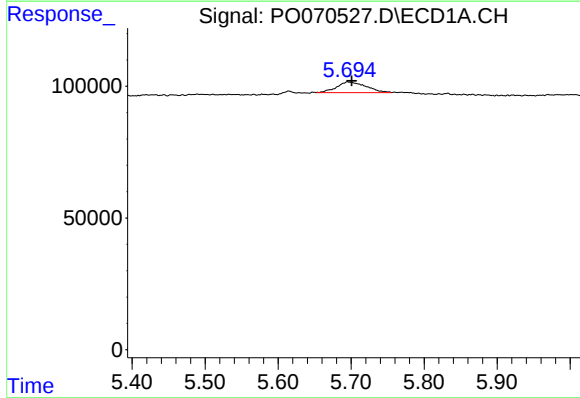


#13 AR-1232-3

R.T.: 5.695 min
Delta R.T.: -0.006 min
Response: 112619
Conc: 63.16 ng/ml

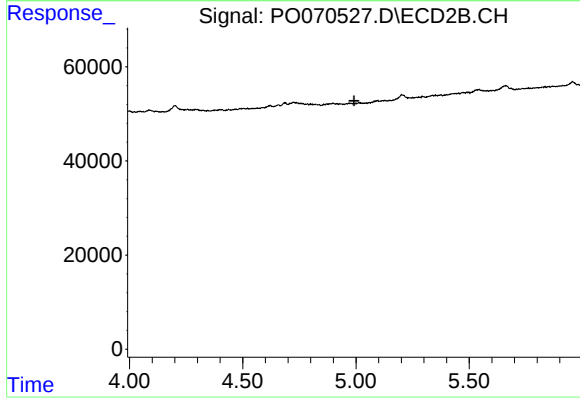

#13 AR-1232-3


R.T.: 0.000 min
Exp R.T. : 4.991 min
Response: 0
Conc: N.D.

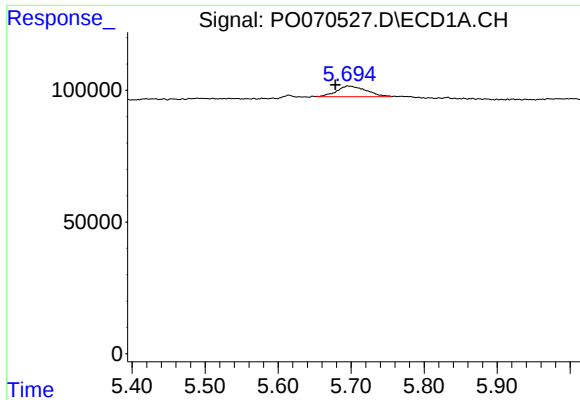

#16 AR-1242-1


R.T.: 5.695 min
Delta R.T.: 0.016 min
Response: 112619
Conc: 47.81 ng/ml

Instrument :
ECD_O
ClientSampleId :

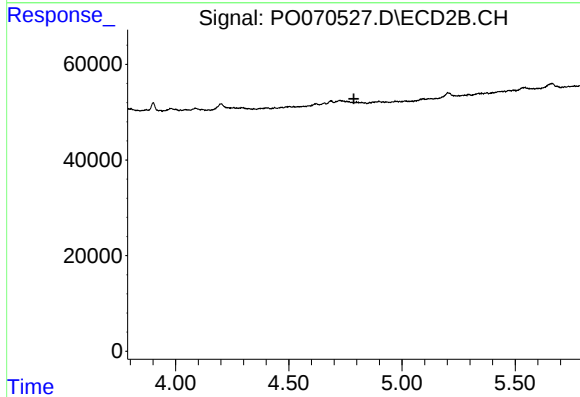


#16 AR-1242-1

R.T.: 0.000 min
Exp R.T. : 4.788 min
Response: 0
Conc: N.D.

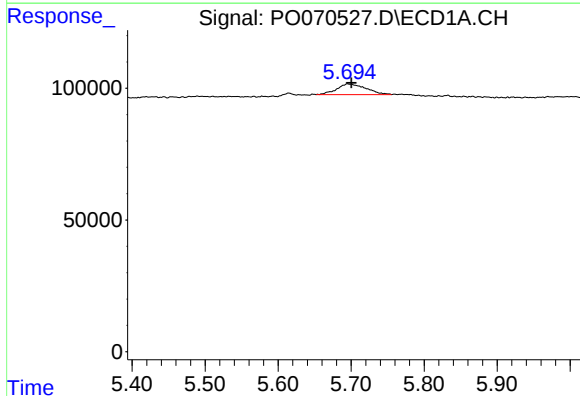


#17 AR-1242-2

R.T.: 5.695 min
Delta R.T.: -0.005 min
Response: 112619
Conc: 33.38 ng/ml

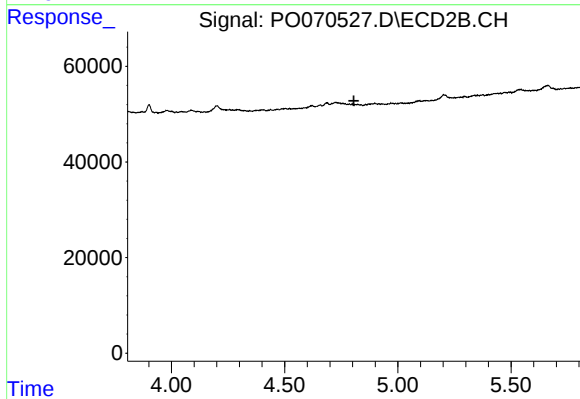

#17 AR-1242-2


R.T.: 0.000 min
Exp R.T. : 4.806 min
Response: 0
Conc: N.D.

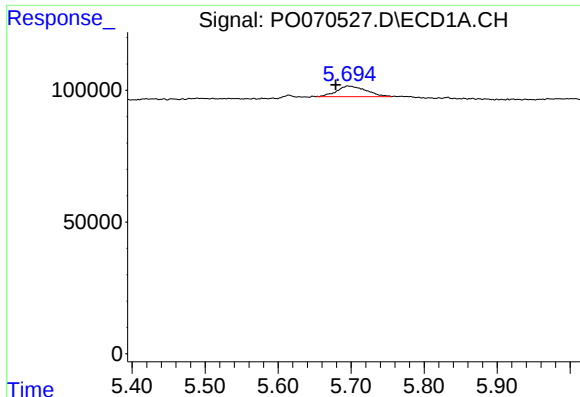

#21 AR-1248-1


R.T.: 5.695 min
Delta R.T.: 0.016 min
Response: 112619
Conc: 63.35 ng/ml

Instrument :
ECD_O
ClientSampleId :

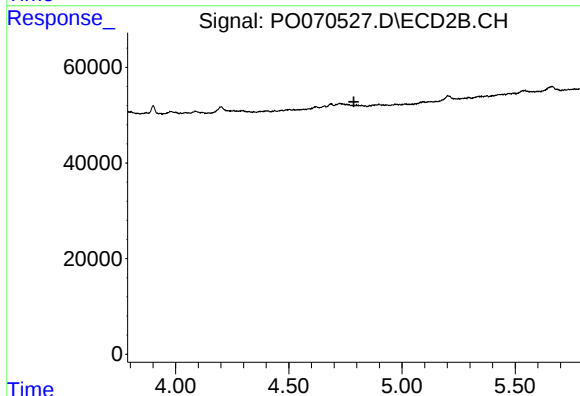


#21 AR-1248-1

R.T.: 0.000 min
Exp R.T. : 4.788 min
Response: 0
Conc: N.D.

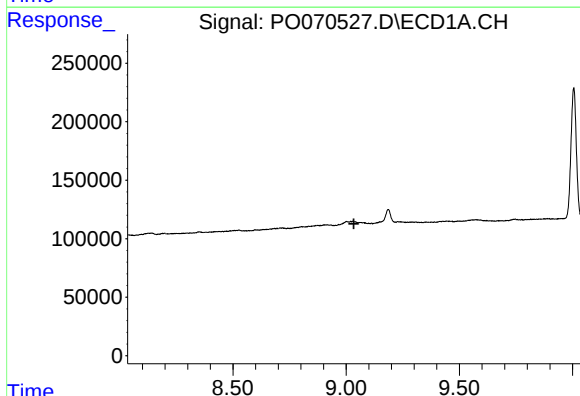

#43 AR-1268-3

R.T.: 0.000 min
Exp R.T. : 9.034 min
Response: 0
Conc: N.D.

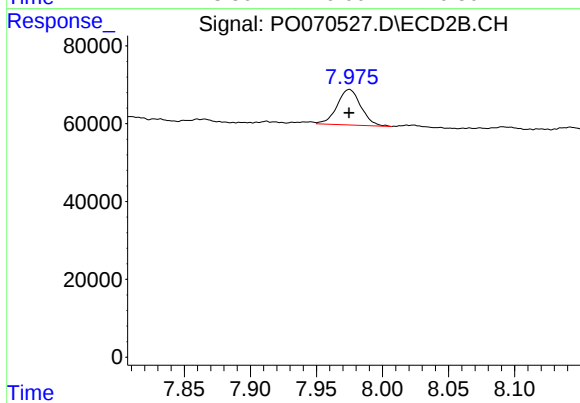

#43 AR-1268-3

R.T.: 7.975 min
Delta R.T.: 0.000 min
Response: 114761
Conc: 14.27 ng/ml