

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081220\
 Data File : P0070504.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Aug 2020 11:38
 Operator : DD\AJ
 Sample : L3650-17RE 5X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PCB-080620-SR-17RE

Manual Integrations
 APPROVED

Ankita
 8/14/2020 8:32:37 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 12 14:07:41 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0080620.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Aug 06 13:04:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.375	3.559	445000	286154	6.730m	6.495m
2) SA Decachlor...	10.004	8.748	587949	572307	6.867	10.310 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081220\
Data File : P0070504.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Aug 2020 11:38
Operator : DD\AJ
Sample : L3650-17RE 5X
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PCB-080620-SR-17RE


Manual Integrations
APPROVED

Ankita
8/14/2020 8:32:37 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 12 14:07:41 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0080620.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Aug 06 13:04:06 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

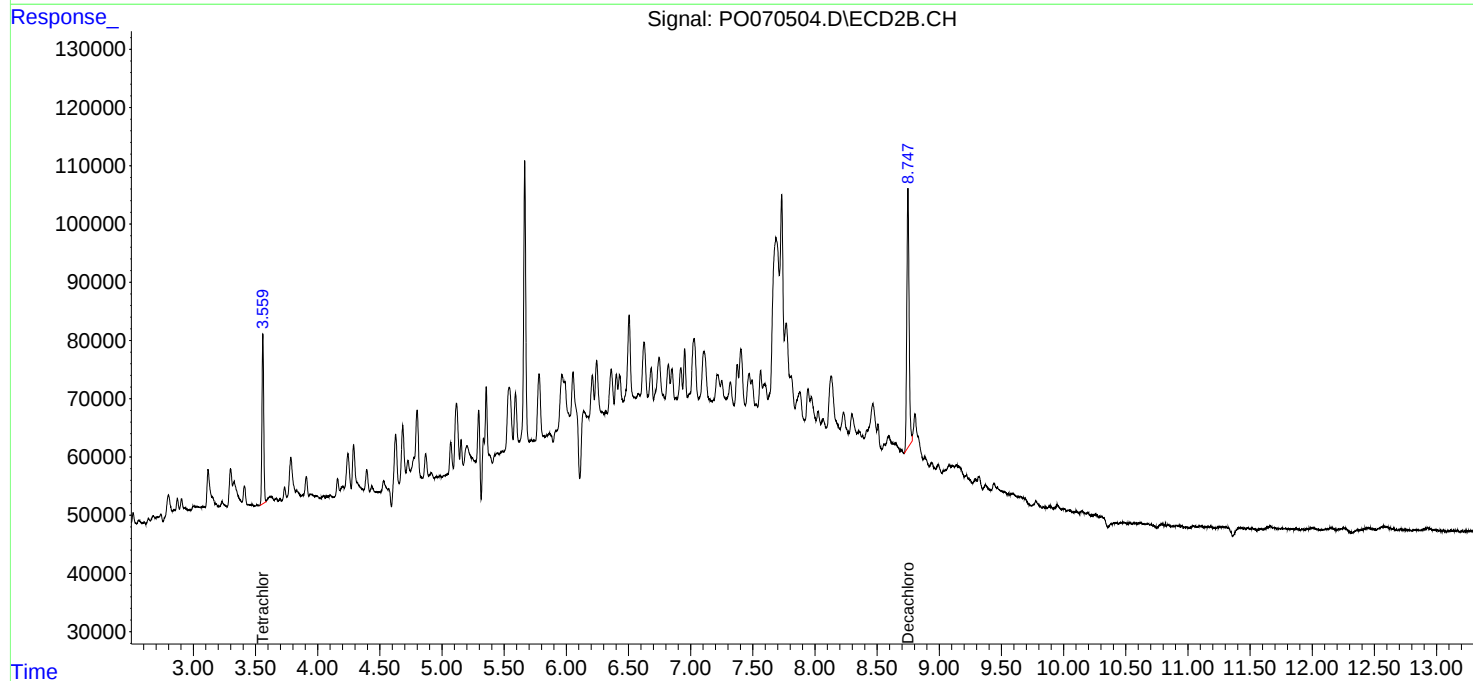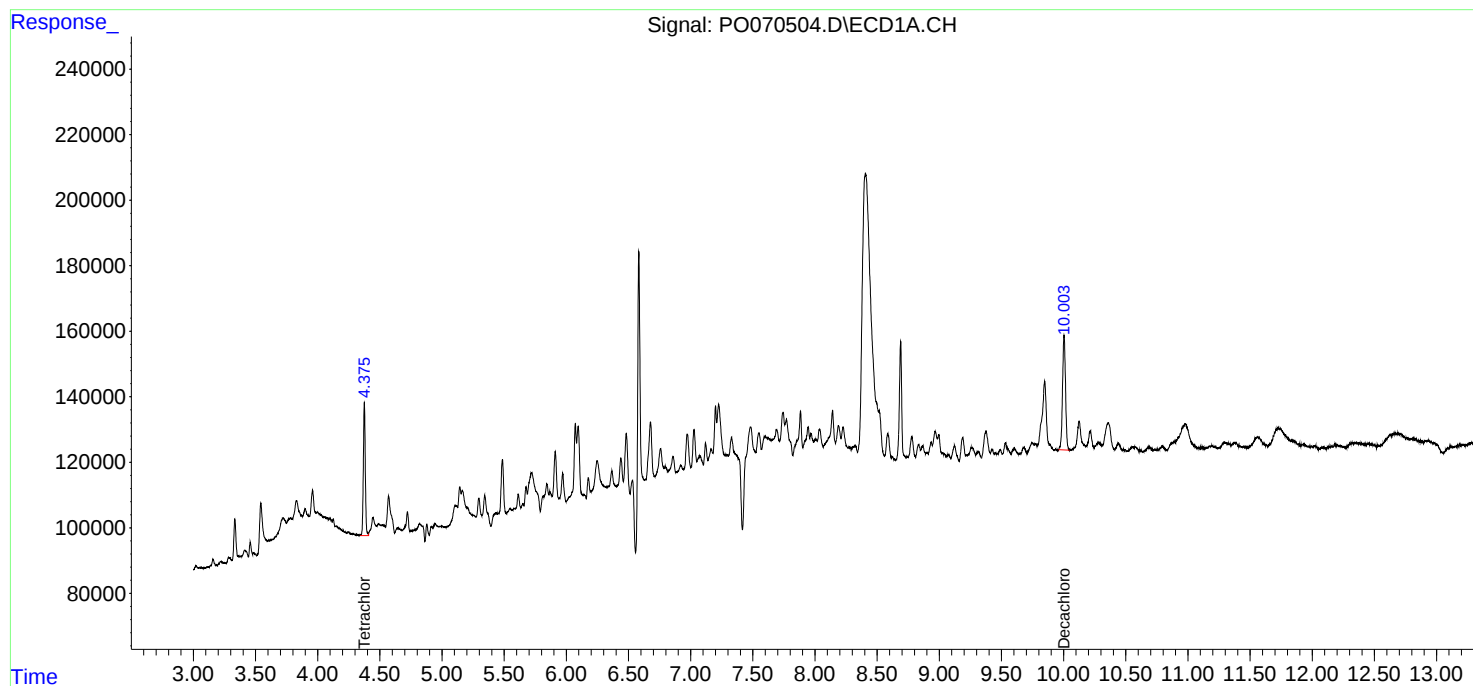

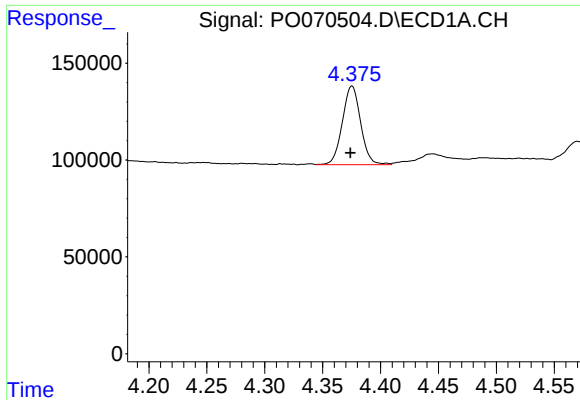


#1 Tetrachloro-m-xylene

R.T.: 4.375 min
Delta R.T.: 0.001 min
Response: 445000
Conc: 6.73 ng/ml m

Instrument :
ECD_O
ClientSampleId :
PCB-080620-SR-17RE


Manual Integrations
APPROVED

Ankita
8/14/2020 8:32:37 AM

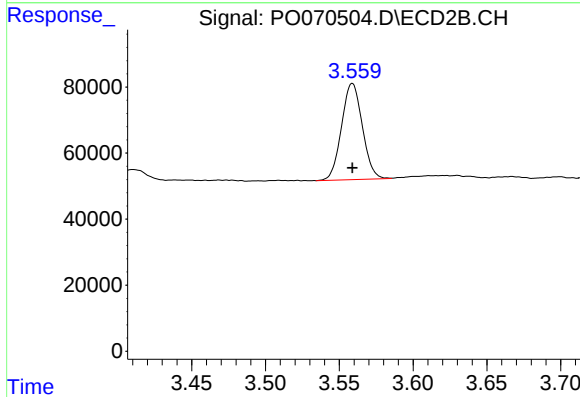


#1 Tetrachloro-m-xylene

R.T.: 3.559 min
Delta R.T.: 0.000 min
Response: 286154
Conc: 6.49 ng/ml m

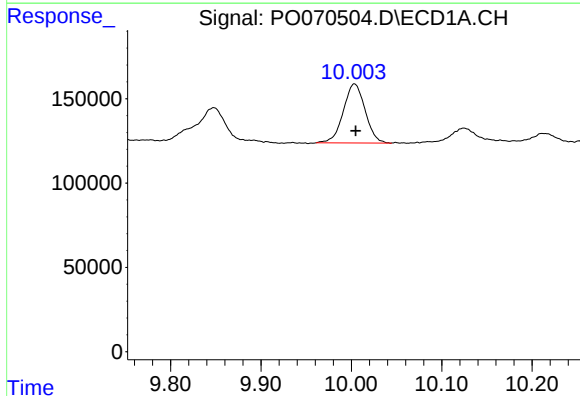

#2 Decachlorobiphenyl

R.T.: 10.004 min
Delta R.T.: -0.001 min
Response: 587949
Conc: 6.87 ng/ml

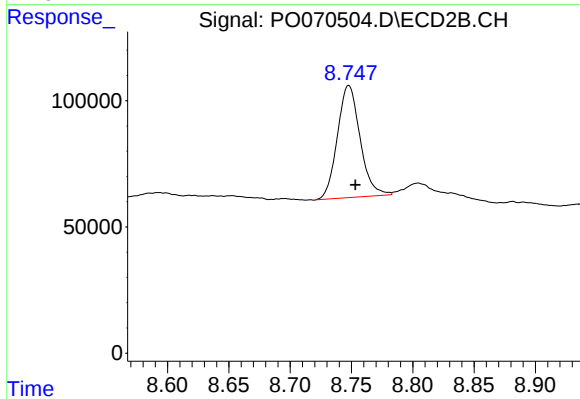

#2 Decachlorobiphenyl

R.T.: 8.748 min
Delta R.T.: -0.005 min
Response: 572307
Conc: 10.31 ng/ml