

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081220\
 Data File : P0070513.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Aug 2020 14:12
 Operator : DD\AJ
 Sample : L3650-07RE 10X
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PCB-080620-SR-07RE

Manual Integrations
 APPROVED

Ankita
 8/14/2020 8:32:57 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 12 15:11:24 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0080620.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Aug 06 13:04:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.374	3.563	171946	290207	2.600m	6.587m#
2) SA Decachlor...	10.005	8.752	291830	131456	3.408	2.368 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081220\
Data File : P0070513.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Aug 2020 14:12
Operator : DD\AJ
Sample : L3650-07RE 10X
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PCB-080620-SR-07RE


Manual Integrations
APPROVED

Ankita
8/14/2020 8:32:57 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 12 15:11:24 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0080620.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Aug 06 13:04:06 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

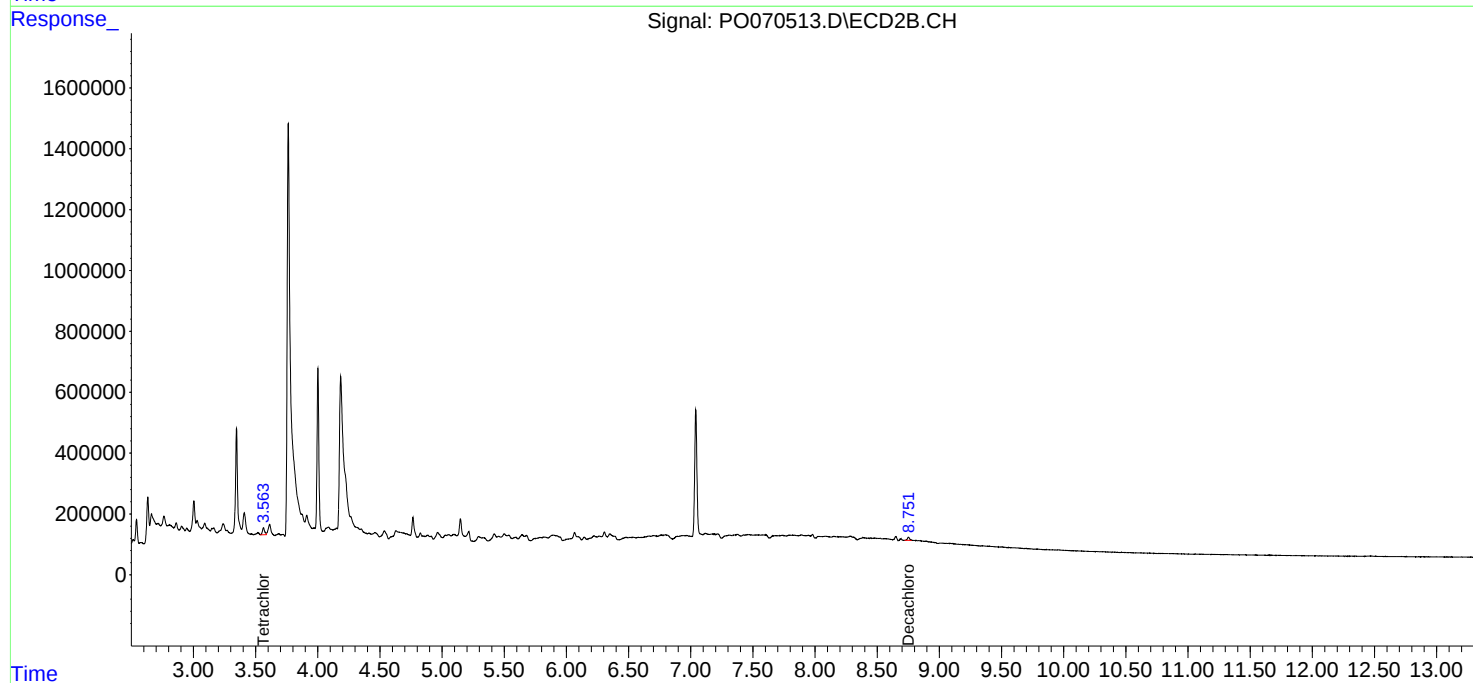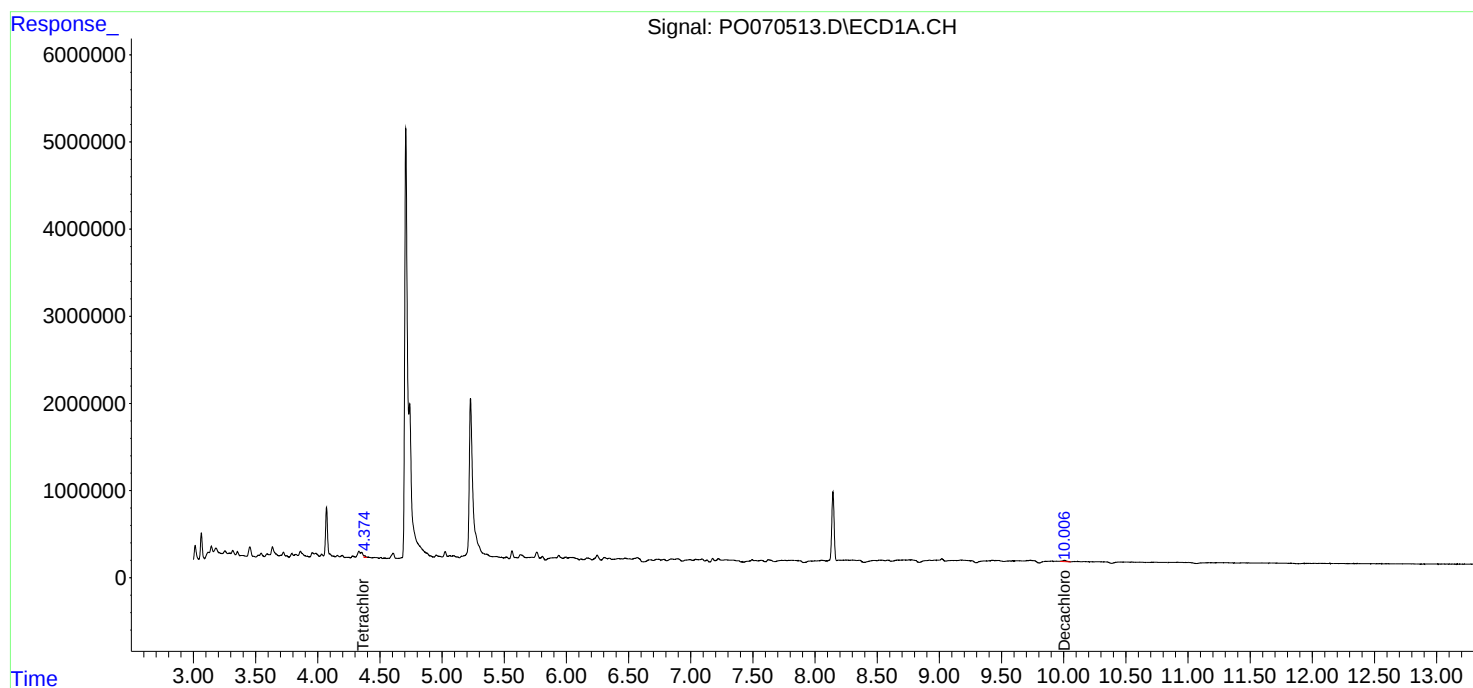

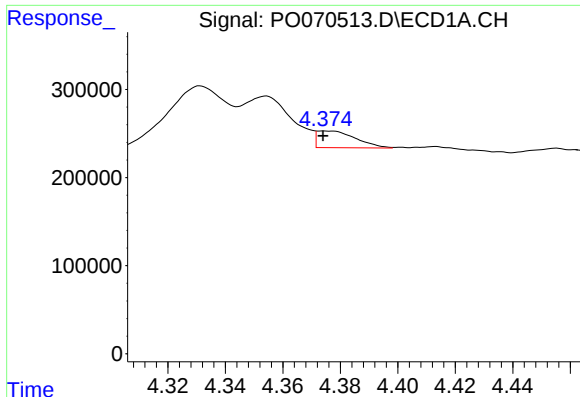


#1 Tetrachloro-m-xylene

R.T.: 4.374 min
Delta R.T.: 0.000 min
Response: 171946
Conc: 2.60 ng/ml m

Instrument :
ECD_O
ClientSampleId :
PCB-080620-SR-07RE


Manual Integrations
APPROVED

Ankita
8/14/2020 8:32:57 AM

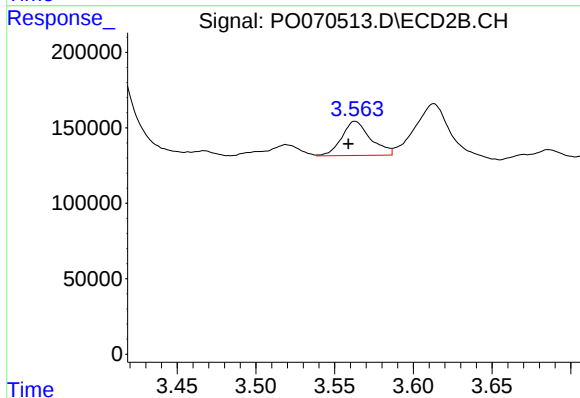


#1 Tetrachloro-m-xylene

R.T.: 3.563 min
Delta R.T.: 0.004 min
Response: 290207
Conc: 6.59 ng/ml m

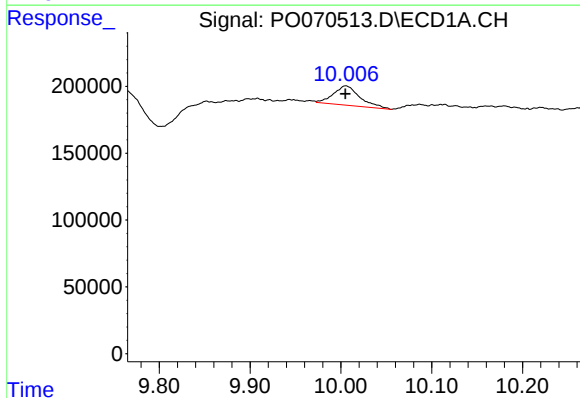

#2 Decachlorobiphenyl

R.T.: 10.005 min
Delta R.T.: 0.000 min
Response: 291830
Conc: 3.41 ng/ml

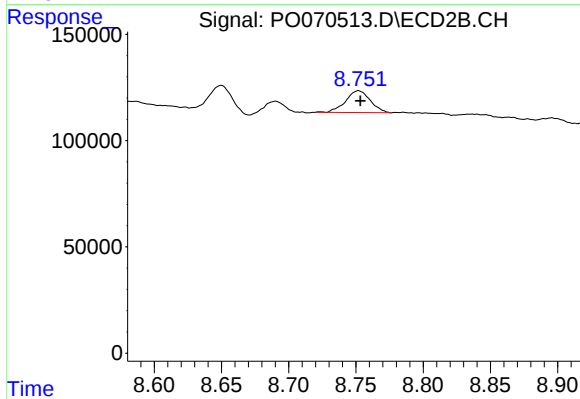

#2 Decachlorobiphenyl

R.T.: 8.752 min
Delta R.T.: -0.001 min
Response: 131456
Conc: 2.37 ng/ml