

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081221\
 Data File : P0080373.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Aug 2021 12:54
 Operator : DD\AJ
 Sample : PB138343BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB138343BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 01:30:47 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 11 05:48:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.992	4.106	1483034	519184	21.417	20.831
2) SA Decachlor...	11.096	9.508	1181000	508341	22.816	22.412
Target Compounds						
8) L2 AR-1221-1	5.246	0.000	230089	0	289.303	N.D. #
9) L2 AR-1221-2	5.346	4.443f	17480	59259	31.933	254.742 #
28) L6 AR-1254-3	7.870f	0.000	40119	0	9.829	N.D. #
32) L7 AR-1260-2	0.000	7.171f	0	14320	N.D.	8.616 #
38) L8 AR-1262-3	9.532	0.000	4658	0	1.556	N.D. #
41) L9 AR-1268-1	9.532	0.000	4658	0	0.583	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081221\
Data File : PO080373.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Aug 2021 12:54
Operator : DD\AJ
Sample : PB138343BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampled :
PB138343BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 13 01:30:47 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081021.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 11 05:48:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

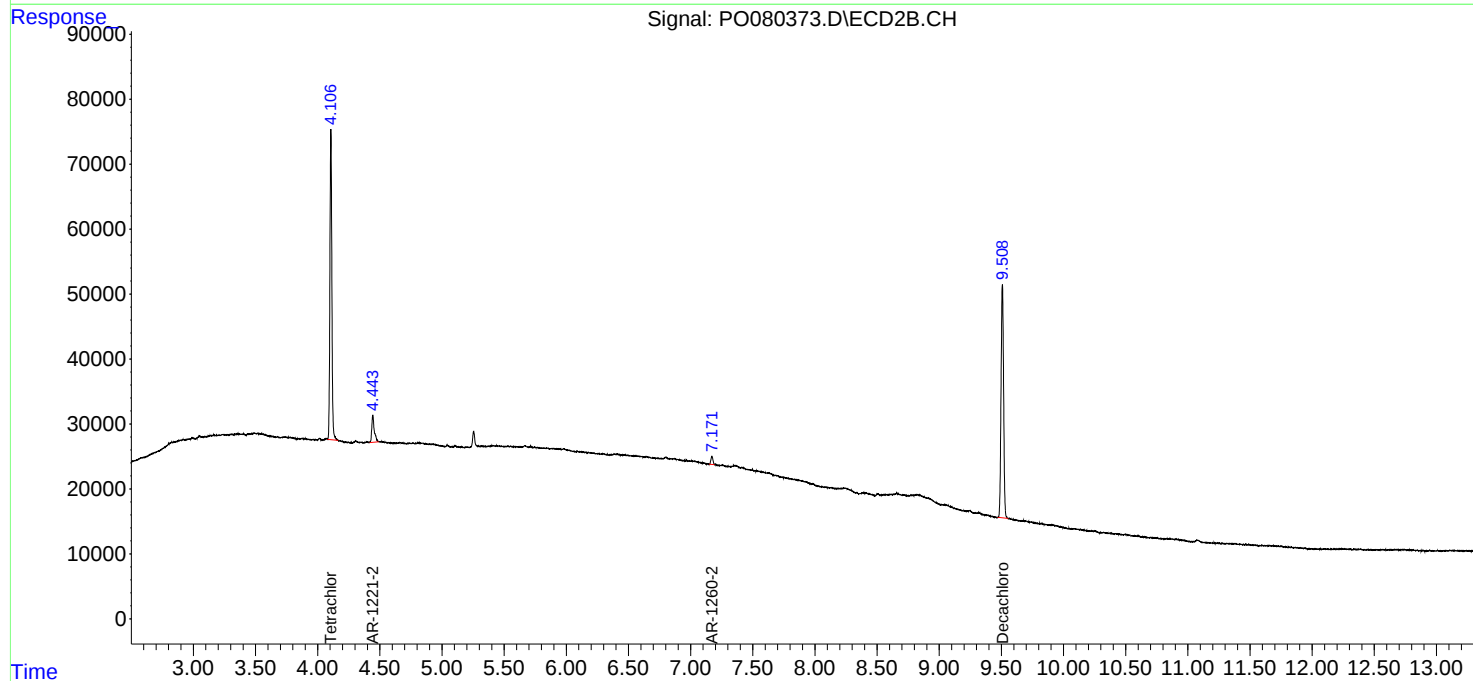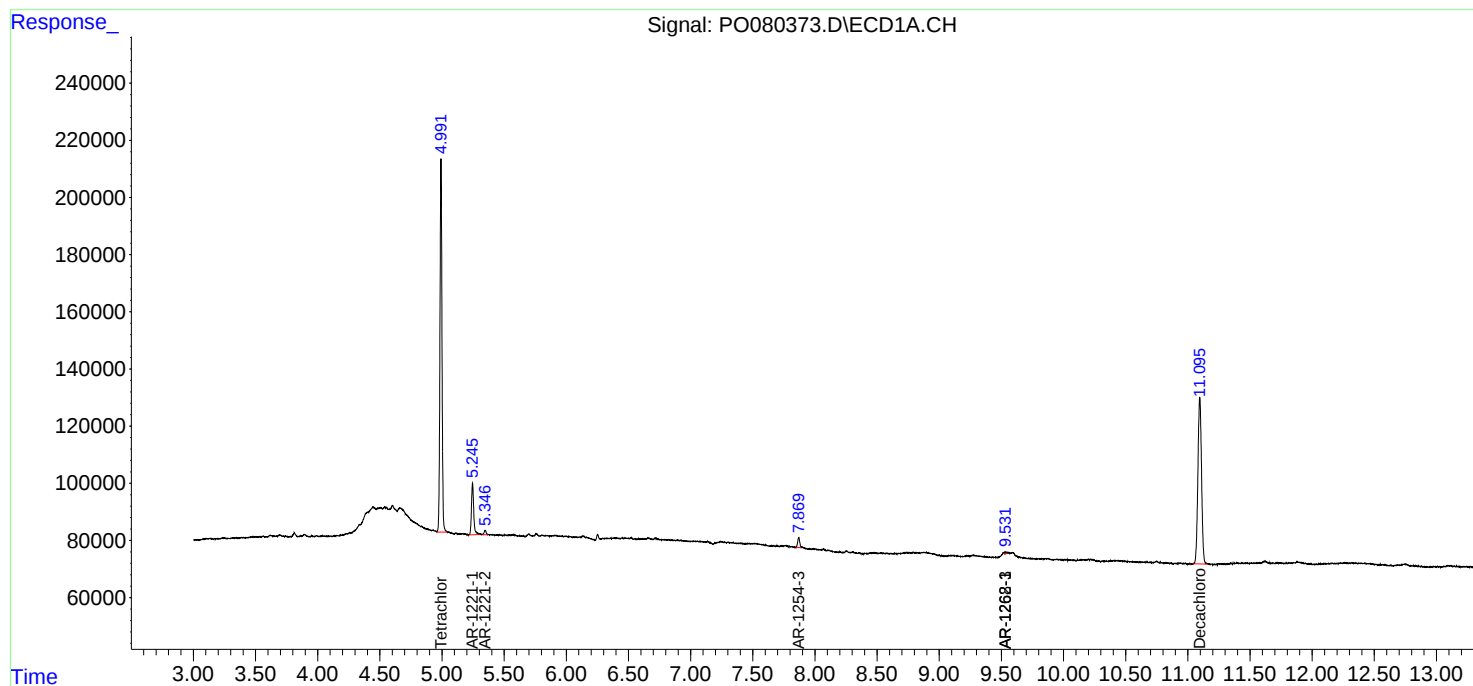


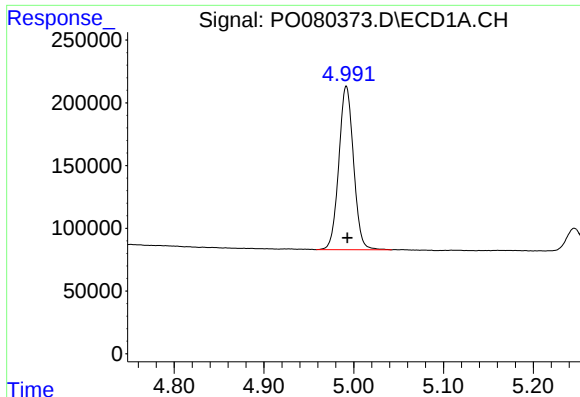

#1 Tetrachloro-m-xylene


R.T.: 4.992 min
Delta R.T.: -0.001 min
Response: 1483034
Conc: 21.42 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB138343BL

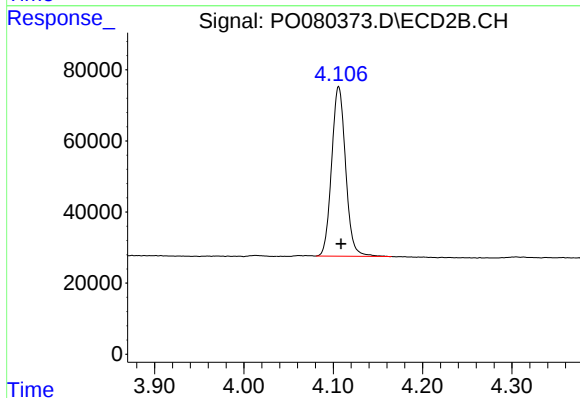


#1 Tetrachloro-m-xylene

R.T.: 4.106 min
Delta R.T.: -0.003 min
Response: 519184
Conc: 20.83 ng/ml

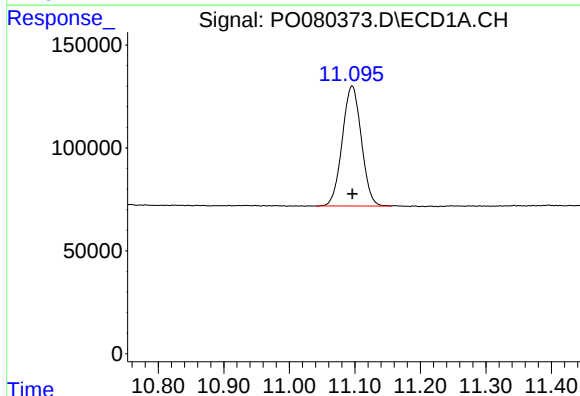


#2 Decachlorobiphenyl

R.T.: 11.096 min
Delta R.T.: 0.000 min
Response: 1181000
Conc: 22.82 ng/ml

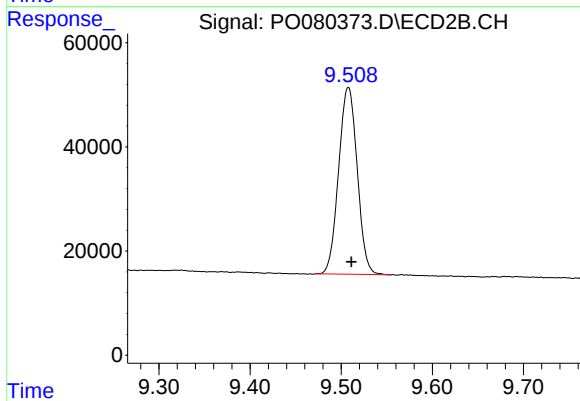

#2 Decachlorobiphenyl


R.T.: 9.508 min
Delta R.T.: -0.003 min
Response: 508341
Conc: 22.41 ng/ml

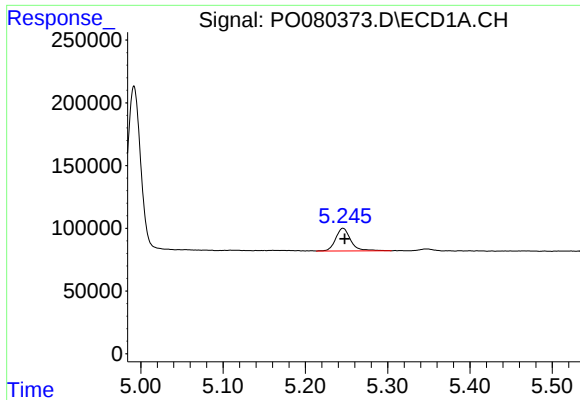

#8 AR-1221-1


R.T.: 5.246 min
Delta R.T.: -0.002 min
Response: 230089
Conc: 289.30 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB138343BL

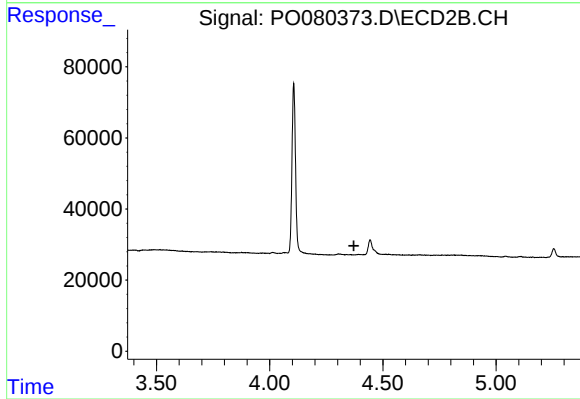


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.372 min
Response: 0
Conc: N.D.

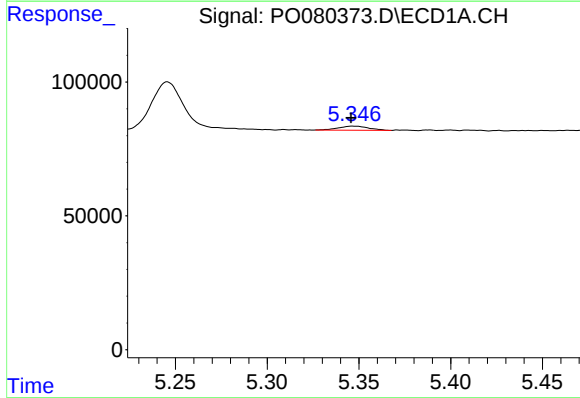


#9 AR-1221-2

R.T.: 5.346 min
Delta R.T.: 0.000 min
Response: 17480
Conc: 31.93 ng/ml

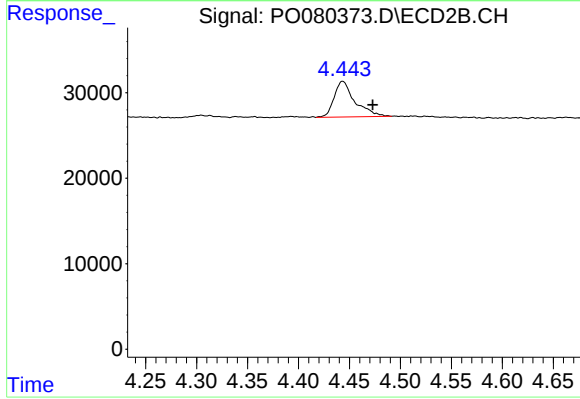

#9 AR-1221-2


R.T.: 4.443 min
Delta R.T.: -0.029 min
Response: 59259
Conc: 254.74 ng/ml

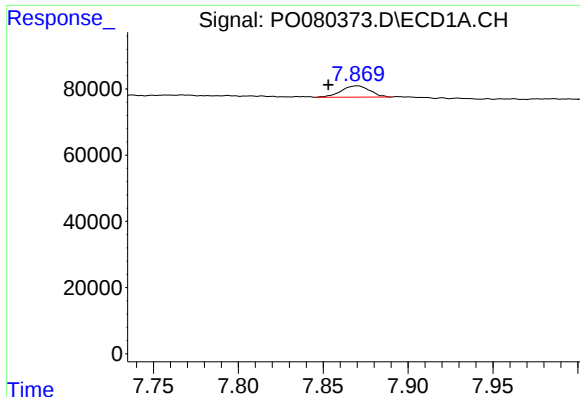

#28 AR-1254-3


R.T.: 7.870 min
Delta R.T.: 0.017 min
Response: 40119
Conc: 9.83 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB138343BL

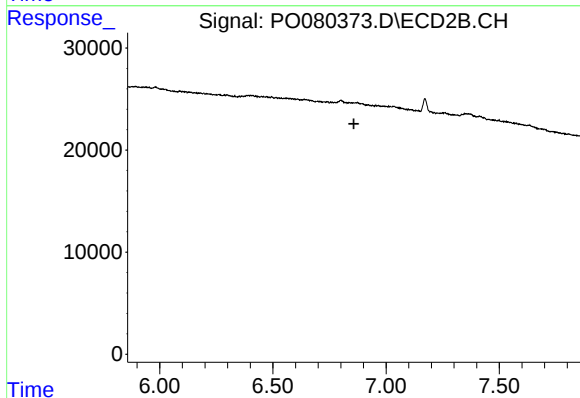


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.858 min
Response: 0
Conc: N.D.

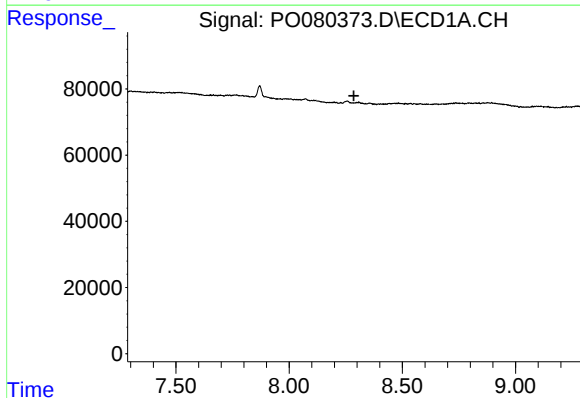


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 8.286 min
Response: 0
Conc: N.D.

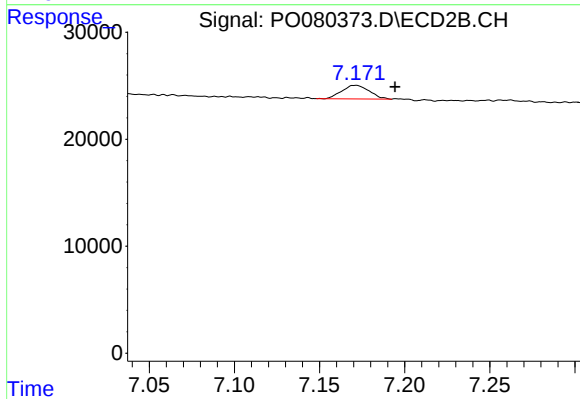

#32 AR-1260-2


R.T.: 7.171 min
Delta R.T.: -0.023 min
Response: 14320
Conc: 8.62 ng/ml

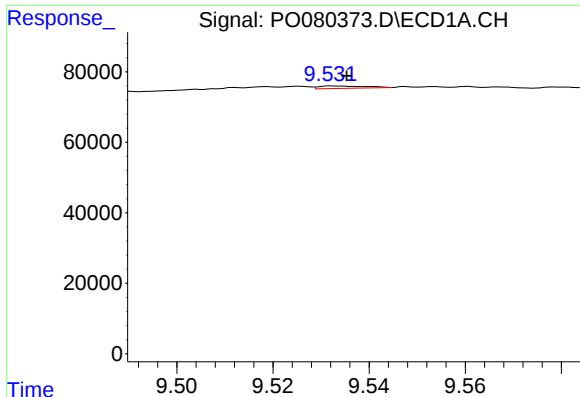

#38 AR-1262-3


R.T.: 9.532 min
Delta R.T.: -0.003 min
Response: 4658
Conc: 1.56 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB138343BL

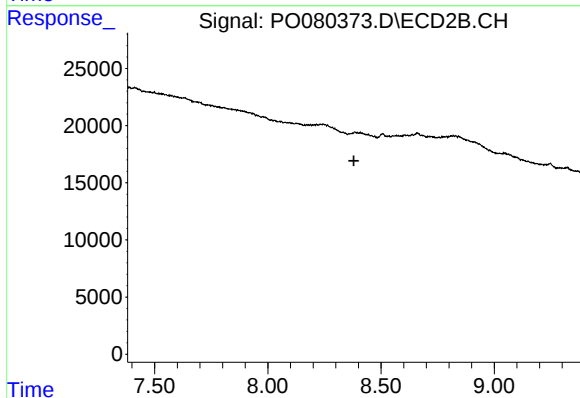


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T. : 8.380 min
Response: 0
Conc: N.D.

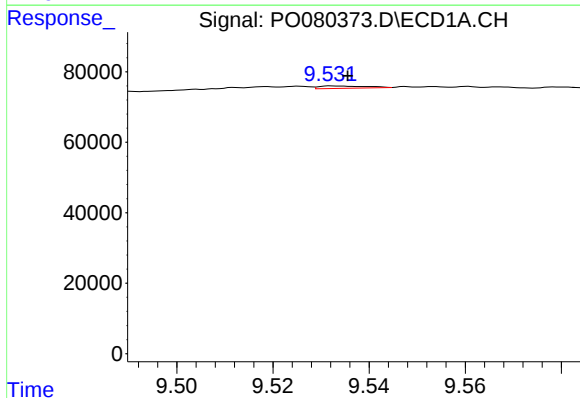

#41 AR-1268-1

R.T.: 9.532 min
Delta R.T.: -0.003 min
Response: 4658
Conc: 0.58 ng/ml

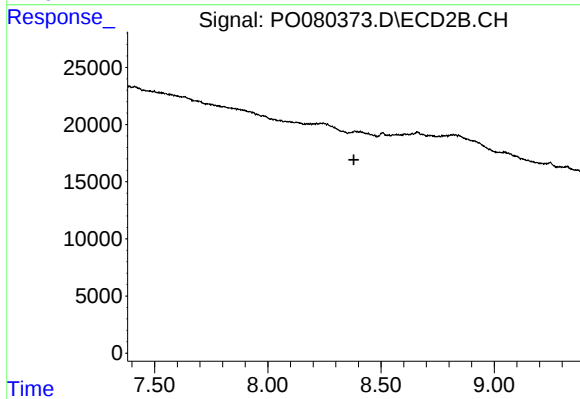

#41 AR-1268-1

R.T.: 0.000 min
Exp R.T. : 8.380 min
Response: 0
Conc: N.D.