

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081221\
 Data File : P0080388.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Aug 2021 18:07
 Operator : DD\AJ
 Sample : M3359-04 10X
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 NO-NUMBER-END-1-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 01:36:36 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 11 05:48:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.994	4.109	112084	42337	1.619	1.699
2) SA Decachlor...	11.098	9.510	105901	46518	2.046	2.051

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081221\
Data File : P0080388.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Aug 2021 18:07
Operator : DD\AJ
Sample : M3359-04 10X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
NO-NUMBER-END-1-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 13 01:36:36 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081021.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 11 05:48:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

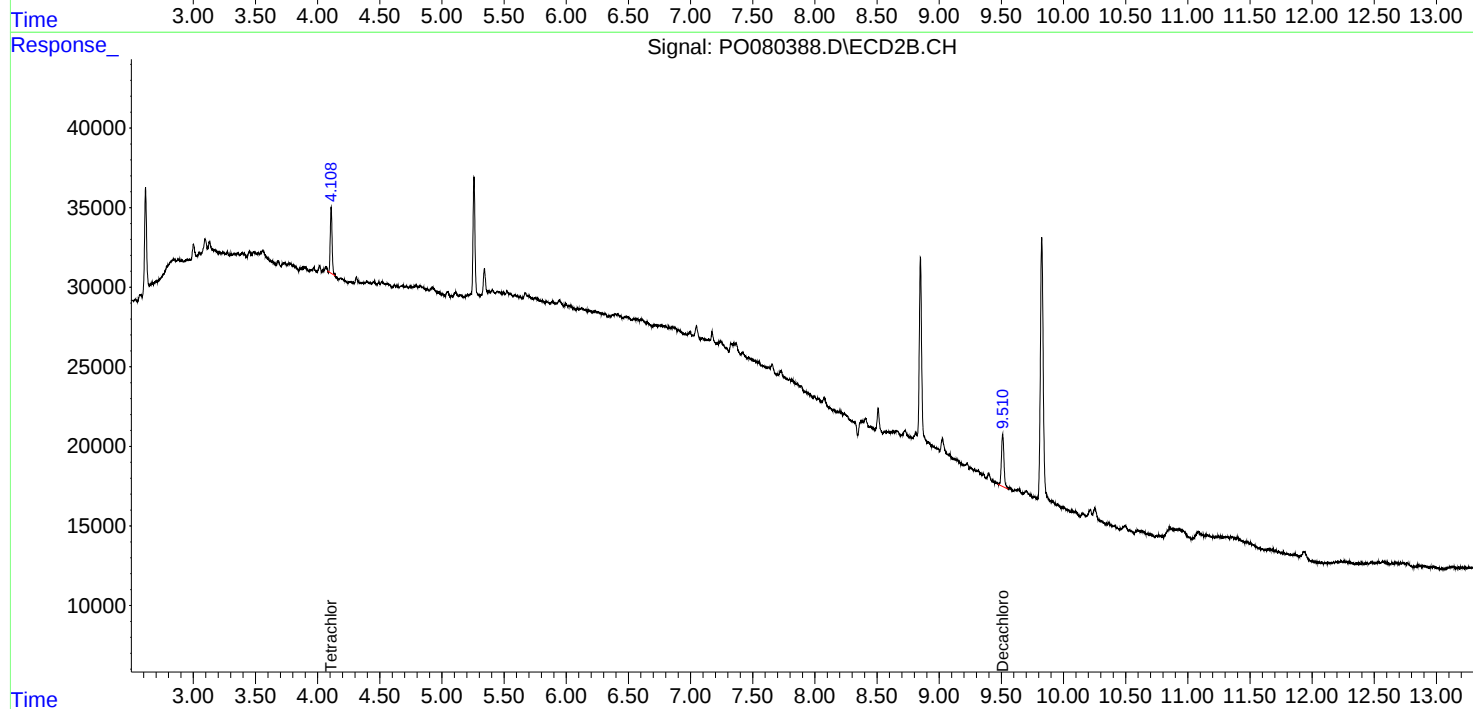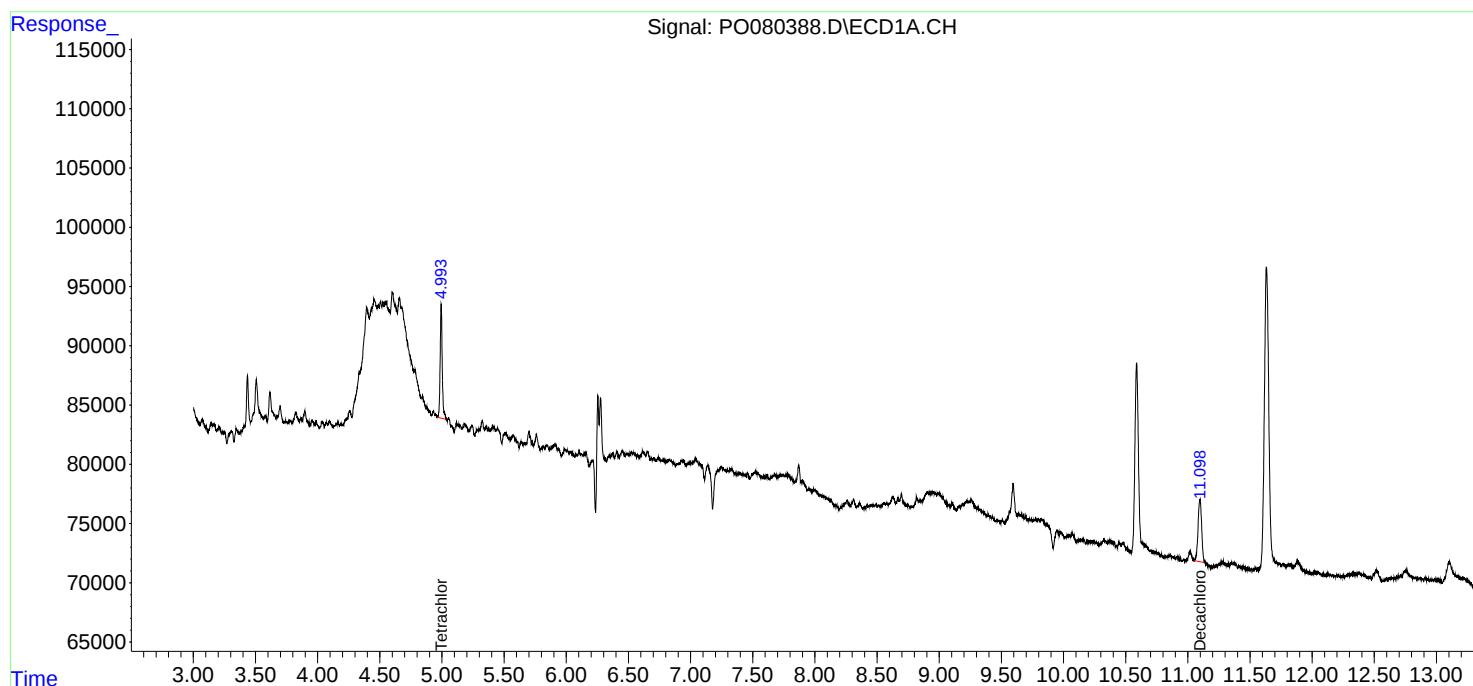


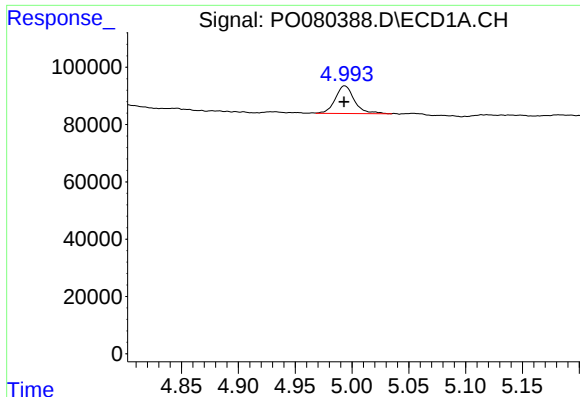

#1 Tetrachloro-m-xylene


R.T.: 4.994 min
Delta R.T.: 0.000 min
Response: 112084
Conc: 1.62 ng/ml

Instrument :
ECD_O
ClientSampleId :
NO-NUMBER-END-1-2

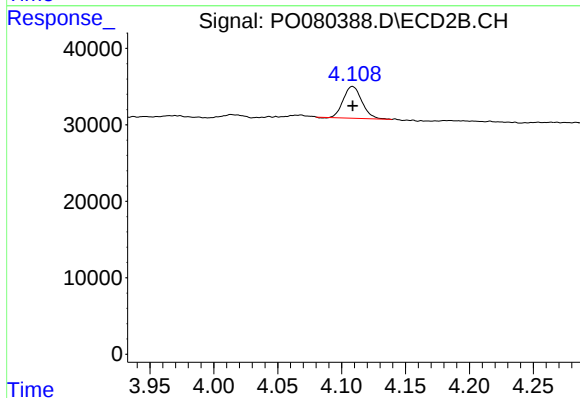


#1 Tetrachloro-m-xylene

R.T.: 4.109 min
Delta R.T.: 0.000 min
Response: 42337
Conc: 1.70 ng/ml

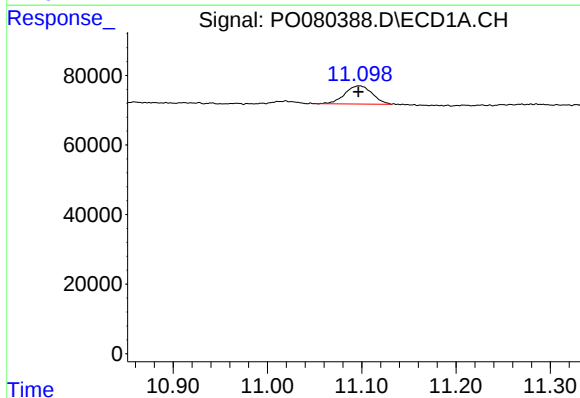

#2 Decachlorobiphenyl

R.T.: 11.098 min
Delta R.T.: 0.002 min
Response: 105901
Conc: 2.05 ng/ml

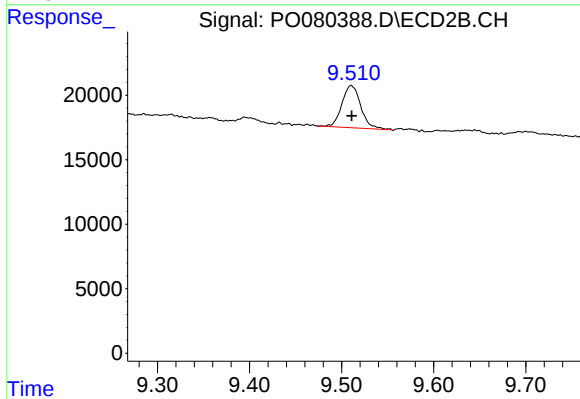

#2 Decachlorobiphenyl

R.T.: 9.510 min
Delta R.T.: 0.000 min
Response: 46518
Conc: 2.05 ng/ml