

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081221\
 Data File : P0080389.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Aug 2021 18:25
 Operator : DD\AJ
 Sample : M3359-01 10X
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 JEH585T-END-1-1

Manual Integrations
 APPROVED

mohammad
 8/13/2021 10:07:49 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 01:36:52 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 11 05:48:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.992	4.108	37274	32343	0.538m	1.298 #
2) SA Decachlor...	11.096	9.510	84534	39296	1.633m	1.733

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081221\
Data File : P0080389.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Aug 2021 18:25
Operator : DD\AJ
Sample : M3359-01 10X
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
JEH585T-END-1-1


Manual Integrations
APPROVED

mohammad
8/13/2021 10:07:49 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 13 01:36:52 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081021.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 11 05:48:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

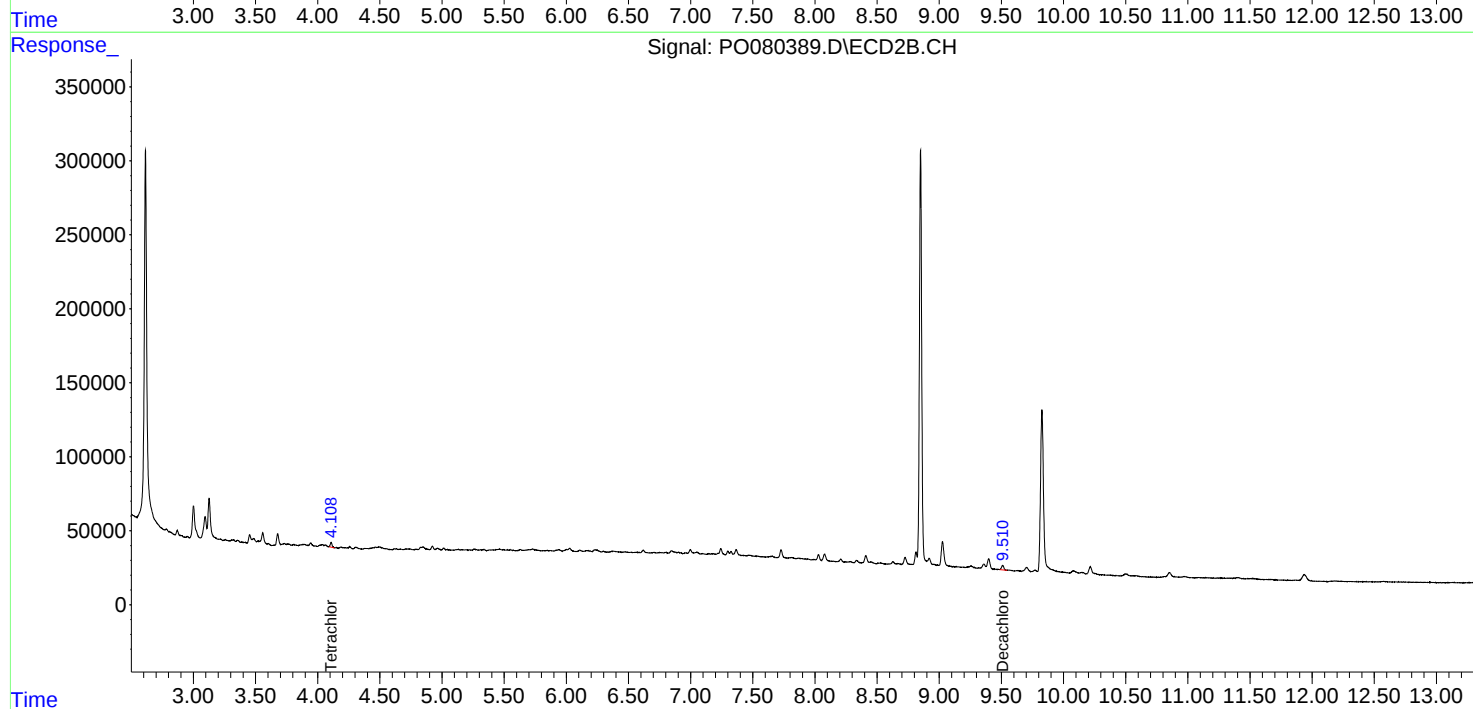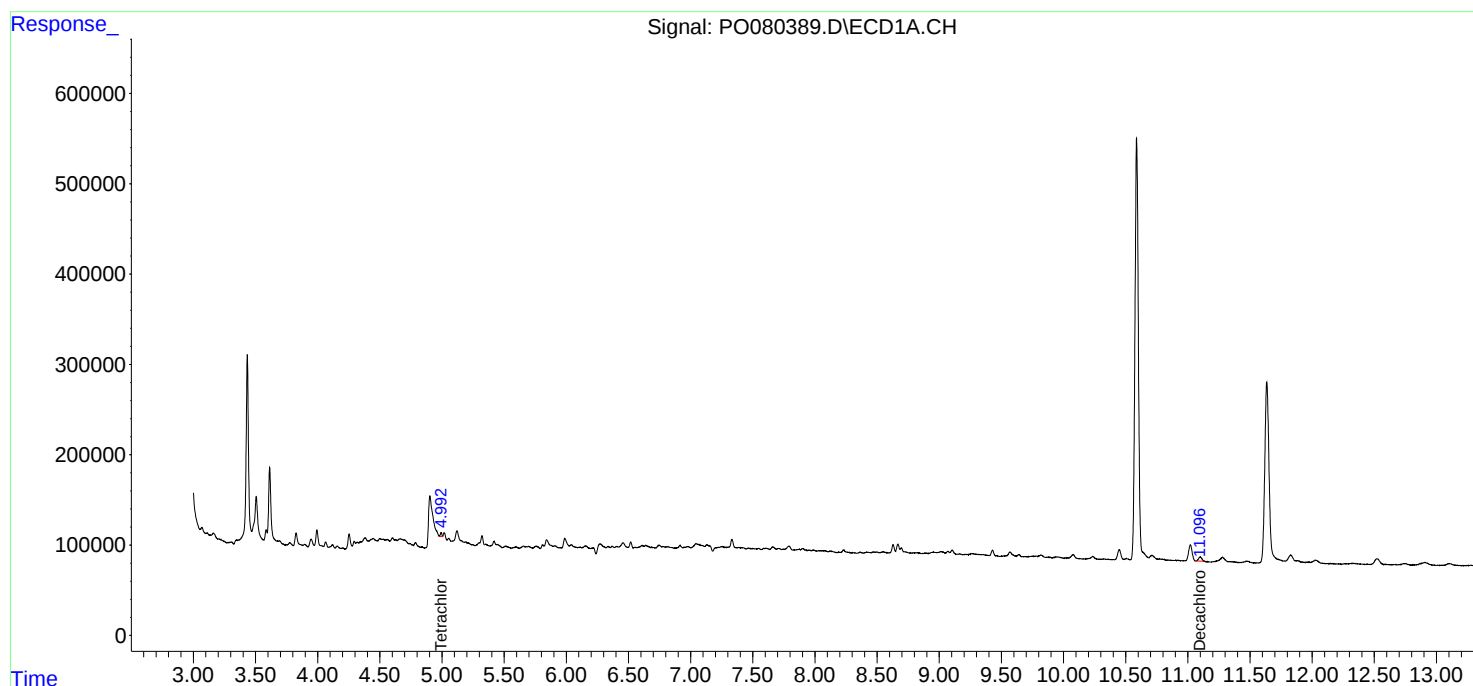

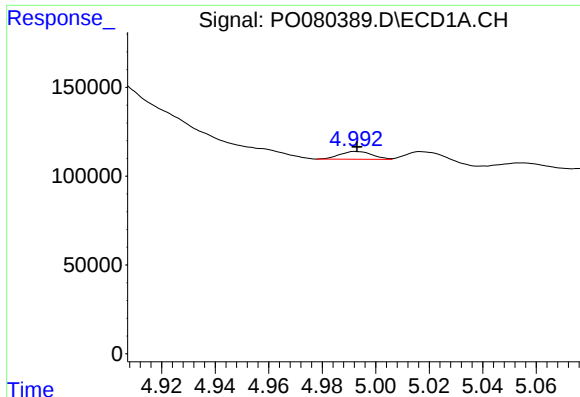


#1 Tetrachloro-m-xylene

R.T.: 4.992 min
Delta R.T.: -0.001 min
Response: 37274
Conc: 0.54 ng/ml m

Instrument :
ECD_O
ClientSampleId :
JEH585T-END-1-1


Manual Integrations
APPROVED

mohammad
8/13/2021 10:07:49 AM

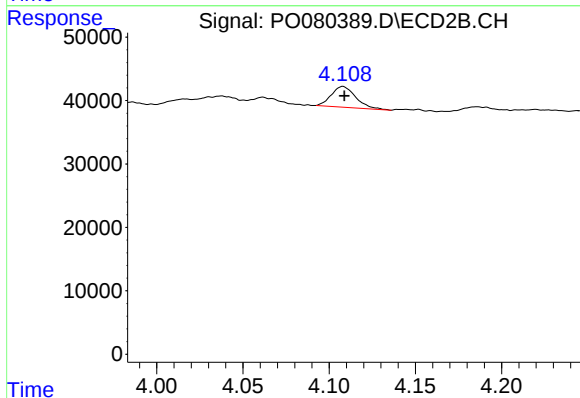


#1 Tetrachloro-m-xylene

R.T.: 4.108 min
Delta R.T.: 0.000 min
Response: 32343
Conc: 1.30 ng/ml

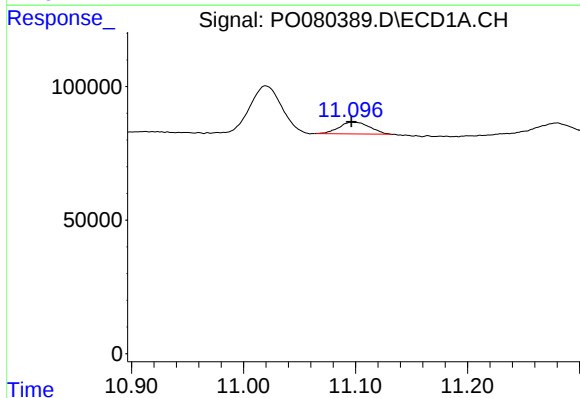

#2 Decachlorobiphenyl

R.T.: 11.096 min
Delta R.T.: 0.000 min
Response: 84534
Conc: 1.63 ng/ml m

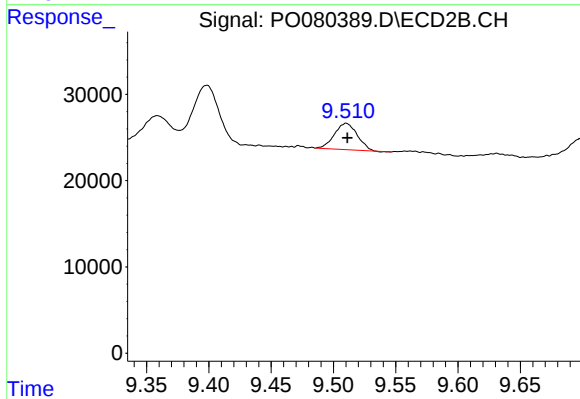

#2 Decachlorobiphenyl

R.T.: 9.510 min
Delta R.T.: 0.000 min
Response: 39296
Conc: 1.73 ng/ml