

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081222\
 Data File : P0088944.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Aug 2022 04:30
 Operator : YP/AJ
 Sample : N4184-06 10X
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BC248150-1-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/15/2022
 Supervised By :Ankita Jodhani 08/15/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 06:09:44 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0080422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 05 23:24:09 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.431	3.589	3534022	1350460	1.310m	1.248m
2) SA Decachlor...	10.266	8.578	3318952	1823472	1.720	1.505

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081222\
Data File : PO088944.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Aug 2022 04:30
Operator : YP/AJ
Sample : N4184-06 10X
Misc :
ALS Vial : 34 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
BC248150-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/15/2022
Supervised By :Ankita Jodhani 08/15/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 13 06:09:44 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO080422.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 05 23:24:09 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

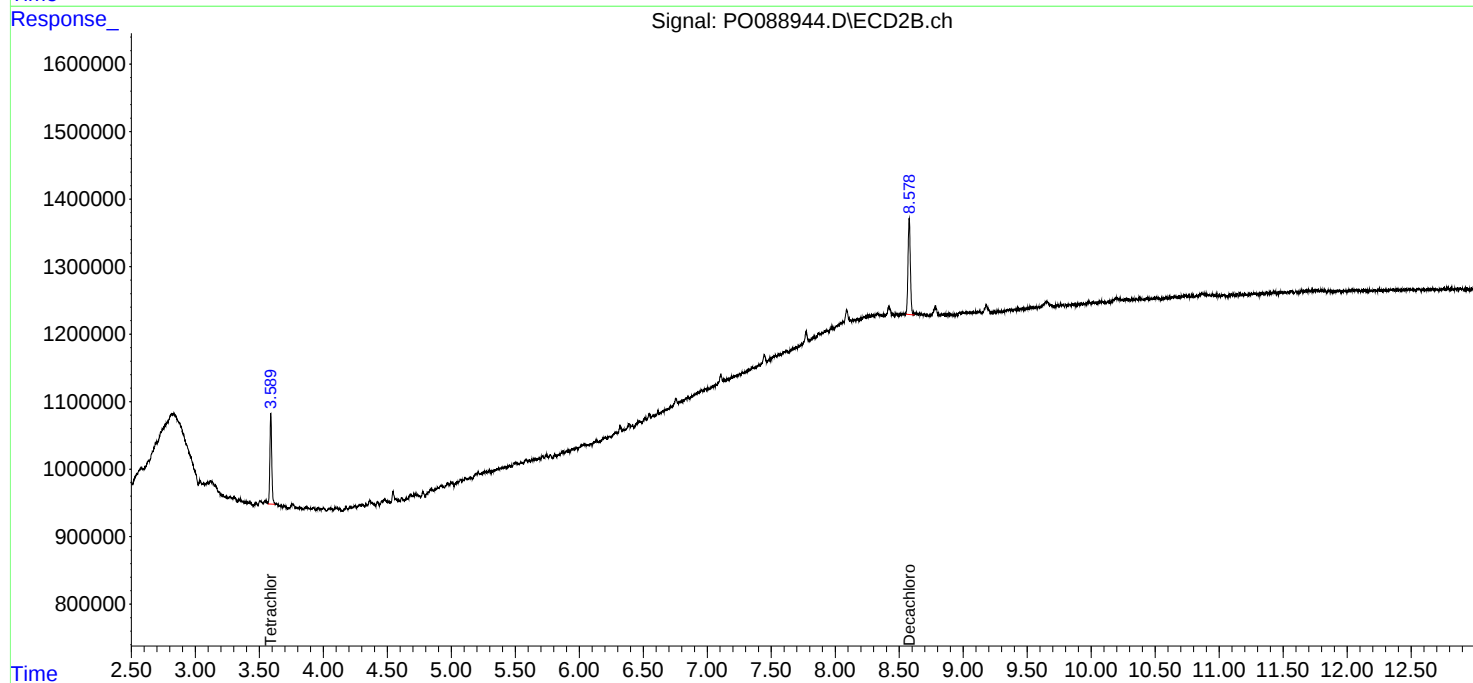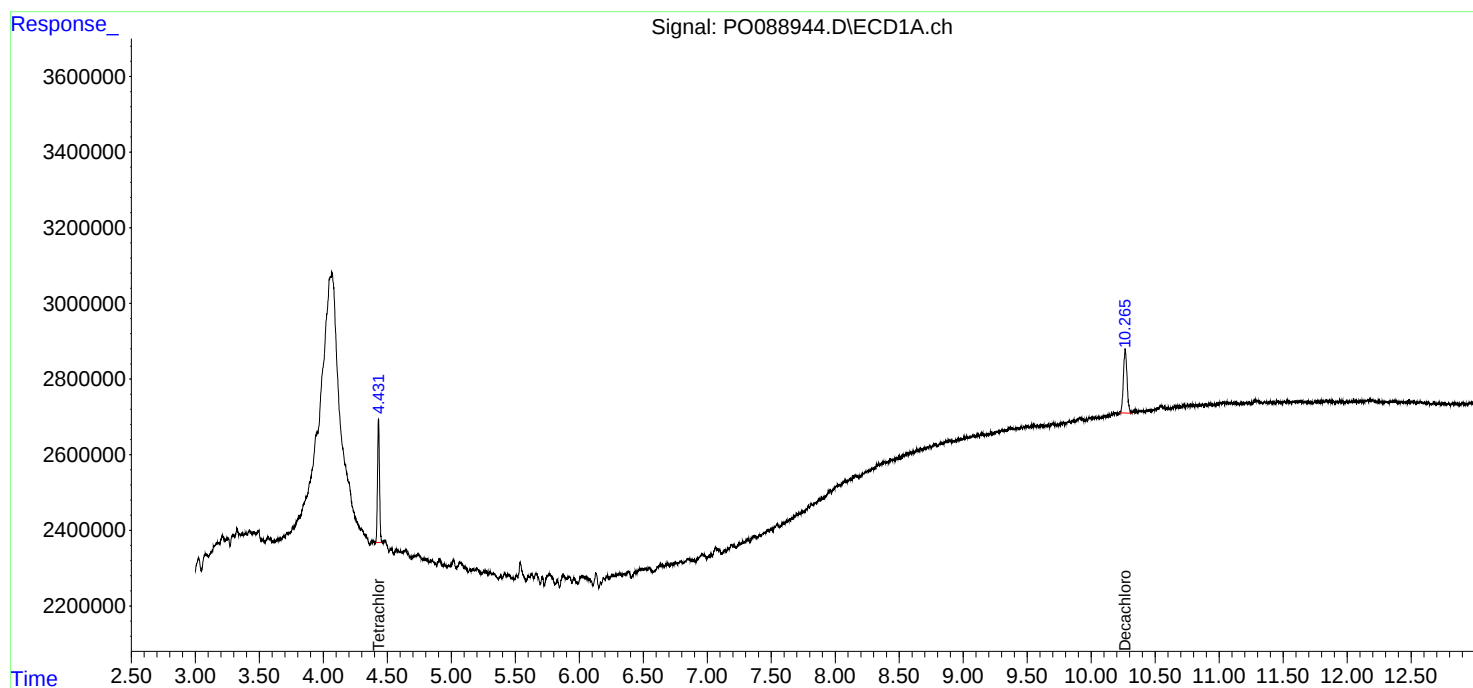

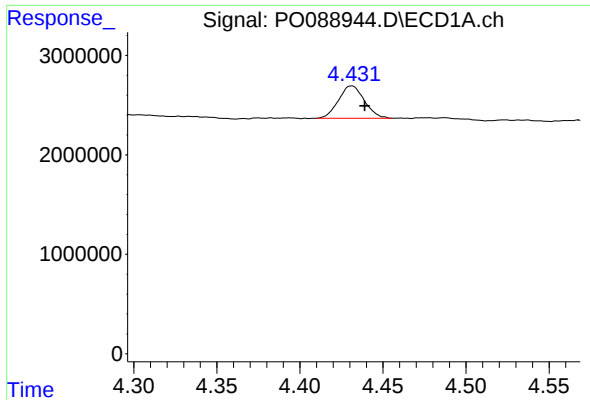


#1 Tetrachloro-m-xylene

R.T.: 4.431 min
Delta R.T.: -0.008 min
Response: 3534022
Conc: 1.31 ng/ml

Instrument :
ECD_O
ClientSampleId :
BC248150-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/15/2022
Supervised By :Ankita Jodhani 08/15/2022

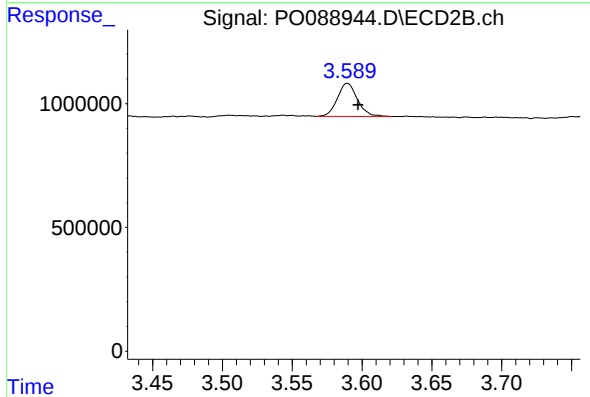


#1 Tetrachloro-m-xylene

R.T.: 3.589 min
Delta R.T.: -0.008 min
Response: 1350460
Conc: 1.25 ng/ml m

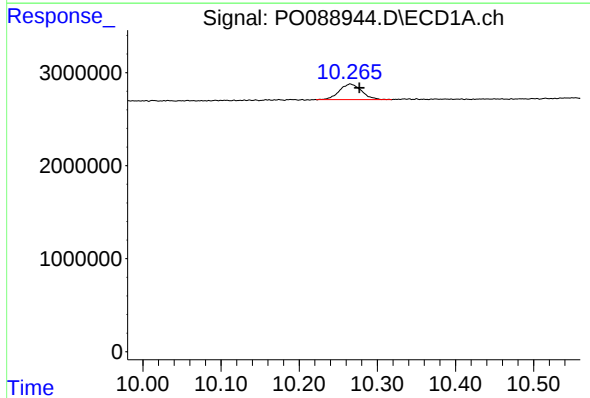

#2 Decachlorobiphenyl

R.T.: 10.266 min
Delta R.T.: -0.011 min
Response: 3318952
Conc: 1.72 ng/ml

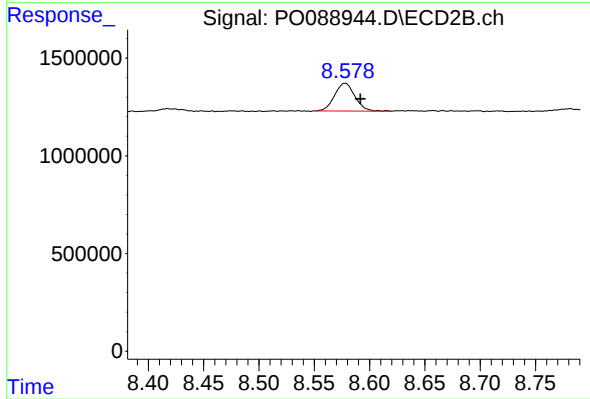

#2 Decachlorobiphenyl

R.T.: 8.578 min
Delta R.T.: -0.014 min
Response: 1823472
Conc: 1.50 ng/ml