

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081224\
 Data File : P0105425.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2024 17:16
 Operator : YP/AJ
 Sample : P3390-07
 Misc : AR1660 LOD 25 PPB
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 02:29:15 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081024.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 10 04:08:56 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.428	3.536	122.2E6	42788027	13.989	13.623
2)	SA Decachlor...	10.218	8.427	88874860	25750083	15.450	14.545
Target Compounds							
3)	L1 AR-1016-1	5.598	4.591	5643436	2232265	18.656	19.863
4)	L1 AR-1016-2	5.621	4.609	8265851	2891169	19.336	18.571
5)	L1 AR-1016-3	5.683	4.780	4756228	1526597	18.537	18.229
6)	L1 AR-1016-4	5.783	4.822	5623271	1231676	25.711	18.291 #
7)	L1 AR-1016-5	6.079	5.030	4963242	1899817	23.198	22.700
8)	L2 AR-1221-1	4.625	3.743	1367061	312221	12.190	7.910 #
9)	L2 AR-1221-2	4.732	3.827	3322987	1161928	39.204	37.820
10)	L2 AR-1221-3	4.797	3.900	3910154	1187895	16.072	13.275
11)	L3 AR-1232-1	4.797	3.900	3910154	1187895	19.557	16.266
12)	L3 AR-1232-2	5.329	4.609	4231410	2891169	39.975	41.176
13)	L3 AR-1232-3	5.621	4.780	8265851	1526597	43.184	39.945
14)	L3 AR-1232-4	5.783	4.862	5623271	1617515	57.655	46.494
15)	L3 AR-1232-5	5.873	5.030	4289166	1899817	59.520	53.821
16)	L4 AR-1242-1	5.598	4.591	5643436	2232265	24.283	25.309
17)	L4 AR-1242-2	5.621	4.609	8265851	2891169	25.363	24.350
18)	L4 AR-1242-3	5.683	4.780	4756228	1526597	24.110	23.509
19)	L4 AR-1242-4	5.783	4.862	5623271	1617515	32.958	24.389 #
20)	L4 AR-1242-5	6.527	5.376	2981005	1944853	17.057	23.668 #
21)	L5 AR-1248-1	5.598	4.591	5643436	2232265	30.906	31.962
22)	L5 AR-1248-2	5.873	4.822	4289166	1231676	17.029	12.979
23)	L5 AR-1248-3	6.079	4.862	4963242	1617515	17.558	16.204
24)	L5 AR-1248-4	6.485	5.030	2607897	1899817	8.156	16.832 #
25)	L5 AR-1248-5	6.527	5.415	2981005	812944	9.637	7.219 #
26)	L6 AR-1254-1	6.460	5.376	5528704	1944853	17.630	11.946 #
27)	L6 AR-1254-2	6.680	5.520	3141058	1792092	6.960	12.251 #
28)	L6 AR-1254-3	7.051	5.932	3651961	2584681	7.698	11.458 #
29)	L6 AR-1254-4	7.335	6.142	4089371	436391	11.416	3.093 #
30)	L6 AR-1254-5	7.757	6.553	19733644	3994298	49.711	19.937 #
31)	L7 AR-1260-1	7.215	6.045	8608603	4017603	23.488	25.738
32)	L7 AR-1260-2	7.473	6.231	11350861	4217480	27.262	22.315
33)	L7 AR-1260-3	7.836	6.382	11870945	6026666	45.866	32.623 #
34)	L7 AR-1260-4	8.063	6.847	20323530	2666103	61.600	21.812 #
35)	L7 AR-1260-5	8.387	7.086	19484748	6109428	32.755	21.951 #
36)	L8 AR-1262-1	7.757	6.553	19733644	3994298	62.127	37.540 #
37)	L8 AR-1262-2	8.387	6.847	19484748	2666103	25.904	15.690 #
38)	L8 AR-1262-3	8.715	7.367	9895029	1665982	20.108	13.196 #
39)	L8 AR-1262-4	8.795	7.429	1700459	4660129	4.631	20.131 #
40)	L8 AR-1262-5	9.457	7.919	2392957	1428706	8.935	14.216 #
41)	L9 AR-1268-1	8.715	7.367	9895029	1665982	12.166	4.772 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081224\
 Data File : P0105425.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2024 17:16
 Operator : YP/AJ
 Sample : P3390-07
 Misc : AR1660 LOD 25 PPB
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 02:29:15 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081024.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 10 04:08:56 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.795	7.429	1700459	4660129	2.339	14.937 #
43) L9	AR-1268-3	9.023	7.637	1019878	593021	1.580	2.346 #
44) L9	AR-1268-4	9.457	7.919	2392957	1428706	8.594	13.284 #
45) L9	AR-1268-5	9.881	8.192	2426581	501009	1.161	0.749 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081224\
Data File : PO105425.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Aug 2024 17:16
Operator : YP/AJ
Sample : P3390-07
Misc : AR1660 LOD 25 PPB
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 13 02:29:15 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081024.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Aug 10 04:08:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

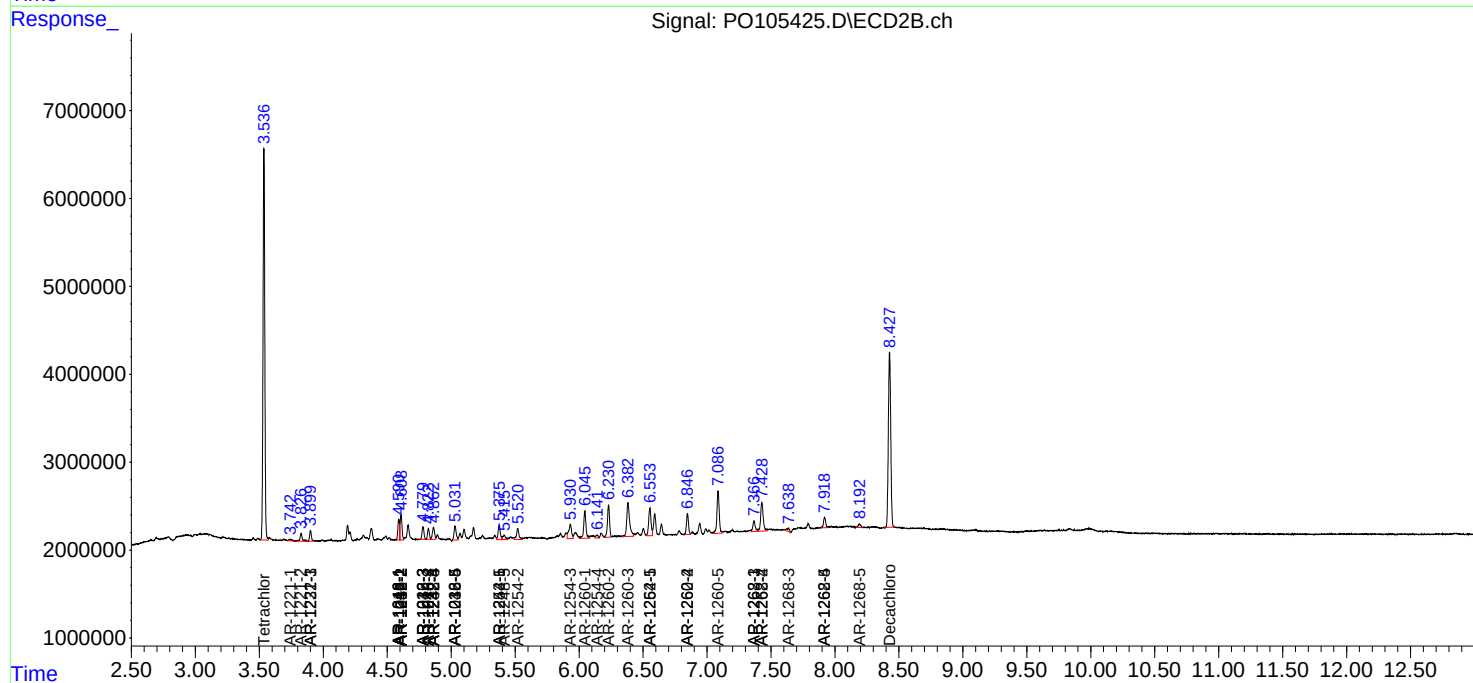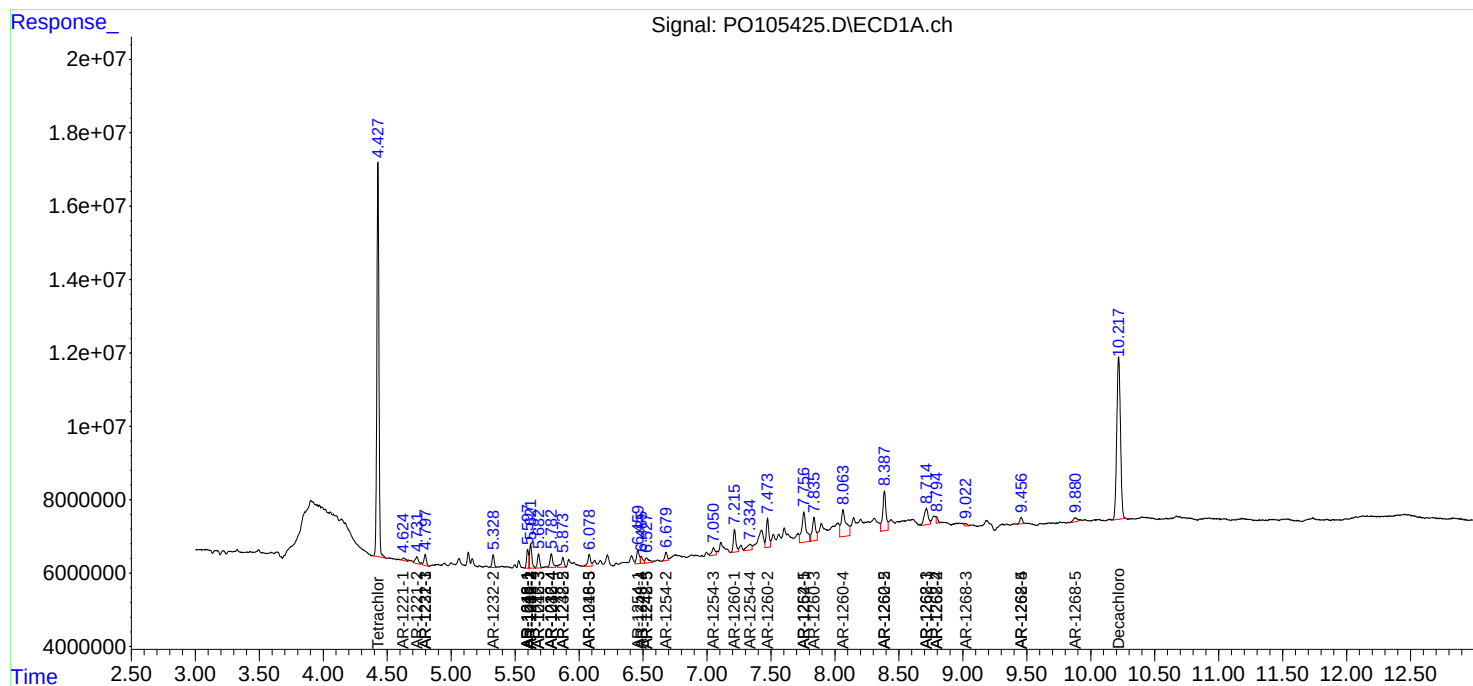


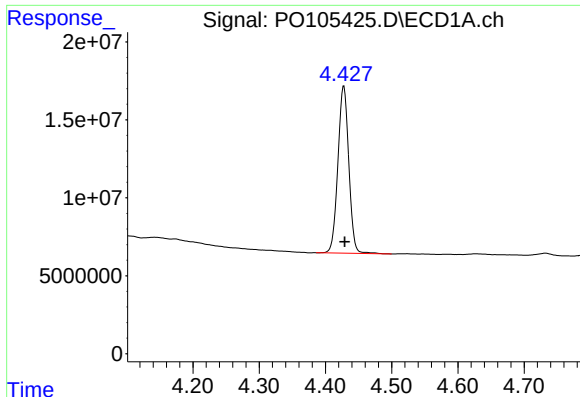

#1 Tetrachloro-m-xylene


R.T.: 4.428 min
Delta R.T.: -0.001 min
Response: 122183374
Conc: 13.99 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

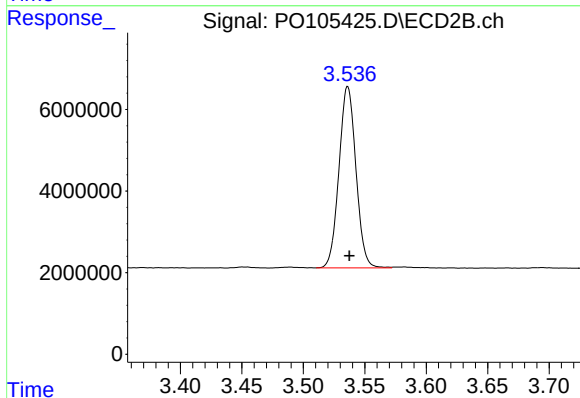


#1 Tetrachloro-m-xylene

R.T.: 3.536 min
Delta R.T.: -0.001 min
Response: 42788027
Conc: 13.62 ng/ml

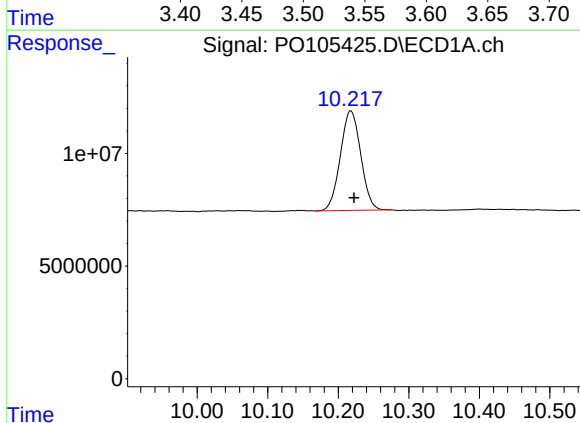


#2 Decachlorobiphenyl

R.T.: 10.218 min
Delta R.T.: -0.005 min
Response: 88874860
Conc: 15.45 ng/ml

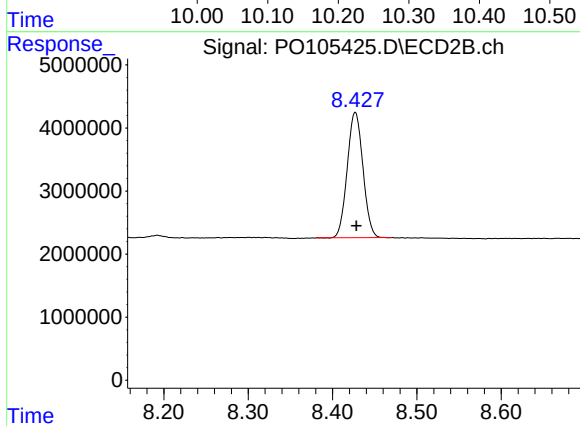

#2 Decachlorobiphenyl


R.T.: 8.427 min
Delta R.T.: -0.001 min
Response: 25750083
Conc: 14.55 ng/ml

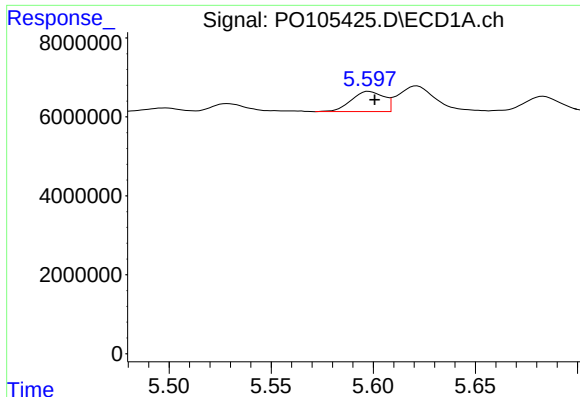

#3 AR-1016-1


R.T.: 5.598 min
Delta R.T.: -0.003 min
Response: 5643436
Conc: 18.66 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

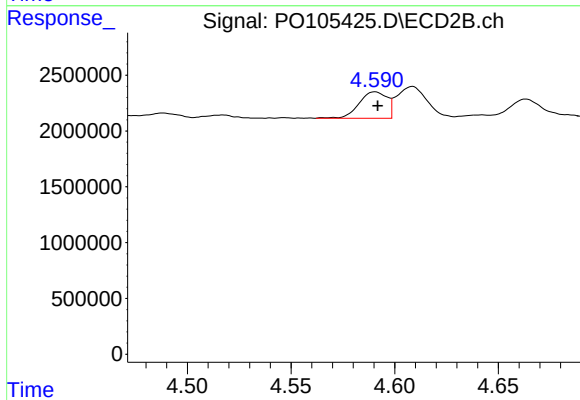


#3 AR-1016-1

R.T.: 4.591 min
Delta R.T.: -0.001 min
Response: 2232265
Conc: 19.86 ng/ml

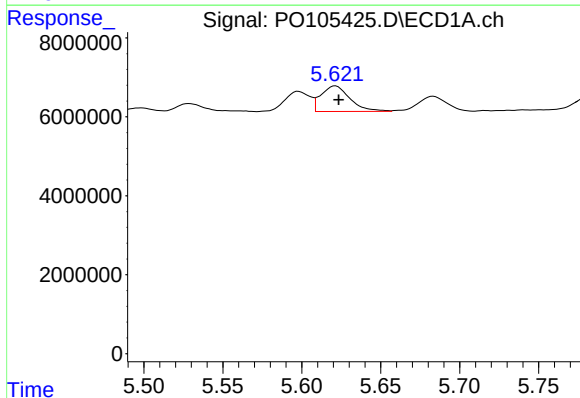


#4 AR-1016-2

R.T.: 5.621 min
Delta R.T.: -0.002 min
Response: 8265851
Conc: 19.34 ng/ml

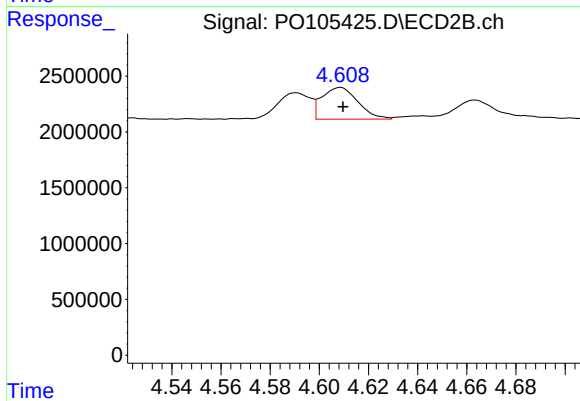

#4 AR-1016-2


R.T.: 4.609 min
Delta R.T.: -0.001 min
Response: 2891169
Conc: 18.57 ng/ml

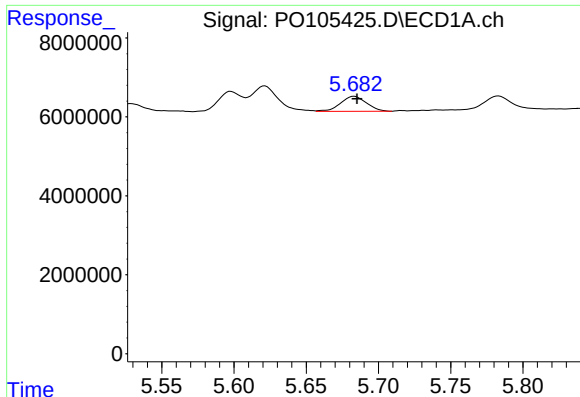

#5 AR-1016-3


R.T.: 5.683 min
Delta R.T.: -0.002 min
Response: 4756228
Conc: 18.54 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

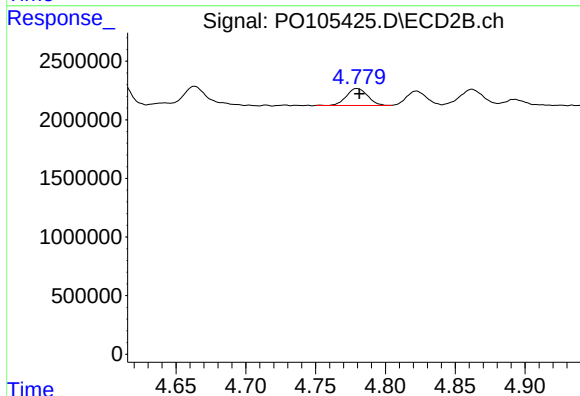


#5 AR-1016-3

R.T.: 4.780 min
Delta R.T.: -0.002 min
Response: 1526597
Conc: 18.23 ng/ml

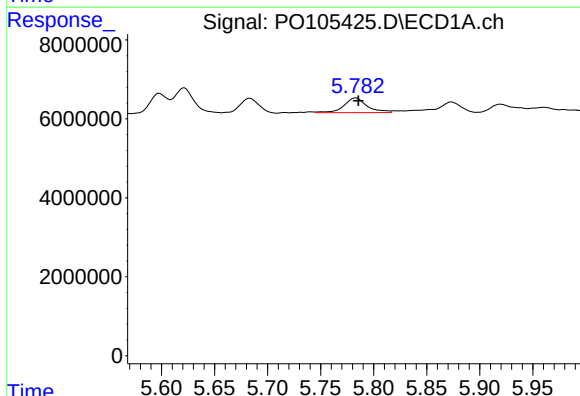


#6 AR-1016-4

R.T.: 5.783 min
Delta R.T.: -0.002 min
Response: 5623271
Conc: 25.71 ng/ml

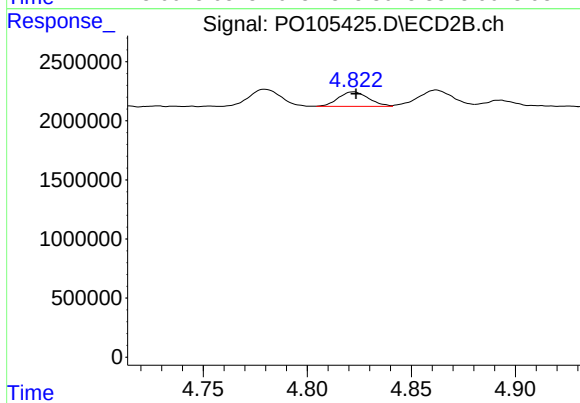

#6 AR-1016-4


R.T.: 4.822 min
Delta R.T.: -0.001 min
Response: 1231676
Conc: 18.29 ng/ml

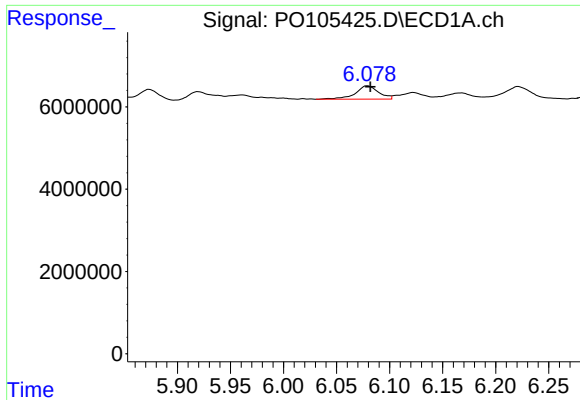

#7 AR-1016-5


R.T.: 6.079 min
Delta R.T.: -0.003 min
Response: 4963242
Conc: 23.20 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

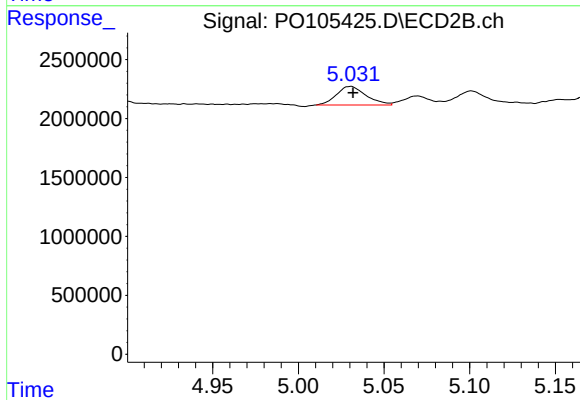


#7 AR-1016-5

R.T.: 5.030 min
Delta R.T.: -0.001 min
Response: 1899817
Conc: 22.70 ng/ml

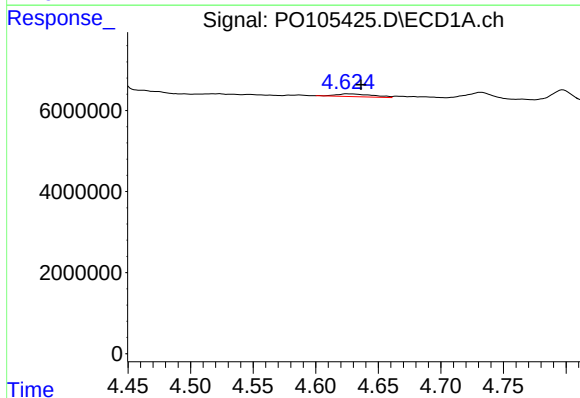


#8 AR-1221-1

R.T.: 4.625 min
Delta R.T.: -0.011 min
Response: 1367061
Conc: 12.19 ng/ml

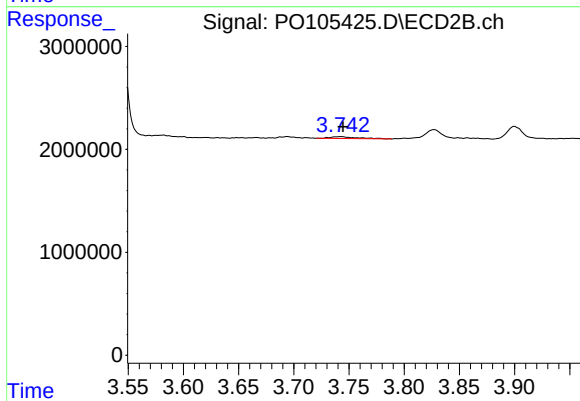

#8 AR-1221-1


R.T.: 3.743 min
Delta R.T.: -0.002 min
Response: 312221
Conc: 7.91 ng/ml

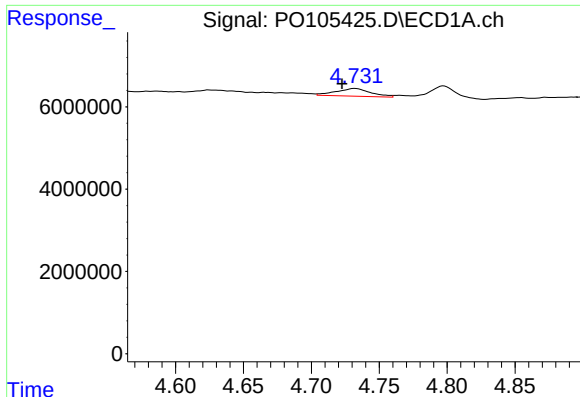

#9 AR-1221-2


R.T.: 4.732 min
Delta R.T.: 0.009 min
Response: 3322987
Conc: 39.20 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

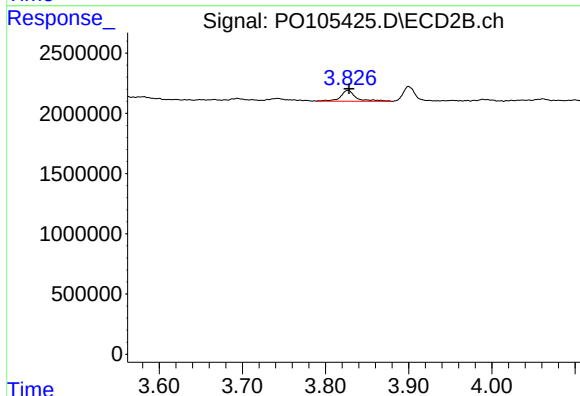


#9 AR-1221-2

R.T.: 3.827 min
Delta R.T.: -0.001 min
Response: 1161928
Conc: 37.82 ng/ml

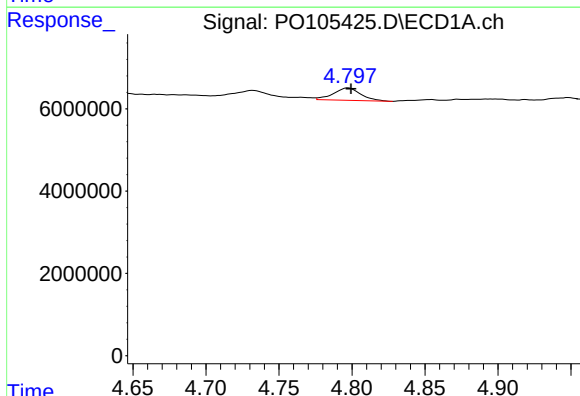


#10 AR-1221-3

R.T.: 4.797 min
Delta R.T.: -0.002 min
Response: 3910154
Conc: 16.07 ng/ml

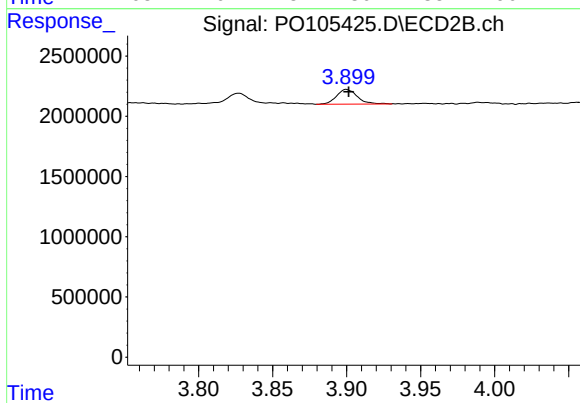

#10 AR-1221-3


R.T.: 3.900 min
Delta R.T.: -0.002 min
Response: 1187895
Conc: 13.28 ng/ml

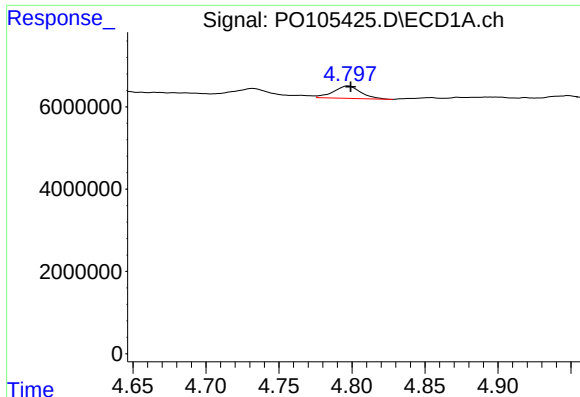

#11 AR-1232-1


R.T.: 4.797 min
Delta R.T.: -0.002 min
Response: 3910154
Conc: 19.56 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

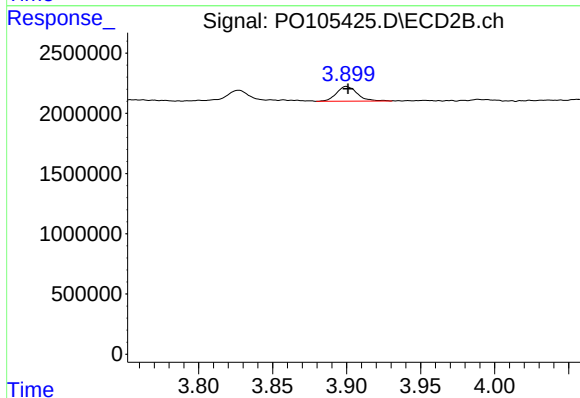


#11 AR-1232-1

R.T.: 3.900 min
Delta R.T.: -0.001 min
Response: 1187895
Conc: 16.27 ng/ml

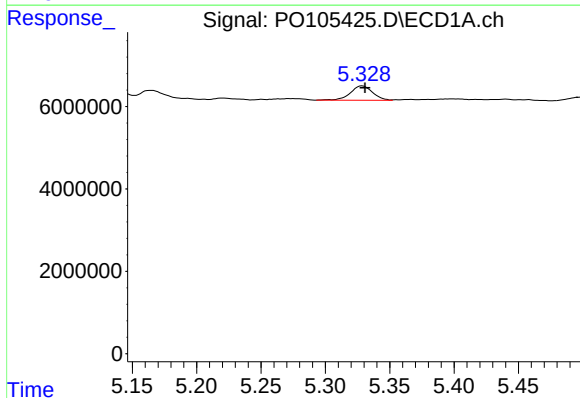


#12 AR-1232-2

R.T.: 5.329 min
Delta R.T.: -0.002 min
Response: 4231410
Conc: 39.98 ng/ml

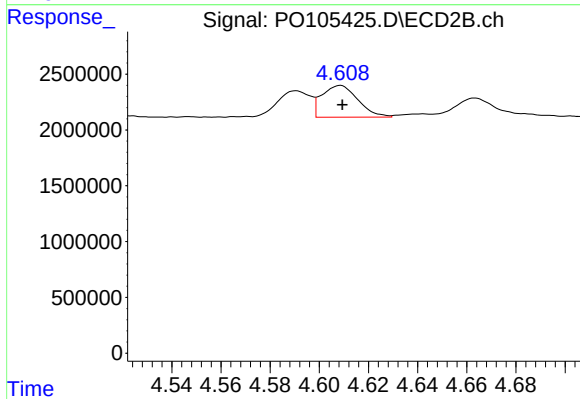

#12 AR-1232-2


R.T.: 4.609 min
Delta R.T.: 0.000 min
Response: 2891169
Conc: 41.18 ng/ml

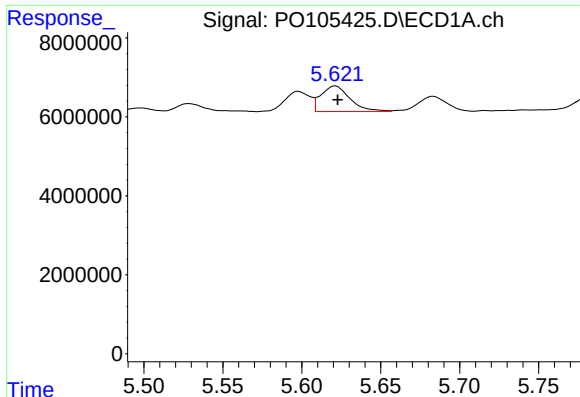

#13 AR-1232-3


R.T.: 5.621 min
Delta R.T.: -0.002 min
Response: 8265851
Conc: 43.18 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

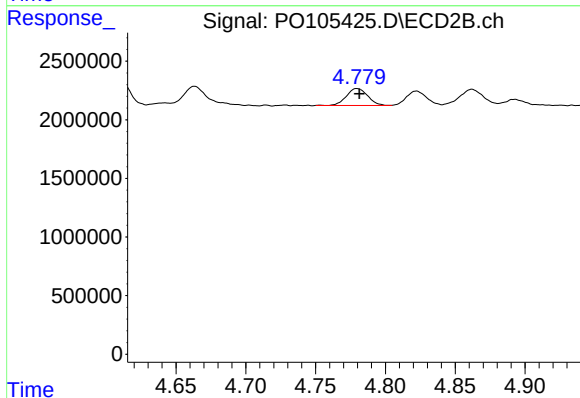


#13 AR-1232-3

R.T.: 4.780 min
Delta R.T.: -0.002 min
Response: 1526597
Conc: 39.95 ng/ml

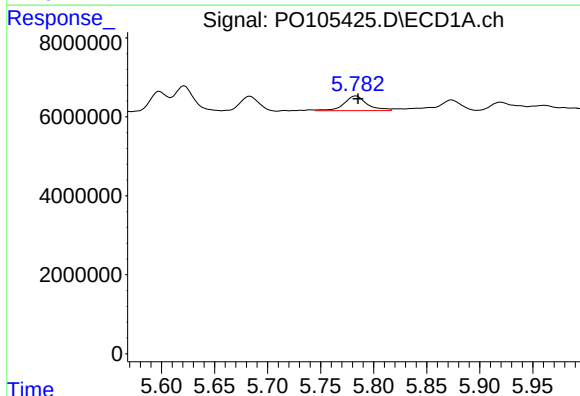


#14 AR-1232-4

R.T.: 5.783 min
Delta R.T.: -0.002 min
Response: 5623271
Conc: 57.65 ng/ml

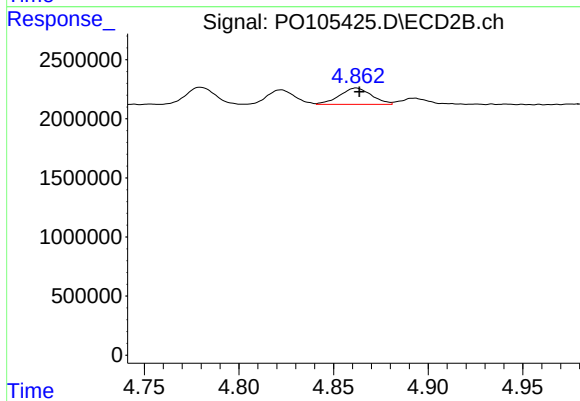

#14 AR-1232-4


R.T.: 4.862 min
Delta R.T.: -0.002 min
Response: 1617515
Conc: 46.49 ng/ml

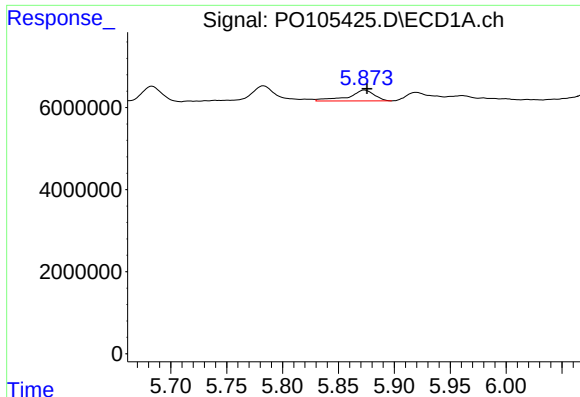

#15 AR-1232-5


R.T.: 5.873 min
Delta R.T.: -0.002 min
Response: 4289166
Conc: 59.52 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

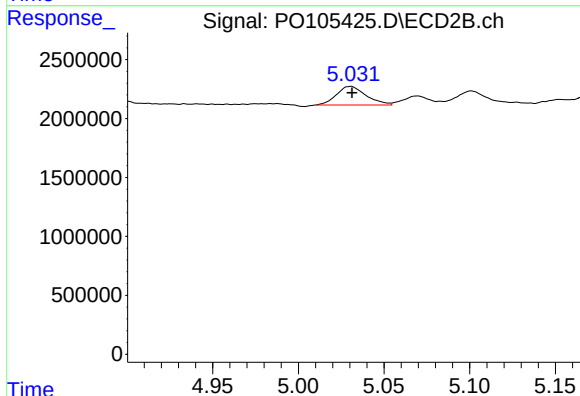


#15 AR-1232-5

R.T.: 5.030 min
Delta R.T.: 0.000 min
Response: 1899817
Conc: 53.82 ng/ml

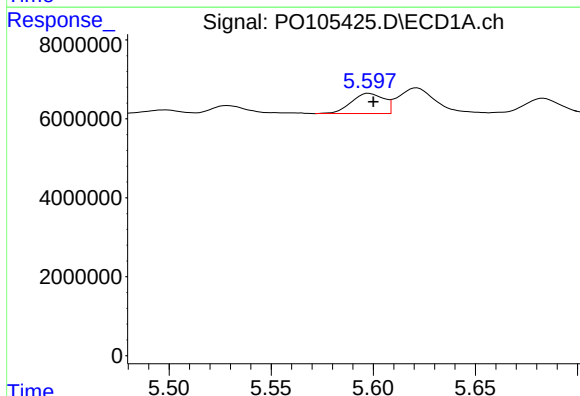


#16 AR-1242-1

R.T.: 5.598 min
Delta R.T.: -0.002 min
Response: 5643436
Conc: 24.28 ng/ml

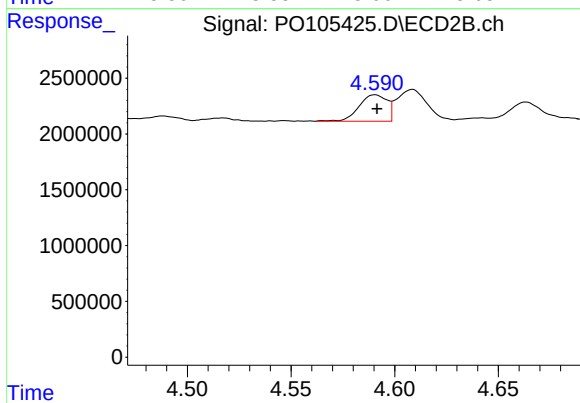

#16 AR-1242-1


R.T.: 4.591 min
Delta R.T.: 0.000 min
Response: 2232265
Conc: 25.31 ng/ml

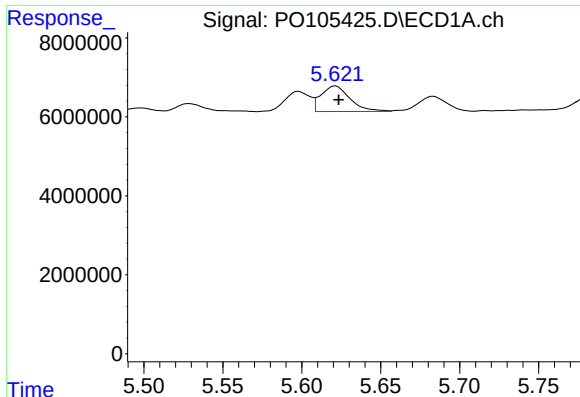

#17 AR-1242-2


R.T.: 5.621 min
Delta R.T.: -0.002 min
Response: 8265851
Conc: 25.36 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

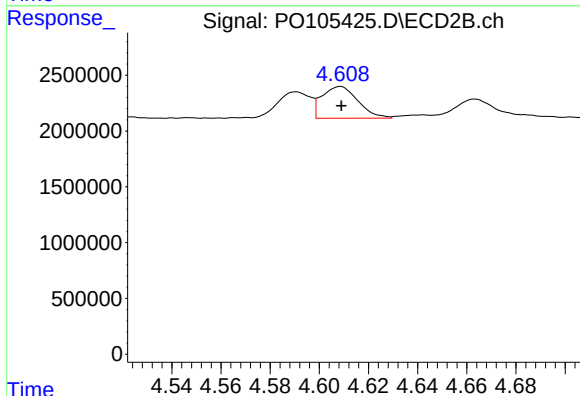


#17 AR-1242-2

R.T.: 4.609 min
Delta R.T.: 0.000 min
Response: 2891169
Conc: 24.35 ng/ml

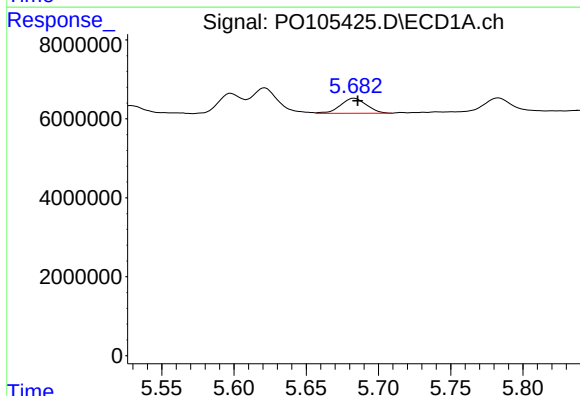


#18 AR-1242-3

R.T.: 5.683 min
Delta R.T.: -0.002 min
Response: 4756228
Conc: 24.11 ng/ml

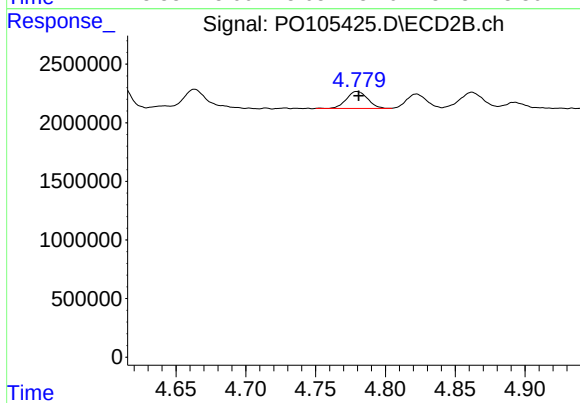

#18 AR-1242-3


R.T.: 4.780 min
Delta R.T.: -0.001 min
Response: 1526597
Conc: 23.51 ng/ml

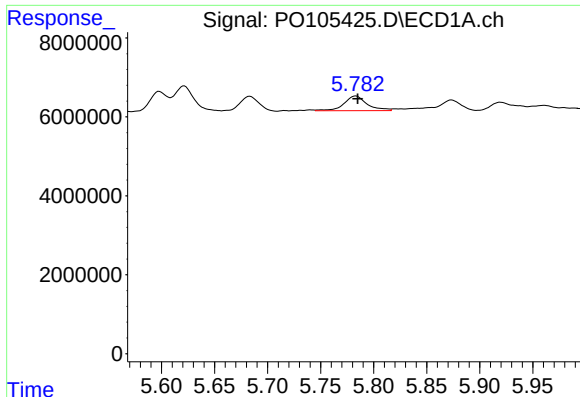

#19 AR-1242-4


R.T.: 5.783 min
Delta R.T.: -0.002 min
Response: 5623271
Conc: 32.96 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

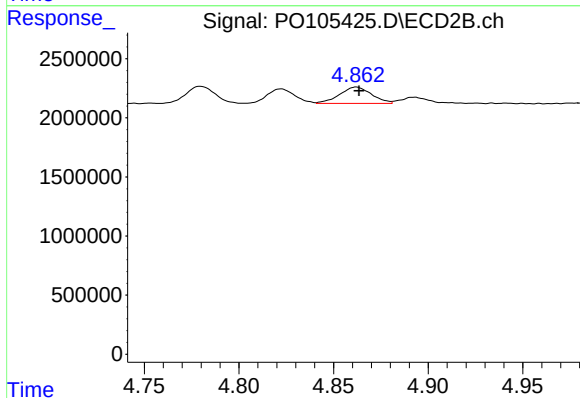


#19 AR-1242-4

R.T.: 4.862 min
Delta R.T.: -0.002 min
Response: 1617515
Conc: 24.39 ng/ml

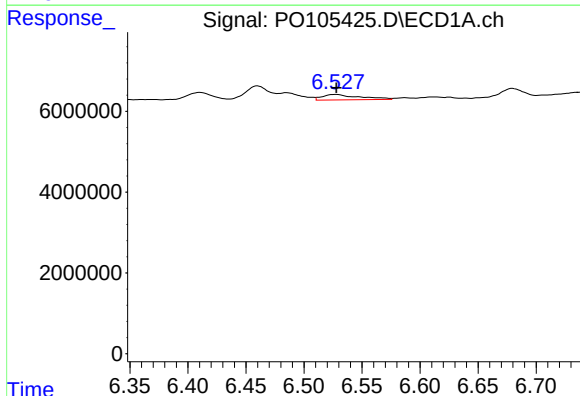


#20 AR-1242-5

R.T.: 6.527 min
Delta R.T.: 0.000 min
Response: 2981005
Conc: 17.06 ng/ml

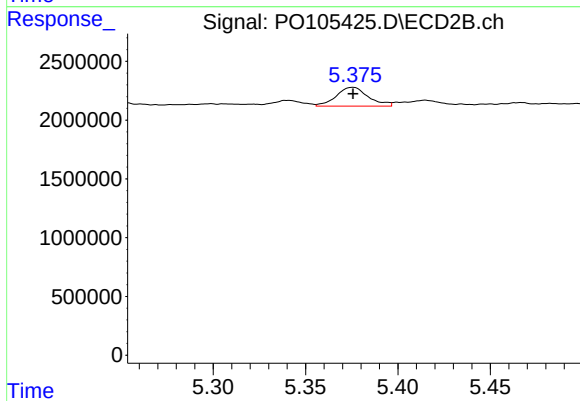

#20 AR-1242-5


R.T.: 5.376 min
Delta R.T.: 0.000 min
Response: 1944853
Conc: 23.67 ng/ml

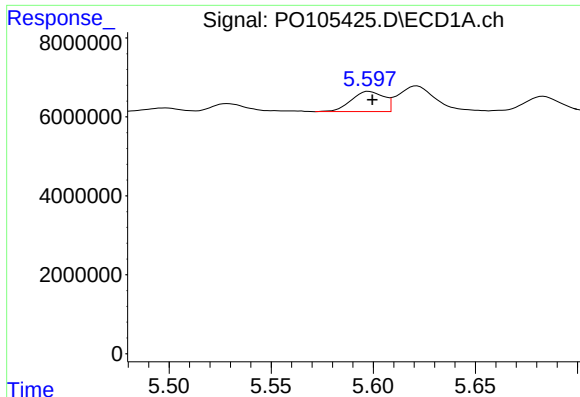

#21 AR-1248-1


R.T.: 5.598 min
Delta R.T.: -0.002 min
Response: 5643436
Conc: 30.91 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

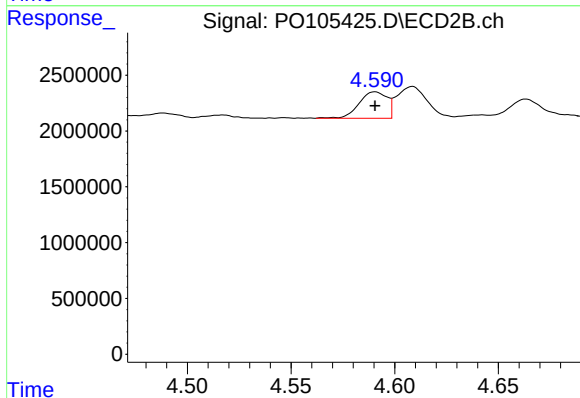


#21 AR-1248-1

R.T.: 4.591 min
Delta R.T.: 0.000 min
Response: 2232265
Conc: 31.96 ng/ml

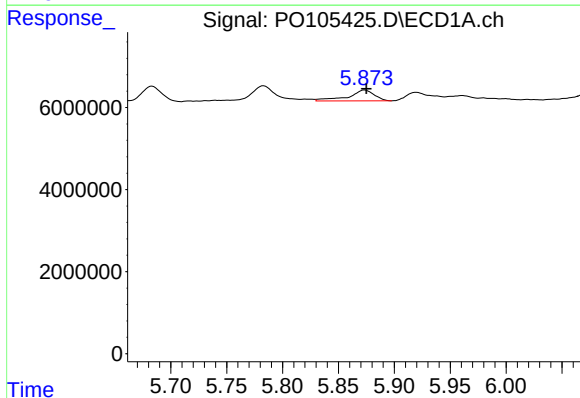


#22 AR-1248-2

R.T.: 5.873 min
Delta R.T.: -0.002 min
Response: 4289166
Conc: 17.03 ng/ml

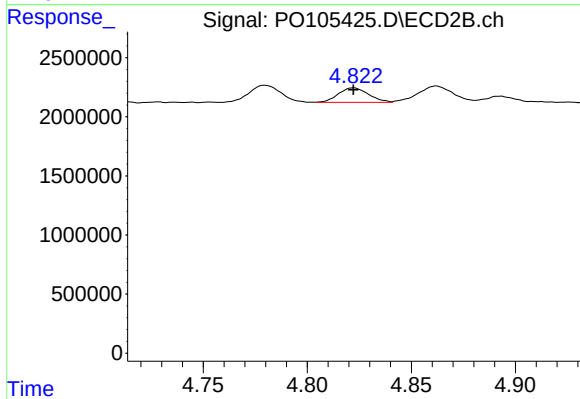

#22 AR-1248-2


R.T.: 4.822 min
Delta R.T.: 0.000 min
Response: 1231676
Conc: 12.98 ng/ml

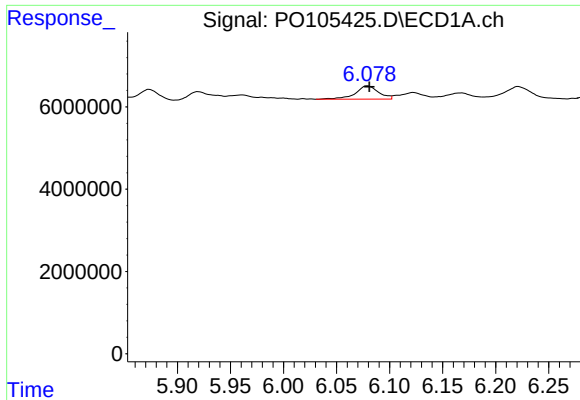

#23 AR-1248-3


R.T.: 6.079 min
Delta R.T.: -0.002 min
Response: 4963242
Conc: 17.56 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

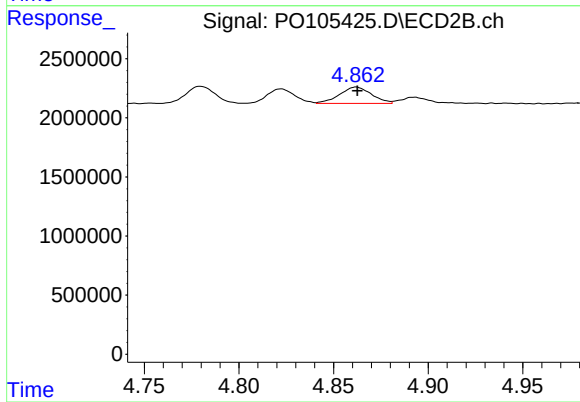


#23 AR-1248-3

R.T.: 4.862 min
Delta R.T.: 0.000 min
Response: 1617515
Conc: 16.20 ng/ml

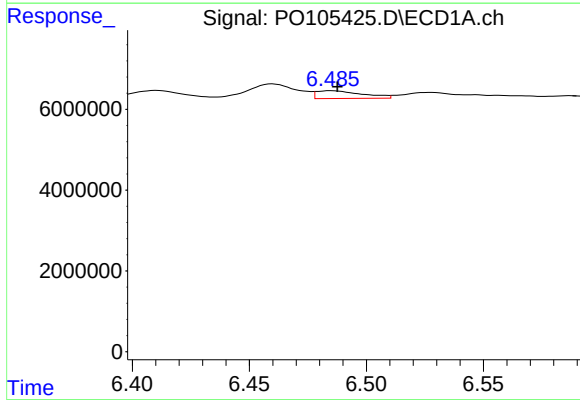


#24 AR-1248-4

R.T.: 6.485 min
Delta R.T.: -0.002 min
Response: 2607897
Conc: 8.16 ng/ml

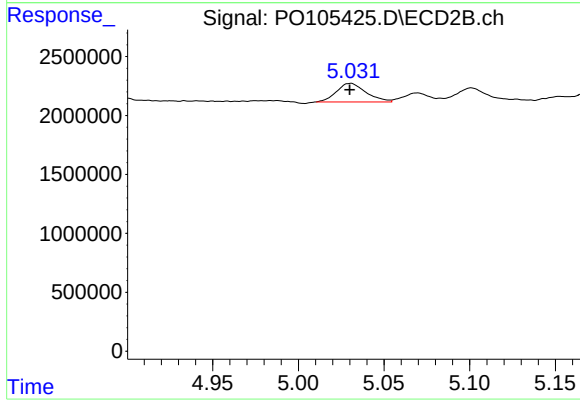

#24 AR-1248-4


R.T.: 5.030 min
Delta R.T.: 0.000 min
Response: 1899817
Conc: 16.83 ng/ml

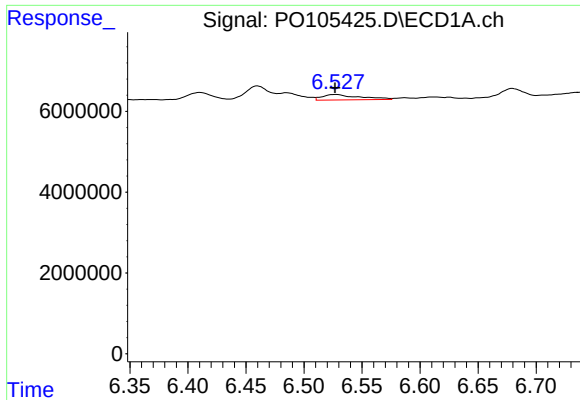

#25 AR-1248-5


R.T.: 6.527 min
Delta R.T.: 0.000 min
Response: 2981005
Conc: 9.64 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

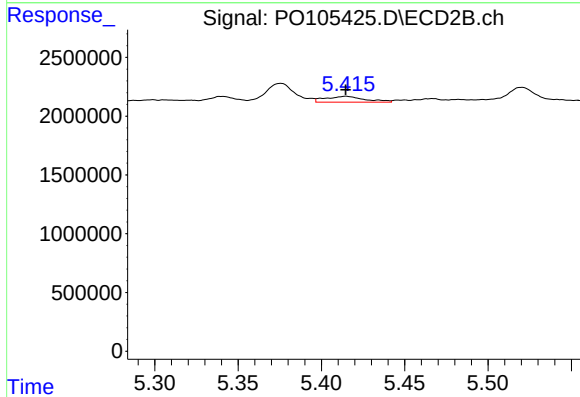


#25 AR-1248-5

R.T.: 5.415 min
Delta R.T.: 0.000 min
Response: 812944
Conc: 7.22 ng/ml

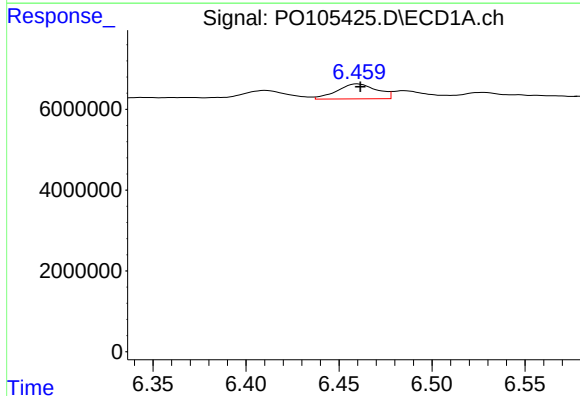


#26 AR-1254-1

R.T.: 6.460 min
Delta R.T.: -0.001 min
Response: 5528704
Conc: 17.63 ng/ml

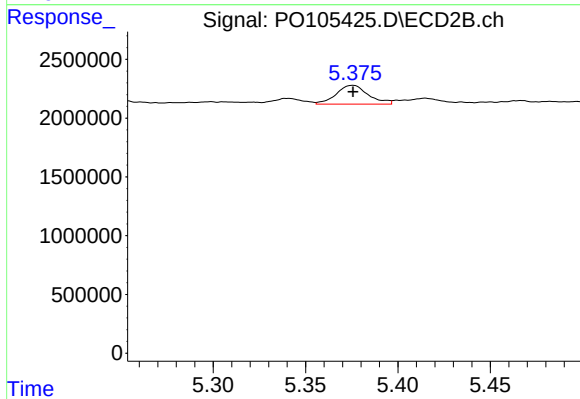

#26 AR-1254-1


R.T.: 5.376 min
Delta R.T.: 0.000 min
Response: 1944853
Conc: 11.95 ng/ml

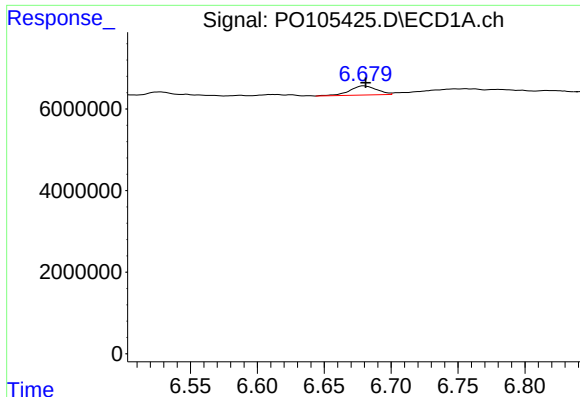

#27 AR-1254-2


R.T.: 6.680 min
Delta R.T.: -0.001 min
Response: 3141058
Conc: 6.96 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

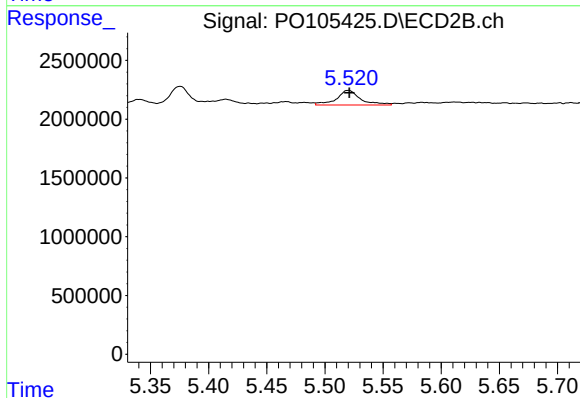


#27 AR-1254-2

R.T.: 5.520 min
Delta R.T.: 0.000 min
Response: 1792092
Conc: 12.25 ng/ml

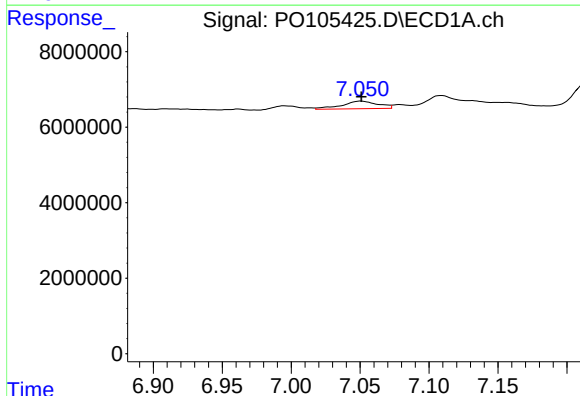


#28 AR-1254-3

R.T.: 7.051 min
Delta R.T.: 0.000 min
Response: 3651961
Conc: 7.70 ng/ml

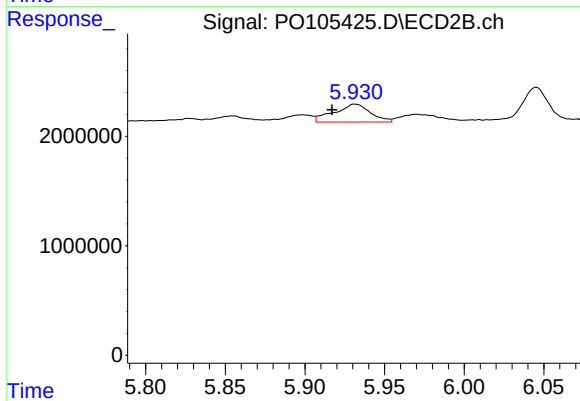

#28 AR-1254-3


R.T.: 5.932 min
Delta R.T.: 0.014 min
Response: 2584681
Conc: 11.46 ng/ml

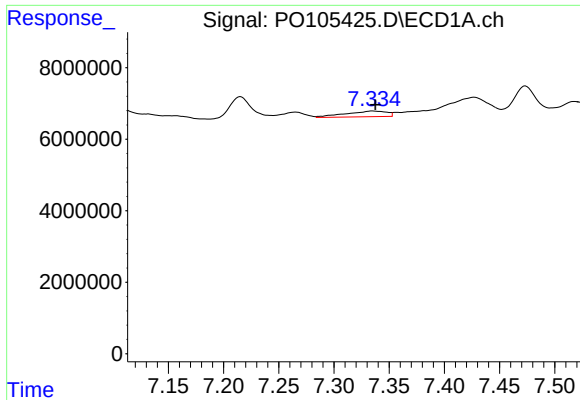

#29 AR-1254-4


R.T.: 7.335 min
Delta R.T.: -0.003 min
Response: 4089371
Conc: 11.42 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

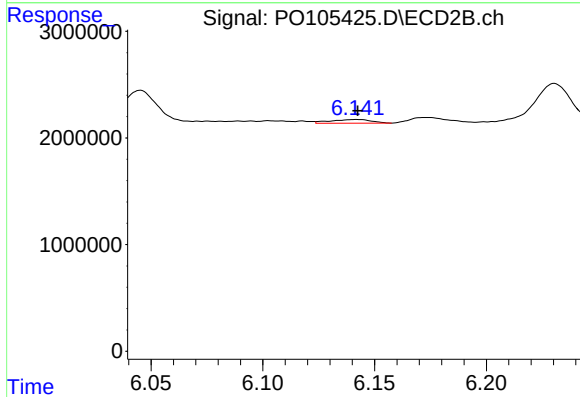


#29 AR-1254-4

R.T.: 6.142 min
Delta R.T.: 0.000 min
Response: 436391
Conc: 3.09 ng/ml

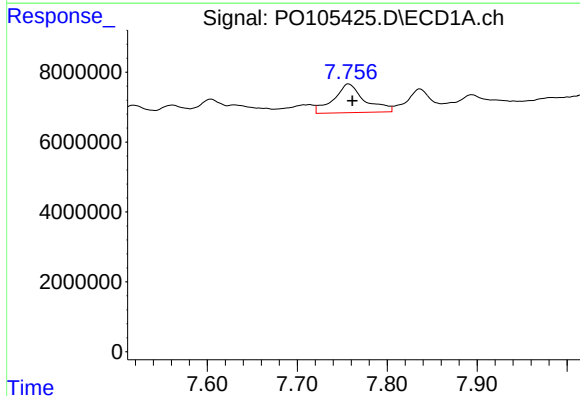


#30 AR-1254-5

R.T.: 7.757 min
Delta R.T.: -0.004 min
Response: 19733644
Conc: 49.71 ng/ml

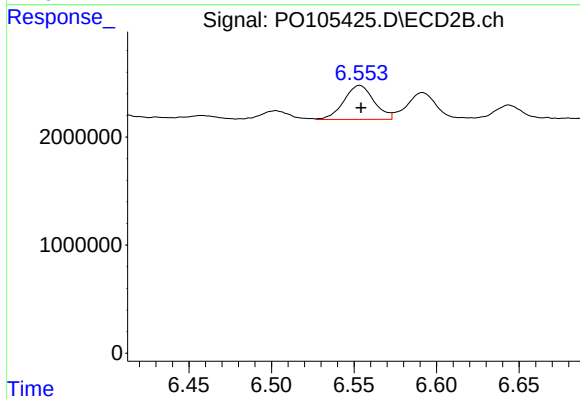

#30 AR-1254-5


R.T.: 6.553 min
Delta R.T.: 0.000 min
Response: 3994298
Conc: 19.94 ng/ml

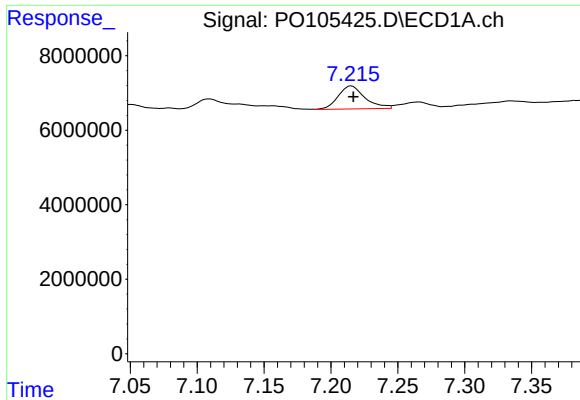

#31 AR-1260-1


R.T.: 7.215 min
Delta R.T.: -0.002 min
Response: 8608603
Conc: 23.49 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

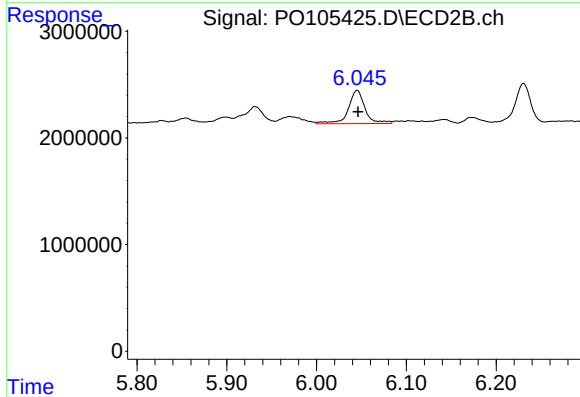


#31 AR-1260-1

R.T.: 6.045 min
Delta R.T.: -0.001 min
Response: 4017603
Conc: 25.74 ng/ml

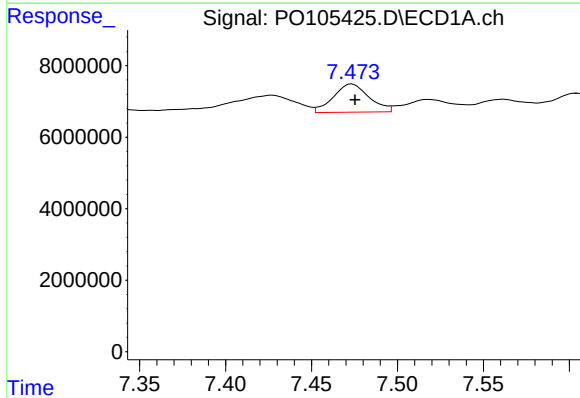


#32 AR-1260-2

R.T.: 7.473 min
Delta R.T.: -0.002 min
Response: 11350861
Conc: 27.26 ng/ml

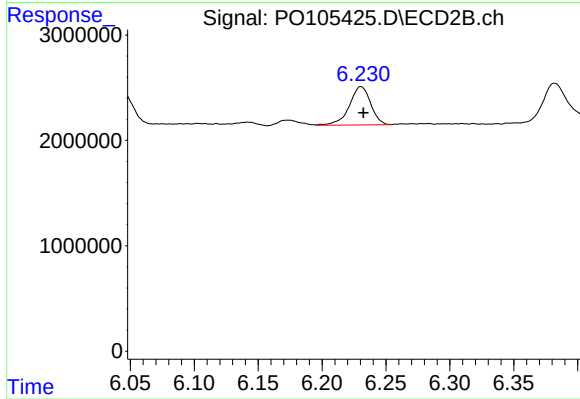

#32 AR-1260-2


R.T.: 6.231 min
Delta R.T.: -0.002 min
Response: 4217480
Conc: 22.31 ng/ml

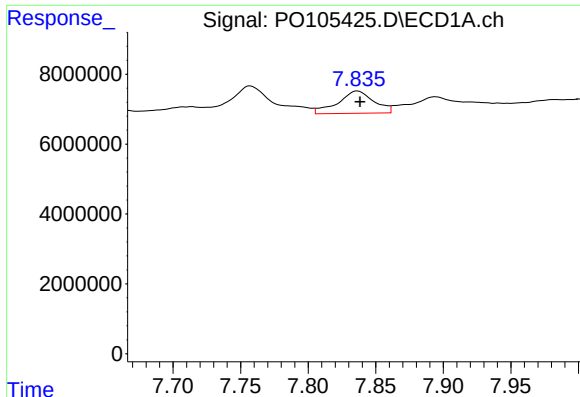

#33 AR-1260-3


R.T.: 7.836 min
Delta R.T.: -0.002 min
Response: 11870945
Conc: 45.87 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

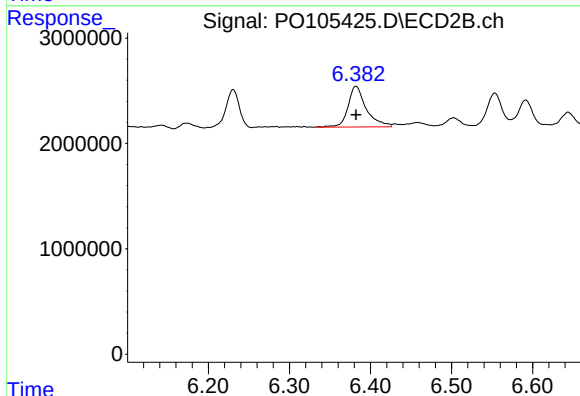


#33 AR-1260-3

R.T.: 6.382 min
Delta R.T.: 0.000 min
Response: 6026666
Conc: 32.62 ng/ml

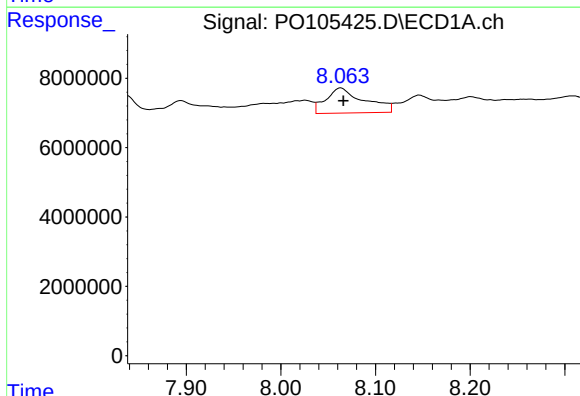


#34 AR-1260-4

R.T.: 8.063 min
Delta R.T.: -0.003 min
Response: 20323530
Conc: 61.60 ng/ml

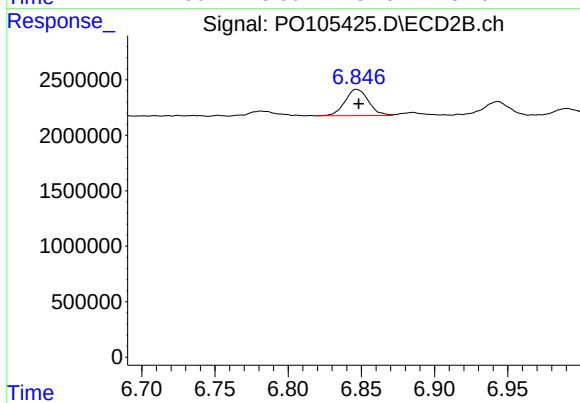

#34 AR-1260-4


R.T.: 6.847 min
Delta R.T.: -0.001 min
Response: 2666103
Conc: 21.81 ng/ml

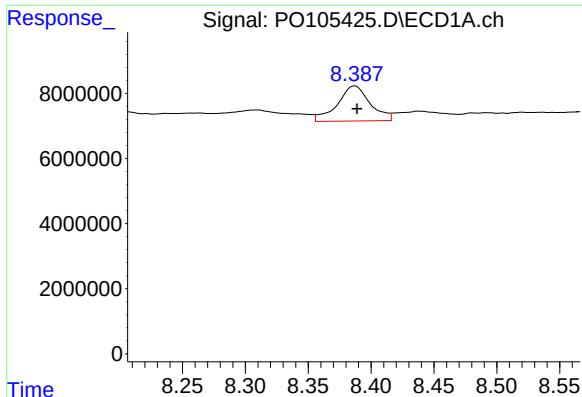

#35 AR-1260-5


R.T.: 8.387 min
Delta R.T.: -0.002 min
Response: 19484748
Conc: 32.75 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

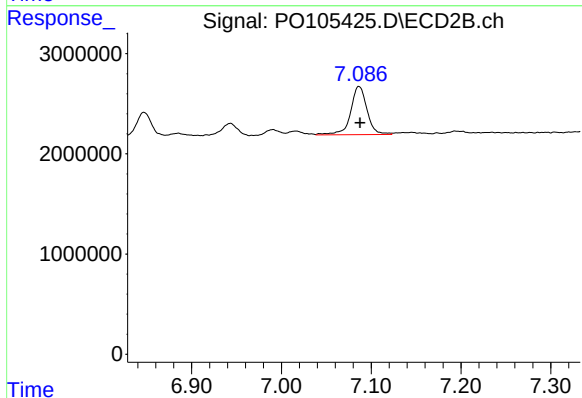


#35 AR-1260-5

R.T.: 7.086 min
Delta R.T.: -0.001 min
Response: 6109428
Conc: 21.95 ng/ml

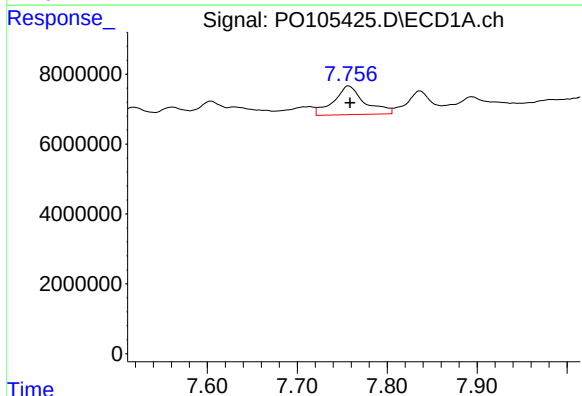


#36 AR-1262-1

R.T.: 7.757 min
Delta R.T.: -0.002 min
Response: 19733644
Conc: 62.13 ng/ml

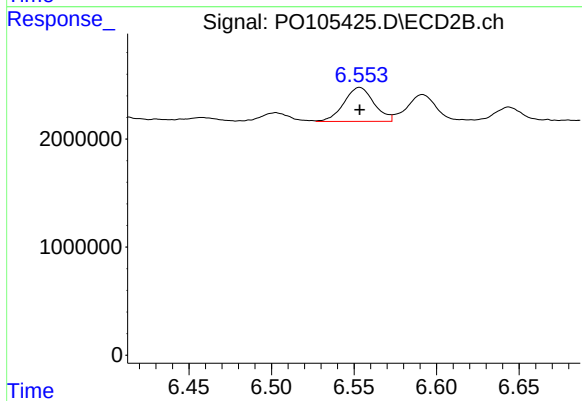

#36 AR-1262-1


R.T.: 6.553 min
Delta R.T.: 0.000 min
Response: 3994298
Conc: 37.54 ng/ml

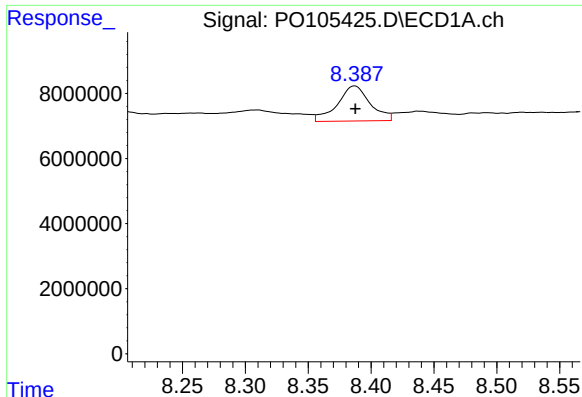

#37 AR-1262-2


R.T.: 8.387 min
Delta R.T.: 0.000 min
Response: 19484748
Conc: 25.90 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

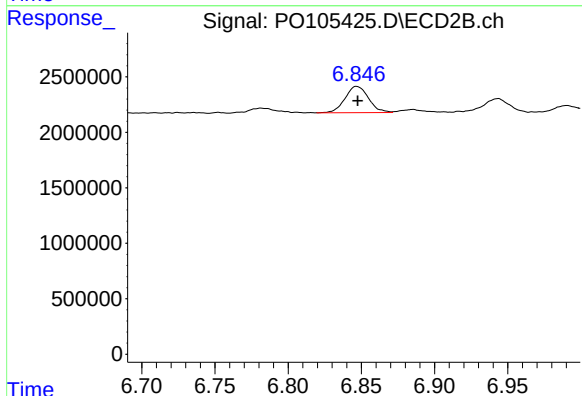


#37 AR-1262-2

R.T.: 6.847 min
Delta R.T.: 0.000 min
Response: 2666103
Conc: 15.69 ng/ml

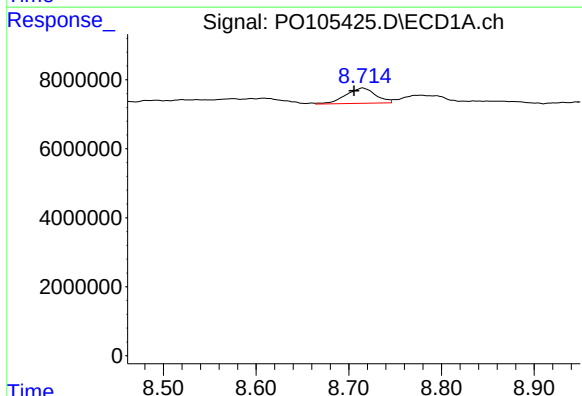


#38 AR-1262-3

R.T.: 8.715 min
Delta R.T.: 0.009 min
Response: 9895029
Conc: 20.11 ng/ml

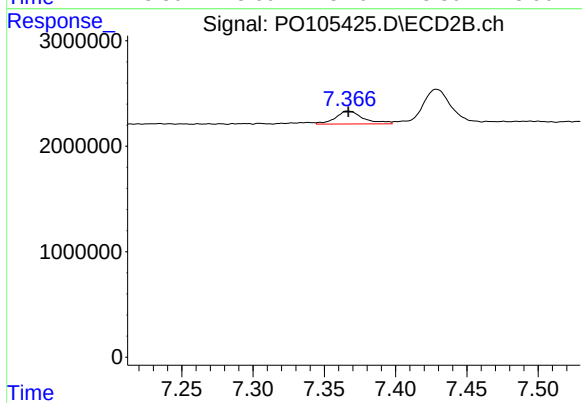

#38 AR-1262-3


R.T.: 7.367 min
Delta R.T.: 0.000 min
Response: 1665982
Conc: 13.20 ng/ml

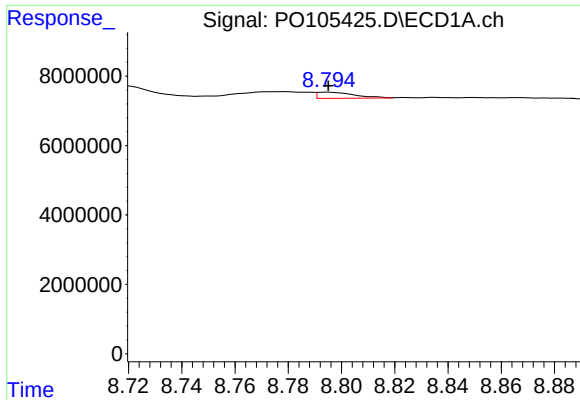

#39 AR-1262-4


R.T.: 8.795 min
Delta R.T.: 0.000 min
Response: 1700459
Conc: 4.63 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

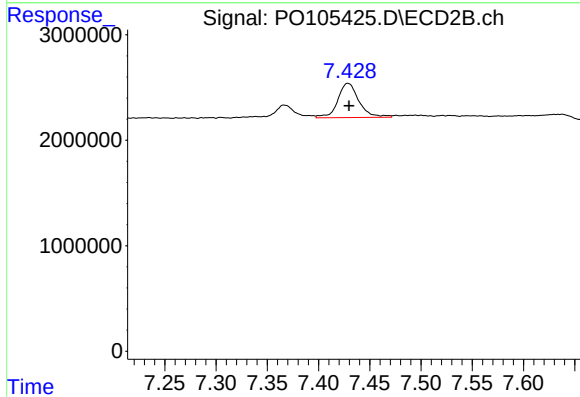


#39 AR-1262-4

R.T.: 7.429 min
Delta R.T.: -0.001 min
Response: 4660129
Conc: 20.13 ng/ml

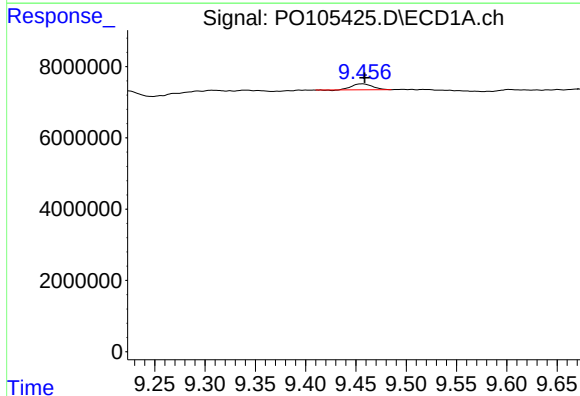


#40 AR-1262-5

R.T.: 9.457 min
Delta R.T.: -0.002 min
Response: 2392957
Conc: 8.94 ng/ml

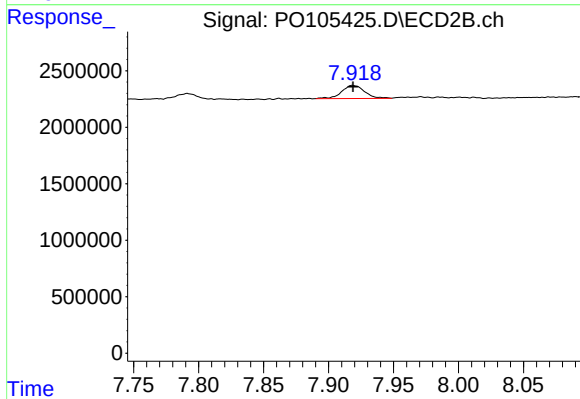

#40 AR-1262-5


R.T.: 7.919 min
Delta R.T.: 0.000 min
Response: 1428706
Conc: 14.22 ng/ml

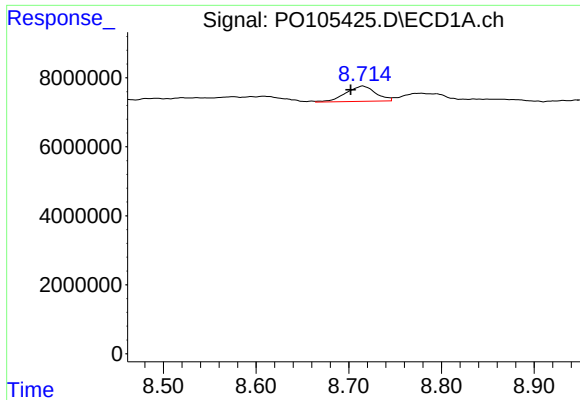

#41 AR-1268-1


R.T.: 8.715 min
Delta R.T.: 0.013 min
Response: 9895029
Conc: 12.17 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

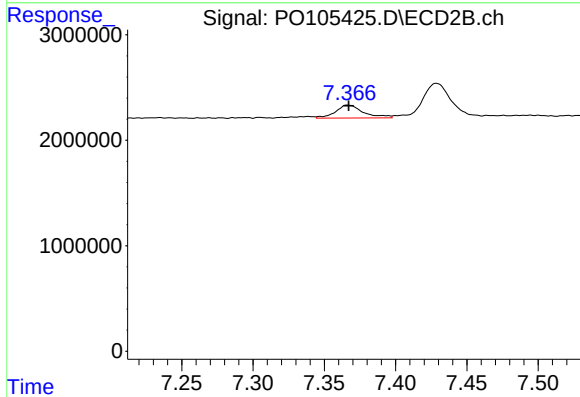


#41 AR-1268-1

R.T.: 7.367 min
Delta R.T.: 0.000 min
Response: 1665982
Conc: 4.77 ng/ml

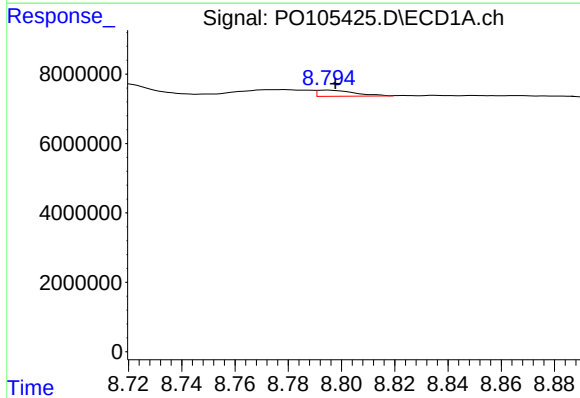


#42 AR-1268-2

R.T.: 8.795 min
Delta R.T.: -0.003 min
Response: 1700459
Conc: 2.34 ng/ml

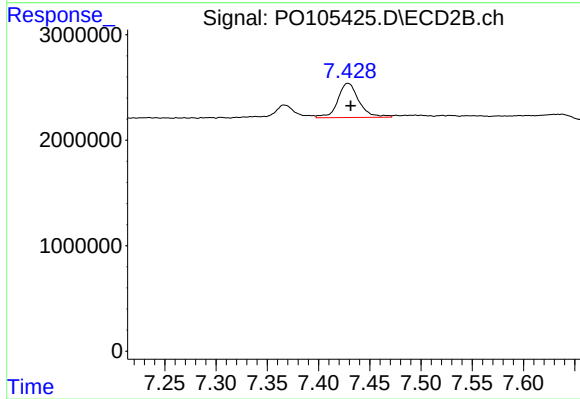

#42 AR-1268-2


R.T.: 7.429 min
Delta R.T.: -0.003 min
Response: 4660129
Conc: 14.94 ng/ml

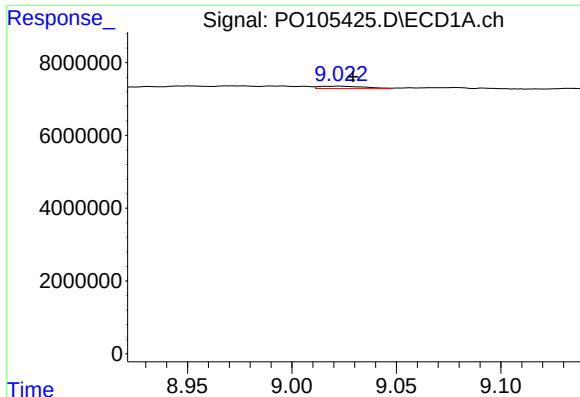

#43 AR-1268-3


R.T.: 9.023 min
Delta R.T.: -0.006 min
Response: 1019878
Conc: 1.58 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

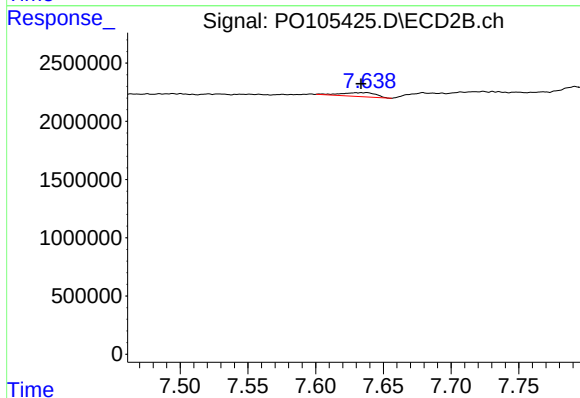


#43 AR-1268-3

R.T.: 7.637 min
Delta R.T.: 0.004 min
Response: 593021
Conc: 2.35 ng/ml

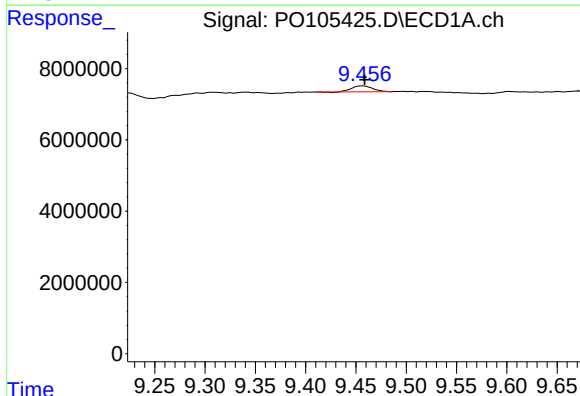


#44 AR-1268-4

R.T.: 9.457 min
Delta R.T.: -0.002 min
Response: 2392957
Conc: 8.59 ng/ml

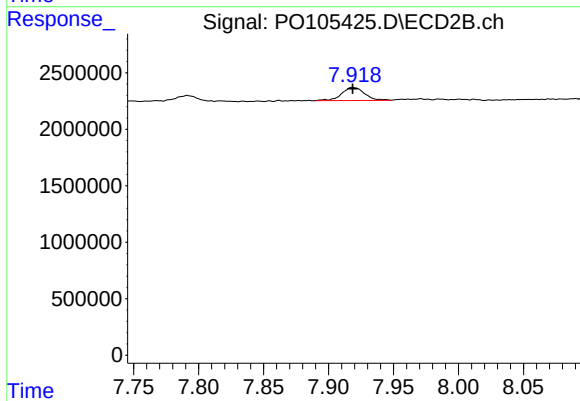

#44 AR-1268-4


R.T.: 7.919 min
Delta R.T.: 0.000 min
Response: 1428706
Conc: 13.28 ng/ml

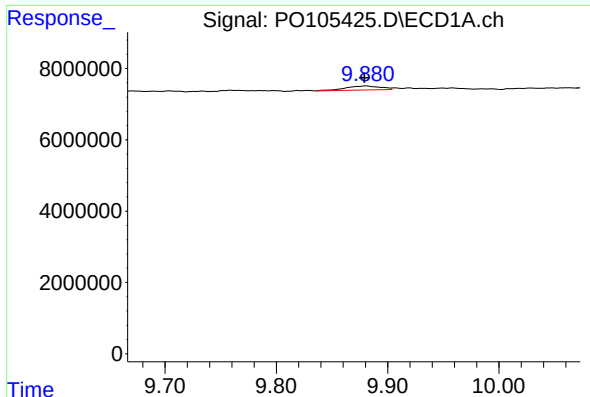

#45 AR-1268-5

R.T.: 9.881 min
Delta R.T.: 0.001 min
Response: 2426581
Conc: 1.16 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

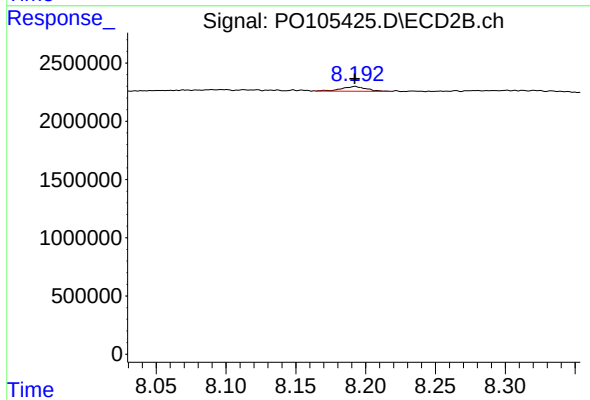

#45 AR-1268-5

R.T.: 8.192 min
Delta R.T.: 0.000 min
Response: 501009
Conc: 0.75 ng/ml