

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081224\
 Data File : P0105426.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2024 17:33
 Operator : YP/AJ
 Sample : P3390-07
 Misc : AR1221 LOD 25 PPB
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 02:29:48 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081024.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 10 04:08:56 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.428	3.537	138.8E6	48433213	15.896	15.420
2)	SA Decachlor...	10.219	8.428	100.1E6	29183875	17.406	16.485
Target Compounds							
3)	L1 AR-1016-1	5.596	4.591	404512	215153	1.337	1.914 #
4)	L1 AR-1016-2	5.621	4.610	966730	309796	2.261	1.990
5)	L1 AR-1016-3	5.684	4.778	676761	138600	2.638	1.655 #
6)	L1 AR-1016-4	5.787	4.832	1212765	56466	5.545	0.839 #
7)	L1 AR-1016-5	6.089	5.037	663378	291362	3.101	3.481
8)	L2 AR-1221-1	4.635	3.744	3354580	842947	29.914	21.356 #
9)	L2 AR-1221-2	4.730	3.828	4117075	1650910	48.573	53.736
10)	L2 AR-1221-3	4.798	3.901	6313761	2095144	25.952	23.414
11)	L3 AR-1232-1	4.798	3.901	6313761	2095144	31.579	28.689
12)	L3 AR-1232-2	5.333	4.610	611681	309796	5.779	4.412
13)	L3 AR-1232-3	5.621	4.778	966730	138600	5.051	3.627 #
14)	L3 AR-1232-4	5.787	4.862	1212765	139476	12.434	4.009 #
15)	L3 AR-1232-5	5.870	5.037	392834	291362	5.451	8.254 #
16)	L4 AR-1242-1	5.596	4.591	404512	215153	1.741	2.439 #
17)	L4 AR-1242-2	5.621	4.610	966730	309796	2.966	2.609
18)	L4 AR-1242-3	5.684	4.778	676761	138600	3.431	2.134 #
19)	L4 AR-1242-4	5.787	4.862	1212765	139476	7.108	2.103 #
20)	L4 AR-1242-5	6.514	5.398	456446	943507	2.612	11.482 #
21)	L5 AR-1248-1	5.596	4.591	404512	215153	2.215	3.081 #
22)	L5 AR-1248-2	5.870	4.832	392834	56466	1.560	0.595 #
23)	L5 AR-1248-3	6.089	4.862	663378	139476	2.347	1.397 #
24)	L5 AR-1248-4	6.487	5.037	1393396	291362	4.358	2.581 #
25)	L5 AR-1248-5	6.514	5.398	456446	943507	1.476	8.379 #
26)	L6 AR-1254-1	6.474	5.398	2658829	943507	8.479	5.795 #
27)	L6 AR-1254-2	6.683	5.523	787868	541424	1.746	3.701 #
28)	L6 AR-1254-3	7.055	5.918	3913217	610498	8.249	2.706 #
29)	L6 AR-1254-4	7.329	6.144	2977913	226830	8.313	1.607 #
30)	L6 AR-1254-5	7.750	6.554	16125924	191970	40.623	0.958 #
31)	L7 AR-1260-1	7.227	6.050	2224504	317628	6.069	2.035 #
32)	L7 AR-1260-2	7.488	6.217	2391914	785774	5.745	4.158 #
33)	L7 AR-1260-3	7.835	6.393	4615393	3066125	17.833	16.597
34)	L7 AR-1260-4	8.069	6.849	8371700	127912	25.374	1.047 #
35)	L7 AR-1260-5	8.398	7.087	7784661	452163	13.086	1.625 #
36)	L8 AR-1262-1	7.750	6.554	16125924	191970	50.769	1.804 #
37)	L8 AR-1262-2	8.398	6.849	7784661	127912	10.349	0.753 #
38)	L8 AR-1262-3	8.709	7.338	573949	232531	1.166	1.842 #
39)	L8 AR-1262-4	8.803	7.428	284609	1327252	0.775	5.734 #
40)	L8 AR-1262-5	9.459	7.921	167705	105313	0.626	1.048 #
41)	L9 AR-1268-1	8.696	7.338	961870	232531	1.183	0.666 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081224\
Data File : P0105426.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Aug 2024 17:33
Operator : YP/AJ
Sample : P3390-07
Misc : AR1221 LOD 25 PPB
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 13 02:29:48 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081024.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Aug 10 04:08:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.803	7.428	284609	1327252	0.392	4.254 #
43) L9	AR-1268-3	9.049	7.633	289469	615168	0.448	2.434 #
44) L9	AR-1268-4	9.459	7.921	167705	105313	0.602	0.979 #
45) L9	AR-1268-5	9.877	8.191	1064758	362358	0.509	0.542



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081224\
Data File : PO105426.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Aug 2024 17:33
Operator : YP/AJ
Sample : P3390-07
Misc : AR1221 LOD 25 PPB
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 13 02:29:48 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081024.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Aug 10 04:08:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

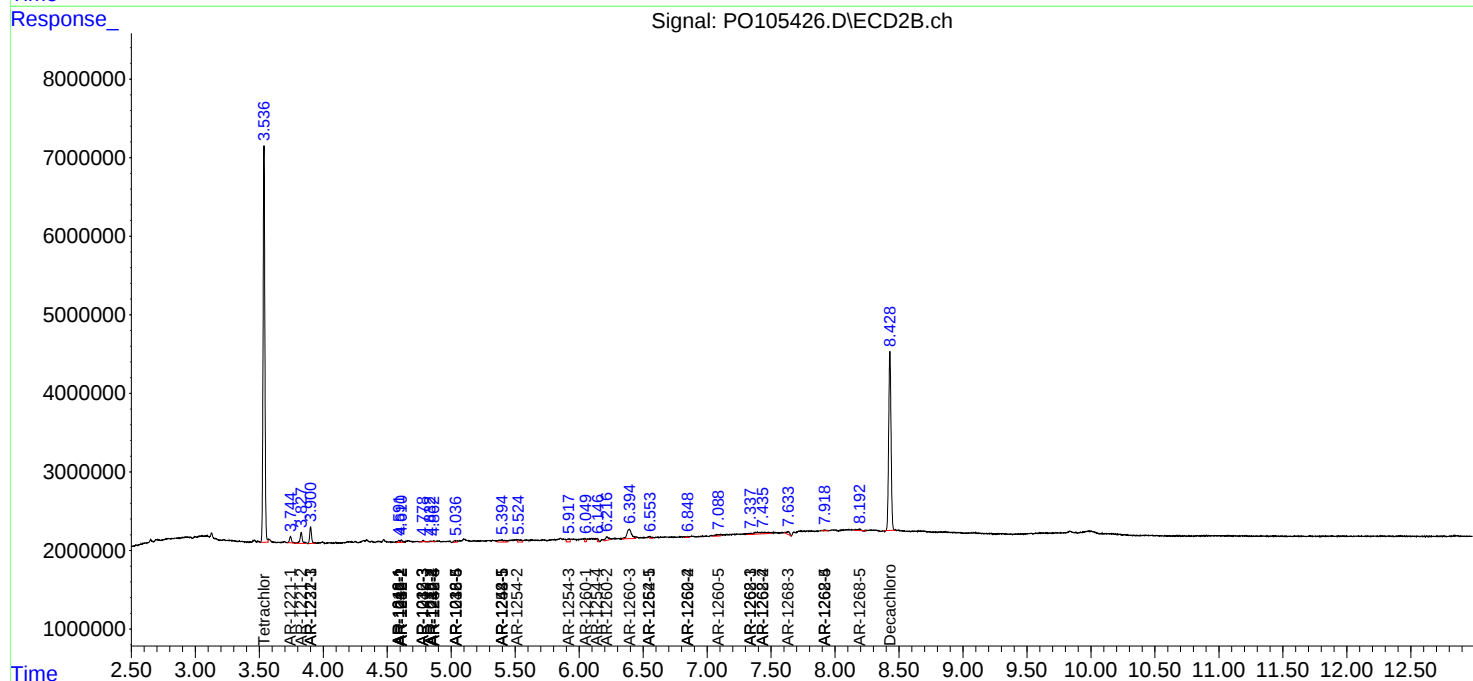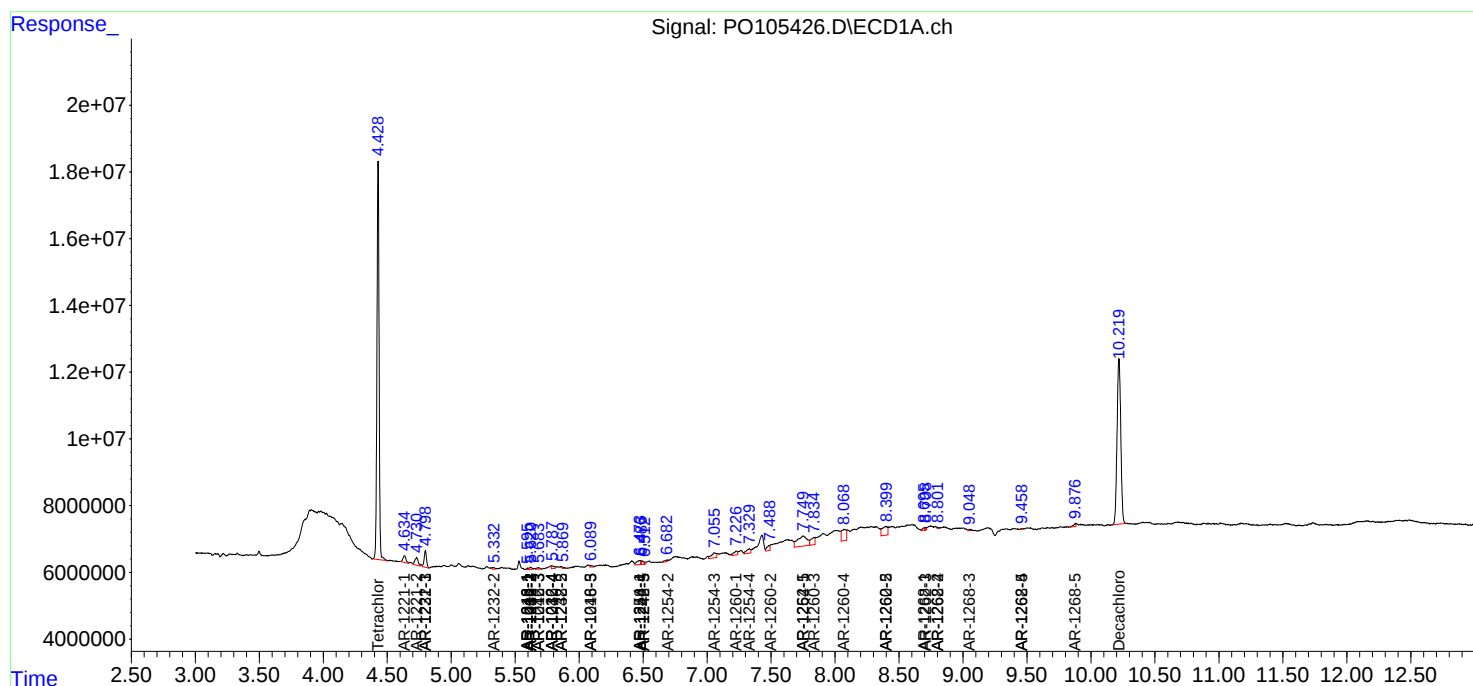


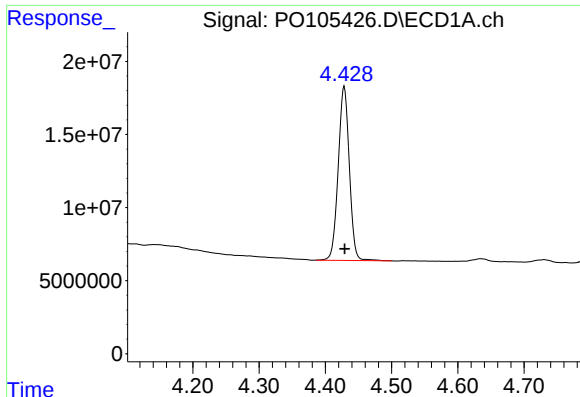

#1 Tetrachloro-m-xylene


R.T.: 4.428 min
Delta R.T.: 0.000 min
Response: 138840299
Conc: 15.90 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

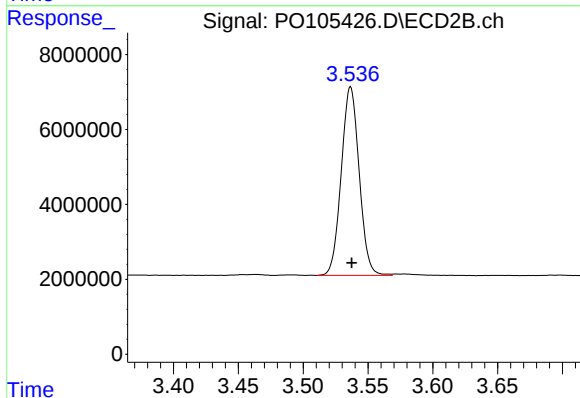


#1 Tetrachloro-m-xylene

R.T.: 3.537 min
Delta R.T.: 0.000 min
Response: 48433213
Conc: 15.42 ng/ml

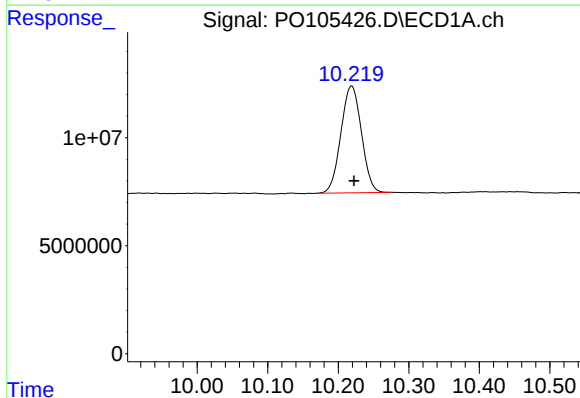


#2 Decachlorobiphenyl

R.T.: 10.219 min
Delta R.T.: -0.004 min
Response: 100129911
Conc: 17.41 ng/ml

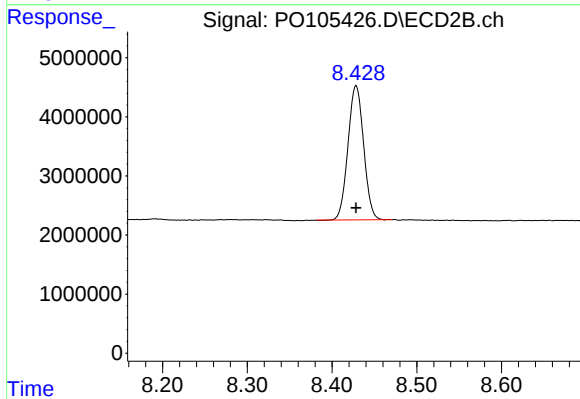

#2 Decachlorobiphenyl


R.T.: 8.428 min
Delta R.T.: 0.000 min
Response: 29183875
Conc: 16.48 ng/ml

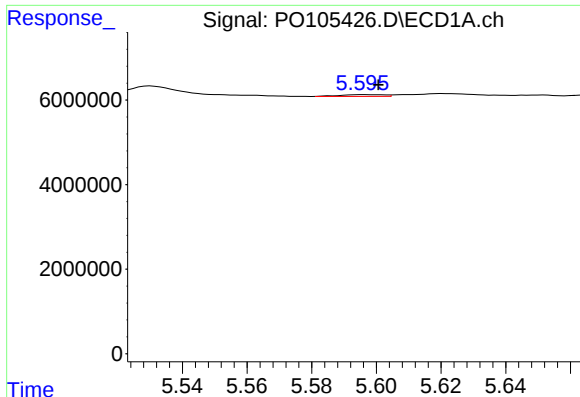

#3 AR-1016-1


R.T.: 5.596 min
Delta R.T.: -0.005 min
Response: 404512
Conc: 1.34 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

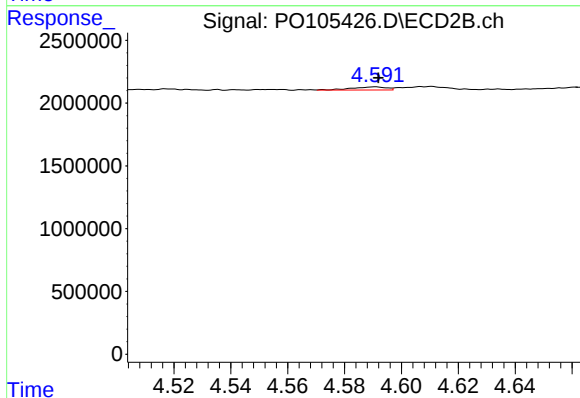


#3 AR-1016-1

R.T.: 4.591 min
Delta R.T.: -0.001 min
Response: 215153
Conc: 1.91 ng/ml

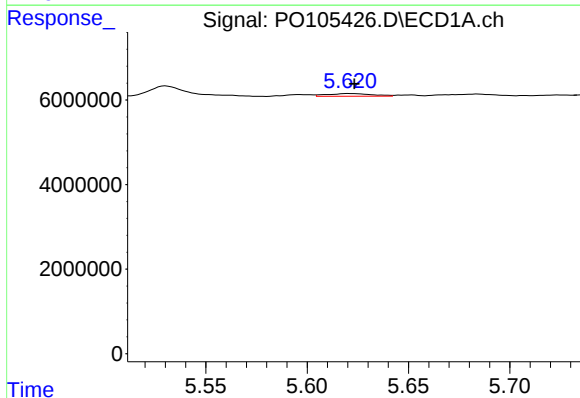


#4 AR-1016-2

R.T.: 5.621 min
Delta R.T.: -0.002 min
Response: 966730
Conc: 2.26 ng/ml

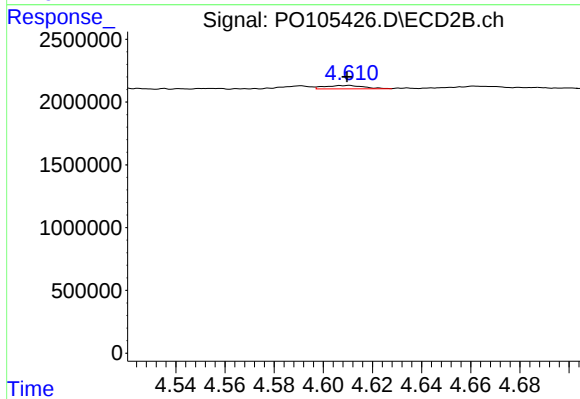

#4 AR-1016-2


R.T.: 4.610 min
Delta R.T.: 0.000 min
Response: 309796
Conc: 1.99 ng/ml

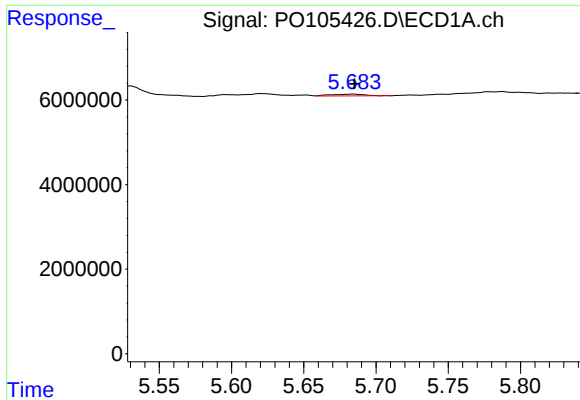

#5 AR-1016-3


R.T.: 5.684 min
Delta R.T.: 0.000 min
Response: 676761
Conc: 2.64 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

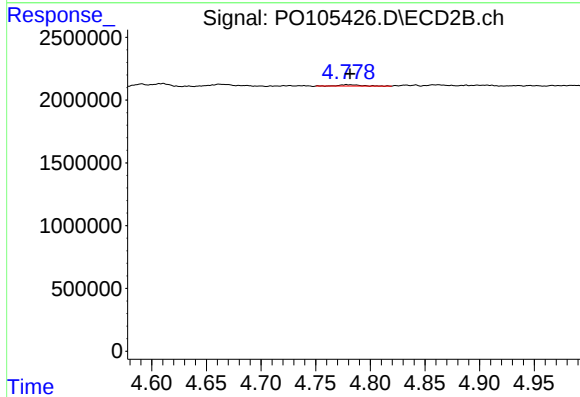


#5 AR-1016-3

R.T.: 4.778 min
Delta R.T.: -0.003 min
Response: 138600
Conc: 1.65 ng/ml

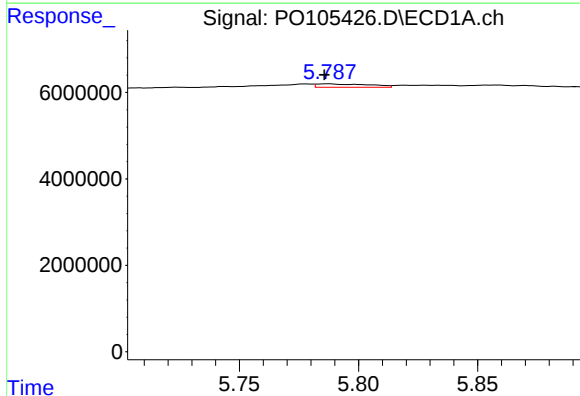


#6 AR-1016-4

R.T.: 5.787 min
Delta R.T.: 0.002 min
Response: 1212765
Conc: 5.55 ng/ml

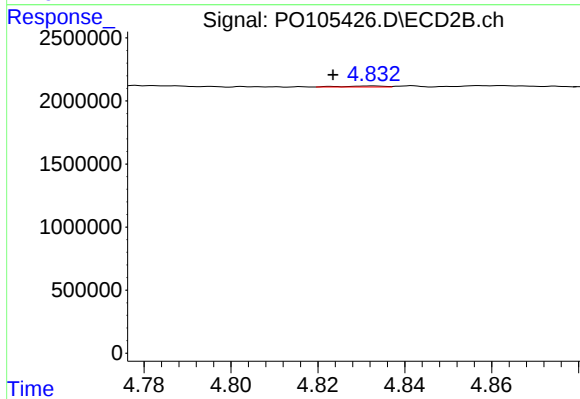

#6 AR-1016-4


R.T.: 4.832 min
Delta R.T.: 0.009 min
Response: 56466
Conc: 0.84 ng/ml

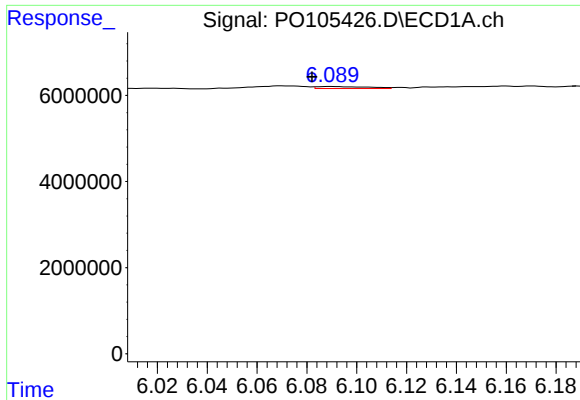

#7 AR-1016-5


R.T.: 6.089 min
Delta R.T.: 0.007 min
Response: 663378
Conc: 3.10 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

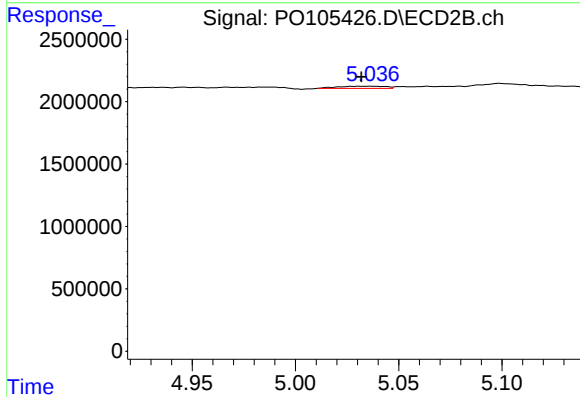


#7 AR-1016-5

R.T.: 5.037 min
Delta R.T.: 0.005 min
Response: 291362
Conc: 3.48 ng/ml

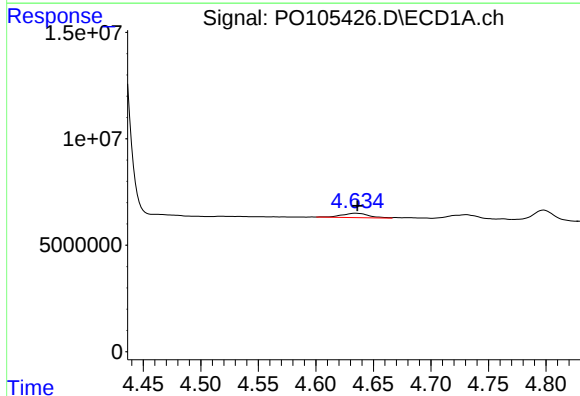


#8 AR-1221-1

R.T.: 4.635 min
Delta R.T.: -0.002 min
Response: 3354580
Conc: 29.91 ng/ml

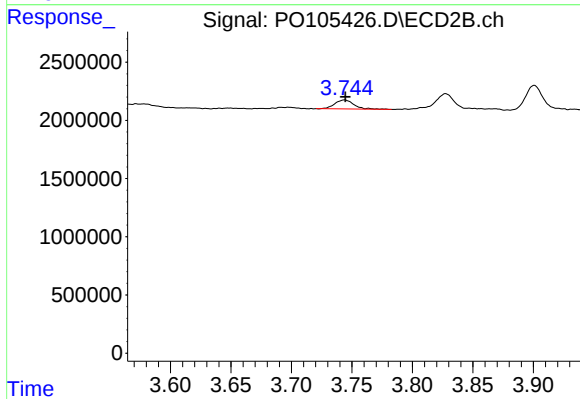

#8 AR-1221-1


R.T.: 3.744 min
Delta R.T.: 0.000 min
Response: 842947
Conc: 21.36 ng/ml

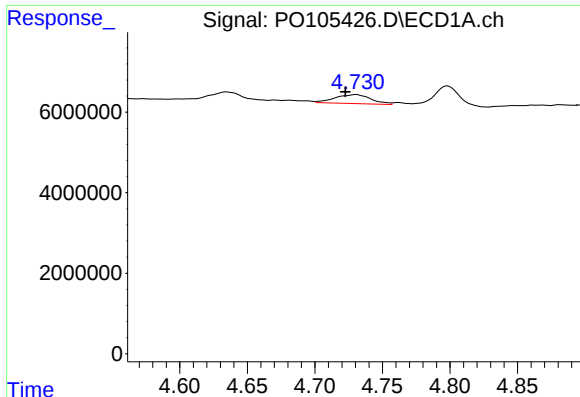

#9 AR-1221-2


R.T.: 4.730 min
Delta R.T.: 0.008 min
Response: 4117075
Conc: 48.57 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

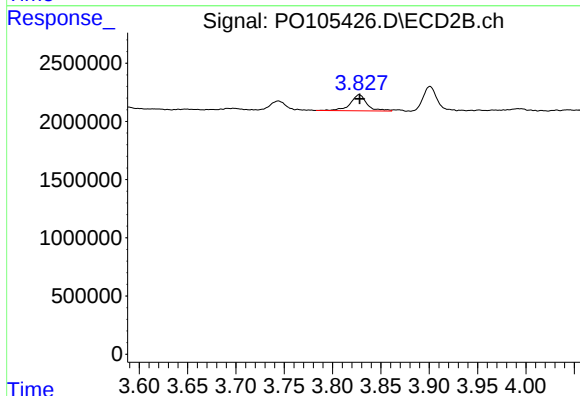


#9 AR-1221-2

R.T.: 3.828 min
Delta R.T.: 0.000 min
Response: 1650910
Conc: 53.74 ng/ml

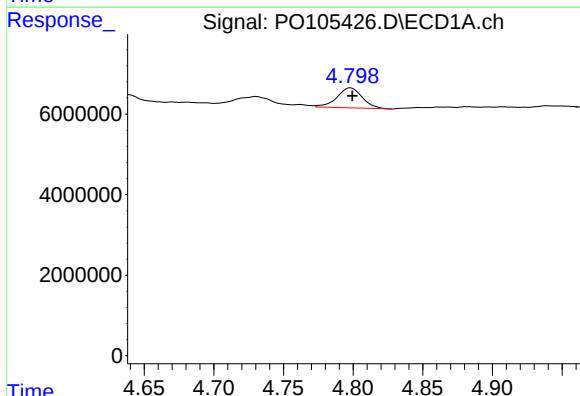


#10 AR-1221-3

R.T.: 4.798 min
Delta R.T.: -0.001 min
Response: 6313761
Conc: 25.95 ng/ml

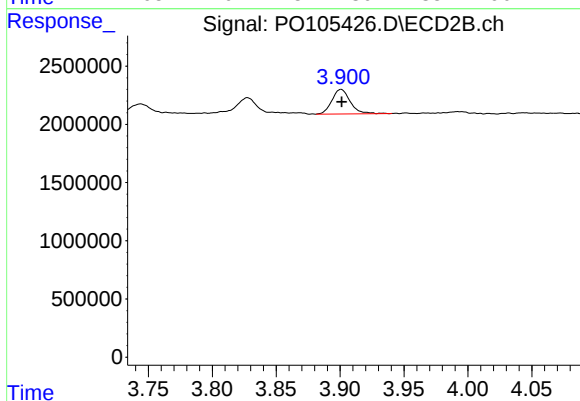

#10 AR-1221-3


R.T.: 3.901 min
Delta R.T.: 0.000 min
Response: 2095144
Conc: 23.41 ng/ml

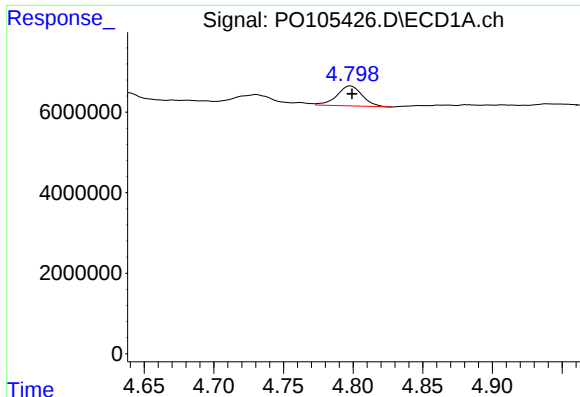

#11 AR-1232-1


R.T.: 4.798 min
Delta R.T.: 0.000 min
Response: 6313761
Conc: 31.58 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

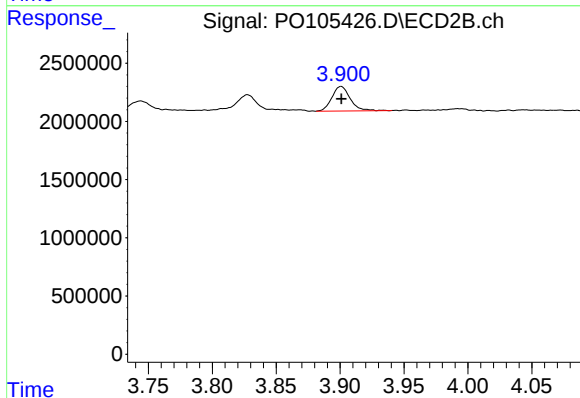


#11 AR-1232-1

R.T.: 3.901 min
Delta R.T.: 0.000 min
Response: 2095144
Conc: 28.69 ng/ml

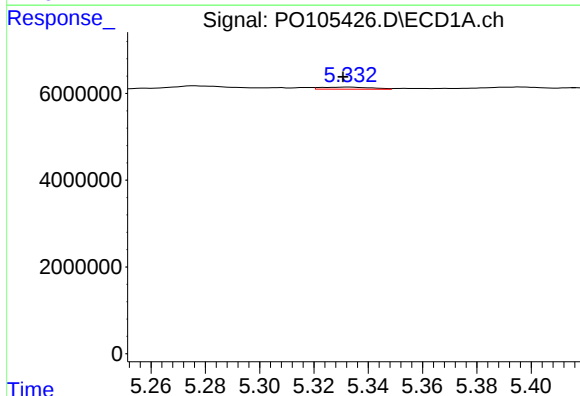


#12 AR-1232-2

R.T.: 5.333 min
Delta R.T.: 0.002 min
Response: 611681
Conc: 5.78 ng/ml

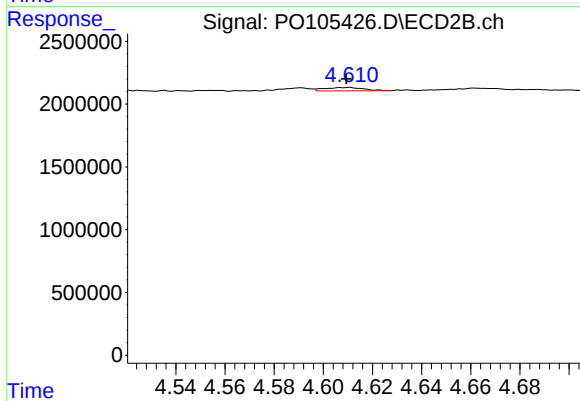

#12 AR-1232-2


R.T.: 4.610 min
Delta R.T.: 0.000 min
Response: 309796
Conc: 4.41 ng/ml

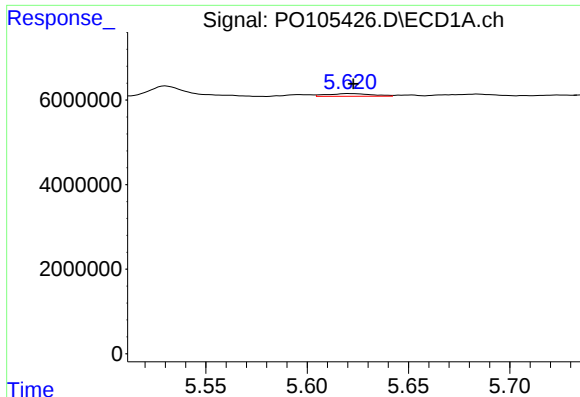

#13 AR-1232-3


R.T.: 5.621 min
Delta R.T.: -0.002 min
Response: 966730
Conc: 5.05 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

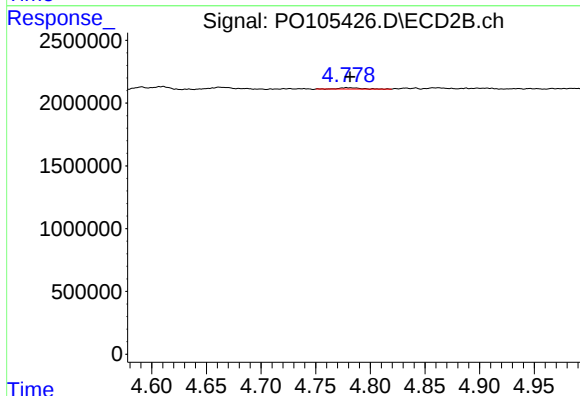


#13 AR-1232-3

R.T.: 4.778 min
Delta R.T.: -0.003 min
Response: 138600
Conc: 3.63 ng/ml

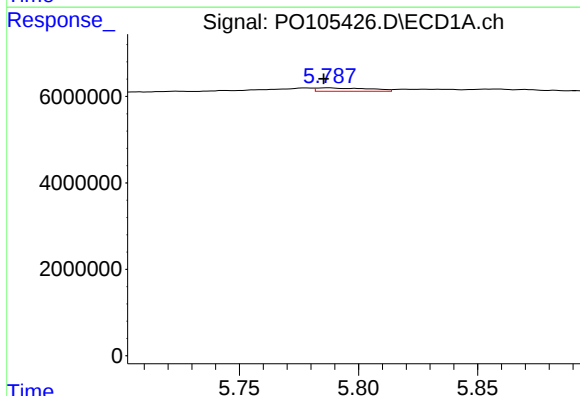


#14 AR-1232-4

R.T.: 5.787 min
Delta R.T.: 0.002 min
Response: 1212765
Conc: 12.43 ng/ml

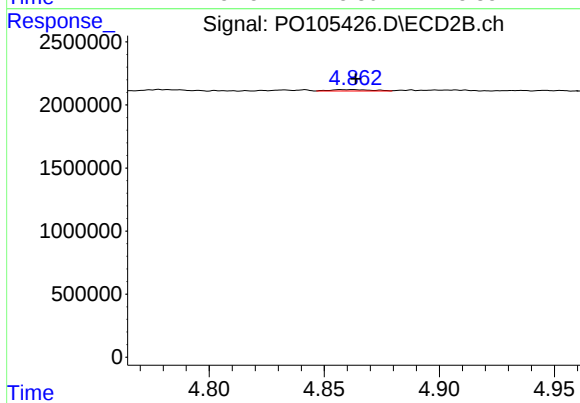

#14 AR-1232-4


R.T.: 4.862 min
Delta R.T.: -0.001 min
Response: 139476
Conc: 4.01 ng/ml

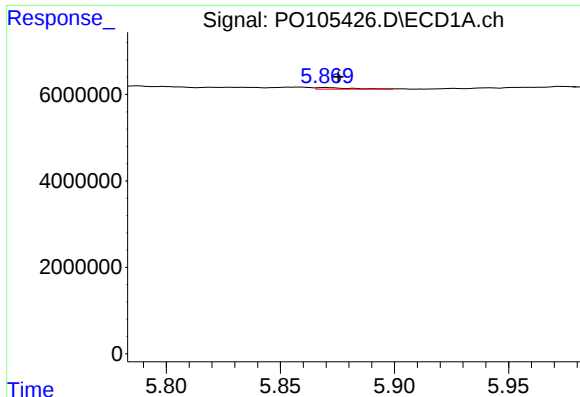

#15 AR-1232-5


R.T.: 5.870 min
Delta R.T.: -0.006 min
Response: 392834
Conc: 5.45 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

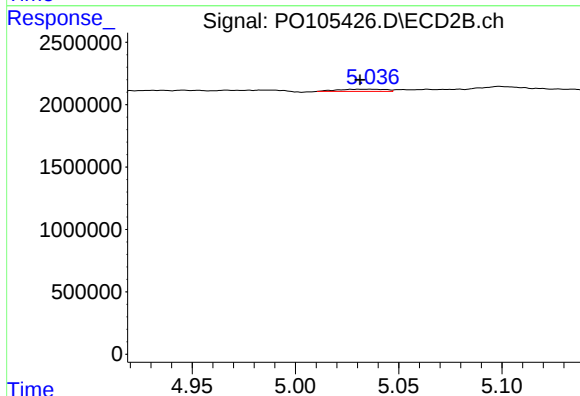


#15 AR-1232-5

R.T.: 5.037 min
Delta R.T.: 0.005 min
Response: 291362
Conc: 8.25 ng/ml

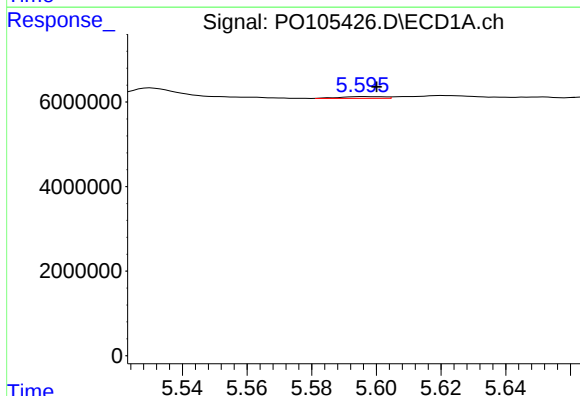


#16 AR-1242-1

R.T.: 5.596 min
Delta R.T.: -0.004 min
Response: 404512
Conc: 1.74 ng/ml

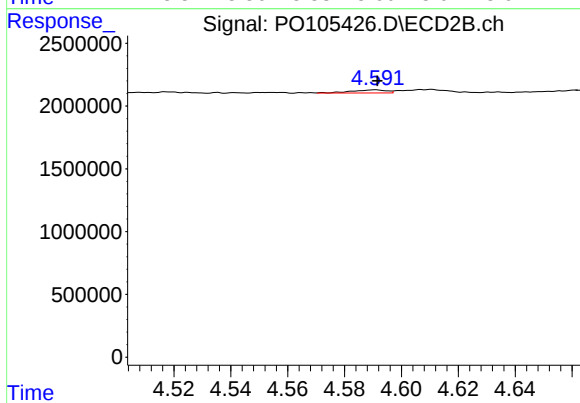

#16 AR-1242-1


R.T.: 4.591 min
Delta R.T.: 0.000 min
Response: 215153
Conc: 2.44 ng/ml

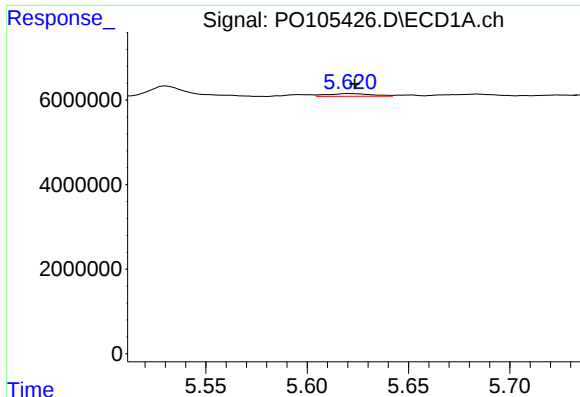

#17 AR-1242-2


R.T.: 5.621 min
Delta R.T.: -0.002 min
Response: 966730
Conc: 2.97 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

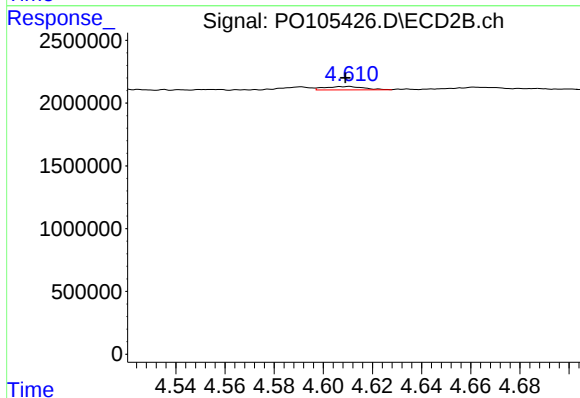


#17 AR-1242-2

R.T.: 4.610 min
Delta R.T.: 0.000 min
Response: 309796
Conc: 2.61 ng/ml

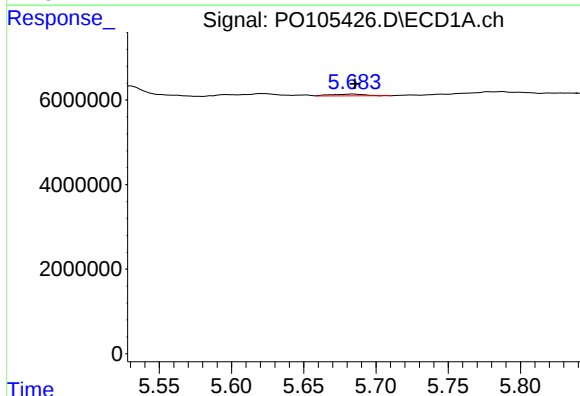


#18 AR-1242-3

R.T.: 5.684 min
Delta R.T.: -0.001 min
Response: 676761
Conc: 3.43 ng/ml

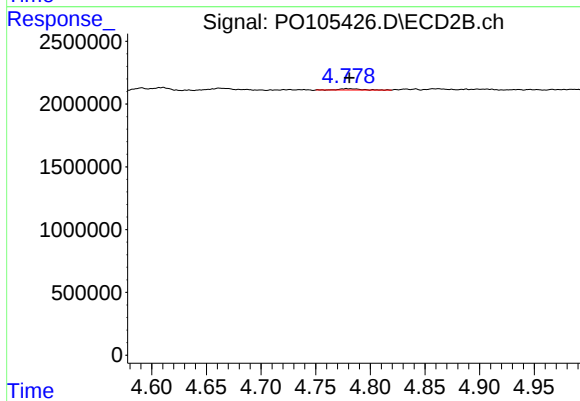

#18 AR-1242-3


R.T.: 4.778 min
Delta R.T.: -0.002 min
Response: 138600
Conc: 2.13 ng/ml

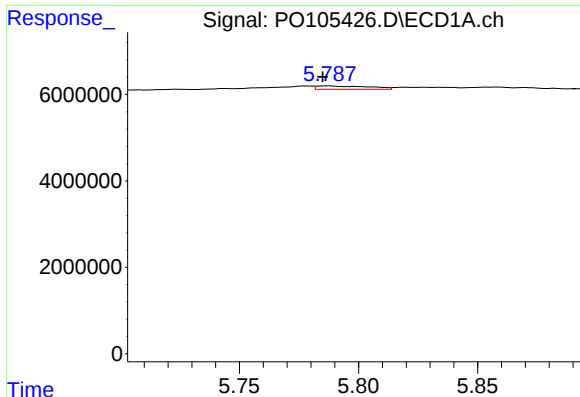

#19 AR-1242-4


R.T.: 5.787 min
Delta R.T.: 0.002 min
Response: 1212765
Conc: 7.11 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

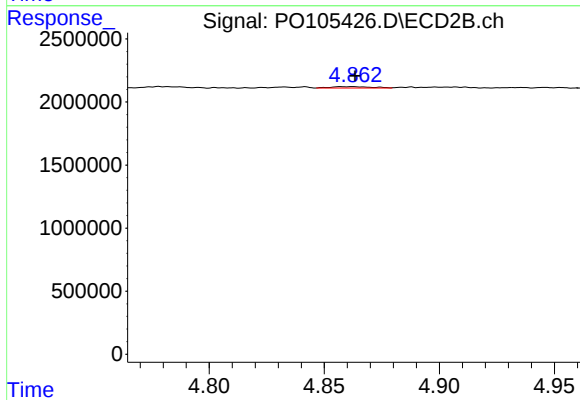


#19 AR-1242-4

R.T.: 4.862 min
Delta R.T.: -0.001 min
Response: 139476
Conc: 2.10 ng/ml

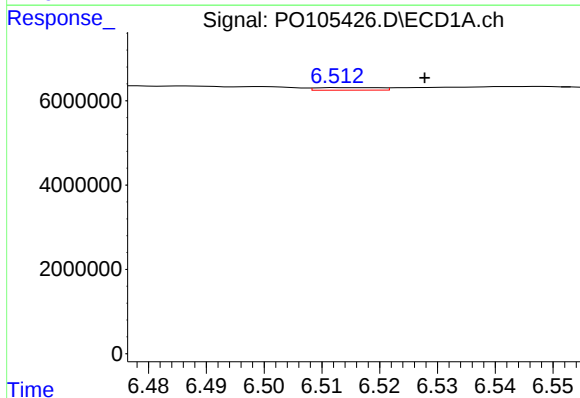


#20 AR-1242-5

R.T.: 6.514 min
Delta R.T.: -0.014 min
Response: 456446
Conc: 2.61 ng/ml

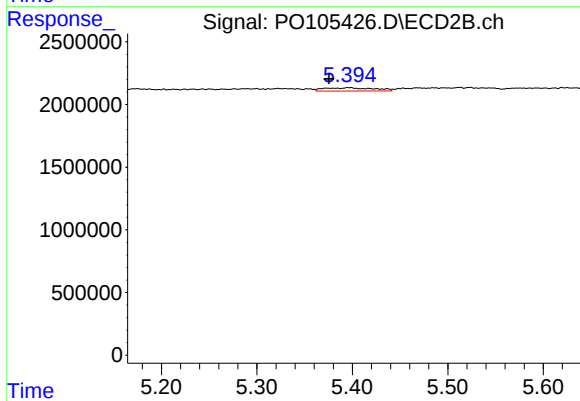

#20 AR-1242-5


R.T.: 5.398 min
Delta R.T.: 0.023 min
Response: 943507
Conc: 11.48 ng/ml

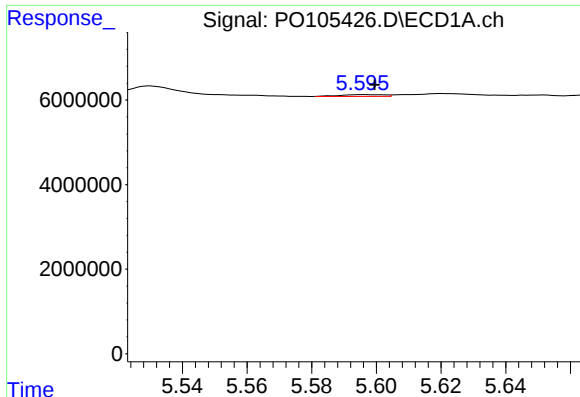

#21 AR-1248-1


R.T.: 5.596 min
Delta R.T.: -0.004 min
Response: 404512
Conc: 2.22 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

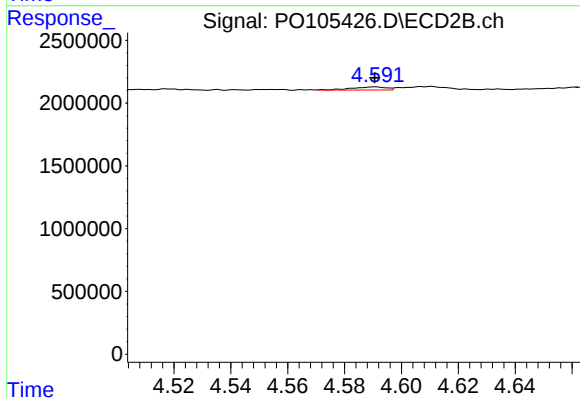


#21 AR-1248-1

R.T.: 4.591 min
Delta R.T.: 0.000 min
Response: 215153
Conc: 3.08 ng/ml

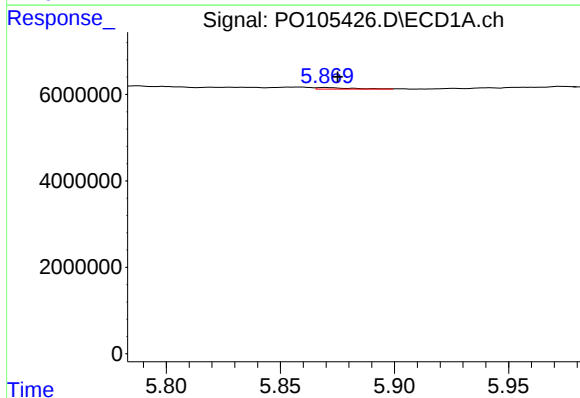


#22 AR-1248-2

R.T.: 5.870 min
Delta R.T.: -0.006 min
Response: 392834
Conc: 1.56 ng/ml

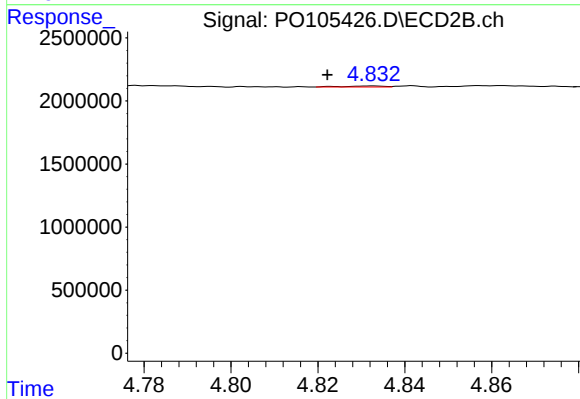

#22 AR-1248-2


R.T.: 4.832 min
Delta R.T.: 0.010 min
Response: 56466
Conc: 0.60 ng/ml

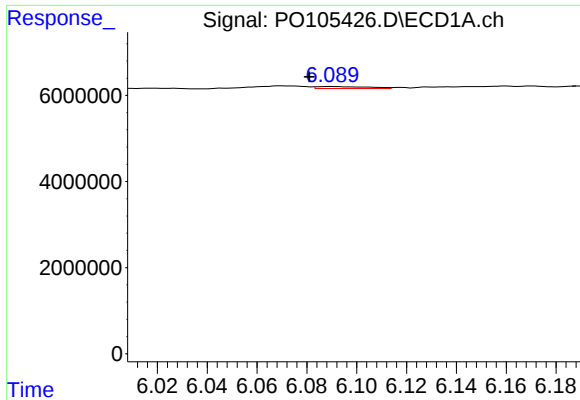

#23 AR-1248-3


R.T.: 6.089 min
Delta R.T.: 0.008 min
Response: 663378
Conc: 2.35 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

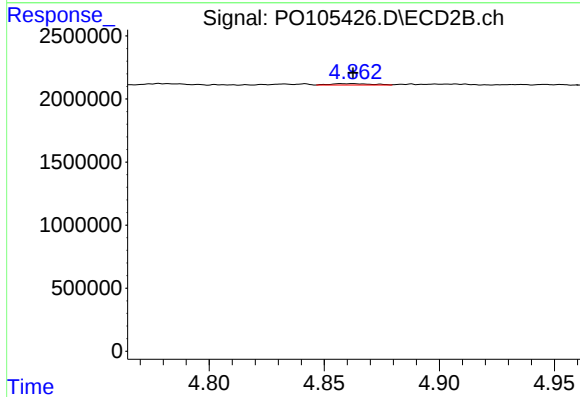


#23 AR-1248-3

R.T.: 4.862 min
Delta R.T.: 0.000 min
Response: 139476
Conc: 1.40 ng/ml

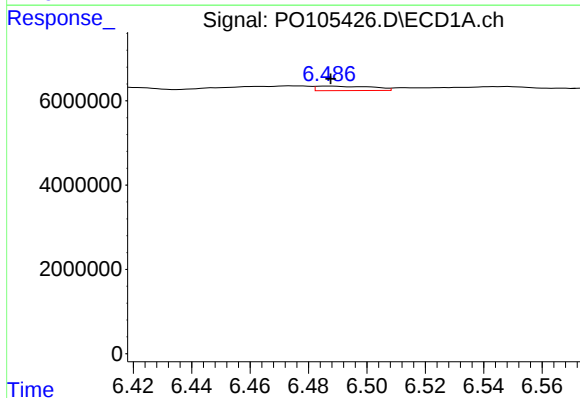


#24 AR-1248-4

R.T.: 6.487 min
Delta R.T.: 0.000 min
Response: 1393396
Conc: 4.36 ng/ml

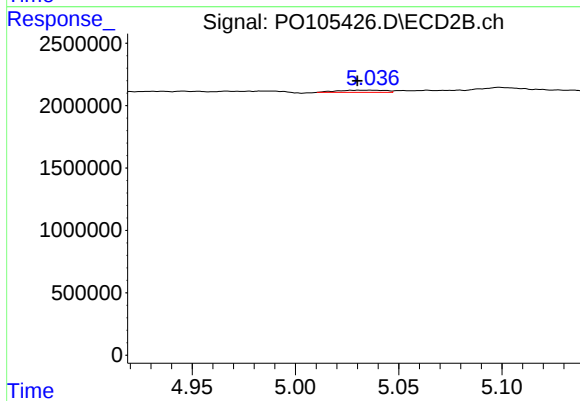

#24 AR-1248-4


R.T.: 5.037 min
Delta R.T.: 0.007 min
Response: 291362
Conc: 2.58 ng/ml

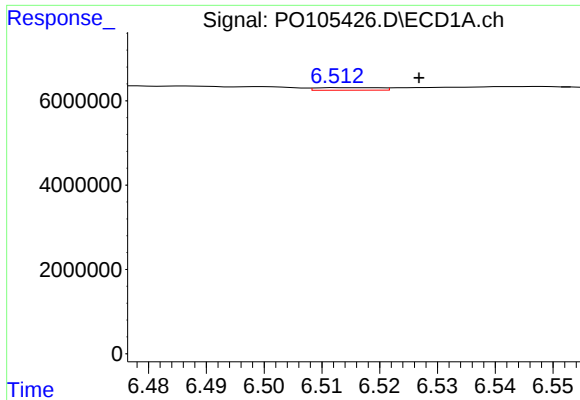

#25 AR-1248-5


R.T.: 6.514 min
Delta R.T.: -0.013 min
Response: 456446
Conc: 1.48 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

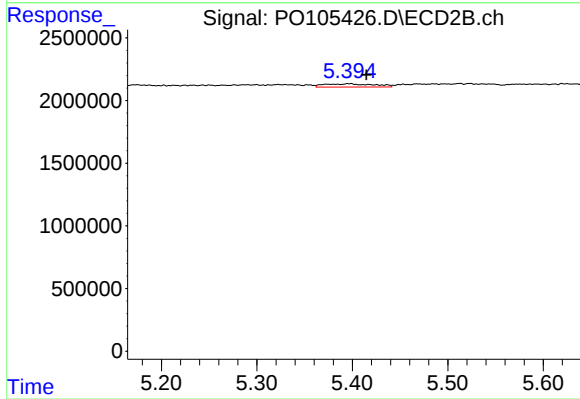


#25 AR-1248-5

R.T.: 5.398 min
Delta R.T.: -0.016 min
Response: 943507
Conc: 8.38 ng/ml

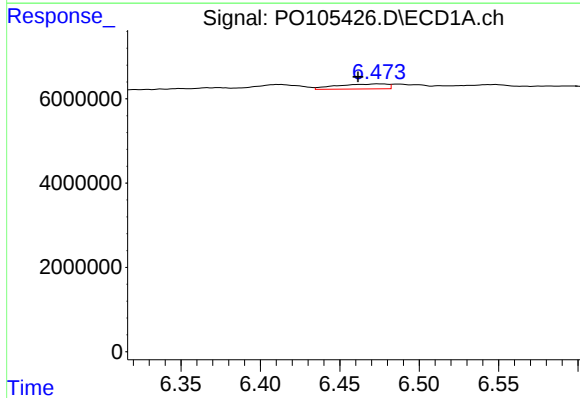


#26 AR-1254-1

R.T.: 6.474 min
Delta R.T.: 0.012 min
Response: 2658829
Conc: 8.48 ng/ml

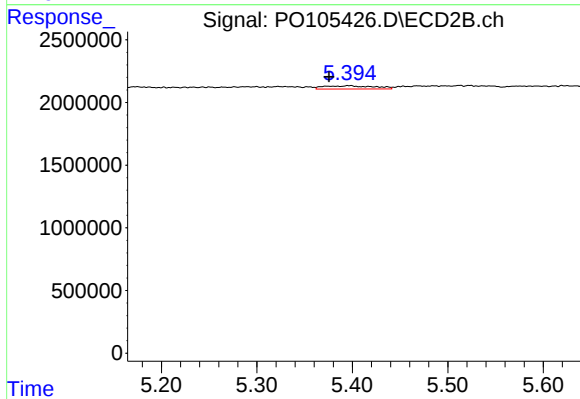

#26 AR-1254-1


R.T.: 5.398 min
Delta R.T.: 0.022 min
Response: 943507
Conc: 5.80 ng/ml

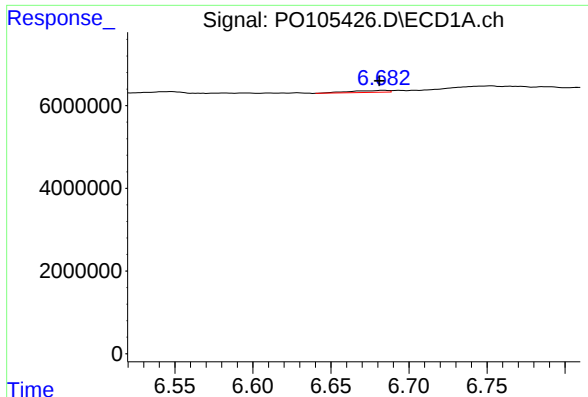

#27 AR-1254-2


R.T.: 6.683 min
Delta R.T.: 0.002 min
Response: 787868
Conc: 1.75 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

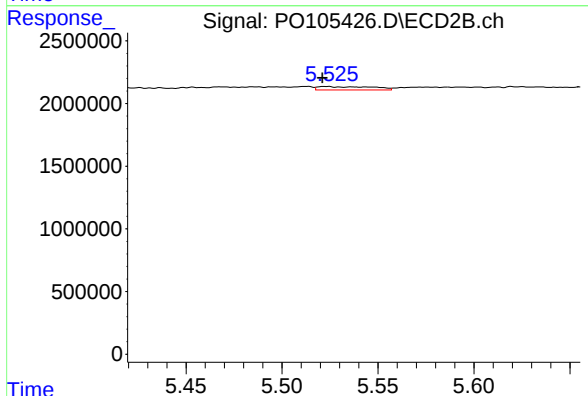


#27 AR-1254-2

R.T.: 5.523 min
Delta R.T.: 0.002 min
Response: 541424
Conc: 3.70 ng/ml

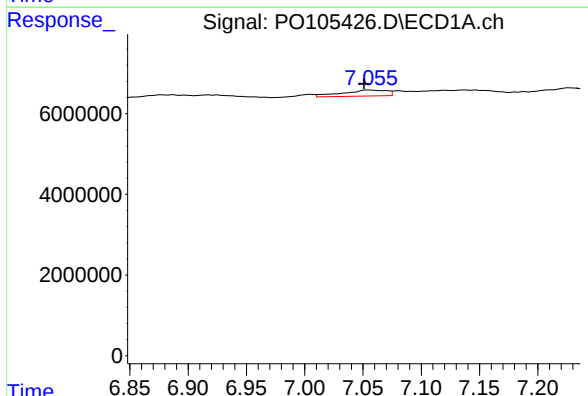


#28 AR-1254-3

R.T.: 7.055 min
Delta R.T.: 0.004 min
Response: 3913217
Conc: 8.25 ng/ml

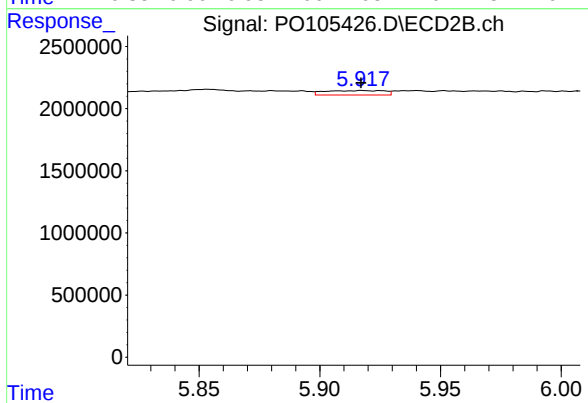

#28 AR-1254-3


R.T.: 5.918 min
Delta R.T.: 0.000 min
Response: 610498
Conc: 2.71 ng/ml

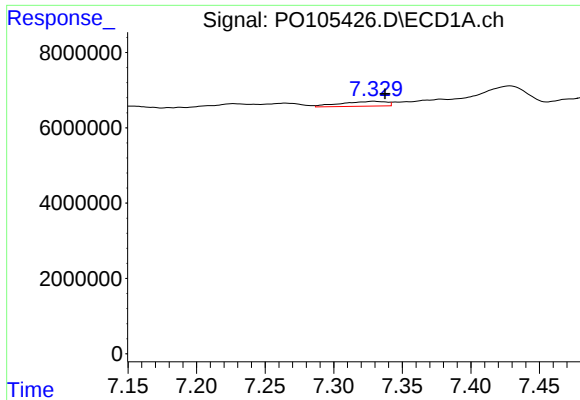

#29 AR-1254-4


R.T.: 7.329 min
Delta R.T.: -0.008 min
Response: 2977913
Conc: 8.31 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

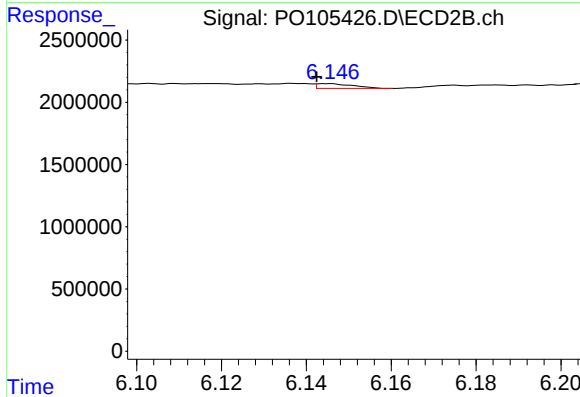


#29 AR-1254-4

R.T.: 6.144 min
Delta R.T.: 0.002 min
Response: 226830
Conc: 1.61 ng/ml

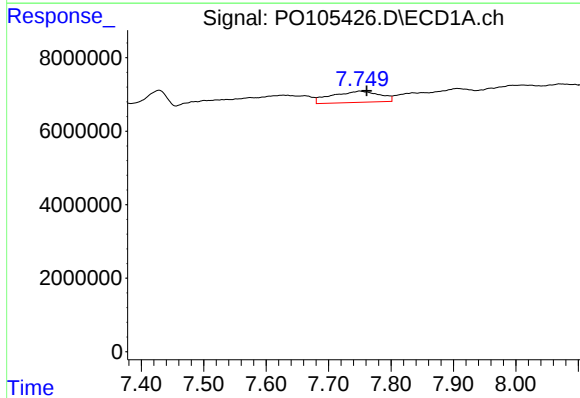


#30 AR-1254-5

R.T.: 7.750 min
Delta R.T.: -0.011 min
Response: 16125924
Conc: 40.62 ng/ml

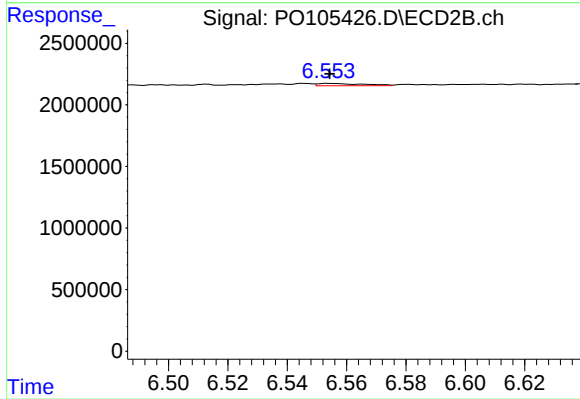

#30 AR-1254-5


R.T.: 6.554 min
Delta R.T.: 0.000 min
Response: 191970
Conc: 0.96 ng/ml

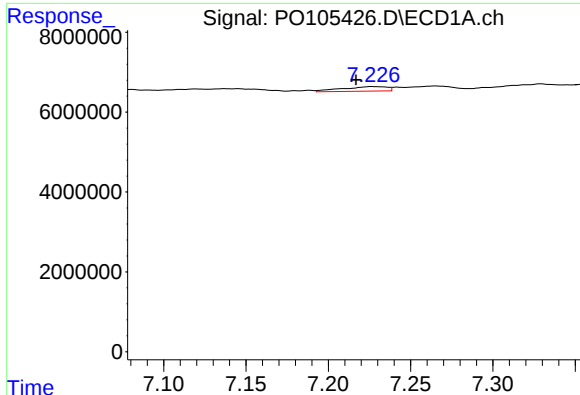

#31 AR-1260-1


R.T.: 7.227 min
Delta R.T.: 0.010 min
Response: 2224504
Conc: 6.07 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

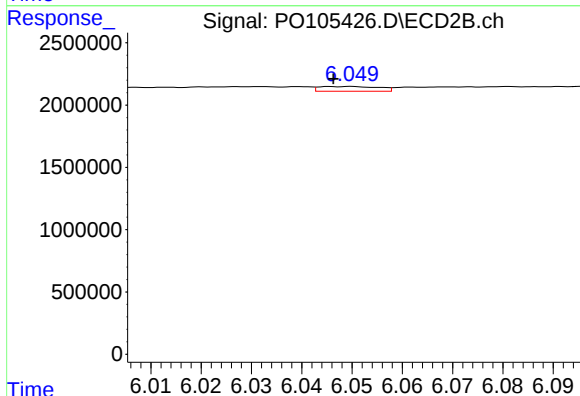


#31 AR-1260-1

R.T.: 6.050 min
Delta R.T.: 0.003 min
Response: 317628
Conc: 2.03 ng/ml

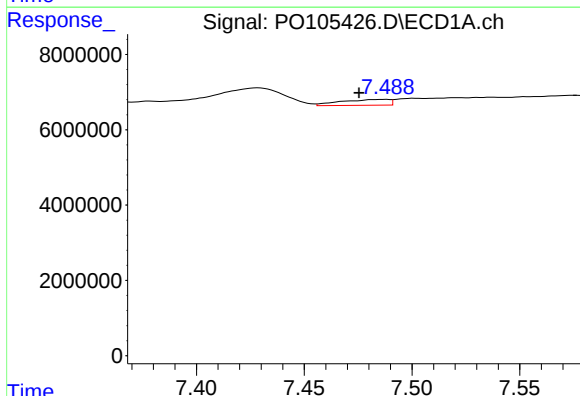


#32 AR-1260-2

R.T.: 7.488 min
Delta R.T.: 0.012 min
Response: 2391914
Conc: 5.74 ng/ml

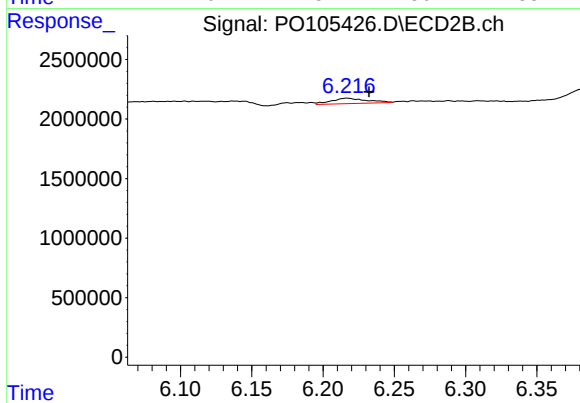

#32 AR-1260-2


R.T.: 6.217 min
Delta R.T.: -0.015 min
Response: 785774
Conc: 4.16 ng/ml

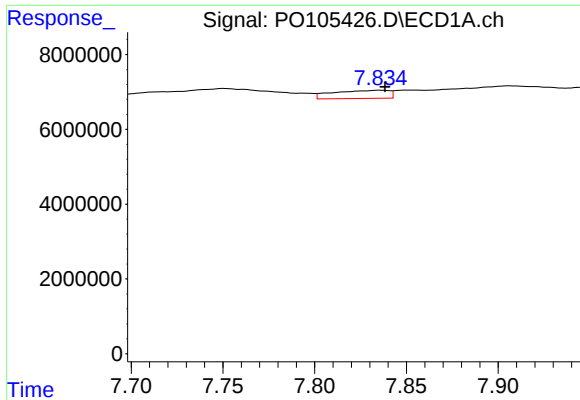

#33 AR-1260-3


R.T.: 7.835 min
Delta R.T.: -0.003 min
Response: 4615393
Conc: 17.83 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

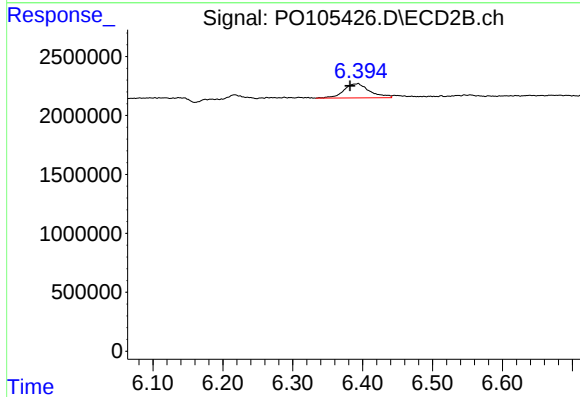


#33 AR-1260-3

R.T.: 6.393 min
Delta R.T.: 0.011 min
Response: 3066125
Conc: 16.60 ng/ml

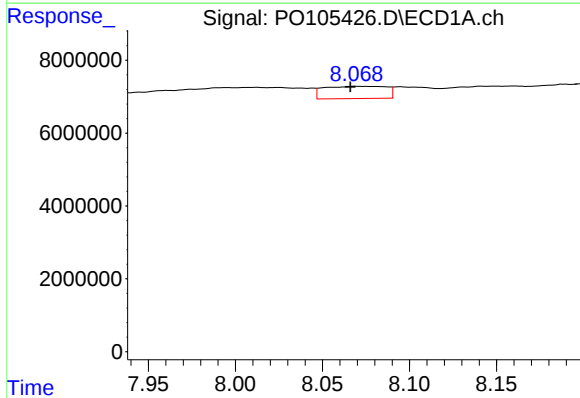


#34 AR-1260-4

R.T.: 8.069 min
Delta R.T.: 0.003 min
Response: 8371700
Conc: 25.37 ng/ml

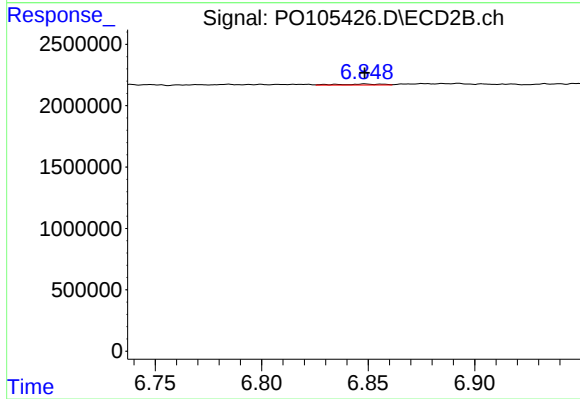

#34 AR-1260-4


R.T.: 6.849 min
Delta R.T.: 0.000 min
Response: 127912
Conc: 1.05 ng/ml

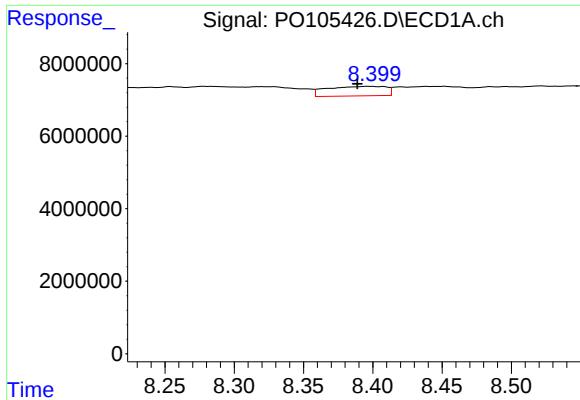

#35 AR-1260-5


R.T.: 8.398 min
Delta R.T.: 0.009 min
Response: 7784661
Conc: 13.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

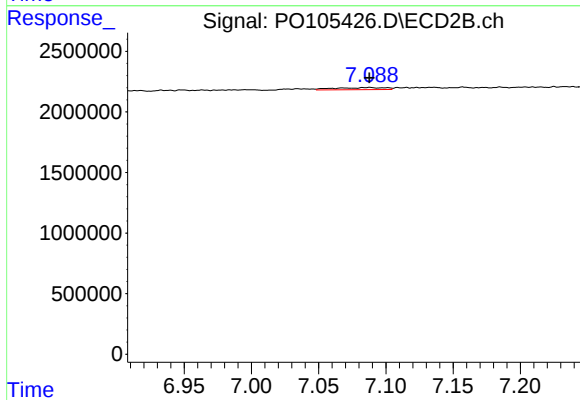


#35 AR-1260-5

R.T.: 7.087 min
Delta R.T.: 0.000 min
Response: 452163
Conc: 1.62 ng/ml

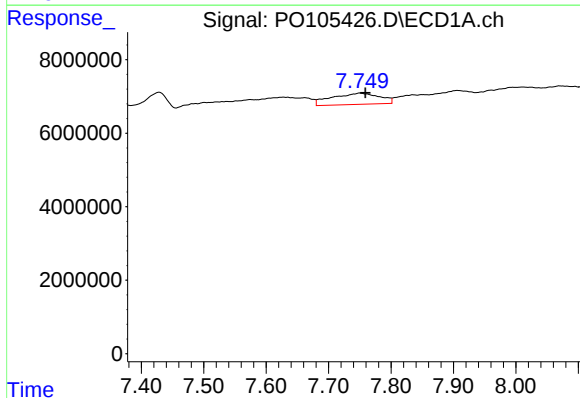


#36 AR-1262-1

R.T.: 7.750 min
Delta R.T.: -0.009 min
Response: 16125924
Conc: 50.77 ng/ml

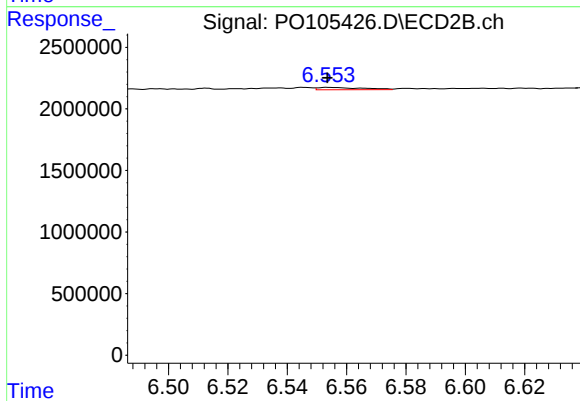

#36 AR-1262-1


R.T.: 6.554 min
Delta R.T.: 0.000 min
Response: 191970
Conc: 1.80 ng/ml

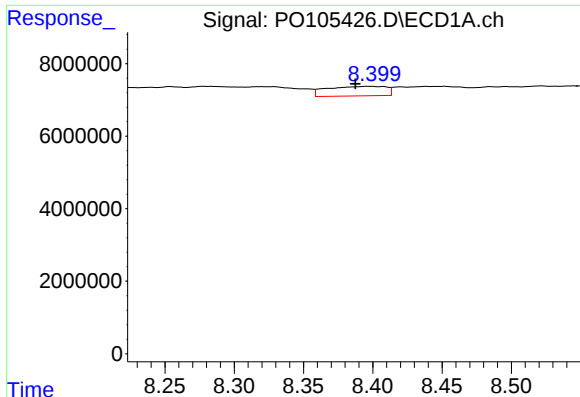

#37 AR-1262-2


R.T.: 8.398 min
Delta R.T.: 0.010 min
Response: 7784661
Conc: 10.35 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

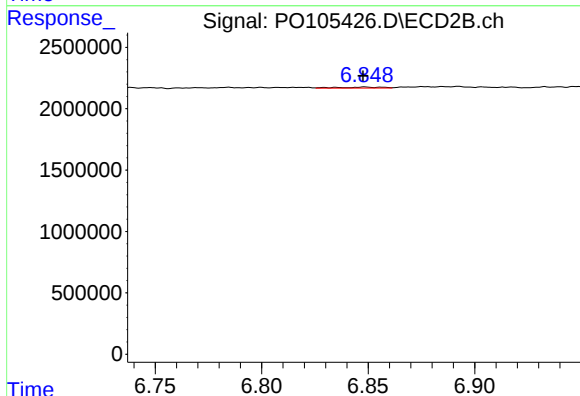


#37 AR-1262-2

R.T.: 6.849 min
Delta R.T.: 0.001 min
Response: 127912
Conc: 0.75 ng/ml

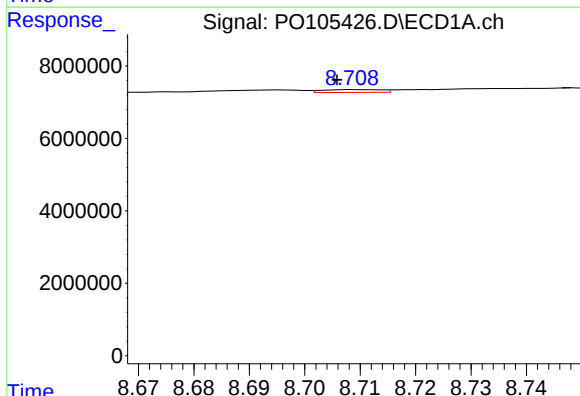


#38 AR-1262-3

R.T.: 8.709 min
Delta R.T.: 0.003 min
Response: 573949
Conc: 1.17 ng/ml

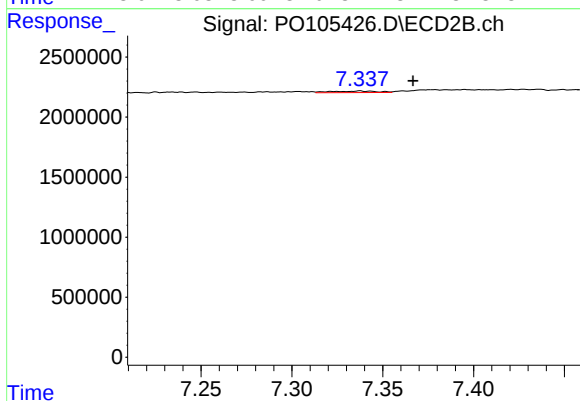

#38 AR-1262-3


R.T.: 7.338 min
Delta R.T.: -0.029 min
Response: 232531
Conc: 1.84 ng/ml

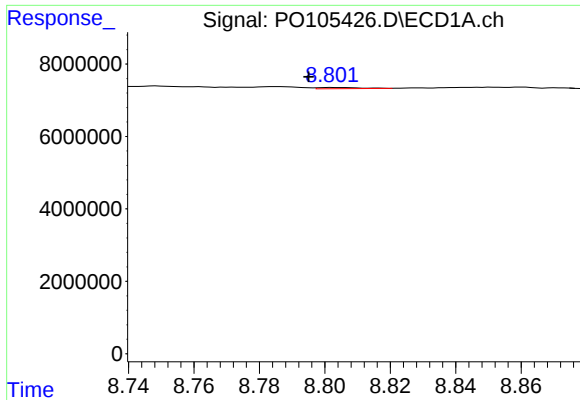

#39 AR-1262-4


R.T.: 8.803 min
Delta R.T.: 0.008 min
Response: 284609
Conc: 0.78 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

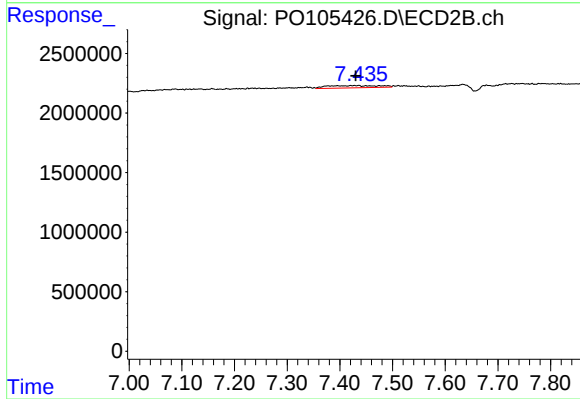


#39 AR-1262-4

R.T.: 7.428 min
Delta R.T.: -0.001 min
Response: 1327252
Conc: 5.73 ng/ml

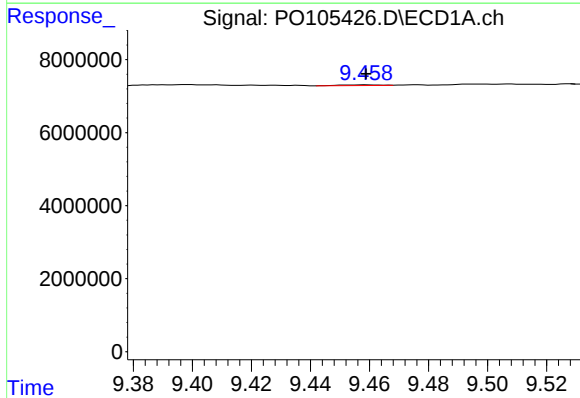


#40 AR-1262-5

R.T.: 9.459 min
Delta R.T.: 0.000 min
Response: 167705
Conc: 0.63 ng/ml

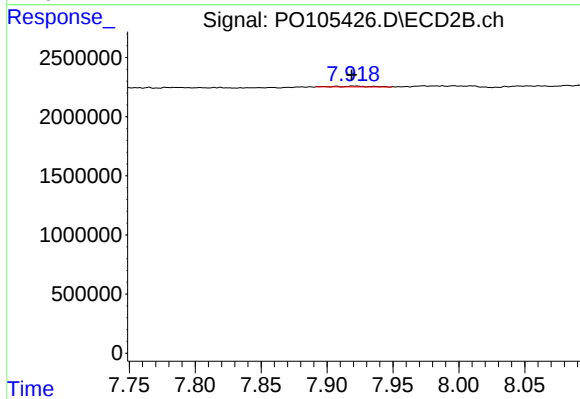

#40 AR-1262-5


R.T.: 7.921 min
Delta R.T.: 0.002 min
Response: 105313
Conc: 1.05 ng/ml

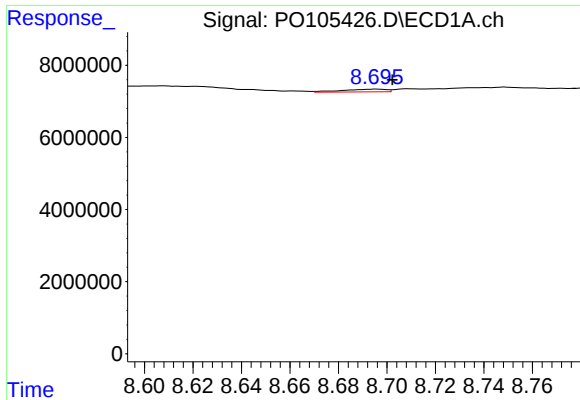

#41 AR-1268-1


R.T.: 8.696 min
Delta R.T.: -0.007 min
Response: 961870
Conc: 1.18 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

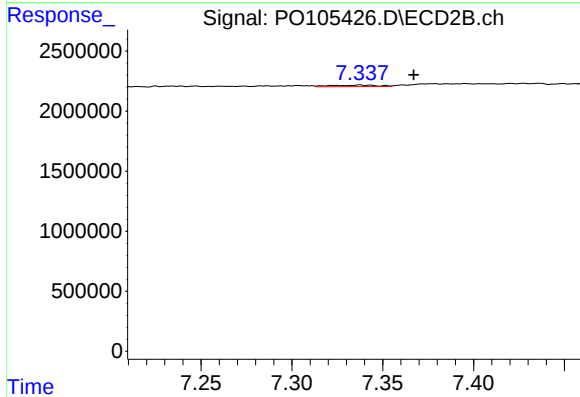


#41 AR-1268-1

R.T.: 7.338 min
Delta R.T.: -0.029 min
Response: 232531
Conc: 0.67 ng/ml

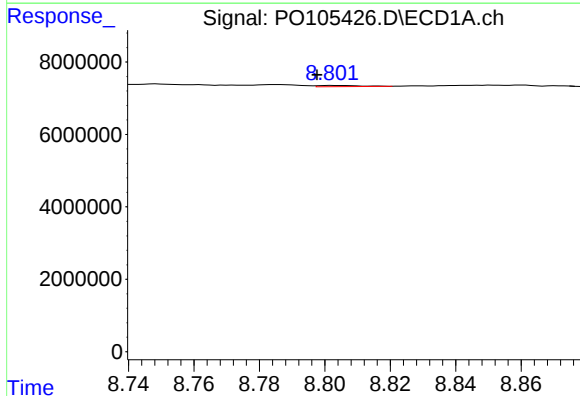


#42 AR-1268-2

R.T.: 8.803 min
Delta R.T.: 0.005 min
Response: 284609
Conc: 0.39 ng/ml

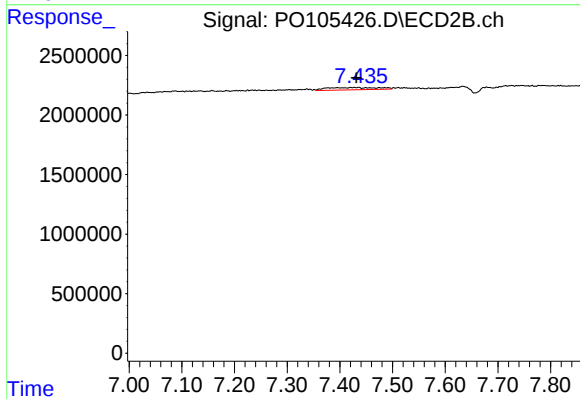

#42 AR-1268-2


R.T.: 7.428 min
Delta R.T.: -0.003 min
Response: 1327252
Conc: 4.25 ng/ml

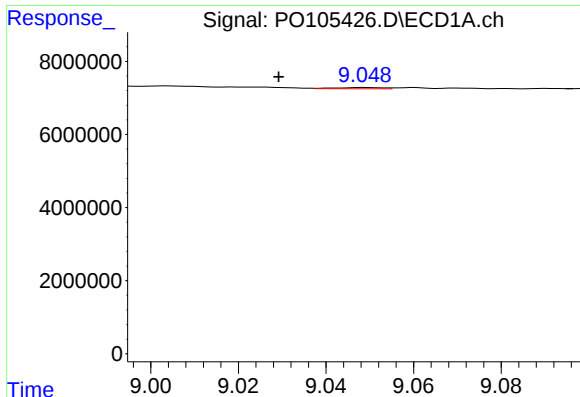

#43 AR-1268-3


R.T.: 9.049 min
Delta R.T.: 0.020 min
Response: 289469
Conc: 0.45 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

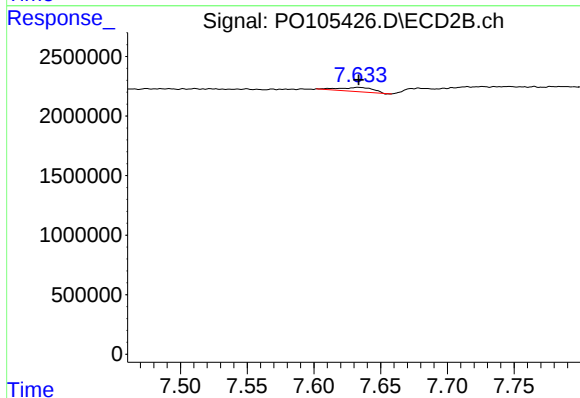


#43 AR-1268-3

R.T.: 7.633 min
Delta R.T.: 0.000 min
Response: 615168
Conc: 2.43 ng/ml

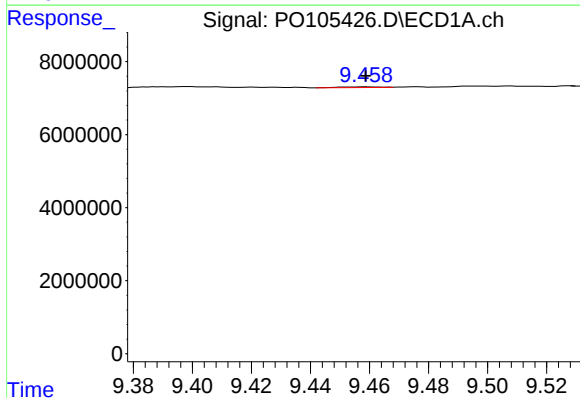


#44 AR-1268-4

R.T.: 9.459 min
Delta R.T.: 0.000 min
Response: 167705
Conc: 0.60 ng/ml

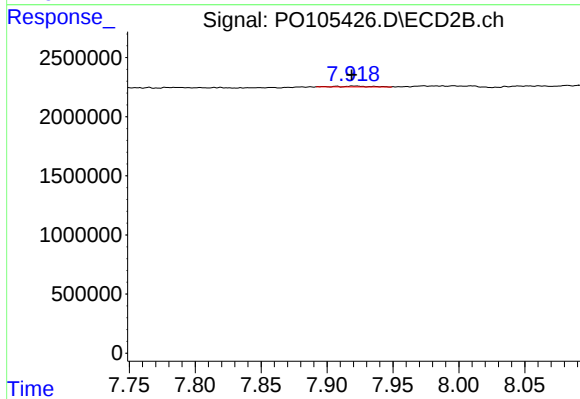

#44 AR-1268-4


R.T.: 7.921 min
Delta R.T.: 0.002 min
Response: 105313
Conc: 0.98 ng/ml

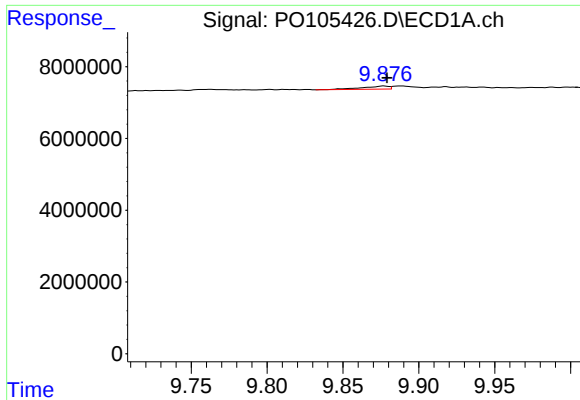

#45 AR-1268-5

R.T.: 9.877 min
Delta R.T.: -0.002 min
Response: 1064758
Conc: 0.51 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

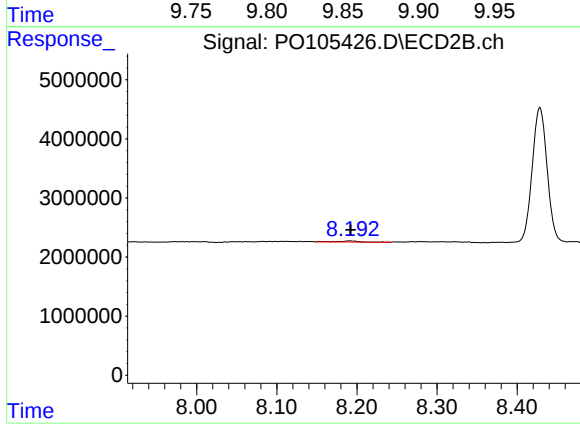

#45 AR-1268-5

R.T.: 8.191 min
Delta R.T.: -0.001 min
Response: 362358
Conc: 0.54 ng/ml