

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081224\
 Data File : P0105430.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2024 18:43
 Operator : YP/AJ
 Sample : P3390-07
 Misc : AR1254 LOD 25 PPB
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 02:31:58 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081024.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 10 04:08:56 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.428	3.536	119.5E6	42631394	13.682	13.573
2)	SA Decachlor...	10.219	8.428	87142843	26042173	15.149	14.710
Target Compounds							
3)	L1 AR-1016-1	5.599	4.592	71167	97314	0.235	0.866 #
4)	L1 AR-1016-2	5.614	4.611	253944	63158	0.594	0.406 #
5)	L1 AR-1016-3	5.681	4.779	151601	50022	0.591	0.597
6)	L1 AR-1016-4	5.785	4.822	1462136	1531096	6.685	22.737 #
7)	L1 AR-1016-5	6.081	5.030	2931575	1026092	13.702	12.260
8)	L2 AR-1221-1	4.634	3.757	437401	21519	3.900	0.545 #
9)	L2 AR-1221-2	4.734	3.827	2509690	808924	29.609	26.330
10)	L2 AR-1221-3	4.772	3.901	1187175	37143	4.880	0.415 #
11)	L3 AR-1232-1	4.772	3.901	1187175	37143	5.938	0.509 #
12)	L3 AR-1232-2	5.325	4.611	279541	63158	2.641	0.900 #
13)	L3 AR-1232-3	5.614	4.779	253944	50022	1.327	1.309
14)	L3 AR-1232-4	5.785	4.863	1462136	476450	14.991	13.695
15)	L3 AR-1232-5	5.874	5.030	3601700	1026092	49.980	29.069 #
16)	L4 AR-1242-1	5.599	4.592	71167	97314	0.306	1.103 #
17)	L4 AR-1242-2	5.614	4.611	253944	63158	0.779	0.532 #
18)	L4 AR-1242-3	5.681	4.779	151601	50022	0.768	0.770
19)	L4 AR-1242-4	5.785	4.863	1462136	476450	8.569	7.184
20)	L4 AR-1242-5	6.528	5.375	3896543	3683990	22.296	44.832 #
21)	L5 AR-1248-1	5.599	4.592	71167	97314	0.390	1.393 #
22)	L5 AR-1248-2	5.874	4.822	3601700	1531096	14.300	16.134
23)	L5 AR-1248-3	6.081	4.863	2931575	476450	10.371	4.773 #
24)	L5 AR-1248-4	6.486	5.030	4055539	1026092	12.684	9.091 #
25)	L5 AR-1248-5	6.528	5.415	3896543	486997	12.597	4.325 #
26)	L6 AR-1254-1	6.461	5.375	7601536	3683990	24.240	22.628
27)	L6 AR-1254-2	6.681	5.520	8940074	3331119	19.811	22.772
28)	L6 AR-1254-3	7.050	5.917	10824682	4987605	22.819	22.111
29)	L6 AR-1254-4	7.337	6.142	7974602	3098786	22.262	21.960
30)	L6 AR-1254-5	7.760	6.554	17396666	4272264	43.824	21.325 #
31)	L7 AR-1260-1	7.218	6.045	3564115	2857501	9.724	18.306 #
32)	L7 AR-1260-2	7.474	6.231	4978546	2170524	11.957	11.484
33)	L7 AR-1260-3	7.840	6.381	2218320	4600268	8.571	24.902 #
34)	L7 AR-1260-4	8.054	6.848	20056709	320286	60.791	2.620 #
35)	L7 AR-1260-5	8.395	7.089	5063919	668744	8.513	2.403 #
36)	L8 AR-1262-1	7.760	6.554	17396666	4272264	54.769	40.152 #
37)	L8 AR-1262-2	8.395	6.848	5063919	320286	6.732	1.885 #
38)	L8 AR-1262-3	8.720	7.369	2039497	347599	4.145	2.753 #
39)	L8 AR-1262-4	8.788	7.429	452835	980737	1.233	4.237 #
40)	L8 AR-1262-5	9.469	7.925	102825	93336	0.384	0.929 #
41)	L9 AR-1268-1	8.720	7.369	2039497	347599	2.508	0.996 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081224\
Data File : P0105430.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Aug 2024 18:43
Operator : YP/AJ
Sample : P3390-07
Misc : AR1254 LOD 25 PPB
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 13 02:31:58 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081024.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Aug 10 04:08:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42)	L9 AR-1268-2	8.788	7.429	452835	980737	0.623	3.144 #
43)	L9 AR-1268-3	9.025	7.635	822510	1034223	1.274	4.092 #
44)	L9 AR-1268-4	9.469	7.925	102825	93336	0.369	0.868 #
45)	L9 AR-1268-5	9.892	8.188	2078178	341561	0.994	0.511 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO081224\
Data File : PO105430.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Aug 2024 18:43
Operator : YP/AJ
Sample : P3390-07
Misc : AR1254 LOD 25 PPB
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_0
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 13 02:31:58 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO081024.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Aug 10 04:08:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

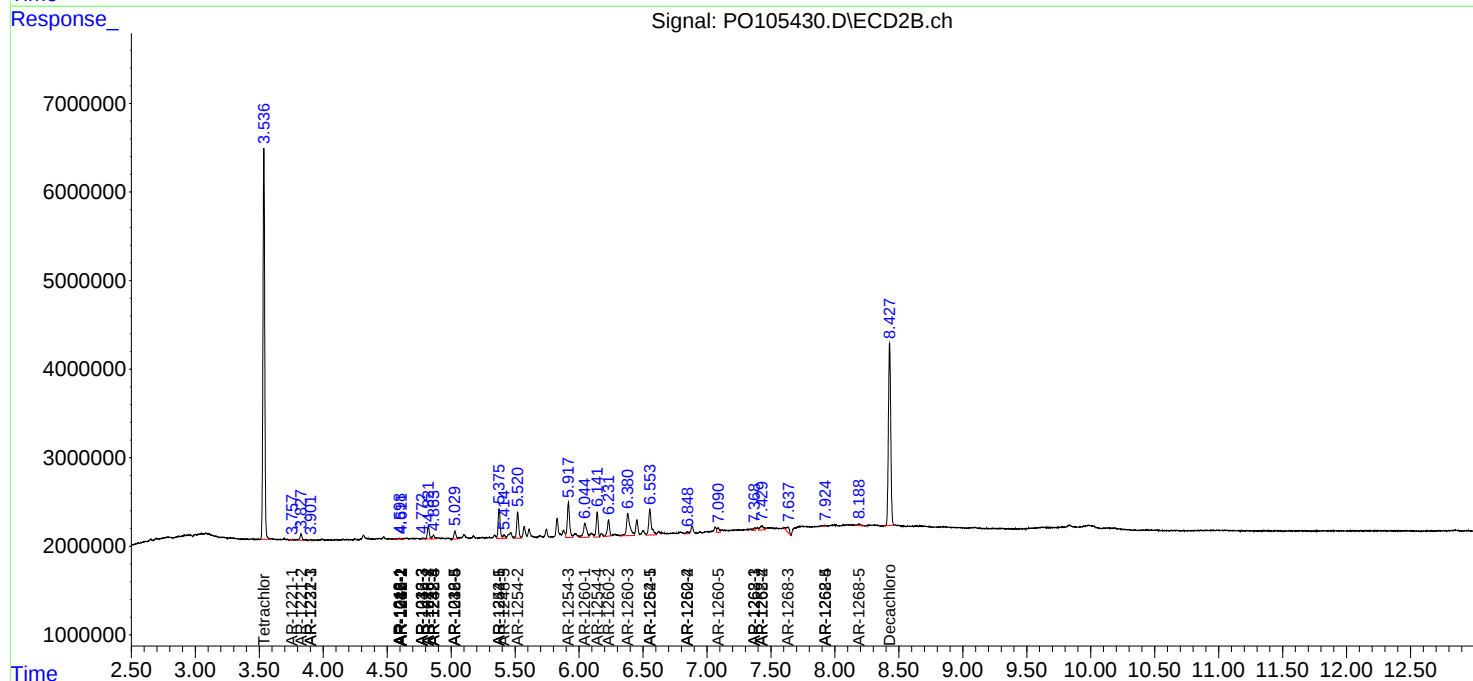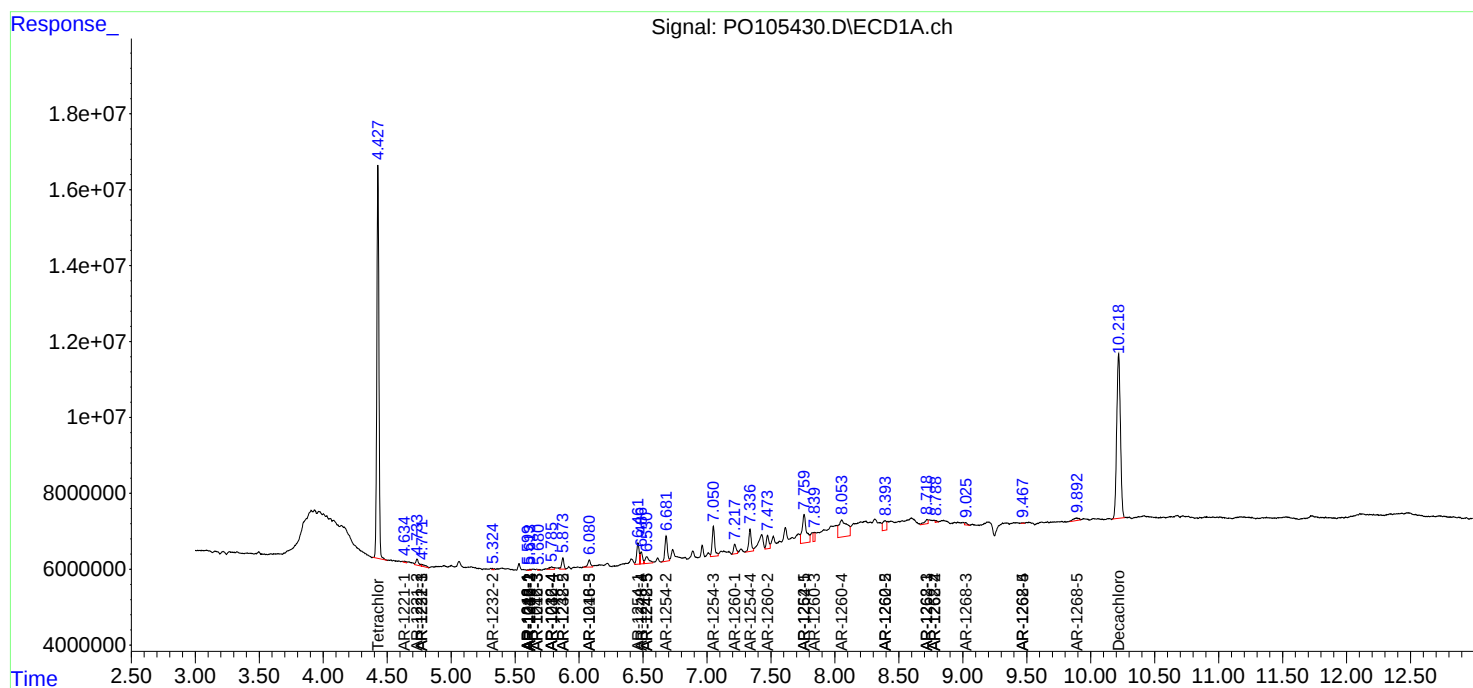


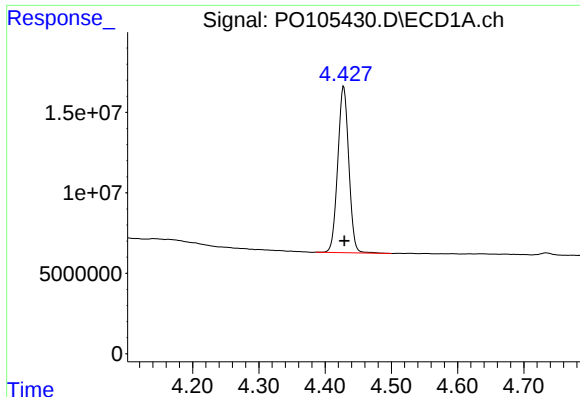

#1 Tetrachloro-m-xylene


R.T.: 4.428 min
Delta R.T.: 0.000 min
Response: 119500163
Conc: 13.68 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

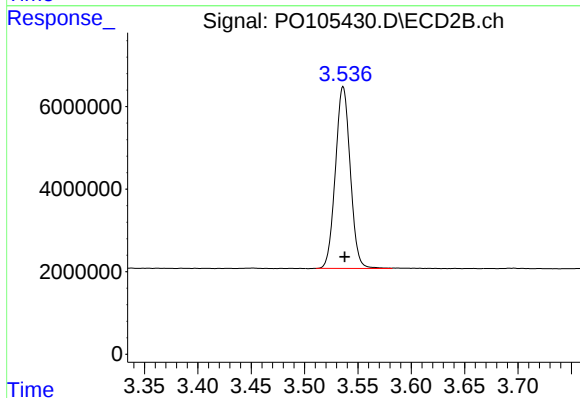


#1 Tetrachloro-m-xylene

R.T.: 3.536 min
Delta R.T.: -0.001 min
Response: 42631394
Conc: 13.57 ng/ml

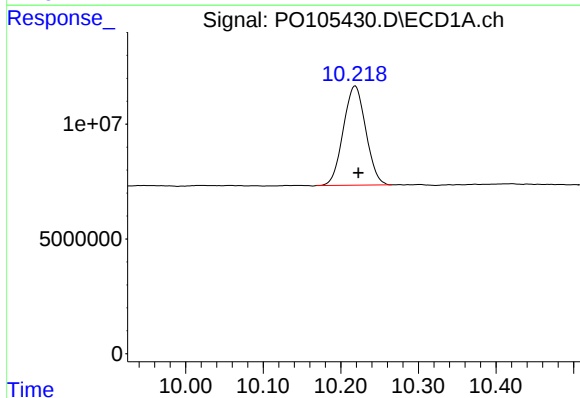


#2 Decachlorobiphenyl

R.T.: 10.219 min
Delta R.T.: -0.004 min
Response: 87142843
Conc: 15.15 ng/ml

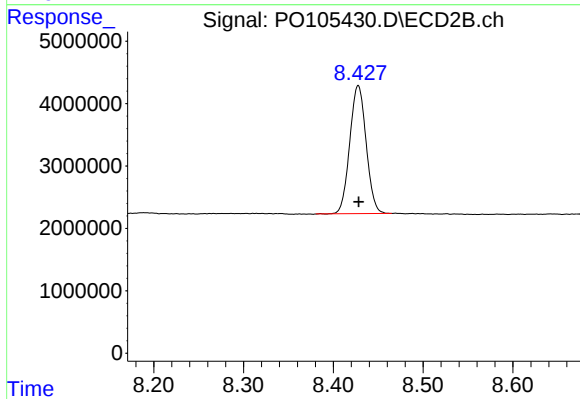

#2 Decachlorobiphenyl


R.T.: 8.428 min
Delta R.T.: 0.000 min
Response: 26042173
Conc: 14.71 ng/ml

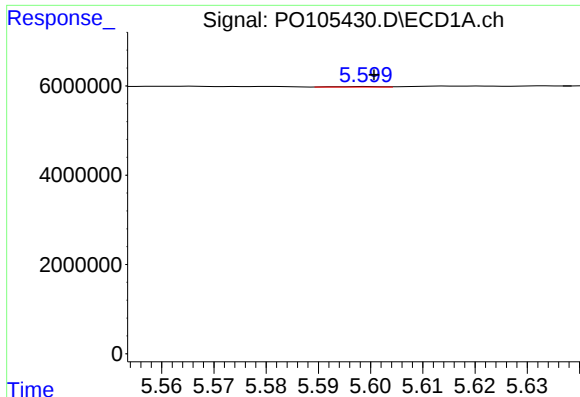

#3 AR-1016-1


R.T.: 5.599 min
Delta R.T.: -0.001 min
Response: 71167
Conc: 0.24 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

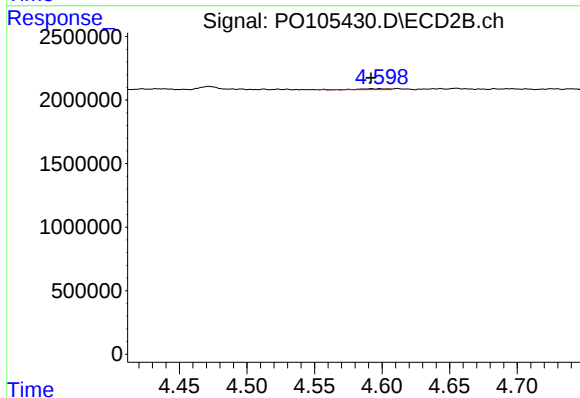


#3 AR-1016-1

R.T.: 4.592 min
Delta R.T.: 0.000 min
Response: 97314
Conc: 0.87 ng/ml

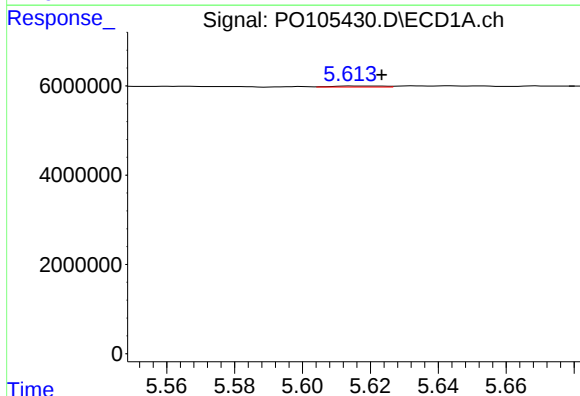


#4 AR-1016-2

R.T.: 5.614 min
Delta R.T.: -0.009 min
Response: 253944
Conc: 0.59 ng/ml

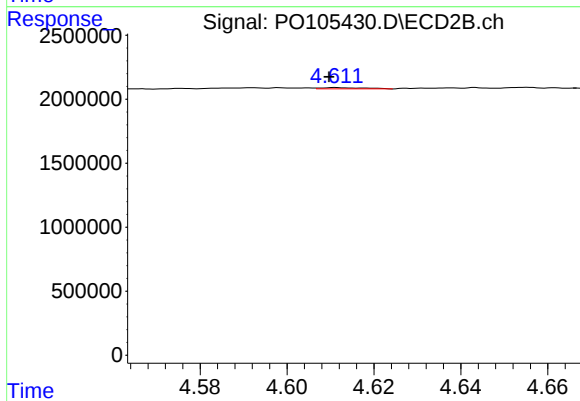

#4 AR-1016-2


R.T.: 4.611 min
Delta R.T.: 0.002 min
Response: 63158
Conc: 0.41 ng/ml

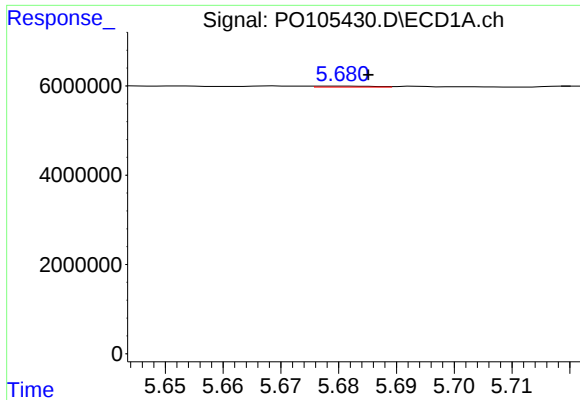

#5 AR-1016-3


R.T.: 5.681 min
Delta R.T.: -0.005 min
Response: 151601
Conc: 0.59 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

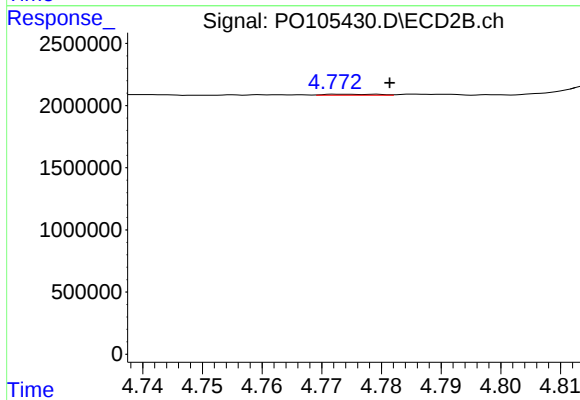


#5 AR-1016-3

R.T.: 4.779 min
Delta R.T.: -0.003 min
Response: 50022
Conc: 0.60 ng/ml

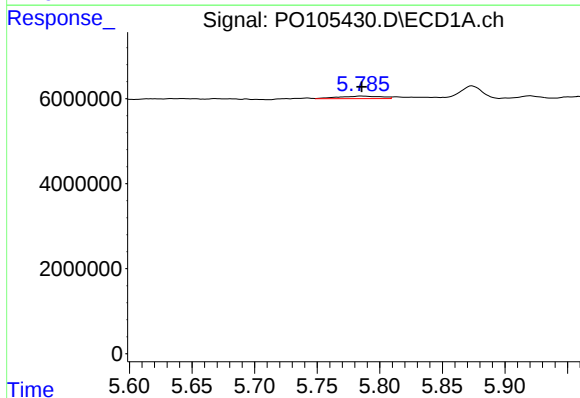


#6 AR-1016-4

R.T.: 5.785 min
Delta R.T.: 0.000 min
Response: 1462136
Conc: 6.69 ng/ml

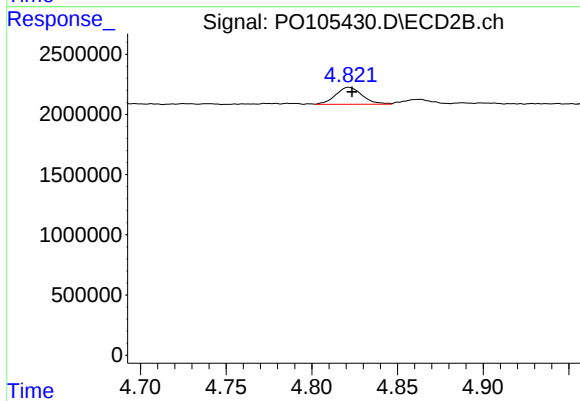

#6 AR-1016-4


R.T.: 4.822 min
Delta R.T.: -0.002 min
Response: 1531096
Conc: 22.74 ng/ml

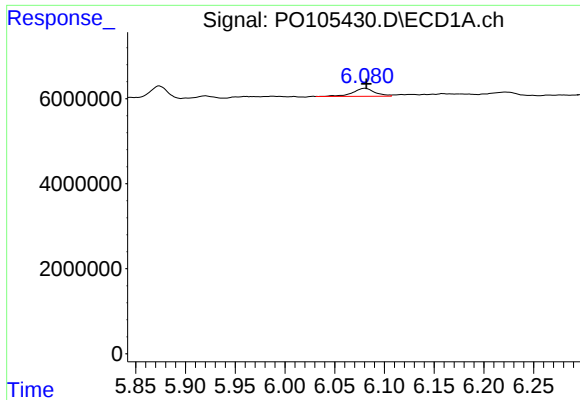

#7 AR-1016-5


R.T.: 6.081 min
Delta R.T.: -0.002 min
Response: 2931575
Conc: 13.70 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

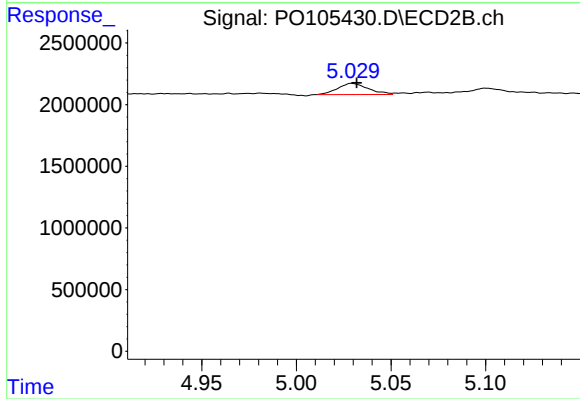


#7 AR-1016-5

R.T.: 5.030 min
Delta R.T.: -0.002 min
Response: 1026092
Conc: 12.26 ng/ml

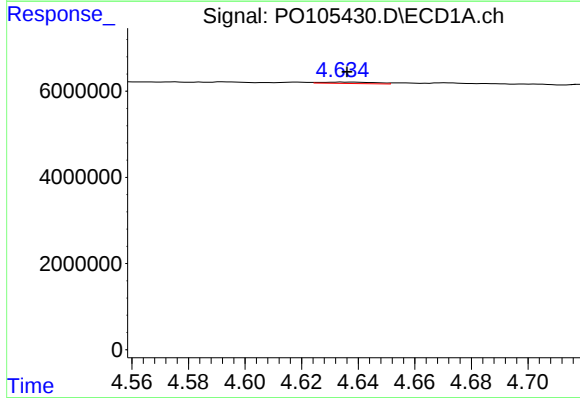


#8 AR-1221-1

R.T.: 4.634 min
Delta R.T.: -0.002 min
Response: 437401
Conc: 3.90 ng/ml

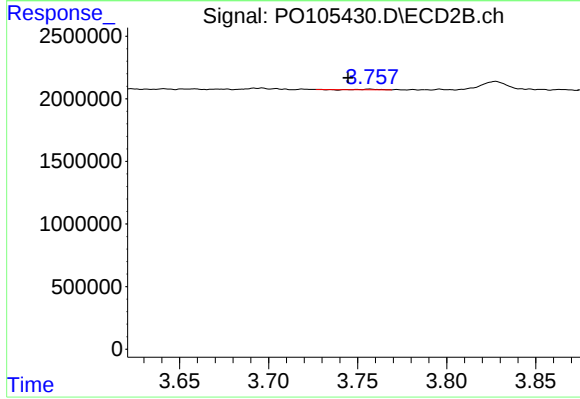

#8 AR-1221-1


R.T.: 3.757 min
Delta R.T.: 0.012 min
Response: 21519
Conc: 0.55 ng/ml

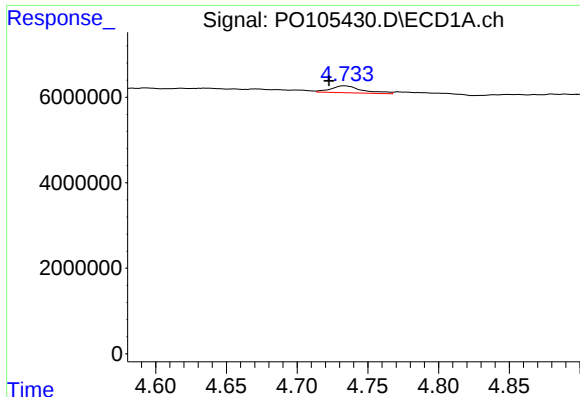

#9 AR-1221-2


R.T.: 4.734 min
Delta R.T.: 0.011 min
Response: 2509690
Conc: 29.61 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

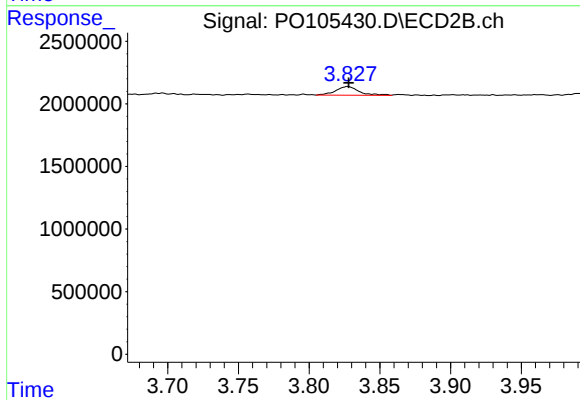


#9 AR-1221-2

R.T.: 3.827 min
Delta R.T.: 0.000 min
Response: 808924
Conc: 26.33 ng/ml

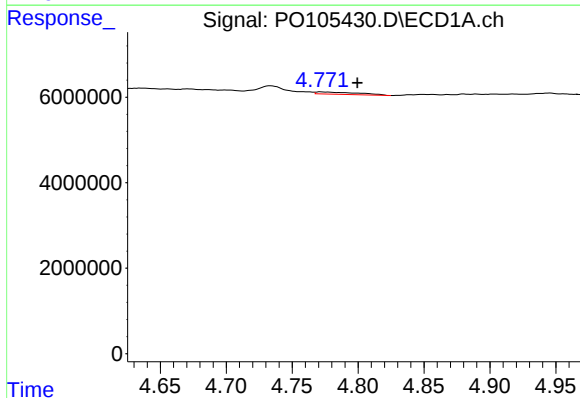


#10 AR-1221-3

R.T.: 4.772 min
Delta R.T.: -0.028 min
Response: 1187175
Conc: 4.88 ng/ml

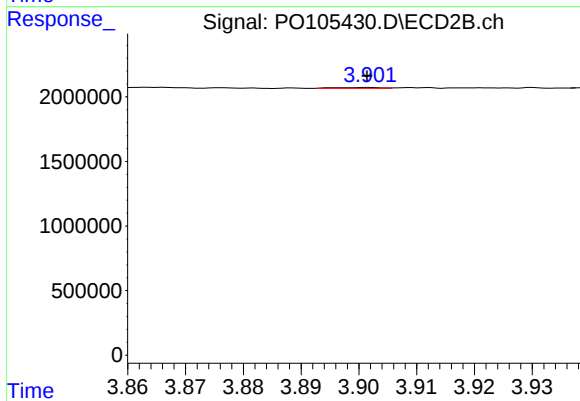

#10 AR-1221-3


R.T.: 3.901 min
Delta R.T.: 0.000 min
Response: 37143
Conc: 0.42 ng/ml

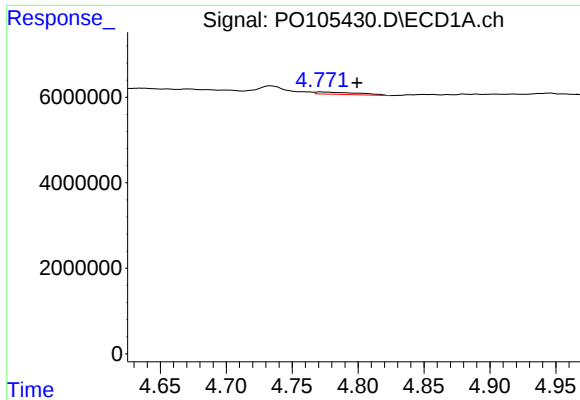

#11 AR-1232-1


R.T.: 4.772 min
Delta R.T.: -0.027 min
Response: 1187175
Conc: 5.94 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

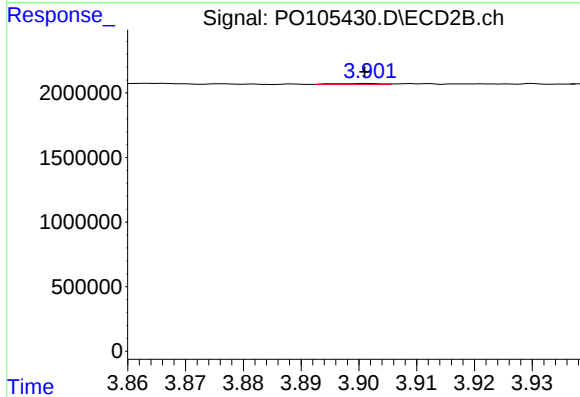


#11 AR-1232-1

R.T.: 3.901 min
Delta R.T.: 0.000 min
Response: 37143
Conc: 0.51 ng/ml

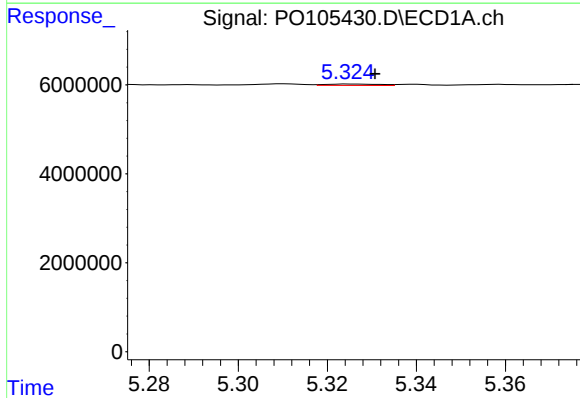


#12 AR-1232-2

R.T.: 5.325 min
Delta R.T.: -0.005 min
Response: 279541
Conc: 2.64 ng/ml

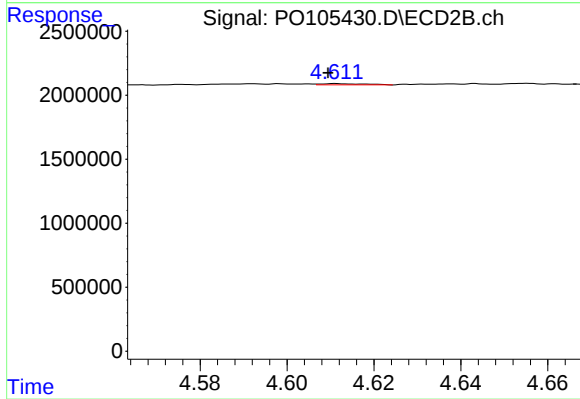

#12 AR-1232-2


R.T.: 4.611 min
Delta R.T.: 0.002 min
Response: 63158
Conc: 0.90 ng/ml

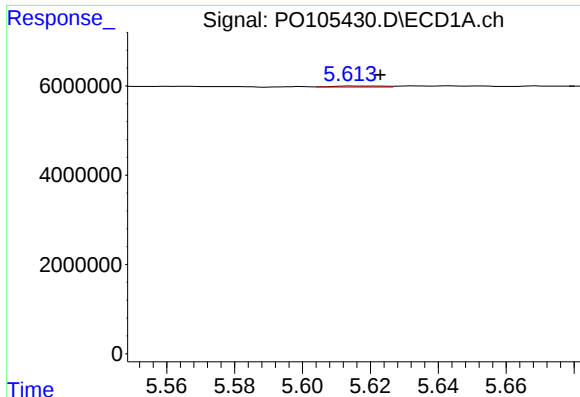

#13 AR-1232-3


R.T.: 5.614 min
Delta R.T.: -0.009 min
Response: 253944
Conc: 1.33 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

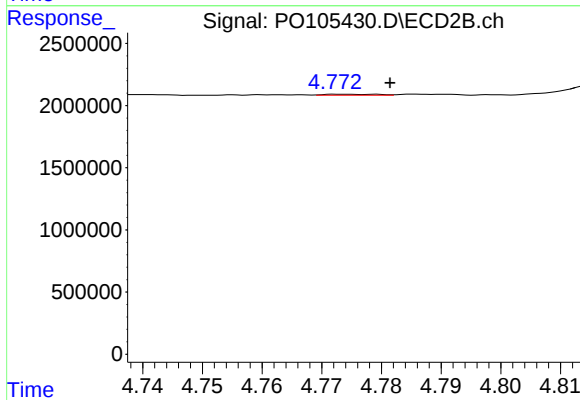


#13 AR-1232-3

R.T.: 4.779 min
Delta R.T.: -0.003 min
Response: 50022
Conc: 1.31 ng/ml

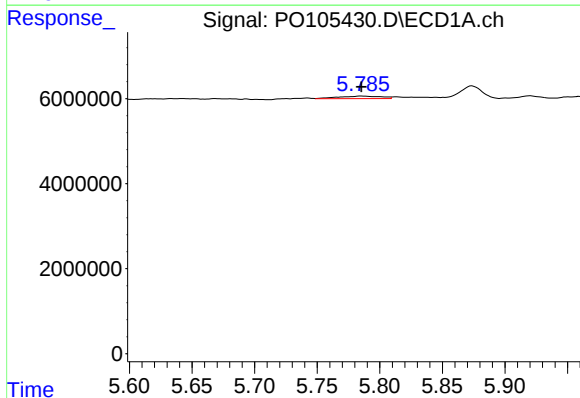


#14 AR-1232-4

R.T.: 5.785 min
Delta R.T.: 0.000 min
Response: 1462136
Conc: 14.99 ng/ml

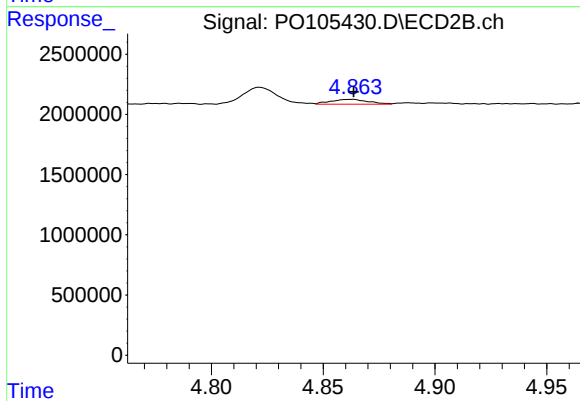

#14 AR-1232-4


R.T.: 4.863 min
Delta R.T.: 0.000 min
Response: 476450
Conc: 13.70 ng/ml

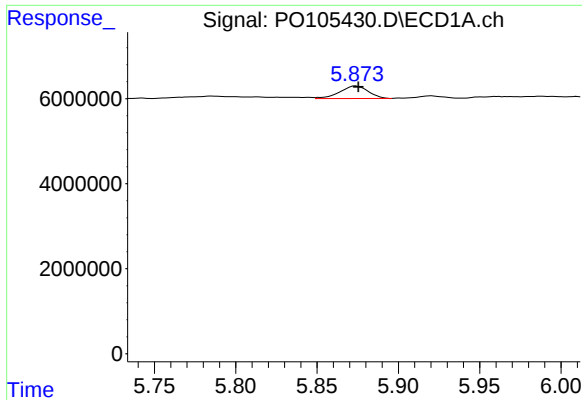

#15 AR-1232-5


R.T.: 5.874 min
Delta R.T.: -0.002 min
Response: 3601700
Conc: 49.98 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

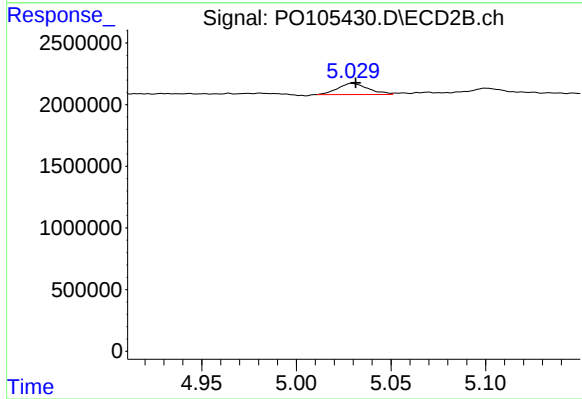


#15 AR-1232-5

R.T.: 5.030 min
Delta R.T.: -0.002 min
Response: 1026092
Conc: 29.07 ng/ml

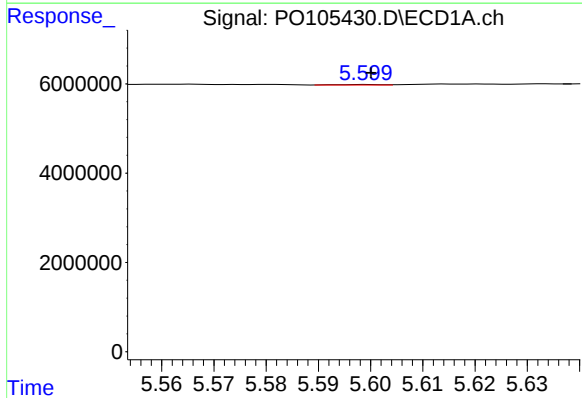


#16 AR-1242-1

R.T.: 5.599 min
Delta R.T.: 0.000 min
Response: 71167
Conc: 0.31 ng/ml

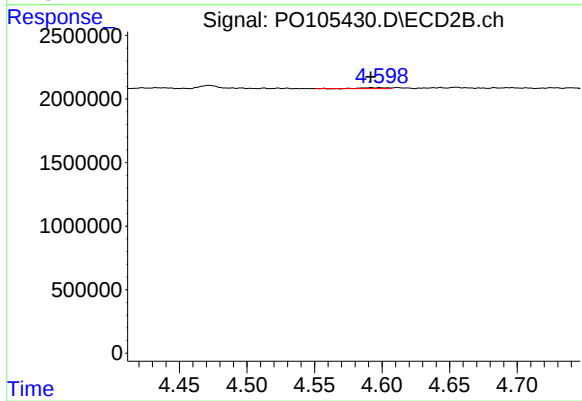

#16 AR-1242-1


R.T.: 4.592 min
Delta R.T.: 0.000 min
Response: 97314
Conc: 1.10 ng/ml

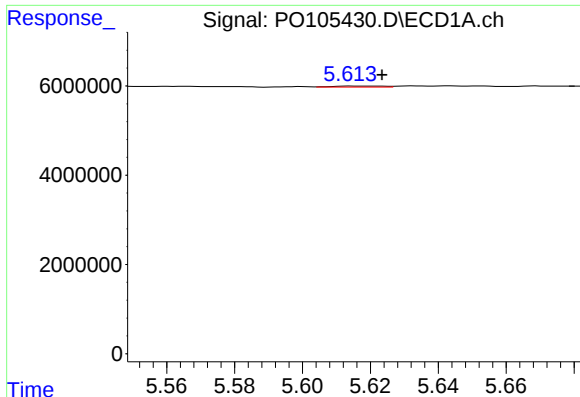

#17 AR-1242-2


R.T.: 5.614 min
Delta R.T.: -0.009 min
Response: 253944
Conc: 0.78 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

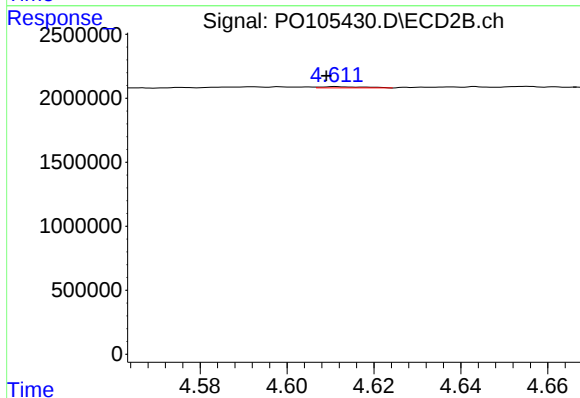


#17 AR-1242-2

R.T.: 4.611 min
Delta R.T.: 0.002 min
Response: 63158
Conc: 0.53 ng/ml

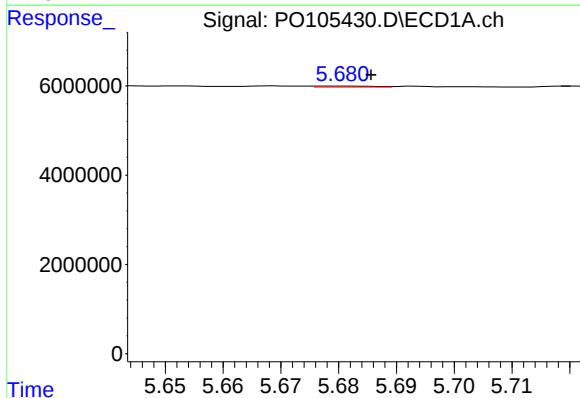


#18 AR-1242-3

R.T.: 5.681 min
Delta R.T.: -0.005 min
Response: 151601
Conc: 0.77 ng/ml

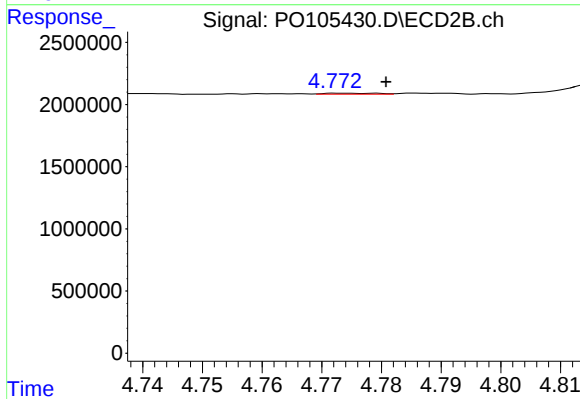

#18 AR-1242-3


R.T.: 4.779 min
Delta R.T.: -0.002 min
Response: 50022
Conc: 0.77 ng/ml

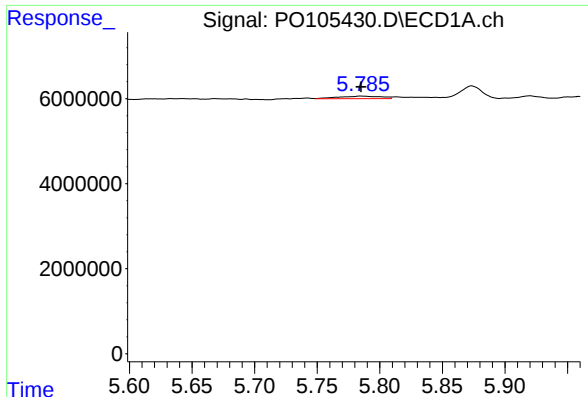

#19 AR-1242-4


R.T.: 5.785 min
Delta R.T.: 0.000 min
Response: 1462136
Conc: 8.57 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

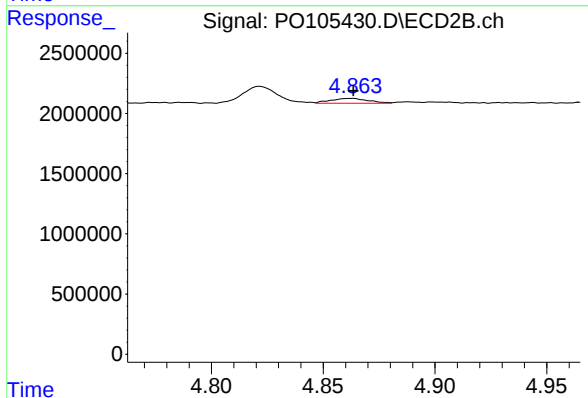


#19 AR-1242-4

R.T.: 4.863 min
Delta R.T.: 0.000 min
Response: 476450
Conc: 7.18 ng/ml

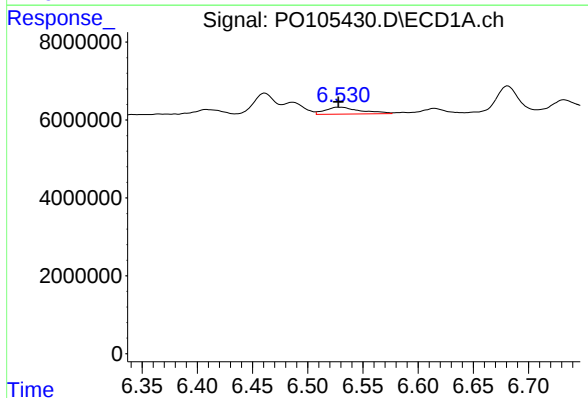


#20 AR-1242-5

R.T.: 6.528 min
Delta R.T.: 0.000 min
Response: 3896543
Conc: 22.30 ng/ml

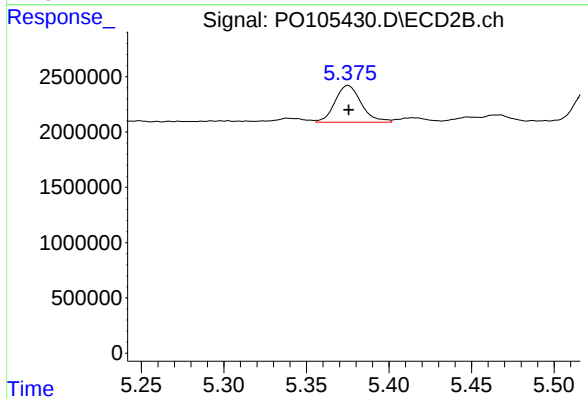

#20 AR-1242-5


R.T.: 5.375 min
Delta R.T.: 0.000 min
Response: 3683990
Conc: 44.83 ng/ml

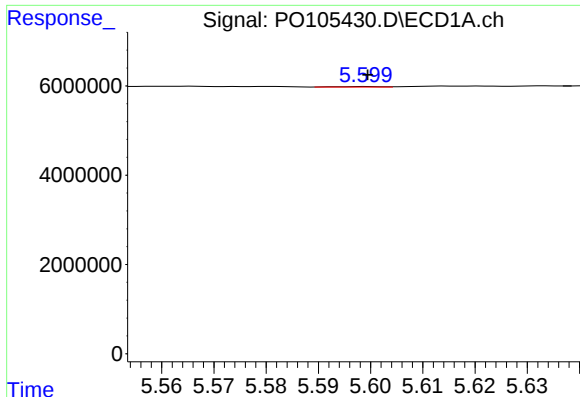

#21 AR-1248-1


R.T.: 5.599 min
Delta R.T.: 0.000 min
Response: 71167
Conc: 0.39 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

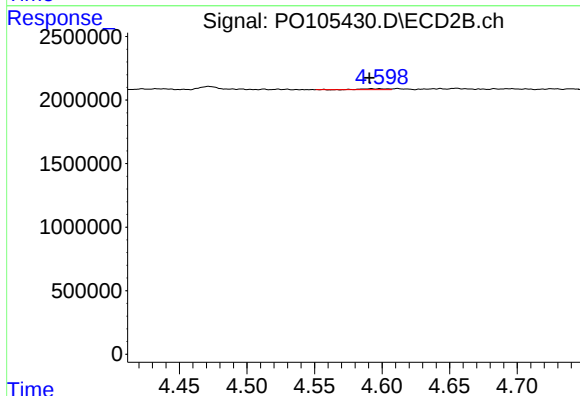


#21 AR-1248-1

R.T.: 4.592 min
Delta R.T.: 0.002 min
Response: 97314
Conc: 1.39 ng/ml

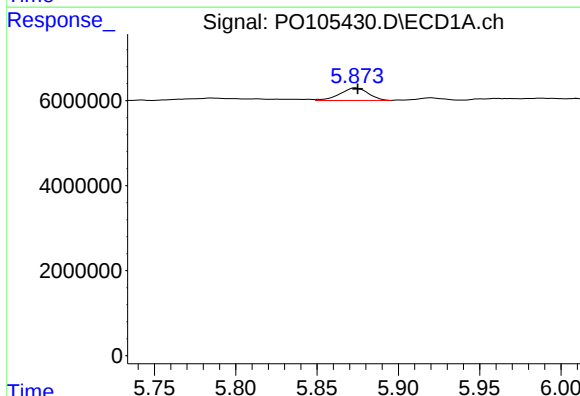


#22 AR-1248-2

R.T.: 5.874 min
Delta R.T.: -0.001 min
Response: 3601700
Conc: 14.30 ng/ml

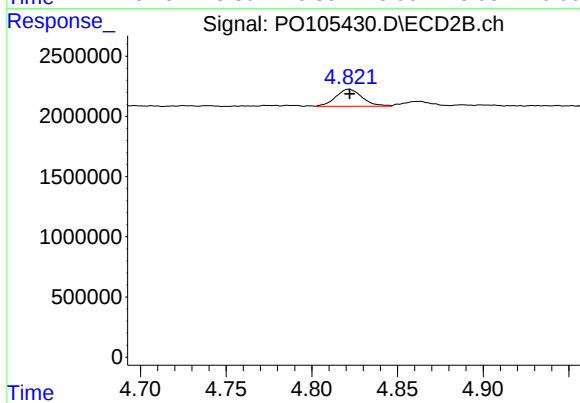

#22 AR-1248-2


R.T.: 4.822 min
Delta R.T.: 0.000 min
Response: 1531096
Conc: 16.13 ng/ml

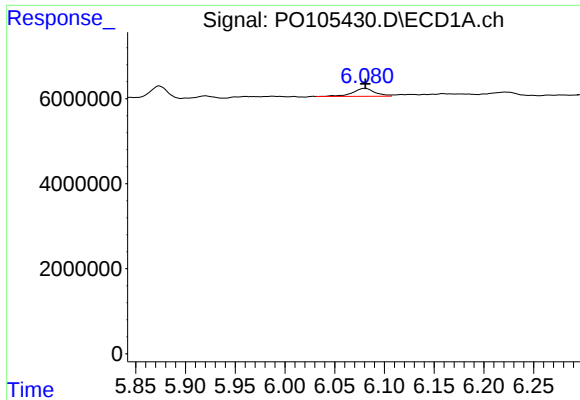

#23 AR-1248-3


R.T.: 6.081 min
Delta R.T.: 0.000 min
Response: 2931575
Conc: 10.37 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

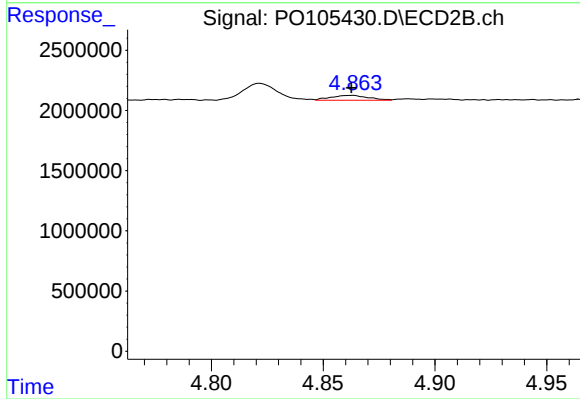


#23 AR-1248-3

R.T.: 4.863 min
Delta R.T.: 0.000 min
Response: 476450
Conc: 4.77 ng/ml

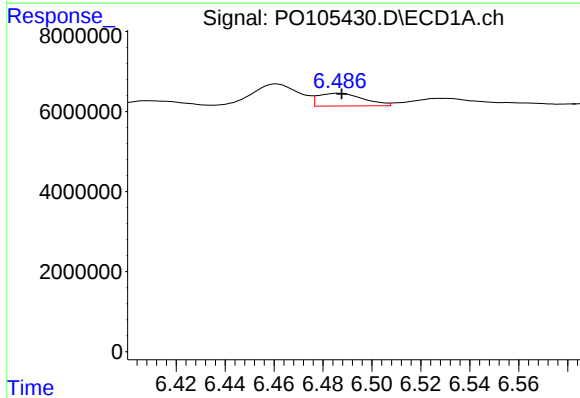


#24 AR-1248-4

R.T.: 6.486 min
Delta R.T.: -0.001 min
Response: 4055539
Conc: 12.68 ng/ml

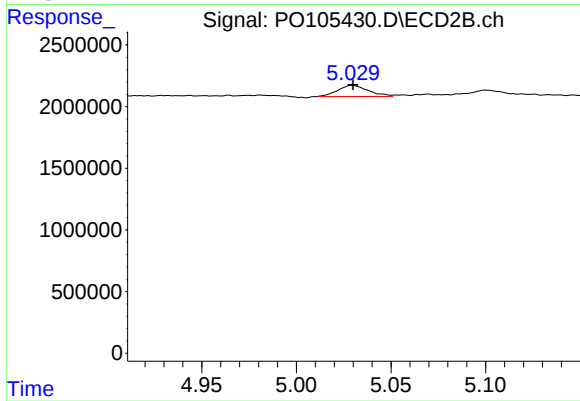

#24 AR-1248-4


R.T.: 5.030 min
Delta R.T.: 0.000 min
Response: 1026092
Conc: 9.09 ng/ml

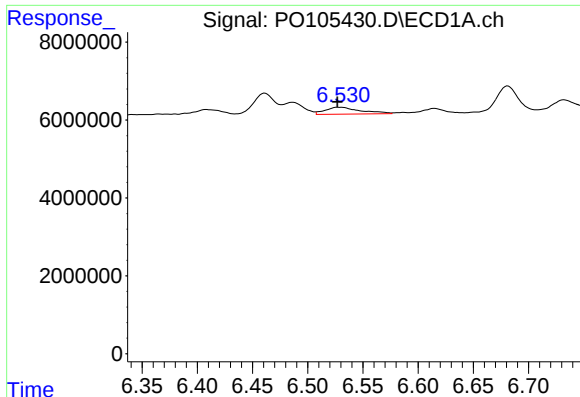

#25 AR-1248-5


R.T.: 6.528 min
Delta R.T.: 0.001 min
Response: 3896543
Conc: 12.60 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

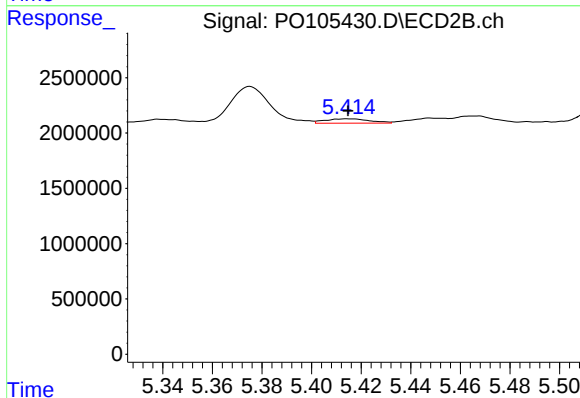


#25 AR-1248-5

R.T.: 5.415 min
Delta R.T.: 0.000 min
Response: 486997
Conc: 4.32 ng/ml

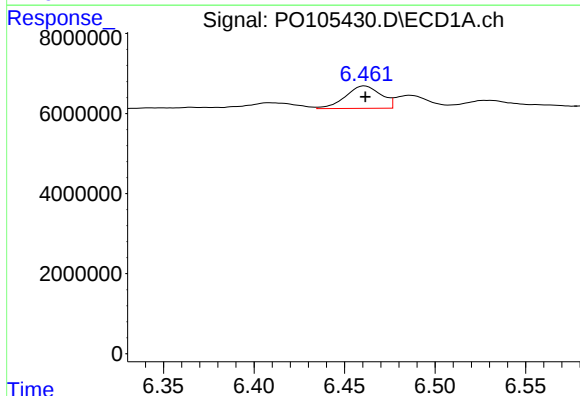


#26 AR-1254-1

R.T.: 6.461 min
Delta R.T.: 0.000 min
Response: 7601536
Conc: 24.24 ng/ml

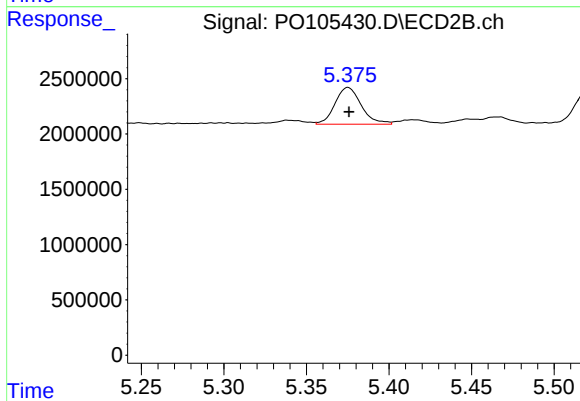

#26 AR-1254-1


R.T.: 5.375 min
Delta R.T.: 0.000 min
Response: 3683990
Conc: 22.63 ng/ml

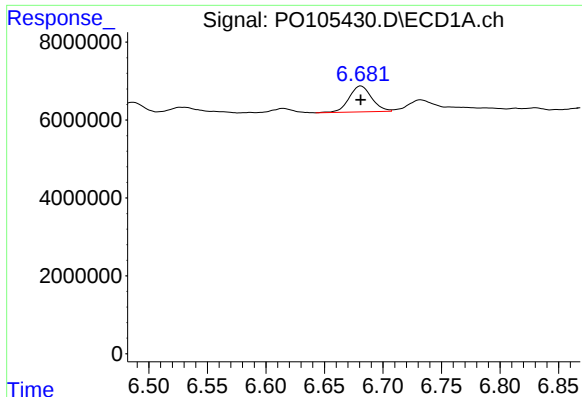

#27 AR-1254-2


R.T.: 6.681 min
Delta R.T.: 0.000 min
Response: 8940074
Conc: 19.81 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

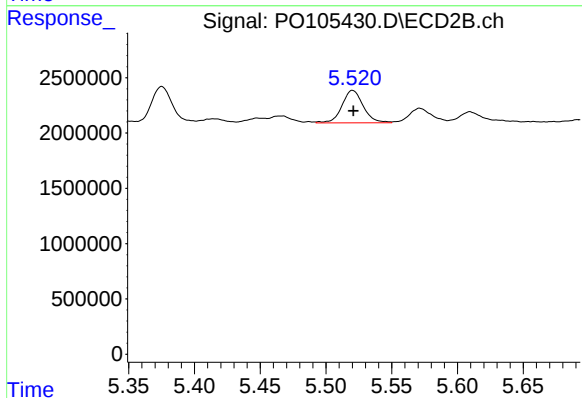


#27 AR-1254-2

R.T.: 5.520 min
Delta R.T.: 0.000 min
Response: 3331119
Conc: 22.77 ng/ml

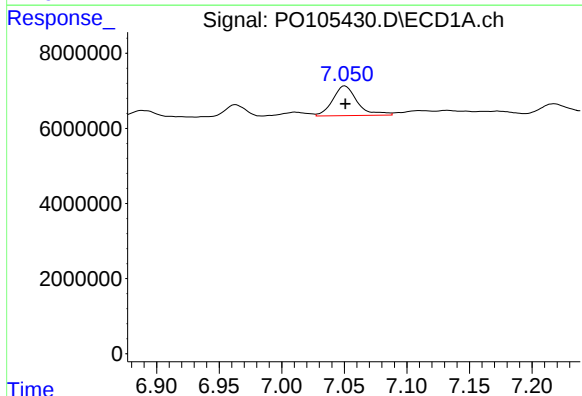


#28 AR-1254-3

R.T.: 7.050 min
Delta R.T.: 0.000 min
Response: 10824682
Conc: 22.82 ng/ml

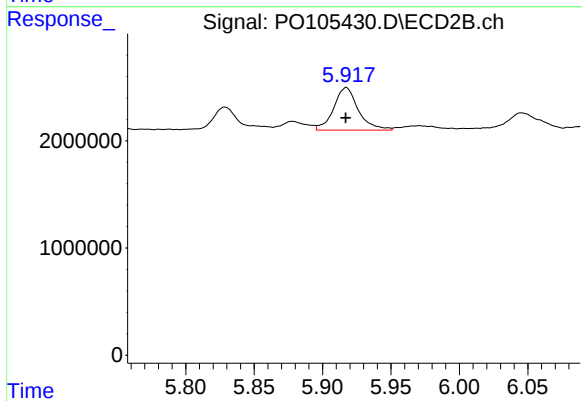

#28 AR-1254-3


R.T.: 5.917 min
Delta R.T.: 0.000 min
Response: 4987605
Conc: 22.11 ng/ml

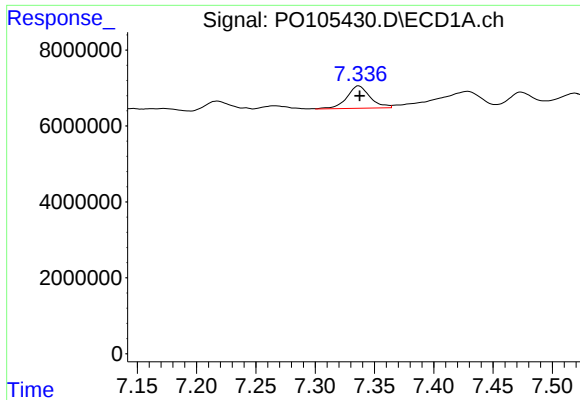

#29 AR-1254-4


R.T.: 7.337 min
Delta R.T.: 0.000 min
Response: 7974602
Conc: 22.26 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

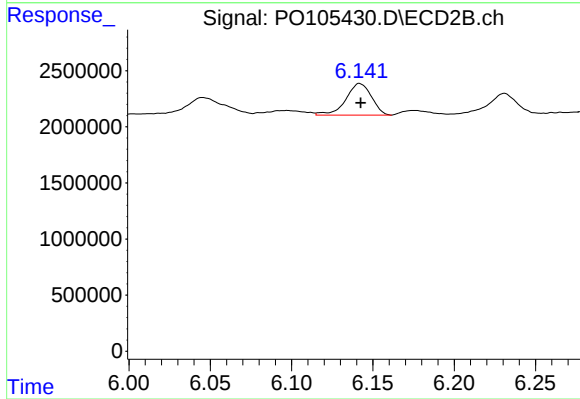


#29 AR-1254-4

R.T.: 6.142 min
Delta R.T.: 0.000 min
Response: 3098786
Conc: 21.96 ng/ml

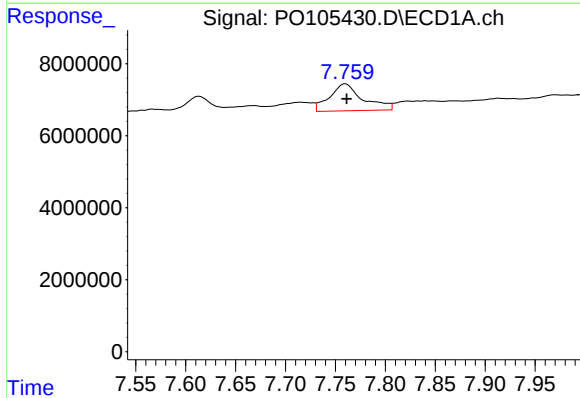


#30 AR-1254-5

R.T.: 7.760 min
Delta R.T.: -0.001 min
Response: 17396666
Conc: 43.82 ng/ml

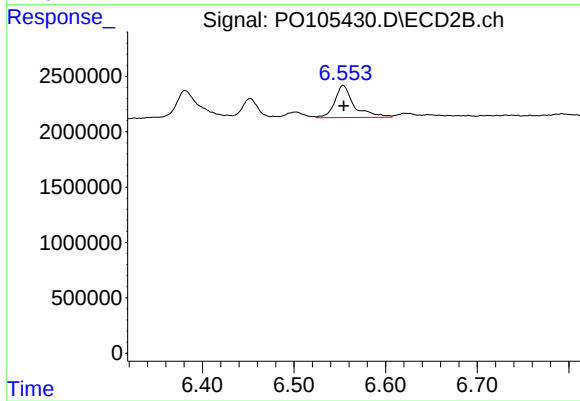

#30 AR-1254-5


R.T.: 6.554 min
Delta R.T.: 0.000 min
Response: 4272264
Conc: 21.32 ng/ml

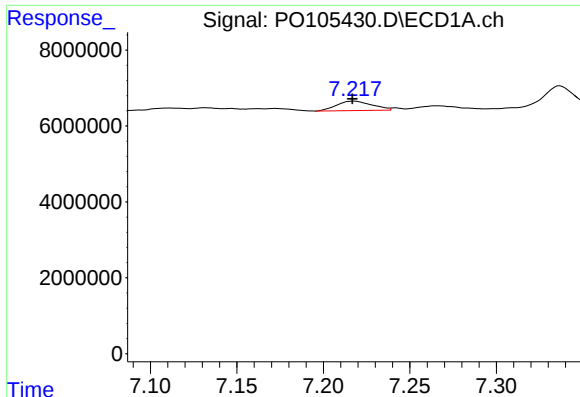

#31 AR-1260-1


R.T.: 7.218 min
Delta R.T.: 0.000 min
Response: 3564115
Conc: 9.72 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

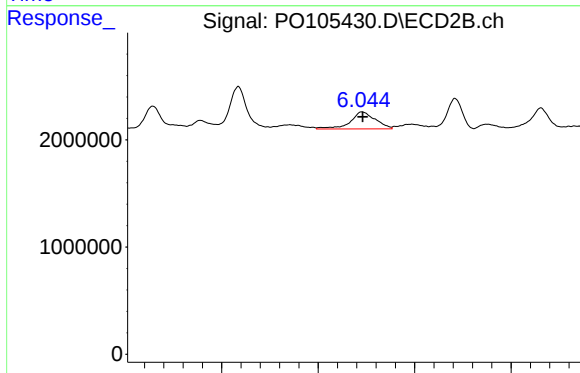


#31 AR-1260-1

R.T.: 6.045 min
Delta R.T.: 0.000 min
Response: 2857501
Conc: 18.31 ng/ml

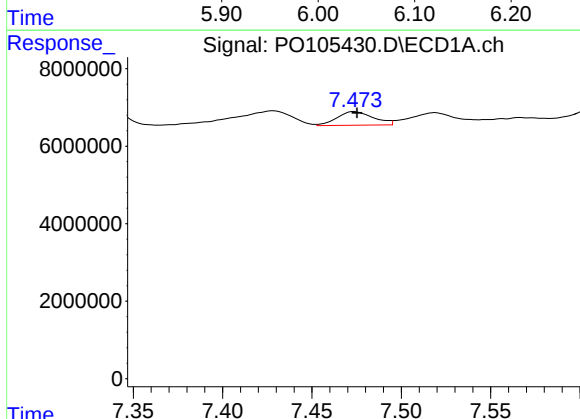


#32 AR-1260-2

R.T.: 7.474 min
Delta R.T.: -0.002 min
Response: 4978546
Conc: 11.96 ng/ml

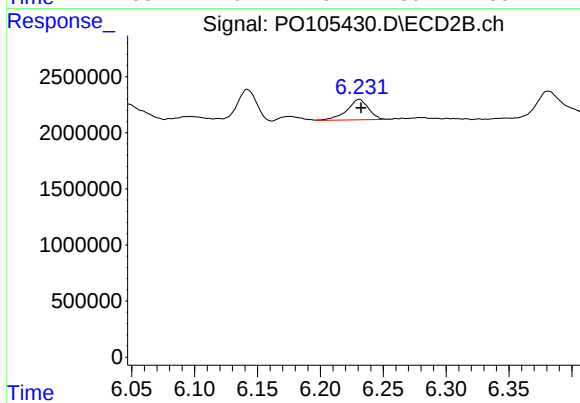

#32 AR-1260-2


R.T.: 6.231 min
Delta R.T.: -0.001 min
Response: 2170524
Conc: 11.48 ng/ml

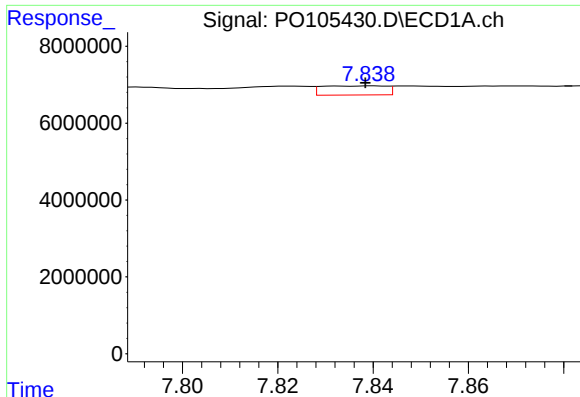

#33 AR-1260-3


R.T.: 7.840 min
Delta R.T.: 0.002 min
Response: 2218320
Conc: 8.57 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

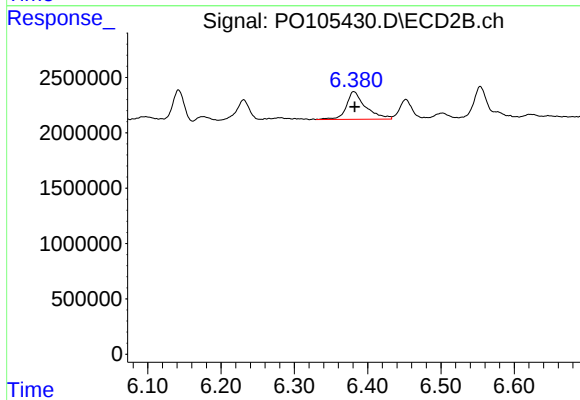


#33 AR-1260-3

R.T.: 6.381 min
Delta R.T.: -0.001 min
Response: 4600268
Conc: 24.90 ng/ml

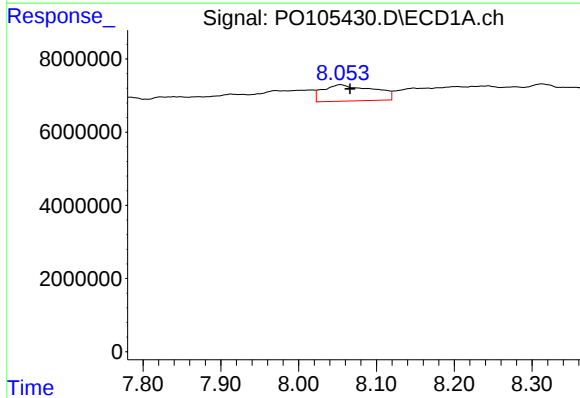


#34 AR-1260-4

R.T.: 8.054 min
Delta R.T.: -0.012 min
Response: 20056709
Conc: 60.79 ng/ml

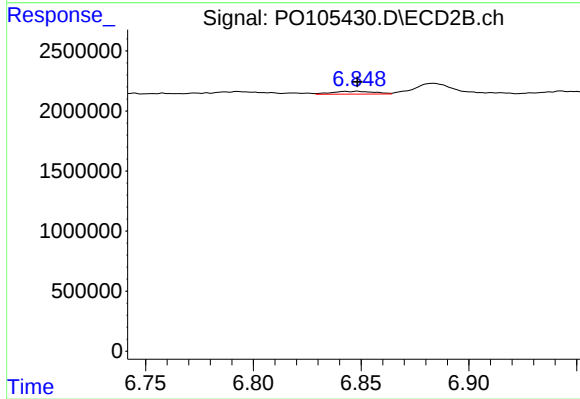

#34 AR-1260-4


R.T.: 6.848 min
Delta R.T.: 0.000 min
Response: 320286
Conc: 2.62 ng/ml

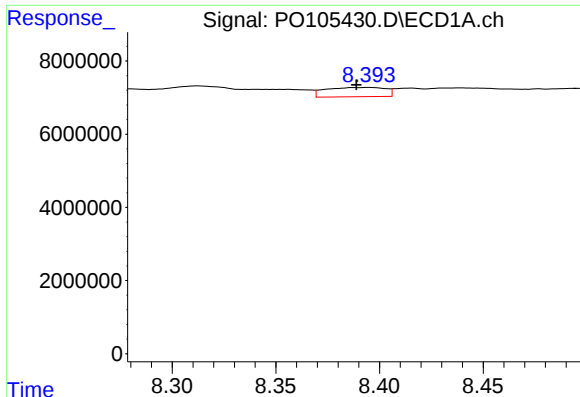

#35 AR-1260-5


R.T.: 8.395 min
Delta R.T.: 0.006 min
Response: 5063919
Conc: 8.51 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

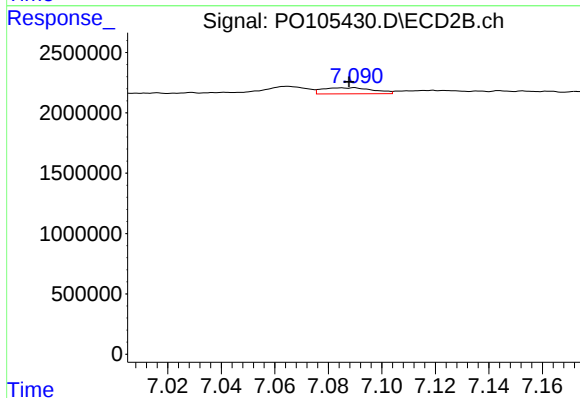


#35 AR-1260-5

R.T.: 7.089 min
Delta R.T.: 0.002 min
Response: 668744
Conc: 2.40 ng/ml

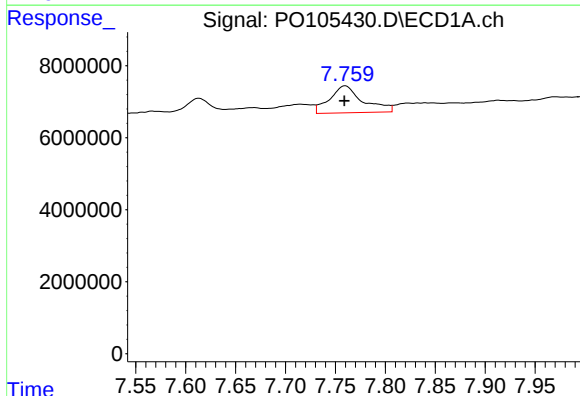


#36 AR-1262-1

R.T.: 7.760 min
Delta R.T.: 0.000 min
Response: 17396666
Conc: 54.77 ng/ml

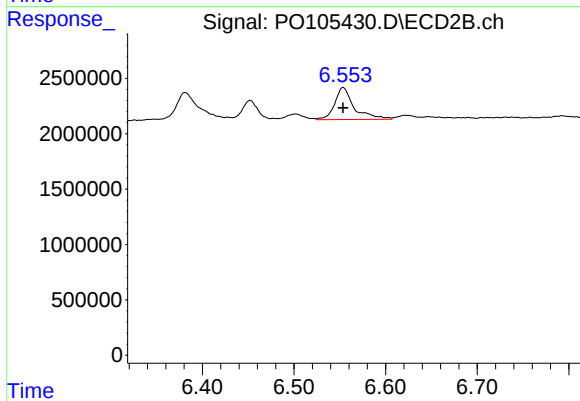

#36 AR-1262-1


R.T.: 6.554 min
Delta R.T.: 0.000 min
Response: 4272264
Conc: 40.15 ng/ml

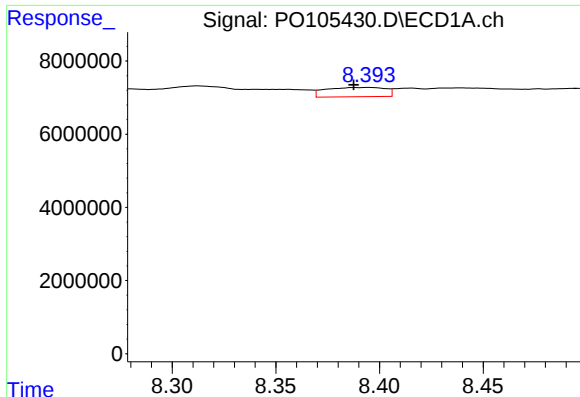

#37 AR-1262-2


R.T.: 8.395 min
Delta R.T.: 0.007 min
Response: 5063919
Conc: 6.73 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

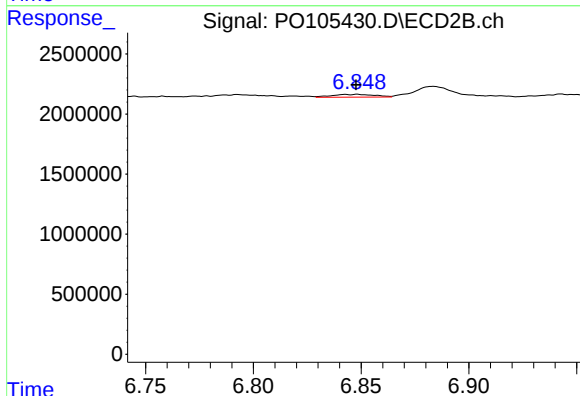


#37 AR-1262-2

R.T.: 6.848 min
Delta R.T.: 0.000 min
Response: 320286
Conc: 1.88 ng/ml

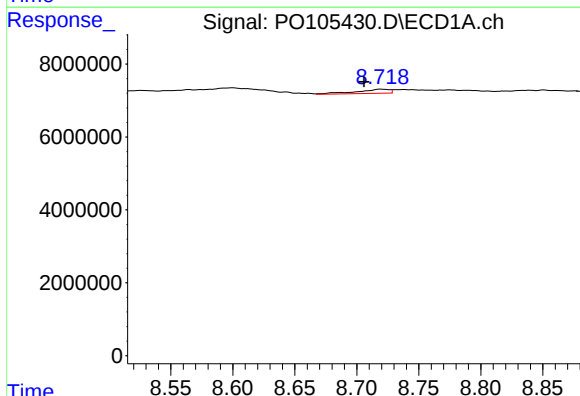


#38 AR-1262-3

R.T.: 8.720 min
Delta R.T.: 0.014 min
Response: 2039497
Conc: 4.14 ng/ml

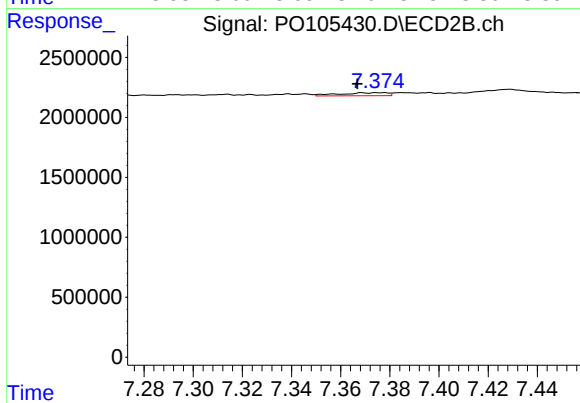

#38 AR-1262-3


R.T.: 7.369 min
Delta R.T.: 0.002 min
Response: 347599
Conc: 2.75 ng/ml

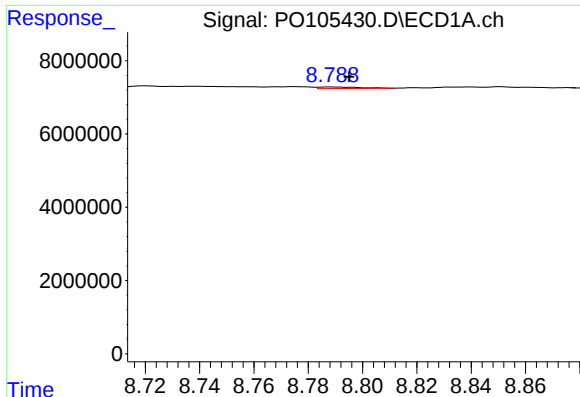

#39 AR-1262-4


R.T.: 8.788 min
Delta R.T.: -0.007 min
Response: 452835
Conc: 1.23 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

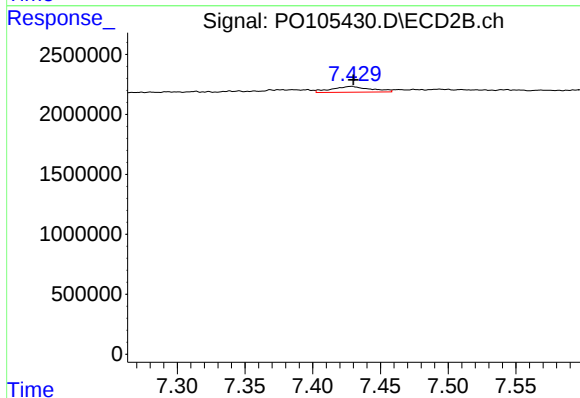


#39 AR-1262-4

R.T.: 7.429 min
Delta R.T.: -0.001 min
Response: 980737
Conc: 4.24 ng/ml

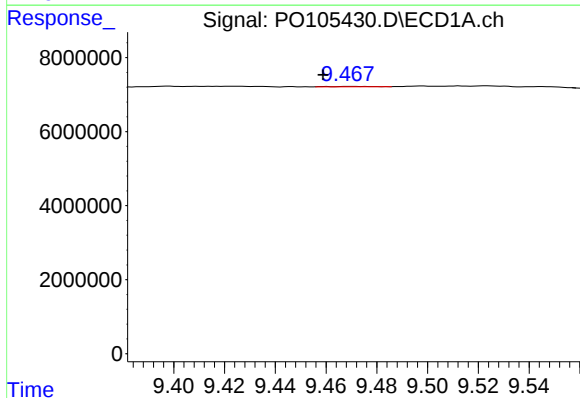


#40 AR-1262-5

R.T.: 9.469 min
Delta R.T.: 0.010 min
Response: 102825
Conc: 0.38 ng/ml

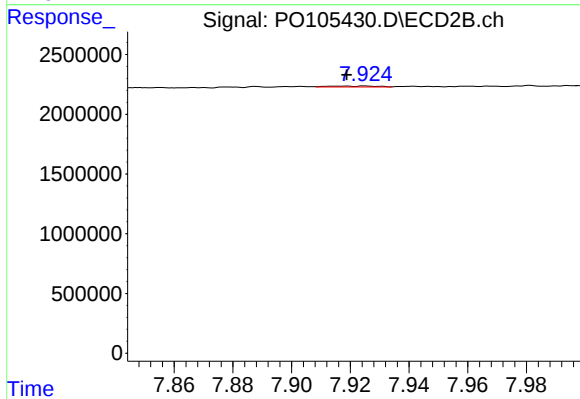

#40 AR-1262-5


R.T.: 7.925 min
Delta R.T.: 0.006 min
Response: 93336
Conc: 0.93 ng/ml

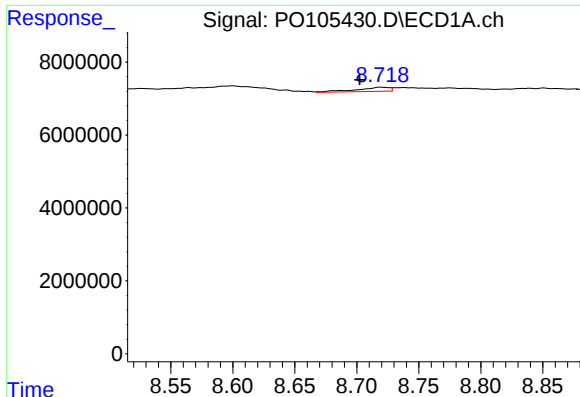

#41 AR-1268-1


R.T.: 8.720 min
Delta R.T.: 0.017 min
Response: 2039497
Conc: 2.51 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

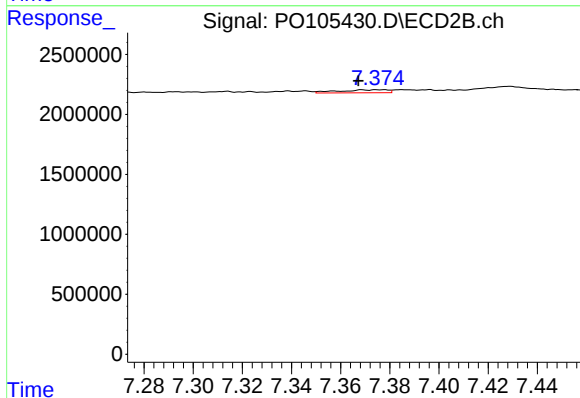


#41 AR-1268-1

R.T.: 7.369 min
Delta R.T.: 0.002 min
Response: 347599
Conc: 1.00 ng/ml

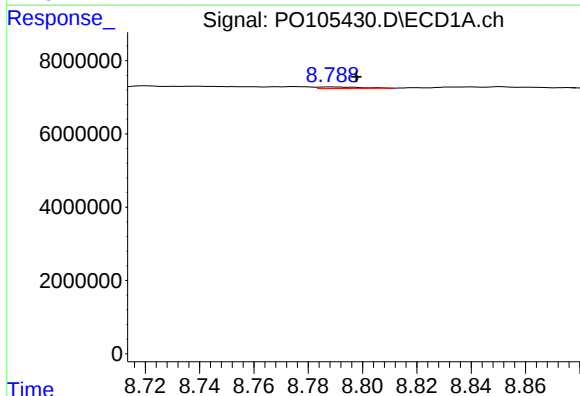


#42 AR-1268-2

R.T.: 8.788 min
Delta R.T.: -0.009 min
Response: 452835
Conc: 0.62 ng/ml

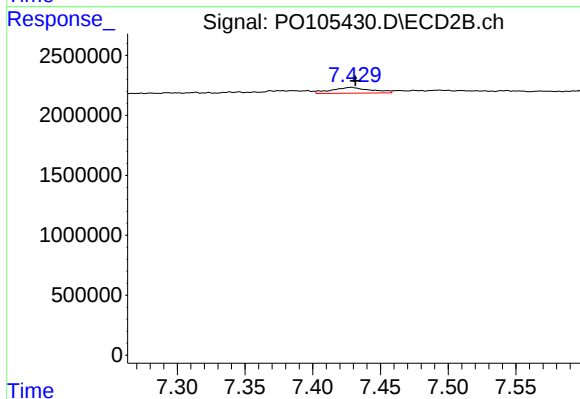

#42 AR-1268-2


R.T.: 7.429 min
Delta R.T.: -0.003 min
Response: 980737
Conc: 3.14 ng/ml

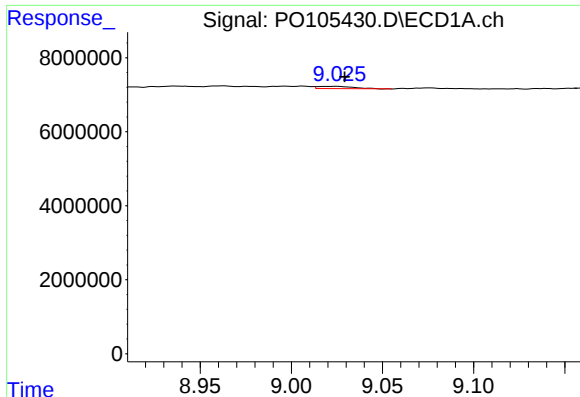

#43 AR-1268-3


R.T.: 9.025 min
Delta R.T.: -0.004 min
Response: 822510
Conc: 1.27 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

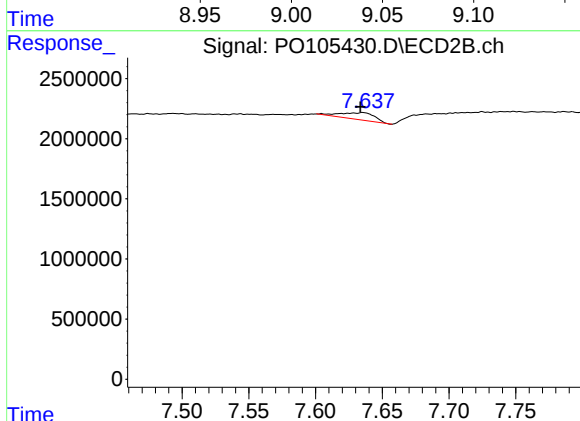


#43 AR-1268-3

R.T.: 7.635 min
Delta R.T.: 0.002 min
Response: 1034223
Conc: 4.09 ng/ml

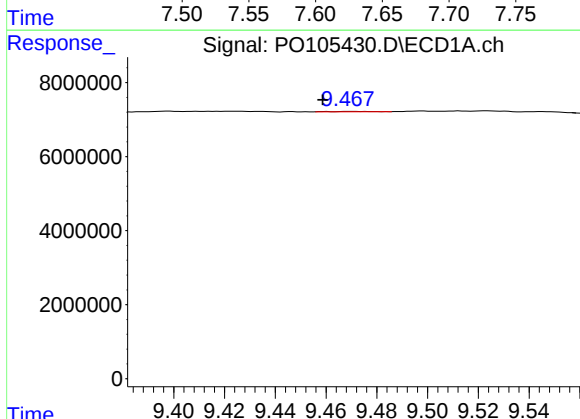


#44 AR-1268-4

R.T.: 9.469 min
Delta R.T.: 0.010 min
Response: 102825
Conc: 0.37 ng/ml

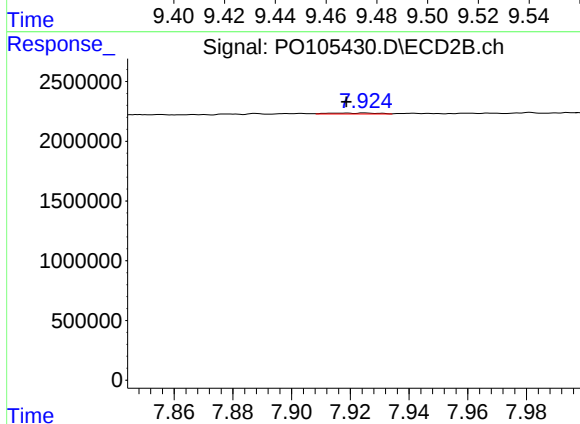

#44 AR-1268-4


R.T.: 7.925 min
Delta R.T.: 0.006 min
Response: 93336
Conc: 0.87 ng/ml

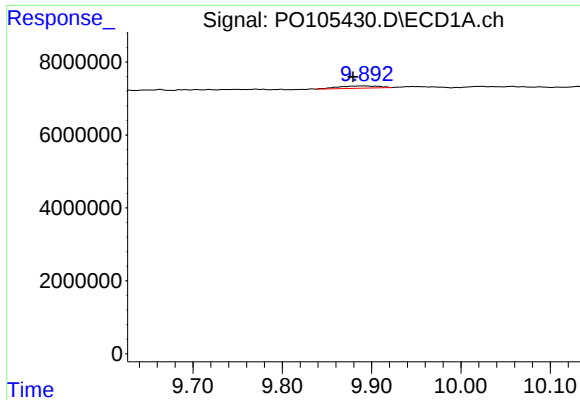

#45 AR-1268-5

R.T.: 9.892 min
Delta R.T.: 0.013 min
Response: 2078178
Conc: 0.99 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

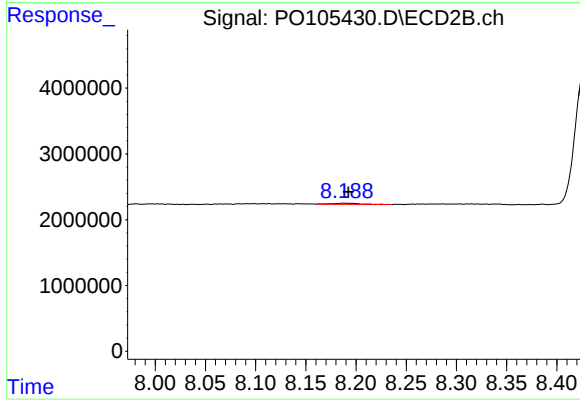

#45 AR-1268-5

R.T.: 8.188 min
Delta R.T.: -0.004 min
Response: 341561
Conc: 0.51 ng/ml