

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0081224\
 Data File : P0105432.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2024 19:17
 Operator : YP/AJ
 Sample : P3390-07
 Misc : AR1268 LOD 25 PPB
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 02:32:57 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0081024.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 10 04:08:56 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.428	3.536	119.1E6	42903912	13.630	13.659
2)	SA Decachlor...	10.217	8.427	94244075	28030984	16.383	15.834
Target Compounds							
3)	L1 AR-1016-1	5.585	4.589	147023	69525	0.486	0.619 #
4)	L1 AR-1016-2	5.628	4.610	587509	112620	1.374	0.723 #
5)	L1 AR-1016-3	5.682	4.786	118781	130059	0.463	1.553 #
6)	L1 AR-1016-4	5.777	4.815	628879	24646	2.875	0.366 #
7)	L1 AR-1016-5	6.078	5.027	355645	549208	1.662	6.562 #
8)	L2 AR-1221-1	4.636	3.764	2932073	31356	26.146	0.794 #
9)	L2 AR-1221-2	4.733	3.826	2689392	1316723	31.729	42.859 #
10)	L2 AR-1221-3	4.793	3.892	862964	53595	3.547	0.599 #
11)	L3 AR-1232-1	4.793	3.892	862964	53595	4.316	0.734 #
12)	L3 AR-1232-2	5.323	4.610	337232	112620	3.186	1.604 #
13)	L3 AR-1232-3	5.628	4.786	587509	130059	3.069	3.403
14)	L3 AR-1232-4	5.777	4.867	628879	182043	6.448	5.233
15)	L3 AR-1232-5	5.870	5.027	167987	549208	2.331	15.559 #
16)	L4 AR-1242-1	5.585	4.589	147023	69525	0.633	0.788
17)	L4 AR-1242-2	5.628	4.610	587509	112620	1.803	0.949 #
18)	L4 AR-1242-3	5.682	4.786	118781	130059	0.602	2.003 #
19)	L4 AR-1242-4	5.777	4.867	628879	182043	3.686	2.745 #
20)	L4 AR-1242-5	6.534	5.398	661614	1493847	3.786	18.179 #
21)	L5 AR-1248-1	5.585	4.589	147023	69525	0.805	0.995
22)	L5 AR-1248-2	5.870	4.815	167987	24646	0.667	0.260 #
23)	L5 AR-1248-3	6.078	4.867	355645	182043	1.258	1.824 #
24)	L5 AR-1248-4	6.489	5.027	740809	549208	2.317	4.866 #
25)	L5 AR-1248-5	6.534	5.398	661614	1493847	2.139	13.266 #
26)	L6 AR-1254-1	6.461	5.398	3319741	1493847	10.586	9.176
27)	L6 AR-1254-2	6.676	5.528	687500	1067652	1.523	7.299 #
28)	L6 AR-1254-3	7.053	5.914	2024623	836121	4.268	3.707
29)	L6 AR-1254-4	7.336	6.117	2215654	1441078	6.185	10.213 #
30)	L6 AR-1254-5	7.750	6.561	8905431	383926	22.434	1.916 #
31)	L7 AR-1260-1	7.230	6.051	2166575	748721	5.911	4.797
32)	L7 AR-1260-2	7.489	6.215	2149038	1005860	5.161	5.322
33)	L7 AR-1260-3	7.835	6.390	10722248	3585431	41.428	19.409 #
34)	L7 AR-1260-4	8.085	6.844	18058673	2029244	54.735	16.602 #
35)	L7 AR-1260-5	8.386	7.087	8034833	1144624	13.507	4.113 #
36)	L8 AR-1262-1	7.750	6.561	8905431	383926	28.037	3.608 #
37)	L8 AR-1262-2	8.386	6.844	8034833	2029244	10.682	11.942
38)	L8 AR-1262-3	8.700	7.367	17618129	7429336	35.803	58.845 #
39)	L8 AR-1262-4	8.796	7.431	15883463	6512737	43.254	28.134 #
40)	L8 AR-1262-5	9.455	7.919	4259013	2112597	15.903	21.020 #
41)	L9 AR-1268-1	8.700	7.367	17618129	7429336	21.662	21.280

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081224\
Data File : P0105432.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Aug 2024 19:17
Operator : YP/AJ
Sample : P3390-07
Misc : AR1268 LOD 25 PPB
ALS Vial : 32 Sample Multiplier: 1


Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 13 02:32:57 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081024.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Aug 10 04:08:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42)	L9 AR-1268-2	8.796	7.431	15883463	6512737	21.850	20.875
43)	L9 AR-1268-3	9.027	7.633	13692004	5067725	21.209	20.051
44)	L9 AR-1268-4	9.455	7.919	4259013	2112597	15.295	19.642 #
45)	L9 AR-1268-5	9.876	8.192	40809866	12924012	19.519	19.321


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

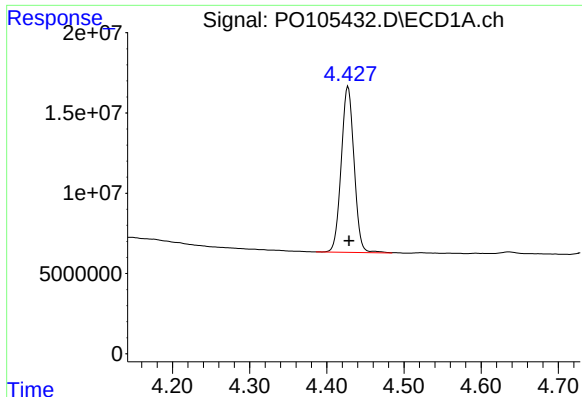

#1 Tetrachloro-m-xylene


R.T.: 4.428 min
Delta R.T.: -0.001 min
Response: 119051887
Conc: 13.63 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

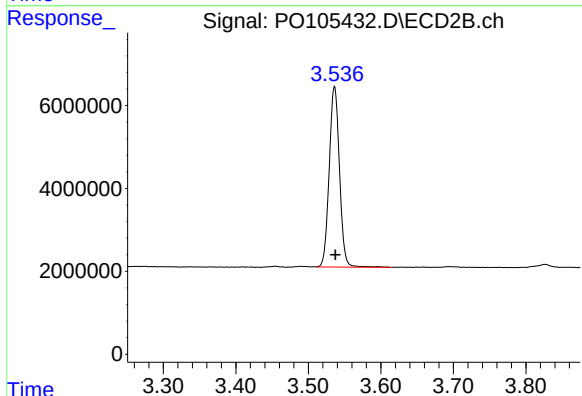


#1 Tetrachloro-m-xylene

R.T.: 3.536 min
Delta R.T.: -0.001 min
Response: 42903912
Conc: 13.66 ng/ml

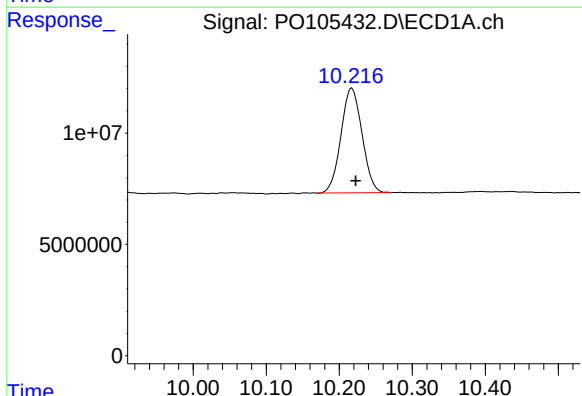


#2 Decachlorobiphenyl

R.T.: 10.217 min
Delta R.T.: -0.006 min
Response: 94244075
Conc: 16.38 ng/ml

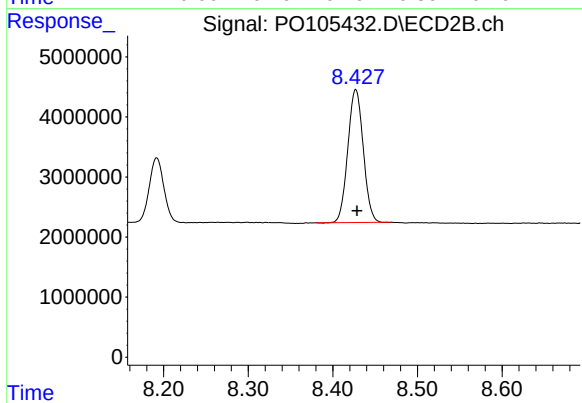

#2 Decachlorobiphenyl


R.T.: 8.427 min
Delta R.T.: -0.001 min
Response: 28030984
Conc: 15.83 ng/ml

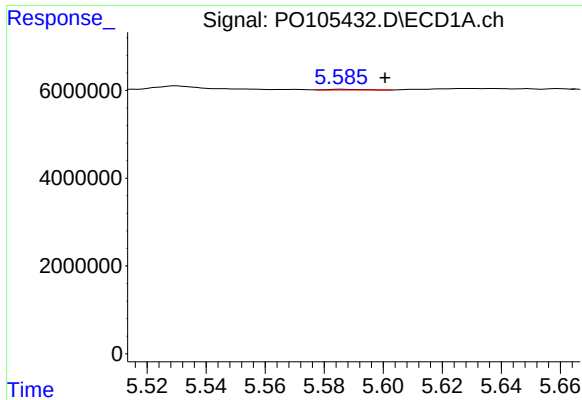

#3 AR-1016-1


R.T.: 5.585 min
Delta R.T.: -0.015 min
Response: 147023
Conc: 0.49 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

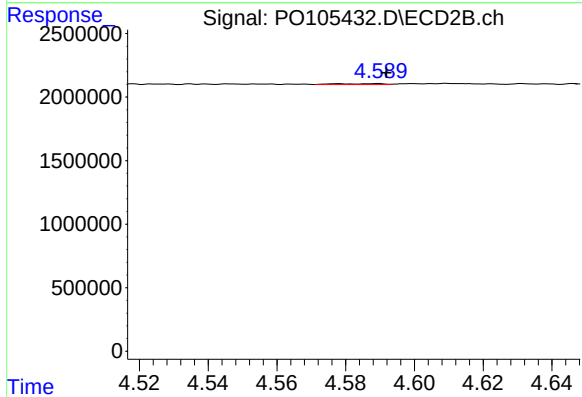


#3 AR-1016-1

R.T.: 4.589 min
Delta R.T.: -0.003 min
Response: 69525
Conc: 0.62 ng/ml

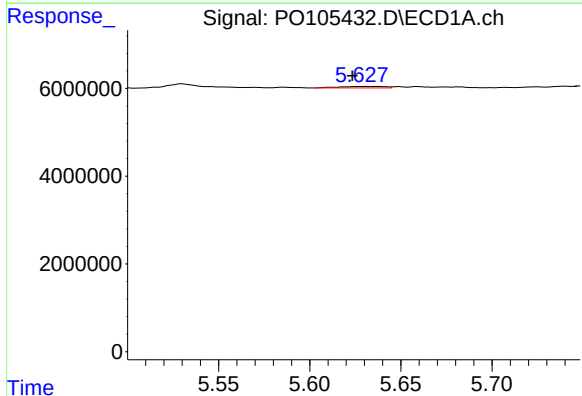


#4 AR-1016-2

R.T.: 5.628 min
Delta R.T.: 0.005 min
Response: 587509
Conc: 1.37 ng/ml

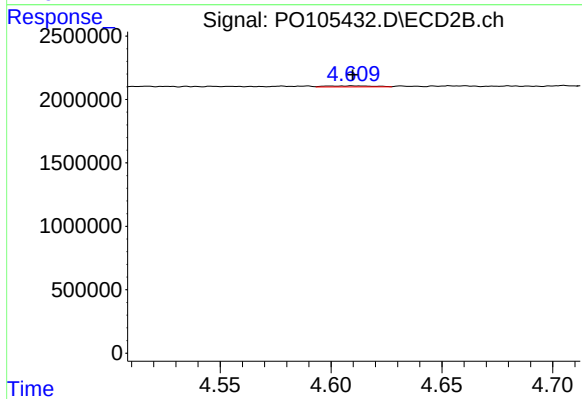

#4 AR-1016-2


R.T.: 4.610 min
Delta R.T.: 0.000 min
Response: 112620
Conc: 0.72 ng/ml

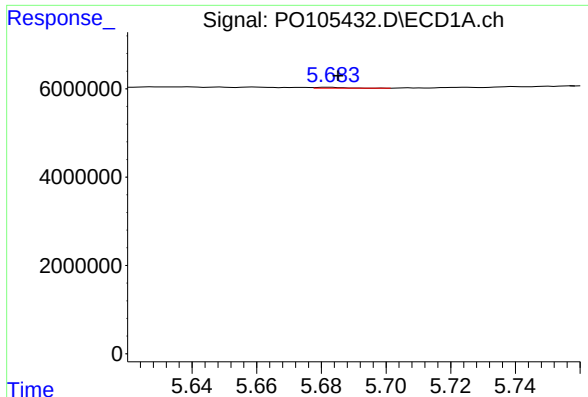

#5 AR-1016-3


R.T.: 5.682 min
Delta R.T.: -0.003 min
Response: 118781
Conc: 0.46 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

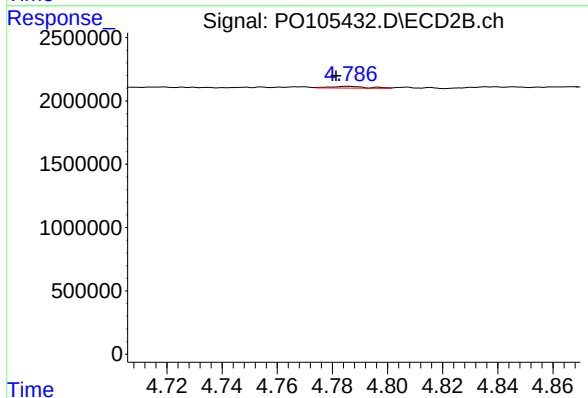


#5 AR-1016-3

R.T.: 4.786 min
Delta R.T.: 0.004 min
Response: 130059
Conc: 1.55 ng/ml

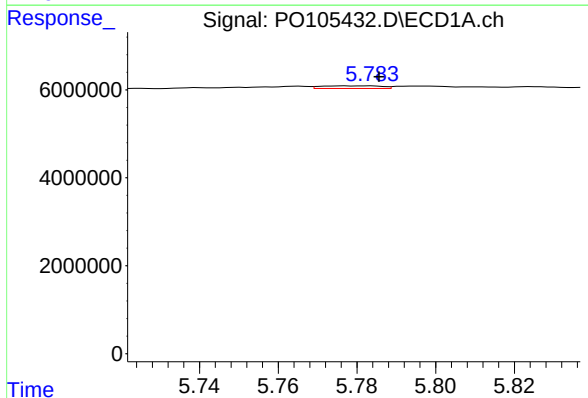


#6 AR-1016-4

R.T.: 5.777 min
Delta R.T.: -0.009 min
Response: 628879
Conc: 2.88 ng/ml

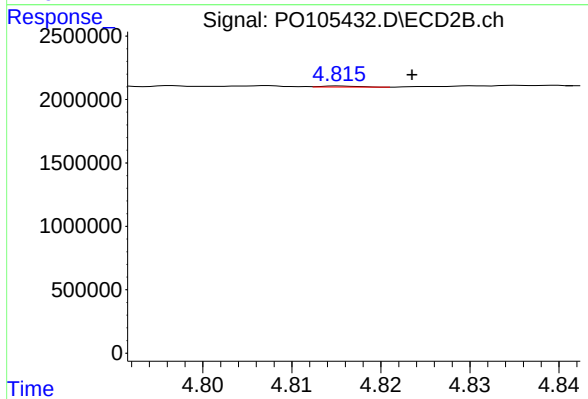

#6 AR-1016-4


R.T.: 4.815 min
Delta R.T.: -0.008 min
Response: 24646
Conc: 0.37 ng/ml

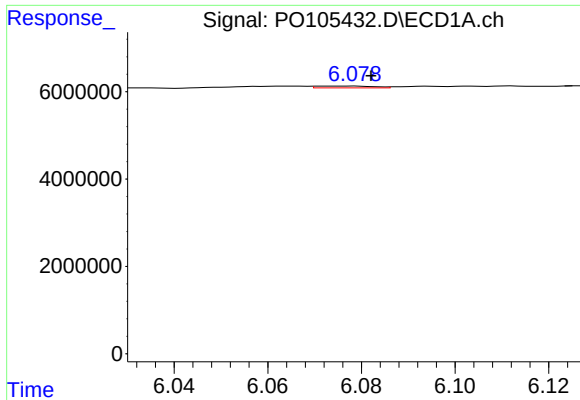

#7 AR-1016-5


R.T.: 6.078 min
Delta R.T.: -0.004 min
Response: 355645
Conc: 1.66 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

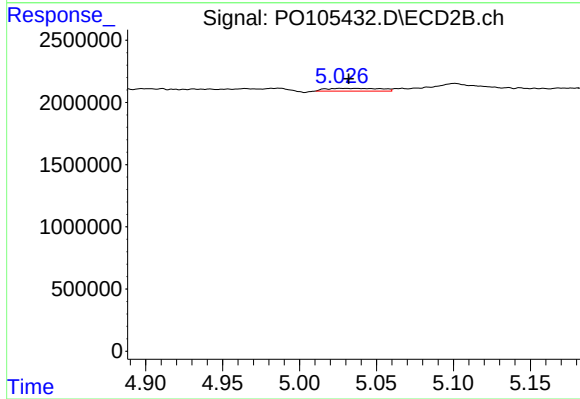


#7 AR-1016-5

R.T.: 5.027 min
Delta R.T.: -0.005 min
Response: 549208
Conc: 6.56 ng/ml

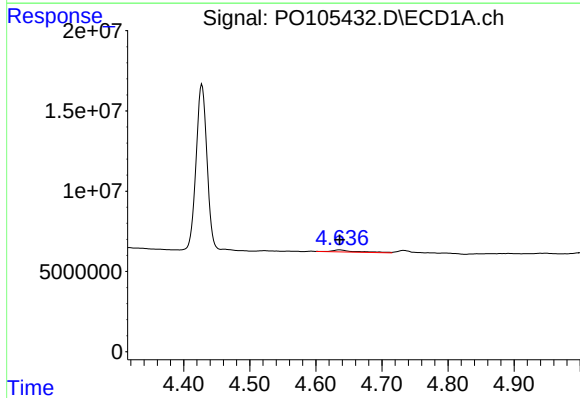


#8 AR-1221-1

R.T.: 4.636 min
Delta R.T.: 0.000 min
Response: 2932073
Conc: 26.15 ng/ml

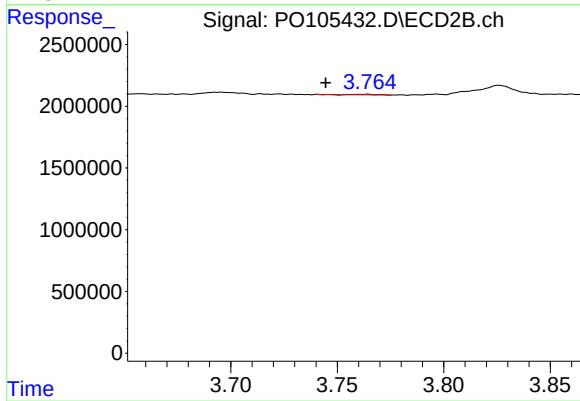

#8 AR-1221-1


R.T.: 3.764 min
Delta R.T.: 0.019 min
Response: 31356
Conc: 0.79 ng/ml

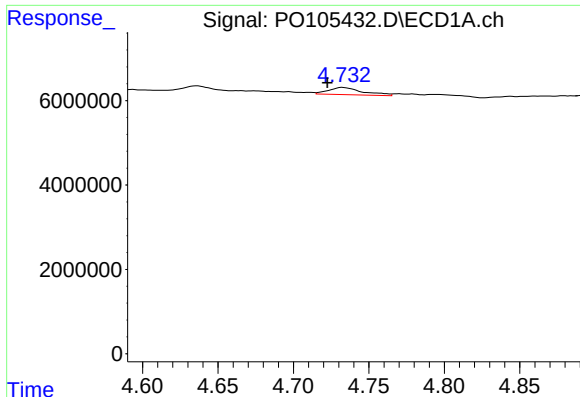

#9 AR-1221-2


R.T.: 4.733 min
Delta R.T.: 0.010 min
Response: 2689392
Conc: 31.73 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

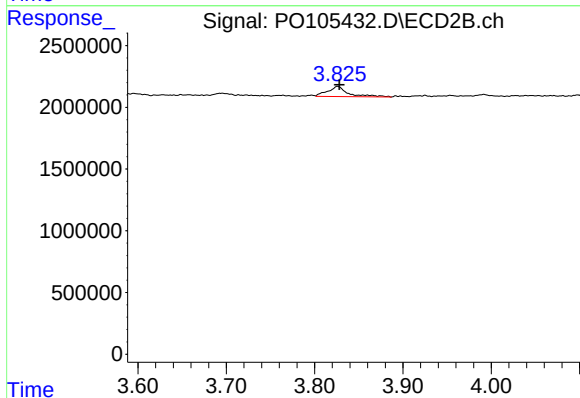


#9 AR-1221-2

R.T.: 3.826 min
Delta R.T.: -0.002 min
Response: 1316723
Conc: 42.86 ng/ml

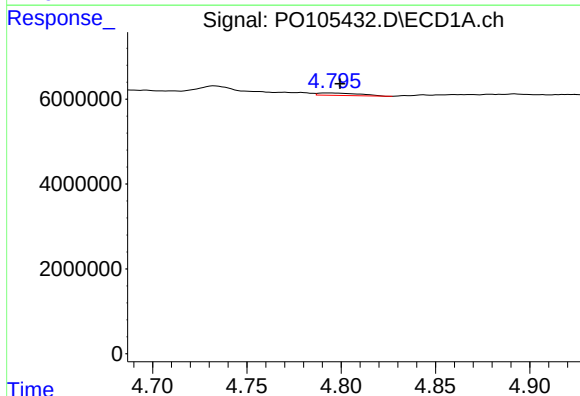


#10 AR-1221-3

R.T.: 4.793 min
Delta R.T.: -0.006 min
Response: 862964
Conc: 3.55 ng/ml

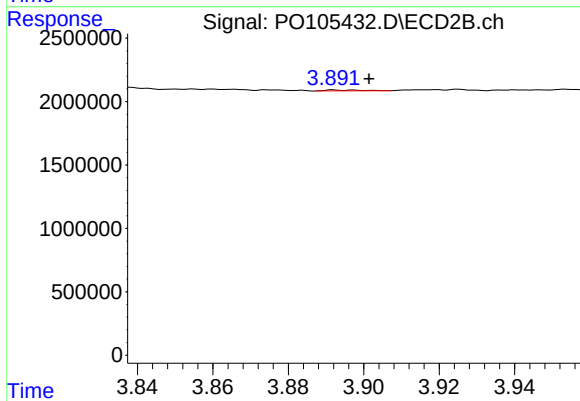

#10 AR-1221-3


R.T.: 3.892 min
Delta R.T.: -0.009 min
Response: 53595
Conc: 0.60 ng/ml

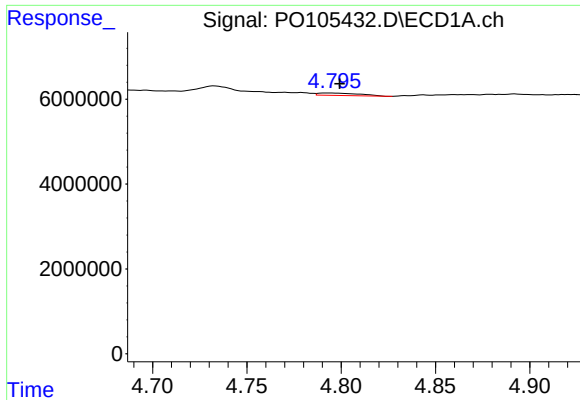

#11 AR-1232-1


R.T.: 4.793 min
Delta R.T.: -0.006 min
Response: 862964
Conc: 4.32 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

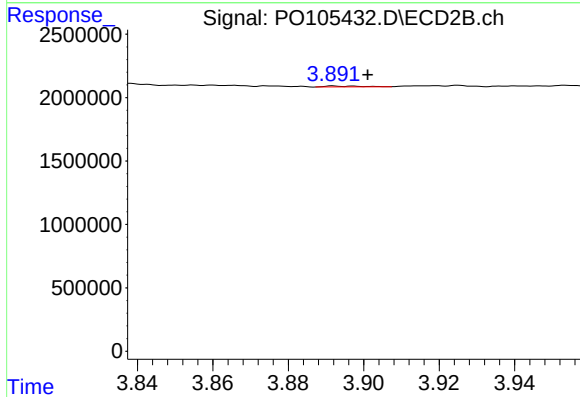


#11 AR-1232-1

R.T.: 3.892 min
Delta R.T.: -0.009 min
Response: 53595
Conc: 0.73 ng/ml

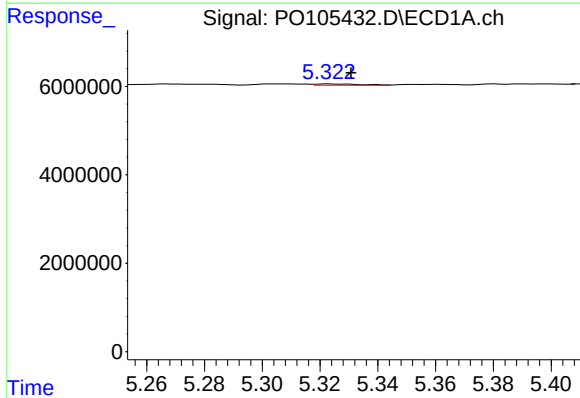


#12 AR-1232-2

R.T.: 5.323 min
Delta R.T.: -0.008 min
Response: 337232
Conc: 3.19 ng/ml

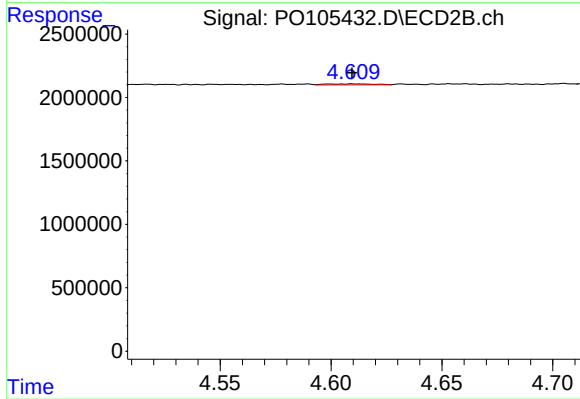

#12 AR-1232-2


R.T.: 4.610 min
Delta R.T.: 0.000 min
Response: 112620
Conc: 1.60 ng/ml

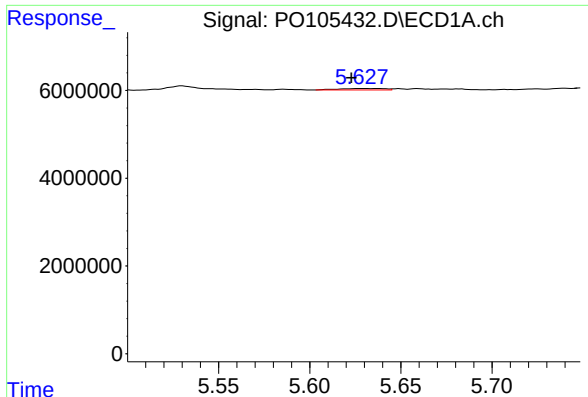

#13 AR-1232-3


R.T.: 5.628 min
Delta R.T.: 0.005 min
Response: 587509
Conc: 3.07 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

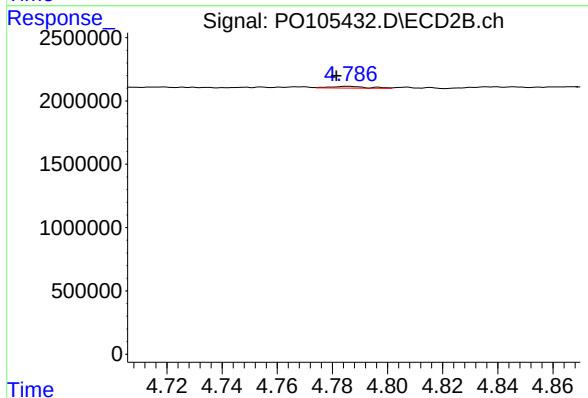


#13 AR-1232-3

R.T.: 4.786 min
Delta R.T.: 0.004 min
Response: 130059
Conc: 3.40 ng/ml

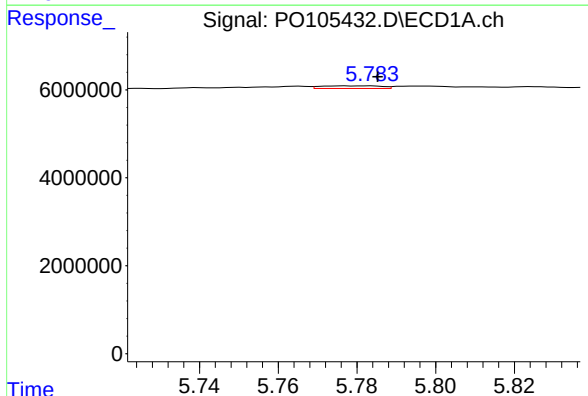


#14 AR-1232-4

R.T.: 5.777 min
Delta R.T.: -0.008 min
Response: 628879
Conc: 6.45 ng/ml

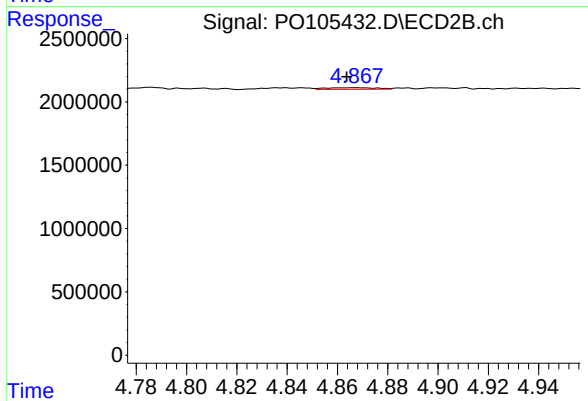

#14 AR-1232-4


R.T.: 4.867 min
Delta R.T.: 0.003 min
Response: 182043
Conc: 5.23 ng/ml

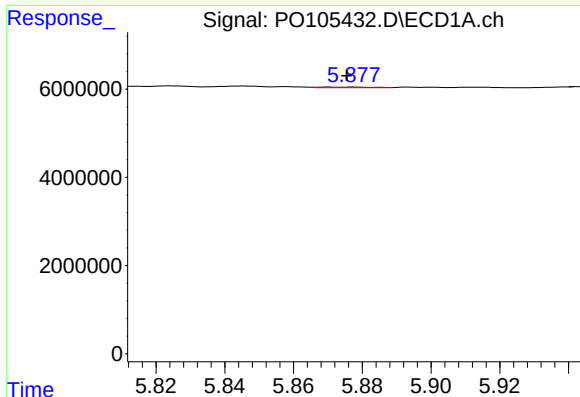

#15 AR-1232-5


R.T.: 5.870 min
Delta R.T.: -0.005 min
Response: 167987
Conc: 2.33 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

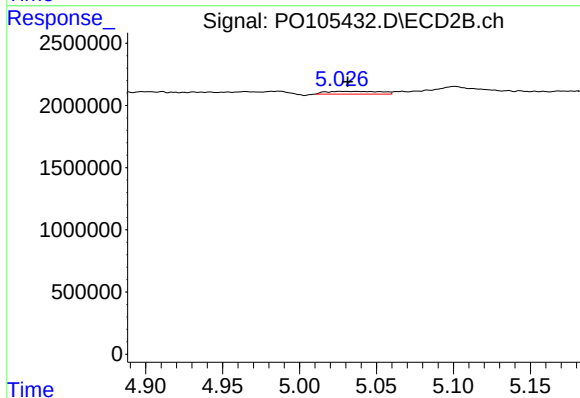


#15 AR-1232-5

R.T.: 5.027 min
Delta R.T.: -0.005 min
Response: 549208
Conc: 15.56 ng/ml

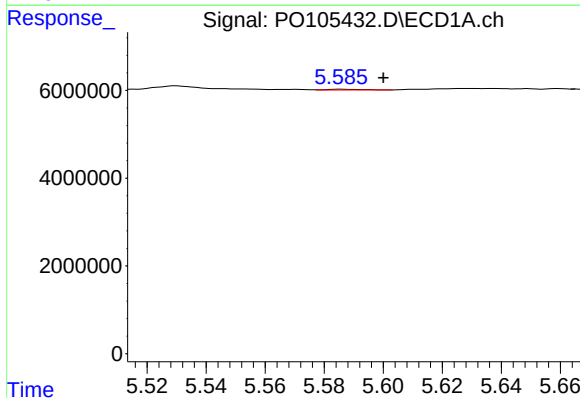


#16 AR-1242-1

R.T.: 5.585 min
Delta R.T.: -0.015 min
Response: 147023
Conc: 0.63 ng/ml

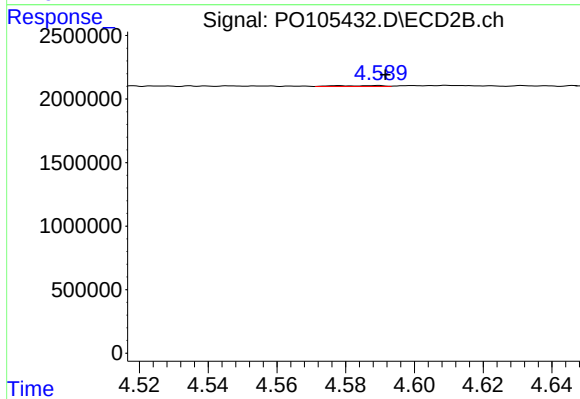

#16 AR-1242-1


R.T.: 4.589 min
Delta R.T.: -0.002 min
Response: 69525
Conc: 0.79 ng/ml

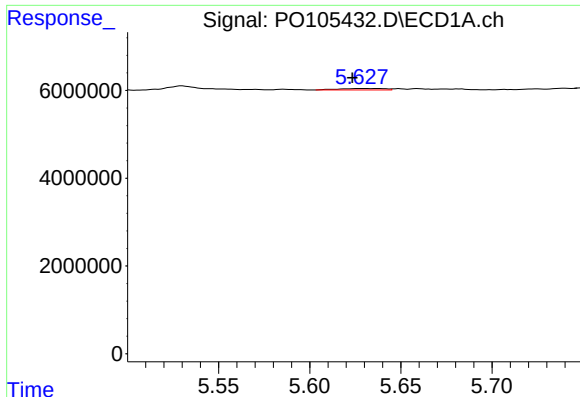

#17 AR-1242-2


R.T.: 5.628 min
Delta R.T.: 0.005 min
Response: 587509
Conc: 1.80 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

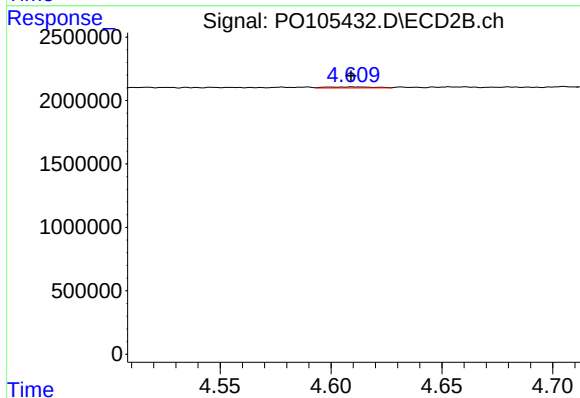


#17 AR-1242-2

R.T.: 4.610 min
Delta R.T.: 0.000 min
Response: 112620
Conc: 0.95 ng/ml

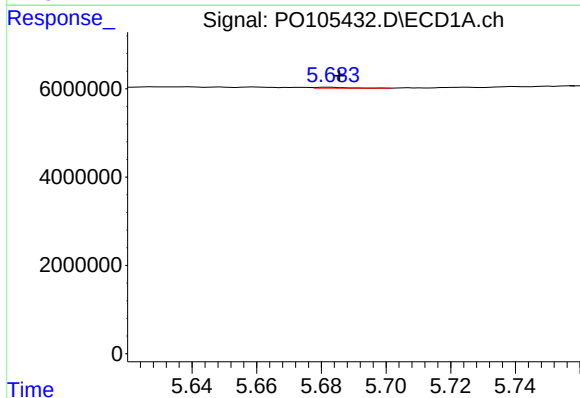


#18 AR-1242-3

R.T.: 5.682 min
Delta R.T.: -0.003 min
Response: 118781
Conc: 0.60 ng/ml

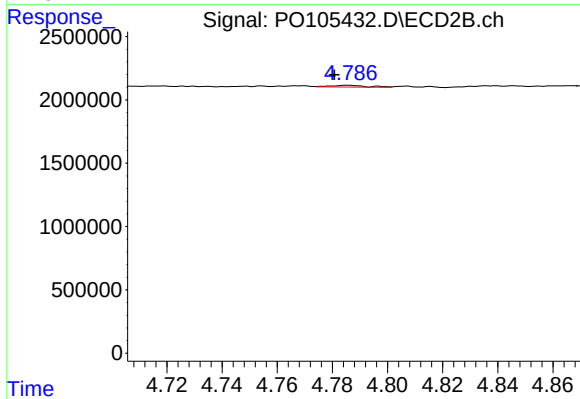

#18 AR-1242-3


R.T.: 4.786 min
Delta R.T.: 0.005 min
Response: 130059
Conc: 2.00 ng/ml

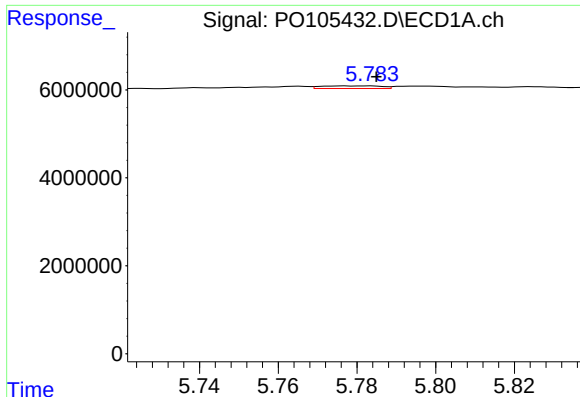

#19 AR-1242-4


R.T.: 5.777 min
Delta R.T.: -0.008 min
Response: 628879
Conc: 3.69 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

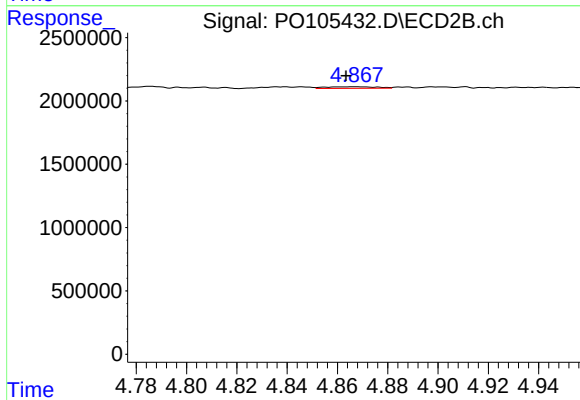


#19 AR-1242-4

R.T.: 4.867 min
Delta R.T.: 0.004 min
Response: 182043
Conc: 2.74 ng/ml

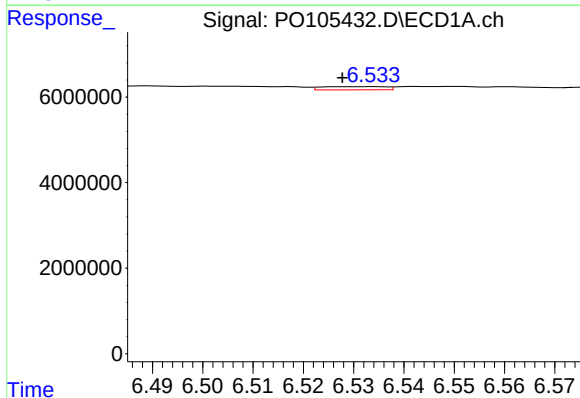


#20 AR-1242-5

R.T.: 6.534 min
Delta R.T.: 0.006 min
Response: 661614
Conc: 3.79 ng/ml

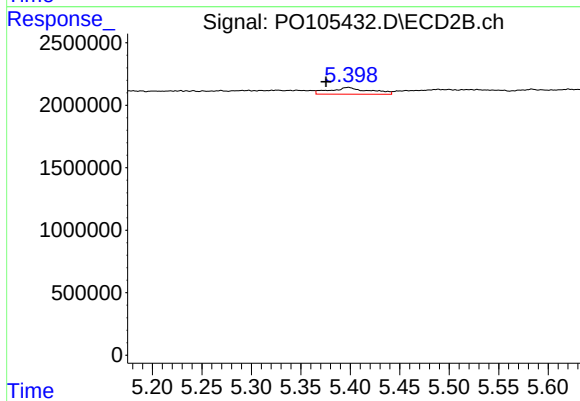

#20 AR-1242-5


R.T.: 5.398 min
Delta R.T.: 0.022 min
Response: 1493847
Conc: 18.18 ng/ml

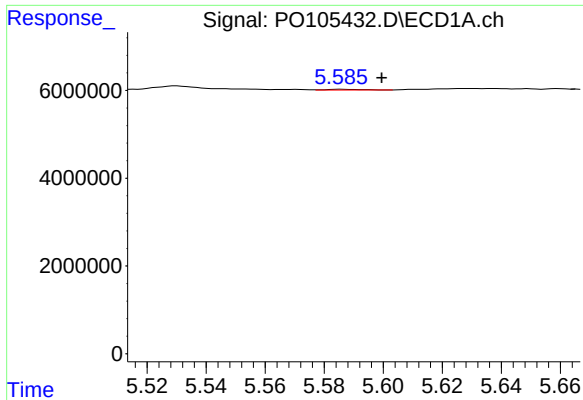

#21 AR-1248-1


R.T.: 5.585 min
Delta R.T.: -0.014 min
Response: 147023
Conc: 0.81 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

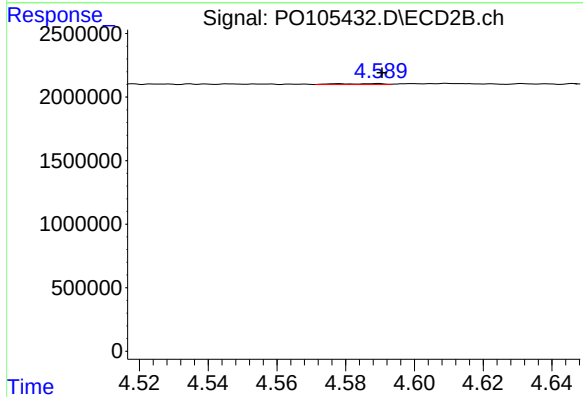


#21 AR-1248-1

R.T.: 4.589 min
Delta R.T.: -0.002 min
Response: 69525
Conc: 1.00 ng/ml

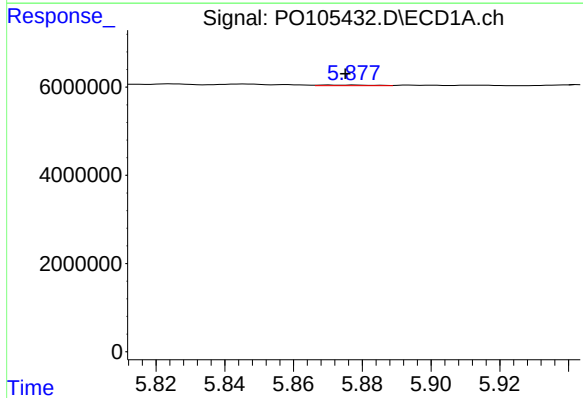


#22 AR-1248-2

R.T.: 5.870 min
Delta R.T.: -0.005 min
Response: 167987
Conc: 0.67 ng/ml

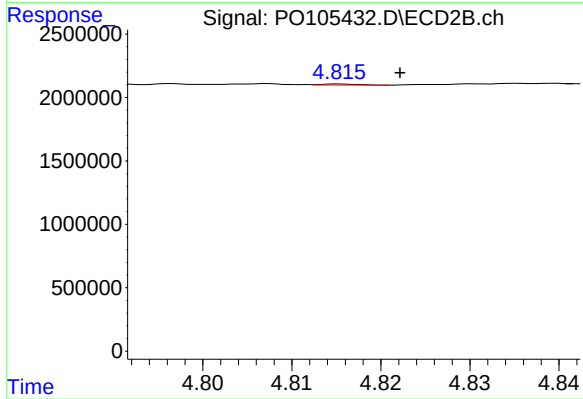

#22 AR-1248-2


R.T.: 4.815 min
Delta R.T.: -0.007 min
Response: 24646
Conc: 0.26 ng/ml

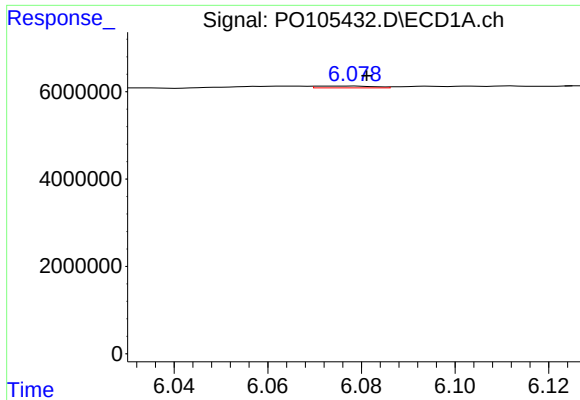

#23 AR-1248-3


R.T.: 6.078 min
Delta R.T.: -0.003 min
Response: 355645
Conc: 1.26 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

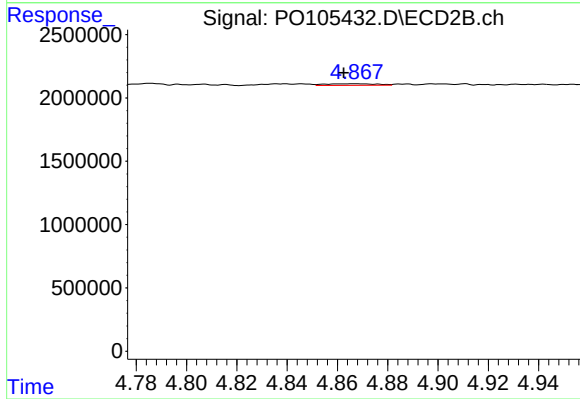


#23 AR-1248-3

R.T.: 4.867 min
Delta R.T.: 0.005 min
Response: 182043
Conc: 1.82 ng/ml

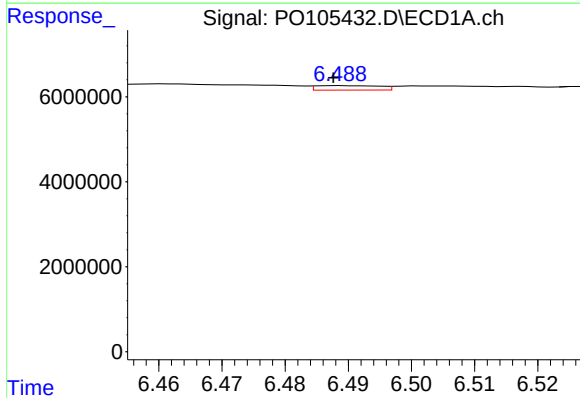


#24 AR-1248-4

R.T.: 6.489 min
Delta R.T.: 0.001 min
Response: 740809
Conc: 2.32 ng/ml

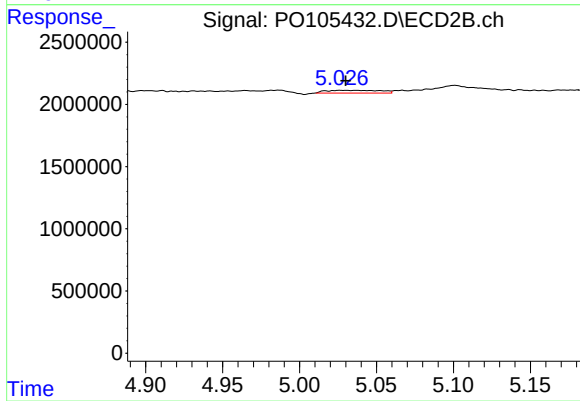

#24 AR-1248-4


R.T.: 5.027 min
Delta R.T.: -0.003 min
Response: 549208
Conc: 4.87 ng/ml

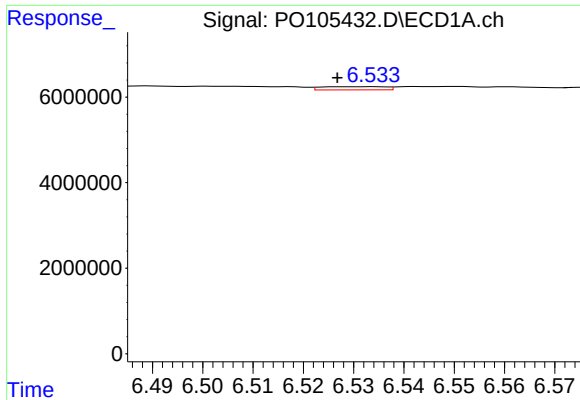

#25 AR-1248-5


R.T.: 6.534 min
Delta R.T.: 0.007 min
Response: 661614
Conc: 2.14 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

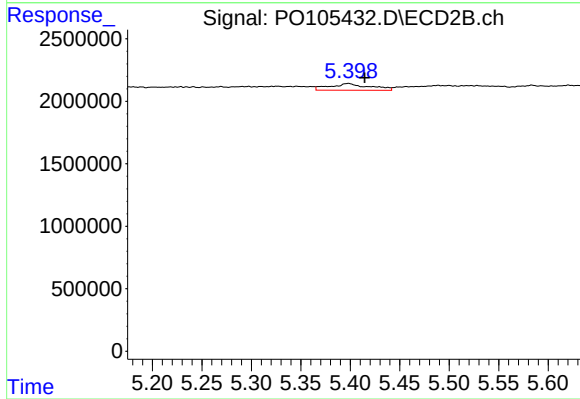


#25 AR-1248-5

R.T.: 5.398 min
Delta R.T.: -0.017 min
Response: 1493847
Conc: 13.27 ng/ml

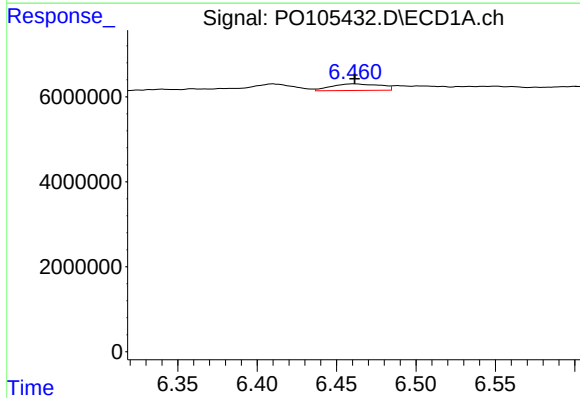


#26 AR-1254-1

R.T.: 6.461 min
Delta R.T.: 0.000 min
Response: 3319741
Conc: 10.59 ng/ml

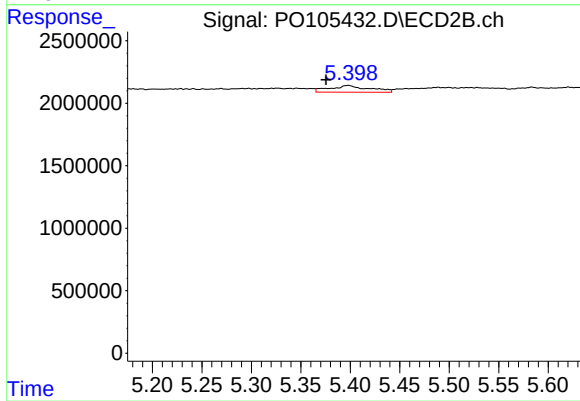

#26 AR-1254-1


R.T.: 5.398 min
Delta R.T.: 0.022 min
Response: 1493847
Conc: 9.18 ng/ml

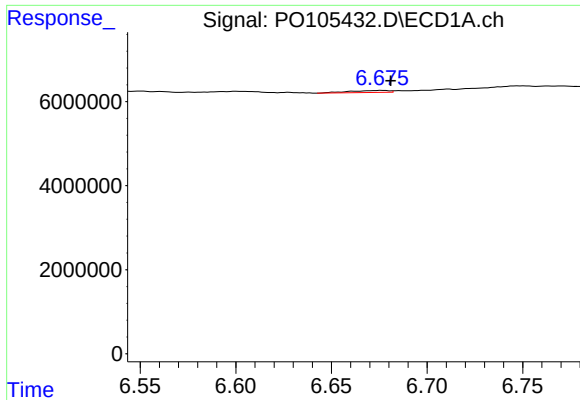

#27 AR-1254-2


R.T.: 6.676 min
Delta R.T.: -0.005 min
Response: 687500
Conc: 1.52 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

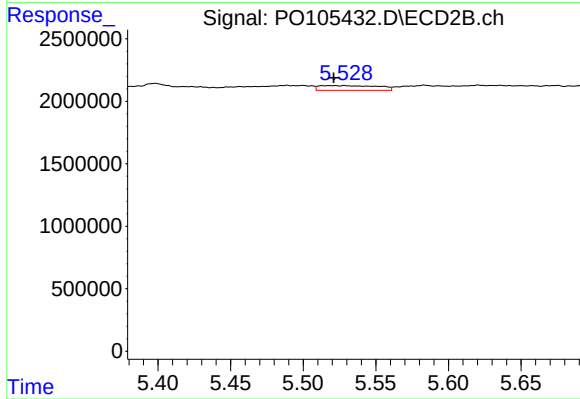


#27 AR-1254-2

R.T.: 5.528 min
Delta R.T.: 0.007 min
Response: 1067652
Conc: 7.30 ng/ml

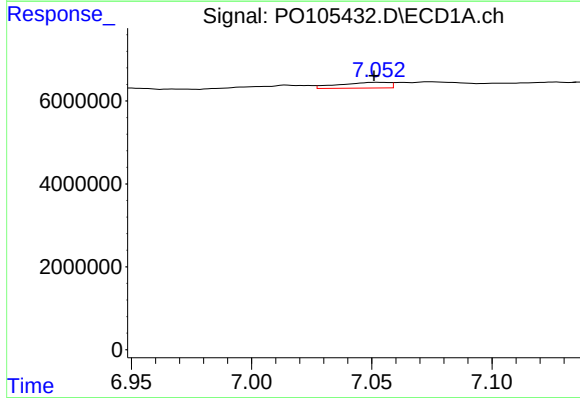


#28 AR-1254-3

R.T.: 7.053 min
Delta R.T.: 0.001 min
Response: 2024623
Conc: 4.27 ng/ml

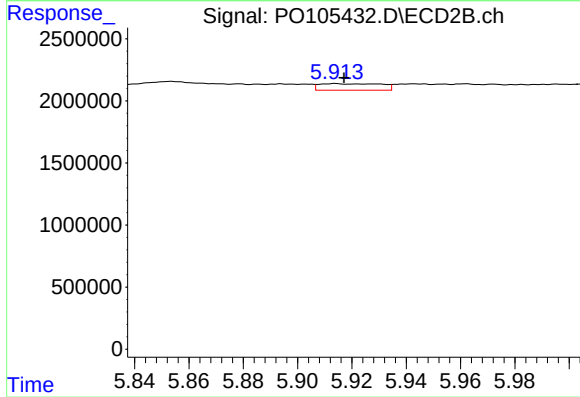

#28 AR-1254-3


R.T.: 5.914 min
Delta R.T.: -0.003 min
Response: 836121
Conc: 3.71 ng/ml

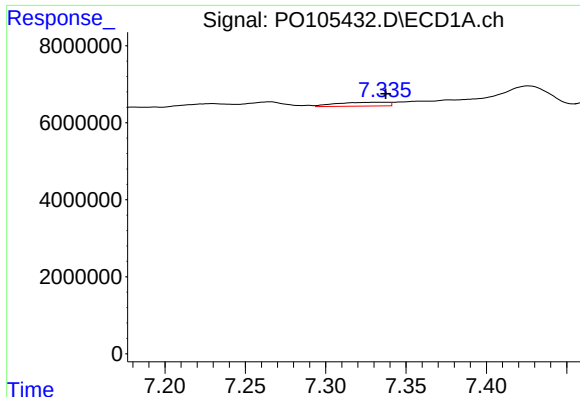

#29 AR-1254-4


R.T.: 7.336 min
Delta R.T.: -0.001 min
Response: 2215654
Conc: 6.19 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

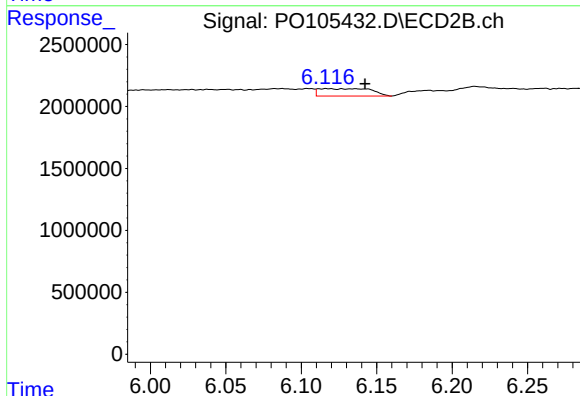


#29 AR-1254-4

R.T.: 6.117 min
Delta R.T.: -0.025 min
Response: 1441078
Conc: 10.21 ng/ml

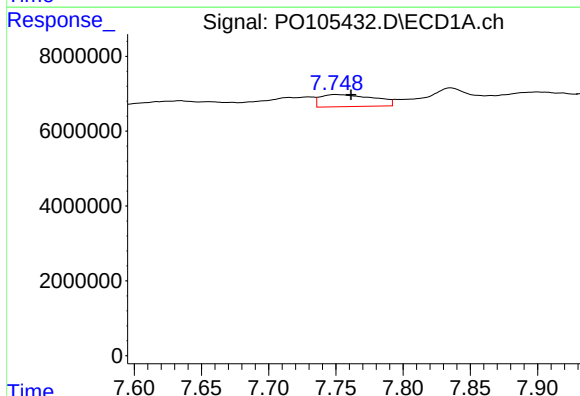


#30 AR-1254-5

R.T.: 7.750 min
Delta R.T.: -0.012 min
Response: 8905431
Conc: 22.43 ng/ml

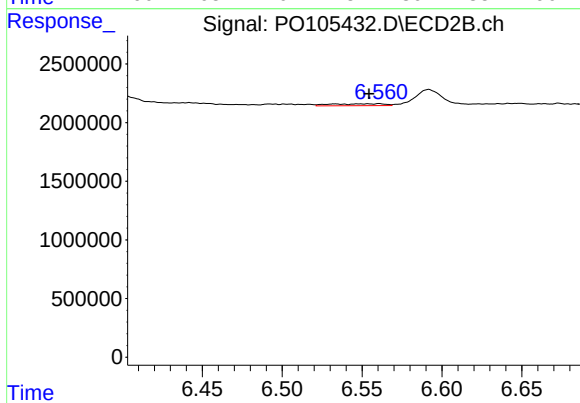

#30 AR-1254-5


R.T.: 6.561 min
Delta R.T.: 0.006 min
Response: 383926
Conc: 1.92 ng/ml

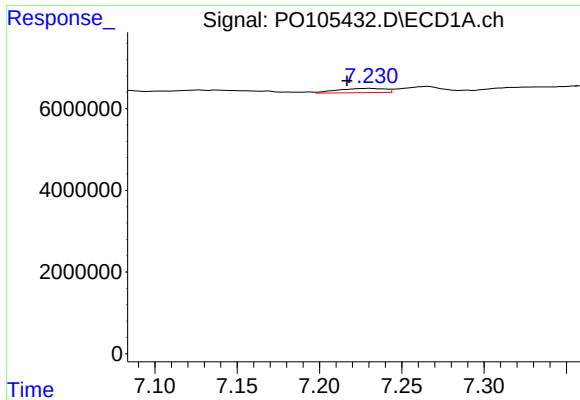

#31 AR-1260-1


R.T.: 7.230 min
Delta R.T.: 0.014 min
Response: 2166575
Conc: 5.91 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

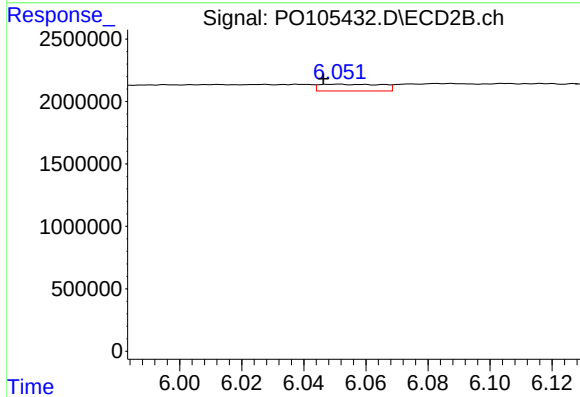


#31 AR-1260-1

R.T.: 6.051 min
Delta R.T.: 0.005 min
Response: 748721
Conc: 4.80 ng/ml

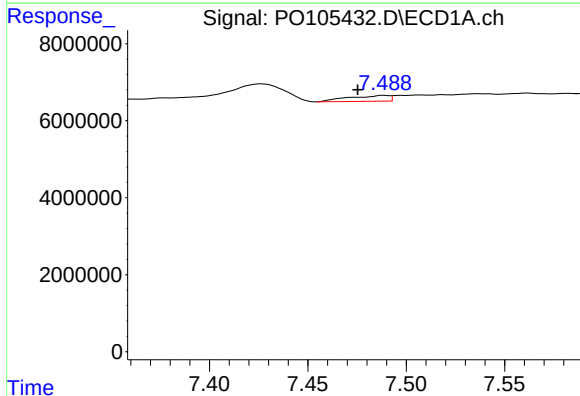


#32 AR-1260-2

R.T.: 7.489 min
Delta R.T.: 0.013 min
Response: 2149038
Conc: 5.16 ng/ml

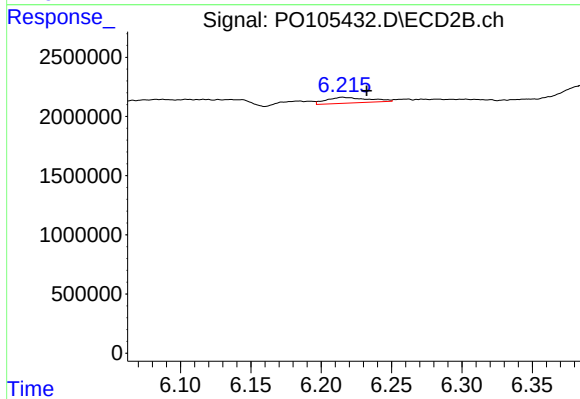

#32 AR-1260-2


R.T.: 6.215 min
Delta R.T.: -0.017 min
Response: 1005860
Conc: 5.32 ng/ml

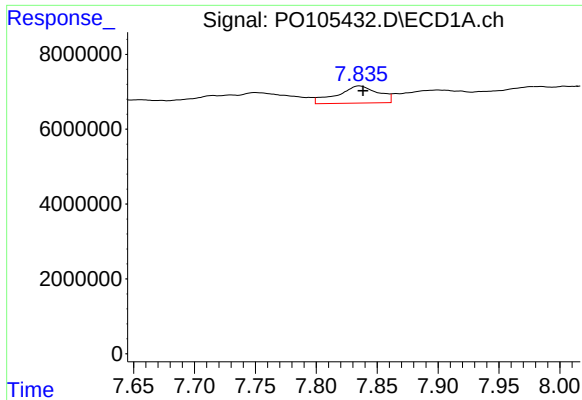

#33 AR-1260-3


R.T.: 7.835 min
Delta R.T.: -0.003 min
Response: 10722248
Conc: 41.43 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

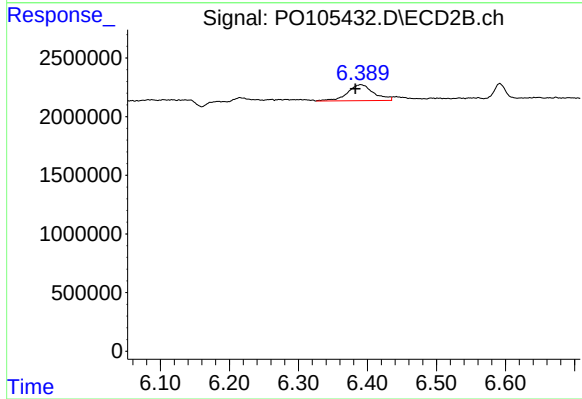


#33 AR-1260-3

R.T.: 6.390 min
Delta R.T.: 0.008 min
Response: 3585431
Conc: 19.41 ng/ml

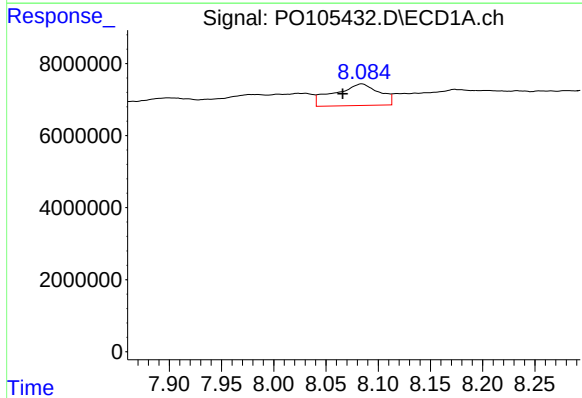


#34 AR-1260-4

R.T.: 8.085 min
Delta R.T.: 0.018 min
Response: 18058673
Conc: 54.73 ng/ml

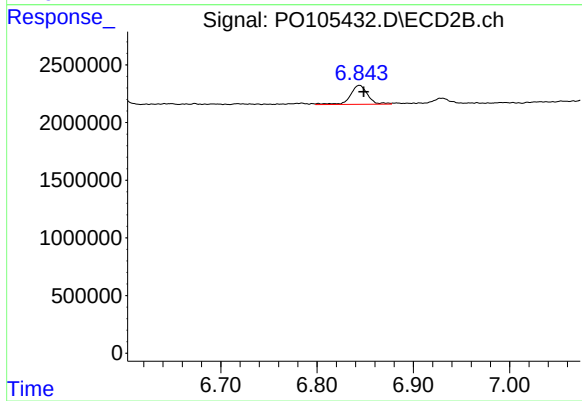

#34 AR-1260-4


R.T.: 6.844 min
Delta R.T.: -0.004 min
Response: 2029244
Conc: 16.60 ng/ml

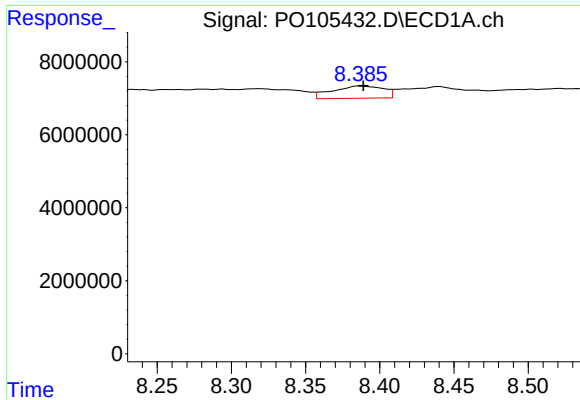

#35 AR-1260-5


R.T.: 8.386 min
Delta R.T.: -0.002 min
Response: 8034833
Conc: 13.51 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

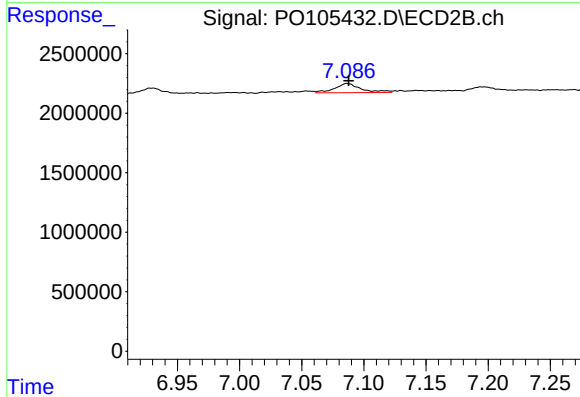


#35 AR-1260-5

R.T.: 7.087 min
Delta R.T.: -0.001 min
Response: 1144624
Conc: 4.11 ng/ml

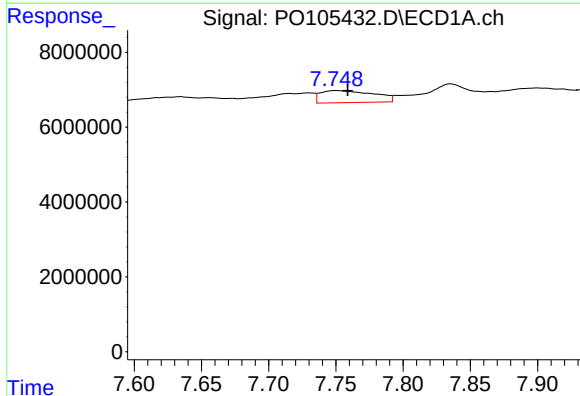


#36 AR-1262-1

R.T.: 7.750 min
Delta R.T.: -0.009 min
Response: 8905431
Conc: 28.04 ng/ml

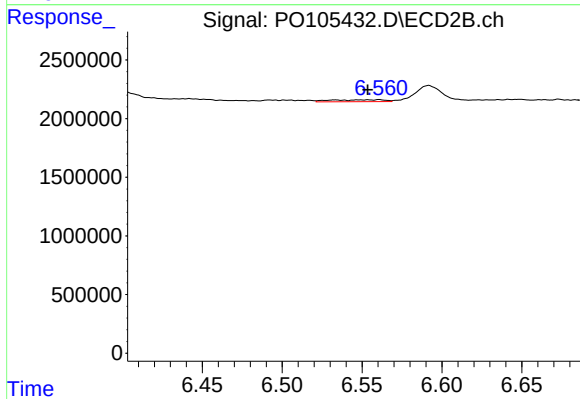

#36 AR-1262-1


R.T.: 6.561 min
Delta R.T.: 0.007 min
Response: 383926
Conc: 3.61 ng/ml

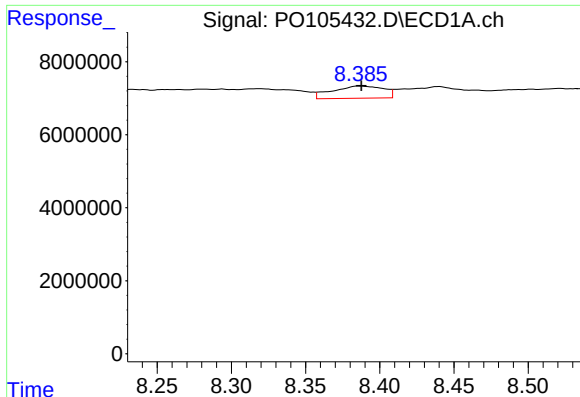

#37 AR-1262-2


R.T.: 8.386 min
Delta R.T.: -0.001 min
Response: 8034833
Conc: 10.68 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

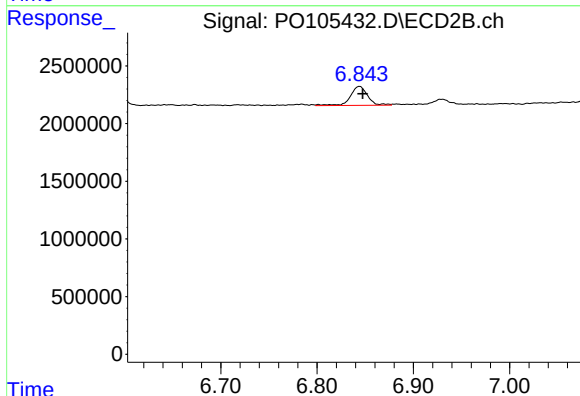


#37 AR-1262-2

R.T.: 6.844 min
Delta R.T.: -0.004 min
Response: 2029244
Conc: 11.94 ng/ml

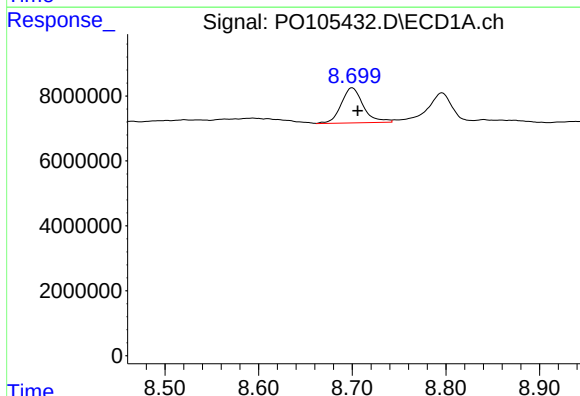


#38 AR-1262-3

R.T.: 8.700 min
Delta R.T.: -0.006 min
Response: 17618129
Conc: 35.80 ng/ml

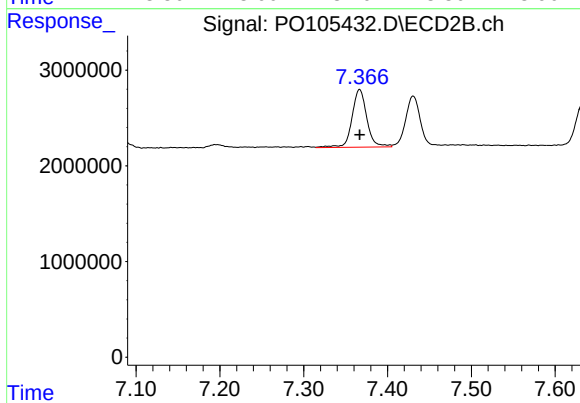

#38 AR-1262-3


R.T.: 7.367 min
Delta R.T.: 0.000 min
Response: 7429336
Conc: 58.85 ng/ml

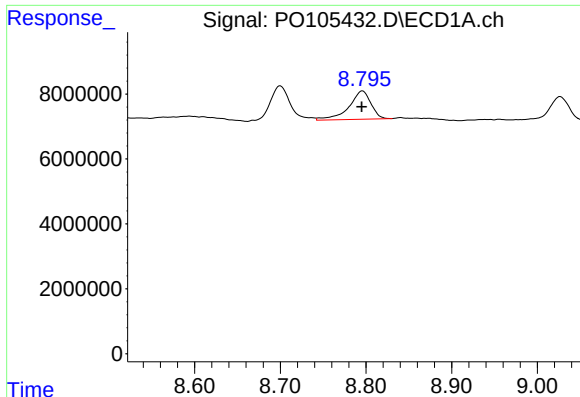

#39 AR-1262-4


R.T.: 8.796 min
Delta R.T.: 0.000 min
Response: 15883463
Conc: 43.25 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

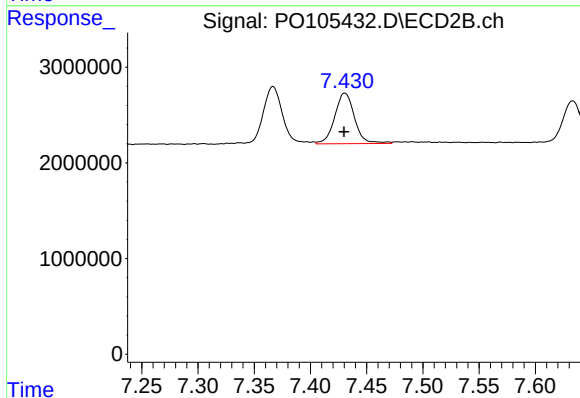


#39 AR-1262-4

R.T.: 7.431 min
Delta R.T.: 0.000 min
Response: 6512737
Conc: 28.13 ng/ml

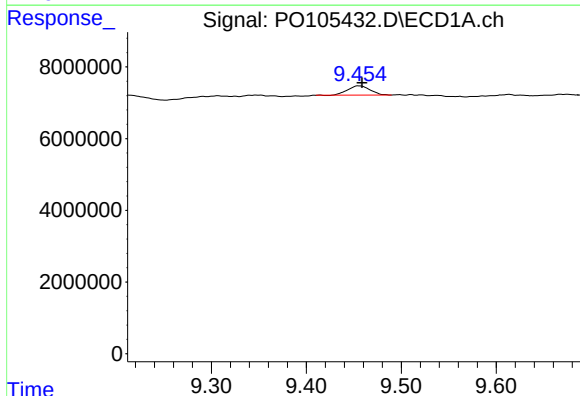


#40 AR-1262-5

R.T.: 9.455 min
Delta R.T.: -0.004 min
Response: 4259013
Conc: 15.90 ng/ml

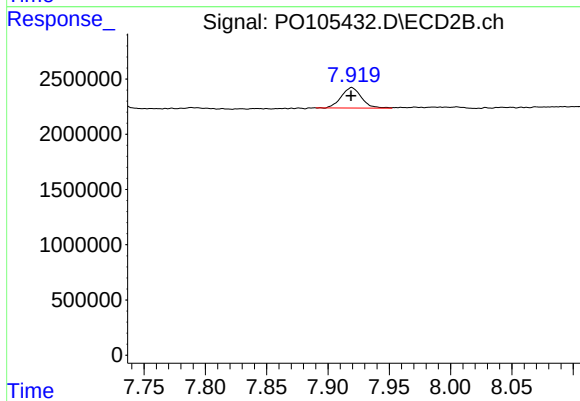

#40 AR-1262-5


R.T.: 7.919 min
Delta R.T.: 0.000 min
Response: 2112597
Conc: 21.02 ng/ml

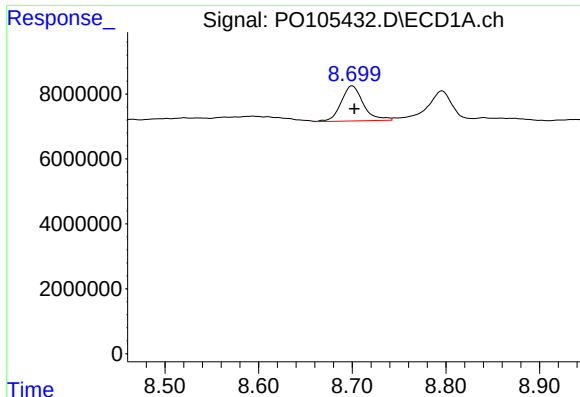

#41 AR-1268-1


R.T.: 8.700 min
Delta R.T.: -0.002 min
Response: 17618129
Conc: 21.66 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

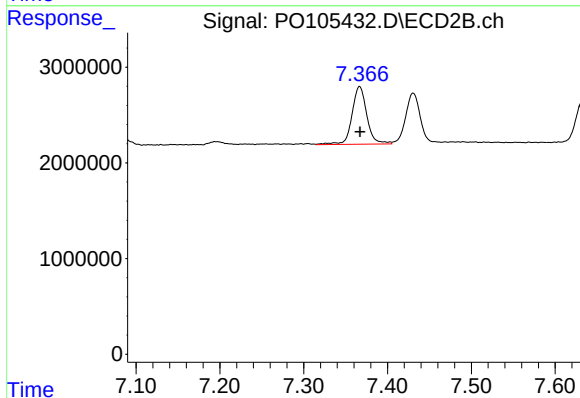


#41 AR-1268-1

R.T.: 7.367 min
Delta R.T.: 0.000 min
Response: 7429336
Conc: 21.28 ng/ml

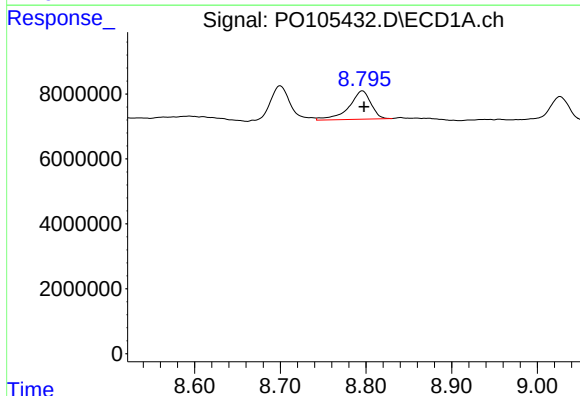


#42 AR-1268-2

R.T.: 8.796 min
Delta R.T.: -0.002 min
Response: 15883463
Conc: 21.85 ng/ml

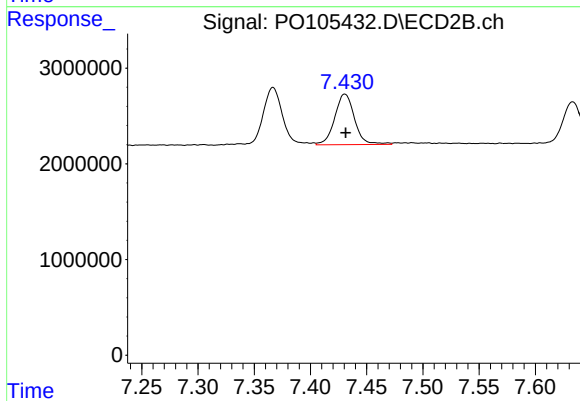

#42 AR-1268-2


R.T.: 7.431 min
Delta R.T.: 0.000 min
Response: 6512737
Conc: 20.88 ng/ml

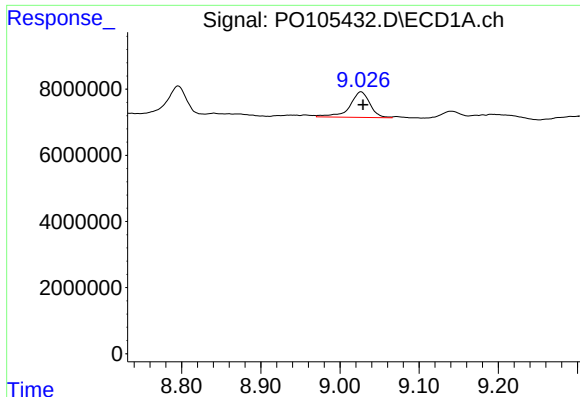

#43 AR-1268-3


R.T.: 9.027 min
Delta R.T.: -0.003 min
Response: 13692004
Conc: 21.21 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

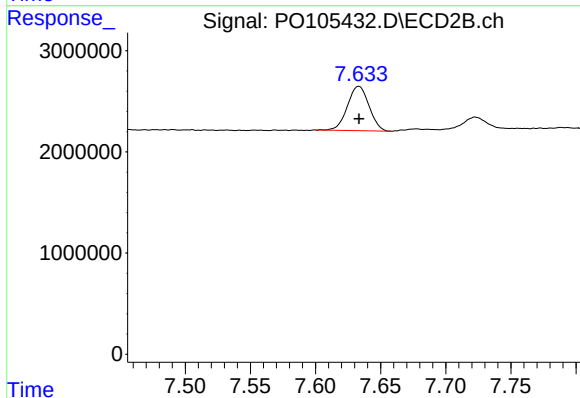


#43 AR-1268-3

R.T.: 7.633 min
Delta R.T.: 0.000 min
Response: 5067725
Conc: 20.05 ng/ml

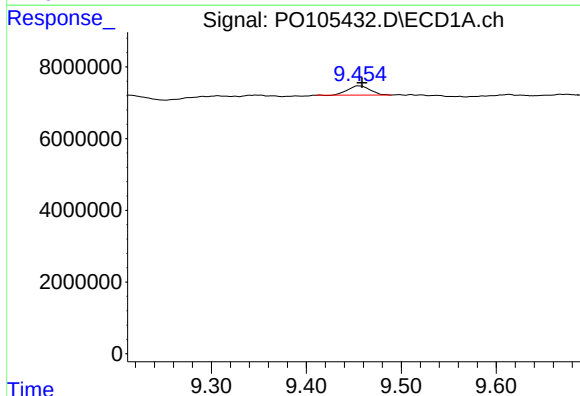


#44 AR-1268-4

R.T.: 9.455 min
Delta R.T.: -0.003 min
Response: 4259013
Conc: 15.30 ng/ml

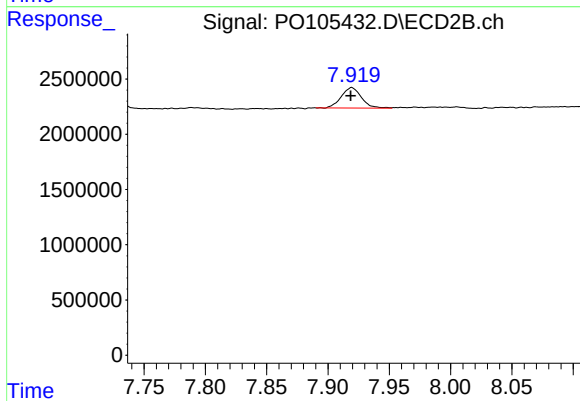

#44 AR-1268-4


R.T.: 7.919 min
Delta R.T.: 0.000 min
Response: 2112597
Conc: 19.64 ng/ml

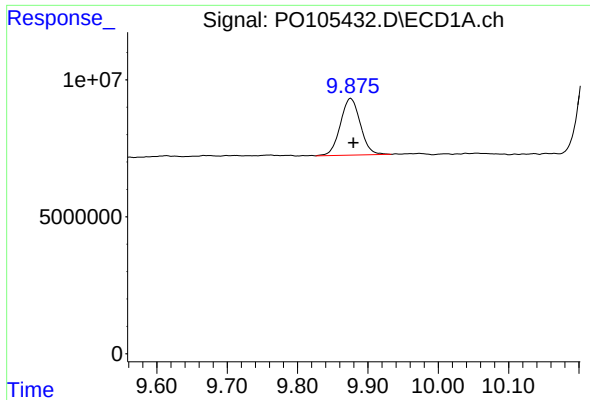

#45 AR-1268-5

R.T.: 9.876 min
Delta R.T.: -0.004 min
Response: 40809866
Conc: 19.52 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

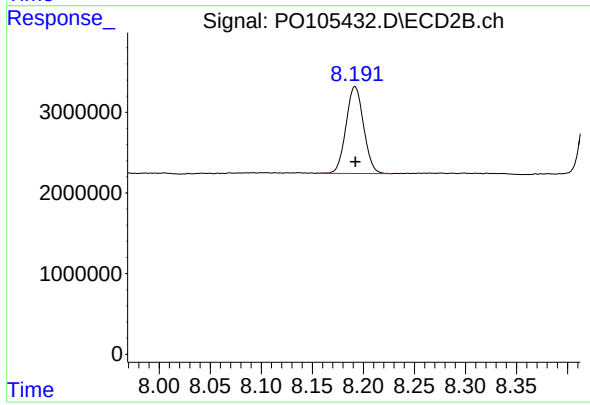

#45 AR-1268-5

R.T.: 8.192 min
Delta R.T.: 0.000 min
Response: 12924012
Conc: 19.32 ng/ml