

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0081224\
 Data File : P0105446.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2024 23:19
 Operator : YP/AJ
 Sample : P3390-07
 Misc : AR1660 LOD 40 PPB
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 02:40:09 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0081024.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 10 04:08:56 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.427	3.536	168.8E6	62966655	19.331	20.047
2)	SA Decachlor...	10.217	8.426	124.9E6	38425478	21.704	21.705
Target Compounds							
3)	L1 AR-1016-1	5.598	4.590	8023724	3301647	26.524	29.379
4)	L1 AR-1016-2	5.621	4.607	11337746	4342830	26.521	27.895
5)	L1 AR-1016-3	5.683	4.779	6770325	2339517	26.386	27.936
6)	L1 AR-1016-4	5.783	4.821	7123134	1901160	32.569	28.233
7)	L1 AR-1016-5	6.079	5.029	6696498	2543157	31.299	30.387
8)	L2 AR-1221-1	4.630	3.741	1100443	319070	9.813	8.083
9)	L2 AR-1221-2	4.732	3.826	3592011	1482694	42.378	48.261
10)	L2 AR-1221-3	4.797	3.899	4533263	1785637	18.634	19.955
11)	L3 AR-1232-1	4.797	3.899	4533263	1785637	22.673	24.451
12)	L3 AR-1232-2	5.327	4.607	5705570	4342830	53.902	61.851
13)	L3 AR-1232-3	5.621	4.779	11337746	2339517	59.233	61.216
14)	L3 AR-1232-4	5.783	4.861	7123134	2481648	73.032	71.332
15)	L3 AR-1232-5	5.873	5.029	5263400	2543157	73.039	72.047
16)	L4 AR-1242-1	5.598	4.590	8023724	3301647	34.525	37.434
17)	L4 AR-1242-2	5.621	4.607	11337746	4342830	34.788	36.577
18)	L4 AR-1242-3	5.683	4.779	6770325	2339517	34.319	36.028
19)	L4 AR-1242-4	5.783	4.861	7123134	2481648	41.748	37.418
20)	L4 AR-1242-5	6.524	5.374	3530210	3379660	20.200	41.129 #
21)	L5 AR-1248-1	5.598	4.590	8023724	3301647	43.942	47.273
22)	L5 AR-1248-2	5.873	4.821	5263400	1901160	20.897	20.034
23)	L5 AR-1248-3	6.079	4.861	6696498	2481648	23.690	24.860
24)	L5 AR-1248-4	6.484	5.029	3609393	2543157	11.288	22.532 #
25)	L5 AR-1248-5	6.524	5.414	3530210	924366	11.413	8.209 #
26)	L6 AR-1254-1	6.460	5.374	7586255	3379660	24.191	20.759
27)	L6 AR-1254-2	6.679	5.519	5381518	3101689	11.925	21.204 #
28)	L6 AR-1254-3	7.049	5.931	5364390	4868770	11.308	21.584 #
29)	L6 AR-1254-4	7.339	6.139	8218443	1481480	22.943	10.499 #
30)	L6 AR-1254-5	7.757	6.552	27413058	6019289	69.056	30.045 #
31)	L7 AR-1260-1	7.215	6.044	13156733	7924651	35.897	50.768 #
32)	L7 AR-1260-2	7.473	6.230	15861455	6680930	38.095	35.349
33)	L7 AR-1260-3	7.835	6.381	18016564	7958130	69.611	43.079 #
34)	L7 AR-1260-4	8.063	6.846	26539089	4160644	80.439	34.040 #
35)	L7 AR-1260-5	8.385	7.086	26804147	9157274	45.059	32.902 #
36)	L8 AR-1262-1	7.757	6.552	27413058	6019289	86.304	56.571 #
37)	L8 AR-1262-2	8.385	6.846	26804147	4160644	35.635	24.485 #
38)	L8 AR-1262-3	8.714	7.365	13208229	2287081	26.841	18.115 #
39)	L8 AR-1262-4	8.791	7.428	3150207	6619376	8.579	28.595 #
40)	L8 AR-1262-5	9.454	7.918	4331938	2055473	16.175	20.452 #
41)	L9 AR-1268-1	8.714	7.365	13208229	2287081	16.240	6.551 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081224\
Data File : P0105446.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Aug 2024 23:19
Operator : YP/AJ
Sample : P3390-07
Misc : AR1660 LOD 40 PPB
ALS Vial : 42 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 13 02:40:09 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081024.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Aug 10 04:08:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.791	7.428	3150207	6619376	4.334	21.217 #
43) L9	AR-1268-3	9.009	7.630	1250358	591221	1.937	2.339
44) L9	AR-1268-4	9.454	7.918	4331938	2055473	15.557	19.111
45) L9	AR-1268-5	9.875	8.190	3047029	770690	1.457	1.152



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081224\
Data File : PO105446.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Aug 2024 23:19
Operator : YP/AJ
Sample : P3390-07
Misc : AR1660 LOD 40 PPB
ALS Vial : 42 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 13 02:40:09 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081024.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Aug 10 04:08:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

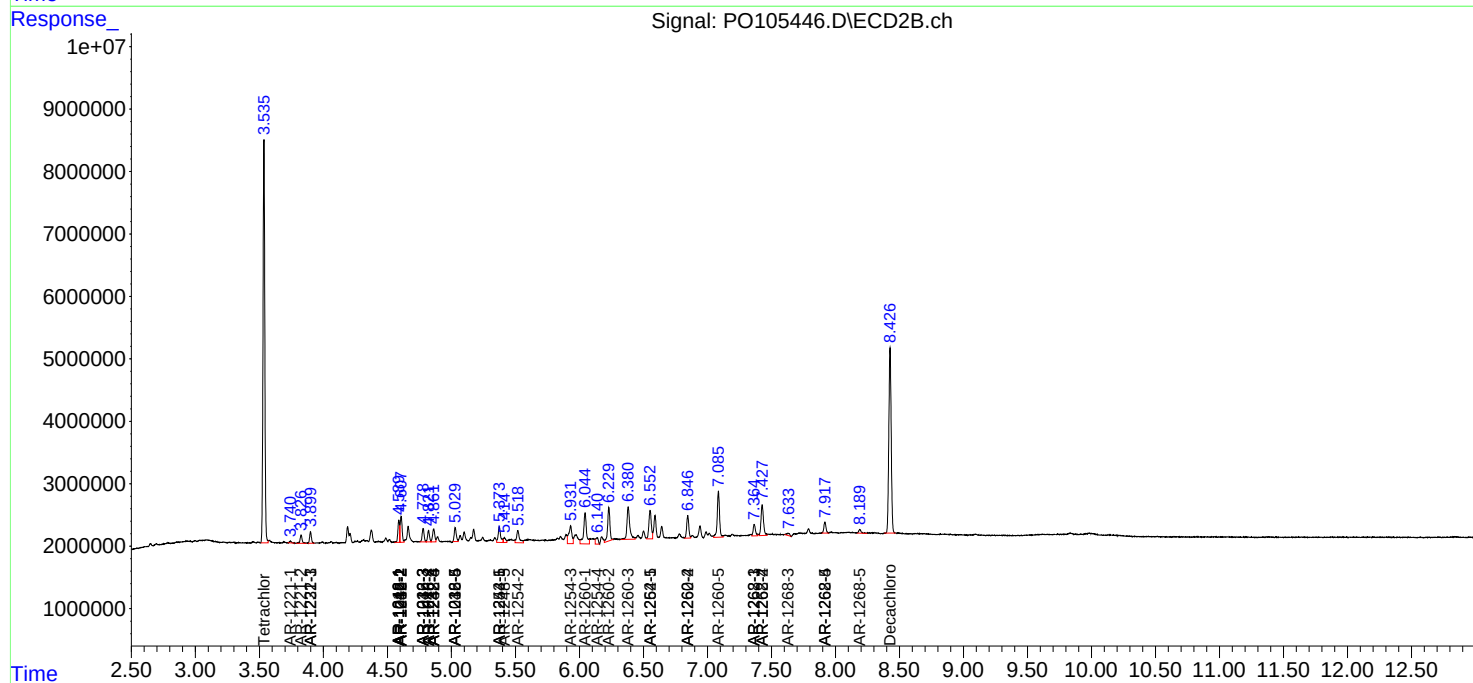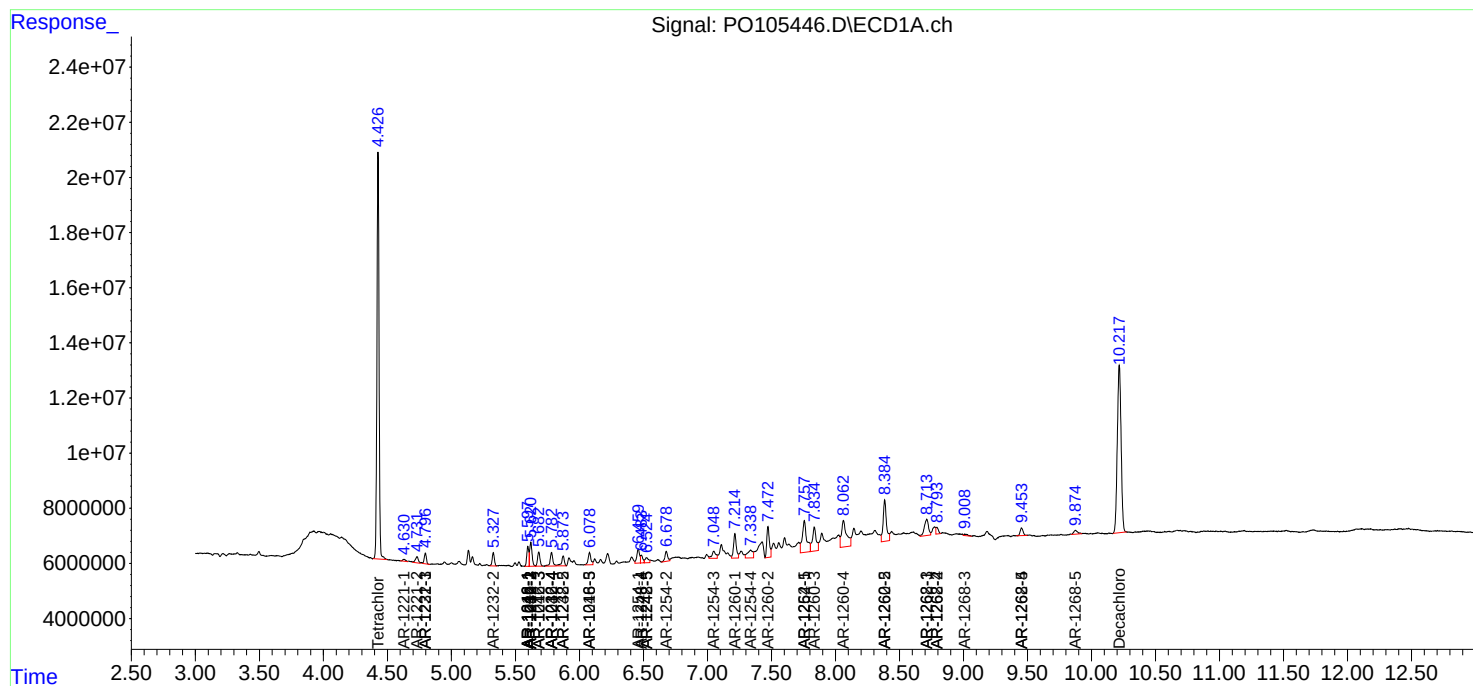


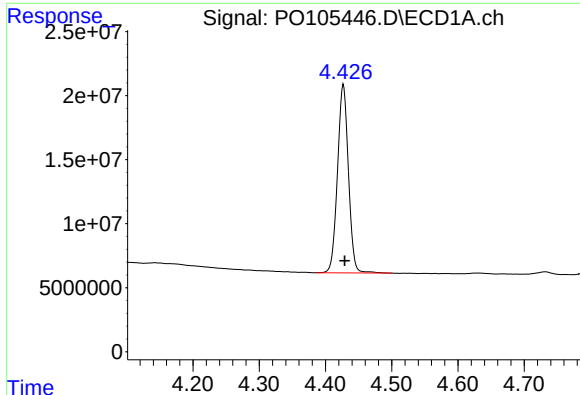

#1 Tetrachloro-m-xylene


R.T.: 4.427 min
Delta R.T.: -0.002 min
Response: 168843940
Conc: 19.33 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

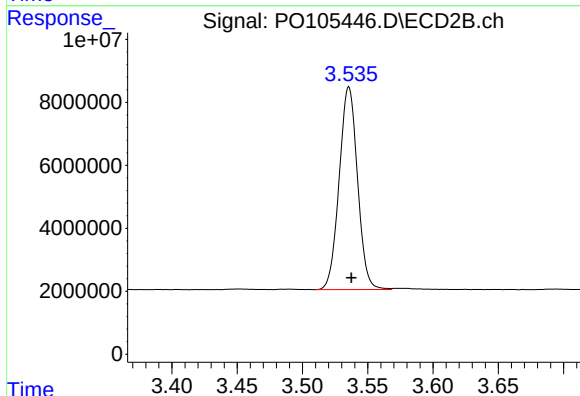


#1 Tetrachloro-m-xylene

R.T.: 3.536 min
Delta R.T.: -0.002 min
Response: 62966655
Conc: 20.05 ng/ml

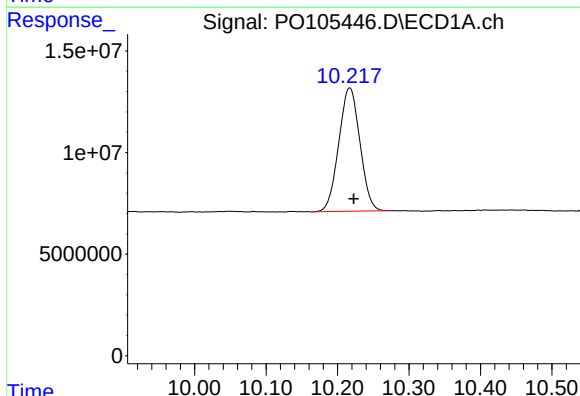


#2 Decachlorobiphenyl

R.T.: 10.217 min
Delta R.T.: -0.005 min
Response: 124852327
Conc: 21.70 ng/ml

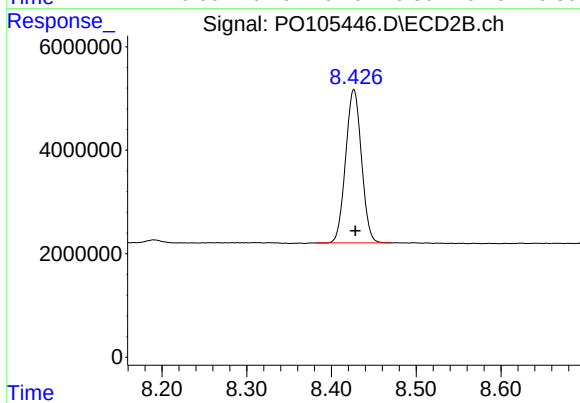

#2 Decachlorobiphenyl


R.T.: 8.426 min
Delta R.T.: -0.002 min
Response: 38425478
Conc: 21.70 ng/ml

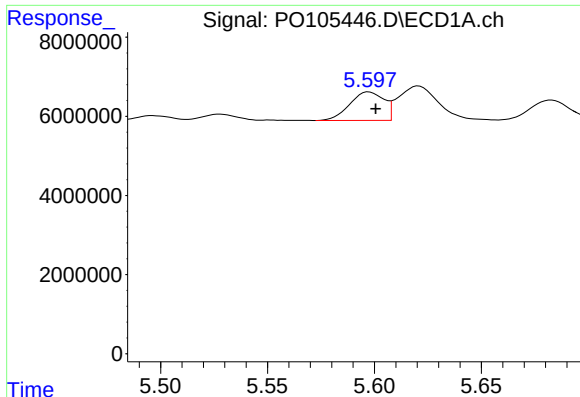

#3 AR-1016-1


R.T.: 5.598 min
Delta R.T.: -0.003 min
Response: 8023724
Conc: 26.52 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

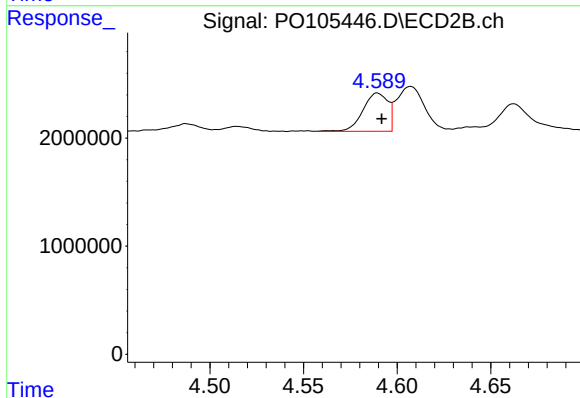


#3 AR-1016-1

R.T.: 4.590 min
Delta R.T.: -0.002 min
Response: 3301647
Conc: 29.38 ng/ml

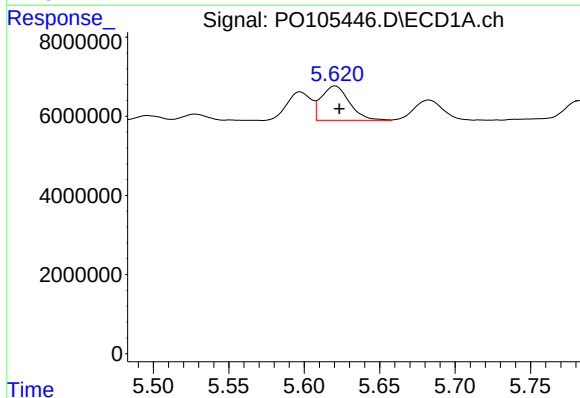


#4 AR-1016-2

R.T.: 5.621 min
Delta R.T.: -0.003 min
Response: 11337746
Conc: 26.52 ng/ml

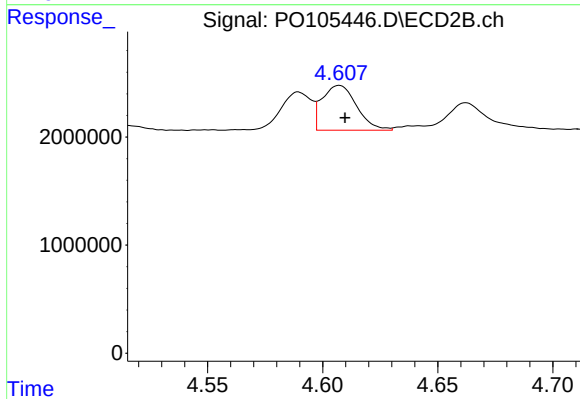

#4 AR-1016-2


R.T.: 4.607 min
Delta R.T.: -0.003 min
Response: 4342830
Conc: 27.89 ng/ml

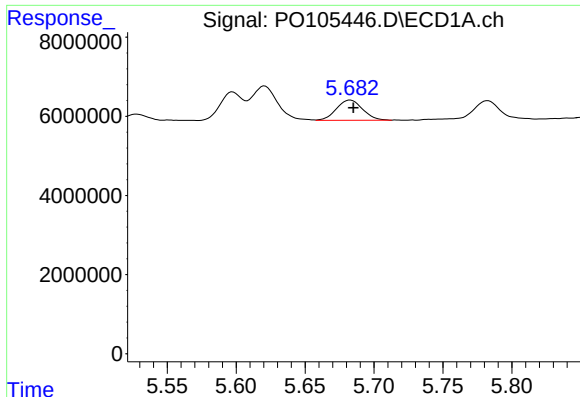

#5 AR-1016-3


R.T.: 5.683 min
Delta R.T.: -0.002 min
Response: 6770325
Conc: 26.39 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

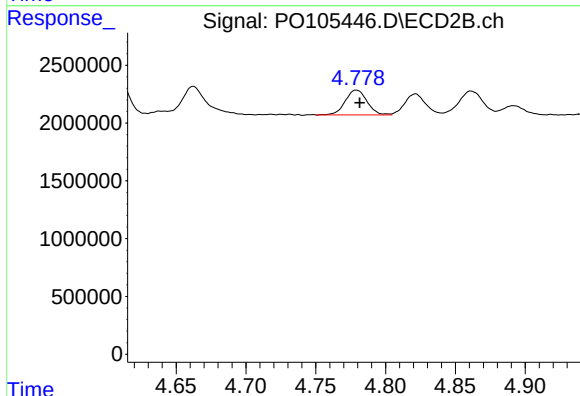


#5 AR-1016-3

R.T.: 4.779 min
Delta R.T.: -0.002 min
Response: 2339517
Conc: 27.94 ng/ml

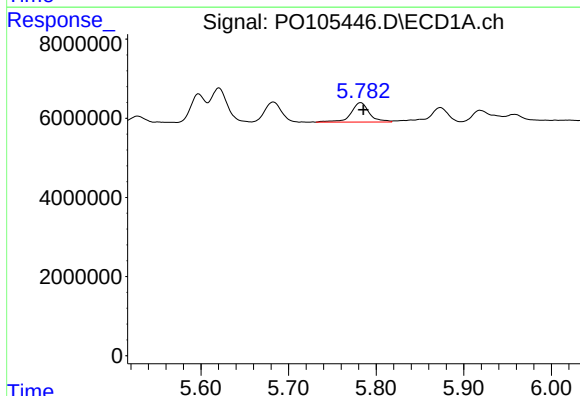


#6 AR-1016-4

R.T.: 5.783 min
Delta R.T.: -0.003 min
Response: 7123134
Conc: 32.57 ng/ml

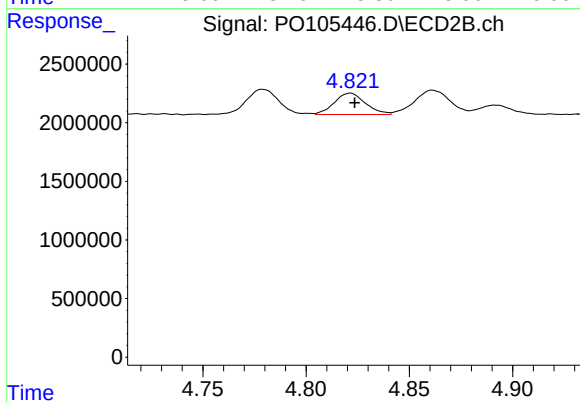

#6 AR-1016-4


R.T.: 4.821 min
Delta R.T.: -0.002 min
Response: 1901160
Conc: 28.23 ng/ml

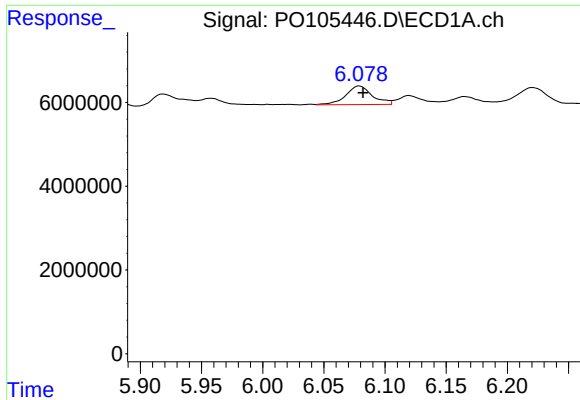

#7 AR-1016-5


R.T.: 6.079 min
Delta R.T.: -0.003 min
Response: 6696498
Conc: 31.30 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

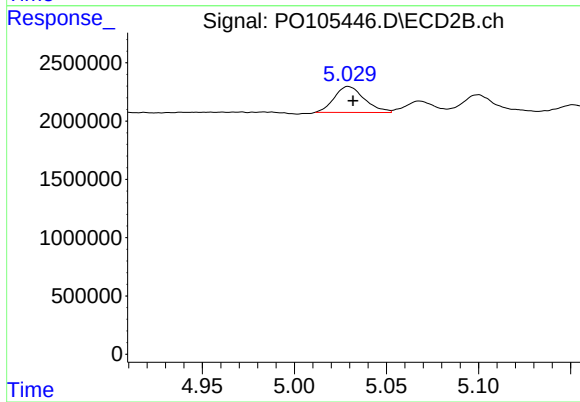


#7 AR-1016-5

R.T.: 5.029 min
Delta R.T.: -0.002 min
Response: 2543157
Conc: 30.39 ng/ml

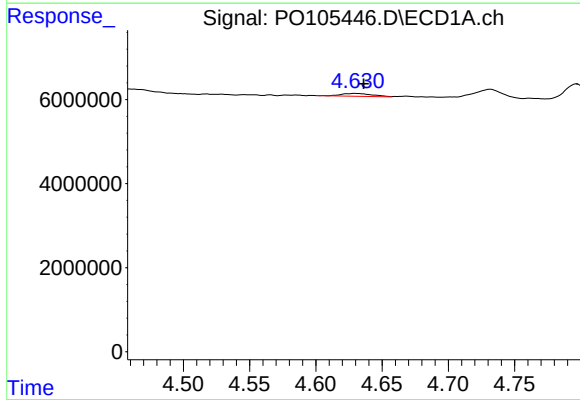


#8 AR-1221-1

R.T.: 4.630 min
Delta R.T.: -0.006 min
Response: 1100443
Conc: 9.81 ng/ml

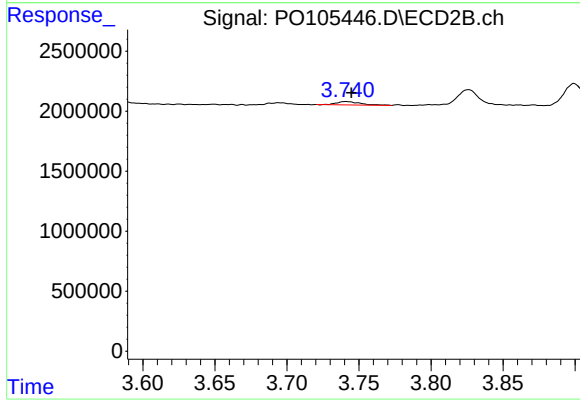

#8 AR-1221-1


R.T.: 3.741 min
Delta R.T.: -0.004 min
Response: 319070
Conc: 8.08 ng/ml

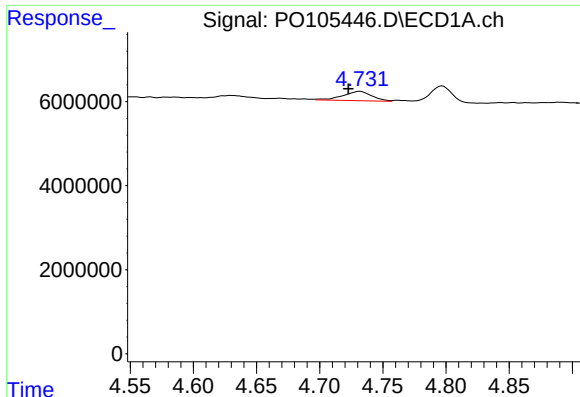

#9 AR-1221-2


R.T.: 4.732 min
Delta R.T.: 0.009 min
Response: 3592011
Conc: 42.38 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

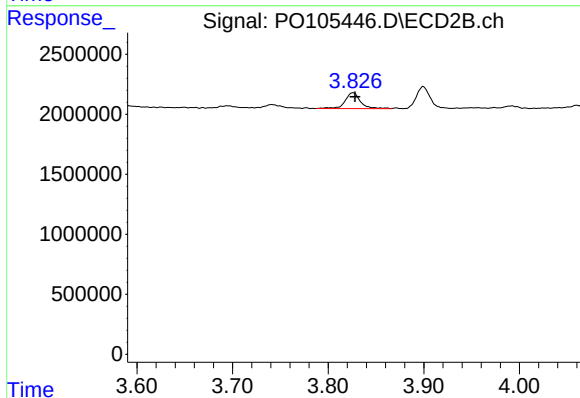


#9 AR-1221-2

R.T.: 3.826 min
Delta R.T.: -0.002 min
Response: 1482694
Conc: 48.26 ng/ml

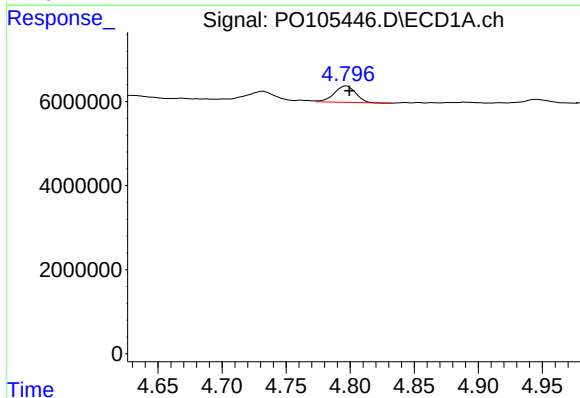


#10 AR-1221-3

R.T.: 4.797 min
Delta R.T.: -0.002 min
Response: 4533263
Conc: 18.63 ng/ml

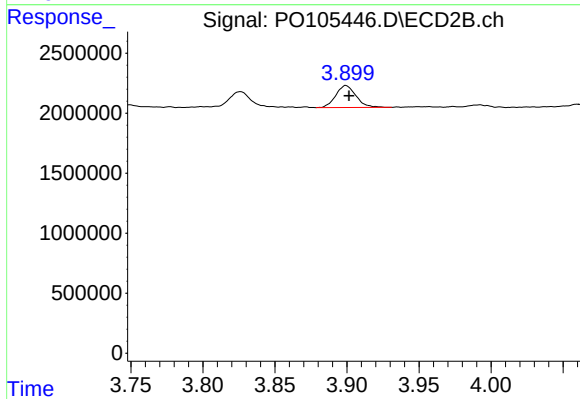

#10 AR-1221-3


R.T.: 3.899 min
Delta R.T.: -0.002 min
Response: 1785637
Conc: 19.96 ng/ml

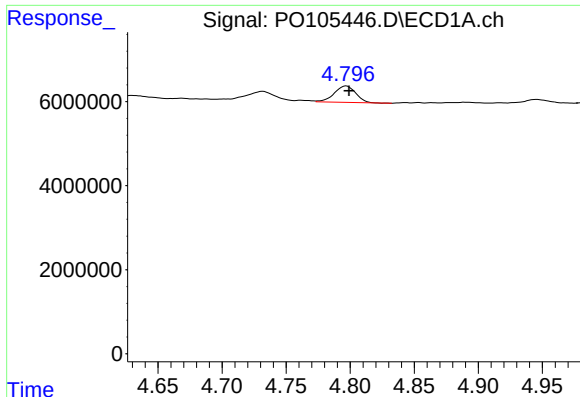

#11 AR-1232-1


R.T.: 4.797 min
Delta R.T.: -0.002 min
Response: 4533263
Conc: 22.67 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

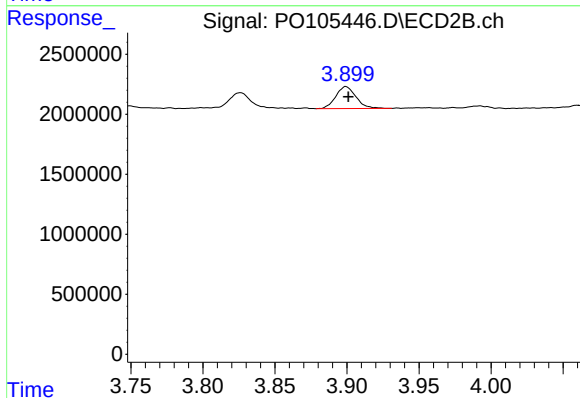


#11 AR-1232-1

R.T.: 3.899 min
Delta R.T.: -0.002 min
Response: 1785637
Conc: 24.45 ng/ml

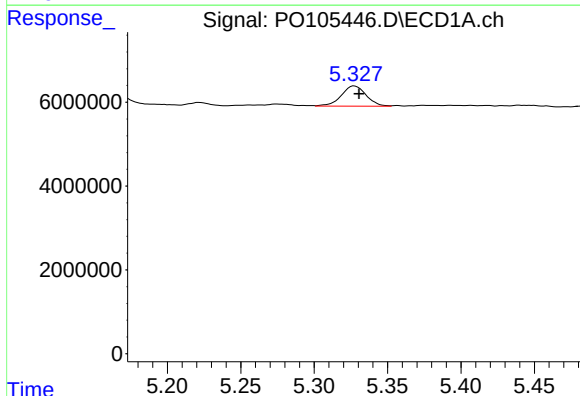


#12 AR-1232-2

R.T.: 5.327 min
Delta R.T.: -0.003 min
Response: 5705570
Conc: 53.90 ng/ml

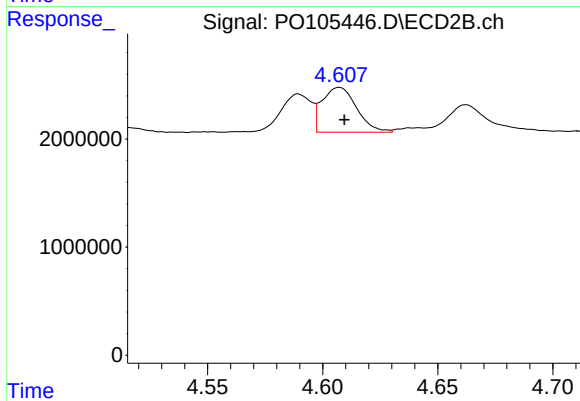

#12 AR-1232-2


R.T.: 4.607 min
Delta R.T.: -0.002 min
Response: 4342830
Conc: 61.85 ng/ml

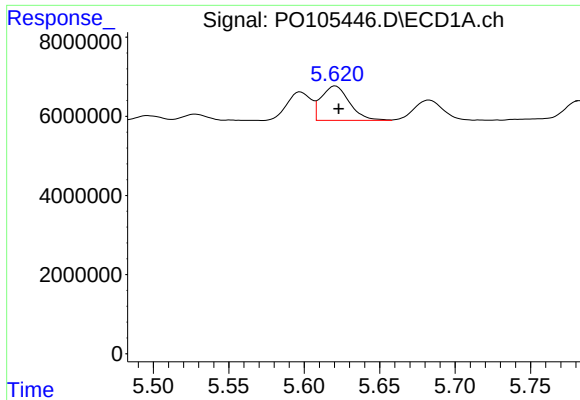

#13 AR-1232-3


R.T.: 5.621 min
Delta R.T.: -0.002 min
Response: 11337746
Conc: 59.23 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

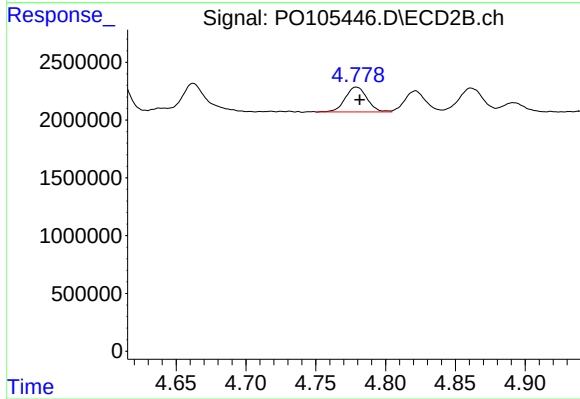


#13 AR-1232-3

R.T.: 4.779 min
Delta R.T.: -0.002 min
Response: 2339517
Conc: 61.22 ng/ml

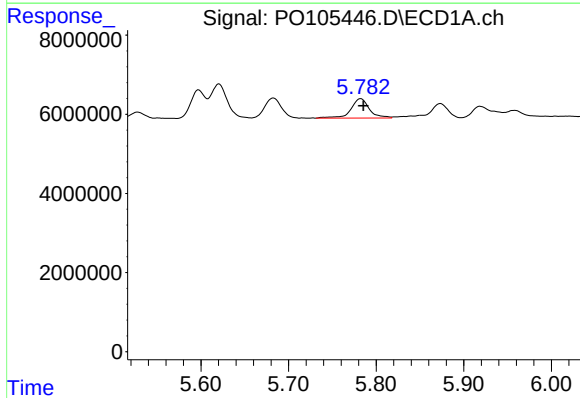


#14 AR-1232-4

R.T.: 5.783 min
Delta R.T.: -0.003 min
Response: 7123134
Conc: 73.03 ng/ml

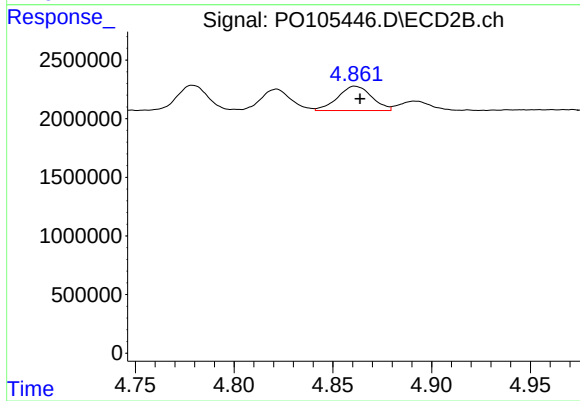

#14 AR-1232-4


R.T.: 4.861 min
Delta R.T.: -0.002 min
Response: 2481648
Conc: 71.33 ng/ml

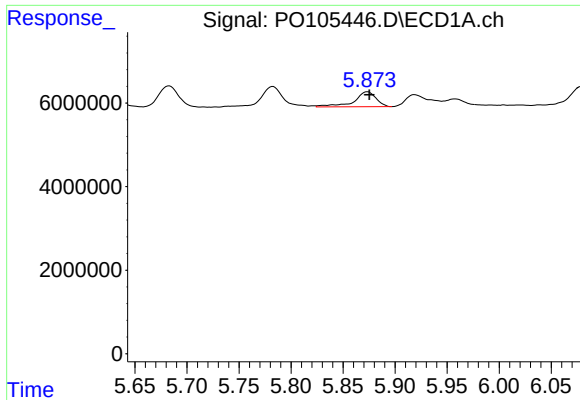

#15 AR-1232-5


R.T.: 5.873 min
Delta R.T.: -0.002 min
Response: 5263400
Conc: 73.04 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

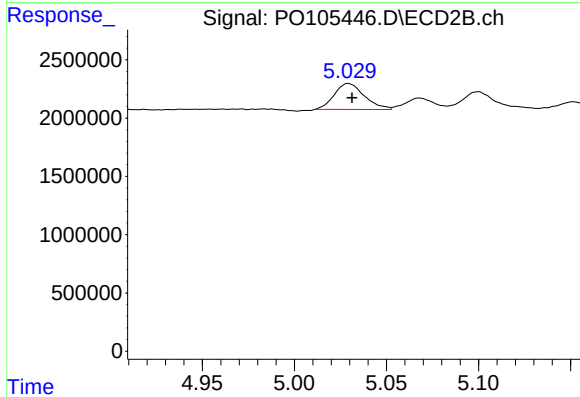


#15 AR-1232-5

R.T.: 5.029 min
Delta R.T.: -0.002 min
Response: 2543157
Conc: 72.05 ng/ml

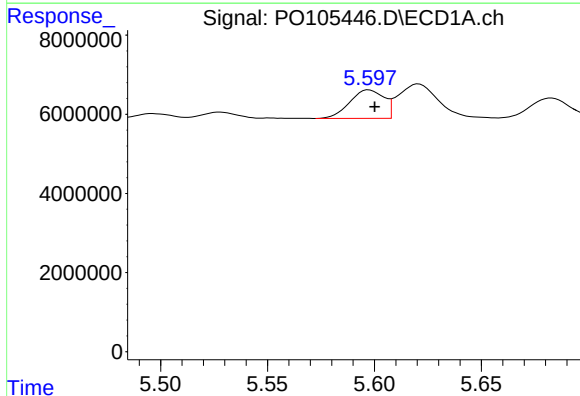


#16 AR-1242-1

R.T.: 5.598 min
Delta R.T.: -0.003 min
Response: 8023724
Conc: 34.53 ng/ml

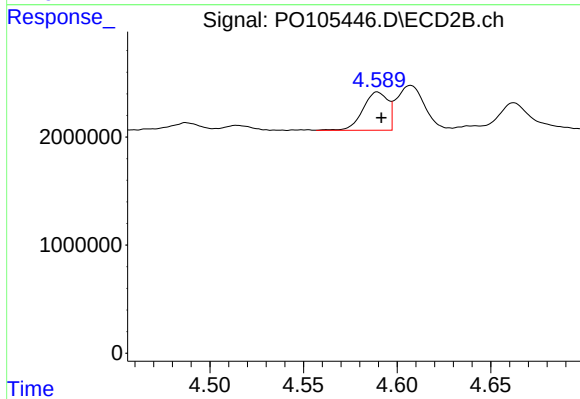

#16 AR-1242-1


R.T.: 4.590 min
Delta R.T.: -0.002 min
Response: 3301647
Conc: 37.43 ng/ml

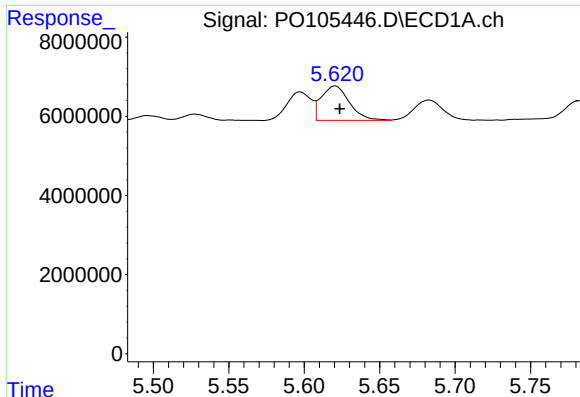

#17 AR-1242-2


R.T.: 5.621 min
Delta R.T.: -0.003 min
Response: 11337746
Conc: 34.79 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

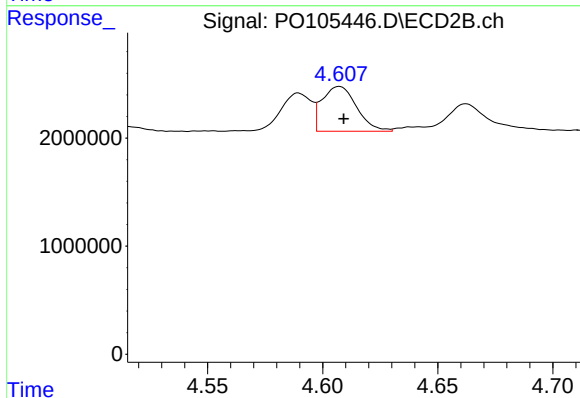


#17 AR-1242-2

R.T.: 4.607 min
Delta R.T.: -0.002 min
Response: 4342830
Conc: 36.58 ng/ml

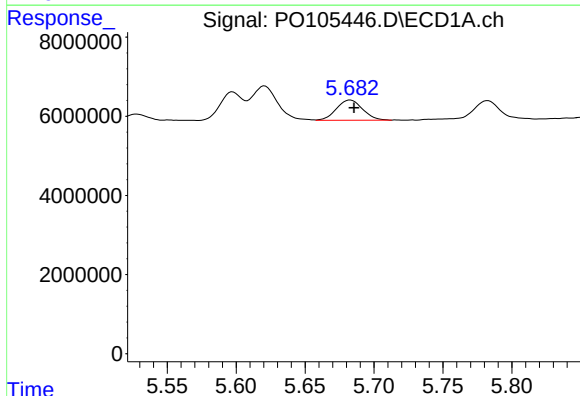


#18 AR-1242-3

R.T.: 5.683 min
Delta R.T.: -0.003 min
Response: 6770325
Conc: 34.32 ng/ml

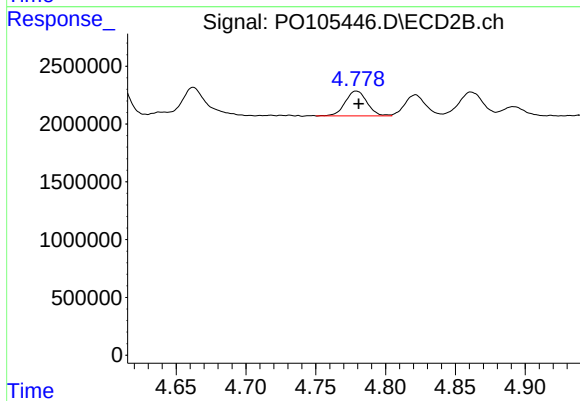

#18 AR-1242-3


R.T.: 4.779 min
Delta R.T.: -0.002 min
Response: 2339517
Conc: 36.03 ng/ml

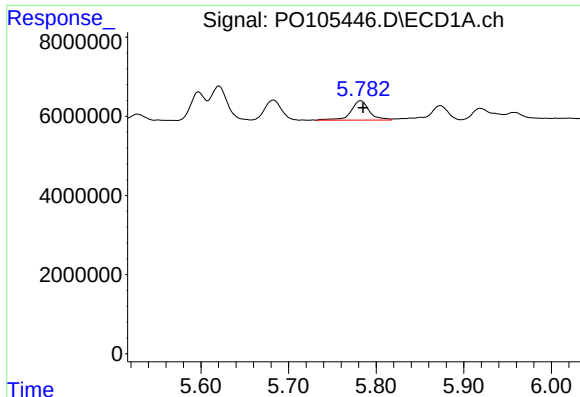

#19 AR-1242-4


R.T.: 5.783 min
Delta R.T.: -0.002 min
Response: 7123134
Conc: 41.75 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

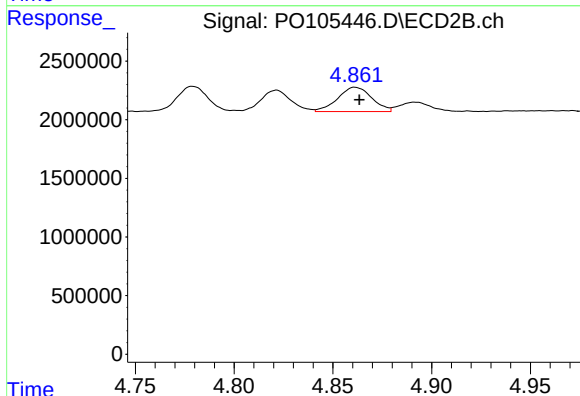


#19 AR-1242-4

R.T.: 4.861 min
Delta R.T.: -0.002 min
Response: 2481648
Conc: 37.42 ng/ml

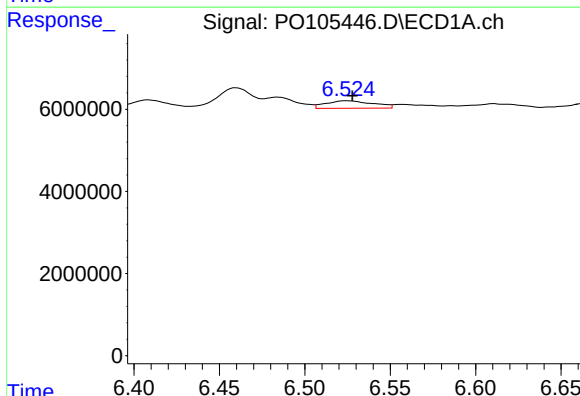


#20 AR-1242-5

R.T.: 6.524 min
Delta R.T.: -0.003 min
Response: 3530210
Conc: 20.20 ng/ml

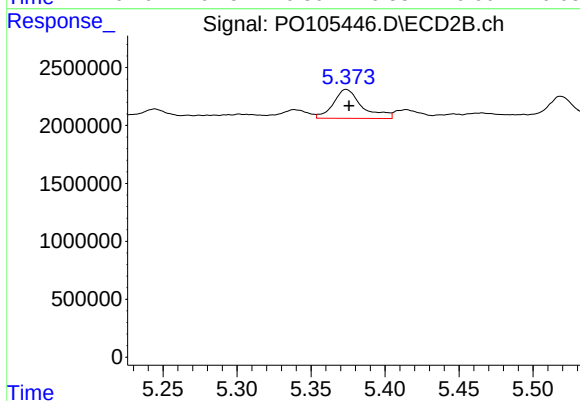

#20 AR-1242-5


R.T.: 5.374 min
Delta R.T.: -0.002 min
Response: 3379660
Conc: 41.13 ng/ml

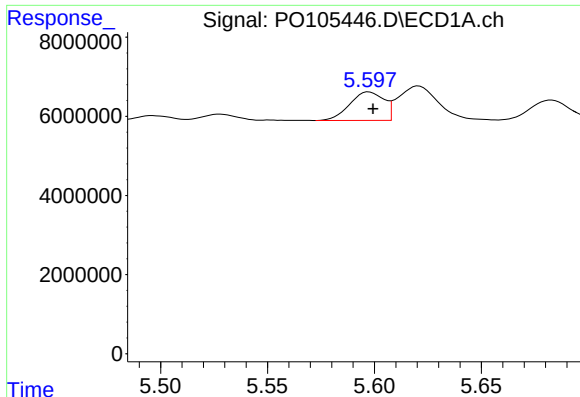

#21 AR-1248-1


R.T.: 5.598 min
Delta R.T.: -0.002 min
Response: 8023724
Conc: 43.94 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

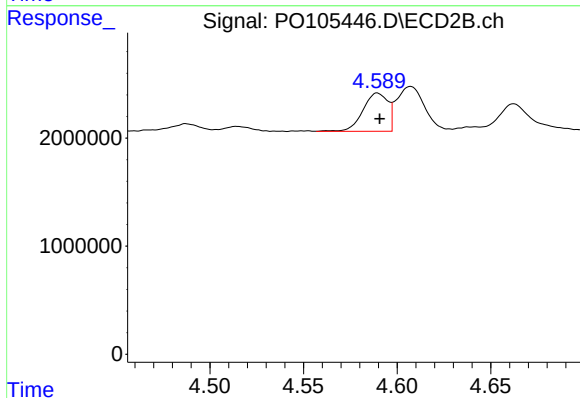


#21 AR-1248-1

R.T.: 4.590 min
Delta R.T.: -0.001 min
Response: 3301647
Conc: 47.27 ng/ml

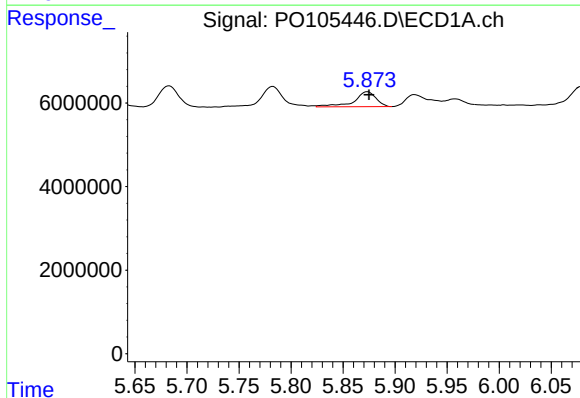


#22 AR-1248-2

R.T.: 5.873 min
Delta R.T.: -0.002 min
Response: 5263400
Conc: 20.90 ng/ml

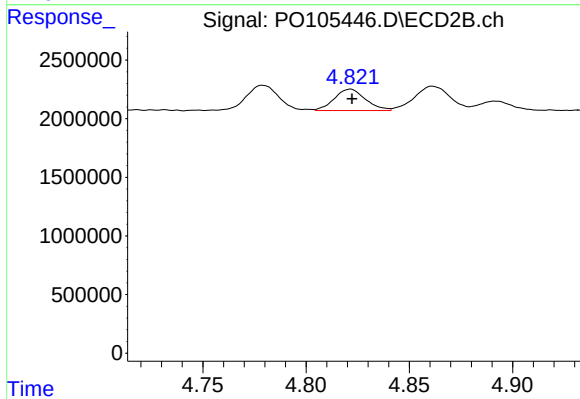

#22 AR-1248-2


R.T.: 4.821 min
Delta R.T.: 0.000 min
Response: 1901160
Conc: 20.03 ng/ml

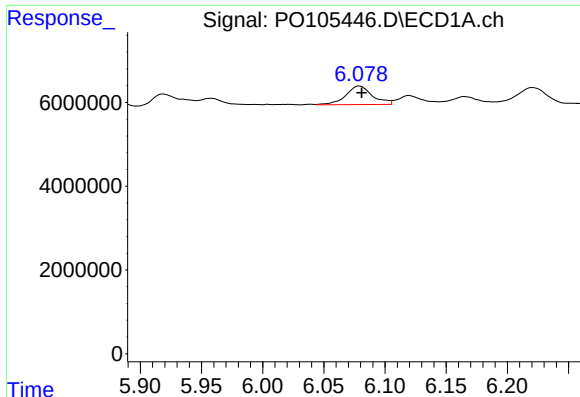

#23 AR-1248-3


R.T.: 6.079 min
Delta R.T.: -0.002 min
Response: 6696498
Conc: 23.69 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

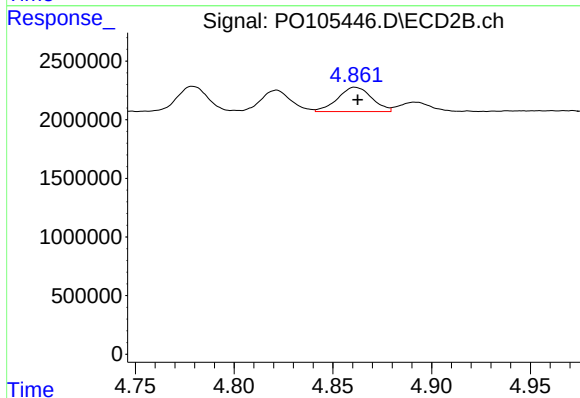


#23 AR-1248-3

R.T.: 4.861 min
Delta R.T.: -0.001 min
Response: 2481648
Conc: 24.86 ng/ml

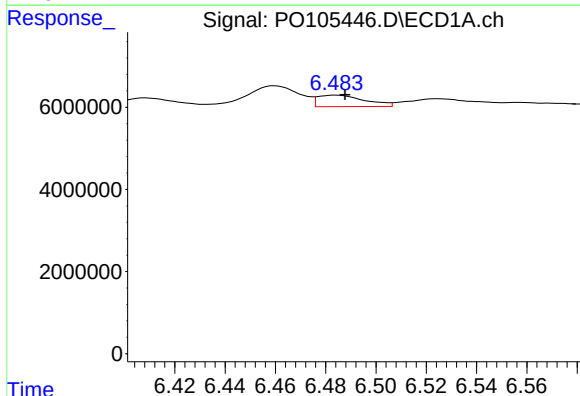


#24 AR-1248-4

R.T.: 6.484 min
Delta R.T.: -0.003 min
Response: 3609393
Conc: 11.29 ng/ml

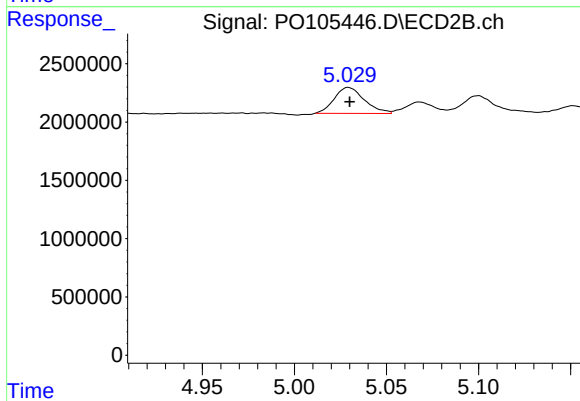

#24 AR-1248-4


R.T.: 5.029 min
Delta R.T.: 0.000 min
Response: 2543157
Conc: 22.53 ng/ml

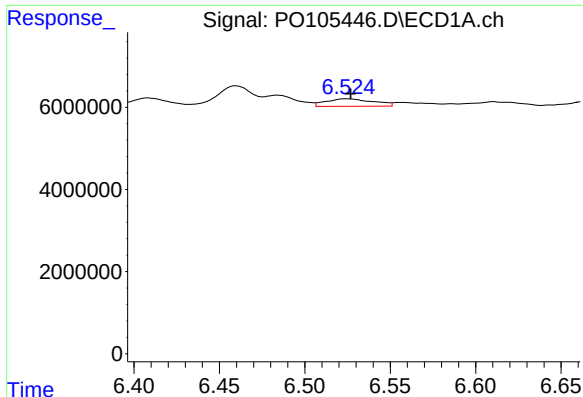

#25 AR-1248-5


R.T.: 6.524 min
Delta R.T.: -0.002 min
Response: 3530210
Conc: 11.41 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

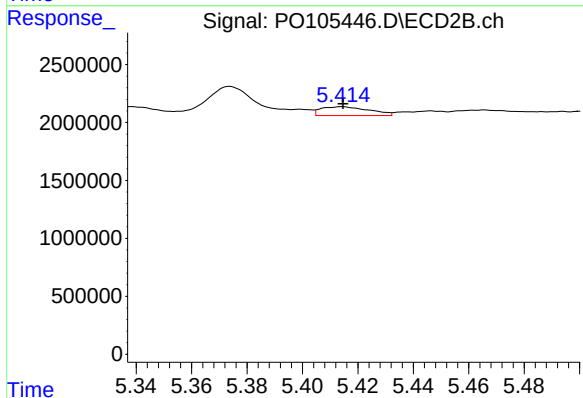


#25 AR-1248-5

R.T.: 5.414 min
Delta R.T.: 0.000 min
Response: 924366
Conc: 8.21 ng/ml

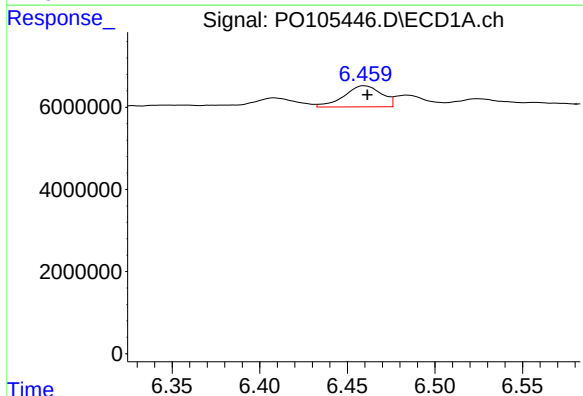


#26 AR-1254-1

R.T.: 6.460 min
Delta R.T.: -0.002 min
Response: 7586255
Conc: 24.19 ng/ml

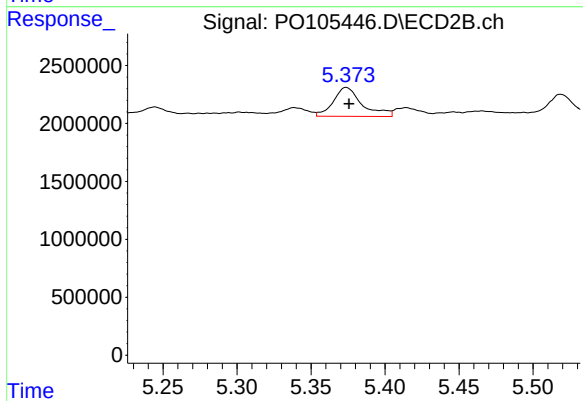

#26 AR-1254-1


R.T.: 5.374 min
Delta R.T.: -0.002 min
Response: 3379660
Conc: 20.76 ng/ml

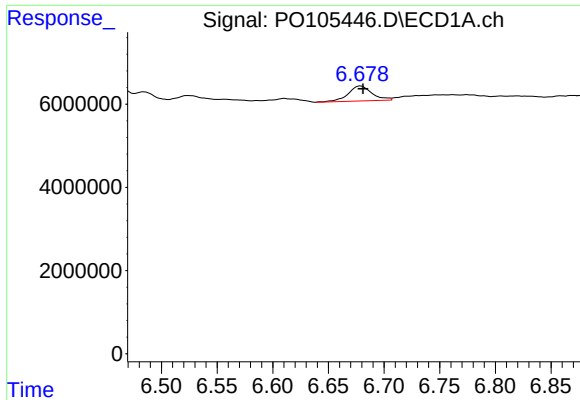

#27 AR-1254-2


R.T.: 6.679 min
Delta R.T.: -0.002 min
Response: 5381518
Conc: 11.93 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

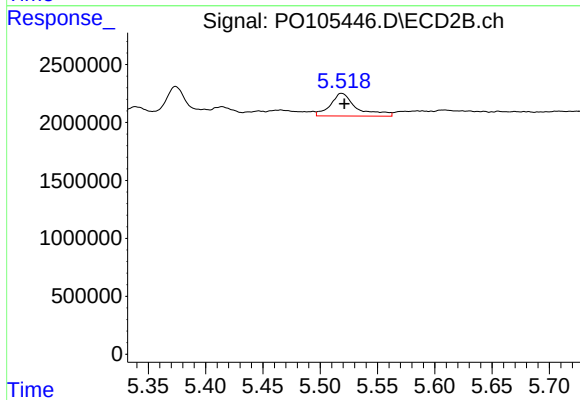


#27 AR-1254-2

R.T.: 5.519 min
Delta R.T.: -0.002 min
Response: 3101689
Conc: 21.20 ng/ml

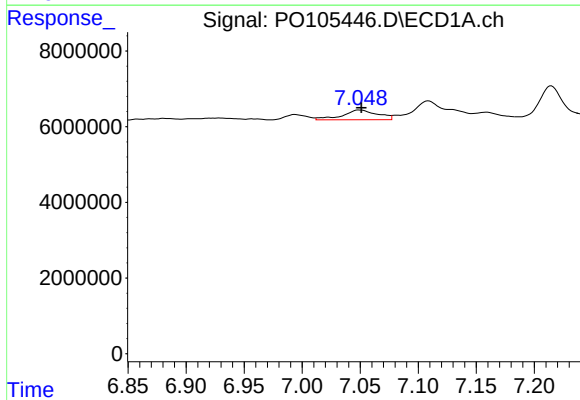


#28 AR-1254-3

R.T.: 7.049 min
Delta R.T.: -0.002 min
Response: 5364390
Conc: 11.31 ng/ml

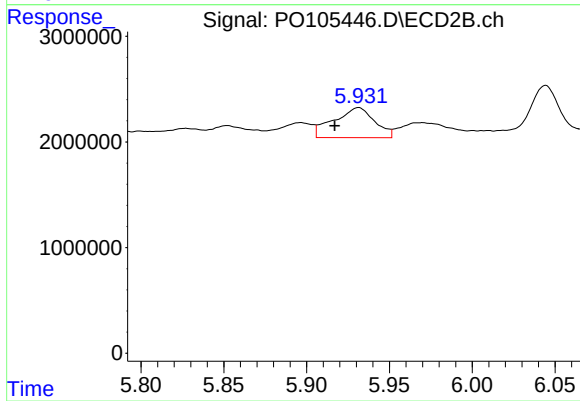

#28 AR-1254-3


R.T.: 5.931 min
Delta R.T.: 0.014 min
Response: 4868770
Conc: 21.58 ng/ml

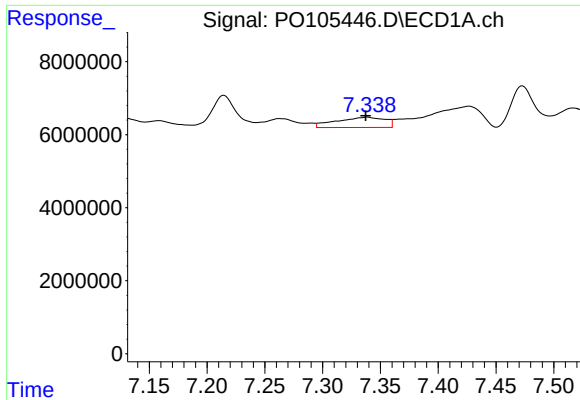

#29 AR-1254-4


R.T.: 7.339 min
Delta R.T.: 0.001 min
Response: 8218443
Conc: 22.94 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

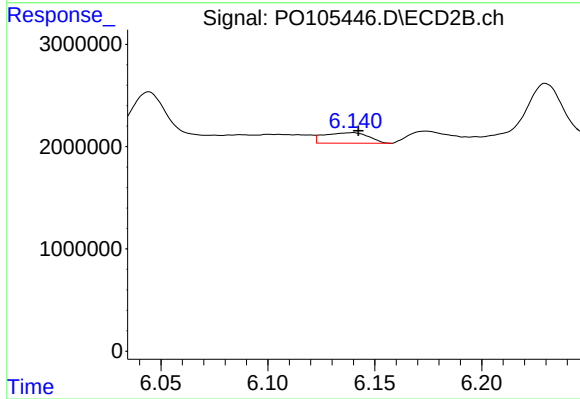


#29 AR-1254-4

R.T.: 6.139 min
Delta R.T.: -0.003 min
Response: 1481480
Conc: 10.50 ng/ml

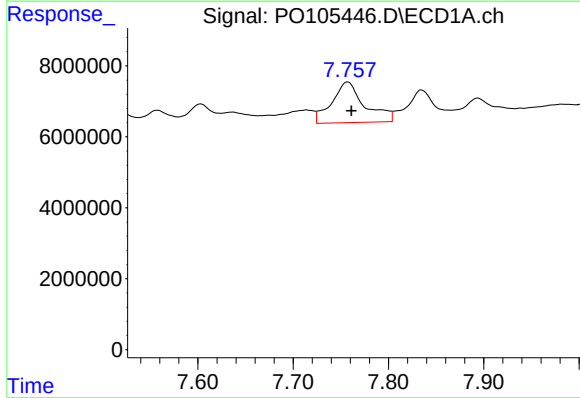


#30 AR-1254-5

R.T.: 7.757 min
Delta R.T.: -0.004 min
Response: 27413058
Conc: 69.06 ng/ml

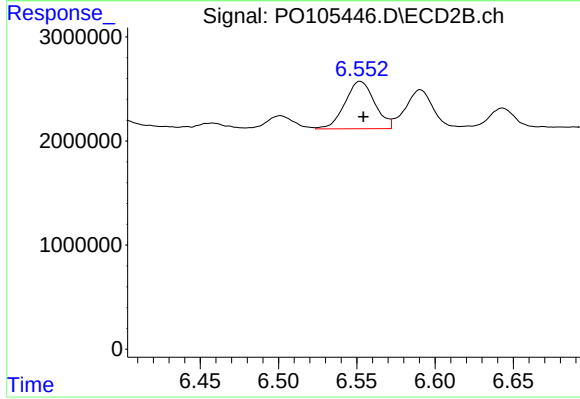

#30 AR-1254-5


R.T.: 6.552 min
Delta R.T.: -0.002 min
Response: 6019289
Conc: 30.04 ng/ml

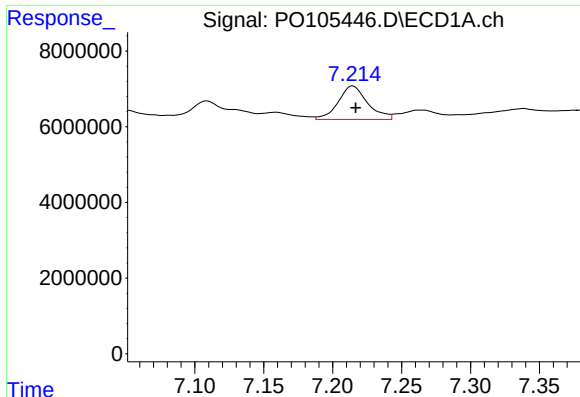

#31 AR-1260-1


R.T.: 7.215 min
Delta R.T.: -0.002 min
Response: 13156733
Conc: 35.90 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

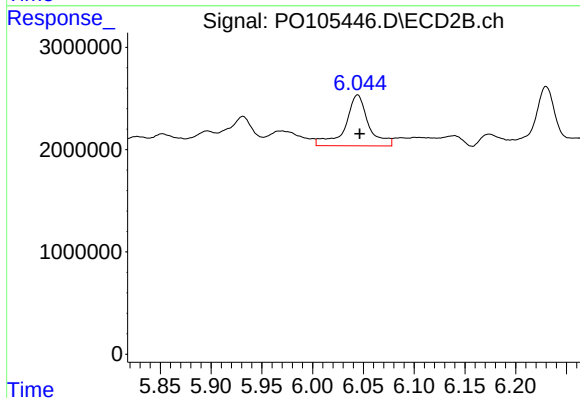


#31 AR-1260-1

R.T.: 6.044 min
Delta R.T.: -0.002 min
Response: 7924651
Conc: 50.77 ng/ml

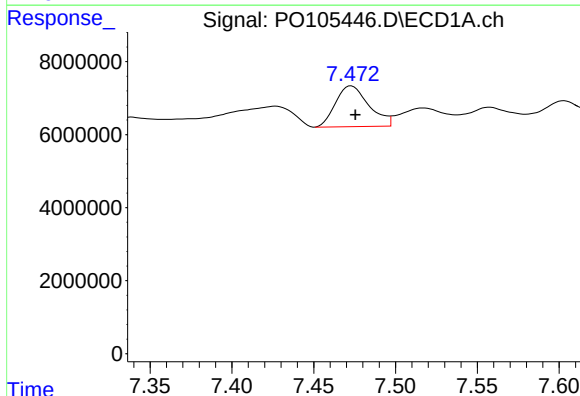


#32 AR-1260-2

R.T.: 7.473 min
Delta R.T.: -0.002 min
Response: 15861455
Conc: 38.09 ng/ml

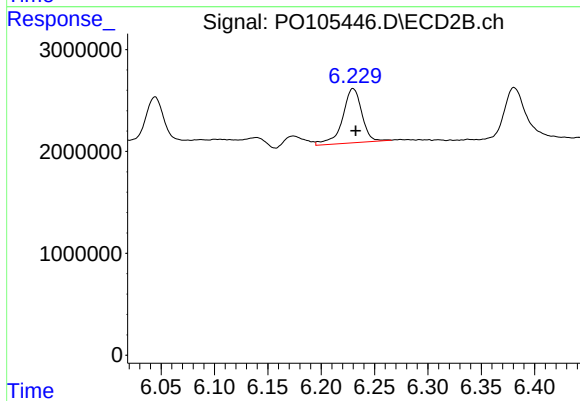

#32 AR-1260-2


R.T.: 6.230 min
Delta R.T.: -0.002 min
Response: 6680930
Conc: 35.35 ng/ml

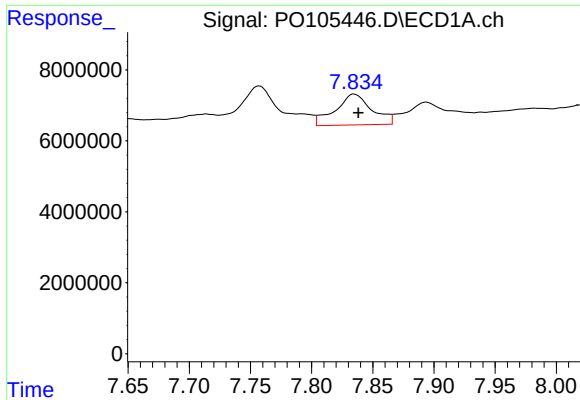

#33 AR-1260-3


R.T.: 7.835 min
Delta R.T.: -0.004 min
Response: 18016564
Conc: 69.61 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

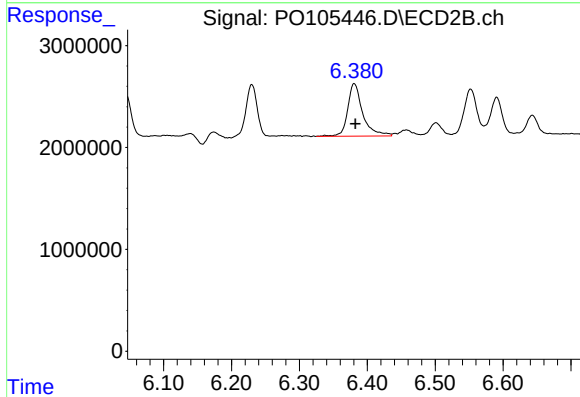


#33 AR-1260-3

R.T.: 6.381 min
Delta R.T.: -0.002 min
Response: 7958130
Conc: 43.08 ng/ml

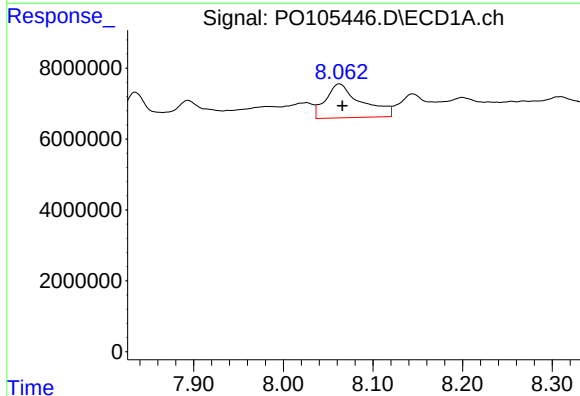


#34 AR-1260-4

R.T.: 8.063 min
Delta R.T.: -0.003 min
Response: 26539089
Conc: 80.44 ng/ml

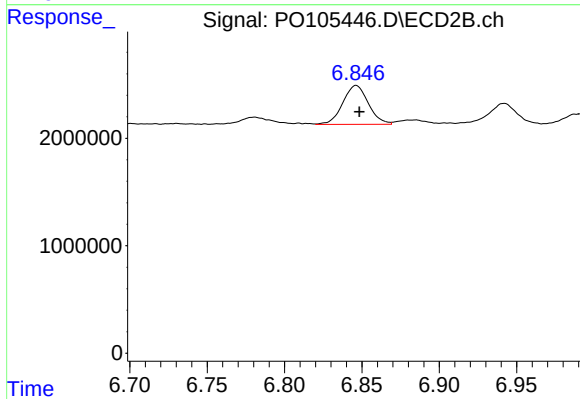

#34 AR-1260-4


R.T.: 6.846 min
Delta R.T.: -0.002 min
Response: 4160644
Conc: 34.04 ng/ml

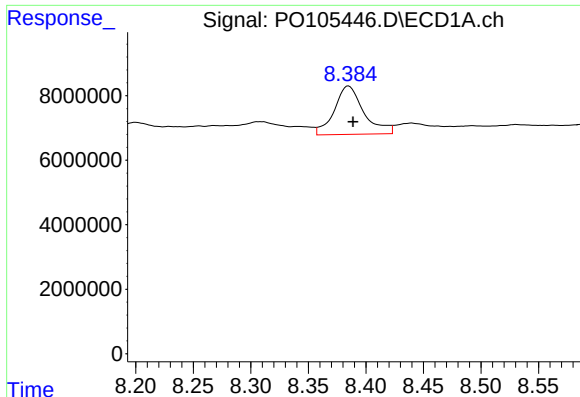

#35 AR-1260-5


R.T.: 8.385 min
Delta R.T.: -0.004 min
Response: 26804147
Conc: 45.06 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

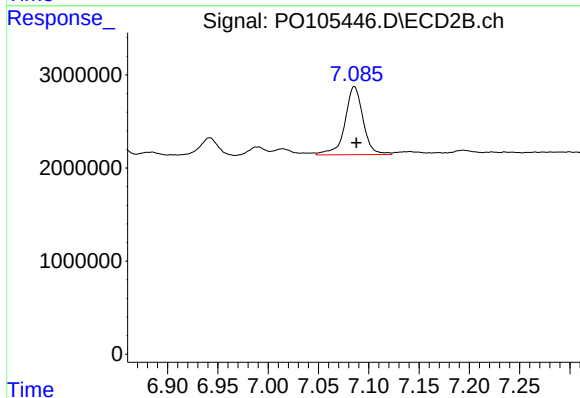


#35 AR-1260-5

R.T.: 7.086 min
Delta R.T.: -0.002 min
Response: 9157274
Conc: 32.90 ng/ml

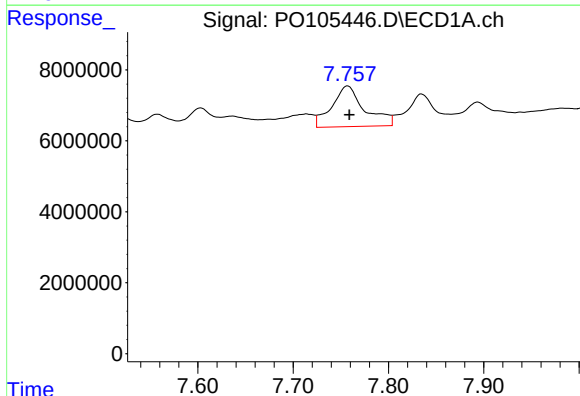


#36 AR-1262-1

R.T.: 7.757 min
Delta R.T.: -0.002 min
Response: 27413058
Conc: 86.30 ng/ml

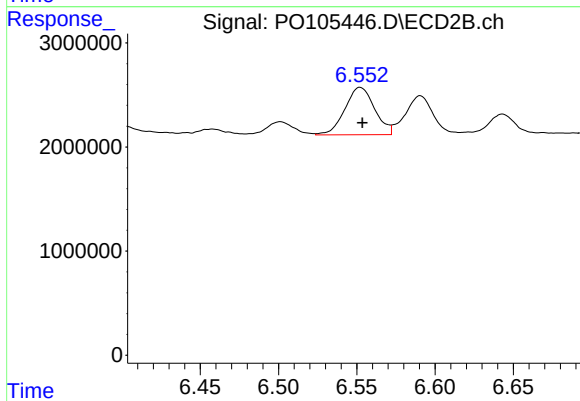

#36 AR-1262-1


R.T.: 6.552 min
Delta R.T.: -0.001 min
Response: 6019289
Conc: 56.57 ng/ml

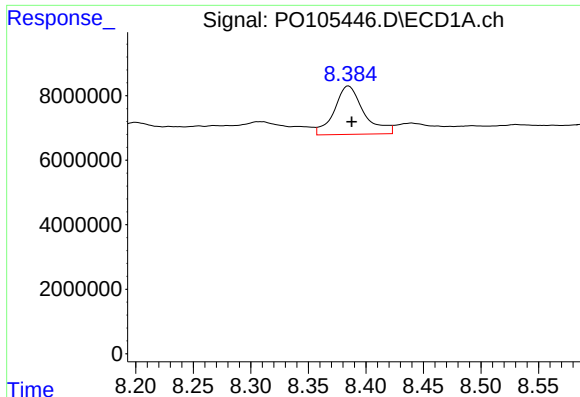

#37 AR-1262-2


R.T.: 8.385 min
Delta R.T.: -0.003 min
Response: 26804147
Conc: 35.64 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

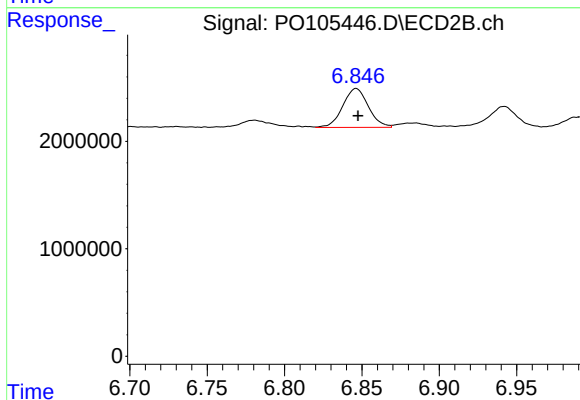


#37 AR-1262-2

R.T.: 6.846 min
Delta R.T.: -0.001 min
Response: 4160644
Conc: 24.48 ng/ml

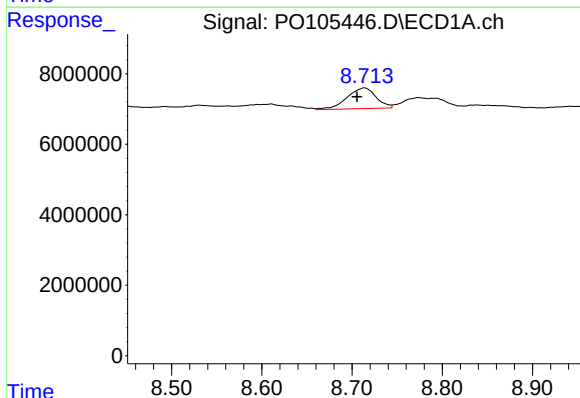


#38 AR-1262-3

R.T.: 8.714 min
Delta R.T.: 0.008 min
Response: 13208229
Conc: 26.84 ng/ml

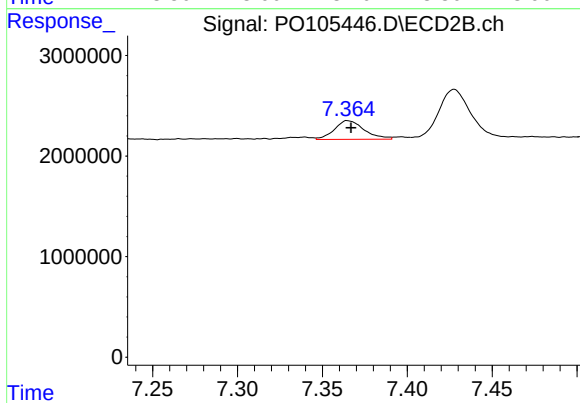

#38 AR-1262-3


R.T.: 7.365 min
Delta R.T.: -0.002 min
Response: 2287081
Conc: 18.12 ng/ml

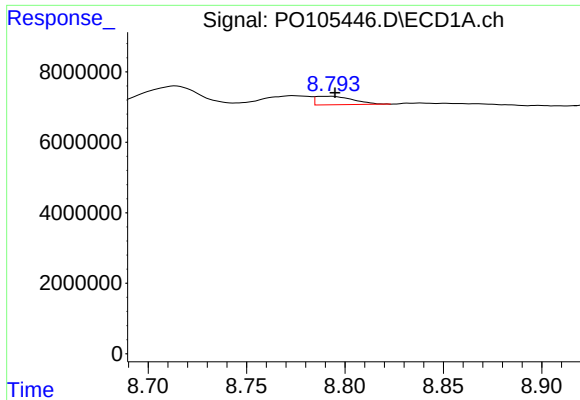

#39 AR-1262-4


R.T.: 8.791 min
Delta R.T.: -0.004 min
Response: 3150207
Conc: 8.58 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

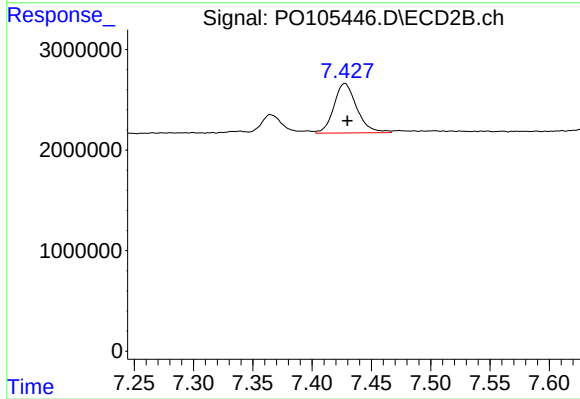


#39 AR-1262-4

R.T.: 7.428 min
Delta R.T.: -0.002 min
Response: 6619376
Conc: 28.59 ng/ml

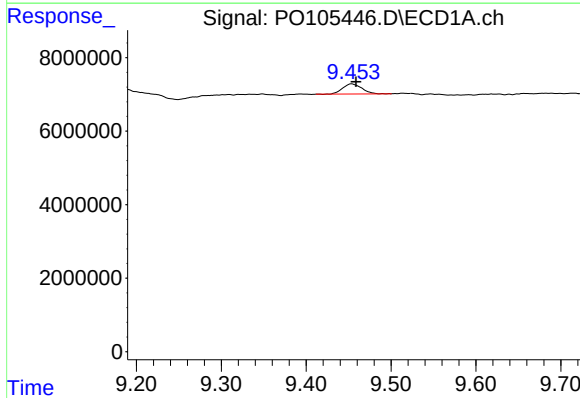


#40 AR-1262-5

R.T.: 9.454 min
Delta R.T.: -0.005 min
Response: 4331938
Conc: 16.17 ng/ml

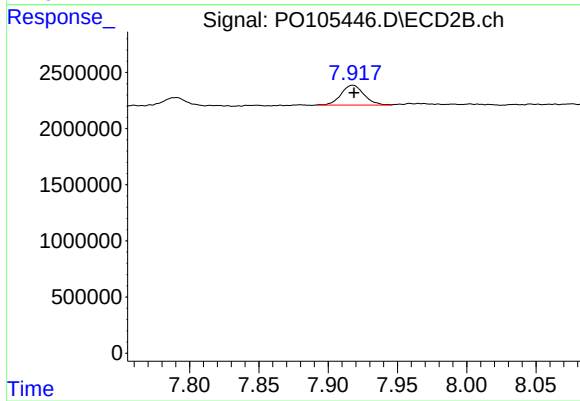

#40 AR-1262-5


R.T.: 7.918 min
Delta R.T.: -0.001 min
Response: 2055473
Conc: 20.45 ng/ml

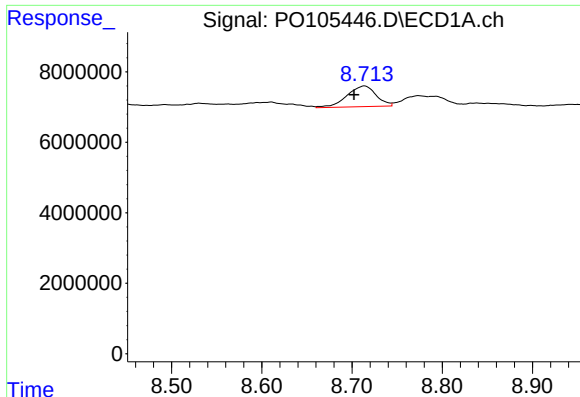

#41 AR-1268-1


R.T.: 8.714 min
Delta R.T.: 0.012 min
Response: 13208229
Conc: 16.24 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

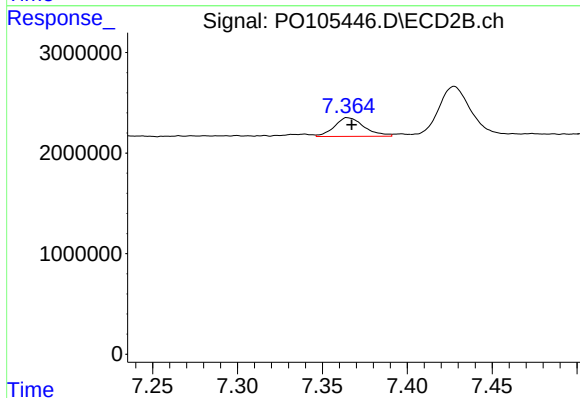


#41 AR-1268-1

R.T.: 7.365 min
Delta R.T.: -0.002 min
Response: 2287081
Conc: 6.55 ng/ml

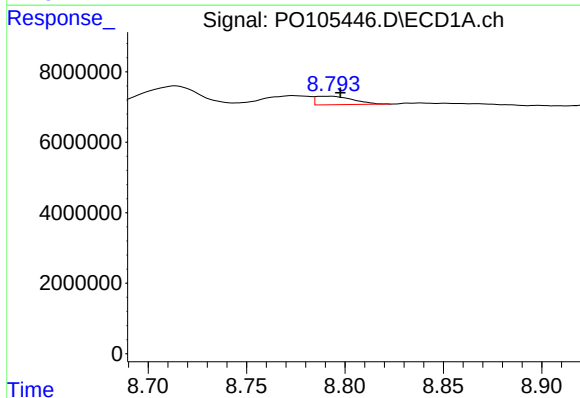


#42 AR-1268-2

R.T.: 8.791 min
Delta R.T.: -0.006 min
Response: 3150207
Conc: 4.33 ng/ml

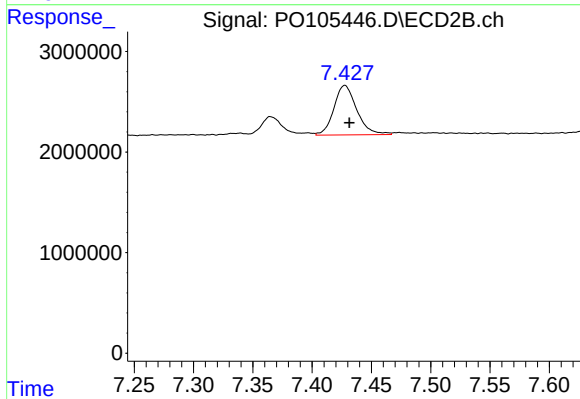

#42 AR-1268-2


R.T.: 7.428 min
Delta R.T.: -0.004 min
Response: 6619376
Conc: 21.22 ng/ml

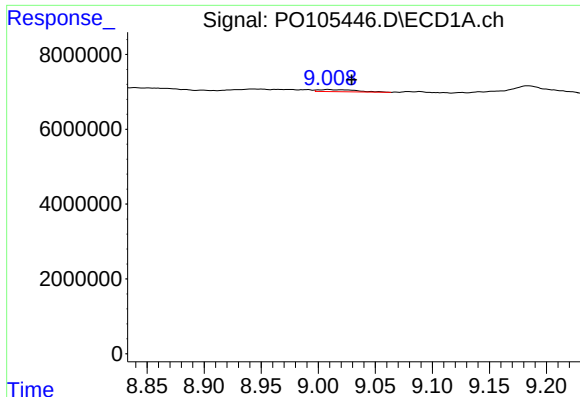

#43 AR-1268-3


R.T.: 9.009 min
Delta R.T.: -0.021 min
Response: 1250358
Conc: 1.94 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

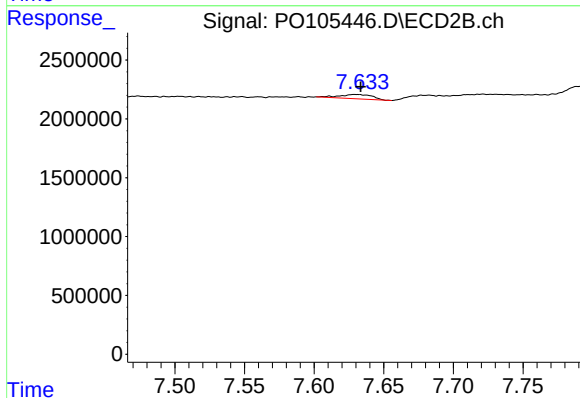


#43 AR-1268-3

R.T.: 7.630 min
Delta R.T.: -0.003 min
Response: 591221
Conc: 2.34 ng/ml

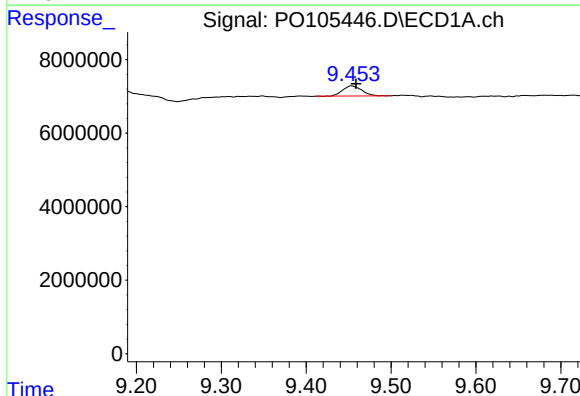


#44 AR-1268-4

R.T.: 9.454 min
Delta R.T.: -0.005 min
Response: 4331938
Conc: 15.56 ng/ml

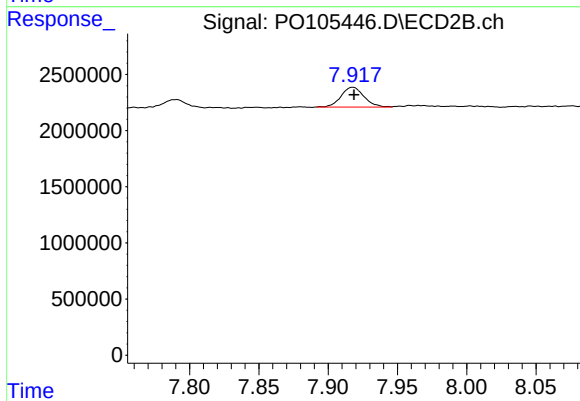

#44 AR-1268-4


R.T.: 7.918 min
Delta R.T.: 0.000 min
Response: 2055473
Conc: 19.11 ng/ml

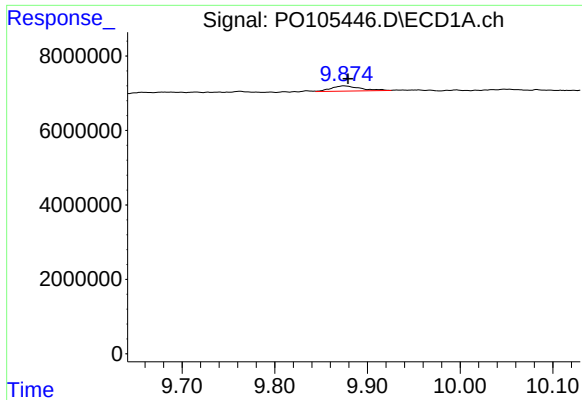

#45 AR-1268-5

R.T.: 9.875 min
Delta R.T.: -0.004 min
Response: 3047029
Conc: 1.46 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

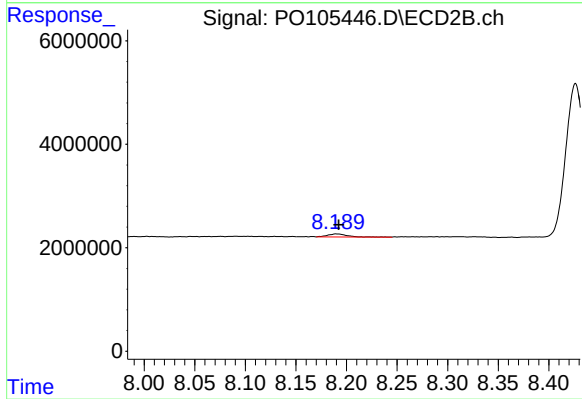

#45 AR-1268-5

R.T.: 8.190 min
Delta R.T.: -0.002 min
Response: 770690
Conc: 1.15 ng/ml