

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0081224\
 Data File : P0105447.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2024 23:36
 Operator : YP/AJ
 Sample : P3390-07
 Misc : AR1221 LOD 40 PPB
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 02:40:39 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0081024.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 10 04:08:56 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.427	3.536	174.4E6	65215037	19.966	20.763
2)	SA Decachlor...	10.216	8.426	127.5E6	39744502	22.156	22.450
Target Compounds							
3)	L1 AR-1016-1	5.597	4.591	378388	320121	1.251	2.848 #
4)	L1 AR-1016-2	5.620	4.607	875079	375797	2.047	2.414
5)	L1 AR-1016-3	5.683	4.780	718732	190280	2.801	2.272
6)	L1 AR-1016-4	5.783	4.824	2174307	115097	9.942	1.709 #
7)	L1 AR-1016-5	6.080	5.030	770499	205949	3.601	2.461 #
8)	L2 AR-1221-1	4.633	3.743	4131946	1204339	36.845	30.511
9)	L2 AR-1221-2	4.729	3.826	5092926	2263357	60.086	73.671
10)	L2 AR-1221-3	4.796	3.900	7871497	2832523	32.355	31.655
11)	L3 AR-1232-1	4.796	3.900	7871497	2832523	39.370	38.787
12)	L3 AR-1232-2	5.327	4.607	829101	375797	7.833	5.352 #
13)	L3 AR-1232-3	5.620	4.780	875079	190280	4.572	4.979
14)	L3 AR-1232-4	5.783	4.862	2174307	175147	22.293	5.034 #
15)	L3 AR-1232-5	5.874	5.030	313628	205949	4.352	5.834 #
16)	L4 AR-1242-1	5.597	4.591	378388	320121	1.628	3.629 #
17)	L4 AR-1242-2	5.620	4.607	875079	375797	2.685	3.165
18)	L4 AR-1242-3	5.683	4.780	718732	190280	3.643	2.930
19)	L4 AR-1242-4	5.783	4.862	2174307	175147	12.743	2.641 #
20)	L4 AR-1242-5	6.542	5.377	2099511	432285	12.013	5.261 #
21)	L5 AR-1248-1	5.597	4.591	378388	320121	2.072	4.584 #
22)	L5 AR-1248-2	5.874	4.824	313628	115097	1.245	1.213
23)	L5 AR-1248-3	6.080	4.862	770499	175147	2.726	1.755 #
24)	L5 AR-1248-4	6.477	5.030	2569722	205949	8.037	1.825 #
25)	L5 AR-1248-5	6.542	5.425	2099511	81790	6.787	0.726 #
26)	L6 AR-1254-1	6.453	5.377	1055576	432285	3.366	2.655
27)	L6 AR-1254-2	6.684	5.526	196676	247761	0.436	1.694 #
28)	L6 AR-1254-3	7.054	5.909	2592120	476254	5.464	2.111 #
29)	L6 AR-1254-4	7.343	6.138	2223549	440920	6.207	3.125 #
30)	L6 AR-1254-5	7.773	6.544	1794788	434092	4.521	2.167 #
31)	L7 AR-1260-1	7.222	6.051	788473	330540	2.151	2.118
32)	L7 AR-1260-2	7.478	6.215	572010	686898	1.374	3.634 #
33)	L7 AR-1260-3	7.841	6.389	3597193	3108619	13.899	16.828
34)	L7 AR-1260-4	8.080	6.857	8746059	32693	26.509	0.267 #
35)	L7 AR-1260-5	8.384	7.078	2069541	273041	3.479	0.981 #
36)	L8 AR-1262-1	7.773	6.544	1794788	434092	5.650	4.080 #
37)	L8 AR-1262-2	8.384	6.857	2069541	32693	2.751	0.192 #
38)	L8 AR-1262-3	8.724	7.379	1493008	312007	3.034	2.471
39)	L8 AR-1262-4	8.790	7.434	603764	132722	1.644	0.573 #
40)	L8 AR-1262-5	9.442	7.920	89000	53695	0.332	0.534 #
41)	L9 AR-1268-1	8.724	7.379	1493008	312007	1.836	0.894 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081224\
Data File : P0105447.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Aug 2024 23:36
Operator : YP/AJ
Sample : P3390-07
Misc : AR1221 LOD 40 PPB
ALS Vial : 43 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 13 02:40:39 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081024.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Aug 10 04:08:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42)	L9 AR-1268-2	8.790	7.434	603764	132722	0.831	0.425 #
43)	L9 AR-1268-3	9.015	7.630	816407	1014215	1.265	4.013 #
44)	L9 AR-1268-4	9.442	7.920	89000	53695	0.320	0.499 #
45)	L9 AR-1268-5	9.886	8.190	542099	393192	0.259	0.588 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081224\
Data File : PO105447.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Aug 2024 23:36
Operator : YP/AJ
Sample : P3390-07
Misc : AR1221 LOD 40 PPB
ALS Vial : 43 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 13 02:40:39 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081024.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Aug 10 04:08:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

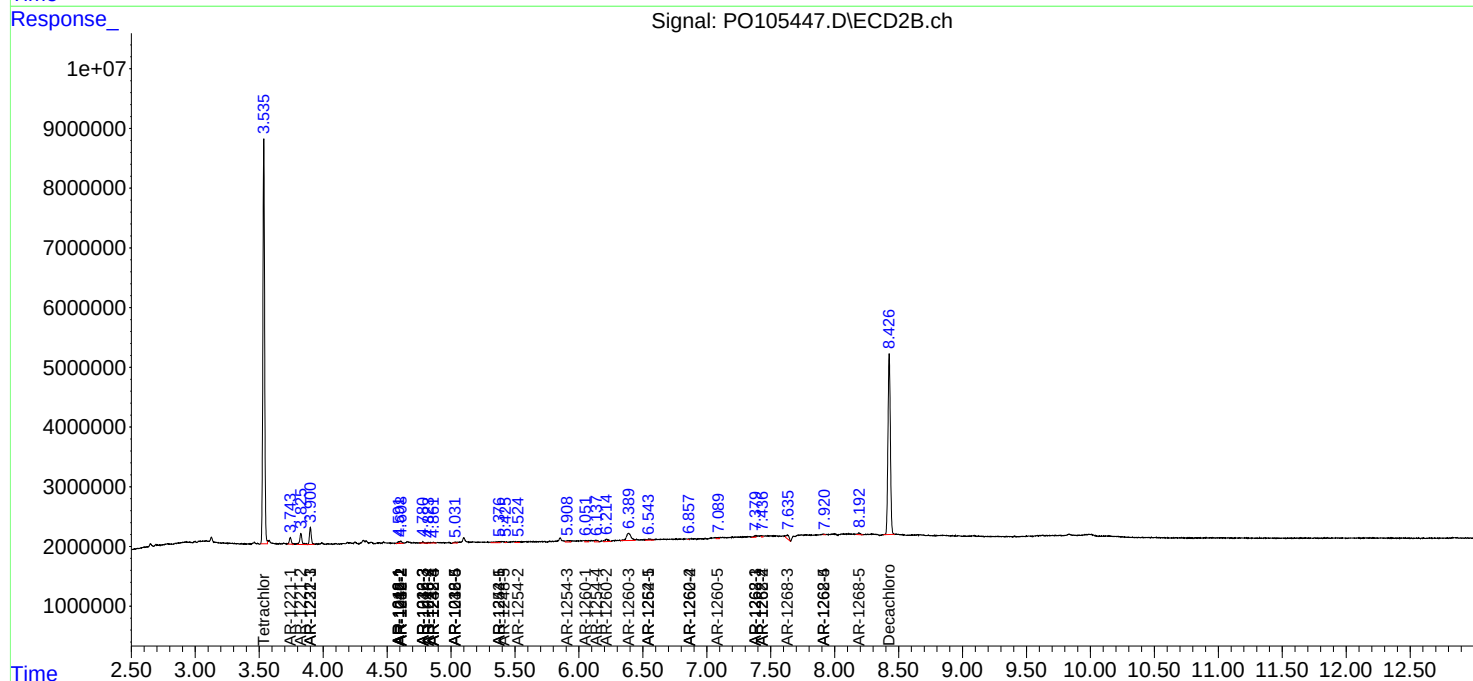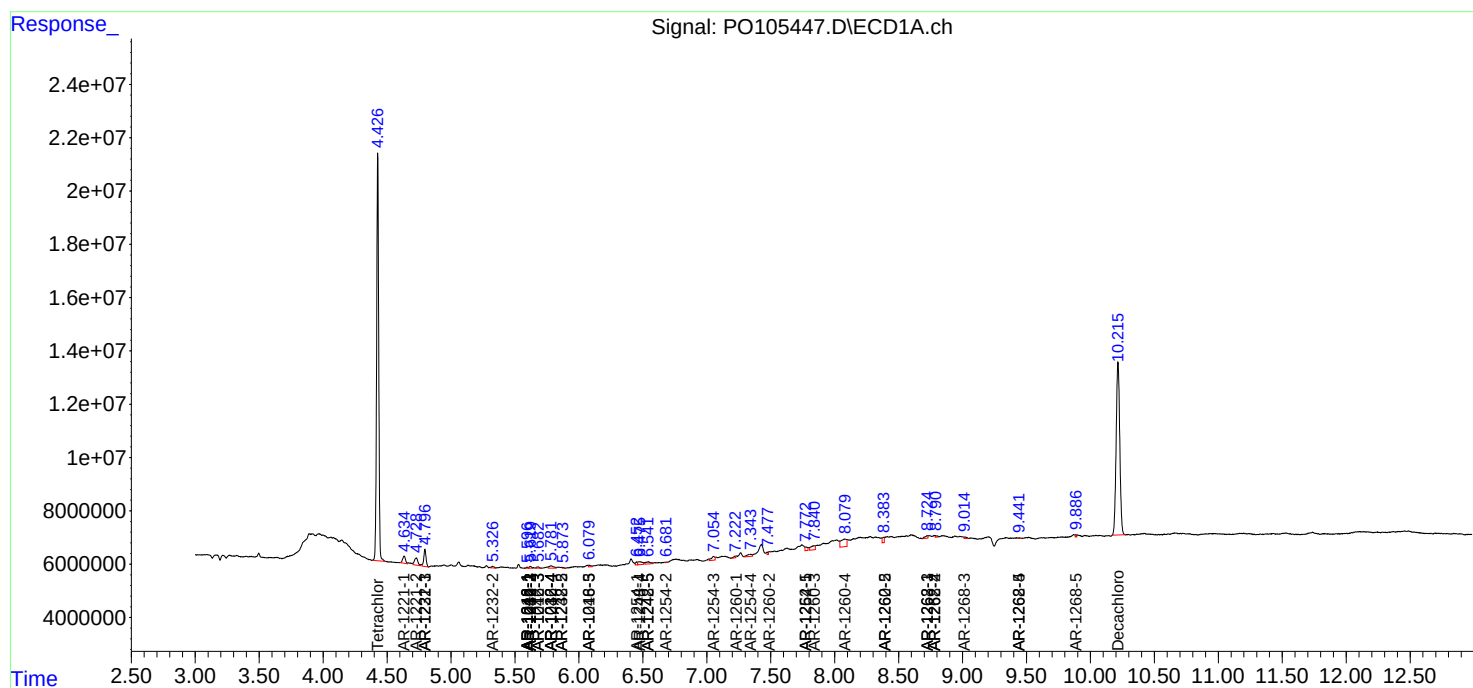


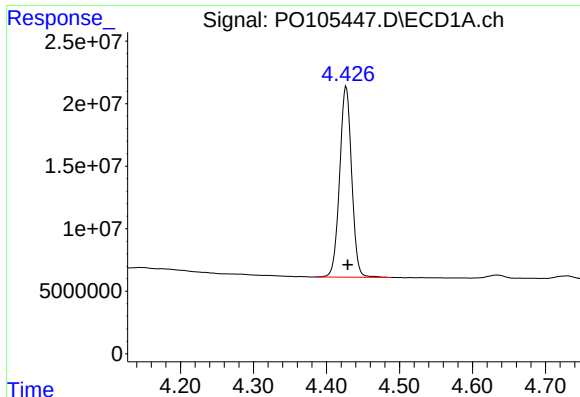

#1 Tetrachloro-m-xylene


R.T.: 4.427 min
Delta R.T.: -0.002 min
Response: 174391538
Conc: 19.97 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

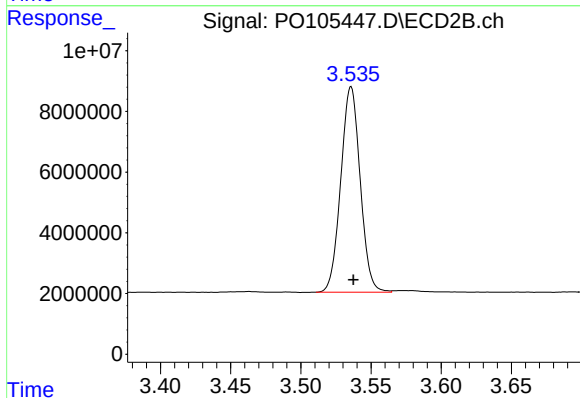


#1 Tetrachloro-m-xylene

R.T.: 3.536 min
Delta R.T.: -0.002 min
Response: 65215037
Conc: 20.76 ng/ml

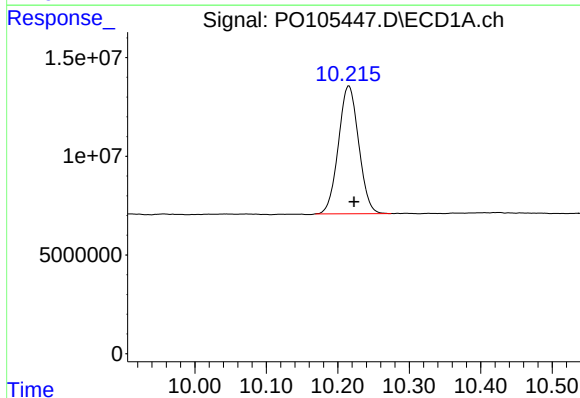


#2 Decachlorobiphenyl

R.T.: 10.216 min
Delta R.T.: -0.007 min
Response: 127452520
Conc: 22.16 ng/ml

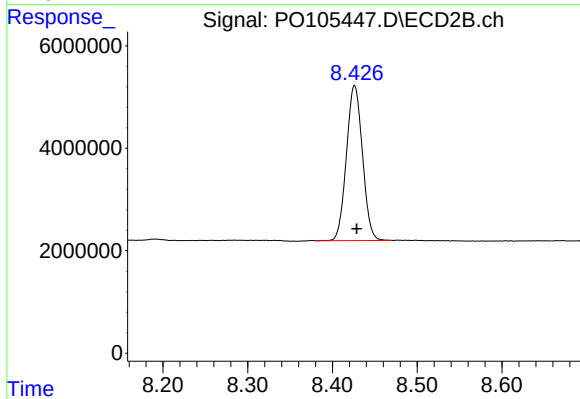

#2 Decachlorobiphenyl


R.T.: 8.426 min
Delta R.T.: -0.002 min
Response: 39744502
Conc: 22.45 ng/ml

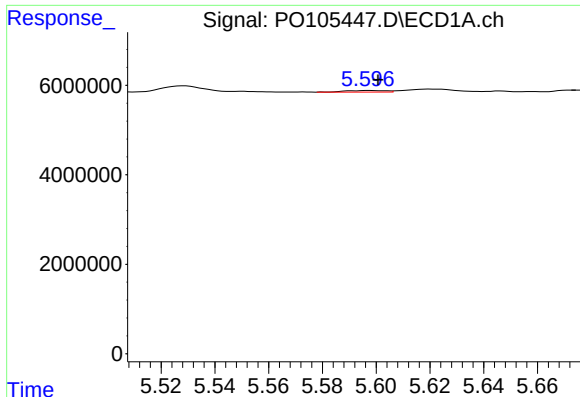

#3 AR-1016-1


R.T.: 5.597 min
Delta R.T.: -0.003 min
Response: 378388
Conc: 1.25 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

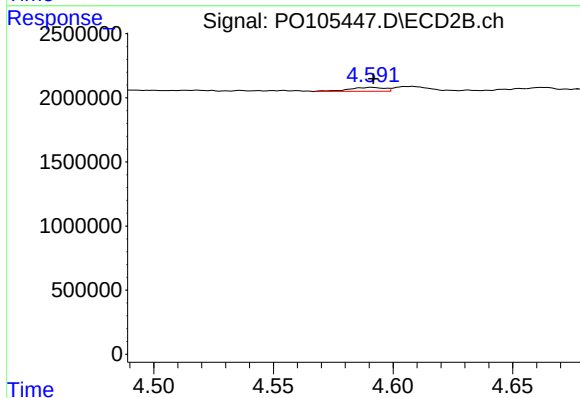


#3 AR-1016-1

R.T.: 4.591 min
Delta R.T.: 0.000 min
Response: 320121
Conc: 2.85 ng/ml

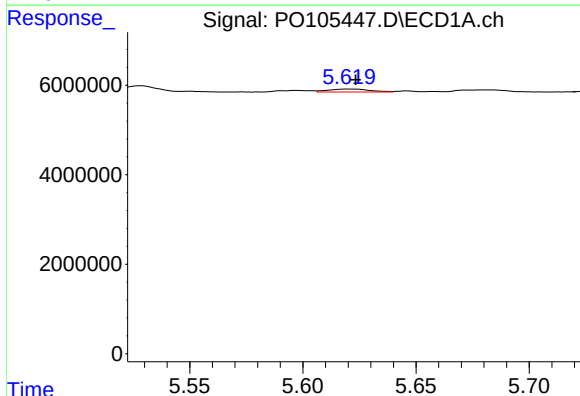


#4 AR-1016-2

R.T.: 5.620 min
Delta R.T.: -0.003 min
Response: 875079
Conc: 2.05 ng/ml

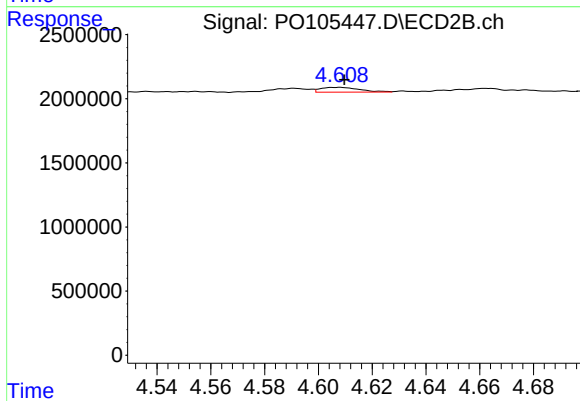

#4 AR-1016-2


R.T.: 4.607 min
Delta R.T.: -0.002 min
Response: 375797
Conc: 2.41 ng/ml

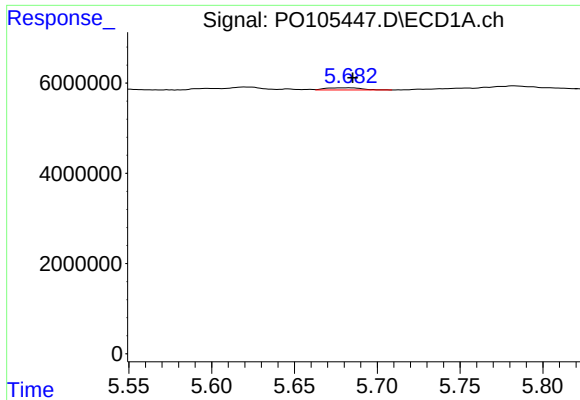

#5 AR-1016-3


R.T.: 5.683 min
Delta R.T.: -0.003 min
Response: 718732
Conc: 2.80 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

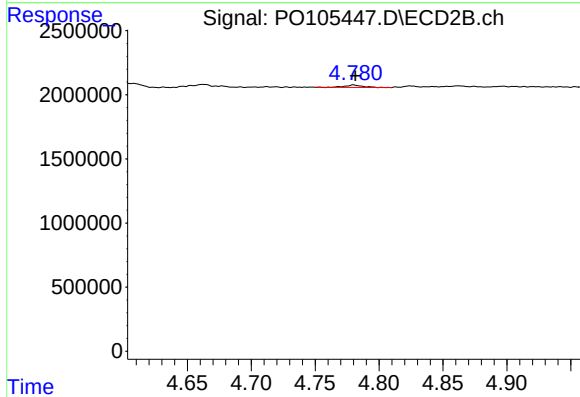


#5 AR-1016-3

R.T.: 4.780 min
Delta R.T.: -0.001 min
Response: 190280
Conc: 2.27 ng/ml

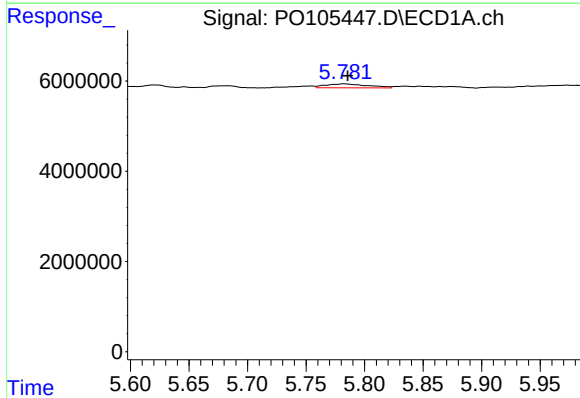


#6 AR-1016-4

R.T.: 5.783 min
Delta R.T.: -0.003 min
Response: 2174307
Conc: 9.94 ng/ml

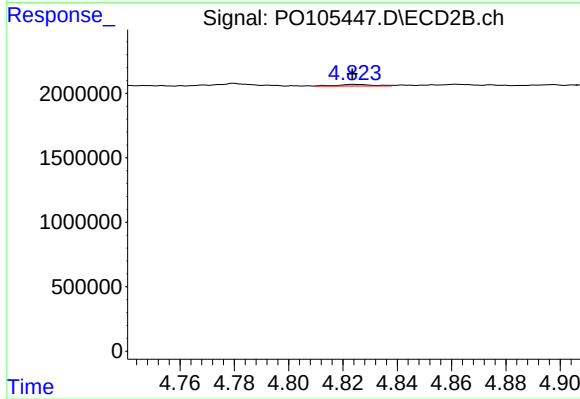

#6 AR-1016-4


R.T.: 4.824 min
Delta R.T.: 0.001 min
Response: 115097
Conc: 1.71 ng/ml

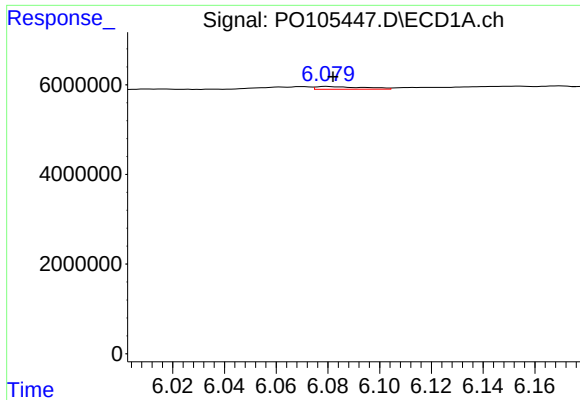

#7 AR-1016-5


R.T.: 6.080 min
Delta R.T.: -0.002 min
Response: 770499
Conc: 3.60 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

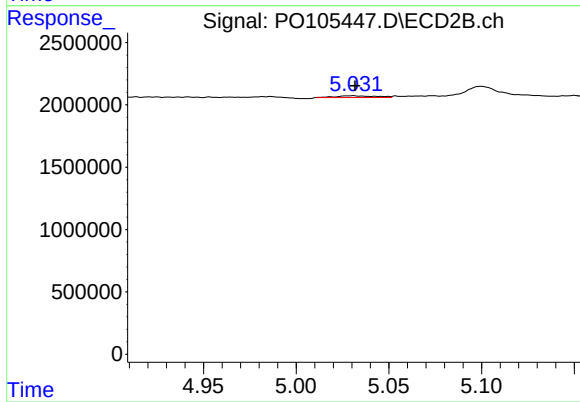


#7 AR-1016-5

R.T.: 5.030 min
Delta R.T.: -0.001 min
Response: 205949
Conc: 2.46 ng/ml

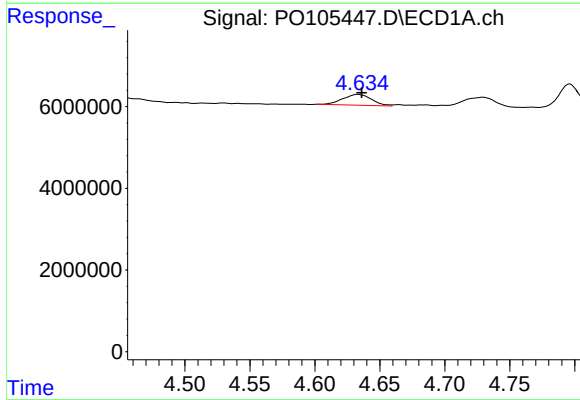


#8 AR-1221-1

R.T.: 4.633 min
Delta R.T.: -0.003 min
Response: 4131946
Conc: 36.85 ng/ml

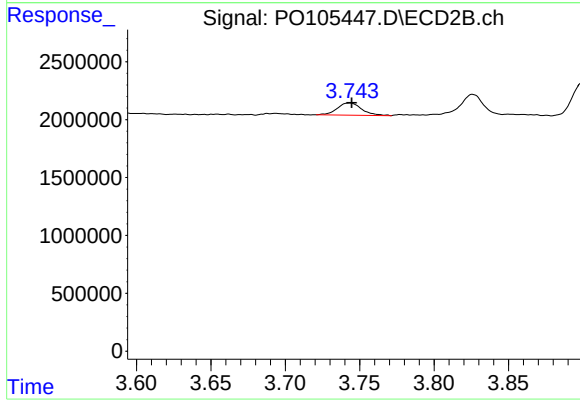

#8 AR-1221-1


R.T.: 3.743 min
Delta R.T.: -0.001 min
Response: 1204339
Conc: 30.51 ng/ml

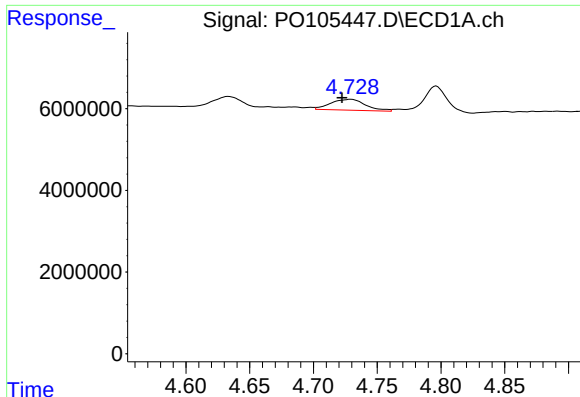

#9 AR-1221-2


R.T.: 4.729 min
Delta R.T.: 0.007 min
Response: 5092926
Conc: 60.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

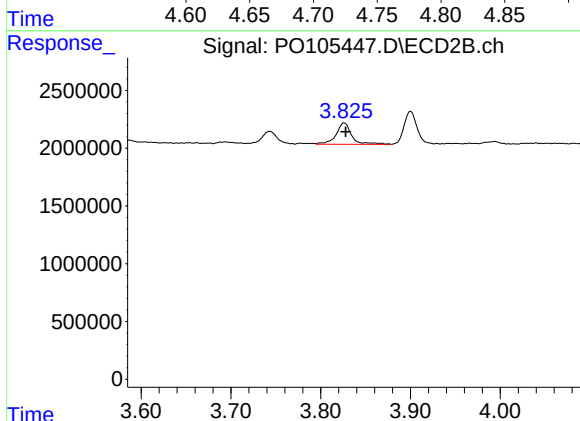


#9 AR-1221-2

R.T.: 3.826 min
Delta R.T.: -0.002 min
Response: 2263357
Conc: 73.67 ng/ml

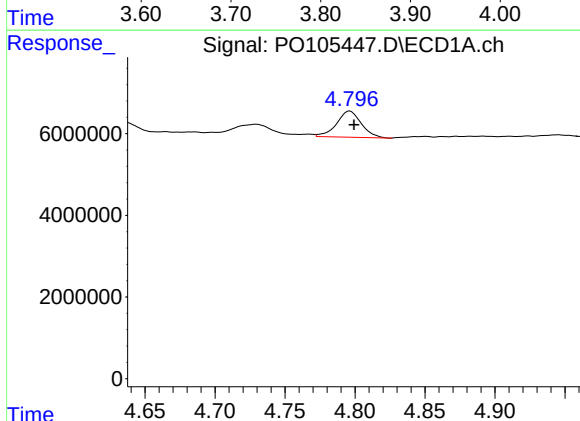


#10 AR-1221-3

R.T.: 4.796 min
Delta R.T.: -0.003 min
Response: 7871497
Conc: 32.36 ng/ml

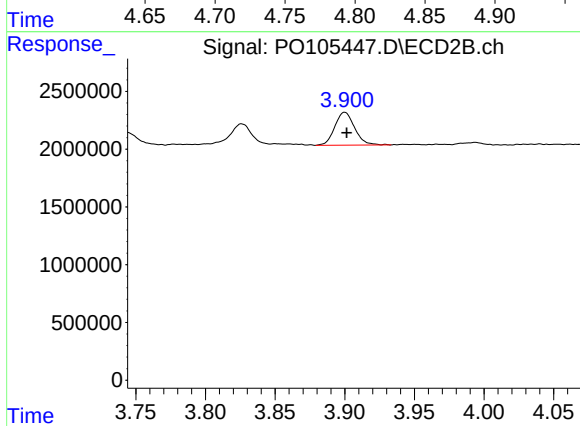

#10 AR-1221-3


R.T.: 3.900 min
Delta R.T.: -0.001 min
Response: 2832523
Conc: 31.65 ng/ml

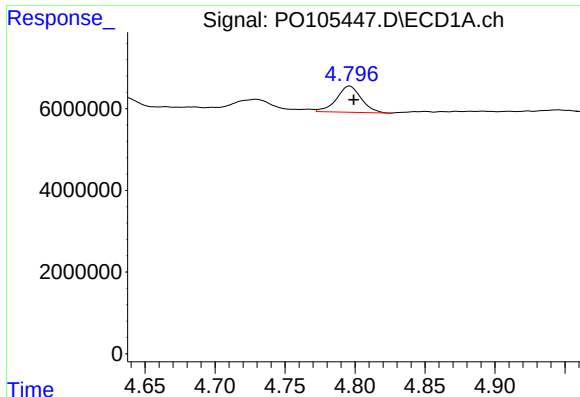

#11 AR-1232-1


R.T.: 4.796 min
Delta R.T.: -0.003 min
Response: 7871497
Conc: 39.37 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

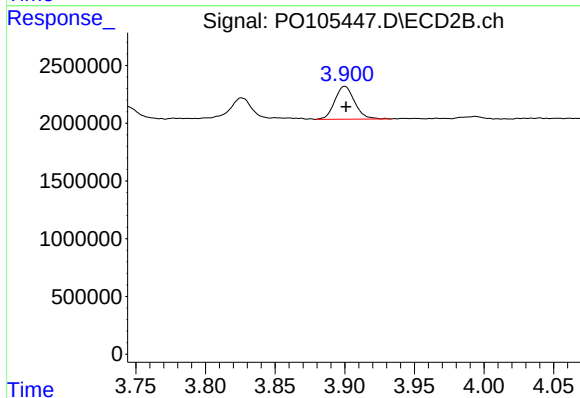


#11 AR-1232-1

R.T.: 3.900 min
Delta R.T.: 0.000 min
Response: 2832523
Conc: 38.79 ng/ml

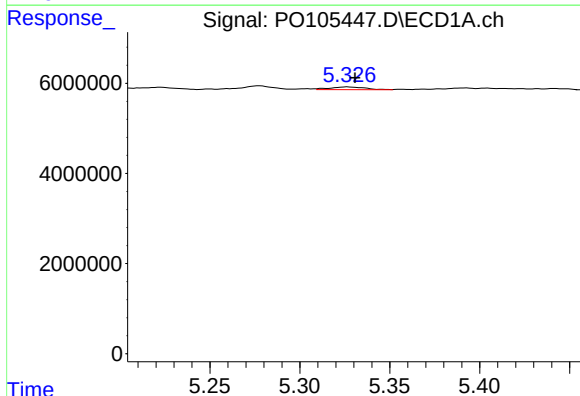


#12 AR-1232-2

R.T.: 5.327 min
Delta R.T.: -0.004 min
Response: 829101
Conc: 7.83 ng/ml

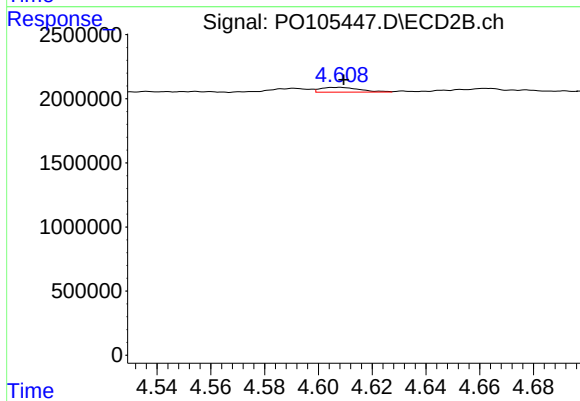

#12 AR-1232-2


R.T.: 4.607 min
Delta R.T.: -0.002 min
Response: 375797
Conc: 5.35 ng/ml

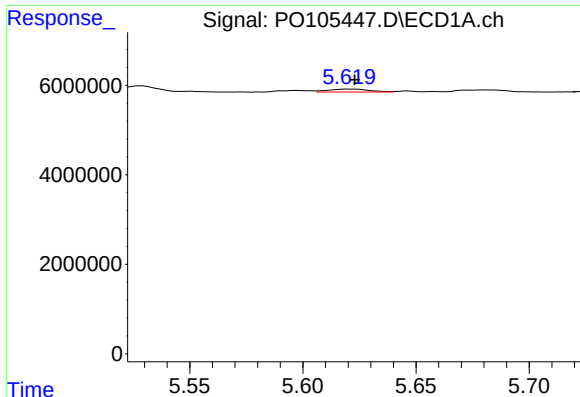

#13 AR-1232-3


R.T.: 5.620 min
Delta R.T.: -0.003 min
Response: 875079
Conc: 4.57 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

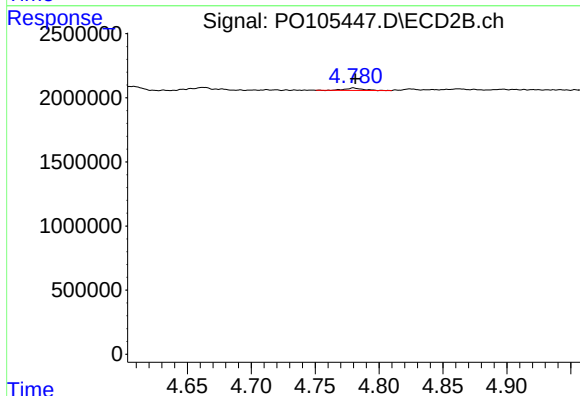


#13 AR-1232-3

R.T.: 4.780 min
Delta R.T.: -0.001 min
Response: 190280
Conc: 4.98 ng/ml

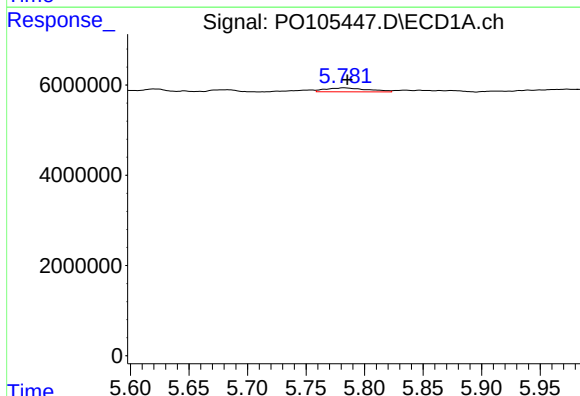


#14 AR-1232-4

R.T.: 5.783 min
Delta R.T.: -0.003 min
Response: 2174307
Conc: 22.29 ng/ml

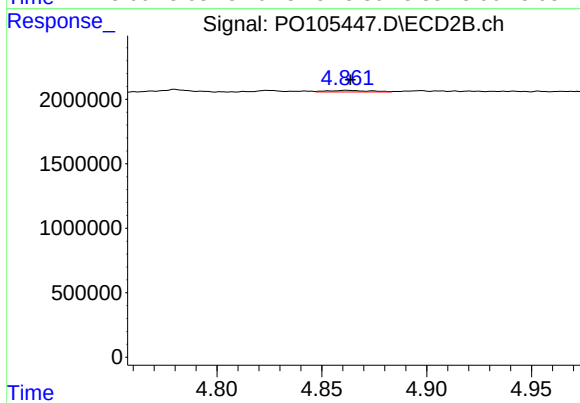

#14 AR-1232-4


R.T.: 4.862 min
Delta R.T.: -0.002 min
Response: 175147
Conc: 5.03 ng/ml

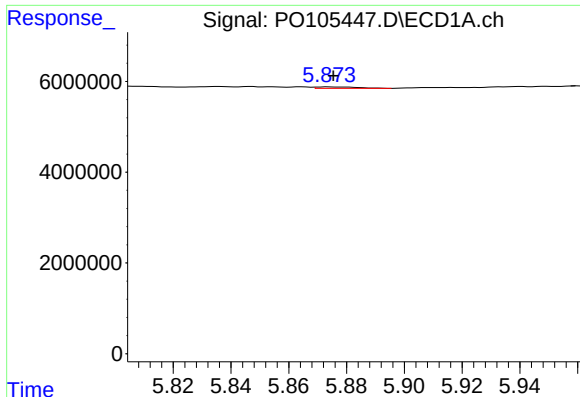

#15 AR-1232-5


R.T.: 5.874 min
Delta R.T.: -0.002 min
Response: 313628
Conc: 4.35 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

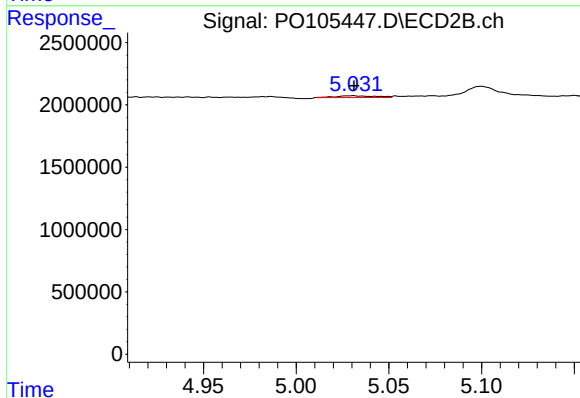


#15 AR-1232-5

R.T.: 5.030 min
Delta R.T.: 0.000 min
Response: 205949
Conc: 5.83 ng/ml

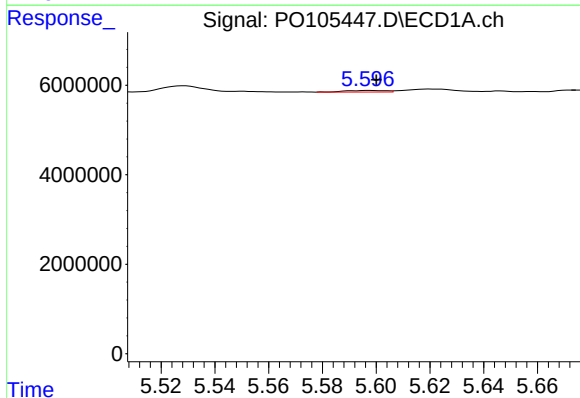


#16 AR-1242-1

R.T.: 5.597 min
Delta R.T.: -0.003 min
Response: 378388
Conc: 1.63 ng/ml

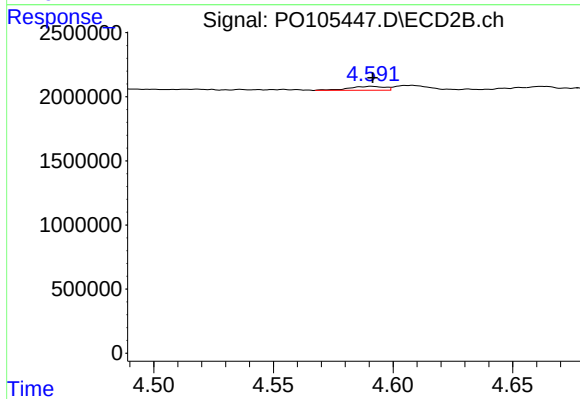

#16 AR-1242-1


R.T.: 4.591 min
Delta R.T.: 0.000 min
Response: 320121
Conc: 3.63 ng/ml

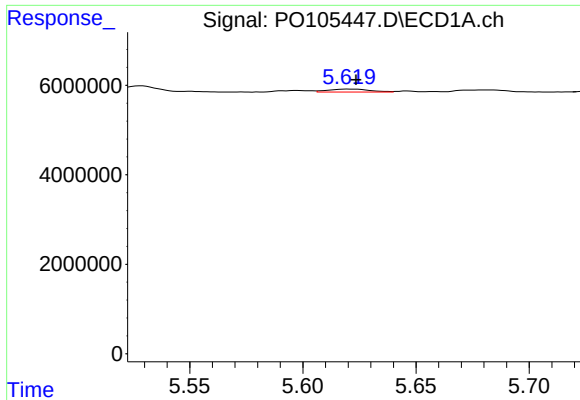

#17 AR-1242-2


R.T.: 5.620 min
Delta R.T.: -0.003 min
Response: 875079
Conc: 2.69 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

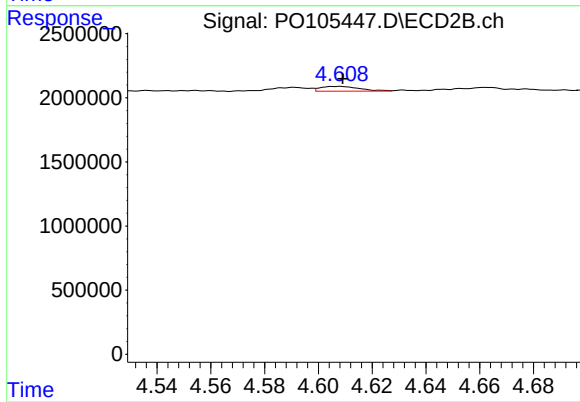


#17 AR-1242-2

R.T.: 4.607 min
Delta R.T.: -0.002 min
Response: 375797
Conc: 3.17 ng/ml

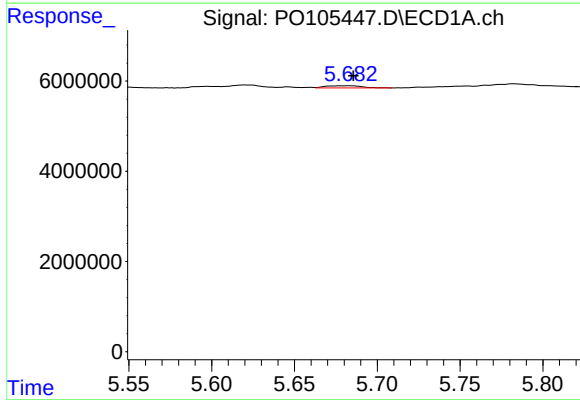


#18 AR-1242-3

R.T.: 5.683 min
Delta R.T.: -0.003 min
Response: 718732
Conc: 3.64 ng/ml

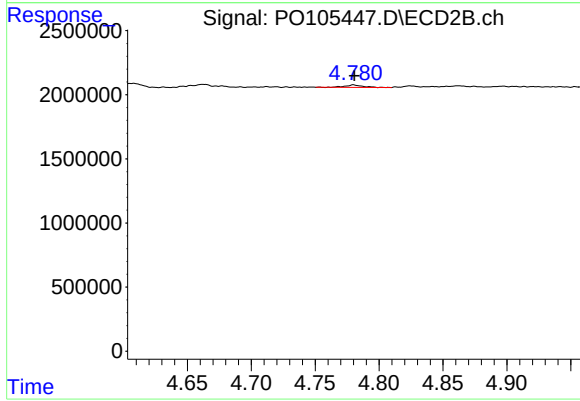

#18 AR-1242-3


R.T.: 4.780 min
Delta R.T.: 0.000 min
Response: 190280
Conc: 2.93 ng/ml

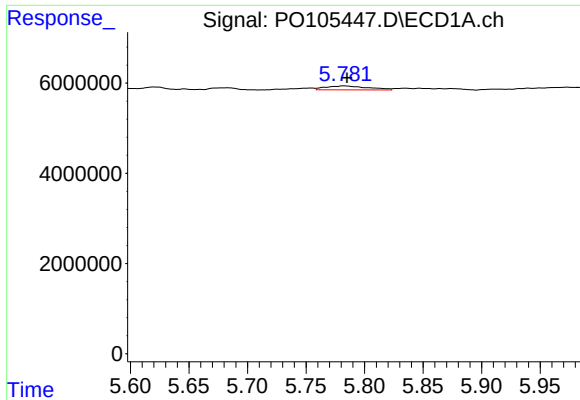

#19 AR-1242-4


R.T.: 5.783 min
Delta R.T.: -0.002 min
Response: 2174307
Conc: 12.74 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

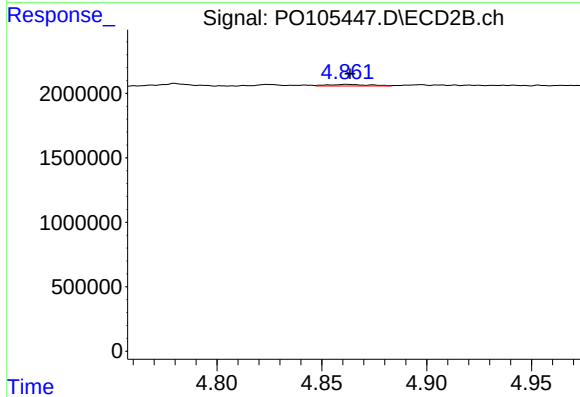


#19 AR-1242-4

R.T.: 4.862 min
Delta R.T.: -0.002 min
Response: 175147
Conc: 2.64 ng/ml

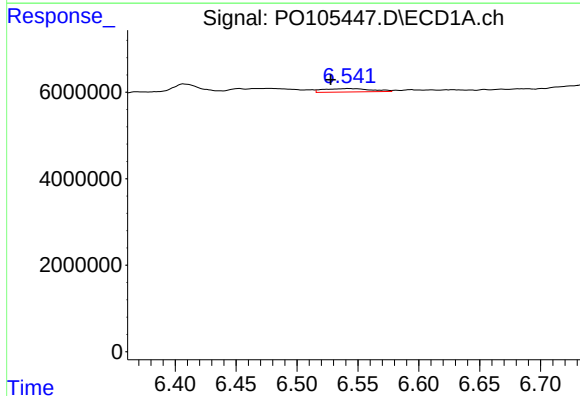


#20 AR-1242-5

R.T.: 6.542 min
Delta R.T.: 0.014 min
Response: 2099511
Conc: 12.01 ng/ml

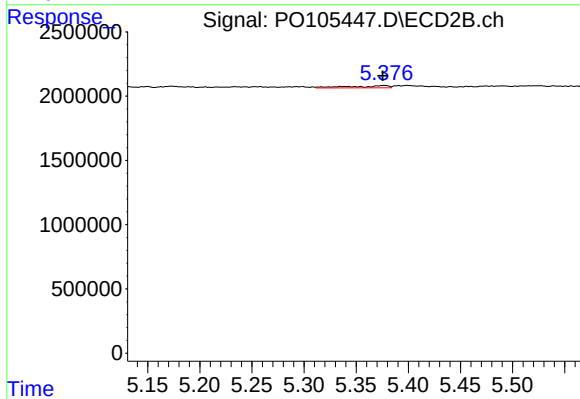

#20 AR-1242-5


R.T.: 5.377 min
Delta R.T.: 0.000 min
Response: 432285
Conc: 5.26 ng/ml

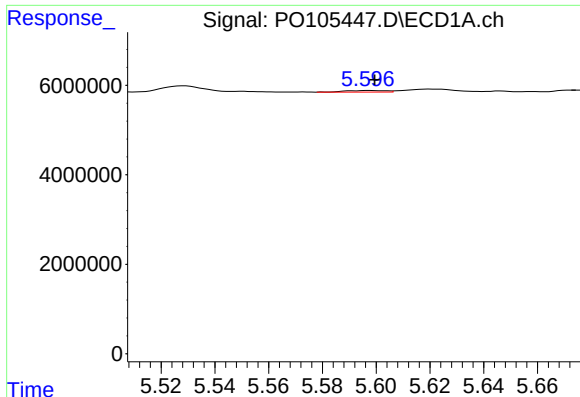

#21 AR-1248-1


R.T.: 5.597 min
Delta R.T.: -0.002 min
Response: 378388
Conc: 2.07 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

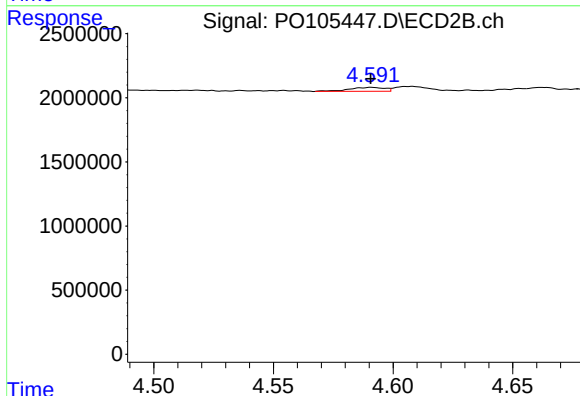


#21 AR-1248-1

R.T.: 4.591 min
Delta R.T.: 0.000 min
Response: 320121
Conc: 4.58 ng/ml

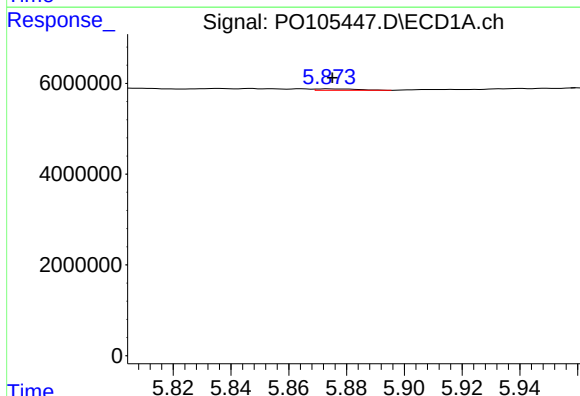


#22 AR-1248-2

R.T.: 5.874 min
Delta R.T.: -0.001 min
Response: 313628
Conc: 1.25 ng/ml

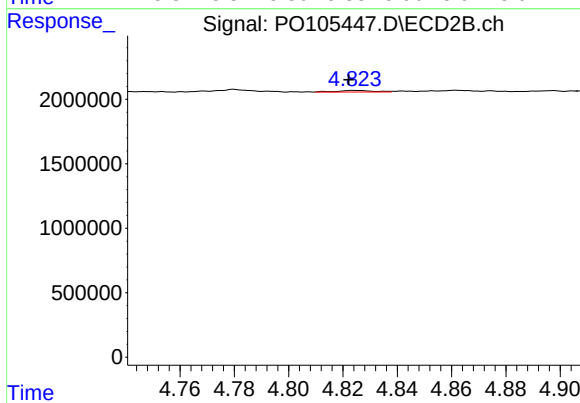

#22 AR-1248-2


R.T.: 4.824 min
Delta R.T.: 0.002 min
Response: 115097
Conc: 1.21 ng/ml

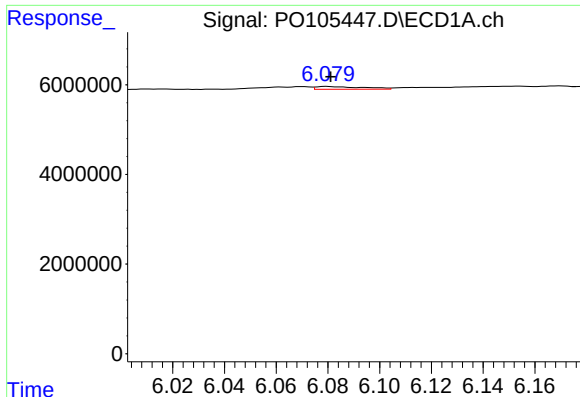

#23 AR-1248-3


R.T.: 6.080 min
Delta R.T.: -0.001 min
Response: 770499
Conc: 2.73 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

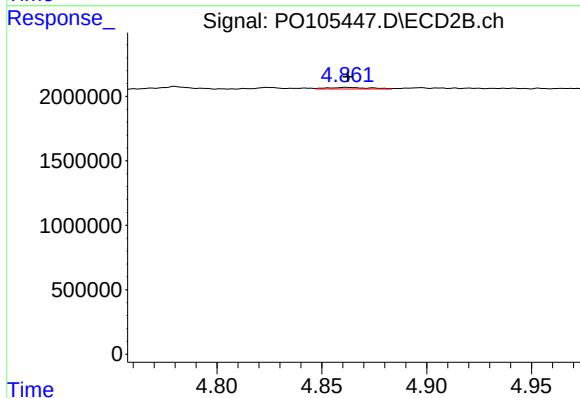


#23 AR-1248-3

R.T.: 4.862 min
Delta R.T.: 0.000 min
Response: 175147
Conc: 1.75 ng/ml

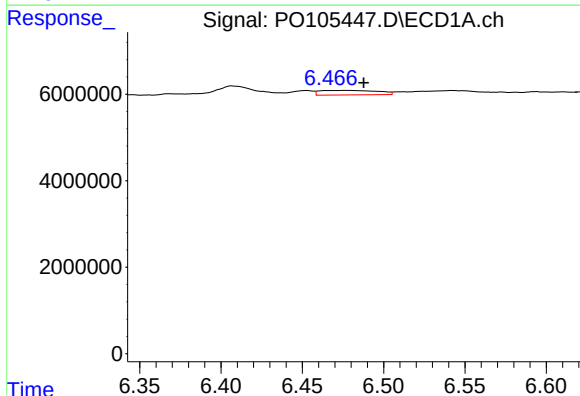


#24 AR-1248-4

R.T.: 6.477 min
Delta R.T.: -0.011 min
Response: 2569722
Conc: 8.04 ng/ml

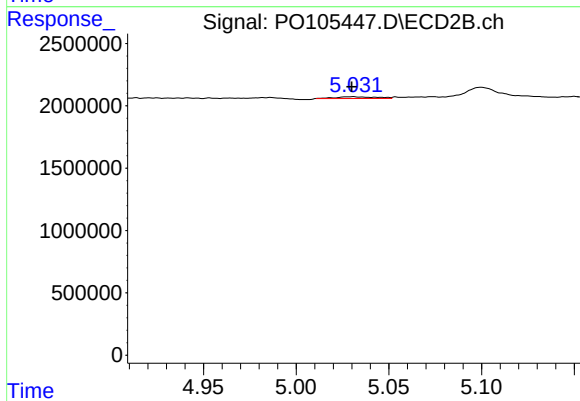

#24 AR-1248-4


R.T.: 5.030 min
Delta R.T.: 0.000 min
Response: 205949
Conc: 1.82 ng/ml

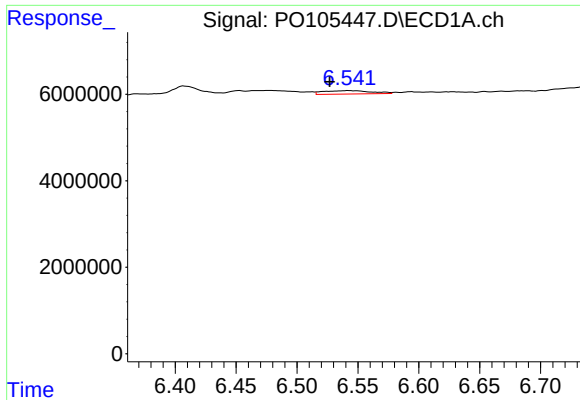

#25 AR-1248-5


R.T.: 6.542 min
Delta R.T.: 0.015 min
Response: 2099511
Conc: 6.79 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

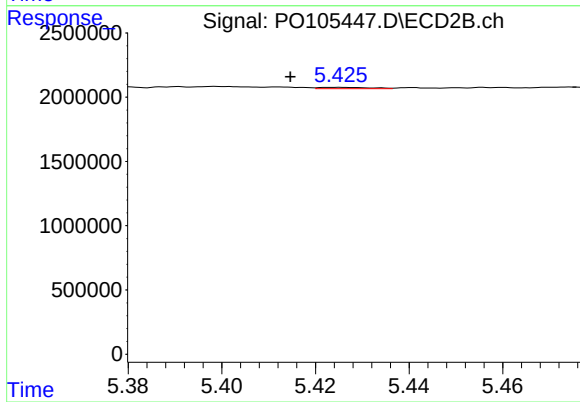


#25 AR-1248-5

R.T.: 5.425 min
Delta R.T.: 0.010 min
Response: 81790
Conc: 0.73 ng/ml

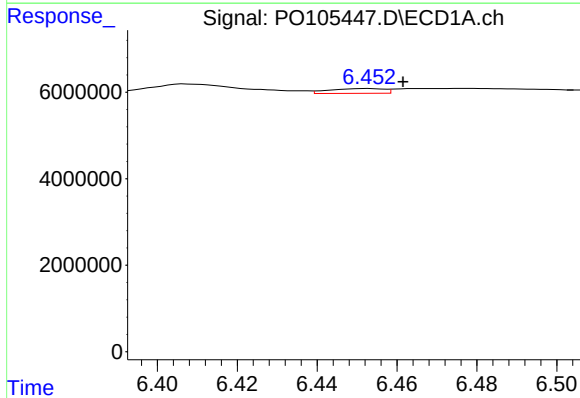


#26 AR-1254-1

R.T.: 6.453 min
Delta R.T.: -0.009 min
Response: 1055576
Conc: 3.37 ng/ml

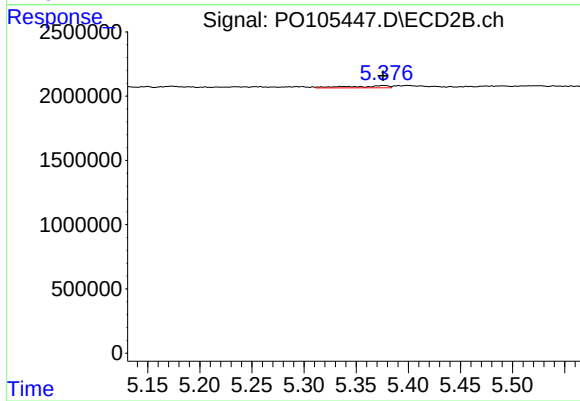

#26 AR-1254-1


R.T.: 5.377 min
Delta R.T.: 0.000 min
Response: 432285
Conc: 2.66 ng/ml

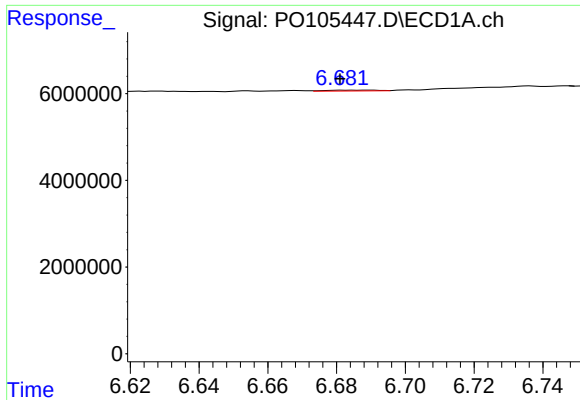

#27 AR-1254-2


R.T.: 6.684 min
Delta R.T.: 0.003 min
Response: 196676
Conc: 0.44 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

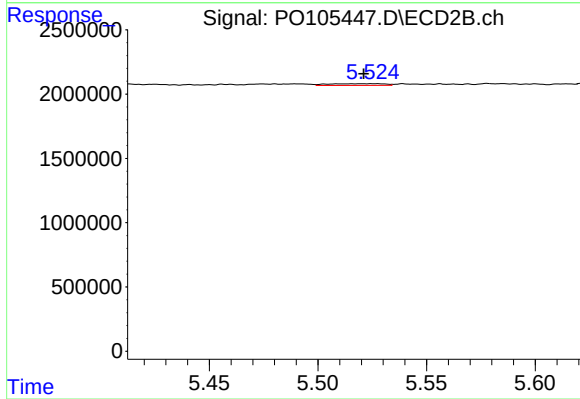


#27 AR-1254-2

R.T.: 5.526 min
Delta R.T.: 0.004 min
Response: 247761
Conc: 1.69 ng/ml

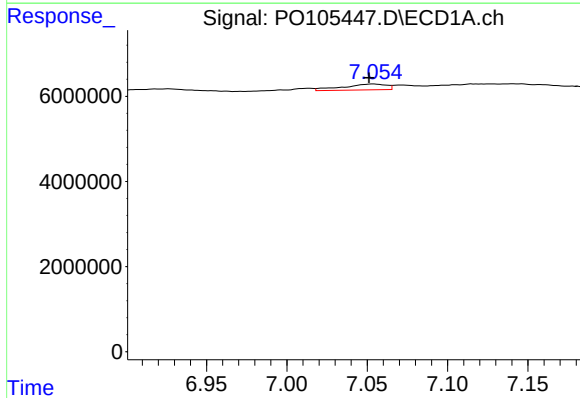


#28 AR-1254-3

R.T.: 7.054 min
Delta R.T.: 0.003 min
Response: 2592120
Conc: 5.46 ng/ml

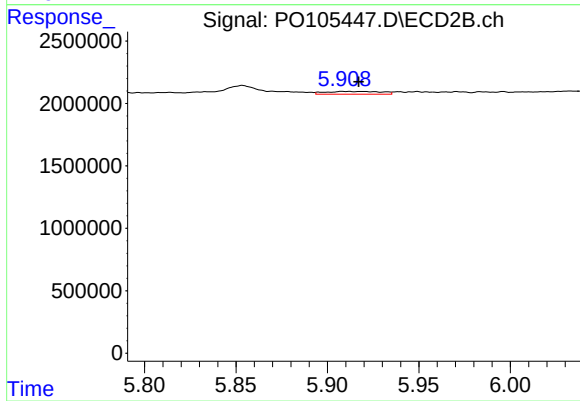

#28 AR-1254-3


R.T.: 5.909 min
Delta R.T.: -0.008 min
Response: 476254
Conc: 2.11 ng/ml

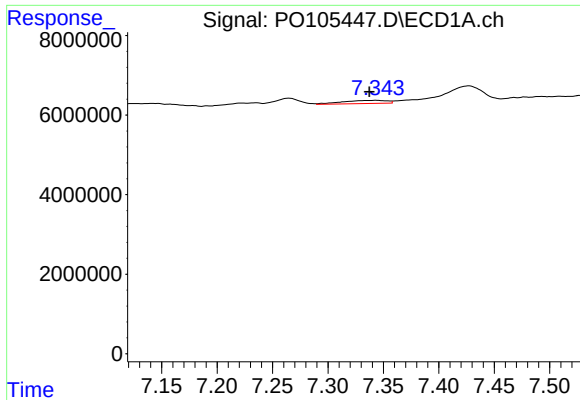

#29 AR-1254-4


R.T.: 7.343 min
Delta R.T.: 0.006 min
Response: 2223549
Conc: 6.21 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

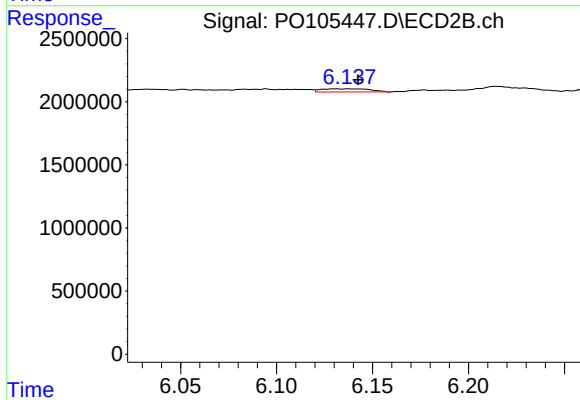


#29 AR-1254-4

R.T.: 6.138 min
Delta R.T.: -0.005 min
Response: 440920
Conc: 3.12 ng/ml

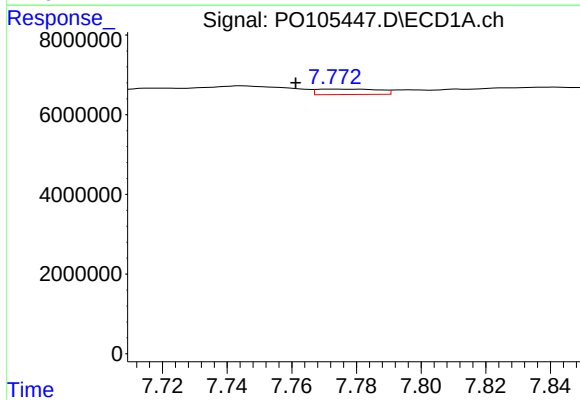


#30 AR-1254-5

R.T.: 7.773 min
Delta R.T.: 0.011 min
Response: 1794788
Conc: 4.52 ng/ml

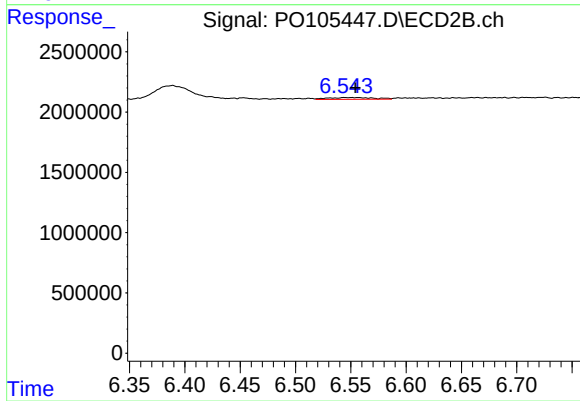

#30 AR-1254-5


R.T.: 6.544 min
Delta R.T.: -0.010 min
Response: 434092
Conc: 2.17 ng/ml

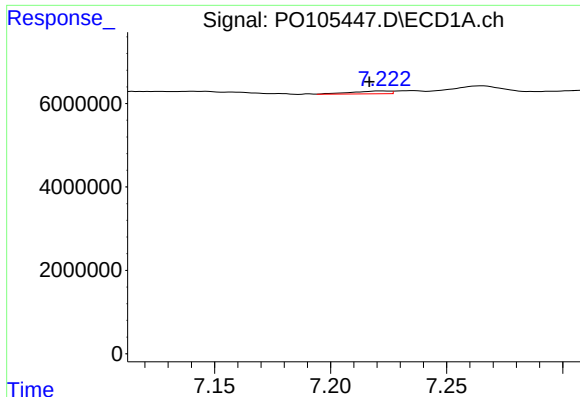

#31 AR-1260-1


R.T.: 7.222 min
Delta R.T.: 0.006 min
Response: 788473
Conc: 2.15 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

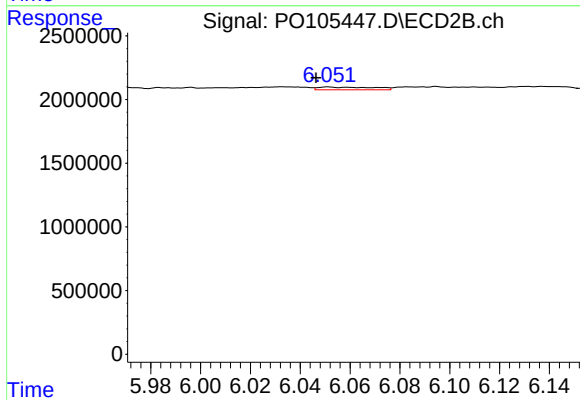


#31 AR-1260-1

R.T.: 6.051 min
Delta R.T.: 0.005 min
Response: 330540
Conc: 2.12 ng/ml

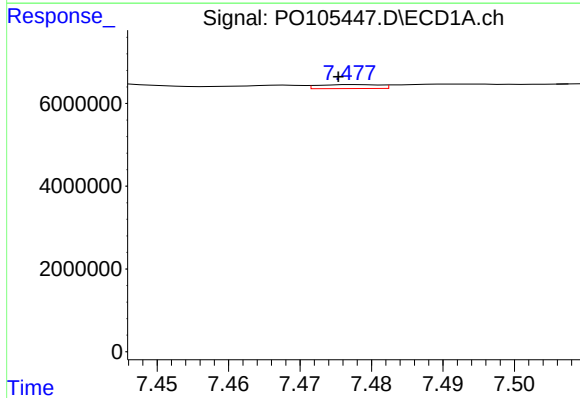


#32 AR-1260-2

R.T.: 7.478 min
Delta R.T.: 0.003 min
Response: 572010
Conc: 1.37 ng/ml

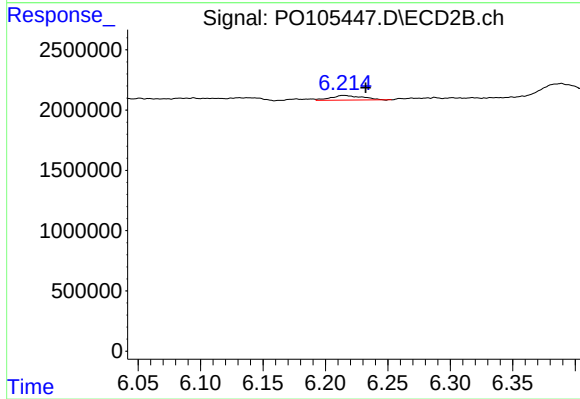

#32 AR-1260-2


R.T.: 6.215 min
Delta R.T.: -0.018 min
Response: 686898
Conc: 3.63 ng/ml

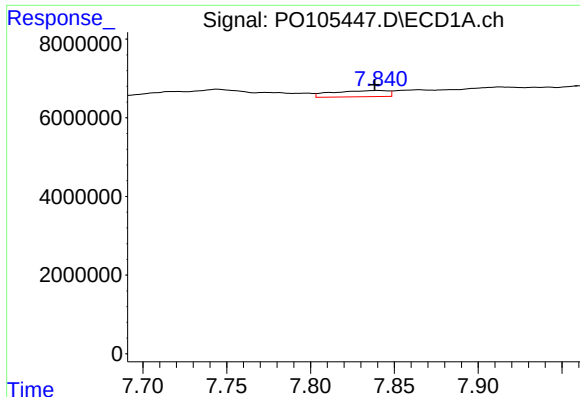

#33 AR-1260-3


R.T.: 7.841 min
Delta R.T.: 0.002 min
Response: 3597193
Conc: 13.90 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

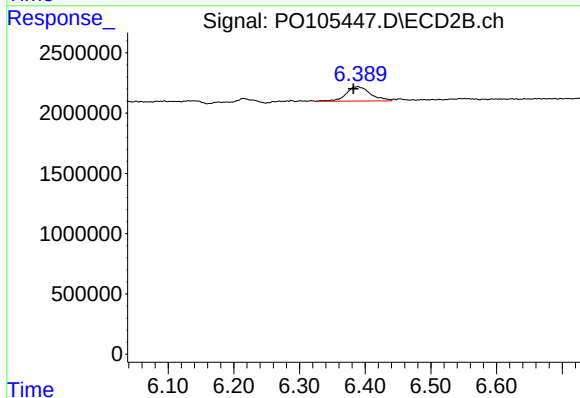


#33 AR-1260-3

R.T.: 6.389 min
Delta R.T.: 0.006 min
Response: 3108619
Conc: 16.83 ng/ml

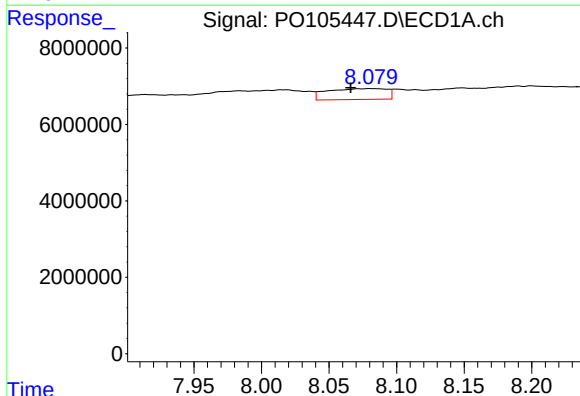


#34 AR-1260-4

R.T.: 8.080 min
Delta R.T.: 0.014 min
Response: 8746059
Conc: 26.51 ng/ml

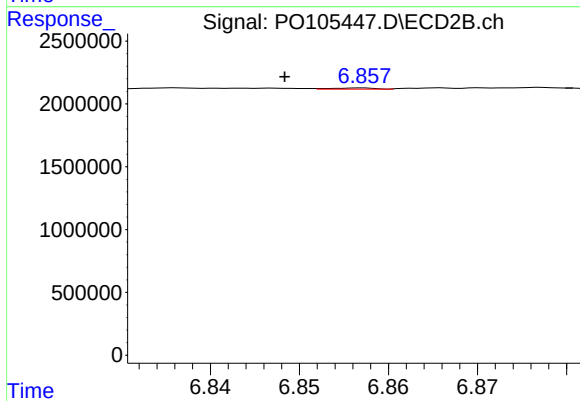

#34 AR-1260-4


R.T.: 6.857 min
Delta R.T.: 0.008 min
Response: 32693
Conc: 0.27 ng/ml

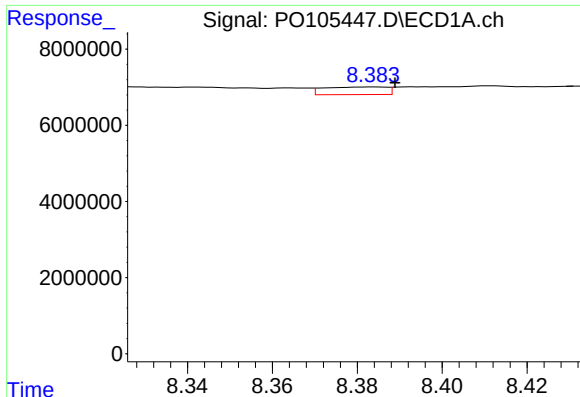

#35 AR-1260-5


R.T.: 8.384 min
Delta R.T.: -0.005 min
Response: 2069541
Conc: 3.48 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

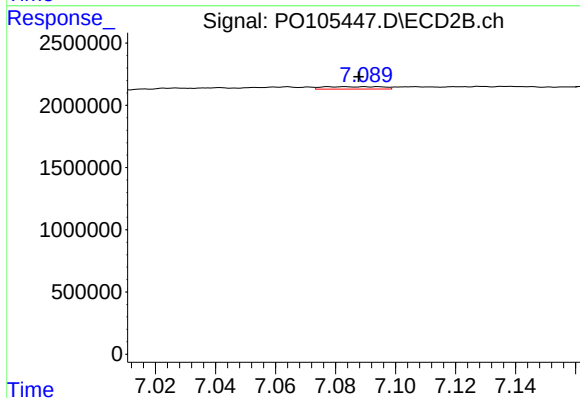


#35 AR-1260-5

R.T.: 7.078 min
Delta R.T.: -0.010 min
Response: 273041
Conc: 0.98 ng/ml

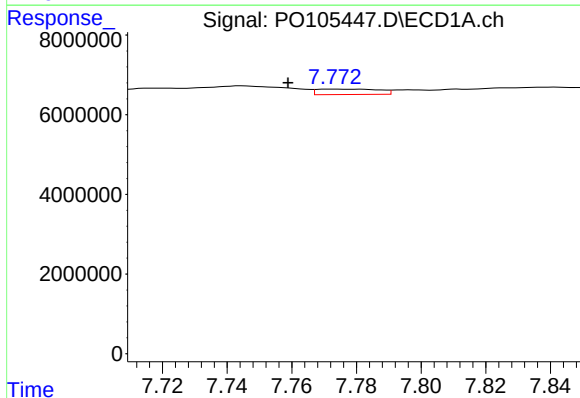


#36 AR-1262-1

R.T.: 7.773 min
Delta R.T.: 0.014 min
Response: 1794788
Conc: 5.65 ng/ml

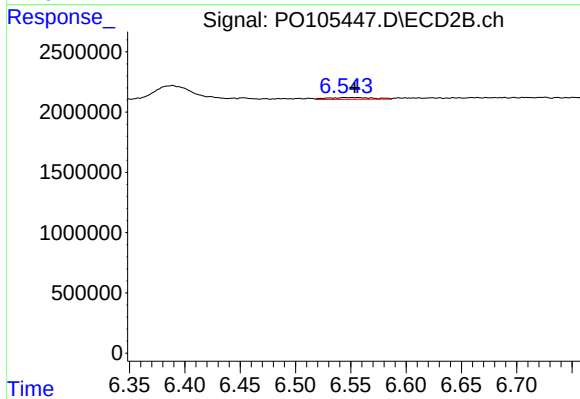

#36 AR-1262-1


R.T.: 6.544 min
Delta R.T.: -0.009 min
Response: 434092
Conc: 4.08 ng/ml

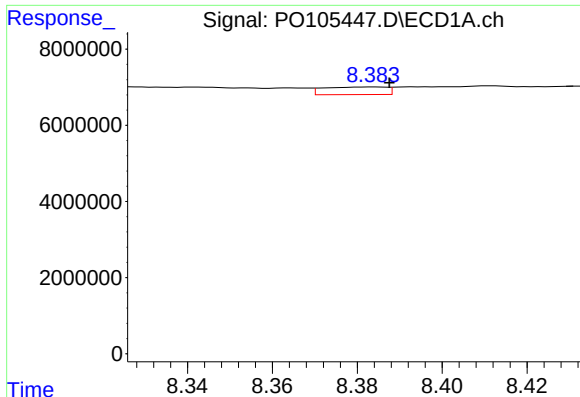

#37 AR-1262-2


R.T.: 8.384 min
Delta R.T.: -0.003 min
Response: 2069541
Conc: 2.75 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

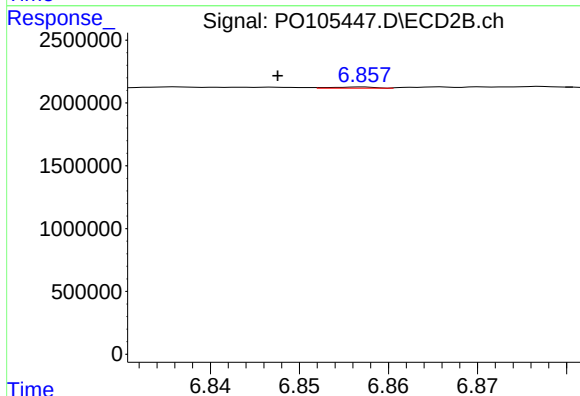


#37 AR-1262-2

R.T.: 6.857 min
Delta R.T.: 0.009 min
Response: 32693
Conc: 0.19 ng/ml

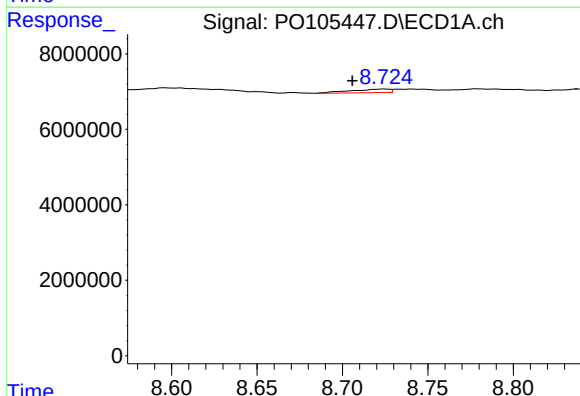


#38 AR-1262-3

R.T.: 8.724 min
Delta R.T.: 0.018 min
Response: 1493008
Conc: 3.03 ng/ml

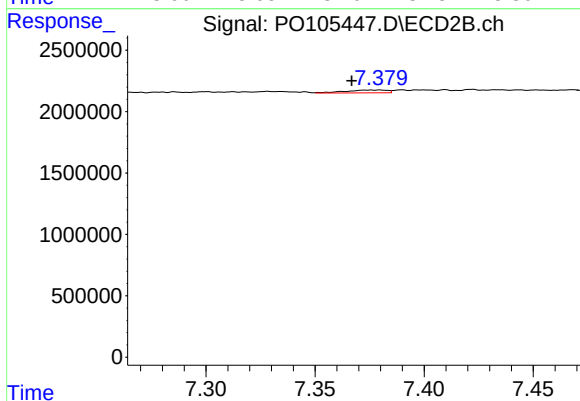

#38 AR-1262-3


R.T.: 7.379 min
Delta R.T.: 0.013 min
Response: 312007
Conc: 2.47 ng/ml

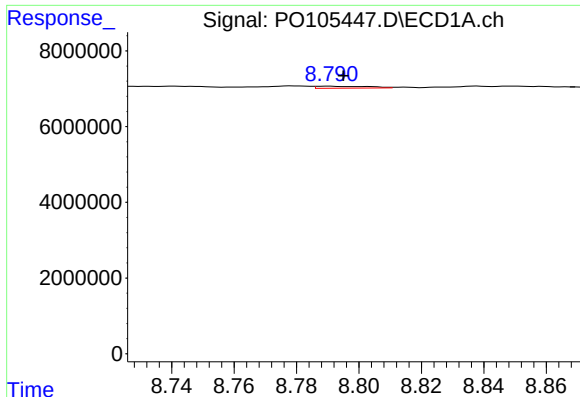

#39 AR-1262-4


R.T.: 8.790 min
Delta R.T.: -0.005 min
Response: 603764
Conc: 1.64 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

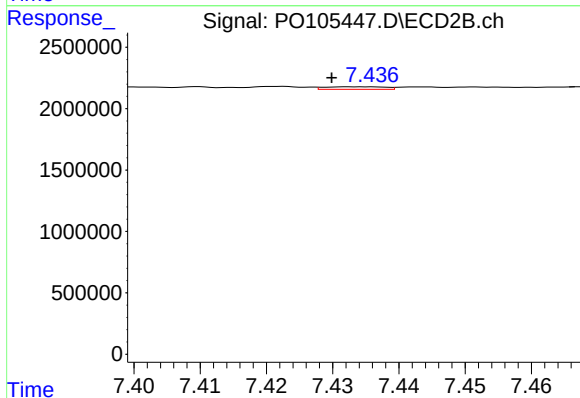


#39 AR-1262-4

R.T.: 7.434 min
Delta R.T.: 0.004 min
Response: 132722
Conc: 0.57 ng/ml

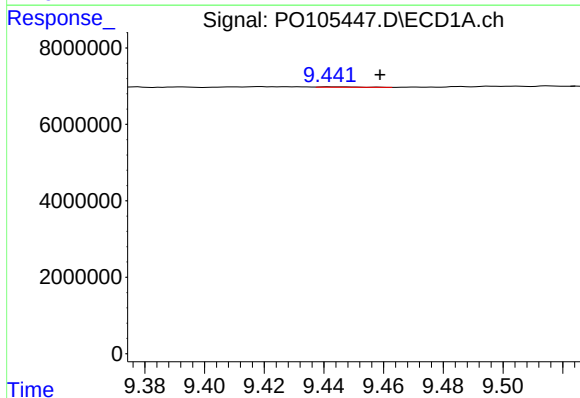


#40 AR-1262-5

R.T.: 9.442 min
Delta R.T.: -0.017 min
Response: 89000
Conc: 0.33 ng/ml

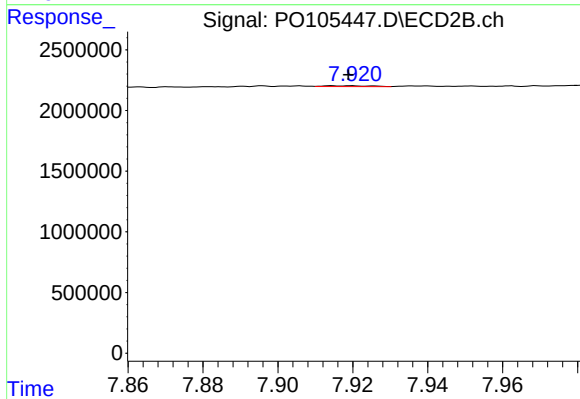

#40 AR-1262-5


R.T.: 7.920 min
Delta R.T.: 0.000 min
Response: 53695
Conc: 0.53 ng/ml

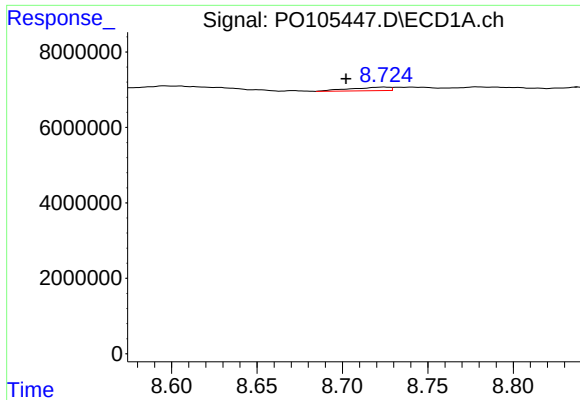

#41 AR-1268-1


R.T.: 8.724 min
Delta R.T.: 0.022 min
Response: 1493008
Conc: 1.84 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

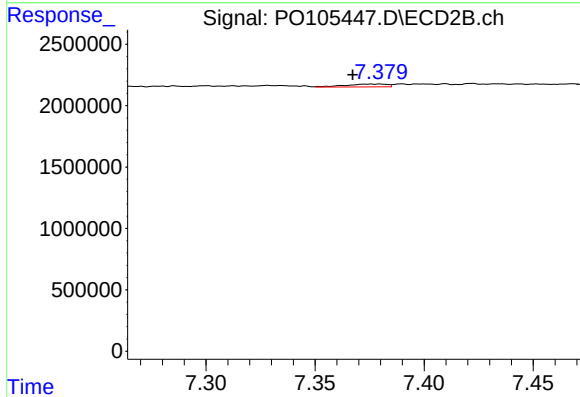


#41 AR-1268-1

R.T.: 7.379 min
Delta R.T.: 0.012 min
Response: 312007
Conc: 0.89 ng/ml

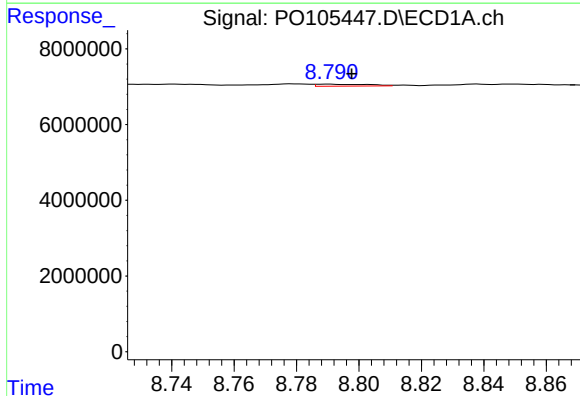


#42 AR-1268-2

R.T.: 8.790 min
Delta R.T.: -0.007 min
Response: 603764
Conc: 0.83 ng/ml

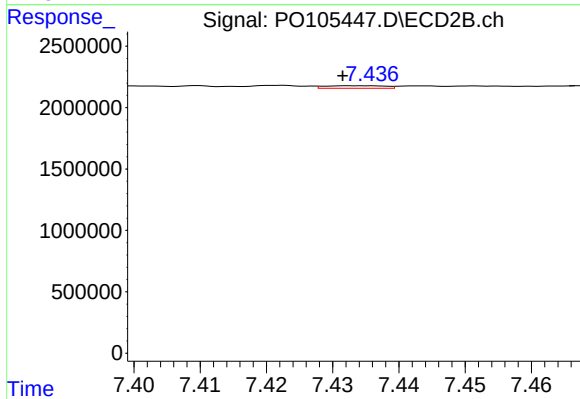

#42 AR-1268-2


R.T.: 7.434 min
Delta R.T.: 0.002 min
Response: 132722
Conc: 0.43 ng/ml

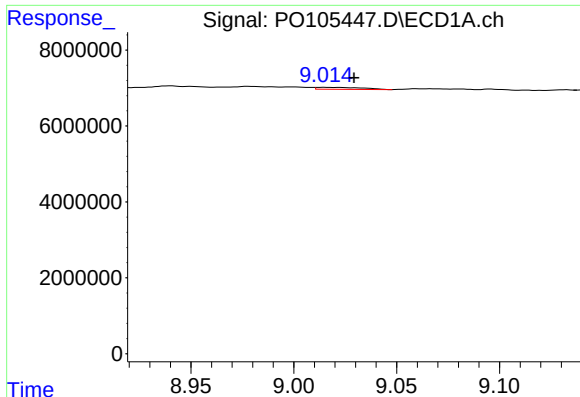

#43 AR-1268-3


R.T.: 9.015 min
Delta R.T.: -0.014 min
Response: 816407
Conc: 1.26 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

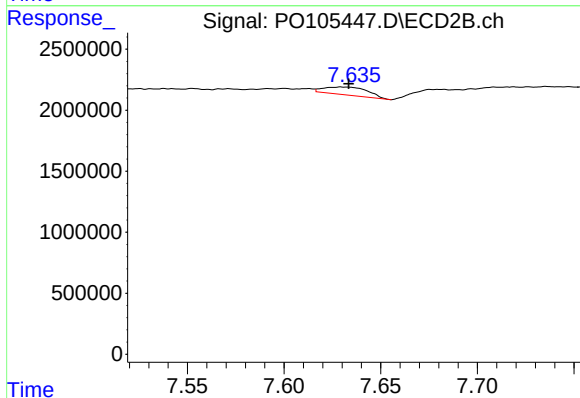


#43 AR-1268-3

R.T.: 7.630 min
Delta R.T.: -0.003 min
Response: 1014215
Conc: 4.01 ng/ml

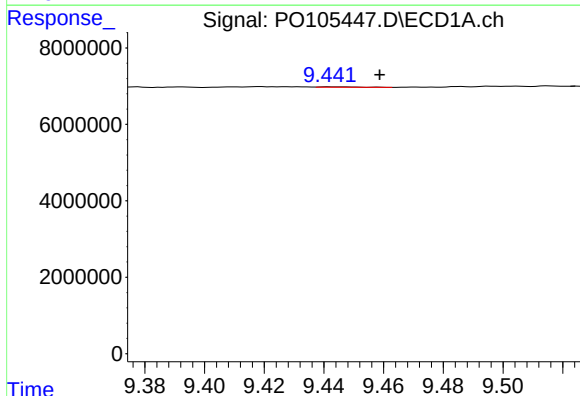


#44 AR-1268-4

R.T.: 9.442 min
Delta R.T.: -0.016 min
Response: 89000
Conc: 0.32 ng/ml

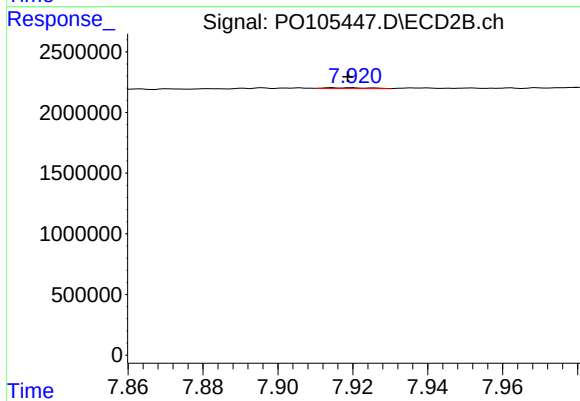

#44 AR-1268-4


R.T.: 7.920 min
Delta R.T.: 0.000 min
Response: 53695
Conc: 0.50 ng/ml

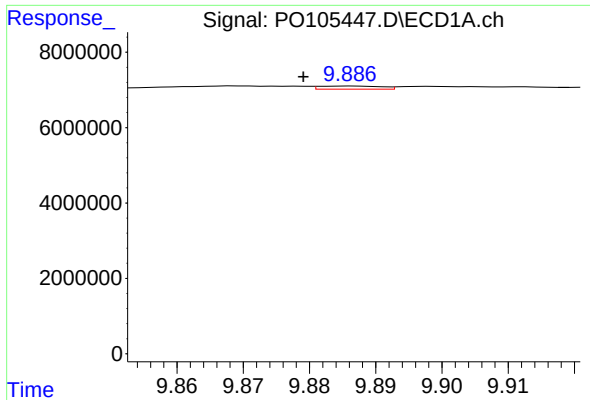

#45 AR-1268-5

R.T.: 9.886 min
Delta R.T.: 0.007 min
Response: 542099
Conc: 0.26 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

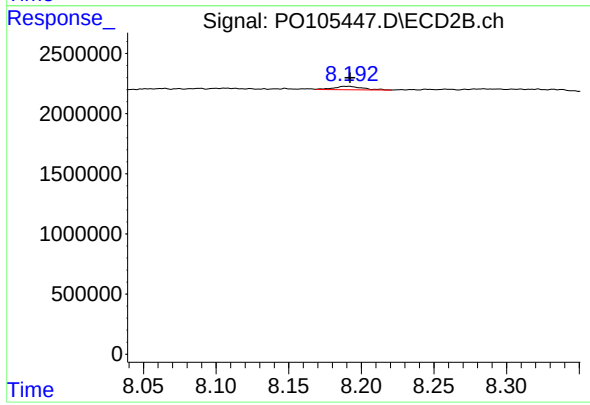

#45 AR-1268-5

R.T.: 8.190 min
Delta R.T.: -0.002 min
Response: 393192
Conc: 0.59 ng/ml